

**WOOD BUFFALO ENVIRONMENTAL ASSOCIATION
MONTHLY AMBIENT AIR QUALITY MONITORING REPORT
JANUARY 2023
REPORT HISTORY**

Original report release data: February 28, 2023

Revised report release date: August 30, 2023

Revision 1 – Submission of H₂S data and Revision of TRS data at Patricia McInnes.

The Patricia McInnes air monitoring station (AMS06) collected H₂S data from January 3, 2023, to June 12, 2023, but it was reported as TRS. On August 30, 2023, the data was resubmitted as H₂S to the Electronic Transfer System (ETS) and the TRS data was revised. The monthly report cover letter, station summary, network summary, and calibration report contained within have been revised to reflect the change.



**WOOD BUFFALO
ENVIRONMENTAL ASSOCIATION**

Unit 3 - 805 Memorial Drive
Fort McMurray, AB T9K 0K4
P: 780.799.4420 E: info@wbea.org
wbea.org

Wood Buffalo Environmental Association

JANUARY 2023

MONTHLY CALIBRATION REPORT

CONTINUOUS MONITORING

August 30, 2023

Revision 01

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association





WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS01 BERTHA GANTER - FORT MCKAY JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Bertha Ganter-Fort McKay	Station number:	AMS01
Calibration Date:	January 5, 2023	Last Cal Date:	December 5, 2022
Start time (MST):	11:28	End time (MST):	15:01
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.19	ppm	Cal Gas Exp Date:	February 23, 2025
Cal Gas Cylinder #:	CC486642			
Removed Cal Gas Conc:	49.19	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	3565
ZAG Make/Model:	Teledyne API T701		Serial Number:	5609

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	JC1501301448
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.998745	0.998187	Backgd or Offset:	19.0	19.1
Calibration intercept:	-0.313576	-0.293417	Coeff or Slope:	0.884	0.891

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4918	81.3	799.9	789.4	1.013
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.3	----
high point	4918	81.3	799.9	798.6	1.002
second point	4959	40.7	400.4	398.8	1.004
third point	4979	20.3	199.7	198.7	1.005
as left zero	5000	0.0	0.0	0.3	----
as left span	4918	81.3	799.9	799.3	1.001
Average Correction Factor					1.004

Baseline Corr As found:	789.30	Previous response	798.62	*% change	-1.2%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds. Adjusted span only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 5, 2023	Previous Calibration:	December 5, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:28	End Time (MST):	15:01
Analyzer make:	Thermo 43i	Analyzer serial #:	JC1501301448

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	0.999997	≥0.995
799.9	798.6	1.0017			
400.4	398.8	1.0041	Slope	0.998187	0.90 - 1.10
199.7	198.7	1.0052			
			Intercept	-0.293417	+/-30

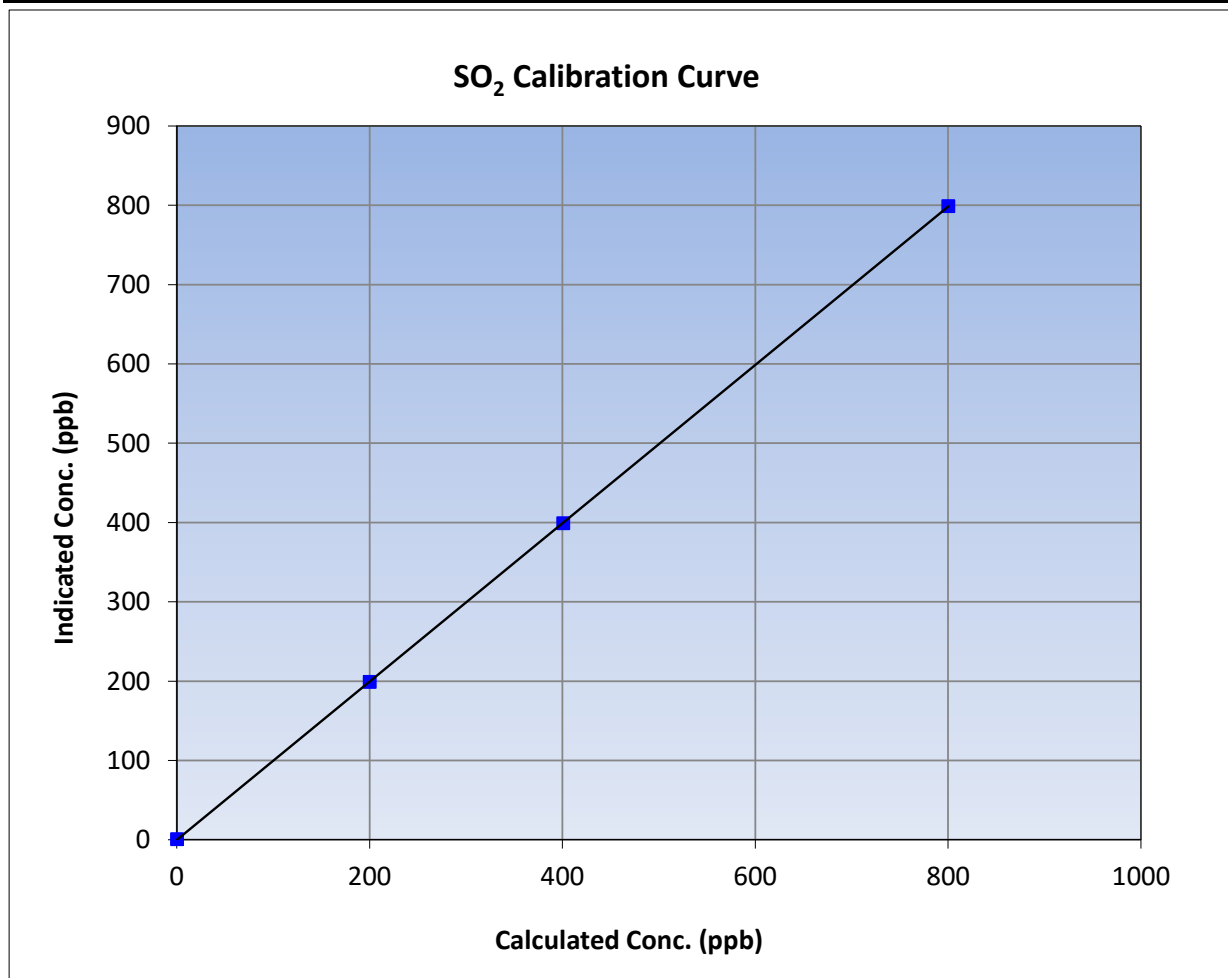

SO2 Calibration Plot

Date: January 5, 2023

Location: Bertha Ganter-Fort McKay

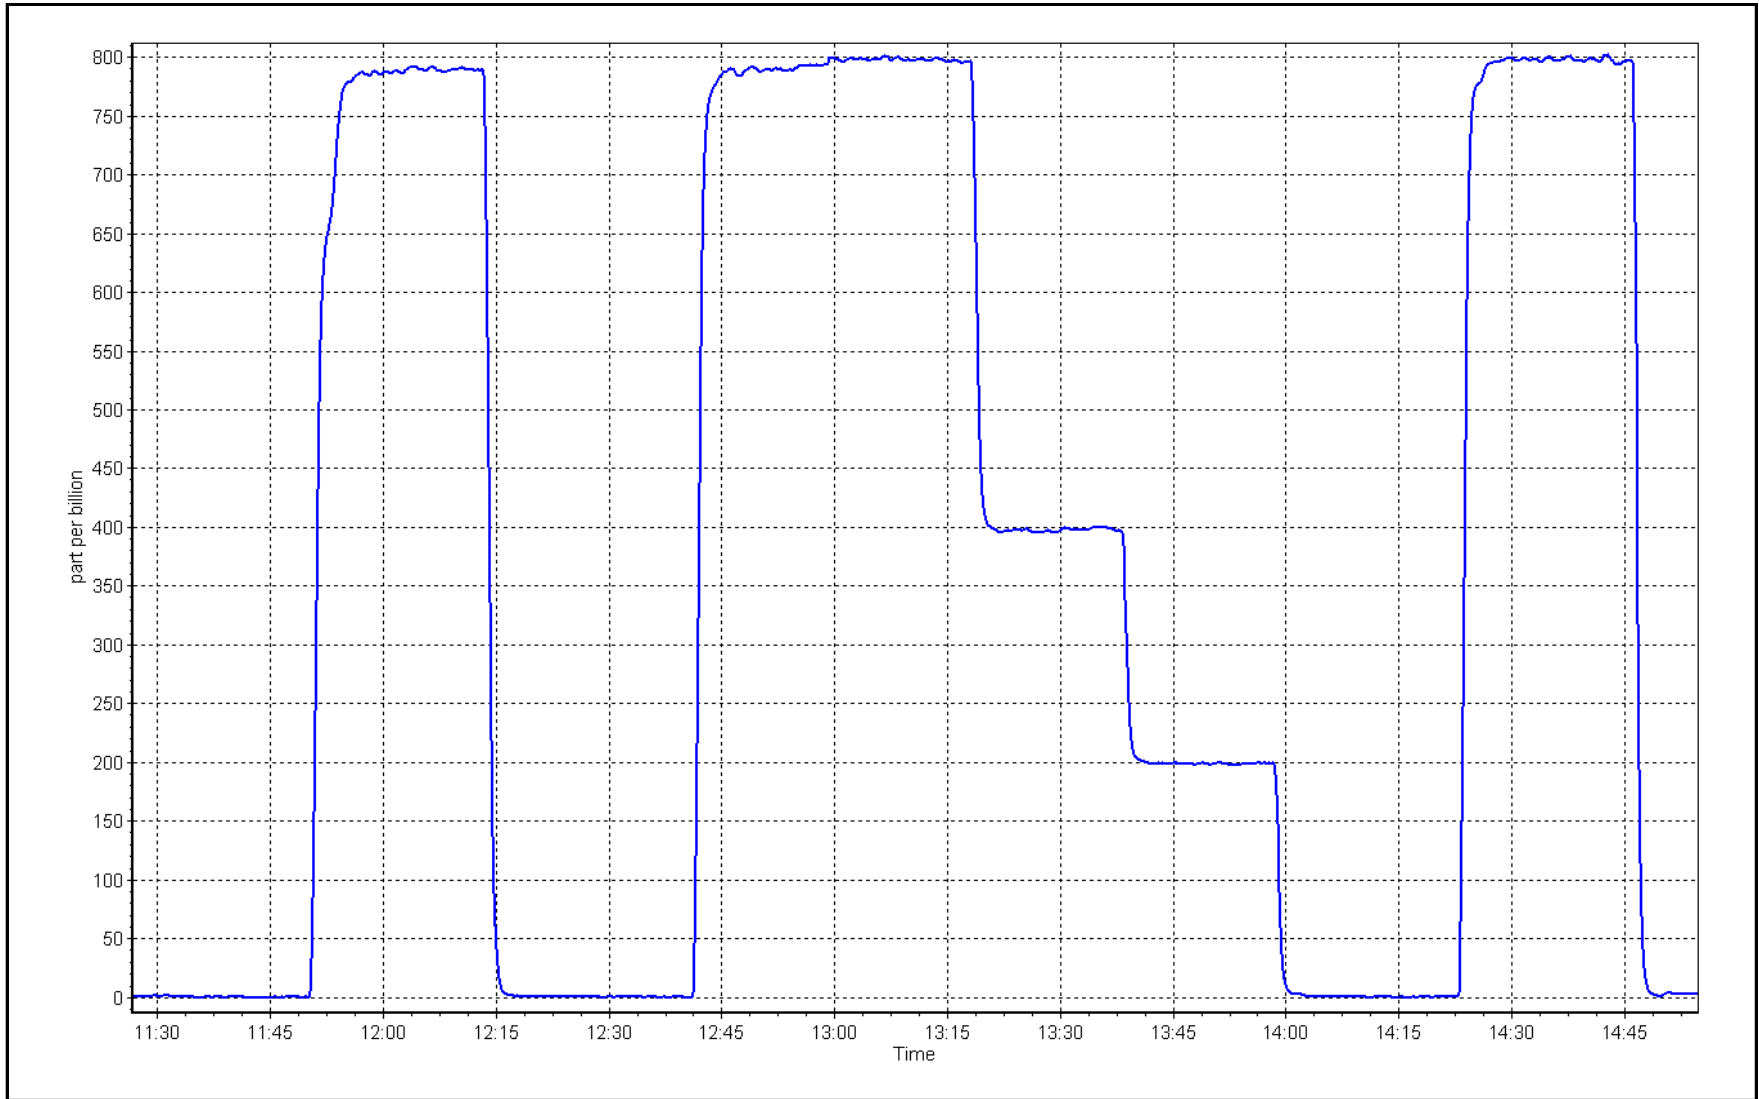



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name: Bertha Ganter-Fort McKay Station number: AMS01
 Calibration Date: January 10, 2023 Last Cal Date: December 13, 2022
 Start time (MST): 10:53 End time (MST): 17:26
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.10 ppm Cal Gas Exp Date: September 16, 2024
 Cal Gas Cylinder #: CC511749
 Removed Cal Gas Conc: 5.10 ppm Rem Gas Exp Date: N/A
 Removed Gas Cyl #: N/A Diff between cyl:
 Calibrator Make/Model: Teledyne API T700 Serial Number: 3565
 ZAG Make/Model: Teledyne API T701 Serial Number: 5609

Analyzer Information

Analyzer make: Thermo 43i-TLE Analyzer serial #: 1218153461
 Converter make: CD Nova Converter serial #: 470
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.999935	0.998364	Backgd or Offset: 2.25	2.29
Calibration intercept:	-0.019999	0.059997	Coeff or Slope: 0.908	0.919

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4921	78.4	80.0	78.8	1.016
as found 2nd point	4960	39.2	40.0	39.7	1.010
as found 3rd point	4980	19.6	20.0	19.9	1.010
new cylinder response					

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.1	----
high point	4921	78.4	80.0	79.9	1.001
second point	4960	39.2	40.0	40.1	0.997
third point	4980	19.6	20.0	19.9	1.005
as left zero	5000	0.0	0.0	0.2	----
as left span	4921	78.4	80.0	79.5	1.006
SO2 Scrubber Check	4919	81.3	813.0	0.0	----
Date of last scrubber change:	December 17, 2021			Ave Corr Factor	1.001
Date of last converter efficiency test:	efficiency				

Baseline Corr As found: 78.7 Prev response: 79.97 *% change: -1.6%
 Baseline Corr 2nd AF pt: 39.6 AF Slope: 0.983649 AF Intercept: 0.199998
 Baseline Corr 3rd AF pt: 19.8 AF Correlation: 0.999987

* = > +/-5% change initiates investigation

Notes: Inlet filter change and scrubber check completed after as founds. Adjusted span only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 13, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	10:53	End Time (MST):	17:26
Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1218153461

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.1	----	Correlation Coefficient	0.999992	≥0.995
80.0	79.9	1.0012			
40.0	40.1	0.9975	Slope	0.998364	0.90 - 1.10
20.0	19.9	1.0049			
			Intercept	0.059997	+/-3

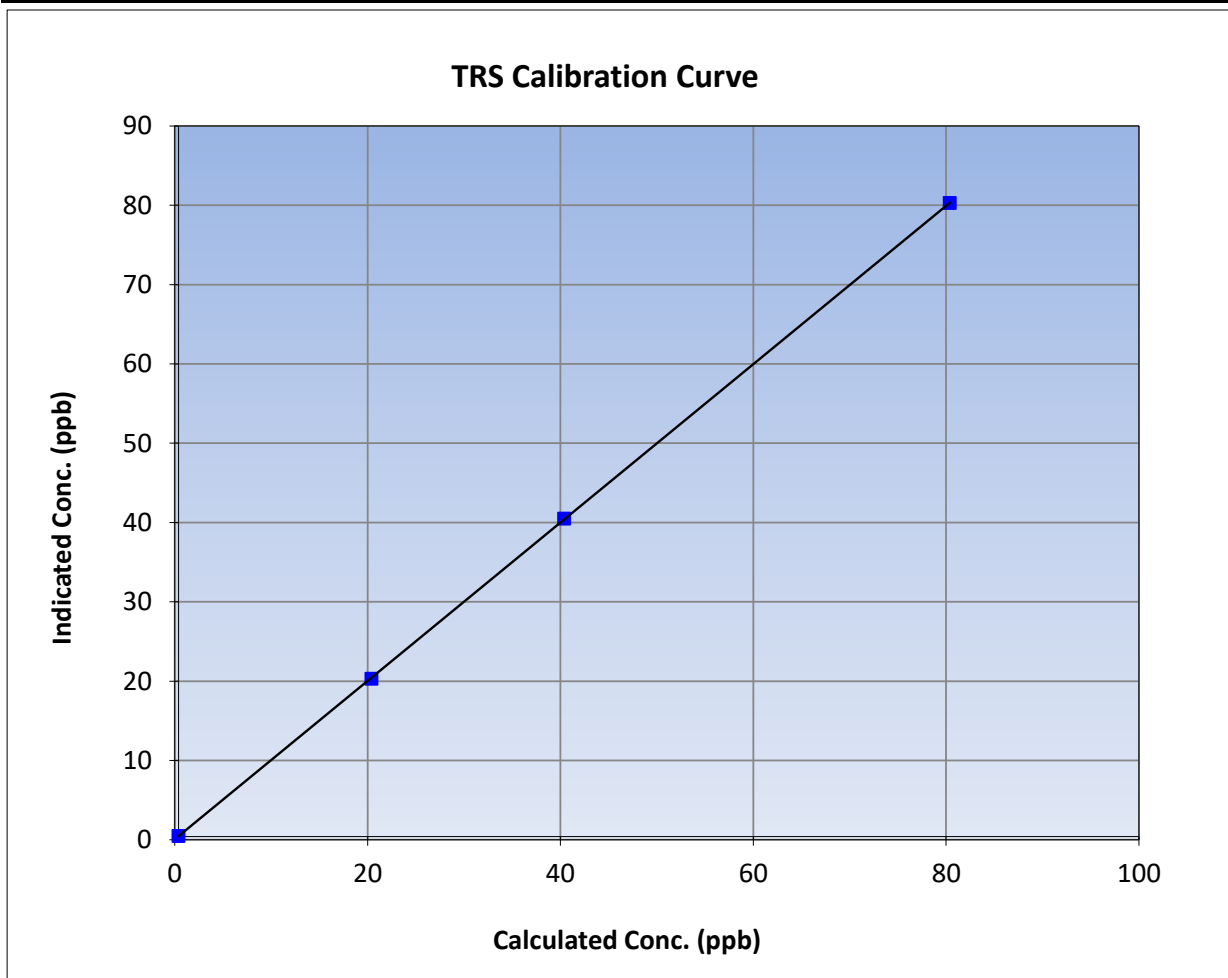

TRS Calibration Plot

Date: January 10, 2023

Location: Bertha Ganter-Fort McKay

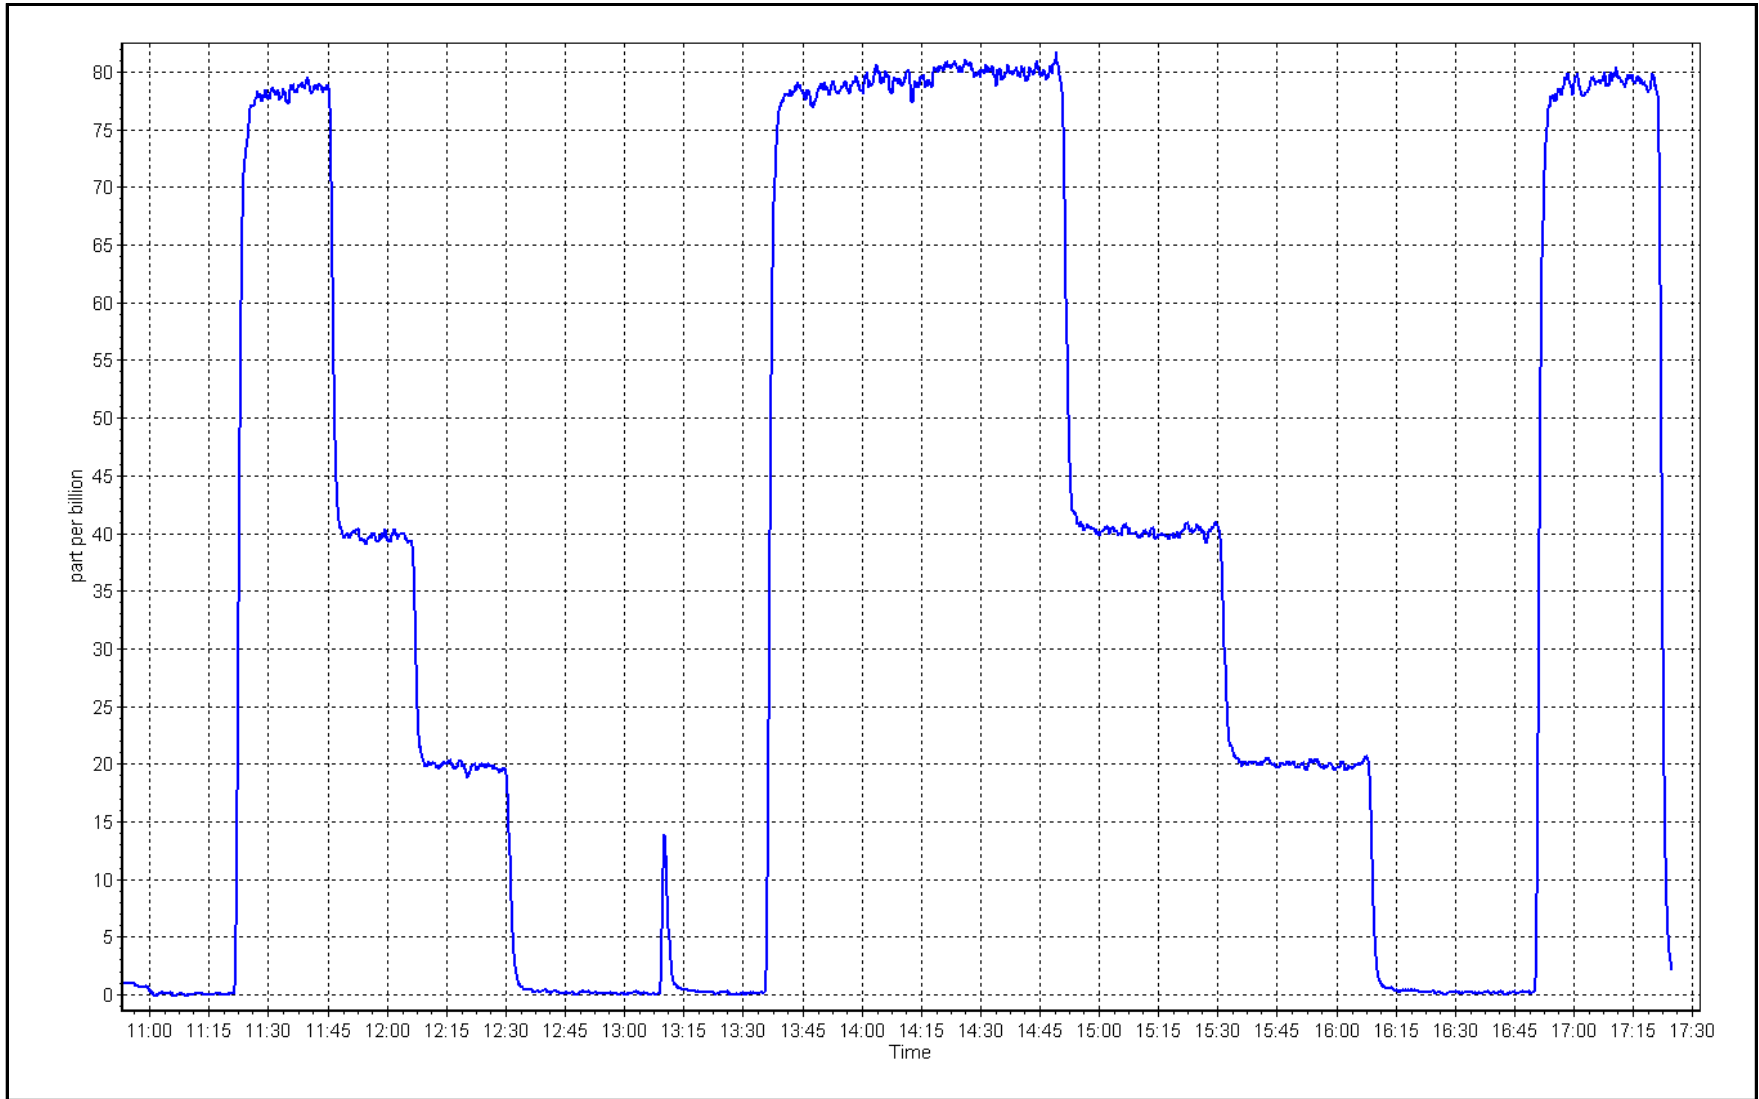



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Bertha Ganter-Fort McKay Station number: AMS01
 Calibration Date: January 10, 2023 Last Cal Date: December 13, 2022
 Start time (MST): 10:53 End time (MST): 17:26
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.10 ppm Cal Gas Exp Date: September 16, 2024
 Cal Gas Cylinder #: CC511749
 Removed Cal Gas Conc: 5.10 ppm Rem Gas Exp Date: N/A
 Removed Gas Cyl #: N/A Diff between cyl:
 Calibrator Make/Model: Teledyne API T700 Serial Number: 3565
 ZAG Make/Model: Teledyne API T701 Serial Number: 5609

Analyzer Information

Analyzer make: Thermo 43iQTL Analyzer serial #: 1200326167
 Converter make: Thermo Converter Converter serial #: N/A
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.997946	0.996946	Backgd or Offset: 1.94	1.94
Calibration intercept:	0.301610	0.161599	Coeff or Slope: 1.014	1.014

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.0	----
as found span	4921	78.4	80.0	79.7	1.003
as found 2nd point	4960	39.2	40.0	40.7	0.983
as found 3rd point	4980	19.6	20.0	20.1	0.995
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.2	----
high point	4921	78.4	80.0	79.9	1.001
second point	4961	39.2	40.0	40.1	0.997
third point	4980	19.6	20.0	20.0	1.000
as left zero	5000	0.0	0.0	0.5	----
as left span	4921	78.4	80.0	78.9	1.014
SO2 Scrubber Check	4919	81.3	813.0	0.0	----
Date of last scrubber change:	March 21, 2022			Ave Corr Factor	0.999
Date of last converter efficiency test:					efficiency

Baseline Corr As found: 79.7 Prev response: 80.11 *% change: -0.5%
 Baseline Corr 2nd AF pt: 40.7 AF Slope: 0.996988 AF Intercept: 0.239990
 Baseline Corr 3rd AF pt: 20.1 AF Correlation: 0.999860

* = > +/-5% change initiates investigation

Notes: Inlet filter change and scrubber check completed after as founds. No adjustments made.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 13, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	10:53	End Time (MST):	17:26
Analyzer make:	Thermo 43iQTL	Analyzer serial #:	1200326167

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999995	≥0.995
80.0	79.9	1.0012			
40.0	40.1	0.9973	Slope	0.996946	0.90 - 1.10
20.0	20.0	0.9999			
			Intercept	0.161599	+/-3

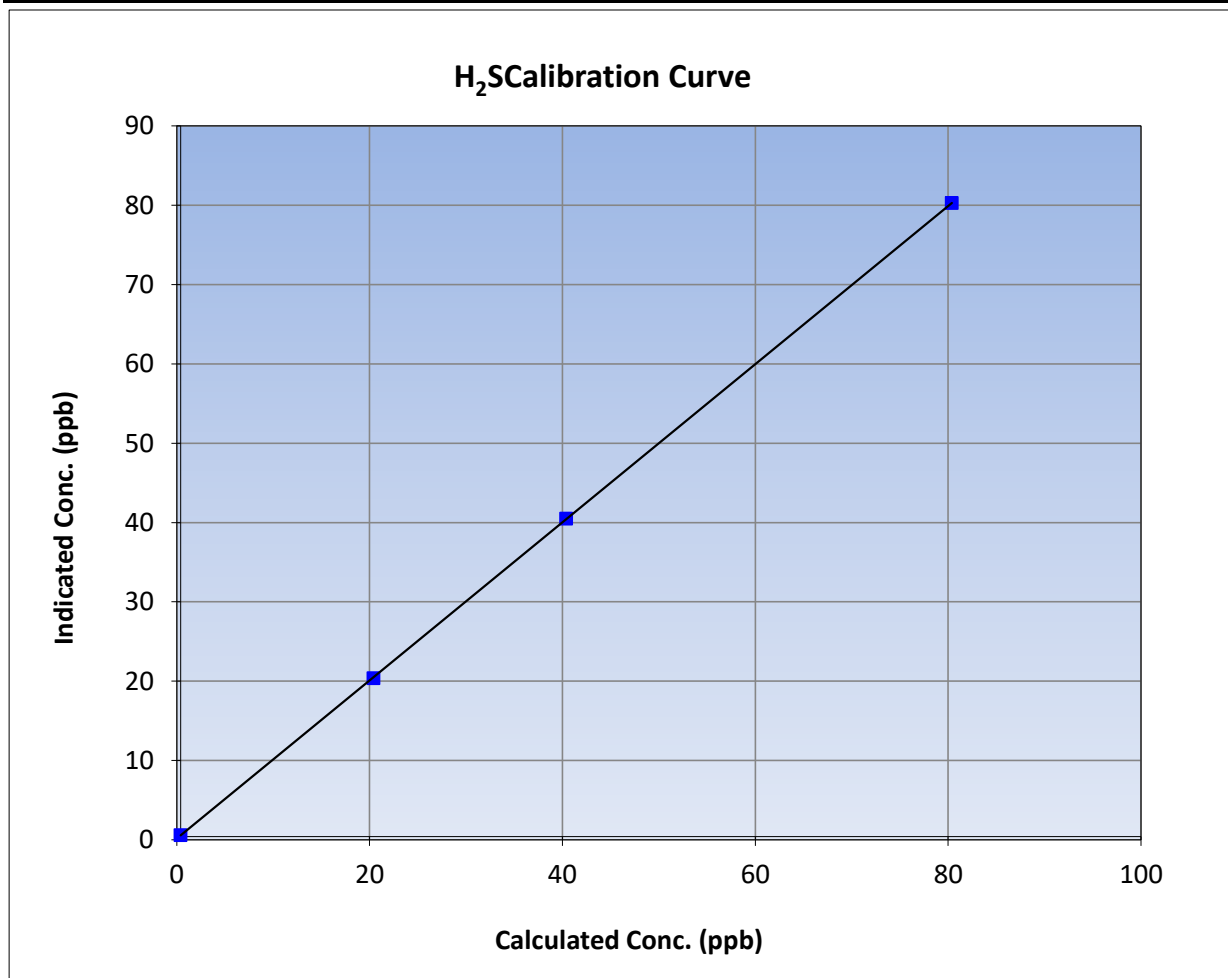

H₂S Calibration Plot

Date: January 10, 2023

Location: Bertha Ganter-Fort McKay

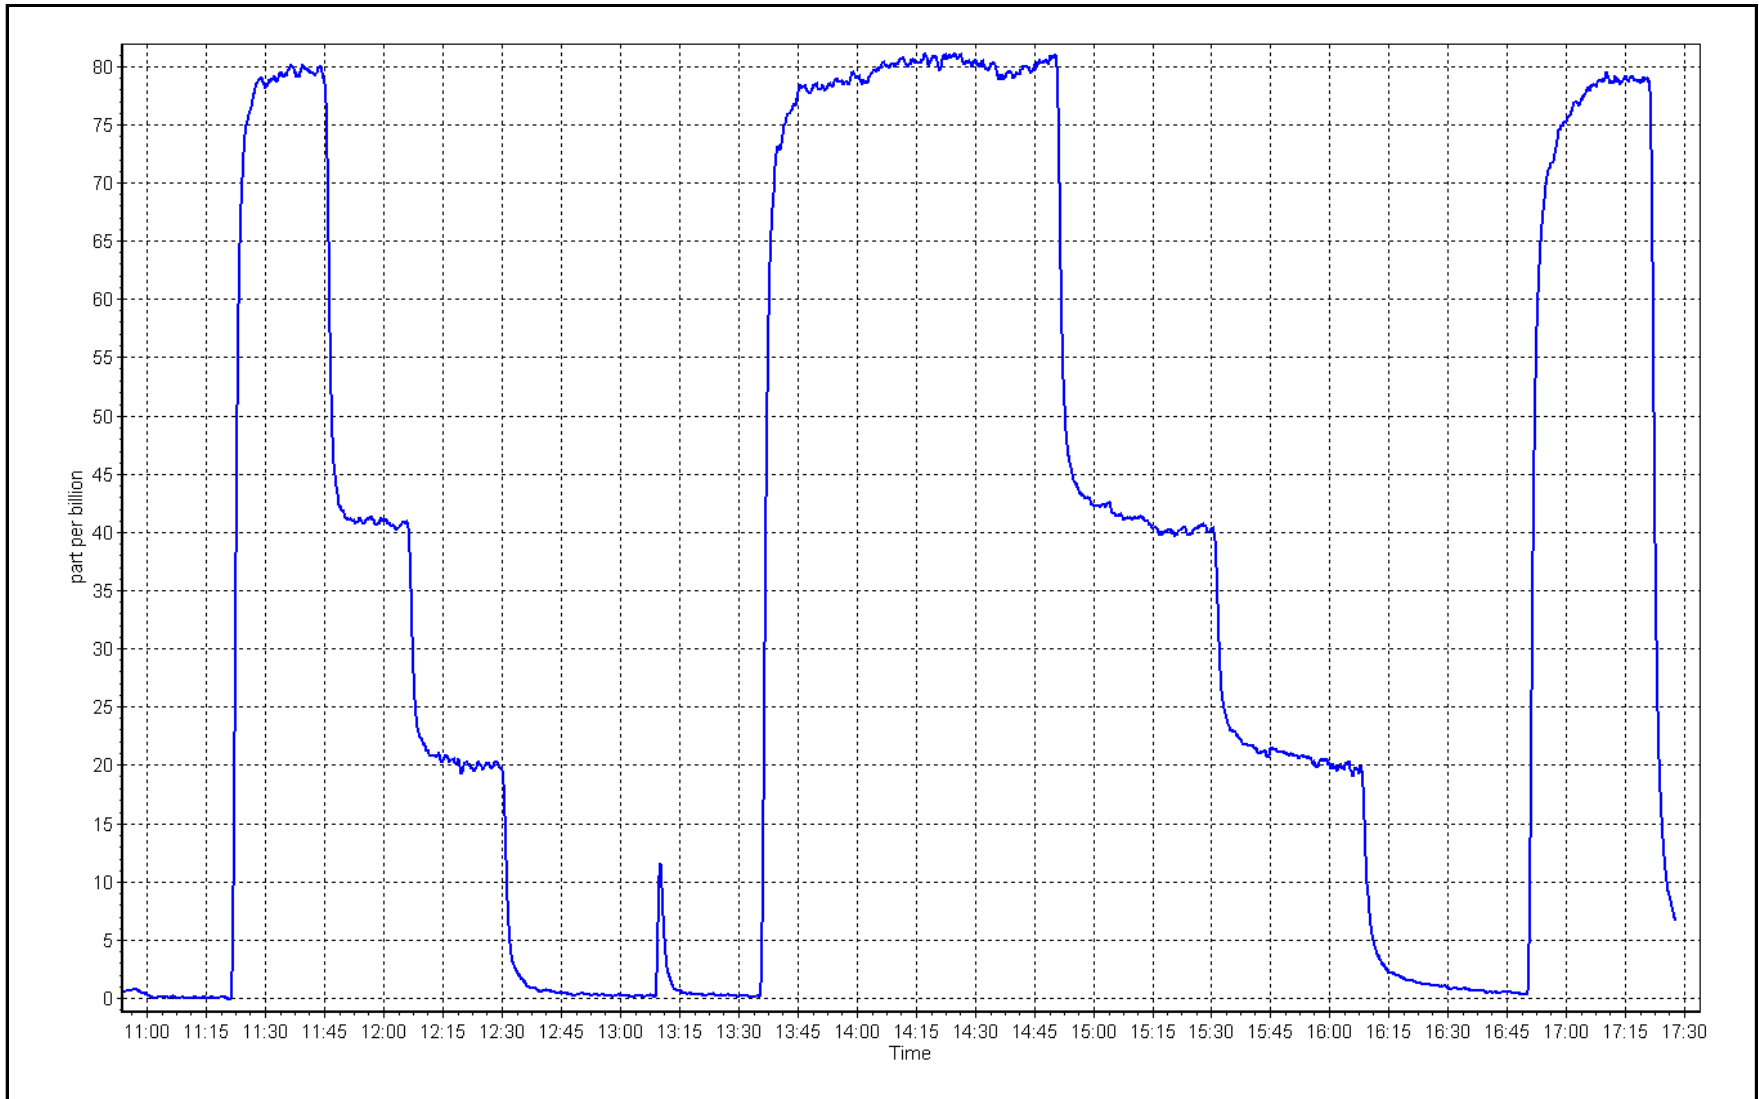



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Bertha Ganter-Fort McKay	Station number:	AMS01
Calibration Date:	January 5, 2023	Last Cal Date:	December 5, 2022
Start time (MST):	11:28	End time (MST):	15:01
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC486642	Cal Gas Expiry Date:	February 23, 2025
CH ₄ Cal Gas Conc.	497.7 ppm	CH ₄ Equiv Conc.	1063.1 ppm
C ₃ H ₈ Cal Gas Conc.	205.6 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	497.7 ppm	CH ₄ Equiv Conc.	1063.1 ppm
Removed C ₃ H ₈ Conc.	205.6 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	Teledyne API T700	Serial Number:	3565
ZAG make/model:	Teledyne API T701	Serial Number:	5609

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1180320040
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	2.50E-04	2.52E-04	NMHC SP Ratio:	5.01E-05
CH ₄ Retention time:	14.4	14.4	NMHC Peak Area:	183290
				179678

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4918	81.3	17.29	17.13	1.010
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4918	81.3	17.29	17.33	0.998
second point	4959	40.7	8.65	8.62	1.004
third point	4979	20.3	4.32	4.33	0.996
as left zero	5000	0.0	0.00	0.00	----
as left span	4918	81.3	17.29	17.40	0.994

Average Correction Factor				0.999
Baseline Corr AF:	17.13	Prev response	17.27	*% change -0.8%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4918	81.3	9.19	9.08	1.012
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4918	81.3	9.19	9.22	0.997
second point	4959	40.7	4.60	4.61	0.999
third point	4979	20.3	2.30	2.32	0.992
as left zero	5000	0	0.00	0.00	----
as left span	4918	81.3	9.19	9.27	0.992
Average Correction Factor					0.996
Baseline Corr AF:	9.08	Prev response	9.18	*% change	-1.1%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4918	81.3	8.09	8.04	1.006
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4918	81.3	8.09	8.11	0.999
second point	4959	40.7	4.05	4.01	1.009
third point	4979	20.3	2.02	2.02	1.002
as left zero	5000	0.0	0.00	0.00	----
as left span	4918	81.3	8.09	8.13	0.996
Average Correction Factor					1.003
Baseline Corr AF:	8.04	Prev response	8.09	*% change	-0.6%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	0.999531	1.001778
THC Cal Offset:	-0.010042	-0.008039
CH ₄ Cal Slope:	1.001390	1.001064
CH ₄ Cal Offset:	-0.012722	-0.011320
NMHC Cal Slope:	0.998342	1.002294
NMHC Cal Offset:	0.002879	0.003480

Notes: Changed the inlet filter after as founds. Adjusted span only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 5, 2023	Previous Calibration:	December 5, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:28	End Time (MST):	15:01
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320040

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999987	≥ 0.995			
17.29	17.33	0.9978						
8.65	8.62	1.0037				Slope	1.001778	0.90 - 1.10
4.32	4.33	0.9965						
			Intercept	-0.008039	± 0.5			

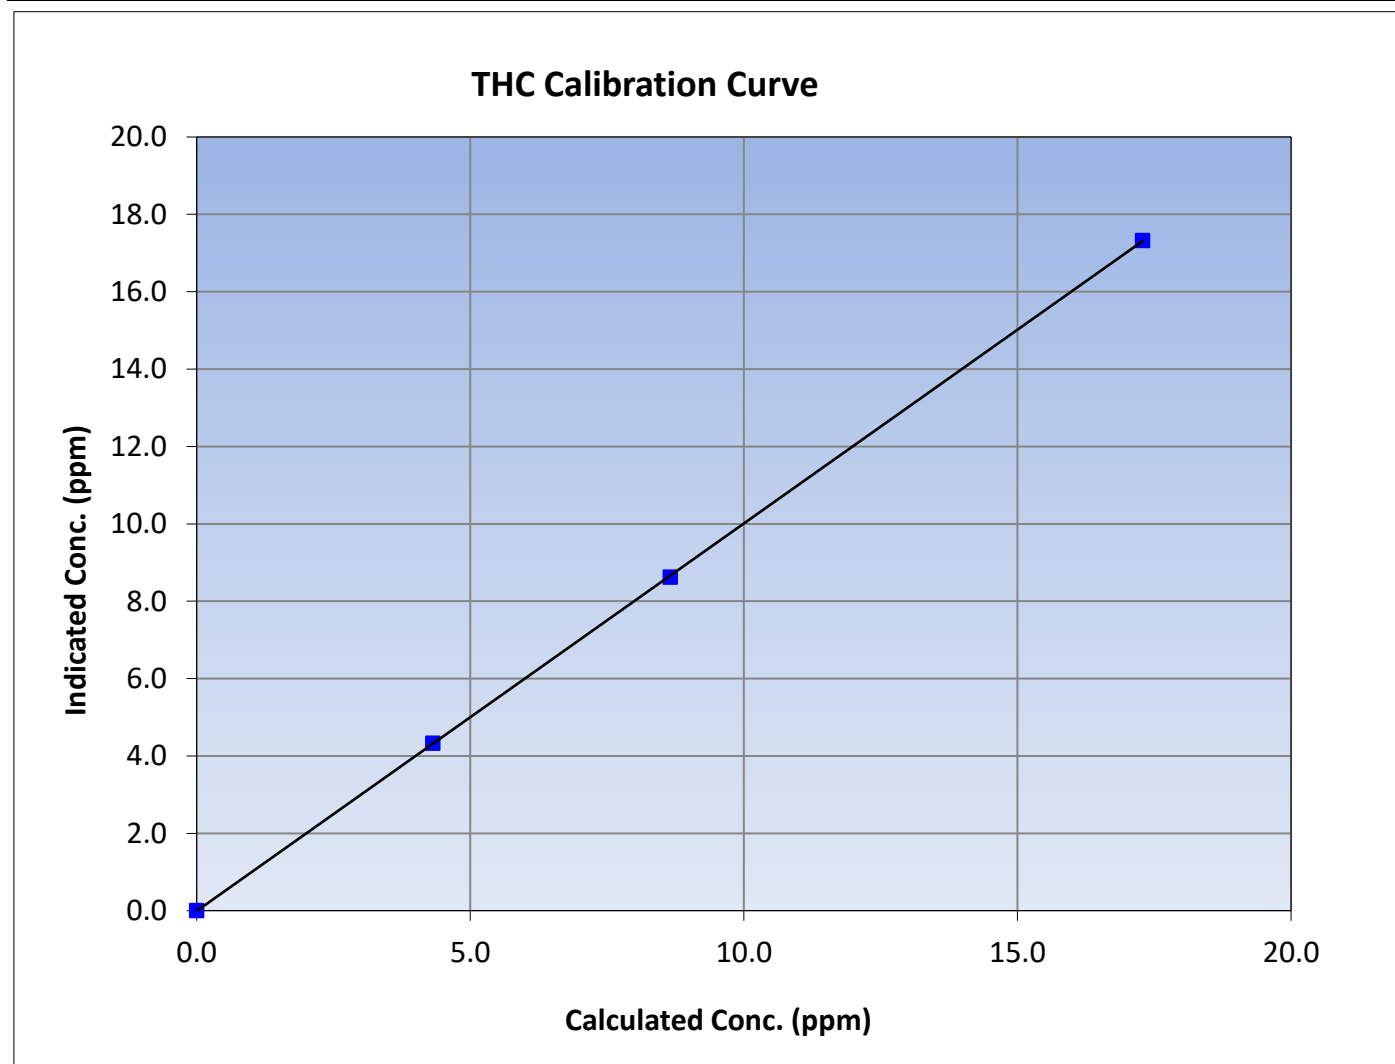



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 5, 2023	Previous Calibration:	December 5, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:28	End Time (MST):	15:01
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320040

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999964	≥ 0.995
8.09	8.11	0.9986			
4.05	4.01	1.0093			
2.02	2.02	1.0020			
			Slope	1.001064	0.90 - 1.10
			Intercept	-0.011320	+/-0.5

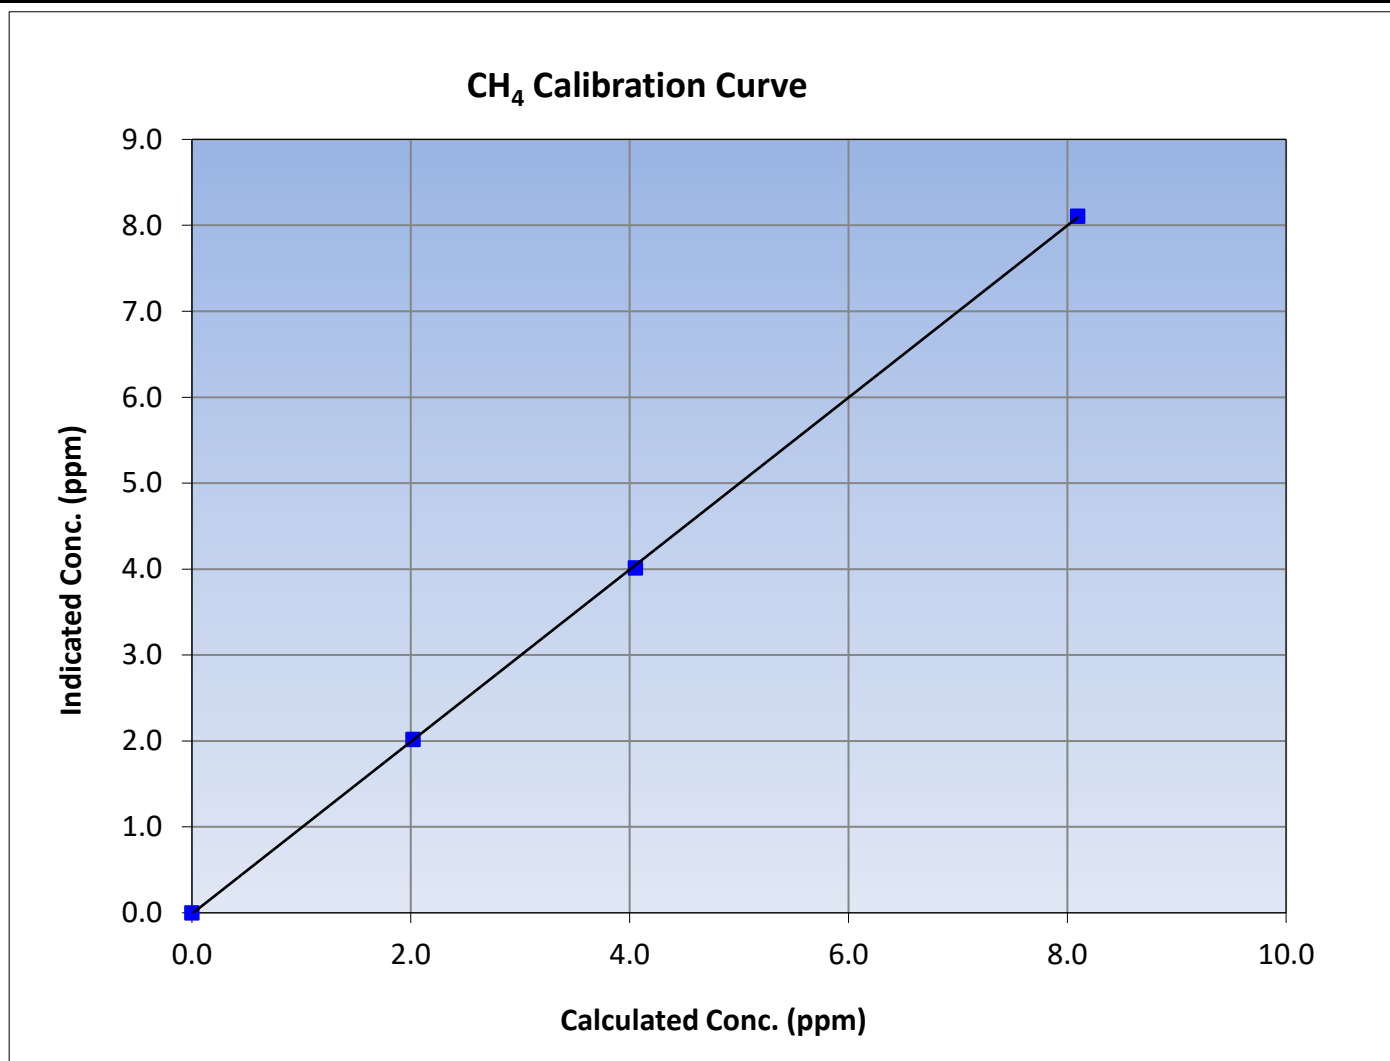



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 5, 2023	Previous Calibration:	December 5, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:28	End Time (MST):	15:01
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320040

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999996	≥ 0.995			
9.19	9.22	0.9971						
4.60	4.61	0.9988				Slope	1.002294	0.90 - 1.10
2.30	2.32	0.9917						
			Intercept	0.003480	± 0.5			

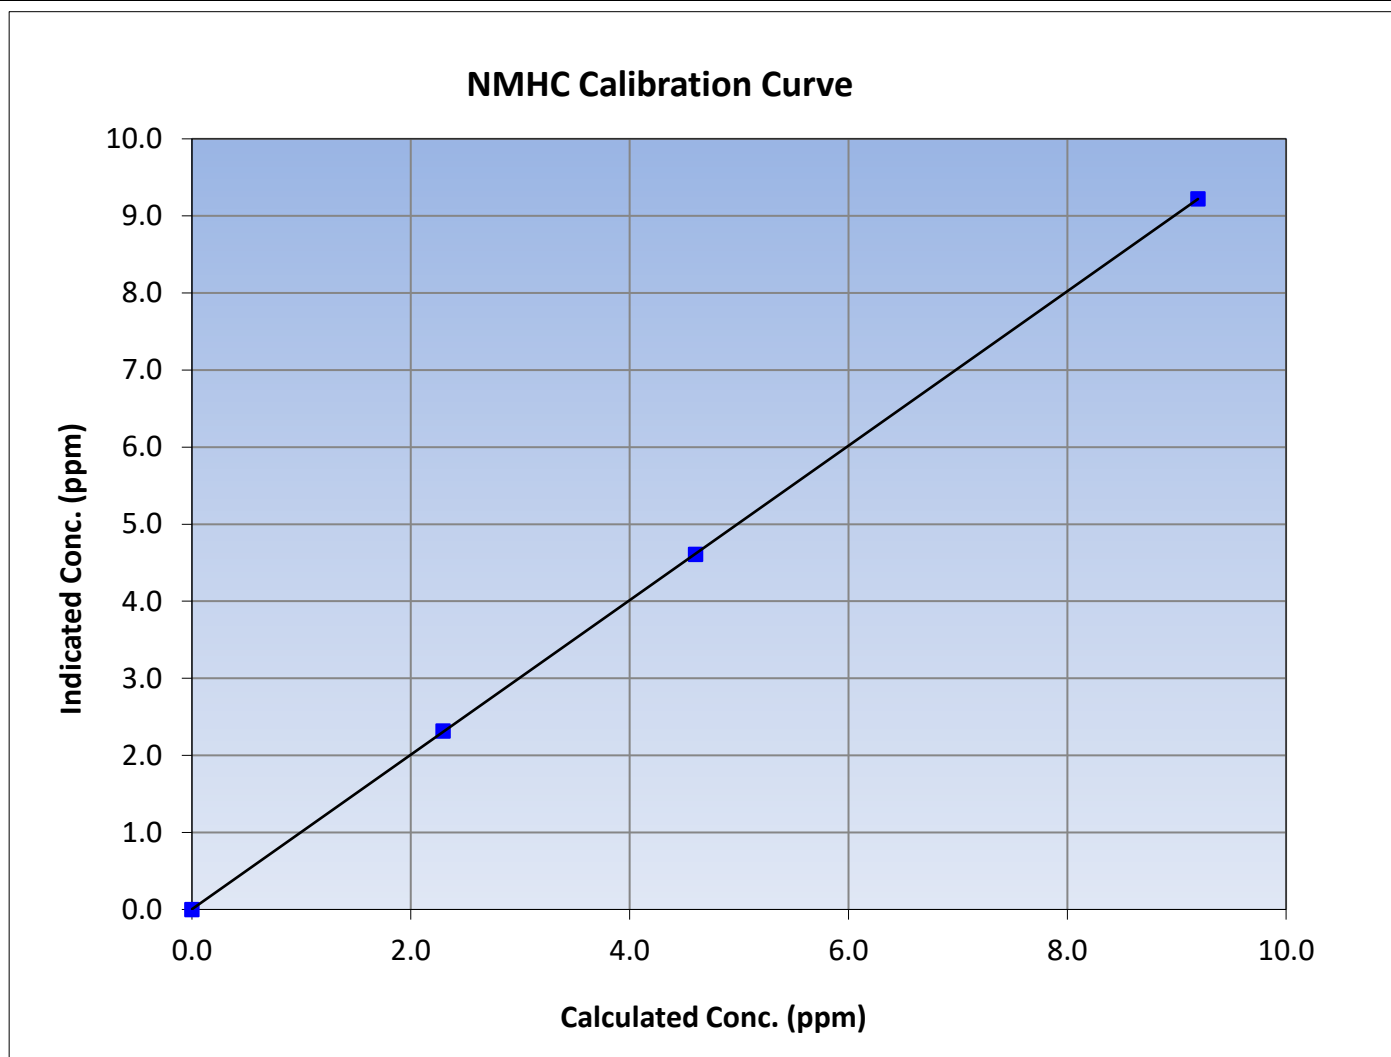

NMHC Calibration Plot

Date: January 5, 2023

Location: Bertha Ganter-Fort McKay

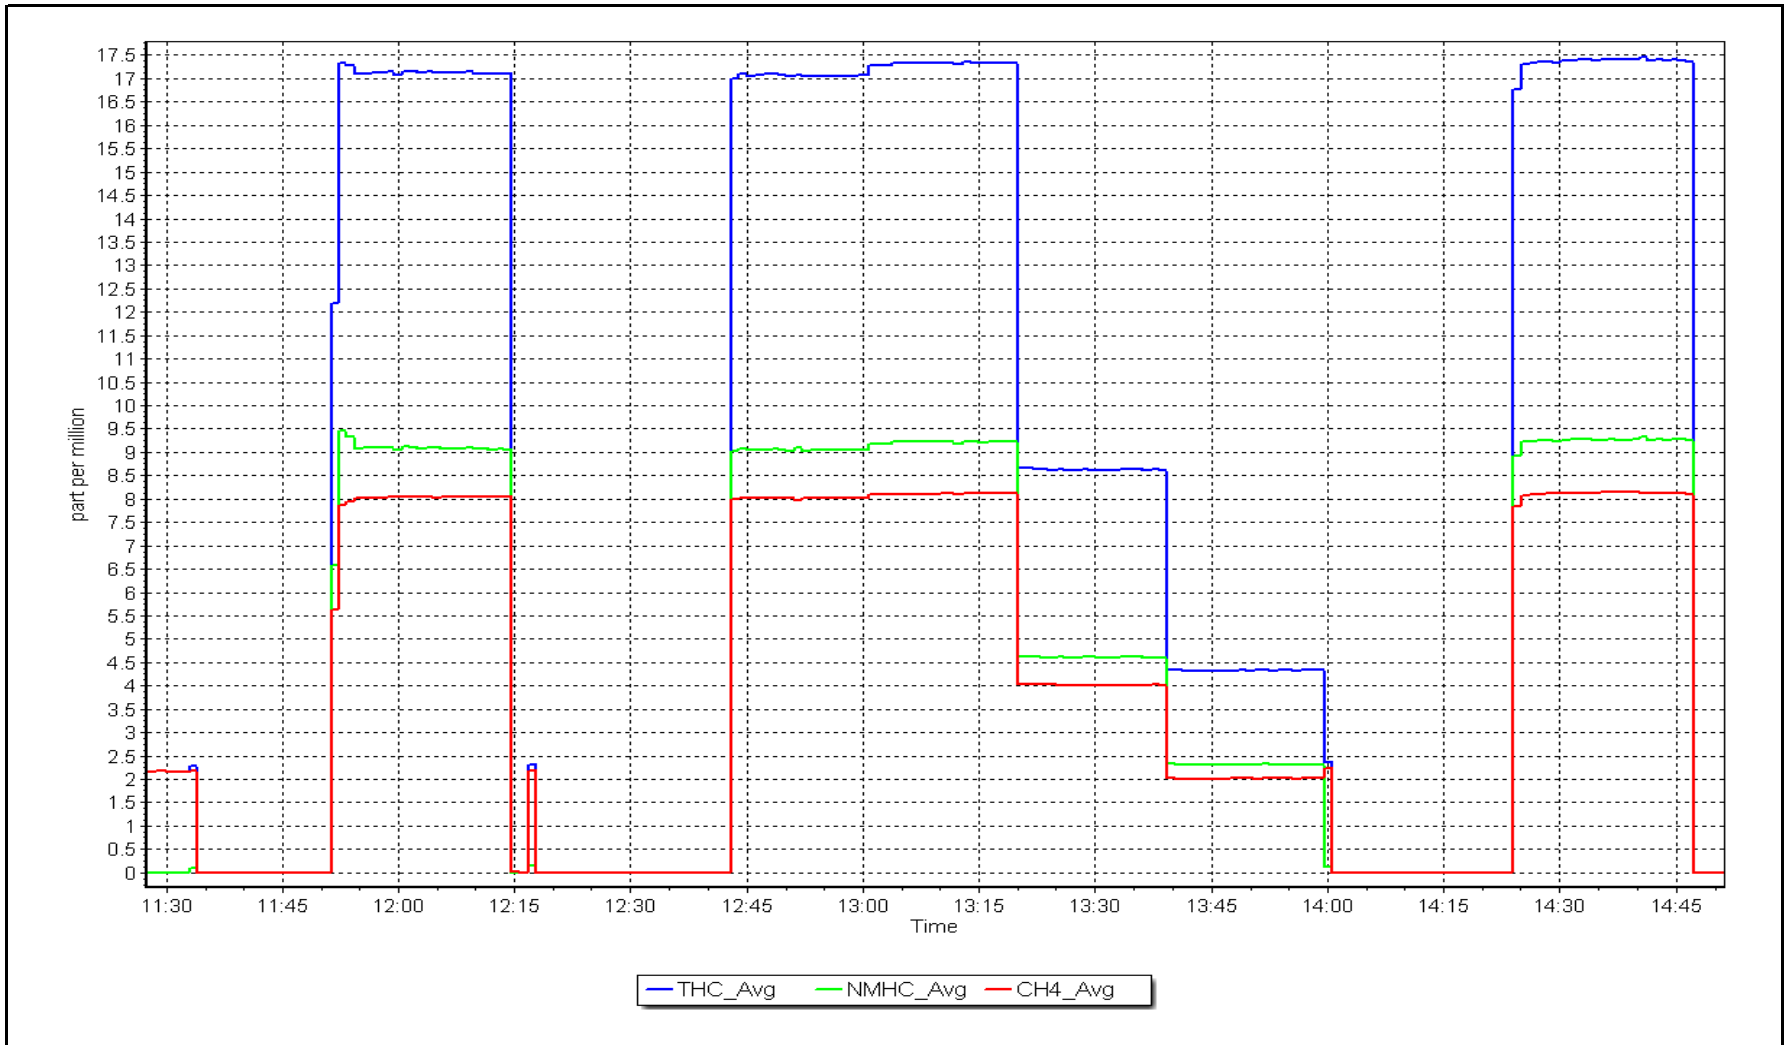



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Bertha Ganter-Fort McKay	Station number:	AMS01
Calibration Date:	January 23, 2023	Last Cal Date:	January 5, 2023
Start time (MST):	11:35	End time (MST):	14:43
Reason:	Cylinder Change		

Calibration Standards

Gas Cert Reference:	CC486642	Cal Gas Expiry Date:	February 23, 2025
CH ₄ Cal Gas Conc.	497.7 ppm	CH ₄ Equiv Conc.	1063.1 ppm
C ₃ H ₈ Cal Gas Conc.	205.6 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	497.7 ppm	CH ₄ Equiv Conc.	1063.1 ppm
Removed C ₃ H ₈ Conc.	205.6 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	Teledyne API T700	Serial Number:	3565
ZAG make/model:	Teledyne API T701	Serial Number:	5609

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1180320040
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	2.52E-04	2.52E-04	NMHC SP Ratio:	5.11E-05
CH ₄ Retention time:	14.4	14.4	NMHC Peak Area:	179678
				5.11E-05
				179678

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4918	81.3	17.29	17.80	0.971
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero					
high point					
second point					
third point					
as left zero	5000	0.0	0.00	0.11	----
as left span	4918	81.3	17.29	18.02	0.960

Average Correction Factor					
Baseline Corr AF:	17.80	Prev response	17.31	*% change	2.8%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4918	81.3	9.19	9.50	0.968
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero					
high point					
second point					
third point					
as left zero	5000	0	0.00	0.00	----
as left span	4918	81.3	9.19	9.50	0.968
Average Correction Factor					
Baseline Corr AF:	9.50	Prev response	9.22	*% change	2.9%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4918	81.3	8.09	8.31	0.974
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero					
high point					
second point					
third point					
as left zero	5000	0.0	0.00	0.11	----
as left span	4918	81.3	8.09	8.52	0.950
Average Correction Factor					
Baseline Corr AF:	8.31	Prev response	8.09	*% change	2.6%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
THC Cal Slope:	1.001778	
THC Cal Offset:	-0.008039	
CH ₄ Cal Slope:	1.001064	
CH ₄ Cal Offset:	-0.011320	
NMHC Cal Slope:	1.002294	
NMHC Cal Offset:	0.003480	


Notes: Swapping out the H2 cylinder. Cylinder was contaminated, swapped the old cylinder back in.

Calibration Performed By: Rene Chamberland

NMHC Calibration Plot

Date: January 23, 2023

Location: Bertha Ganter-Fort McKay

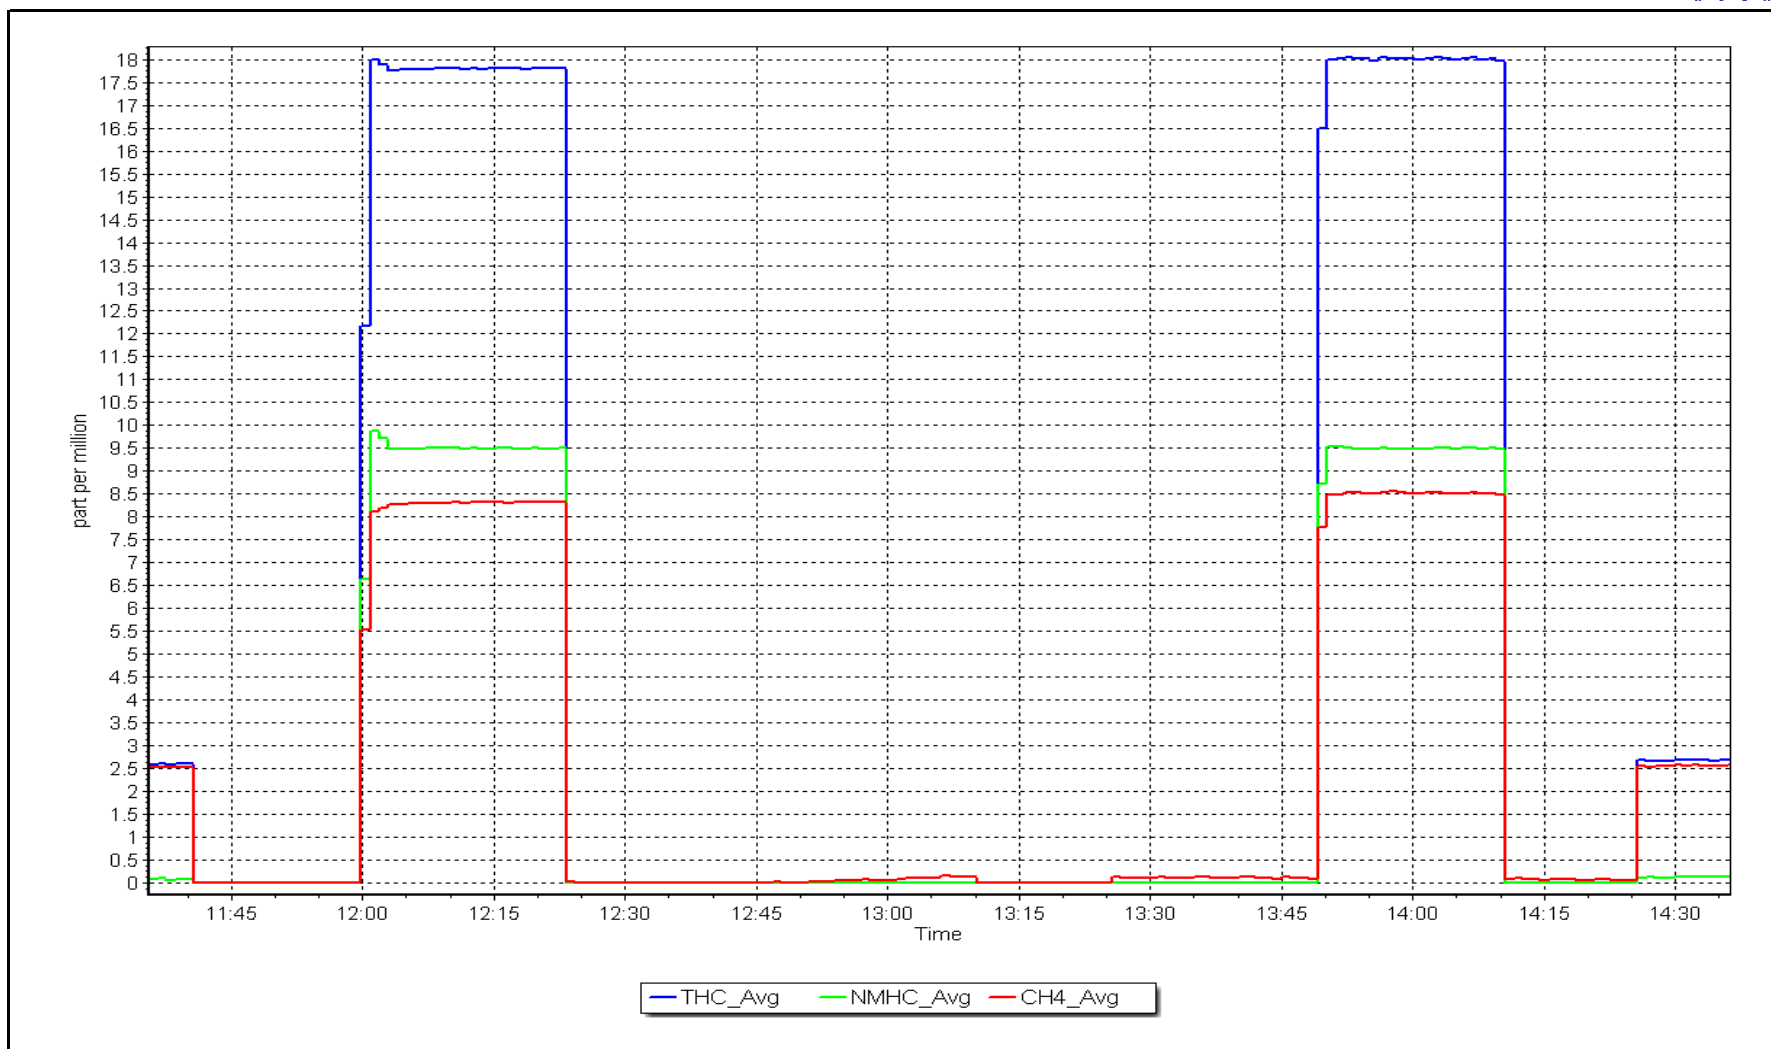



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Bertha Ganter-Fort McKay	Station number:	AMS01
Calibration Date:	January 24, 2023	Last Cal Date:	January 5, 2023
Start time (MST):	11:32	End time (MST):	15:20
Reason:	Cylinder Change		

Calibration Standards

Gas Cert Reference:	CC486642	Cal Gas Expiry Date:	February 23, 2025
CH ₄ Cal Gas Conc.	497.7 ppm	CH ₄ Equiv Conc.	1063.1 ppm
C ₃ H ₈ Cal Gas Conc.	205.6 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	497.7 ppm	CH ₄ Equiv Conc.	1063.1 ppm
Removed C ₃ H ₈ Conc.	205.6 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	Teledyne API T700	Serial Number:	3565
ZAG make/model:	Teledyne API T701	Serial Number:	5609

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1180320040
THC Range (ppm):	0 - 20 ppm	CH ₄ Range (ppm):	0 - 10 ppm
NMHC Range (ppm):	0 - 10 ppm		

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	2.52E-04	2.54E-04	NMHC SP Ratio:	5.11E-05
CH ₄ Retention time:	14.4	14.4	NMHC Peak Area:	179678
				179761

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero					
as found span					
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.02	----
high point	4918	81.3	17.29	17.30	1.000
second point	4959	40.7	8.65	8.63	1.003
third point	4980	20.3	4.32	4.32	0.999
as left zero	5000	0.0	0.00	0.01	----
as left span	4918	81.3	17.29	17.29	1.000

				Average Correction Factor	1.001
Baseline Corr AF:	NA	Prev response	NA	*% change	NA
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero					
as found span					
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4918	81.3	9.19	9.20	1.000
second point	4959	40.7	4.60	4.60	1.000
third point	4980	20.3	2.30	2.31	0.995
as left zero	5000	0	0.00	0.00	----
as left span	4918	81.3	9.19	9.22	0.998
Average Correction Factor					0.998
Baseline Corr AF:	NA	Prev response	NA	*% change	NA
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero					
as found span					
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.02	----
high point	4918	81.3	8.09	8.10	0.999
second point	4959	40.7	4.05	4.03	1.006
third point	4980	20.3	2.02	2.01	1.005
as left zero	5000	0.0	0.00	0.01	----
as left span	4918	81.3	8.09	8.07	1.003
Average Correction Factor					1.003
Baseline Corr AF:	NA	Prev response	NA	*% change	NA
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	1.001778	0.999160
THC Cal Offset:	-0.008039	0.008295
CH ₄ Cal Slope:	1.001064	0.998842
CH ₄ Cal Offset:	-0.011320	0.003433
NMHC Cal Slope:	1.002294	0.999663
NMHC Cal Offset:	0.003480	0.004462

Notes: As founds not completed because the flame was out. Swapping out the H2 cylinder. Enabled the "use zero chromatogram" option. Adjusted span only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	January 5, 2023
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:32	End Time (MST):	15:20
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320040

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.02	----	Correlation Coefficient	0.999993	≥ 0.995			
17.29	17.30	0.9996						
8.65	8.63	1.0030				Slope	0.999160	0.90 - 1.10
4.32	4.32	0.9993						
			Intercept	0.008295	± 0.5			

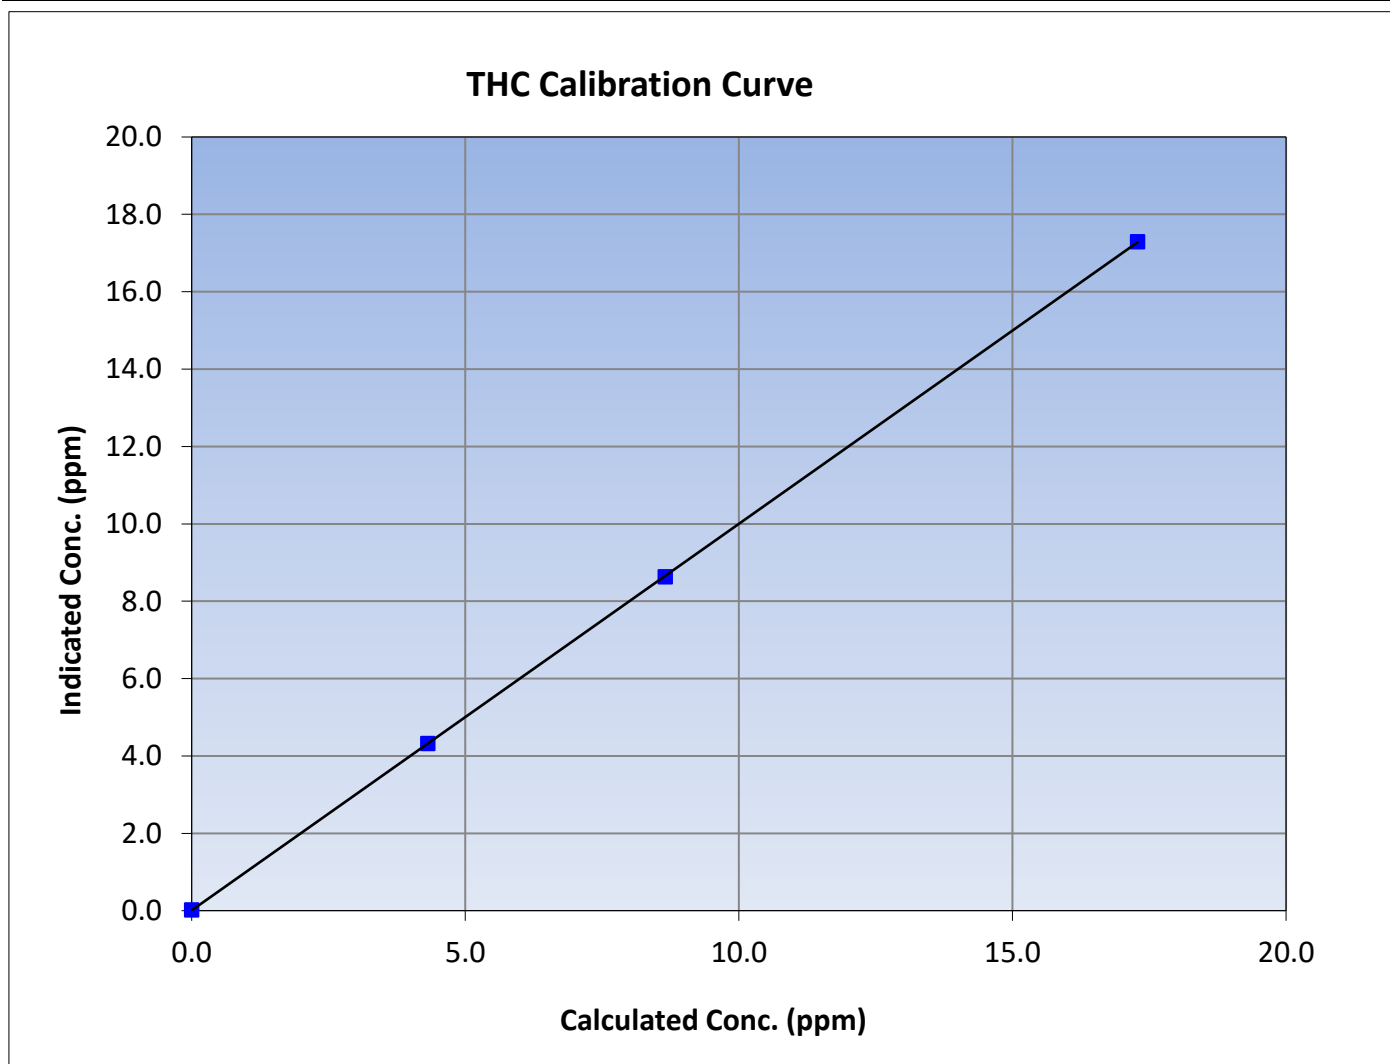



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	January 5, 2023
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:32	End Time (MST):	15:20
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320040

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.02	----	Correlation Coefficient	0.999966	≥ 0.995			
8.09	8.10	0.9990						
4.05	4.03	1.0060				Slope	0.998842	0.90 - 1.10
2.02	2.01	1.0048						
			Intercept	0.003433	± 0.5			

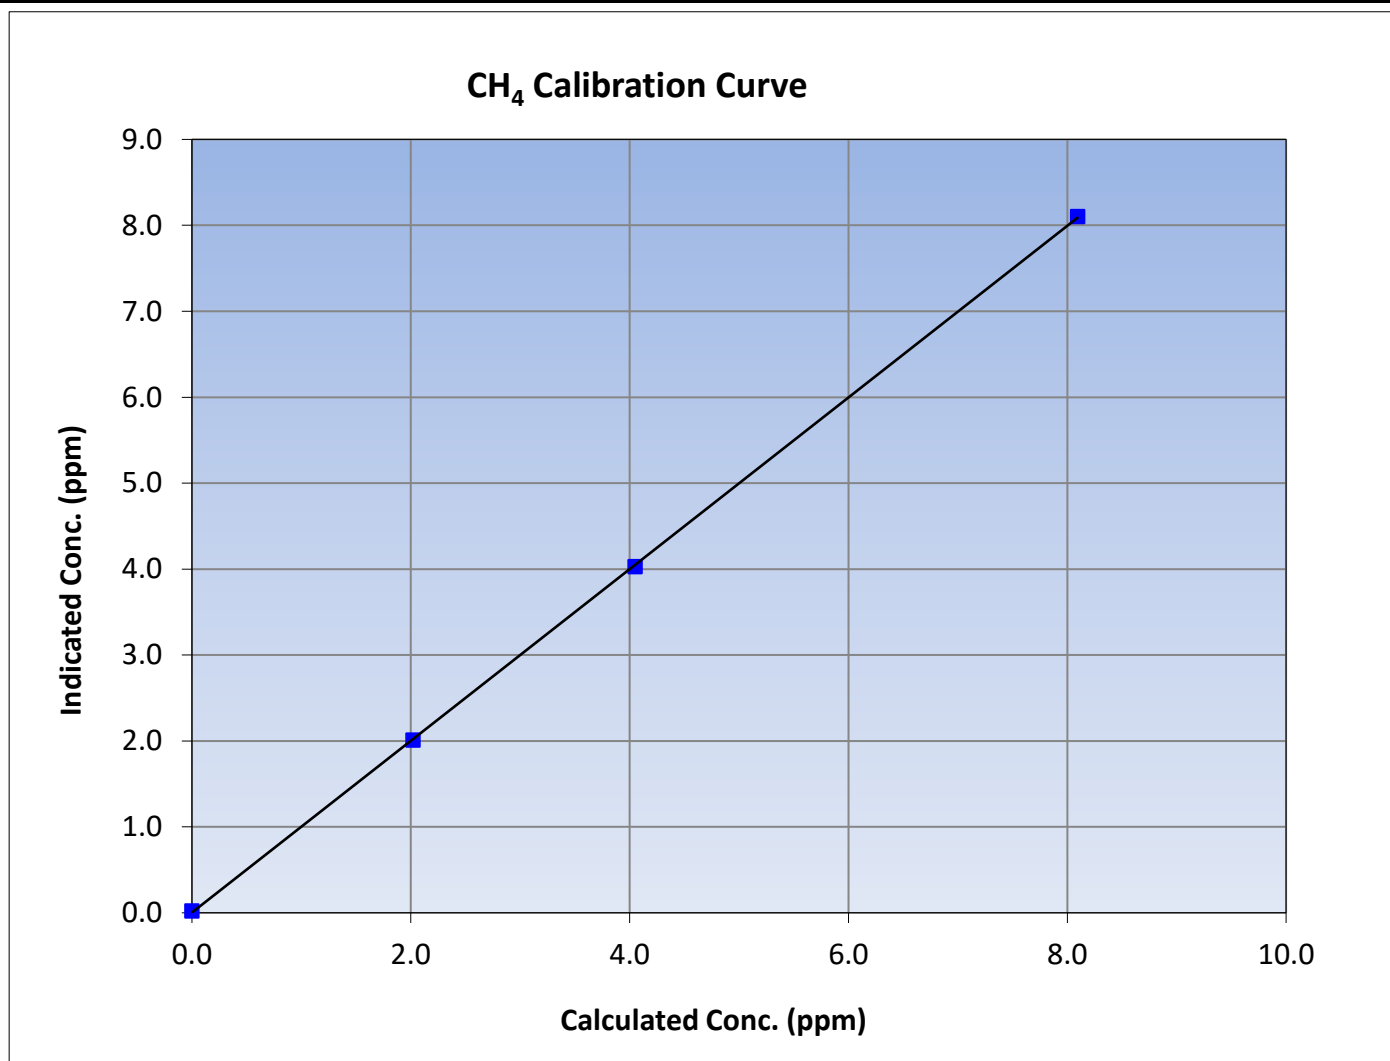



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	January 5, 2023
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:32	End Time (MST):	15:20
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320040

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999998	≥ 0.995			
9.19	9.20	0.9999						
4.60	4.60	1.0003				Slope	0.999663	0.90 - 1.10
2.30	2.31	0.9946						
			Intercept	0.004462	± 0.5			

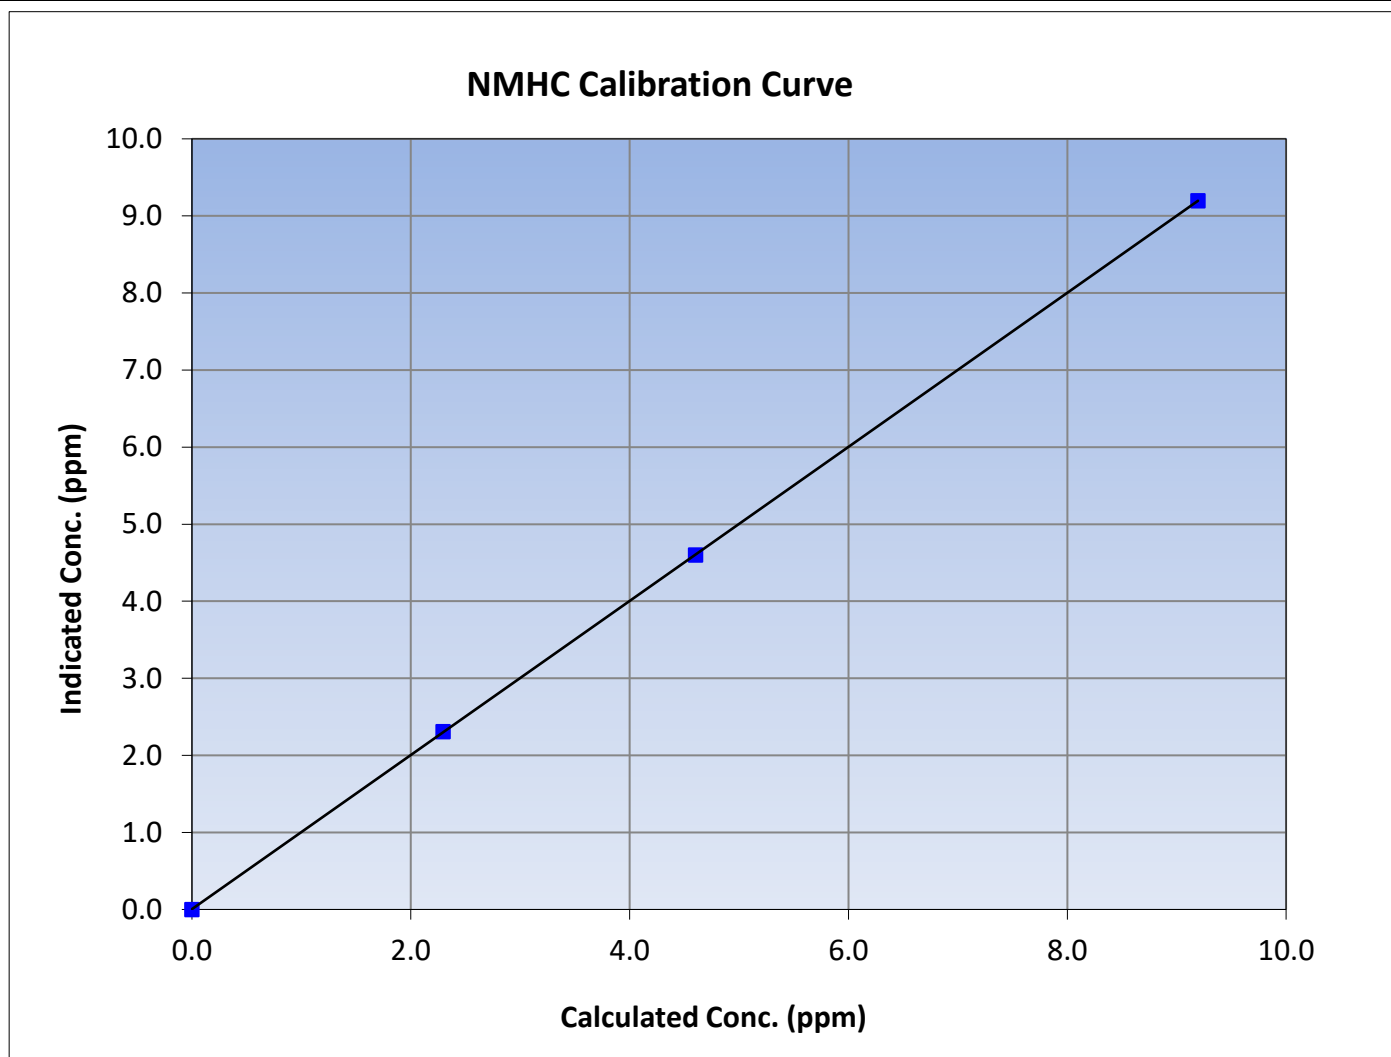

NMHC Calibration Plot

Date: January 24, 2023

Location: Bertha Ganter-Fort McKay

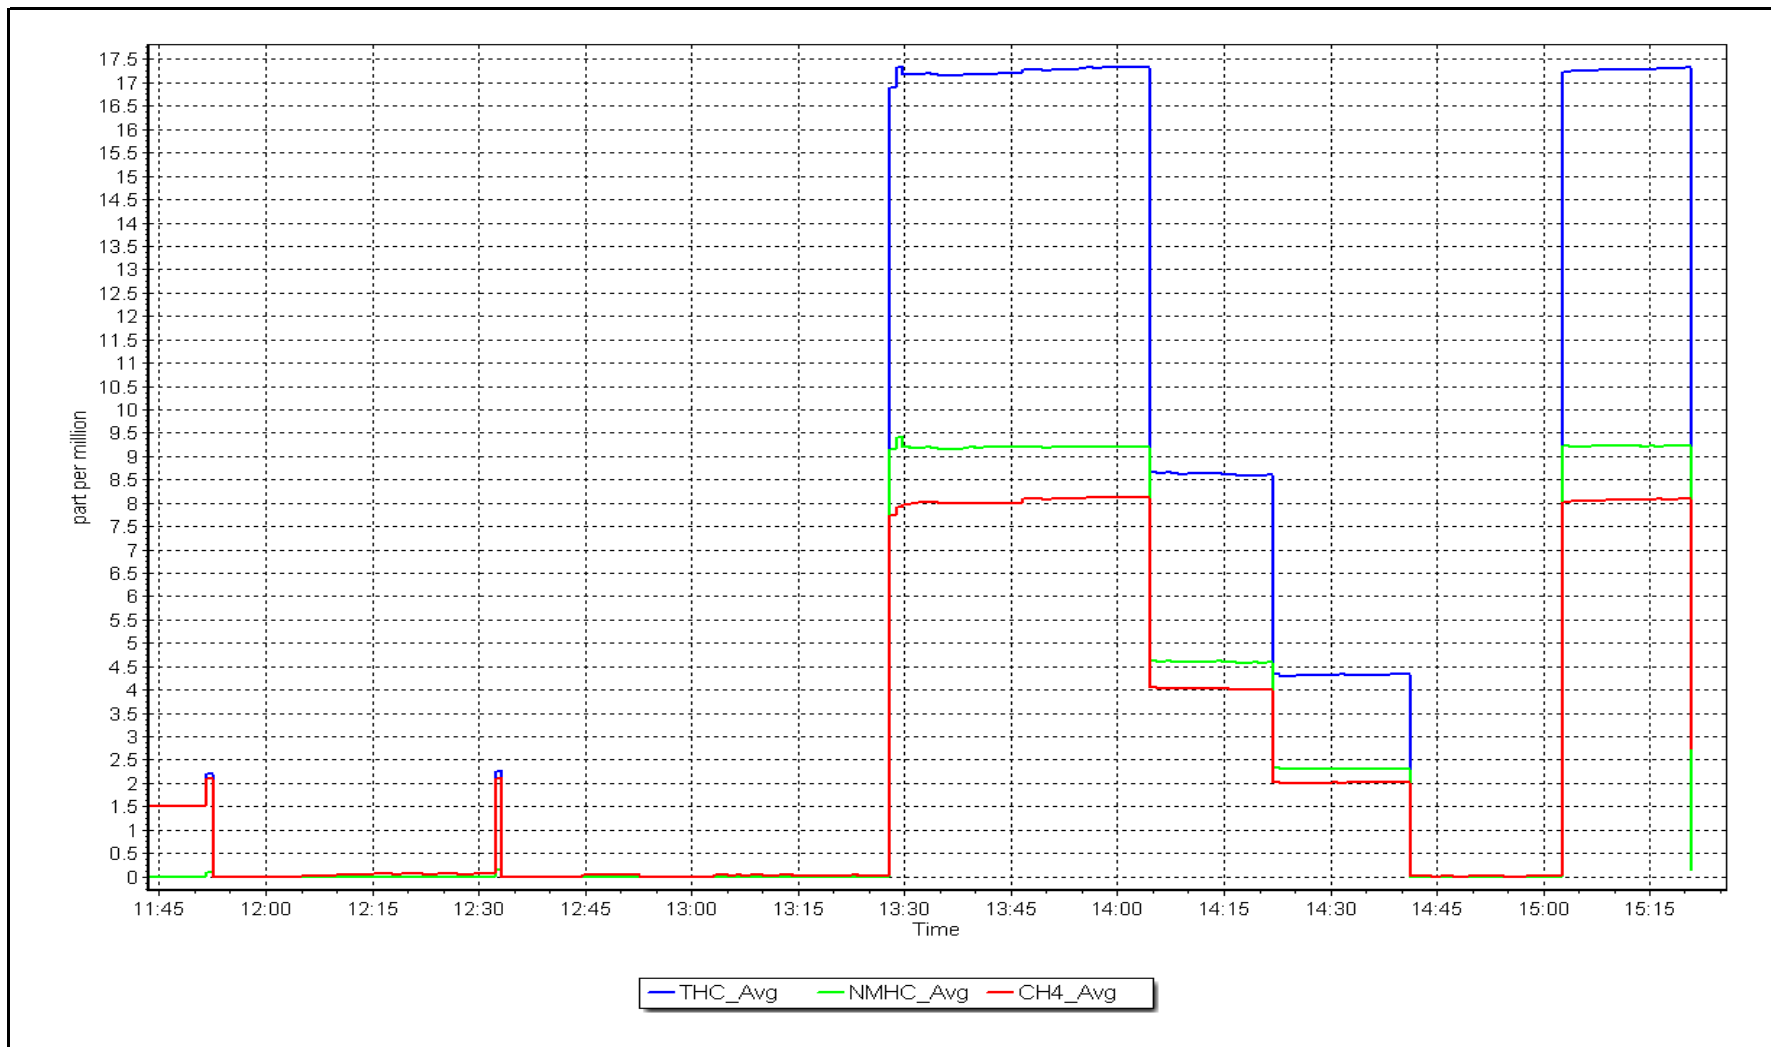



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Bertha Ganter-Fort McKay Station number: AMS01
Calibration Date: January 6, 2023 Last Cal Date: December 19, 2022
Start time (MST): 11:13 End time (MST): 16:15
Reason: Routine

Calibration Standards

NO Gas Cylinder #: T2Y1P9L Cal Gas Expiry Date: December 11, 2023
NOX Cal Gas Conc: 50.84 ppm NO Cal Gas Conc: 50.04 ppm
Removed Cylinder #: NA Removed Gas Exp Date: NA
Removed Gas NOX Conc: 50.84 ppm Removed Gas NO Conc: 50.04 ppm
NOX gas Diff: NO gas Diff:
Calibrator Model: Teledyne API T700 Serial Number: 3565
ZAG make/model: Teledyne API T701 Serial Number: 5609

Analyzer Information

Analyzer make: Thermo 42i Analyzer serial #: 1218153357
NOX Range (ppb): 0 - 1000 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.432	1.453	NO bkgnd or offset:	6.7	6.9
NOX coeff or slope:	0.999	0.990	NOX bkgnd or offset:	6.9	7.0
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	195.4	195.4

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	0.999185	0.999269
NO _x Cal Offset:	-0.340000	-0.220000
NO Cal Slope:	1.000128	1.000842
NO Cal Offset:	-1.100000	-0.900000
NO ₂ Cal Slope:	0.999271	0.996966
NO ₂ Cal Offset:	0.358702	-0.078101



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.0	0.1	-0.1	----	----
as found span	4920	80.0	813.4	800.6	12.8	803.2	789.2	14.0	1.0127	1.0145
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.4	0.3	0.1	----	----
high point	4920	80.0	813.4	800.6	12.8	812.9	800.8	12.3	1.0007	0.9998
second point	4960	40.0	406.7	400.3	6.4	406.0	399.8	6.2	1.0018	1.0013
third point	4980	20.0	203.4	200.2	3.2	202.3	197.8	4.5	1.0052	1.0119
as left zero	5000	0.0	0.0	0.0	0.0	0.5	0.2	0.4	----	----
as left span	4920	80.0	813.4	400.3	413.1	810.3	389.8	420.6	1.0039	1.0270
Average Correction Factor									1.0026	1.0043

Corrected As found	NO _x = 803.2 ppb	NO = 789.1 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -1.2%	
Previous Response	NO _x = 812.4 ppb	NO = 799.6 ppb		*Percent Change	NO = -1.3%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO ₂)						
as found GPT point (200 ppb NO ₂)						
as found GPT point (100 ppb NO ₂)						
1st GPT point (400 ppb O ₃)	797.6	397.3	413.1	412.0	1.0027	99.7%
2nd GPT point (200 ppb O ₃)	797.6	584.2	226.2	225.0	1.0053	99.5%
3rd GPT point (100 ppb O ₃)	797.6	695.6	114.8	114.4	1.0035	99.7%
Average Correction Factor					1.0038	99.6%

Notes: Changed the inlet filter after as founds. Adjusted span only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 6, 2023	Previous Calibration:	December 19, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:13	End Time (MST):	16:15
Analyzer make:	Thermo 42i	Analyzer serial #:	1218153357

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.4	----	Correlation Coefficient	≥0.995	
813.4	812.9	1.0007			
406.7	406.0	1.0018			
203.4	202.3	1.0052			
			Slope	0.999269	0.90 - 1.10
			Intercept	-0.220000	+/-20

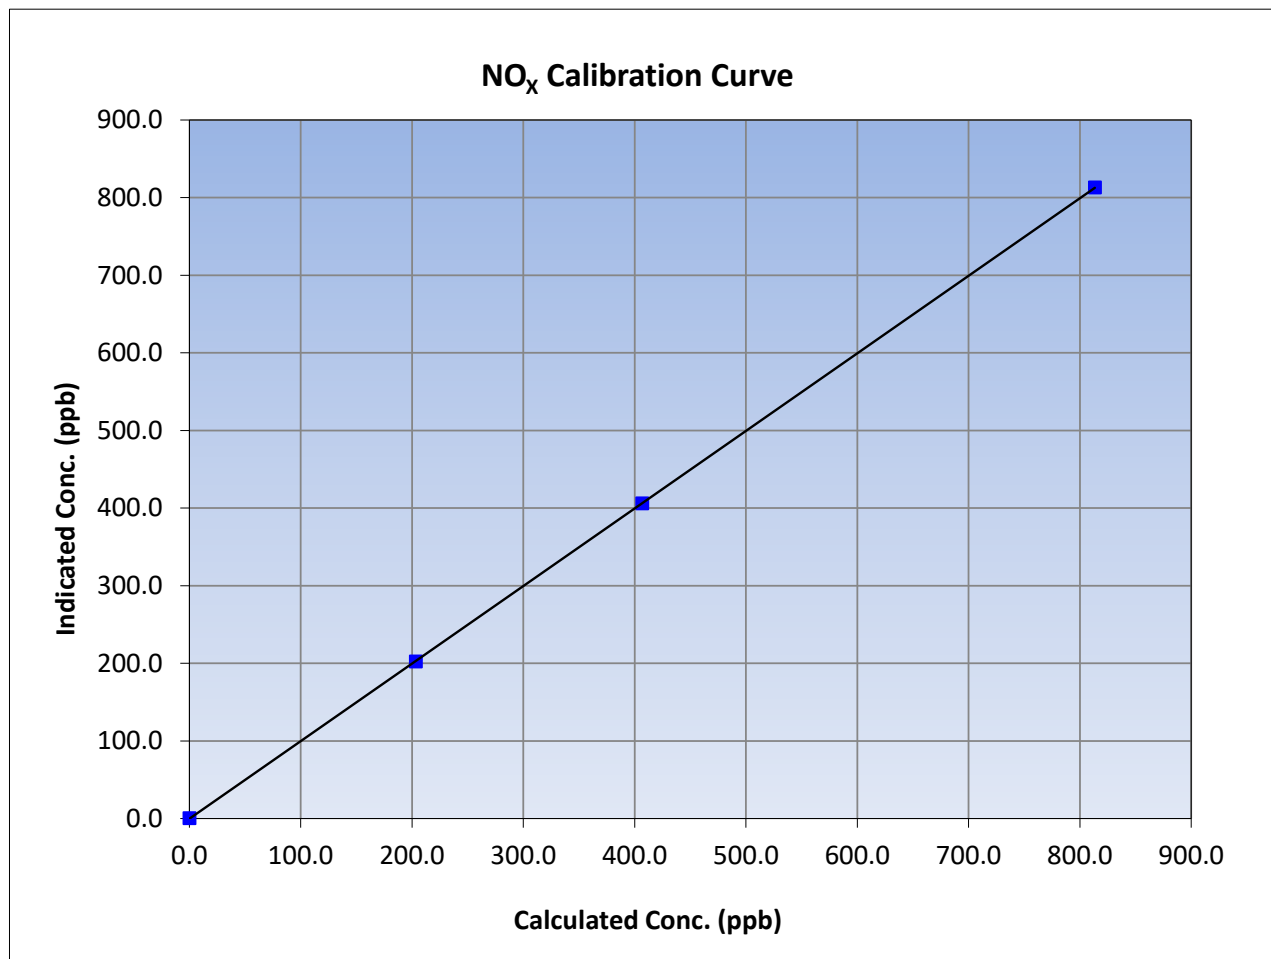



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 6, 2023	Previous Calibration:	December 19, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:13	End Time (MST):	16:15
Analyzer make:	Thermo 42i	Analyzer serial #:	1218153357

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.3	----	Correlation Coefficient	0.999988	≥0.995
800.6	800.8	0.9998			
400.3	399.8	1.0013	Slope	1.000842	0.90 - 1.10
200.2	197.8	1.0119			
			Intercept	-0.900000	+/-20

NO Calibration Curve

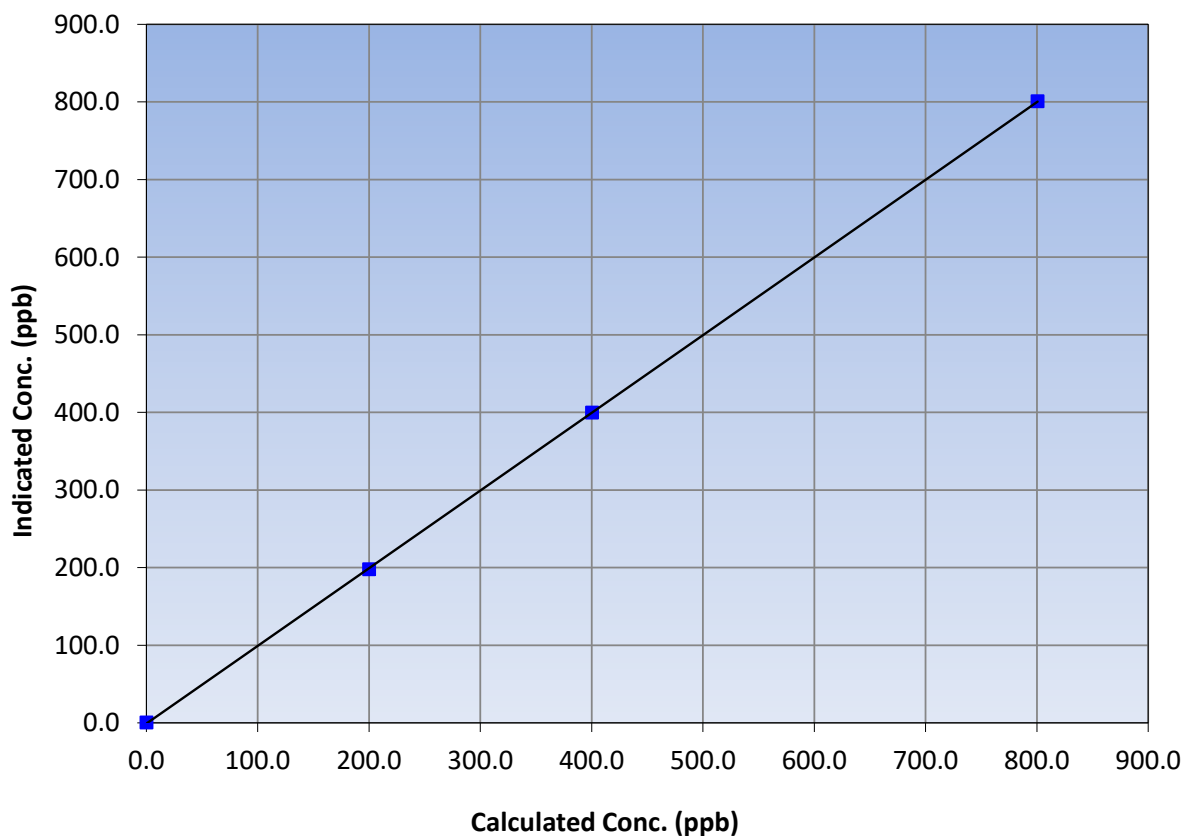



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 6, 2023	Previous Calibration:	December 19, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:13	End Time (MST):	16:15
Analyzer make:	Thermo 42i	Analyzer serial #:	1218153357

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.1	----	Correlation Coefficient	≥0.995	
413.1	412.0	1.0027			
226.2	225.0	1.0053			
114.8	114.4	1.0035			
			Slope	0.996966	0.90 - 1.10
			Intercept	-0.078101	+/-20


NO₂ Calibration Curve

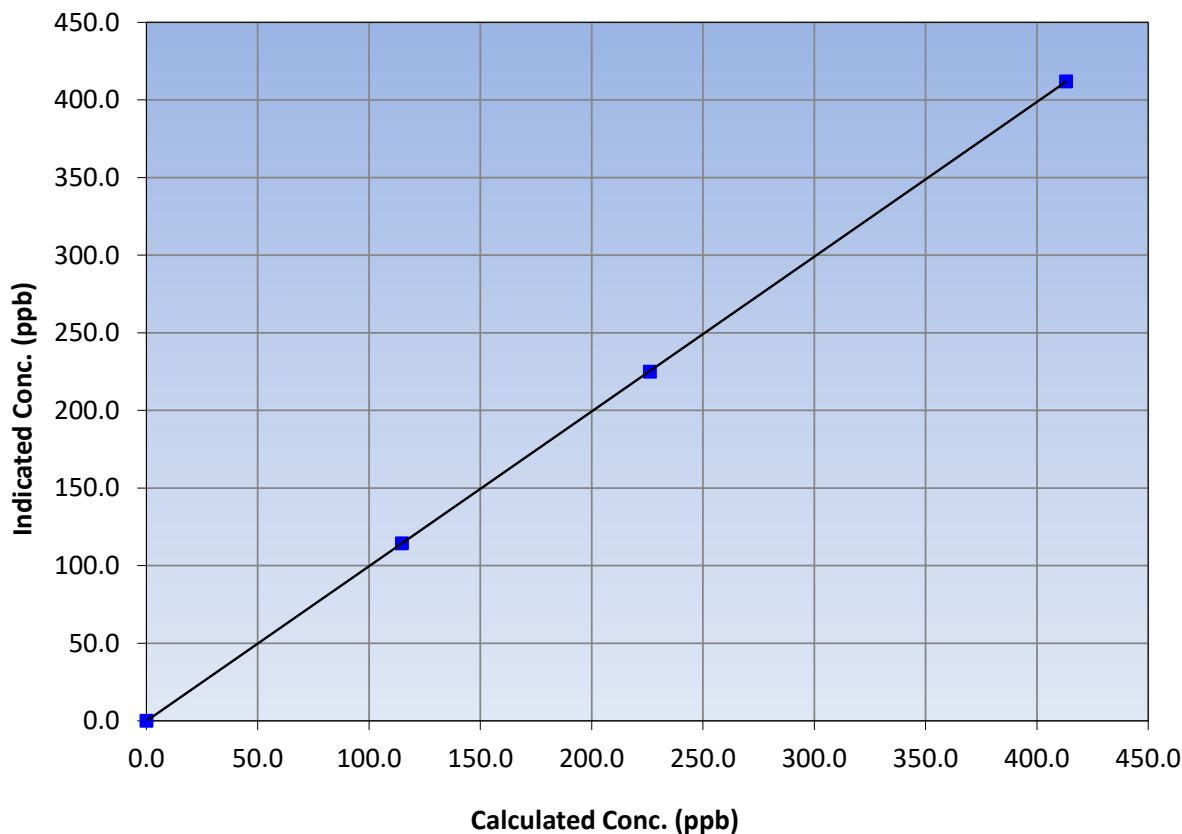

NO_x Calibration Plot

Date: January 6, 2023

Location: Bertha Ganter-Fort McKay

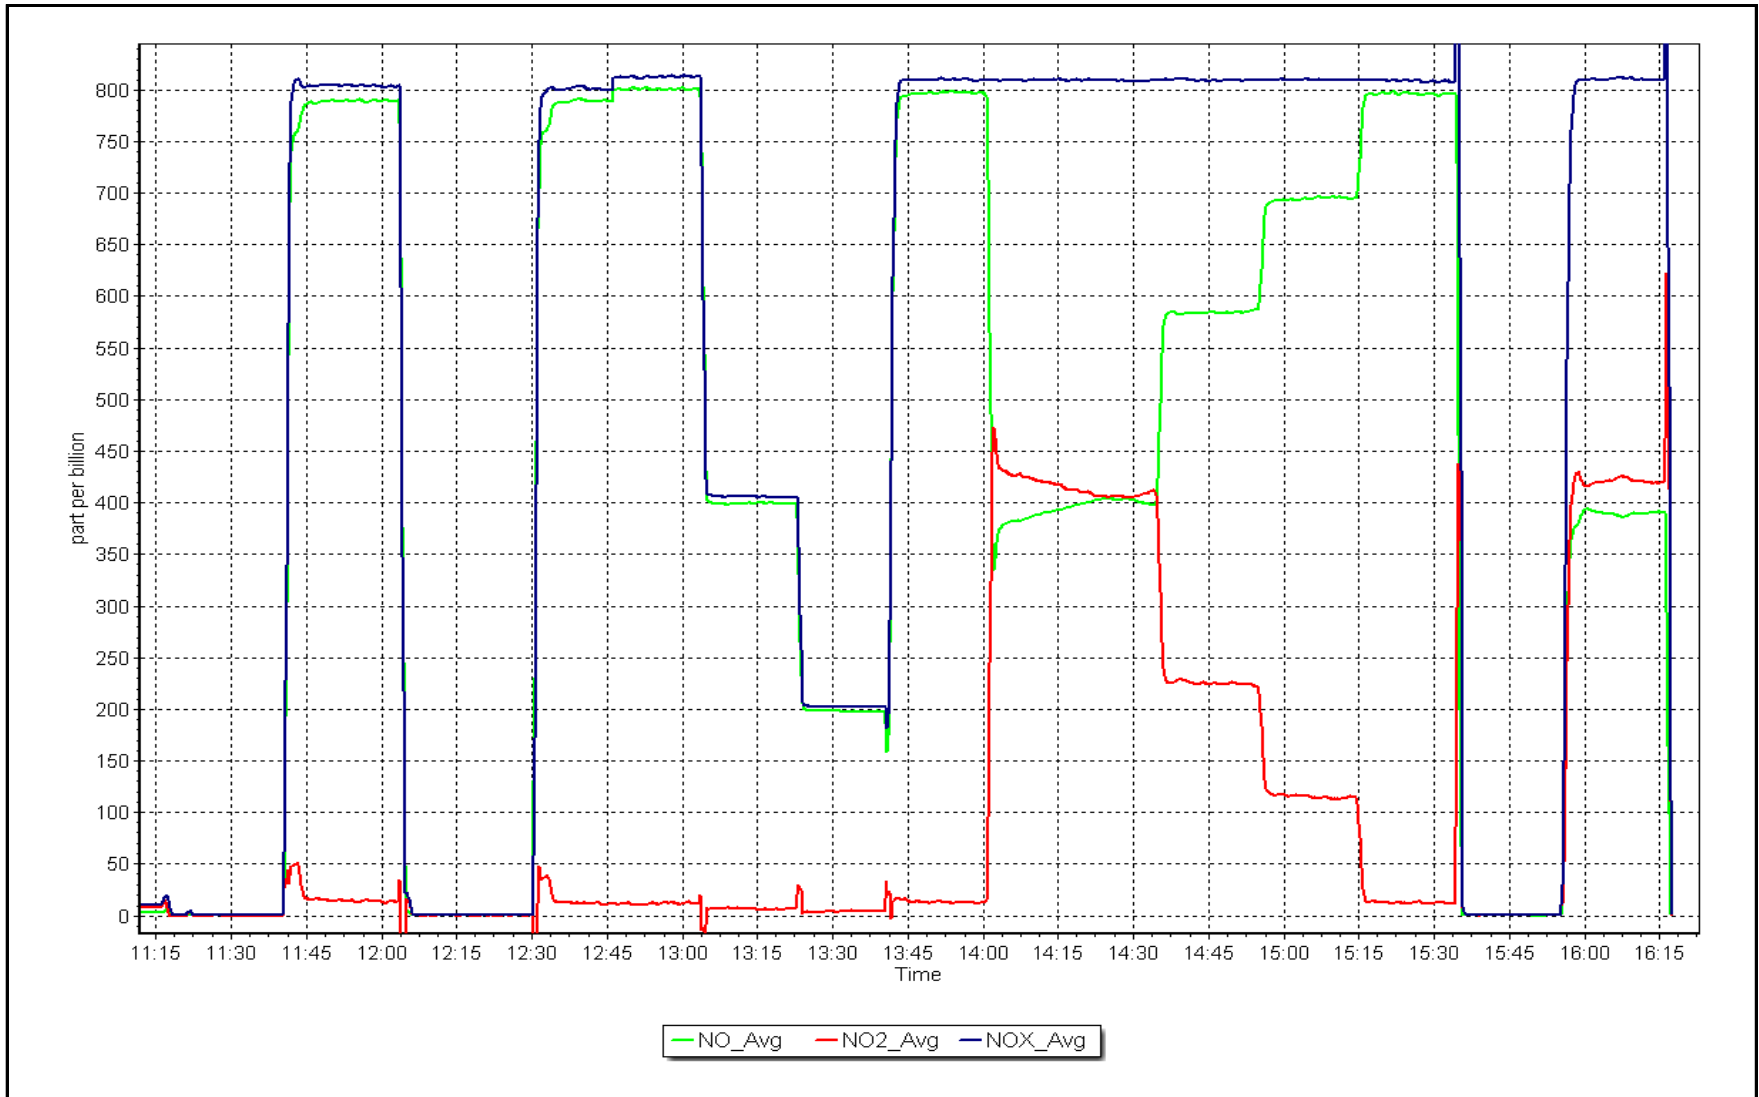



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Bertha Ganter-Fort McKay Station number: AMS01
 Calibration Date: January 4, 2023 Last Cal Date: December 7, 2022
 Start time (MST): 10:54 End time (MST): 14:09
 Reason: Routine

Calibration Standards

O3 generation mode: Photometer
 Calibrator Make/Model: Teledyne API T700 Serial Number: 3565
 ZAG Make/Model: Teledyne API T701 Serial Number: 5609

Analyzer Information

Analyzer make: Teledyne API T400 Analyzer serial #: 1107
 Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.997800	1.001400	Backgd or Offset:	2.0	2.9
Calibration intercept:	0.760000	0.480000	Coeff or Slope:	1.009	1.011

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.3	----
as found span	5000	855.5	400.0	401.2	0.997
as found 2nd point					
as found 3rd point					
calibrator zero	5000	0.0	0.0	0.0	----
high point	5000	855.5	400.0	400.7	0.998
second point	5000	738.6	200.0	201.3	0.994
third point	5000	649.2	100.0	100.9	0.991
as left zero	5000	0.0	0.0	0.2	----
as left span	5000	855.5	400.0	401.8	0.996
Average Correction Factor					0.994

Baseline Corr As found:	400.9	Previous response	399.9	*% change	0.3%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed inlet filter after as founds. Adjusted zero only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 7, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	10:54	End Time (MST):	14:09
Analyzer make:	Teledyne API T400	Analyzer serial #:	1107

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	0.999992	≥0.995
400.0	400.7	0.9983			
200.0	201.3	0.9935	Slope	1.001400	0.90 - 1.10
100.0	100.9	0.9911			
			Intercept	0.480000	+/- 5

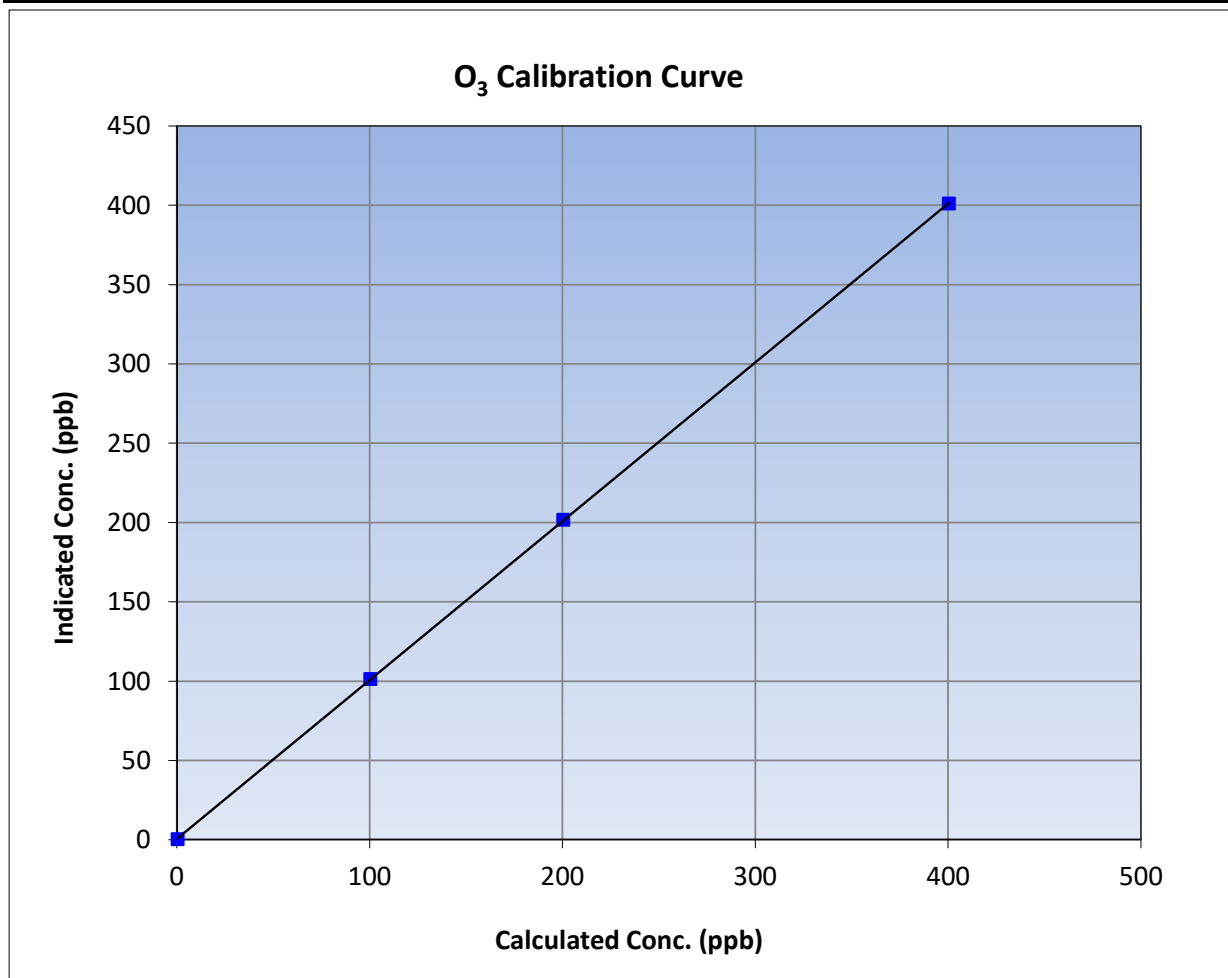

O₃ Calibration Plot

Date: January 4, 2023

Location: Bertha Ganter-Fort McKay

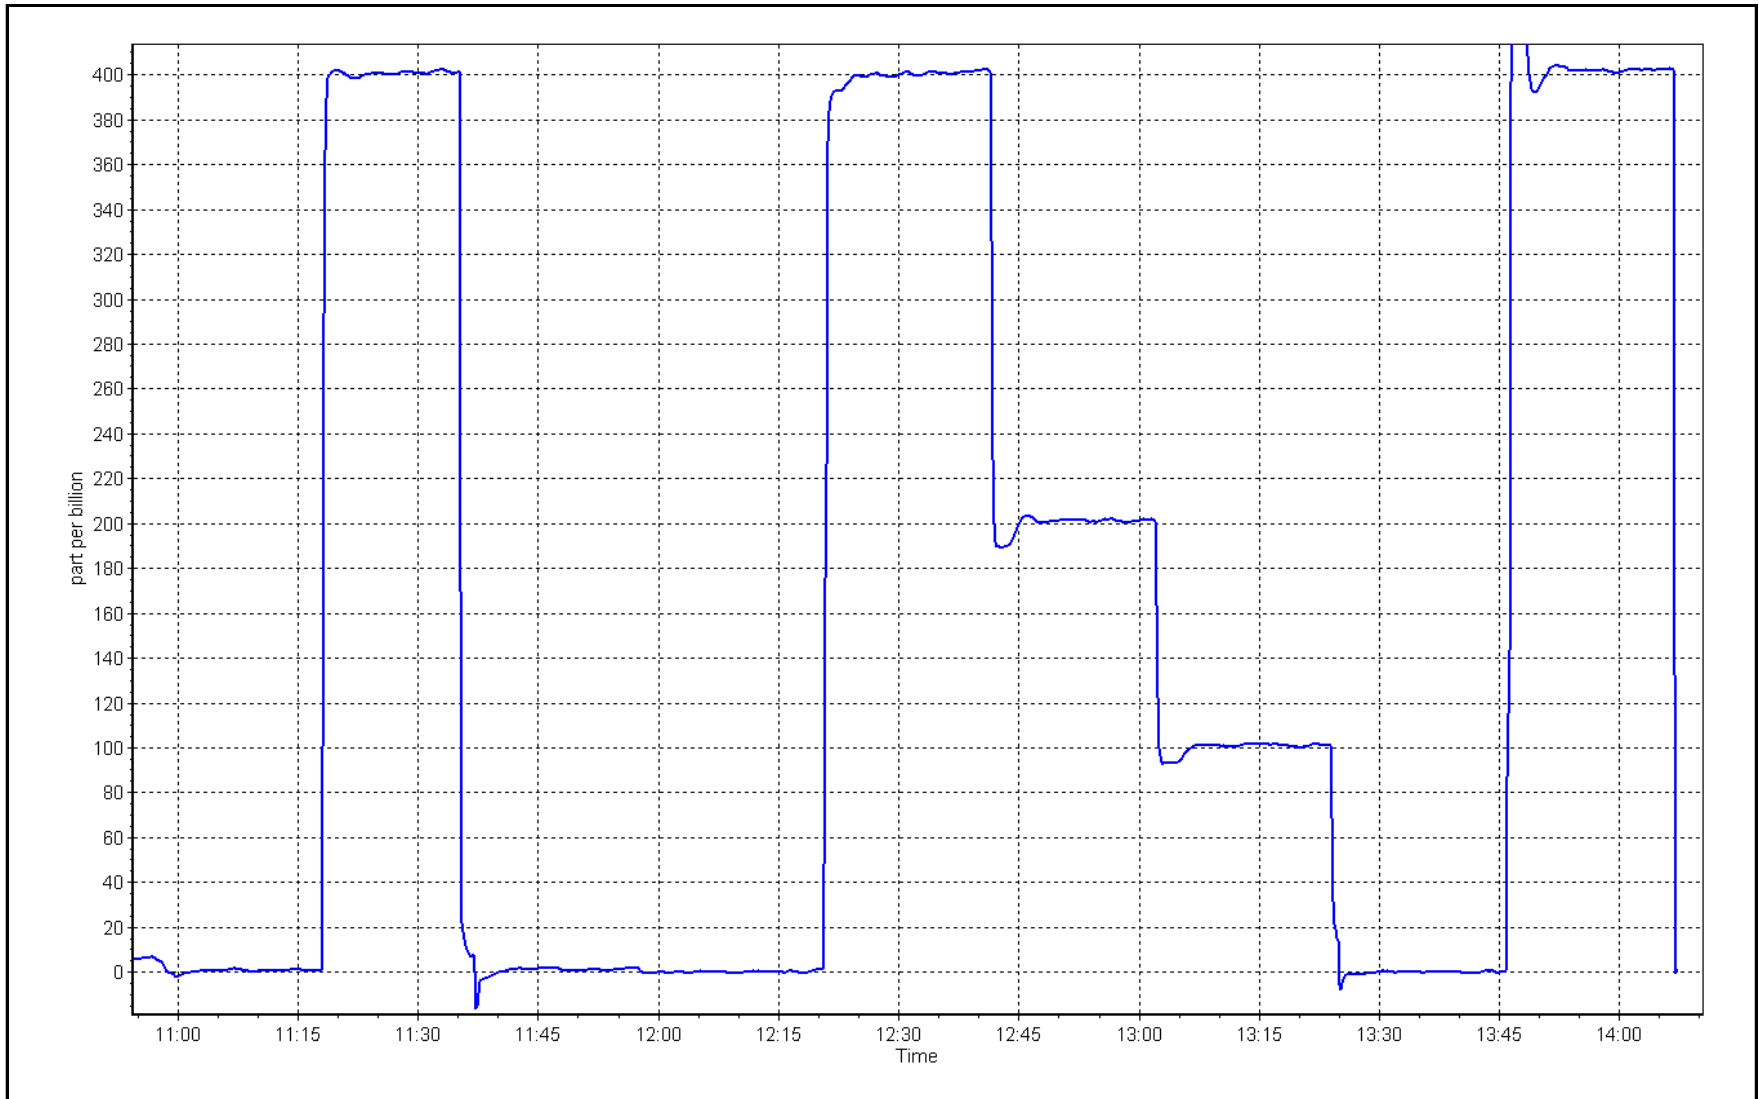



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Fort McKay - Bertha Ganter Station number: AMS 01
Calibration Date: January 24, 2023 Last Cal Date: December 19, 2022
Start time (MST): 13:55 End time (MST): 14:58

Analyzer Make: API T640 S/N: 306
Particulate Fraction: PM2.5

Flow Meter Make/Model: Delta Cal S/N: 1450
Temp/RH standard: Delta Cal S/N: 1450

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-5.3	-5.4	-5.3	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	733.8	733.7	733.8	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	4.99	4.93	4.99	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 24, 2023 Last Cal Date: December 19, 2022
PM w/o HEPA: 6.3 PM w/ HEPA: 0.0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test	---	NA	---	<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: December 19, 2022
Disposable Filter Changed: December 19, 2022

Annual Maintenance

Date Sample Tube Cleaned: August 31, 2022
Date RH/T Sensor Cleaned: December 19, 2022

Notes: Flow, temperature and pressure verified. Leak check passed.

Calibration by: Rene Chamberland



Wood Buffalo Environmental Association

CO Calibration Report

Version-01-2020

Station Information

Station Name:	Bertha Ganter-Fort McKay	Station number:	AMS01
Calibration Date:	January 11, 2023	Last Cal Date:	December 8, 2022
Start time (MST):	11:01	End time (MST):	14:30
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	<u>3040</u>	ppm	Cal Gas Exp Date:	December 1, 2028
Cal Gas Cylinder #:	<u>ALM042207</u>			
Removed Cal Gas Conc:	<u>3040</u>	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	<u>NA</u>		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	3565
ZAG Make/Model:	Teledyne API T701		Serial Number:	5609

Analyzer Information

Analyzer make:	Teledyne API T300	Analyzer serial #:	3520
Analyzer Range:	0 - 50 ppm		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.000946	0.999735	Backgd or Offset:	-0.012	-0.012
Calibration intercept:	0.195852	0.169836	Coeff or Slope:	0.989	0.989

CO Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.2	----
as found span	4933	66.7	40.6	41.0	0.989
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.0	----
high point	4933	66.7	40.6	40.6	1.000
second point	4966	33.3	20.2	20.7	0.978
third point	4983	16.7	10.2	10.3	0.983
as left zero	5000	0.0	0.0	0.0	----
as left span	2960	40.0	40.5	40.3	1.005
Average Correction Factor					0.987

Baseline Corr As found:	40.86	Prev response:	40.79	*% change:	0.2%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed inlet filter after as founds. Adjusted both zero and span.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

CO Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 8, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:01	End Time (MST):	14:30
Analyzer make:	Teledyne API T300	Analyzer serial #:	3520

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	0.999860	≥0.995
40.6	40.6	0.9997			
20.2	20.7	0.9782	Slope	0.999735	0.90 - 1.10
10.2	10.3	0.9830			
			Intercept	0.169836	+/-1.5

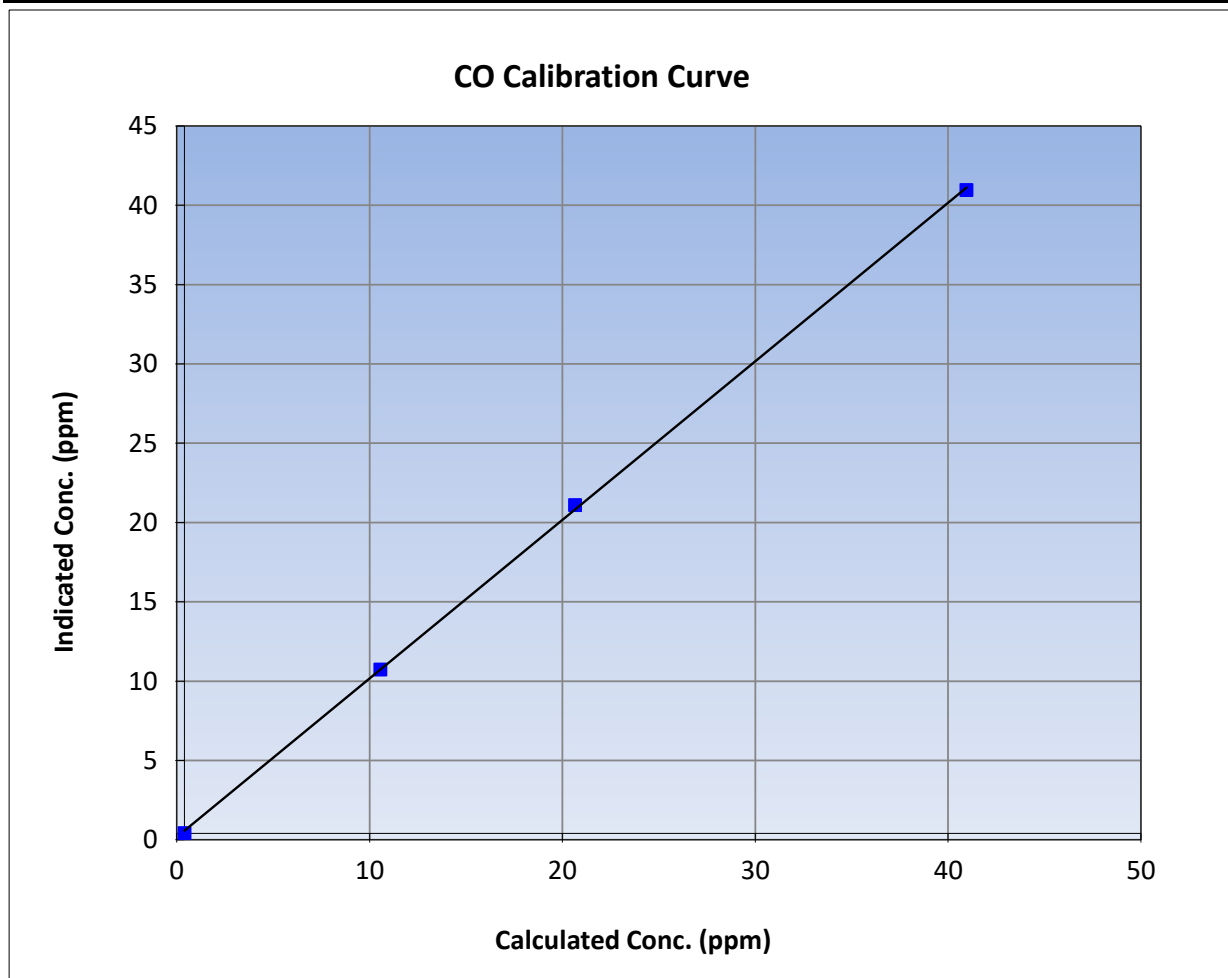

CO Calibration Plot

Date: January 11, 2023

Location: Bertha Ganter-Fort McKay

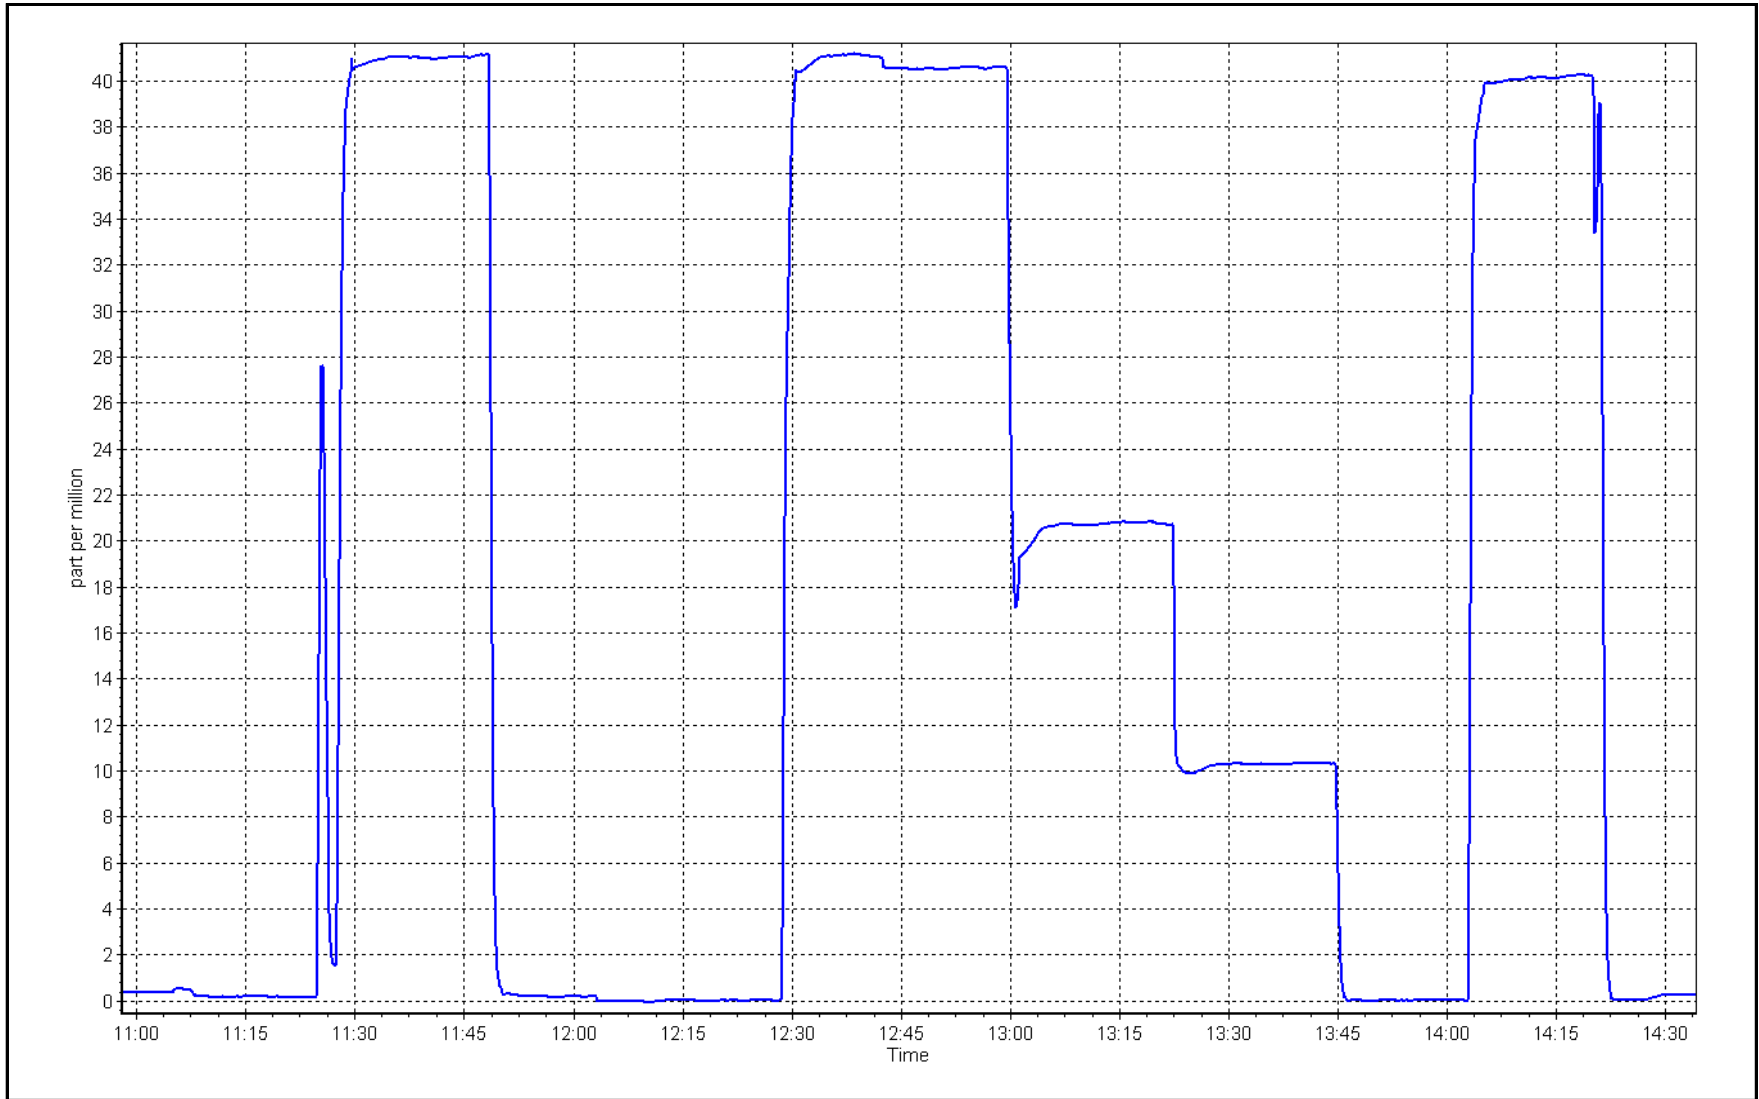



Wood Buffalo Environmental Association

CO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Bertha Ganter-Fort McKay	Station number:	AMS01
Calibration Date:	January 16, 2023	Last Cal Date:	December 12, 2022
Start time (MST):	10:43	End time (MST):	14:35
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	60,200	ppm	Cal Gas Exp Date:	December 1, 2028
Cal Gas Cylinder #:	<u>ALM042207</u>			
Removed Cal Gas Conc:	<u>60,200</u>	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	<u>NA</u>		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	3565
N2 Gen Make/Model:	Peak Sci NG5000		Serial Number:	7220900034

Analyzer Information

Analyzer make: Teledyne API 360	Analyzer serial #: 442
Analyzer Range 0 - 2,000 ppm	

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.000615	1.002131	Backgd or Offset:	0.037	0.037
Calibration intercept:	-2.540000	-6.480000	Coeff or Slope:	0.879	0.883

CO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	3000	0.0	0.0	-0.4	----
as found span	2920	80.0	1605.3	1573.6	1.020
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	3000	0.0	0.0	-0.1	----
high point	2920	80.0	1605.3	1606.4	0.999
second point	2960	40.0	802.7	791.9	1.014
third point	2980	20.0	401.3	391.2	1.026
as left zero	3000	0.0	0.0	-0.2	----
as left span	2960	40.0	802.7	776.0	1.034
Average Correction Factor					1.013

Baseline Corr As found:	1574.00	Prev response:	1603.78	*% change:	-1.9%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds. Adjusted span only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

CO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date	January 16, 2023	Previous Calibration	December 12, 2022
Station Name	Bertha Ganter-Fort McKay	Station Number	AMS01
Start Time (MST)	10:43	End Time (MST)	14:35
Analyzer make	Teledyne API 360	Analyzer serial #	442

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	-0.1	----	Correlation Coefficient	0.999919	≥0.995
1605.3	1606.4	0.9993			
802.7	791.9	1.0136	Slope	1.002131	0.90 - 1.10
401.3	391.2	1.0259			
			Intercept	-6.480000	+/-10

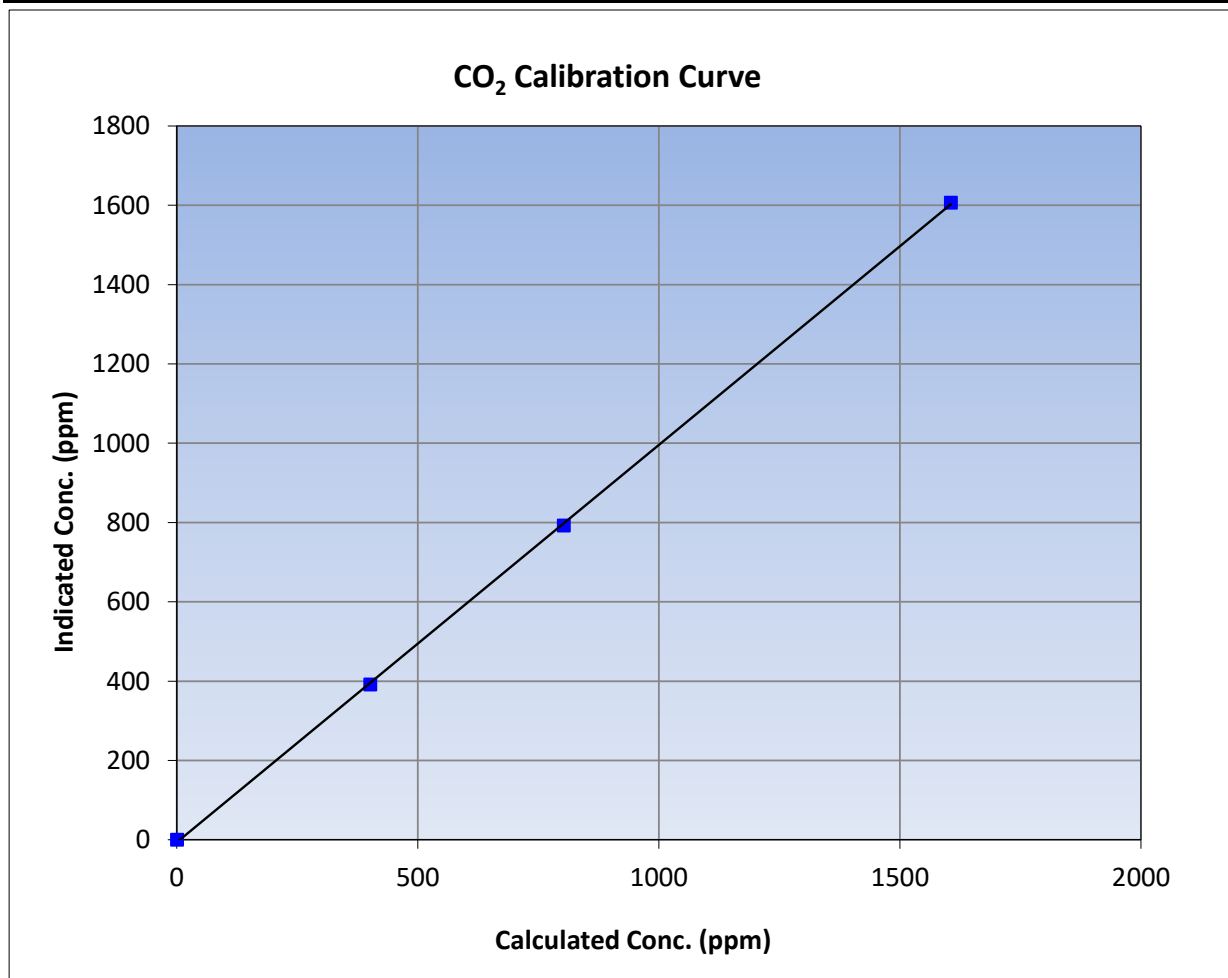

CO₂ Calibration Plot

Date: January 16, 2023

Location: Bertha Ganter-Fort McKay

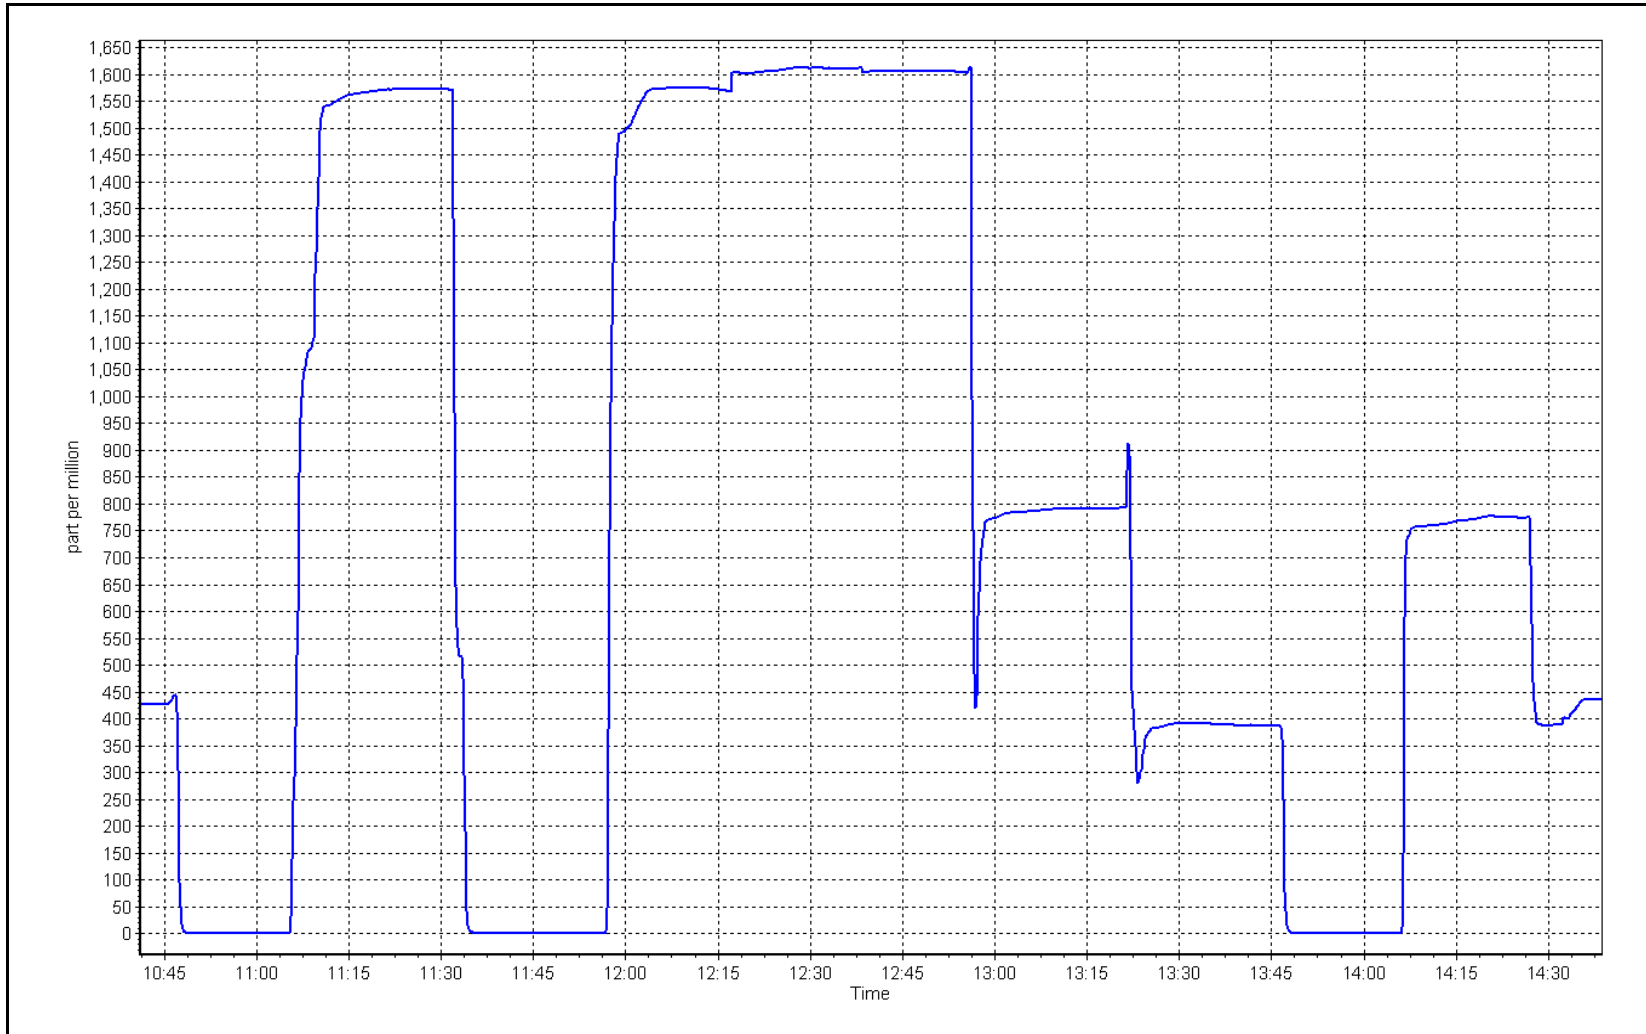



Wood Buffalo Environmental Association

TN - NO_x - NH₃ Calibration Report

Version-11-2021

Station Information

Station Name:	Bertha Ganter-Fort McKay	Station number:	AMS01
NOX Cal Date:	January 12, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	11:29	End time (MST):	15:50
NH3 Cal Date:	January 12, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	16:15	End time (MST):	18:53
Reason:	As Found		

Calibration Standards

NOX Cal Gas Conc:	50.84	ppm	NO Gas Cylinder #:	T2Y1P9L
NO Cal Gas Conc:	50.04	ppm	NO Cal Gas Expiry:	March 3, 2028
Removed NOX Conc:	50.84	ppm	Removed Cylinder #:	NA
Removed NO Conc:	50.04	ppm	Removed cyl Expiry:	NA
NOX gas Diff:			NO gas Diff:	
NH3 Cal Gas Conc:	74.00	ppm	NH3 Gas Cylinder #:	LL119509
			NH3 Cal Gas Expiry:	February 24, 2022
Removed NH3 Conc:	74.00	ppm	Removed Cylinder #:	NA
NH3 gas Diff:			Removed cyl Expiry:	NA
Calibrator Model:	Teledyne API T700		Serial Number:	3565
ZAG make/model:	Teledyne API T701		Serial Number:	5609

Analyzer Information

Analyzer model:	Teledyne API T201	Analyzer serial #:	475
Converter model:	Teledyne API T501	Converter serial #:	484
NH3 Range (ppb):	0 - 2000 ppb	Reaction cell Press:	6.00
NOX Range (ppb):	0 - 1000 ppb	Sample Flow:	527

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coefficient:	1.009	1.001	TN coefficient:	1.009	1.000
NOX coefficient:	1.016	1.008	NO bkgnd:	0.100	0.100
NO2 coefficient:	1.000	1.000	NOX bkgnd:	0.600	0.600
NH3 coefficient:	0.933	0.933	TN bkgnd:	2.300	2.300

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.002501	1.000436
NO _x Cal Offset:	-0.120000	-0.160000
NO Cal Slope:	1.001242	0.999472
NO Cal Offset:	-1.540000	-0.820000
NO ₂ Cal Slope:	1.005272	0.994087
NO ₂ Cal Offset:	0.622766	0.253701
NH3 Cal Slope:	1.000243	1.006531
NH3 Cal Offset:	3.207760	3.444505
TN Cal Slope:	1.002735	1.009328
TN Cal Offset:	3.501910	3.486553



Wood Buffalo Environmental Association

TN - NOX - NH₃ Calibration Report

Version-11-2021

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated TN concentration (ppb) (Cc)	Calculated NOX concentration (ppb) (Cc)	Calculated NH3 concentration (ppb) (Cc)	Indicated TN concentration (ppb) (Ic)	Indicated NOX concentration (ppb) (Ic)	Indicated NH3 concentration (ppb) (Ic)	TN Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NH3 Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-0.9	-0.2	-0.7	----	----
as found NO	4920	80.0	813.4	813.4	----	822.3	820.6	1.9	0.989	----
calibrator zero	5000	0.0	0.0	0.0	0.0	0.0	0.0	0.0	----	----
high NO point	4920	80.0	813.4	813.4	----	812.7	813.1	-0.8	1.001	----
NO/O3 point	4920	80.0	813.4	813.4	----	810.0	808.1	2.1	1.004	----
as found NH3	2927	73.0	1800.7	----	1800.7	1815.7	----	1810.7	0.992	0.994
new NH3 cyl rp							----			
first NH3	2927	73.0	1800.7	----	1800.7	1815.7	----	1810.7	0.992	0.994
second NH3	2960	40.5	999.0	----	999.0	1022.0	----	1019.0	0.977	0.980
third NH3	2980	20.3	500.7	----	500.7	507.4	----	506.0	0.987	0.990
Average Correction Factor									1.0026	0.9881

Corrected As found TN = 823.2 ppb NO_x = 820.8 ppb NH3 = 1811.4 ppb

Previous Response TN = 819.2 ppb NO_x = 815.4 ppb NH3 = 1804.3 ppb

NH3 Previous Converter Efficiency = 93.3%

NH3 Current Converter Efficiency = 93.3%

*Percent Change TN = 0.5%

*Percent Change NO_x = 0.7%

*Percent Change NH3 = 0.4%

* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

NO_x - NO - NO₂ Calibration Report

Version-11-2021

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated TN concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated TN concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-0.2	-0.1	-0.9	----	----
as found span	4920	80.0	813.4	800.6	813.4	820.6	802.0	822.3	0.9913	0.9983
new NO cyl rp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.0	0.1	0.0	----	----
high point	4920	80.0	813.4	800.6	813.4	813.1	799.5	812.7	1.0004	1.0014
second point	4960	40.0	406.7	400.3	406.7	408.5	399.9	409.8	0.9956	1.0011
third point	4980	20.0	203.4	200.2	203.4	201.9	197.6	202.0	1.0072	1.0130
Average Correction Factor									1.0011	1.0051

Baseline Corr As fnd	TN = 823.2 ppb	NO _x = 820.8 ppb	NO = 802.1 ppb	*Percent Change	TN = 0.5%
Previous Response	TN = 819.2 ppb	NO _x = 815.4 ppb	NO = 800.1 ppb	*Percent Change	NO _x = 0.7%
				*Percent Change	NO = 0.3%
				<i>* = > +/-5% change initiates investigation</i>	

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found zero	----	----	0.0	0.0	----	----
calibration zero	----	----	0.0	-0.1	----	----
1st GPT point (400 ppb O3)	798.4	387.9	423.3	420.1	1.0076	99.2%
2nd GPT point (200 ppb O3)	798.4	595.3	215.9	217.5	0.9926	100.7%
3rd GPT point (100 ppb O3)	798.4	686.9	124.3	122.5	1.0147	98.6%
Average Correction Factor					1.0050	99.5%

Notes: Changed the inlet filter after as founds. Adjusted NO_x and TN_x Spans. Used the second GPT reference point. NH₃ calibration failed.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

TN Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 2, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:29	End Time (MST):	15:50
Analyzer make:	Teledyne API T201	Analyzer serial #:	475

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.0	----	Correlation Coefficient	≥0.995	
1800.7	1815.7	0.9917			
999.0	1022.0	0.9775			
500.7	507.4	0.9868			
			Slope	1.009328	0.90 - 1.10
			Intercept	3.486553	+/-20

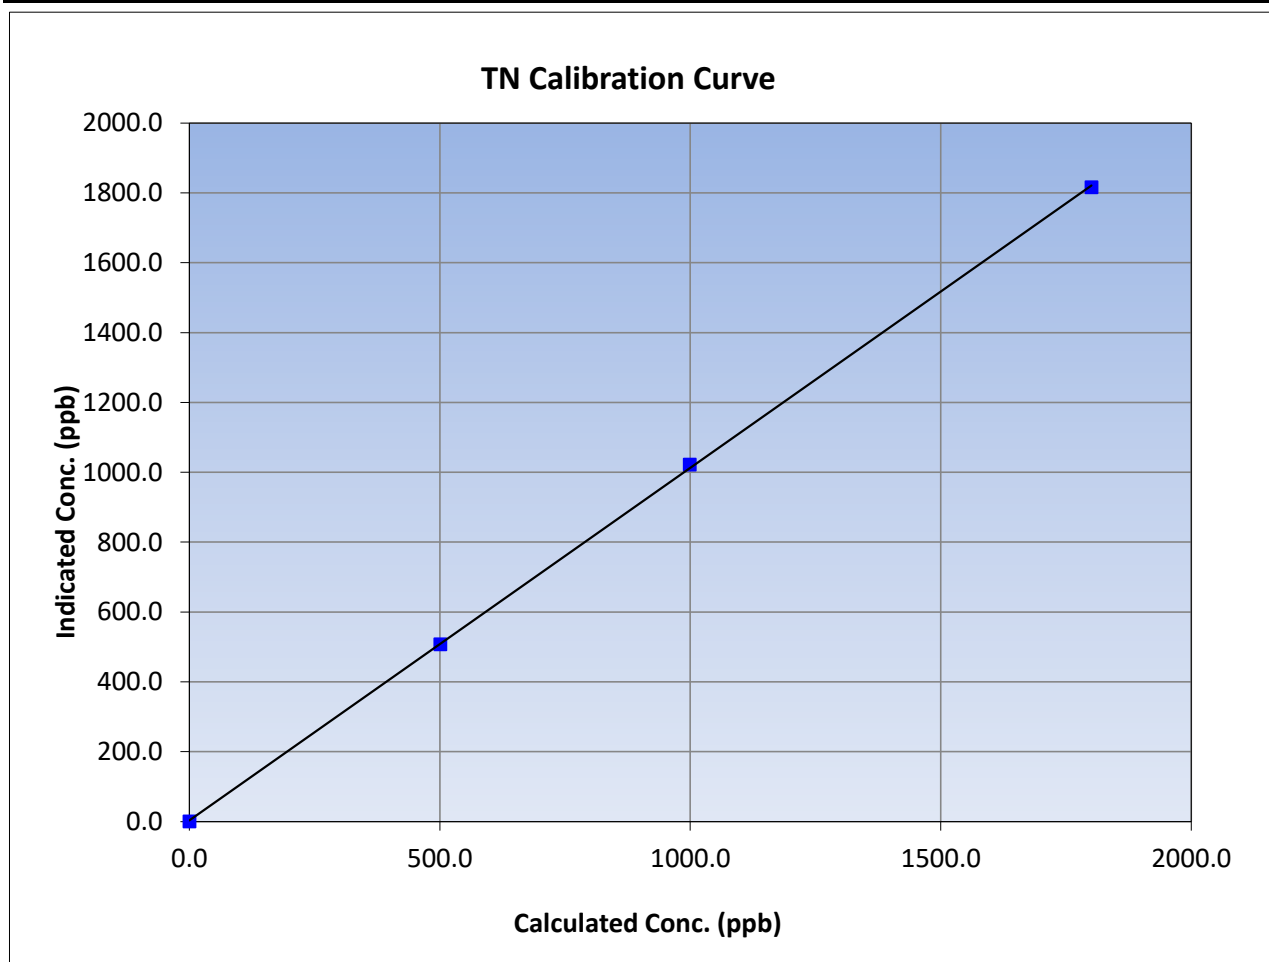



Wood Buffalo Environmental Association

NH₃ Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 2, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:29	End Time (MST):	15:50
Analyzer make:	Teledyne API T201	Analyzer serial #:	475

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.0	----	Correlation Coefficient	≥0.995	
1800.7	1810.7	0.9945			
999.0	1019.0	0.9804			
500.7	506.0	0.9895			
			Slope	1.006531	0.90 - 1.10
			Intercept	3.444505	+/-20

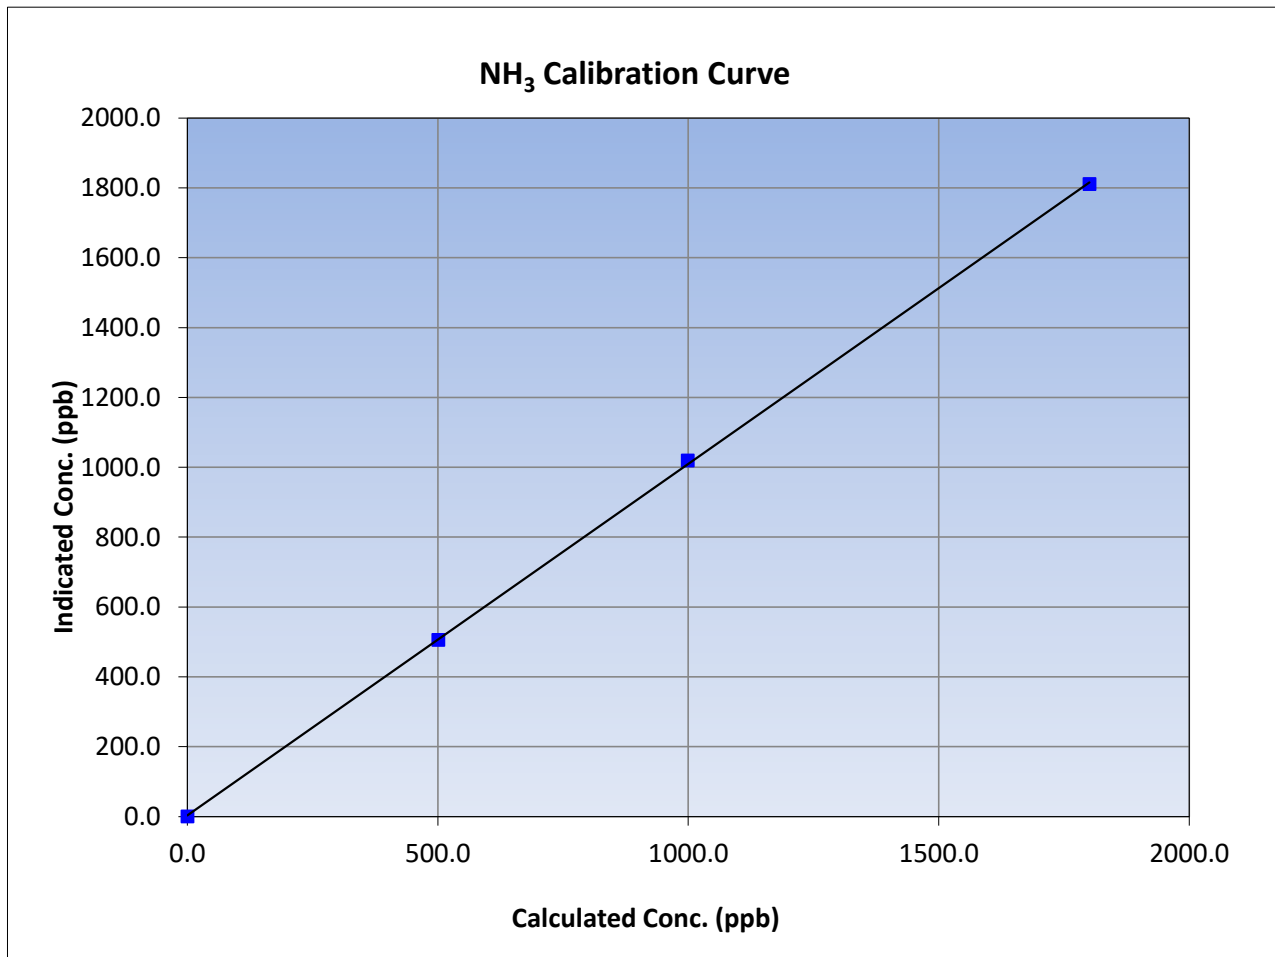



Wood Buffalo Environmental Association

NO_x Calibration Summary

Version-11-2021


Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 2, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:29	End Time (MST):	15:50
Analyzer make:	Teledyne API T201	Analyzer serial #:	475

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
813.4	813.1	1.0004		
406.7	408.5	0.9956		
203.4	201.9	1.0072		
			0.999985	
			1.000436	
			-0.160000	

NO_x Calibration Curve

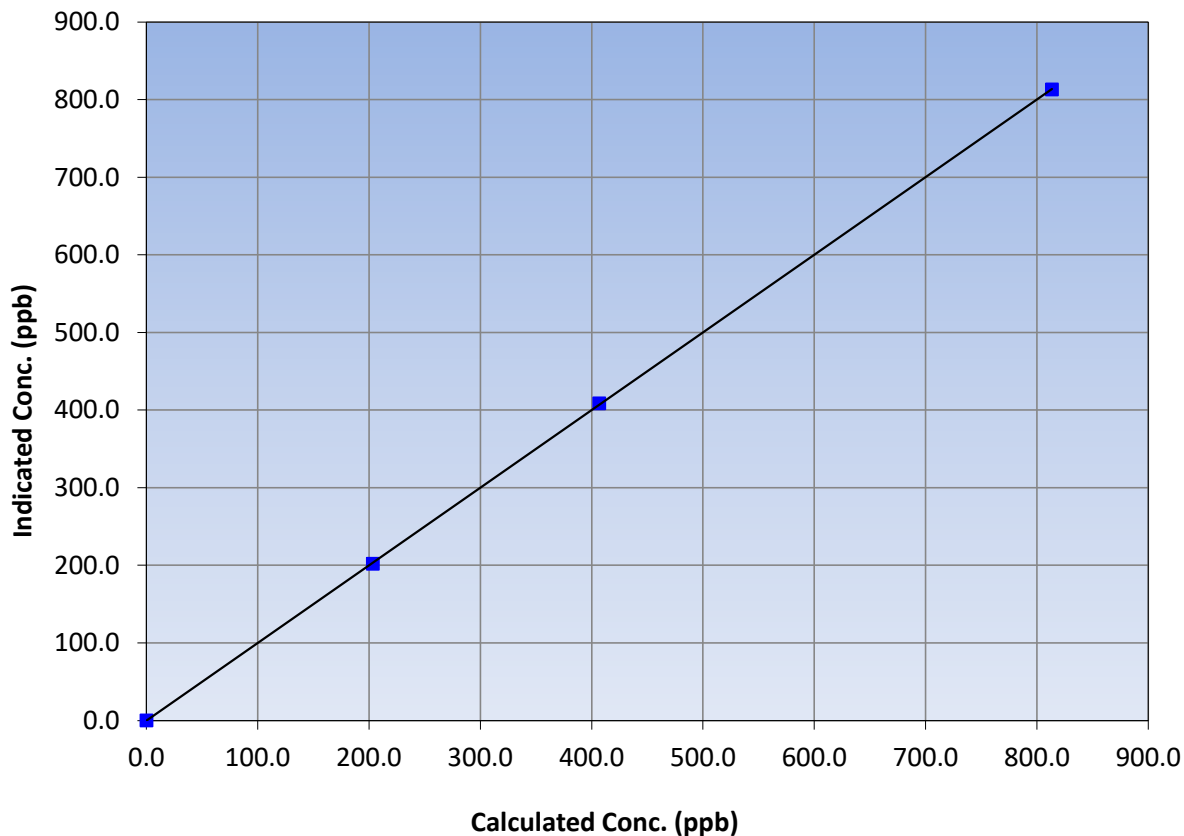



Wood Buffalo Environmental Association

NO Calibration Summary

Version-11-2021


Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 2, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:29	End Time (MST):	15:50
Analyzer make:	Teledyne API T201	Analyzer serial #:	475

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.1	----	Correlation Coefficient	≥0.995	
800.6	799.5	1.0014			
400.3	399.9	1.0011			
200.2	197.6	1.0130			
			Slope	0.999472	0.90 - 1.10
			Intercept	-0.820000	+/-20

NO Calibration Curve

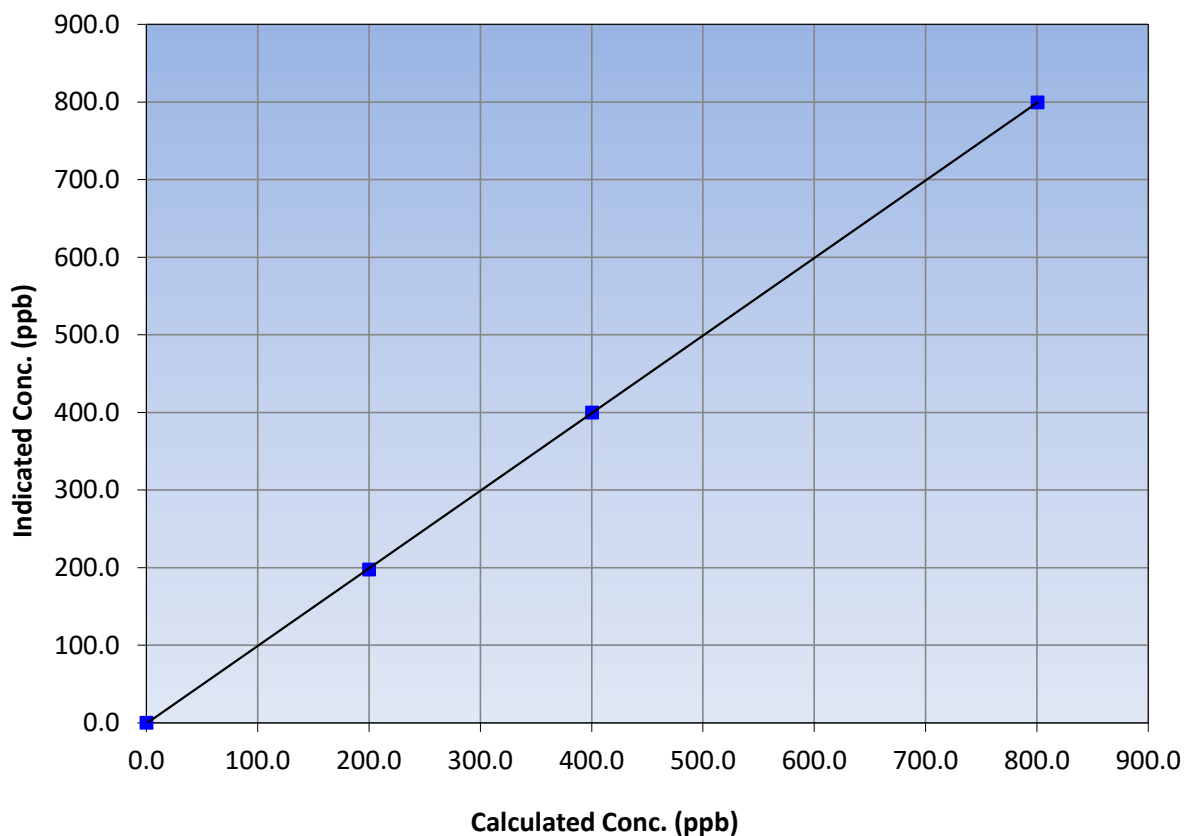



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-11-2021


Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 2, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	11:29	End Time (MST):	15:50
Analyzer make:	Teledyne API T201	Analyzer serial #:	475

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	-0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20	
423.3	420.1	1.0076			
215.9	217.5	0.9926			
124.3	122.5	1.0147			
			Correlation Coefficient	0.999898	≥0.995
			Slope	0.994087	0.90 - 1.10
			Intercept	0.253701	+/-20


NO₂ Calibration Curve

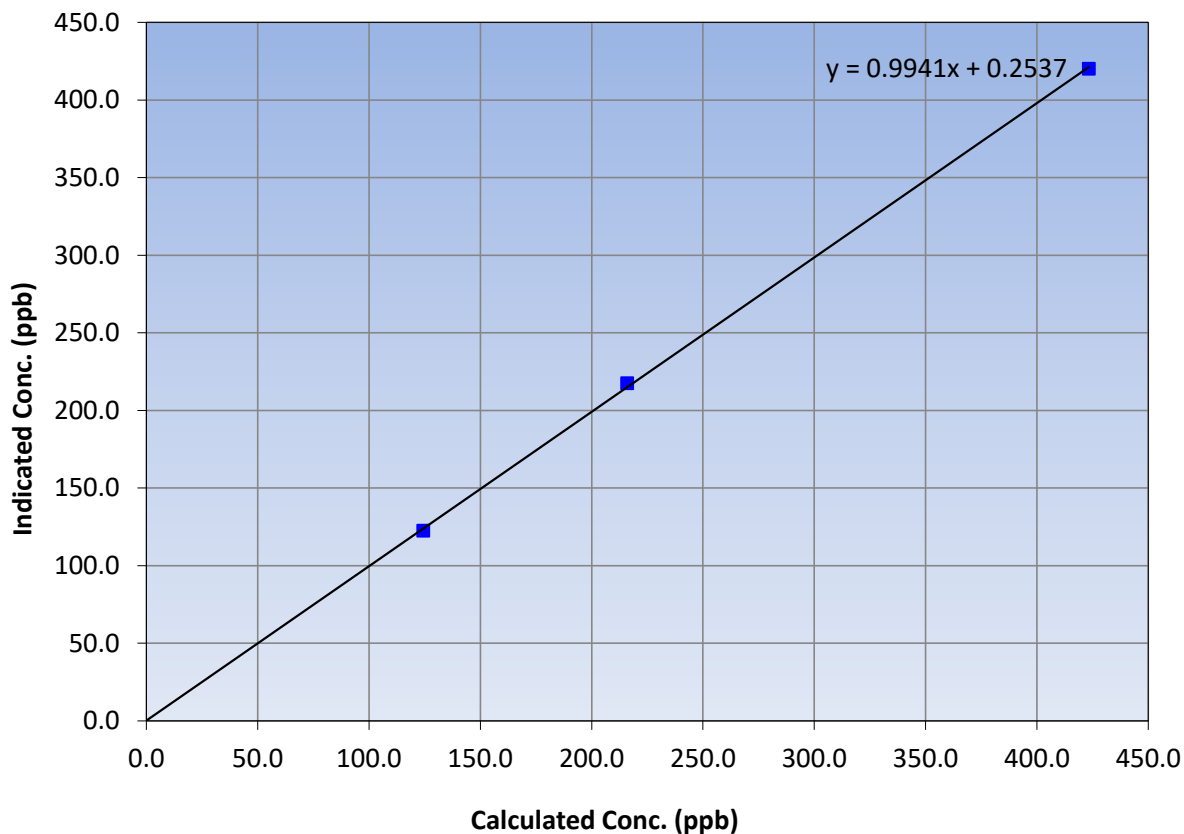

NO_x Calibration Plot

Date: January 12, 2023


Location: Bertha Ganter-Fort McKay

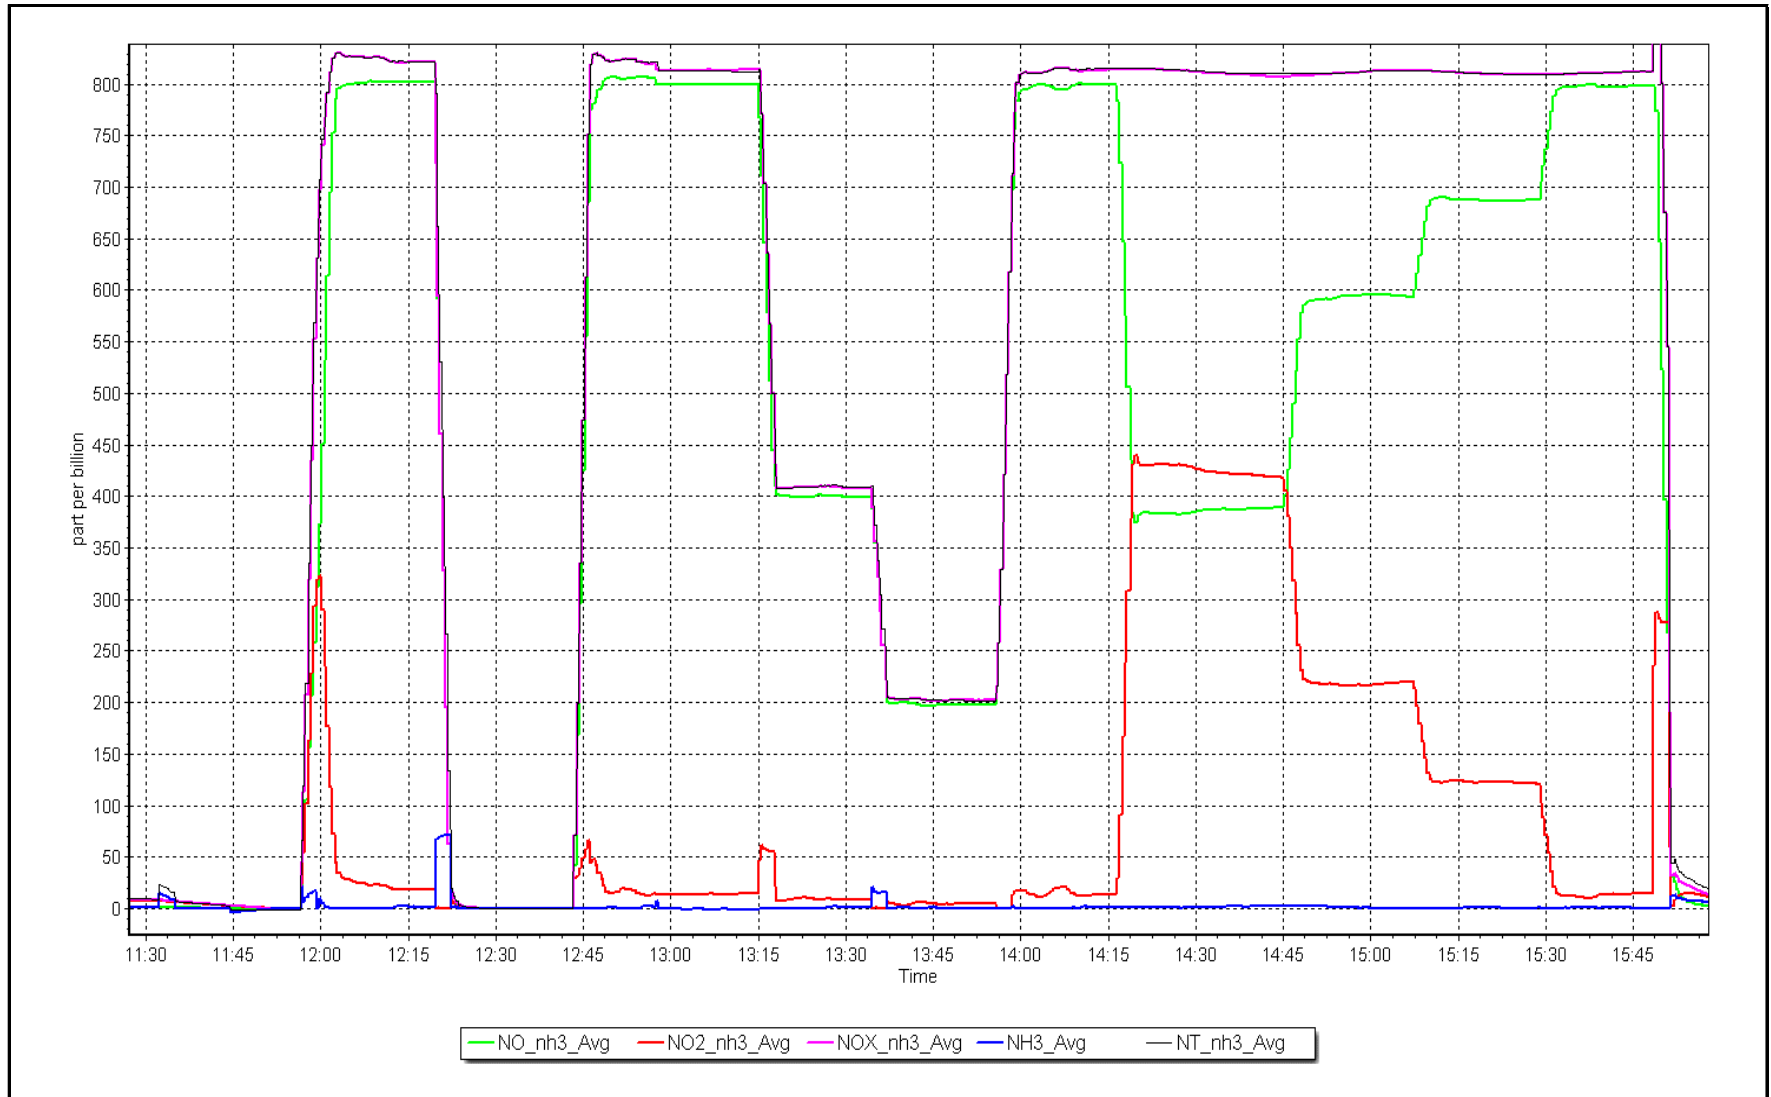

NH₃ Calibration Plot

Date: January 12, 2023

Location: Bertha Ganter-Fort McKay

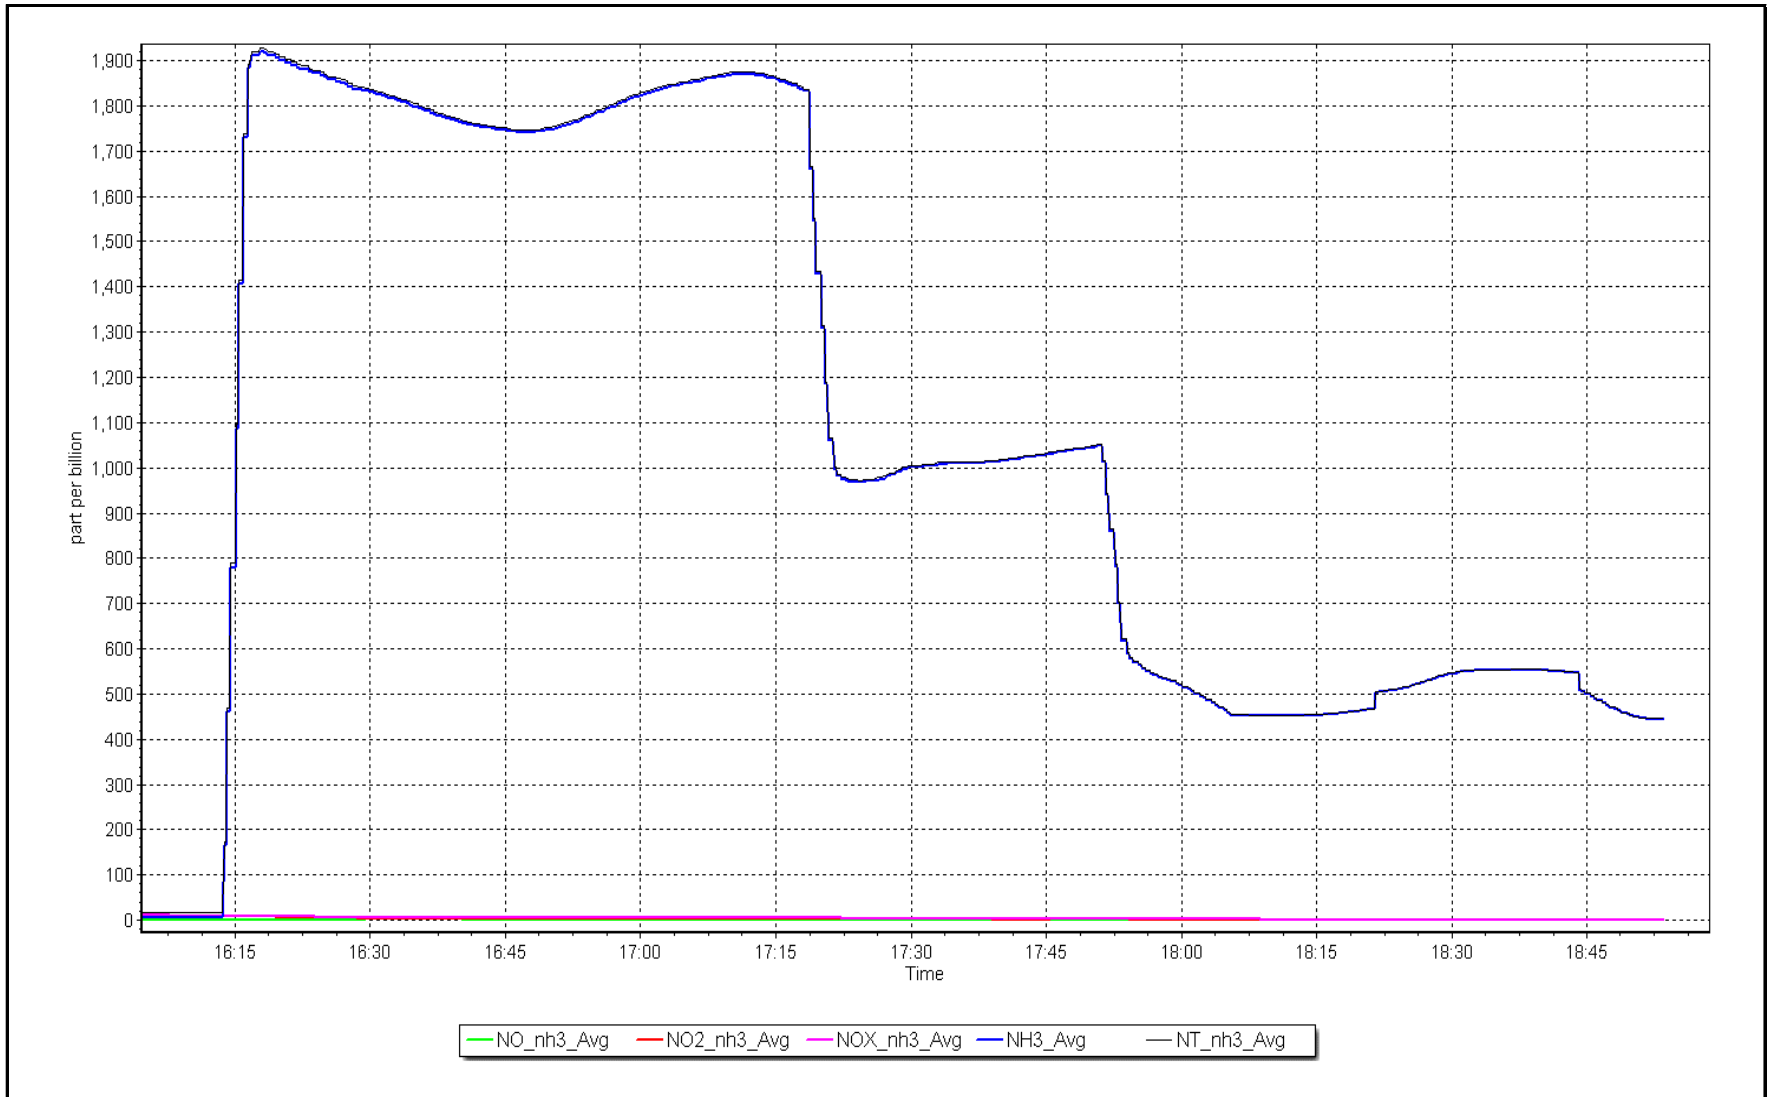



Wood Buffalo Environmental Association

TN - NO_x - NH₃ Calibration Report

Version-11-2021

Station Information

Station Name:	Bertha Ganter-Fort McKay	Station number:	AMS01
NOX Cal Date:	January 13, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	13:00	End time (MST):	14:40
NH3 Cal Date:	January 13, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	15:00	End time (MST):	17:30
Reason:	Maintenance		

Calibration Standards

NOX Cal Gas Conc:	50.84	ppm	NO Gas Cylinder #:	T2Y1P9L
NO Cal Gas Conc:	50.04	ppm	NO Cal Gas Expiry:	March 3, 2028
Removed NOX Conc:	50.84	ppm	Removed Cylinder #:	NA
Removed NO Conc:	50.04	ppm	Removed cyl Expiry:	NA
NOX gas Diff:			NO gas Diff:	
NH3 Cal Gas Conc:	72.93	ppm	NH3 Gas Cylinder #:	CC281298
Removed NH3 Conc:	74.00	ppm	NH3 Cal Gas Expiry:	February 28, 2023
NH3 gas Diff:			Removed Cylinder #:	LL119509
Calibrator Model:	Teledyne API T700		Removed cyl Expiry:	February 24, 2022
ZAG make/model:	Teledyne API T701		Serial Number:	3565
			Serial Number:	5609

Analyzer Information

Analyzer model:	Teledyne API T201	Analyzer serial #:	475
Converter model:	Teledyne API T501	Converter serial #:	217
NH3 Range (ppb):	0 - 2000 ppb	Reaction cell Press:	5.10
NOX Range (ppb):	0 - 1000 ppb	Sample Flow:	505

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coefficient:	1.001	1.046	TN coefficient:	1.000	1.056
NOX coefficient:	1.008	1.050	NO bkgrnd:	0.100	0.000
NO2 coefficient:	1.000	1.000	NOX bkgrnd:	0.600	0.600
NH3 coefficient:	0.933	0.933	TN bkgrnd:	2.300	6.300

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.000436	0.998476
NO _x Cal Offset:	-0.160000	-0.200000
NO Cal Slope:	0.999472	1.000075
NO Cal Offset:	-0.820000	-0.100000
NO ₂ Cal Slope:	0.994087	
NO ₂ Cal Offset:	0.253701	
NH3 Cal Slope:	1.021299	1.004278
NH3 Cal Offset:	3.444505	3.834562
TN Cal Slope:	1.024137	1.007082
TN Cal Offset:	3.486553	3.818565



Wood Buffalo Environmental Association

TN - NOX - NH₃ Calibration Report

Version-11-2021

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated TN concentration (ppb) (Cc)	Calculated NOX concentration (ppb) (Cc)	Calculated NH3 concentration (ppb) (Cc)	Indicated TN concentration (ppb) (Ic)	Indicated NOX concentration (ppb) (Ic)	Indicated NH3 concentration (ppb) (Ic)	TN Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NH3 Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero										
as found NO										
calibrator zero	5000	0.0	0.0	0.0	0.0	-0.3	-0.2	-0.1	----	----
high NO point	4920	80.0	813.4	813.4	----	813.4	812.0	1.3	1.000	----
NO/O3 point										
as found NH3										
new NH3 cyl rp										
first NH3	2926	74.1	1801.4	----	1801.4	1815.7	----	1810.7	0.992	0.995
second NH3	2959	41.2	1001.6	----	1001.6	1014.2	----	1011.5	0.988	0.990
third NH3	2979	20.6	500.8	----	500.8	512.8	----	511.1	0.977	0.980
Average Correction Factor									1.0000	0.9883

Corrected As found TN = NA ppb NO_x = NA ppb NH3 = NA ppb

Previous Response TN = NA ppb NO_x = NA ppb NH3 = NA ppb

NH3 Previous Converter Efficiency = 93.3%

NH3 Current Converter Efficiency = 93.3%

*Percent Change TN = NA

*Percent Change NO_x = NA

*Percent Change NH3 = NA

* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

NO_x - NO - NO₂ Calibration Report

Version-11-2021

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated TN concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated TN concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>		
as found zero												
as found span												
new NO cyl rp												
calibrator zero	5000	0.0	0.0	0.0	0.0	-0.2	-0.1	-0.3	----	----		
high point	4920	80.0	813.4	800.6	813.4	812.0	800.6	813.4	1.0018	1.0000		
second point												
third point												
Average Correction Factor									1.0018	1.0000		
Baseline Corr As fnd	TN =	NA	ppb	NO _x =	NA	ppb	NO =	NA	ppb	*Percent Change	TN =	NA
Previous Response	TN =	NA	ppb	NO _x =	NA	ppb	NO =	NA	ppb	*Percent Change	NO _x =	NA
										*Percent Change	NO =	NA
										* = > +/-5% change initiates investigation		

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found zero						
calibration zero	----	----	0.0	0.0	----	----
1st GPT point (400 ppb O3)						
2nd GPT point (200 ppb O3)						
3rd GPT point (100 ppb O3)						
Average Correction Factor						

Notes: As founds were performed on January 12. Replaced the NH₃ converter, pump, charcoal pack, and calibration gas. Adjusted both zero and span. NH₃ calibration is still failing.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

TN Calibration Summary

Version-11-2021


Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 2, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	13:00	End Time (MST):	14:40
Analyzer make:	Teledyne API T201	Analyzer serial #:	475

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	-0.3	----	Correlation Coefficient	≥0.995	
1801.4	1815.7	0.9921			
1001.6	1014.2	0.9875			
500.8	512.8	0.9766			
			Slope	1.007082	0.90 - 1.10
			Intercept	3.818565	+/-20

TN Calibration Curve

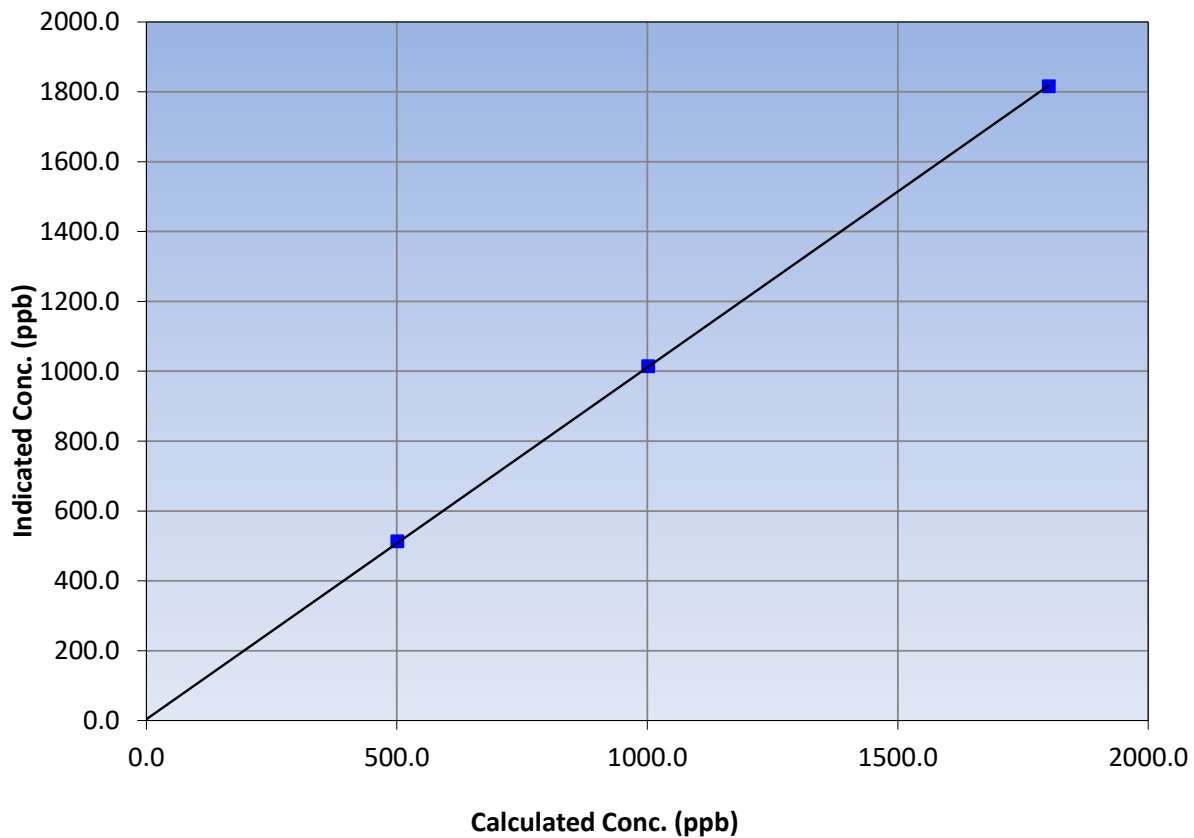



Wood Buffalo Environmental Association

NH₃ Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 2, 2022
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	13:00	End Time (MST):	14:40
Analyzer make:	Teledyne API T201	Analyzer serial #:	475

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	-0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
1801.4	1810.7	0.9948		
1001.6	1011.5	0.9902		
500.8	511.1	0.9798		
			0.999976	
			1.004278	
			3.834562	

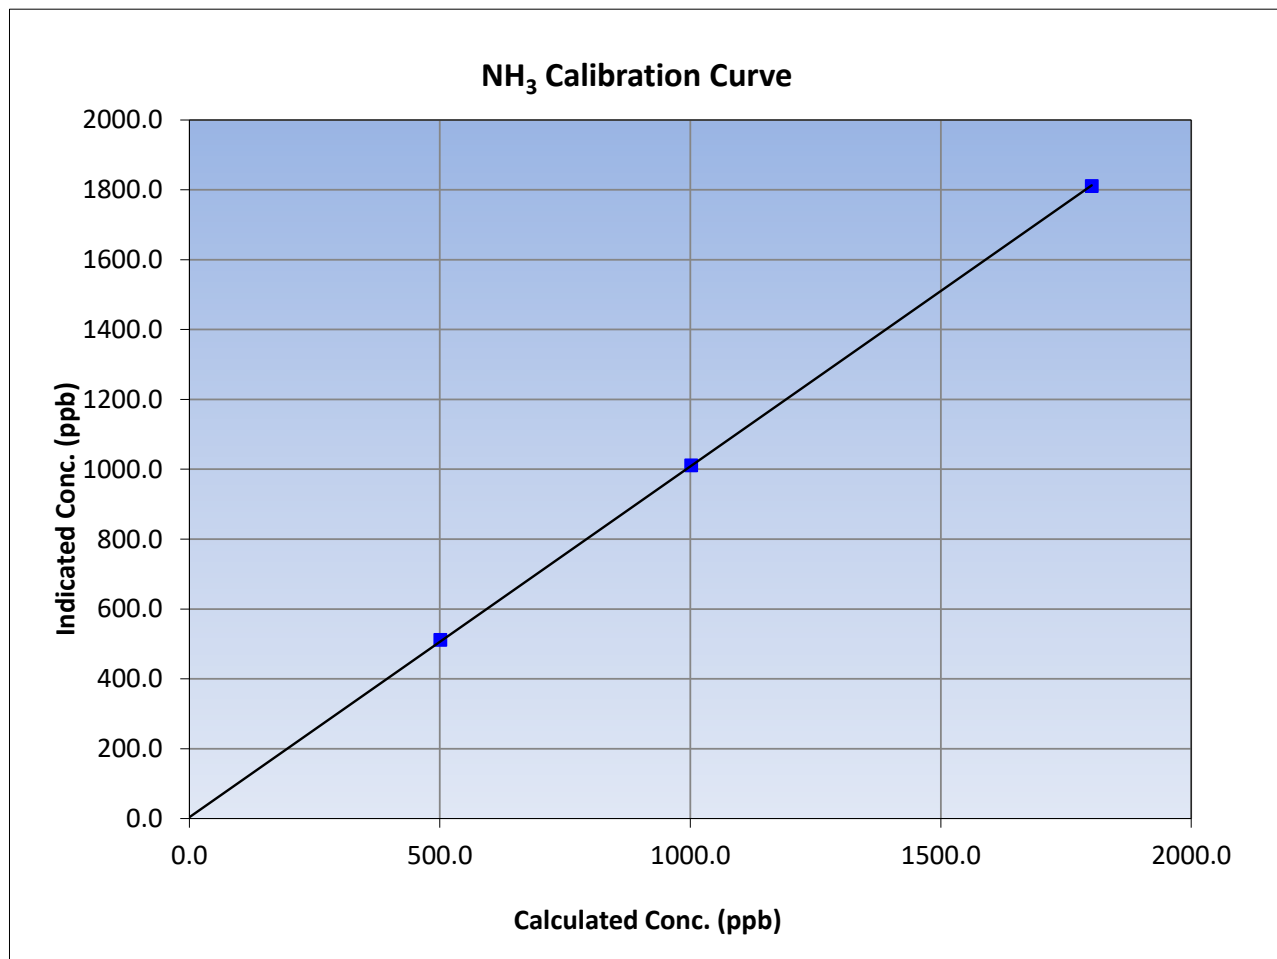

NO_x Calibration Plot

Date: January 13, 2023


Location: Bertha Ganter-Fort McKay

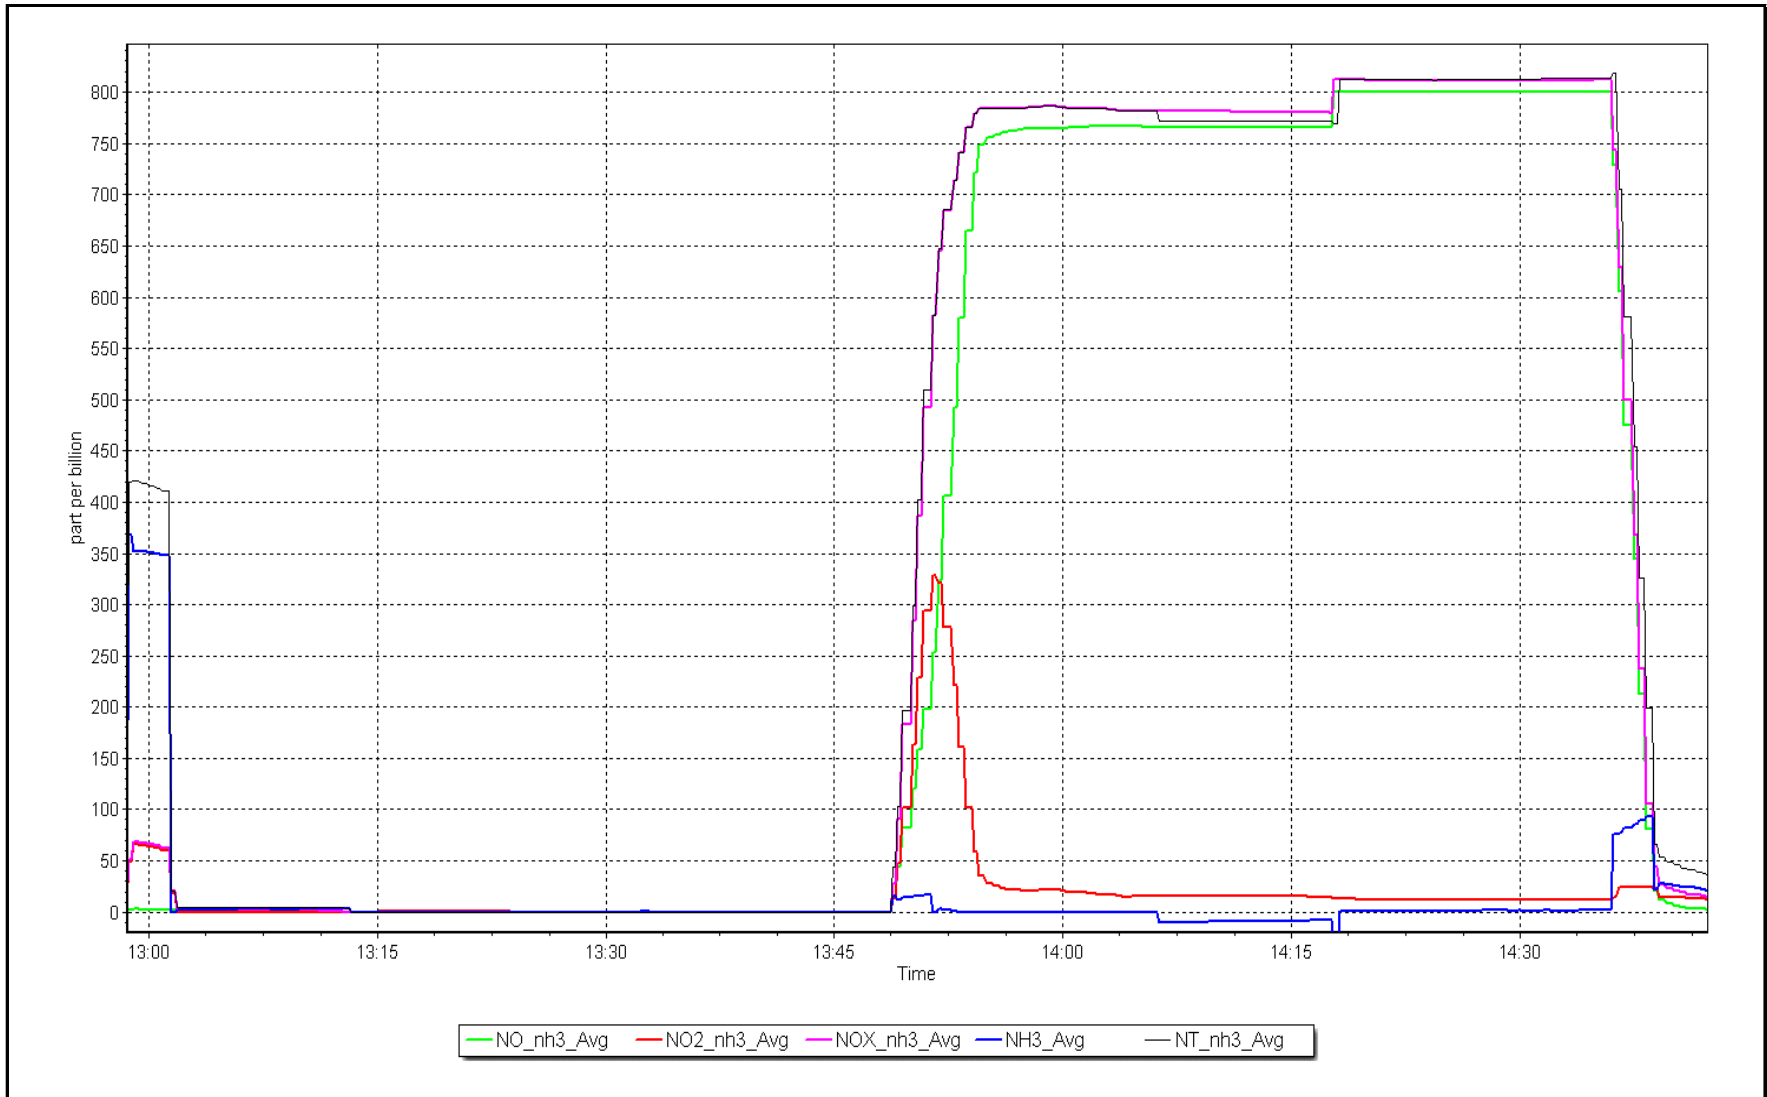

NH₃ Calibration Plot

Date: January 13, 2023

Location: Bertha Ganter-Fort McKay

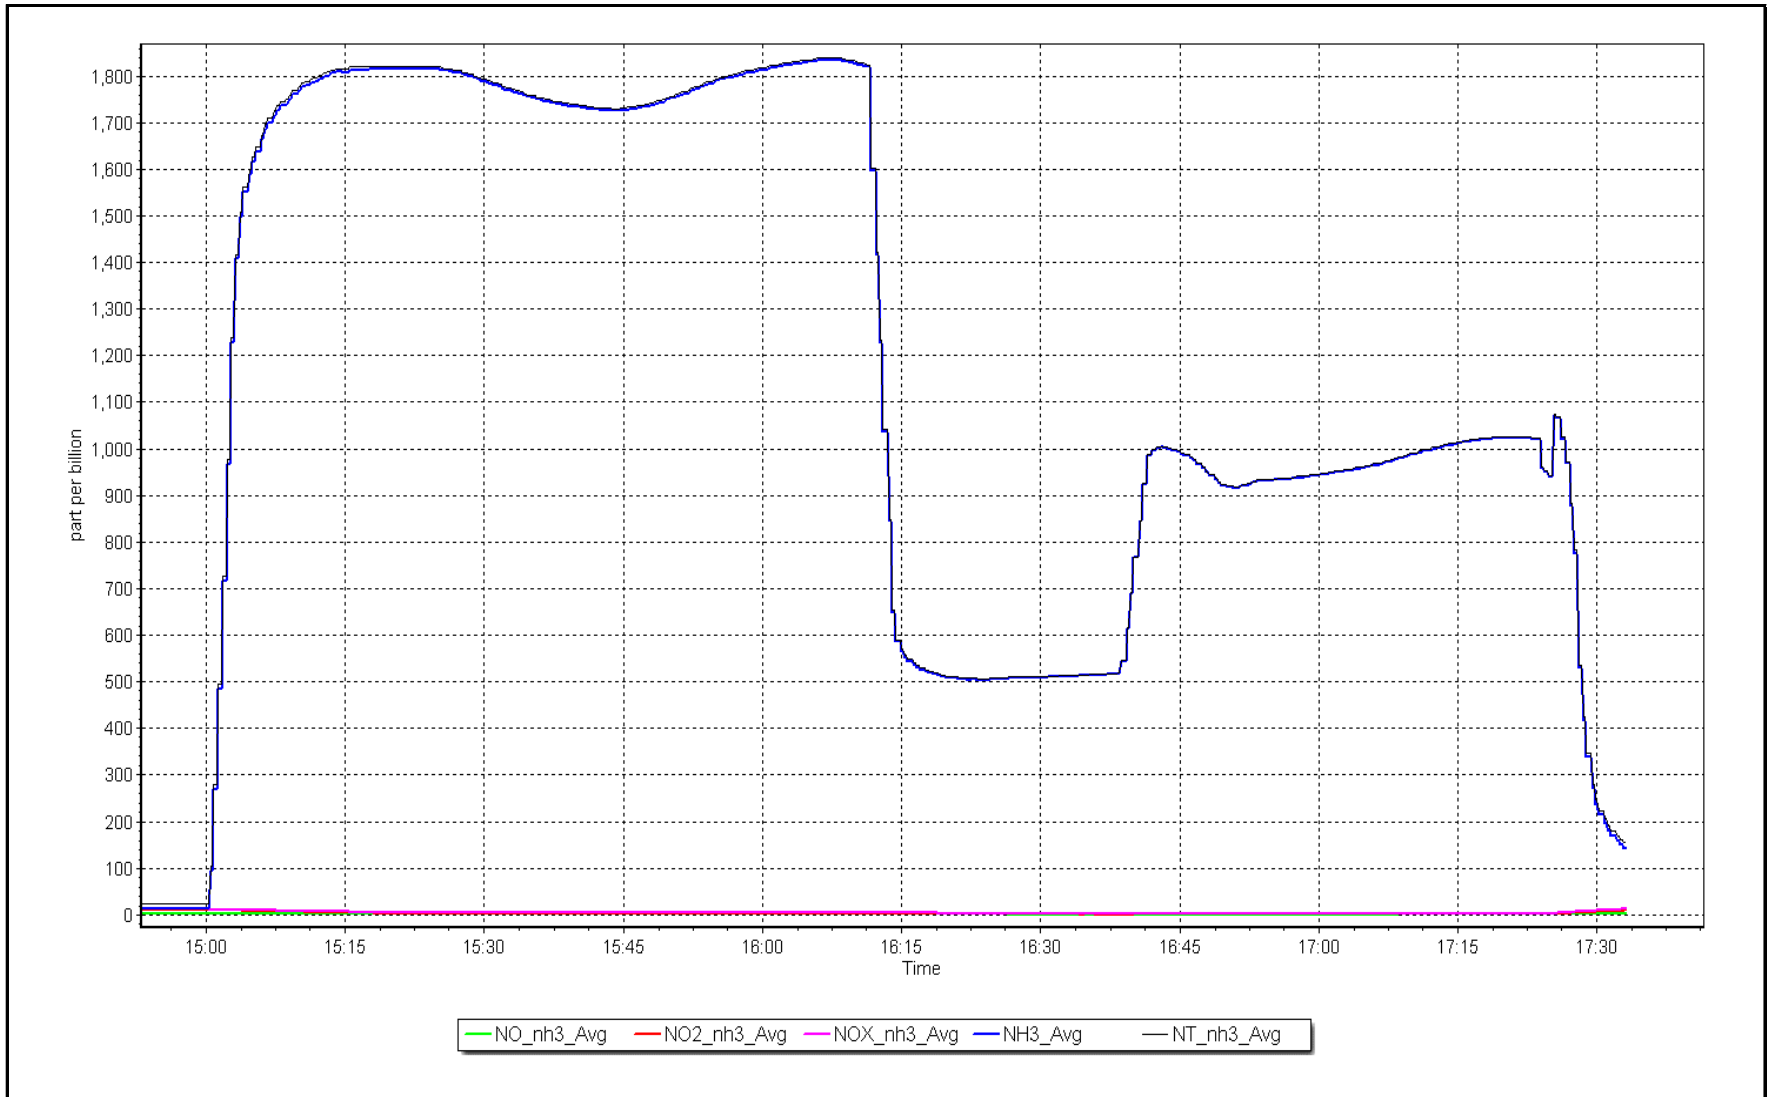



Wood Buffalo Environmental Association

TN - NO_x - NH₃ Calibration Report

Version-11-2021

Station Information

Station Name:	Bertha Ganter-Fort McKay	Station number:	AMS01
NOX Cal Date:	January 26, 2023	Last Cal Date:	N/A
Start time (MST):	13:00	End time (MST):	15:00
NH3 Cal Date:	January 26, 2023	Last Cal Date:	N/A
Start time (MST):	15:00	End time (MST):	17:00
Reason:	Install	Replaced the instrument	

Calibration Standards

NOX Cal Gas Conc:	50.84	ppm	NO Gas Cylinder #:	T2Y1P9L
NO Cal Gas Conc:	50.04	ppm	NO Cal Gas Expiry:	March 3, 2028
Removed NOX Conc:	50.84	ppm	Removed Cylinder #:	NA
Removed NO Conc:	50.04	ppm	Removed cyl Expiry:	NA
NOX gas Diff:			NO gas Diff:	
NH3 Cal Gas Conc:	72.93	ppm	NH3 Gas Cylinder #:	CC281298
Removed NH3 Conc:	72.93	ppm	NH3 Cal Gas Expiry:	February 28, 2023
NH3 gas Diff:			Removed Cylinder #:	
Calibrator Model:	Teledyne API T700		Serial Number:	3565
ZAG make/model:	Teledyne API T701		Serial Number:	5609

Analyzer Information

Analyzer model: Teledyne API T201E	Analyzer serial #: 56
Converter model: Teledyne API T501	Converter serial #: 217
NH3 Range (ppb): 0 - 2000 ppb	Reaction cell Press: 5.10
NOX Range (ppb): 0 - 1000 ppb	Sample Flow: 505

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coefficient:	N/A	0.793	TN coefficient:	N/A	0.806
NOX coefficient:	N/A	0.804	NO bkgrnd:	N/A	-1.500
NO2 coefficient:	N/A	1.000	NOX bkgrnd:	N/A	-0.400
NH3 coefficient:	N/A	0.919	TN bkgrnd:	N/A	3.100

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	N/A	1.001644
NO _x Cal Offset:	N/A	-0.440000
NO Cal Slope:	N/A	1.001856
NO Cal Offset:	N/A	-1.080000
NO ₂ Cal Slope:	N/A	0.999297
NO ₂ Cal Offset:	N/A	0.756159
NH3 Cal Slope:	N/A	0.988888
NH3 Cal Offset:	N/A	14.116543
TN Cal Slope:	N/A	0.996806
TN Cal Offset:	N/A	16.482567



Wood Buffalo Environmental Association

TN - NOX - NH₃ Calibration Report

Version-11-2021

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated TN concentration (ppb) (Cc)	Calculated NOX concentration (ppb) (Cc)	Calculated NH3 concentration (ppb) (Cc)	Indicated TN concentration (ppb) (Ic)	Indicated NOX concentration (ppb) (Ic)	Indicated NH3 concentration (ppb) (Ic)	TN Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NH3 Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	
as found zero											
as found NO											
calibrator zero	5000	0.0	0.0	0.0	0.0	0.5	0.3	0.2	----	----	
high NO point	4920	80.0	813.4	813.4	----	813.1	815.0	-2.0	1.000	----	
NO/O3 point											
as found NH3											
new NH3 cyl rp							----				
first NH3	3413	86.4	1800.6	----	1800.6	1794.1	----	1778.7	1.004	1.012	
second NH3	3452	48.0	1000.2	----	1000.2	1042.4	----	1031.0	0.960	0.970	
third NH3	3476	24.0	500.1	----	500.1	519.3	----	510.8	0.963	0.979	
									Average Correction Factor	1.0004	0.9872

Corrected As found TN = NA ppb NO_x = NA ppb NH3 = NA ppb

Previous Response TN = NA ppb NO_x = NA ppb NH3 = NA ppb

NH3 Previous Converter Efficiency = N/A

NH3 Current Converter Efficiency = 91.9%

*Percent Change TN = NA

*Percent Change NO_x = NA

*Percent Change NH3 = NA

* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

NO_x - NO - NO₂ Calibration Report

Version-11-2021

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated TN concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated TN concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero										
as found span										
new NO cyl rp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.3	0.3	0.5	----	----
high point	4920	80.0	813.4	800.6	813.4	815.0	801.9	813.1	0.9981	0.9984
second point	4960	40.0	406.7	400.3	406.7	405.7	398.8	405.9	1.0025	1.0038
third point	4980	20.0	203.4	200.2	203.4	203.1	198.4	200.9	1.0013	1.0089
Average Correction Factor									1.0006	1.0037

Baseline Corr As fnd TN = NA ppb NO_x = NA ppb NO = NA ppb *Percent Change TN = NA
 Previous Response TN = NA ppb NO_x = NA ppb NO = NA ppb *Percent Change NO_x = NA
 *Percent Change NO = NA
 * = > +/-5% change initiates investigation

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05 As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found zero						
calibration zero	----	----	0.0	-0.1	----	----
1st GPT point (400 ppb O3)	795.5	392.7	415.6	416.8	0.9971	100.3%
2nd GPT point (200 ppb O3)	795.5	581.5	226.8	224.8	1.0089	99.1%
3rd GPT point (100 ppb O3)	795.5	704.1	104.2	107.6	0.9684	103.3%
Average Correction Factor					0.9915	100.9%

Notes: Replaced the NH3 and the converter. Adjusted zero and span.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

TN Calibration Summary

Version-11-2021


Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	N/A
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	13:00	End Time (MST):	15:00
Analyzer make:	Teledyne API T201E	Analyzer serial #:	56

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.5	----	Correlation Coefficient	≥0.995	
1800.6	1794.1	1.0036			
1000.2	1042.4	0.9595			
500.1	519.3	0.9630			
			Slope	0.996806	0.90 - 1.10
			Intercept	16.482567	+/-20

TN Calibration Curve

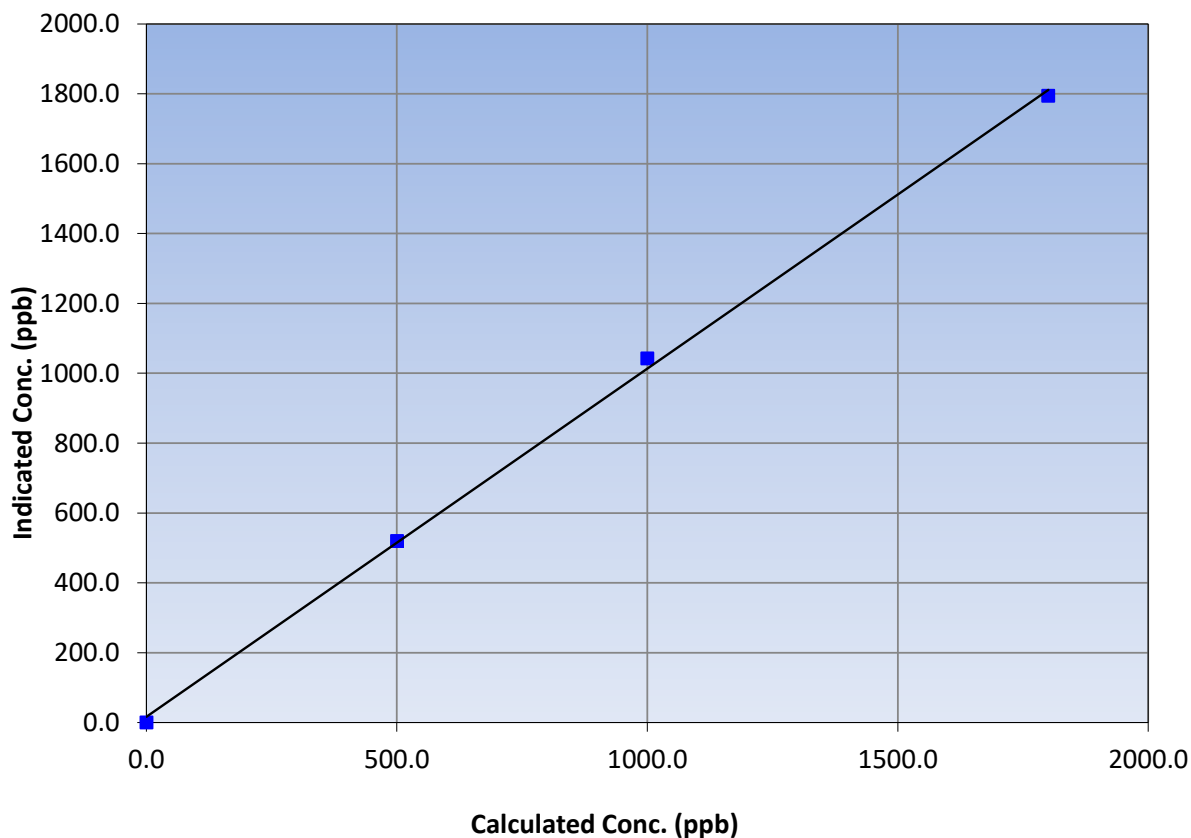



Wood Buffalo Environmental Association

NH₃ Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	N/A
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	13:00	End Time (MST):	15:00
Analyzer make:	Teledyne API T201E	Analyzer serial #:	56

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	0.2	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
1800.6	1778.7	1.0123		
1000.2	1031.0	0.9701		
500.1	510.8	0.9790		

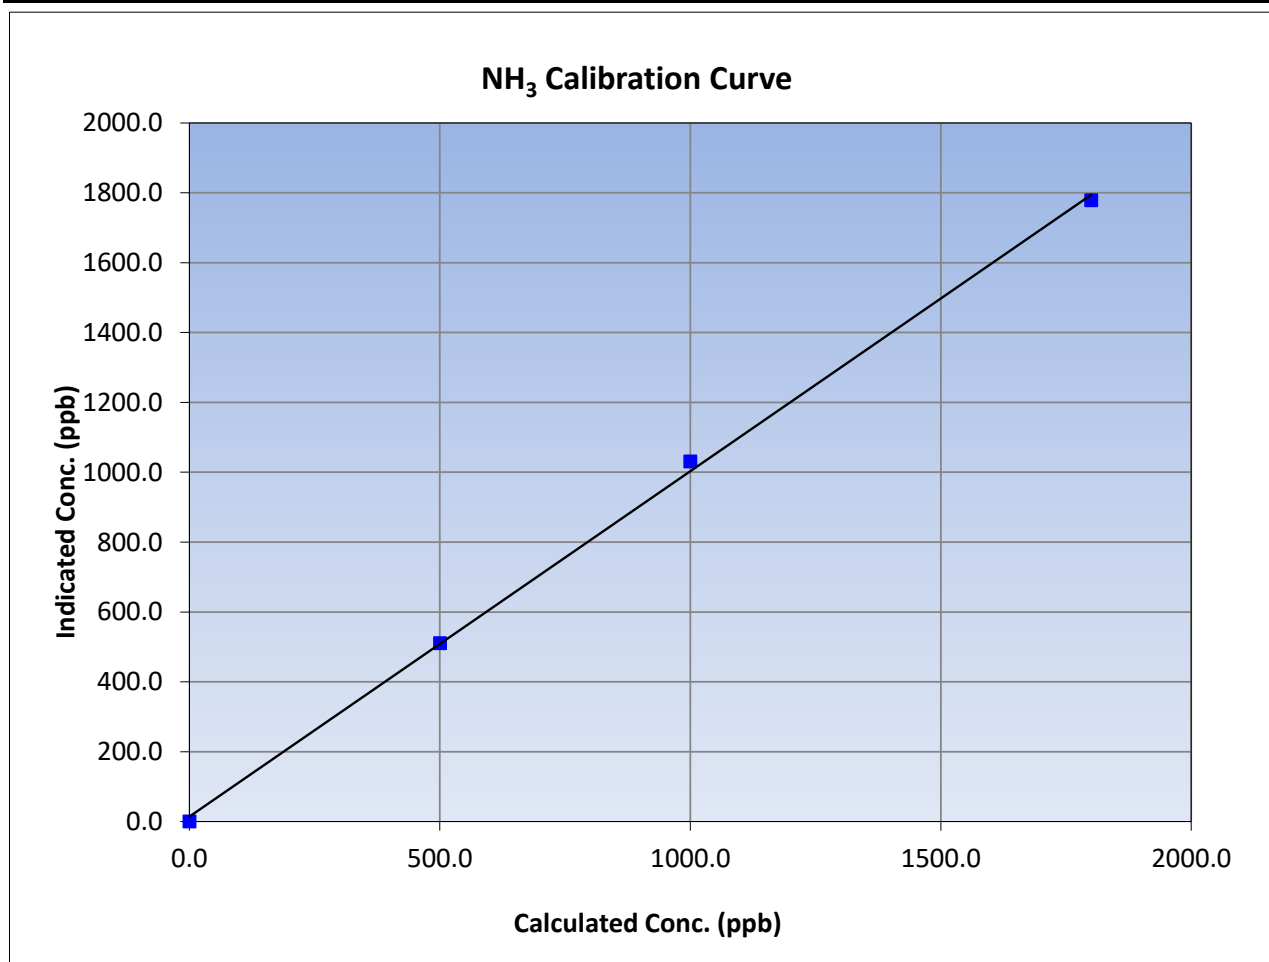



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	N/A
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	13:00	End Time (MST):	15:00
Analyzer make:	Teledyne API T201E	Analyzer serial #:	56

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.3	----	Correlation Coefficient	0.999993	
813.4	815.0	0.9981			≥0.995
406.7	405.7	1.0025	Slope	1.001644	
203.4	203.1	1.0013			0.90 - 1.10
			Intercept	-0.440000	+/-20

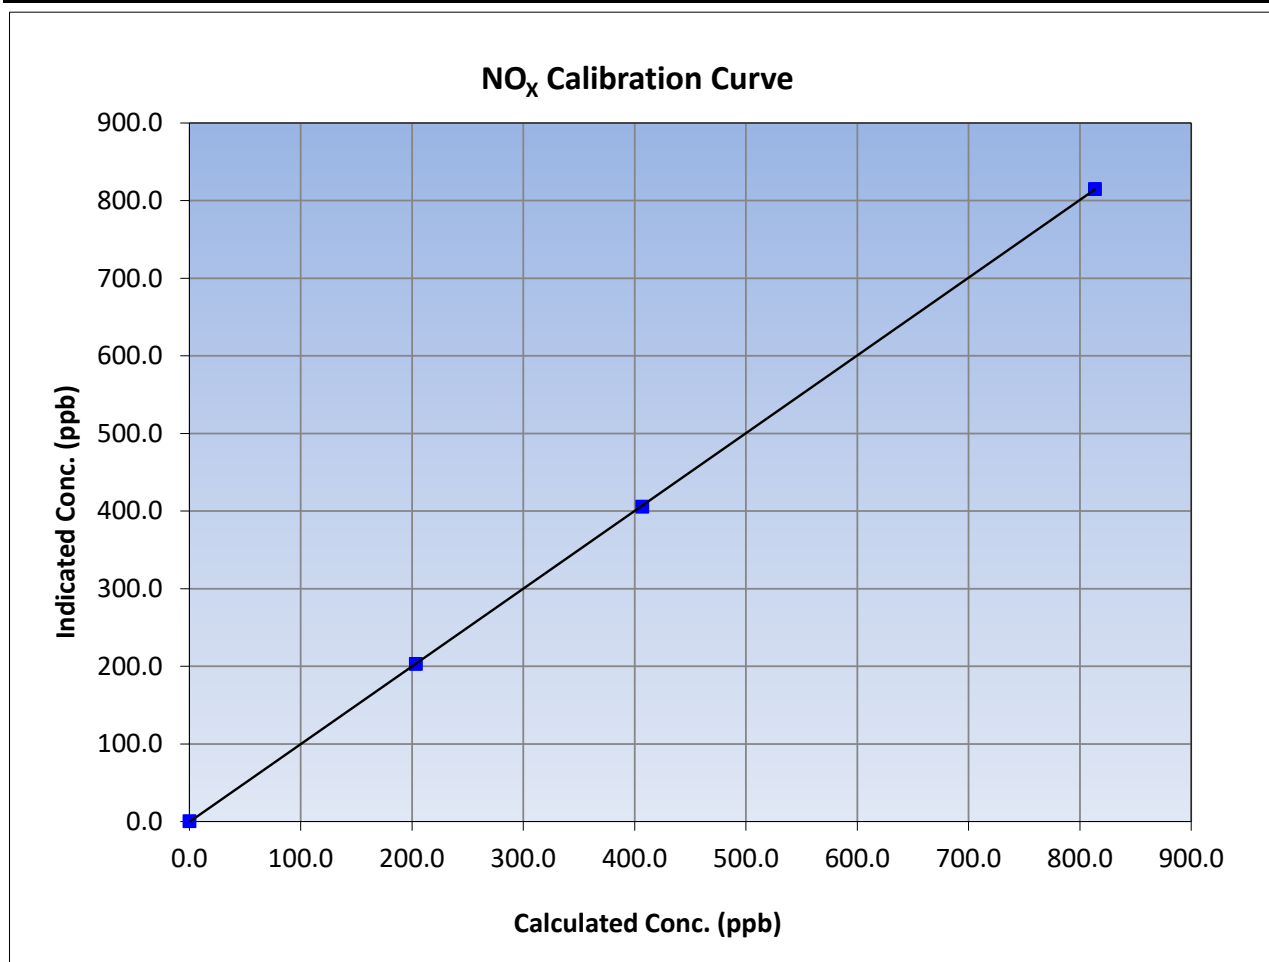



Wood Buffalo Environmental Association

NO Calibration Summary

Version-11-2021


Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	N/A
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	13:00	End Time (MST):	15:00
Analyzer make:	Teledyne API T201E	Analyzer serial #:	56

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.3	----	Correlation Coefficient	≥0.995	
800.6	801.9	0.9984			
400.3	398.8	1.0038			
200.2	198.4	1.0089			
			Slope	1.001856	0.90 - 1.10
			Intercept	-1.080000	+/-20

NO Calibration Curve

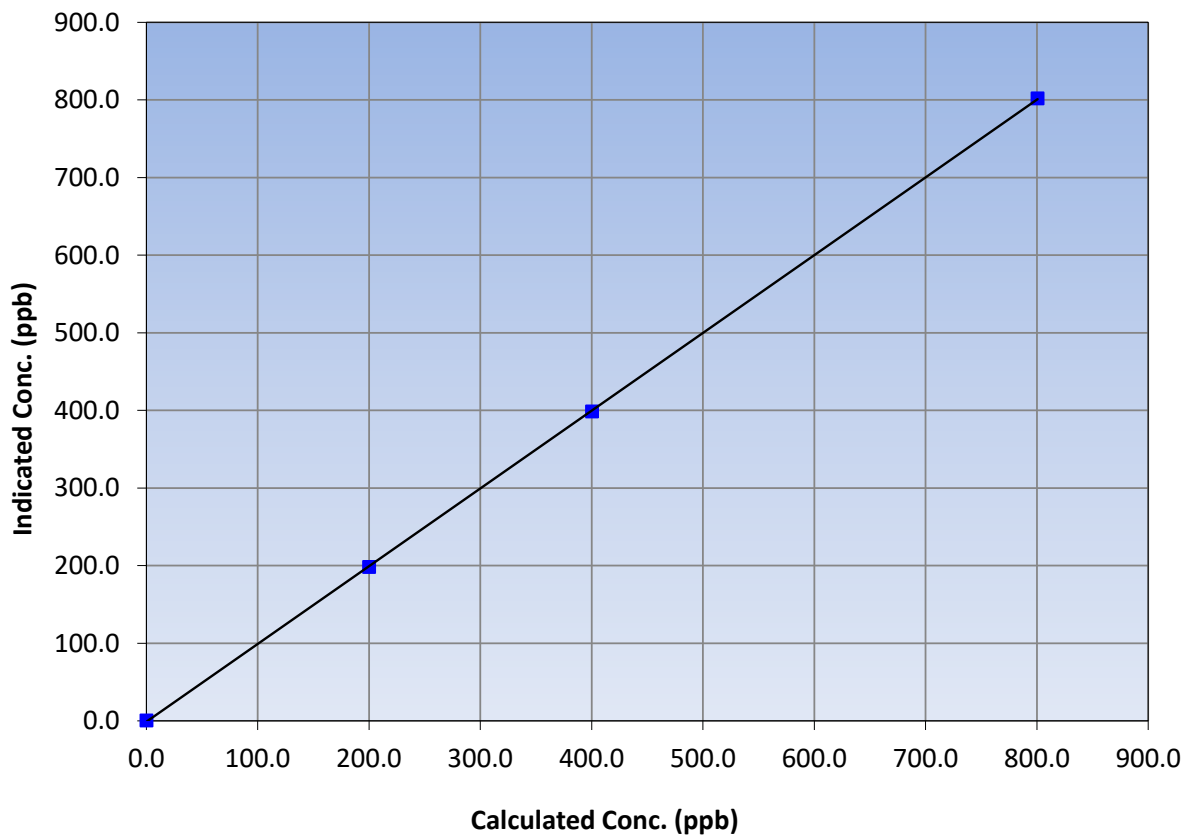



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-11-2021


Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	N/A
Station Name:	Bertha Ganter-Fort McKay	Station Number:	AMS01
Start Time (MST):	13:00	End Time (MST):	15:00
Analyzer make:	Teledyne API T201E	Analyzer serial #:	56

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	-0.1	----	Correlation Coefficient	≥0.995
415.6	416.8	0.9971		
226.8	224.8	1.0089	Slope	0.90 - 1.10
104.2	107.6	0.9684		
			Intercept	+/-20


NO₂ Calibration Curve

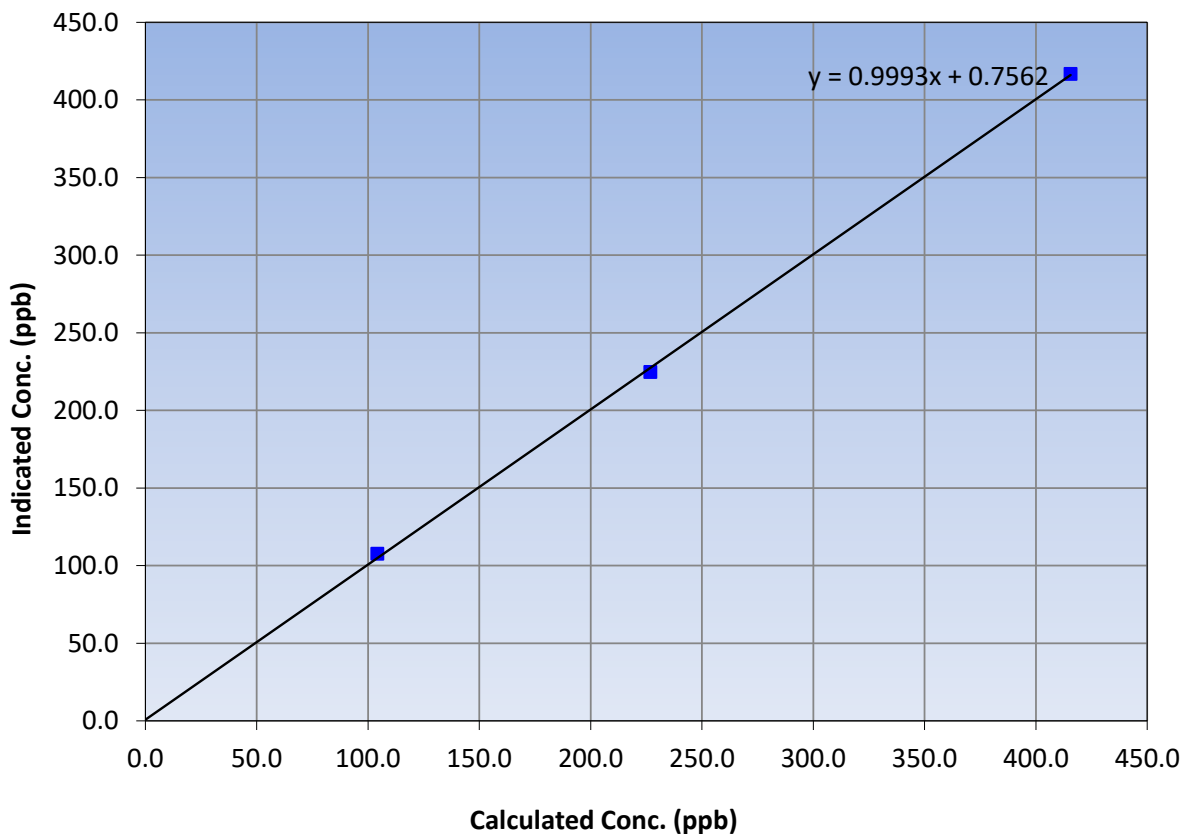

NO_x Calibration Plot

Date: January 26, 2023


Location: Bertha Ganter-Fort McKay

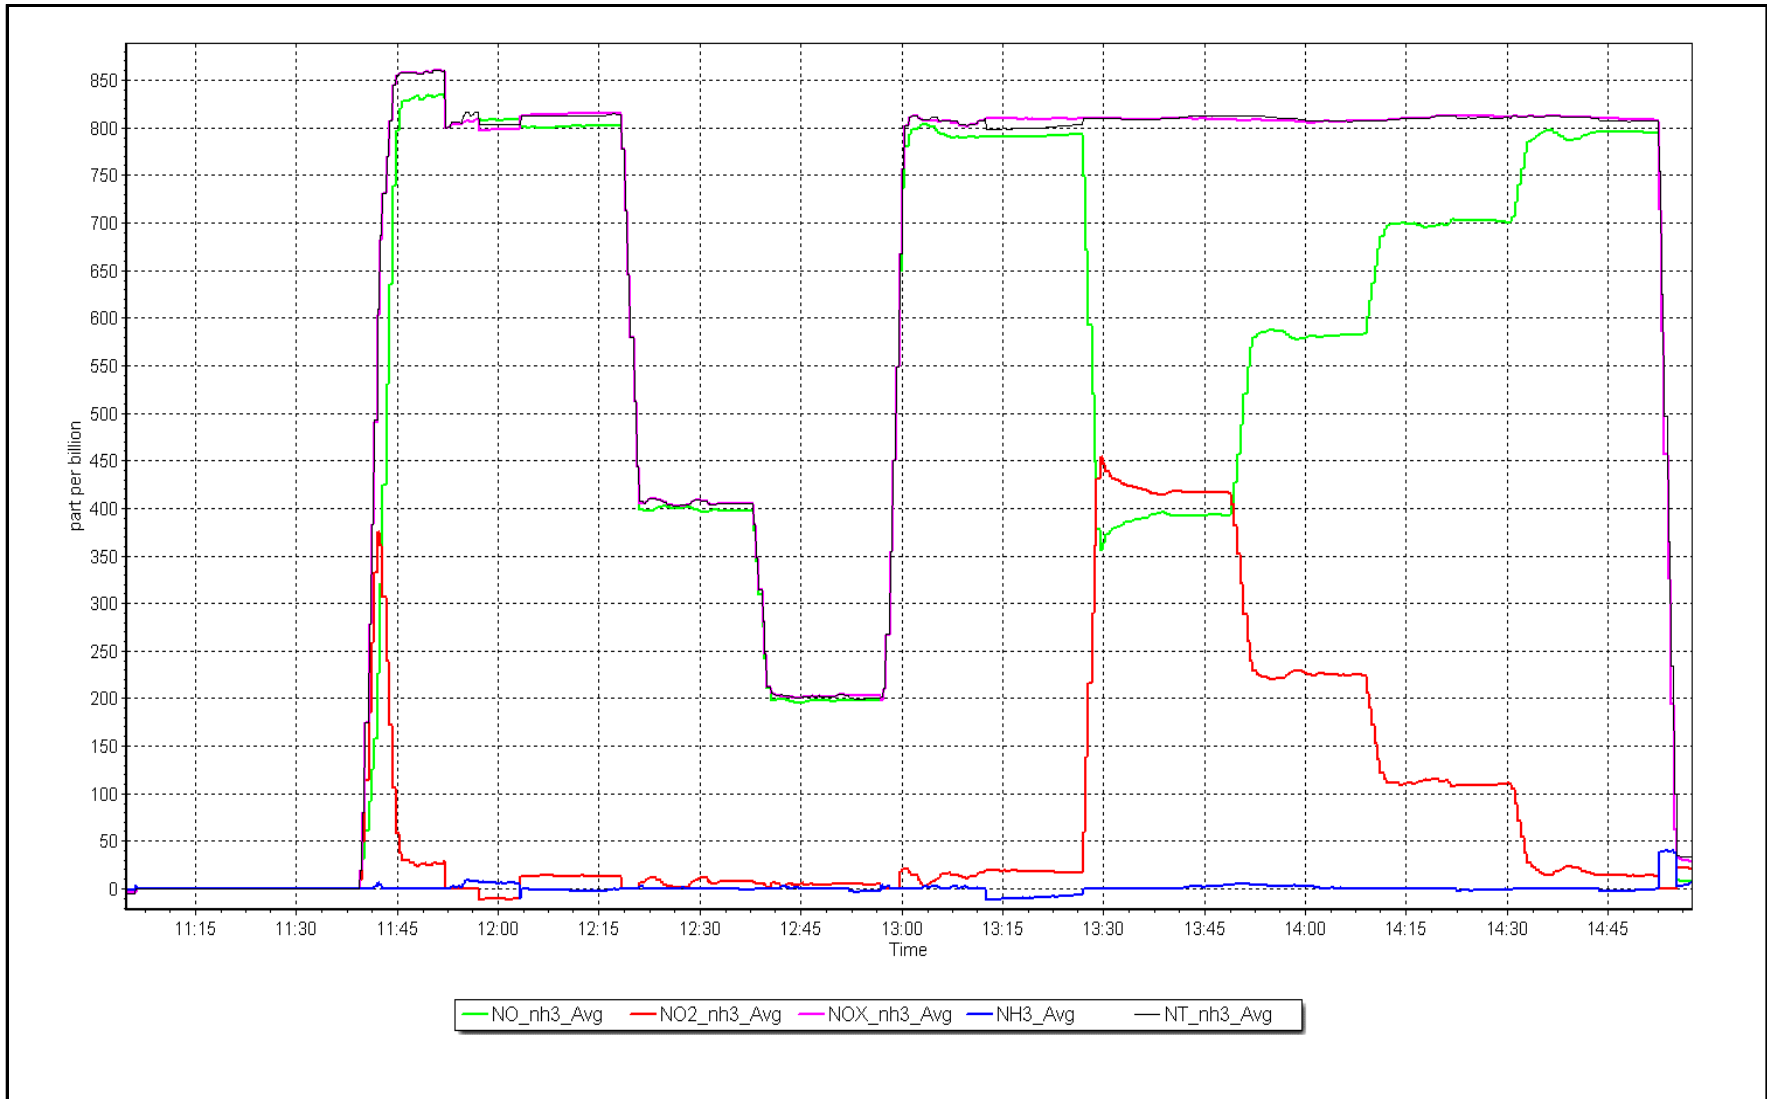

NH₃ Calibration Plot

Date: January 26, 2023

Location: Bertha Ganter-Fort McKay

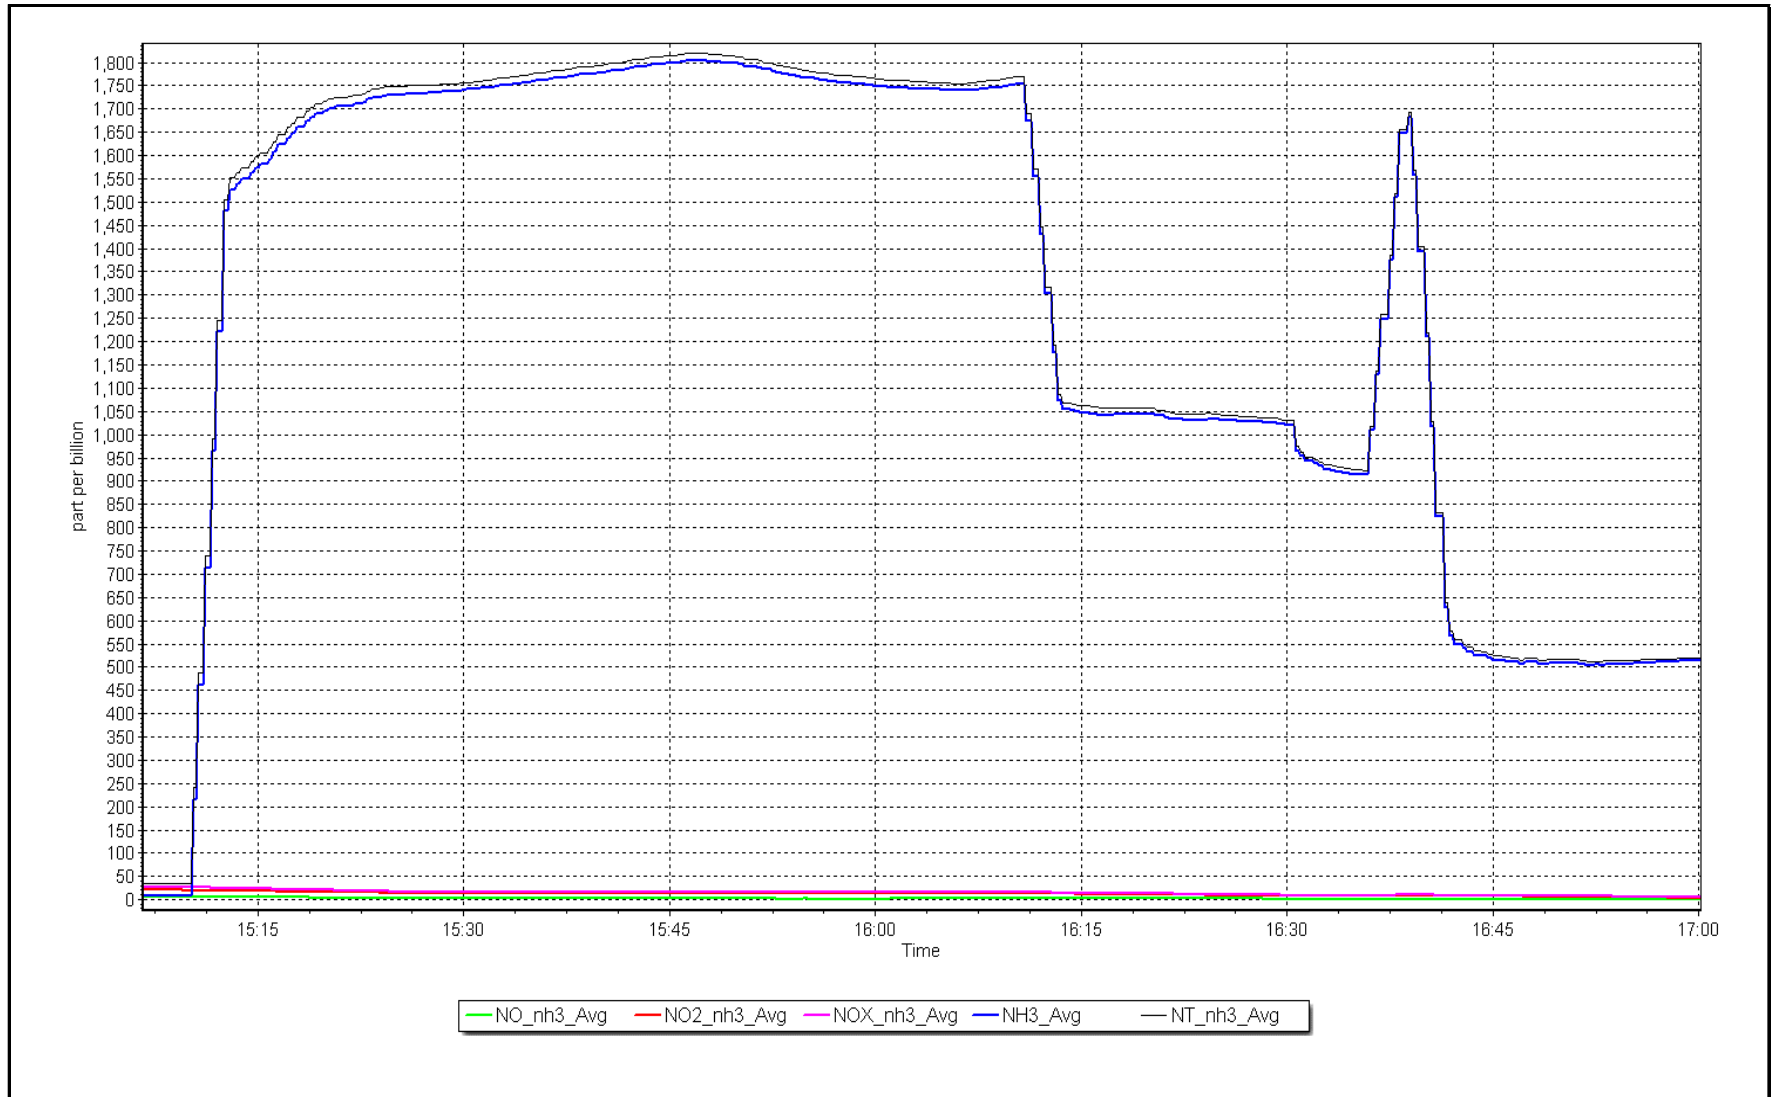



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS02 MILDRED LAKE JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Mildred Lake	Station number:	AMS02
Calibration Date:	January 3, 2023	Last Cal Date:	December 5, 2022
Start time (MST):	11:03	End time (MST):	13:53
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.98	ppm	Cal Gas Exp Date:	August 12, 2024
Cal Gas Cylinder #:	CC501209			
Removed Cal Gas Conc:	49.98	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	1185
ZAG Make/Model:	API T701		Serial Number:	5608

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	JC1404901075
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.997165	0.996082	Backgd or Offset:	17.6	17.8
Calibration intercept:	-0.305608	-0.526045	Coeff or Slope:	0.816	0.816

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4920	80.2	801.6	794.3	1.009
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.5	----
high point	4920	80.2	801.6	798.6	1.004
second point	4960	40.1	400.8	397.9	1.007
third point	4980	20.0	199.9	197.8	1.011
as left zero	5000	0.0	0.0	0.2	----
as left span	4920	80.2	801.6	789.6	1.015
Average Correction Factor					1.007

Baseline Corr As found:	794.20	Previous response	799.07	*% change	-0.6%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed inlet filter after as founds. No adjustments needed.

Calibration Performed By: Ryan Power



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 5, 2022
Station Name:	Mildred Lake	Station Number:	AMS02
Start Time (MST):	11:03	End Time (MST):	13:53
Analyzer make:	Thermo 43i	Analyzer serial #:	JC1404901075

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.5	----	Correlation Coefficient	0.999992	≥0.995
801.6	798.6	1.0038			
400.8	397.9	1.0074	Slope	0.996082	0.90 - 1.10
199.9	197.8	1.0107			
			Intercept	-0.526045	+/-30

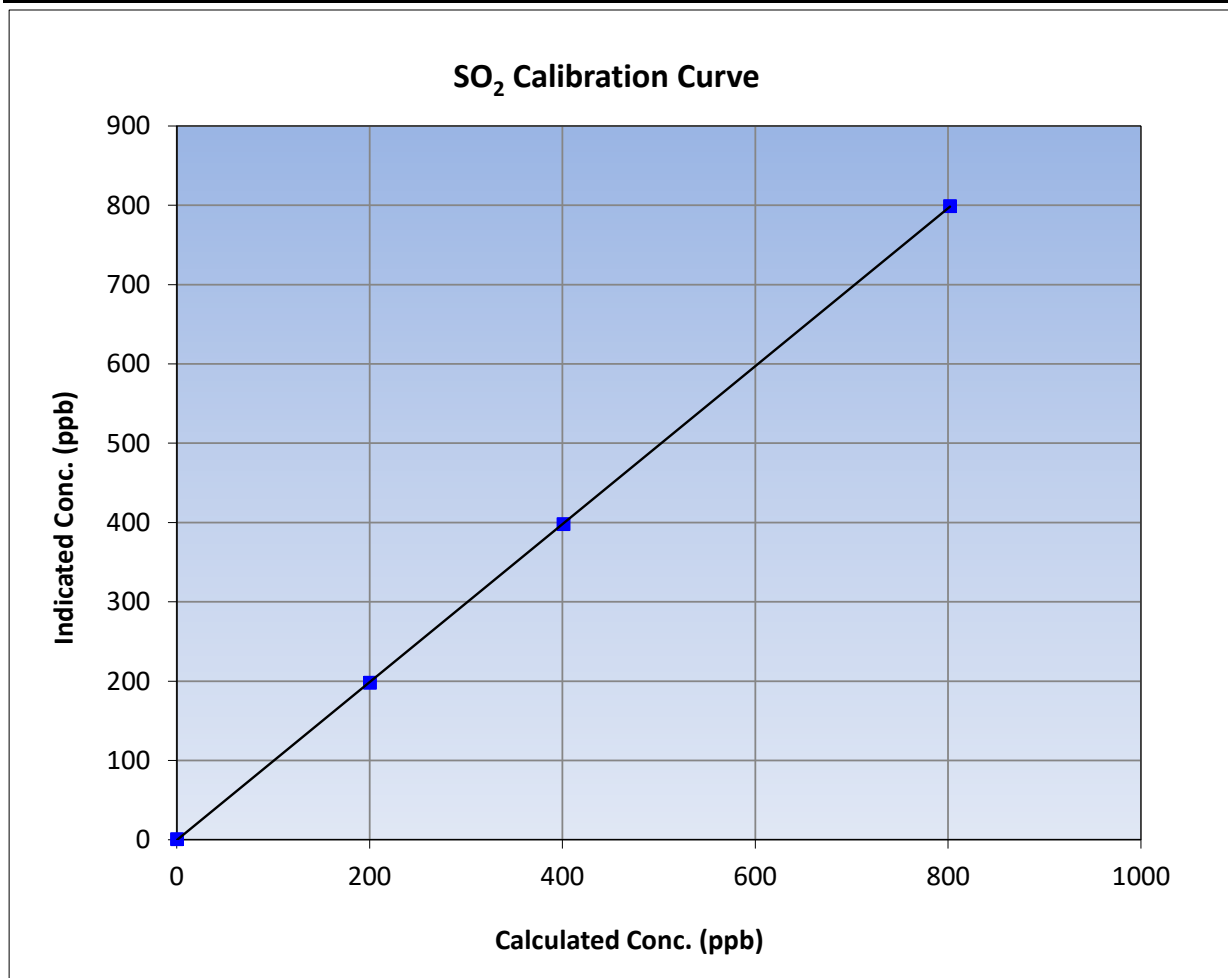

SO2 Calibration Plot

Date: January 3, 2023

Location: Mildred Lake

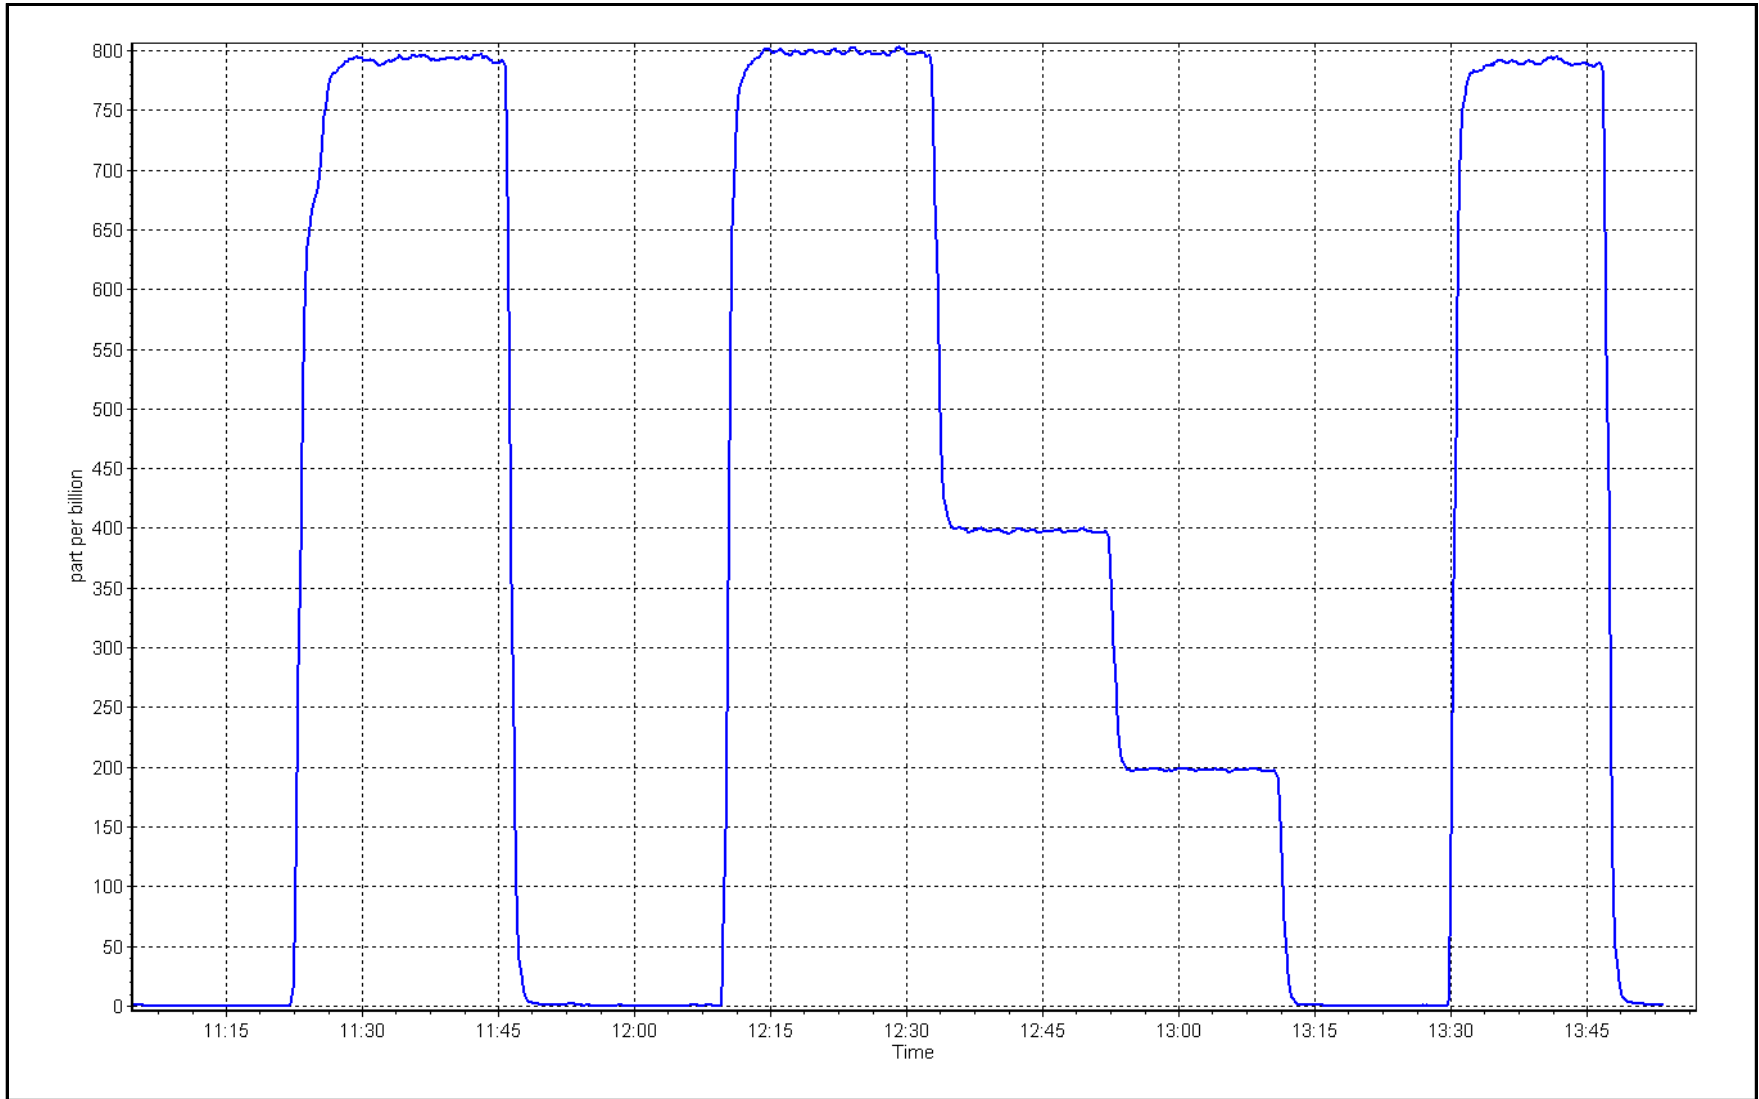



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Mildred Lake Station number: AMS02
 Calibration Date: January 17, 2023 Last Cal Date: December 20, 2022
 Start time (MST): 10:31 End time (MST): 14:39
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.29 ppm Cal Gas Exp Date: January 4, 2025
 Cal Gas Cylinder #: CC345191
 Removed Cal Gas Conc: 5.29 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 1185
 ZAG Make/Model: API T701 Serial Number: 5608

Analyzer Information

Analyzer make: Thermo 43iQTL Analyzer serial #: 12113311966
 Converter make: Global G150 Converter serial #: 2022-198
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	1.012680	1.010965	Backgd or Offset: 1.88	1.83
Calibration intercept:	-0.239192	-0.179192	Coeff or Slope: 0.887	0.844

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	-0.2	----
as found span	4924	75.6	80.0	84.7	0.942
as found 2nd point	4962	37.8	40.0	42.4	0.939
as found 3rd point	4981	18.9	20.0	20.7	0.957
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	-0.1	----
high point	4924	75.6	80.0	80.7	0.991
second point	4962	37.8	40.0	40.3	0.992
third point	4981	18.9	20.0	19.9	1.005
as left zero	5000	0.0	0.0	0.1	----
as left span	4924	75.6	80.0	80.4	0.995
SO2 Scrubber Check	4920	80.2	802.0	0.0	----
Date of last scrubber change:	12-Sep-22			Ave Corr Factor	0.996
Date of last converter efficiency test:	efficiency				

Baseline Corr As found:	84.9	Prev response:	80.77	*% change:	4.9%
Baseline Corr 2nd AF pt:	42.6	AF Slope:	1.062971	AF Intercept:	-0.299150
Baseline Corr 3rd AF pt:	20.9	AF Correlation:	0.999972		

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds. Ran a SO2 scrubber check after calibrator zero. As found points are high, diagnostics are good, suspecting the scrubber bead hydration level change is the cause of these high points. Adjusted the span.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 20, 2022
Station Name:	Mildred Lake	Station Number:	AMS02
Start Time (MST):	10:31	End Time (MST):	14:39
Analyzer make:	API T700	Analyzer serial #:	1185

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	-0.1	----	Correlation Coefficient	0.999992	≥0.995
80.0	80.7	0.9912			
40.0	40.3	0.9924	Slope	1.010965	0.90 - 1.10
20.0	19.9	1.0049			
			Intercept	-0.179192	+/-3

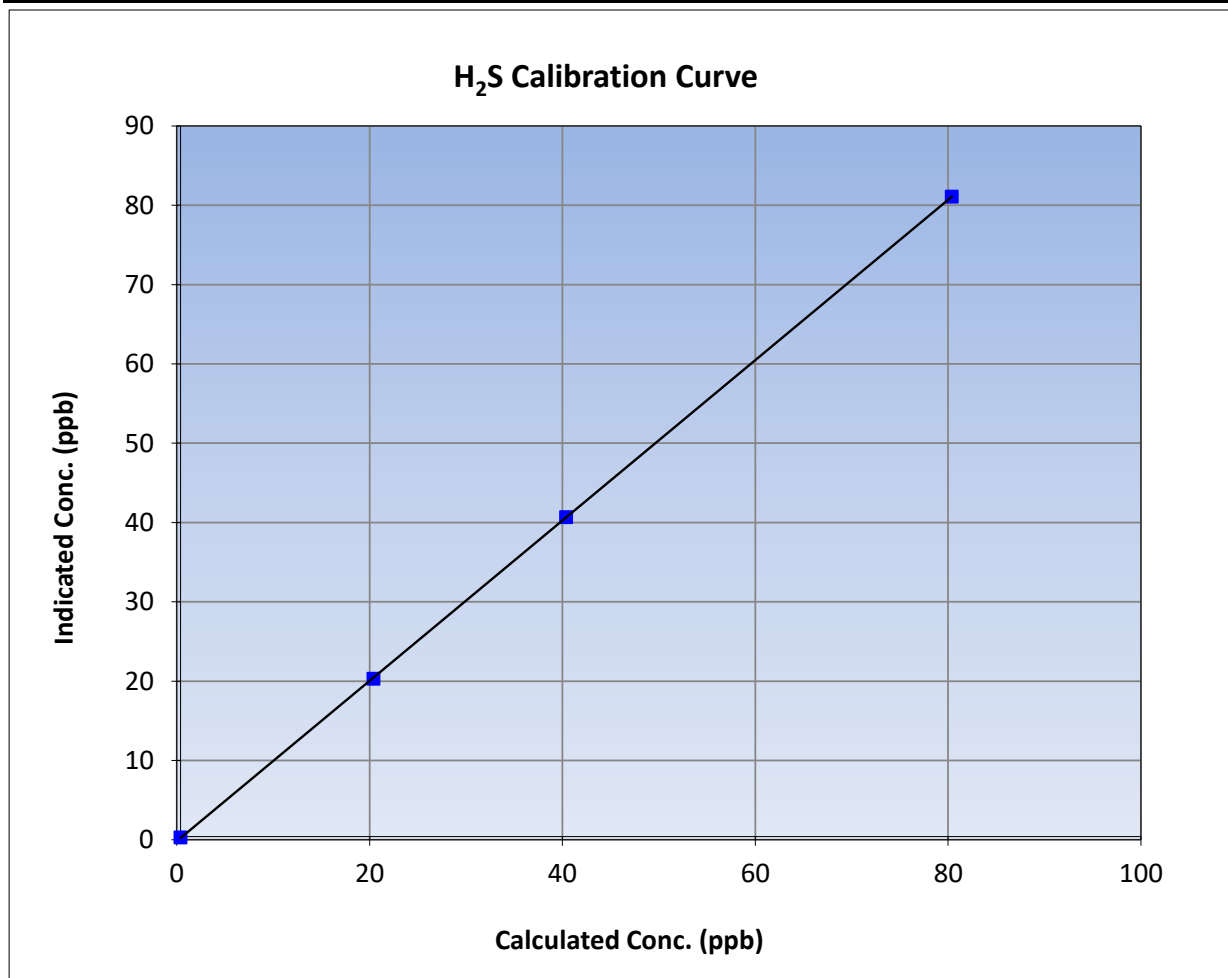

H₂S Calibration Plot

Date: January 17, 2023

Location: Mildred Lake

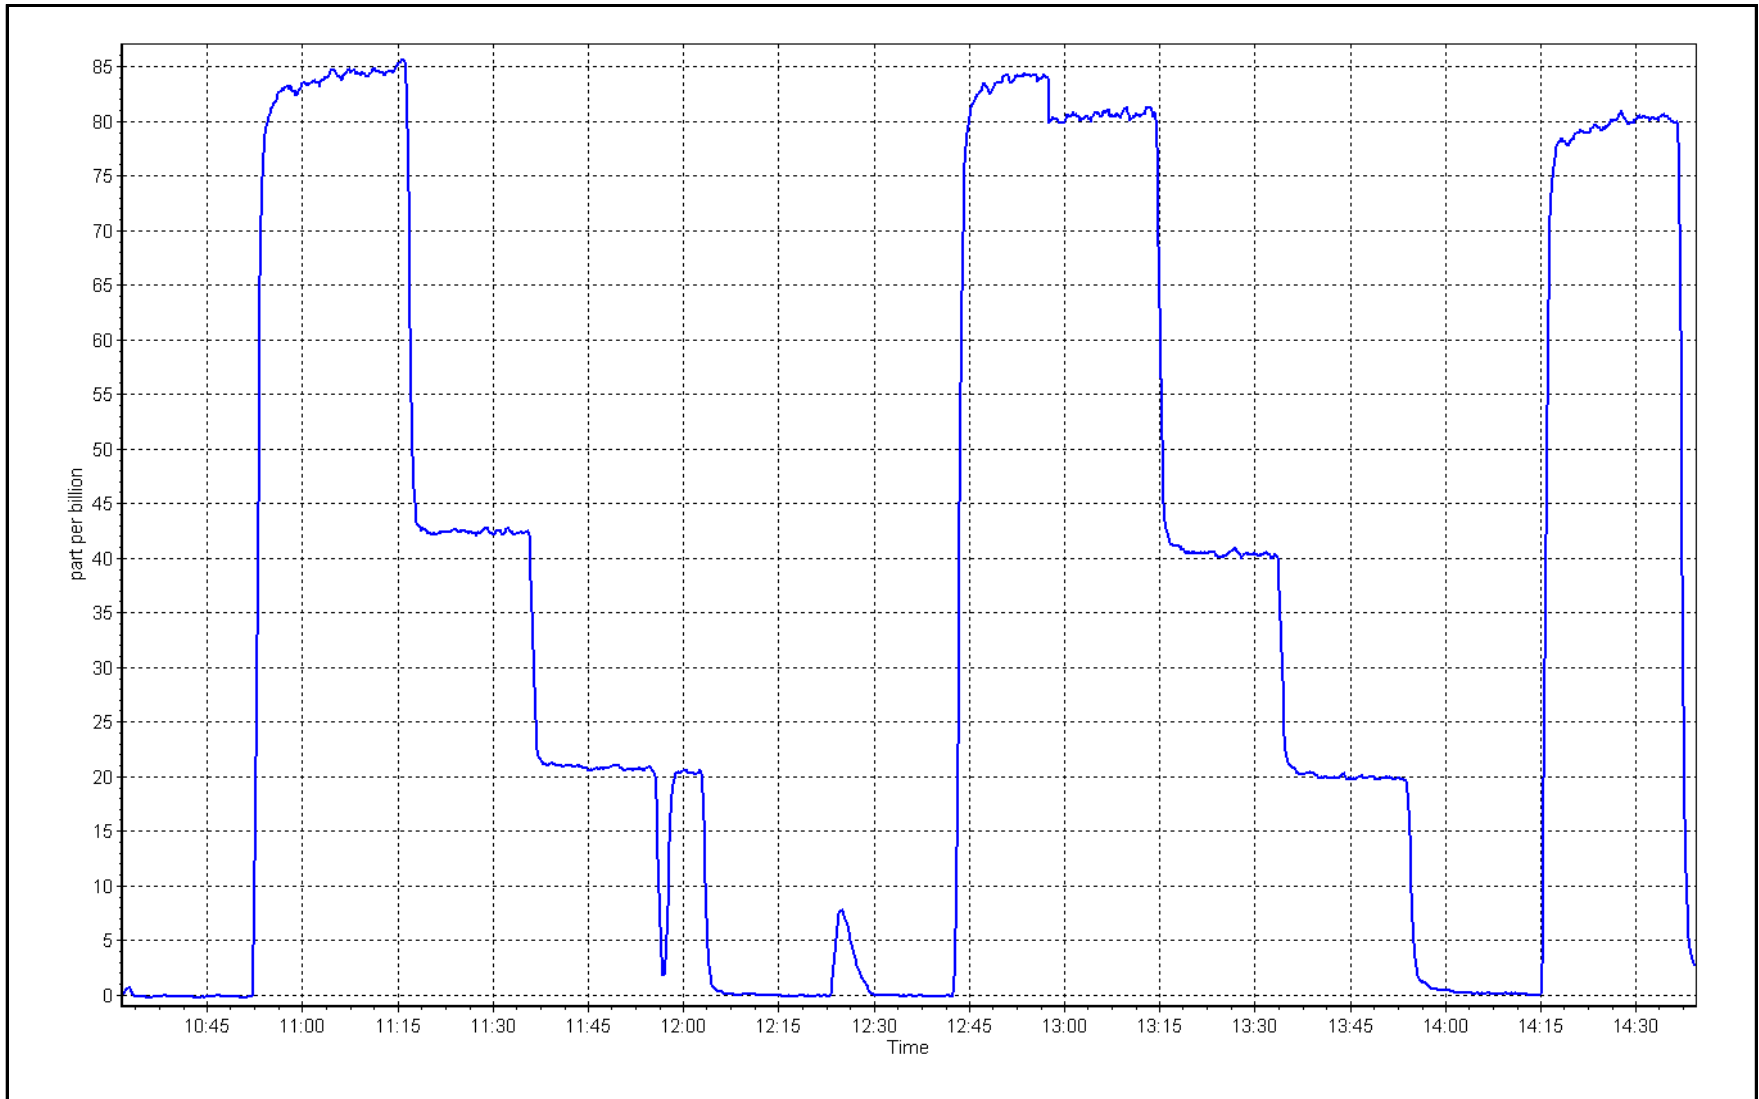



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-06-2022

Station Information

Station Name:	Mildred Lake	Station number:	AMS02
Calibration Date:	January 3, 2023	Last Cal Date:	December 5, 2022
Start time (MST):	11:03	End time (MST):	13:49
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC501209	Cal Gas Expiry Date:	August 12, 2024
CH ₄ Cal Gas Conc.	500.2 ppm	CH ₄ Equiv Conc.	1048.6 ppm
C ₃ H ₈ Cal Gas Conc.	199.4 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	
Removed CH ₄ Conc.	500.2 ppm	CH ₄ Equiv Conc.	1048.6 ppm
Removed C ₃ H ₈ Conc.	199.4 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	Teledyne API T700	Serial Number:	1185
ZAG make/model:	Teledyne API T701	Serial Number:	5608

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1180320038
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	2.87E-04	2.87E-04	NMHC SP Ratio:	4.52E-04
CH ₄ Retention time:	14.6	14.6	NMHC Peak Area:	194883
Zero Chromatogram:	ON	ON	Flat Baseline:	OFF

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.2	16.82	16.89	0.996
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.2	16.82	16.87	0.997
second point	4960	40.1	8.41	8.40	1.001
third point	4980	20.0	4.19	4.18	1.002
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.2	16.82	16.90	0.995
Average Correction Factor					1.000

Baseline Corr AF:	16.89	Prev response	16.79	*% change	0.6%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = +/-5% change initiates investigation	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-06-2022

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.2	8.80	8.82	0.998
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.2	8.80	8.79	1.000
second point	4960	40.1	4.40	4.40	1.000
third point	4980	20.0	2.19	2.20	0.997
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.2	8.80	8.83	0.996
Average Correction Factor					0.999
Baseline Corr AF:	8.82	Prev response	8.78	*% change	0.4%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.2	8.02	8.08	0.993
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.2	8.02	8.07	0.994
second point	4960	40.1	4.01	4.01	1.002
third point	4980	20.0	2.00	1.99	1.008
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.2	8.02	8.06	0.995
Average Correction Factor					1.001
Baseline Corr AF:	8.08	Prev response	8.01	*% change	0.9%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	0.999538	1.003029
THC Cal Offset:	-0.018717	-0.014898
CH ₄ Cal Slope:	1.000755	1.006623
CH ₄ Cal Offset:	-0.017454	-0.017040
NMHC Cal Slope:	0.998193	0.999387
NMHC Cal Offset:	-0.000864	0.002541

Notes: Changed inlet filter and H2 cylinder after As Finds. No adjustments needed

Calibration Performed By: Ryan Power



Wood Buffalo Environmental Association

THC Calibration Summary


Version-06-2022

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 5, 2022
Station Name:	Mildred Lake	Station Number:	AMS02
Start Time (MST):	11:03	End Time (MST):	13:49
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320038

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999995	≥ 0.995			
16.82	16.87	0.9972						
8.41	8.40	1.0009				Slope	1.003029	0.90 - 1.10
4.19	4.18	1.0024						
			Intercept	-0.014898	± 0.5			

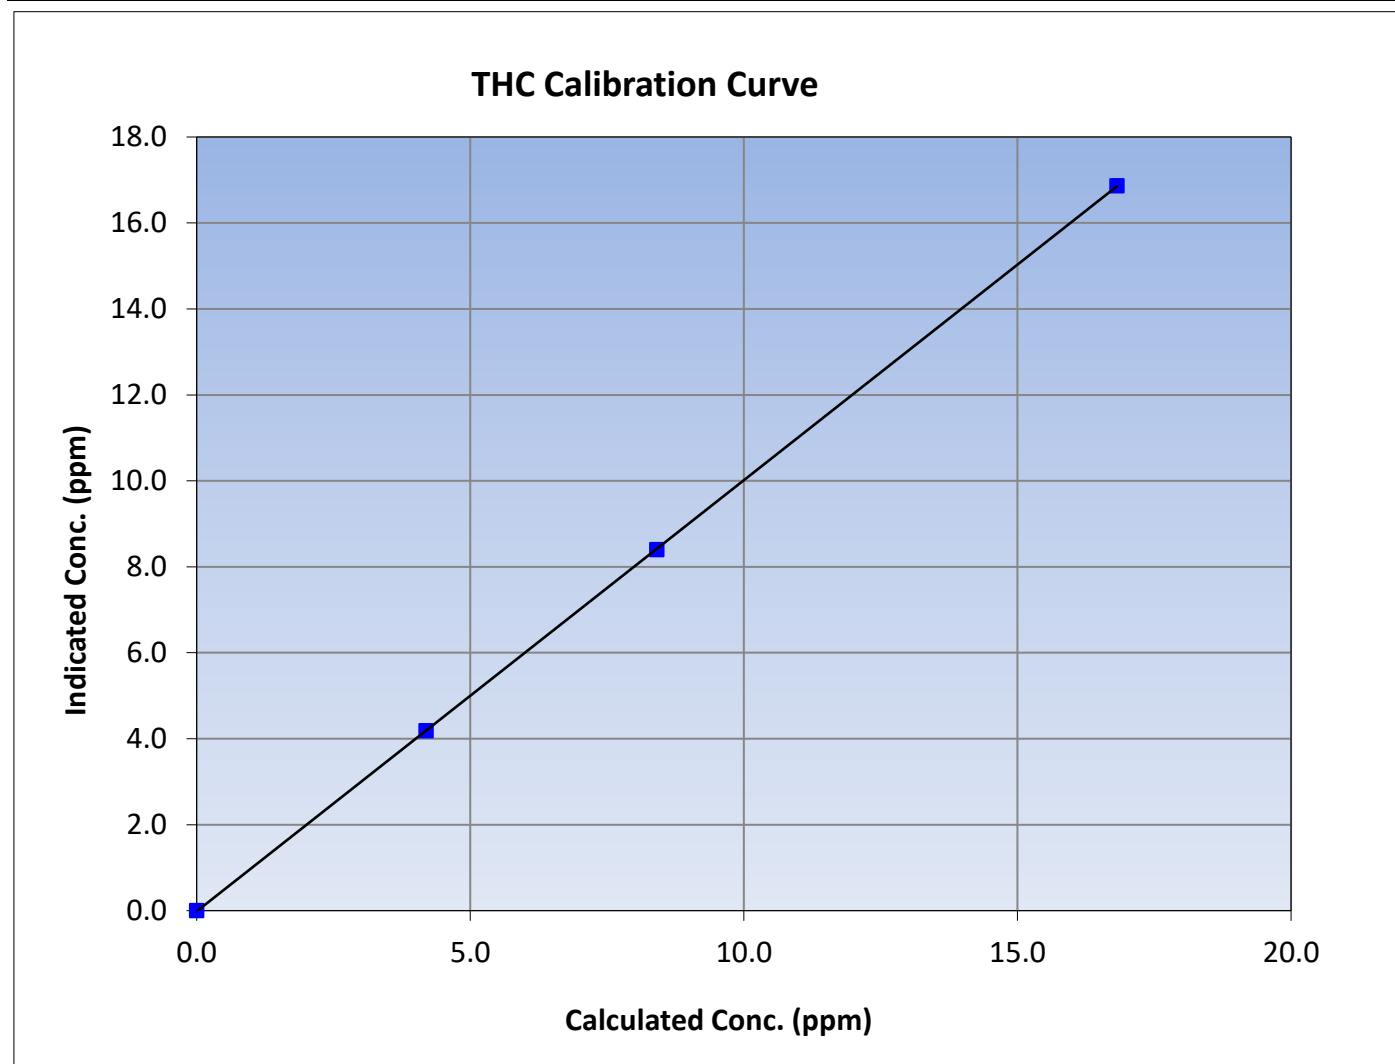



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-06-2022

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 5, 2022
Station Name:	Mildred Lake	Station Number:	AMS02
Start Time (MST):	11:03	End Time (MST):	13:49
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320038

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999977	≥0.995
8.02	8.07	0.9942			
4.01	4.01	1.0016	Slope	1.006623	0.90 - 1.10
2.00	1.99	1.0080			
			Intercept	-0.017040	+/-0.5

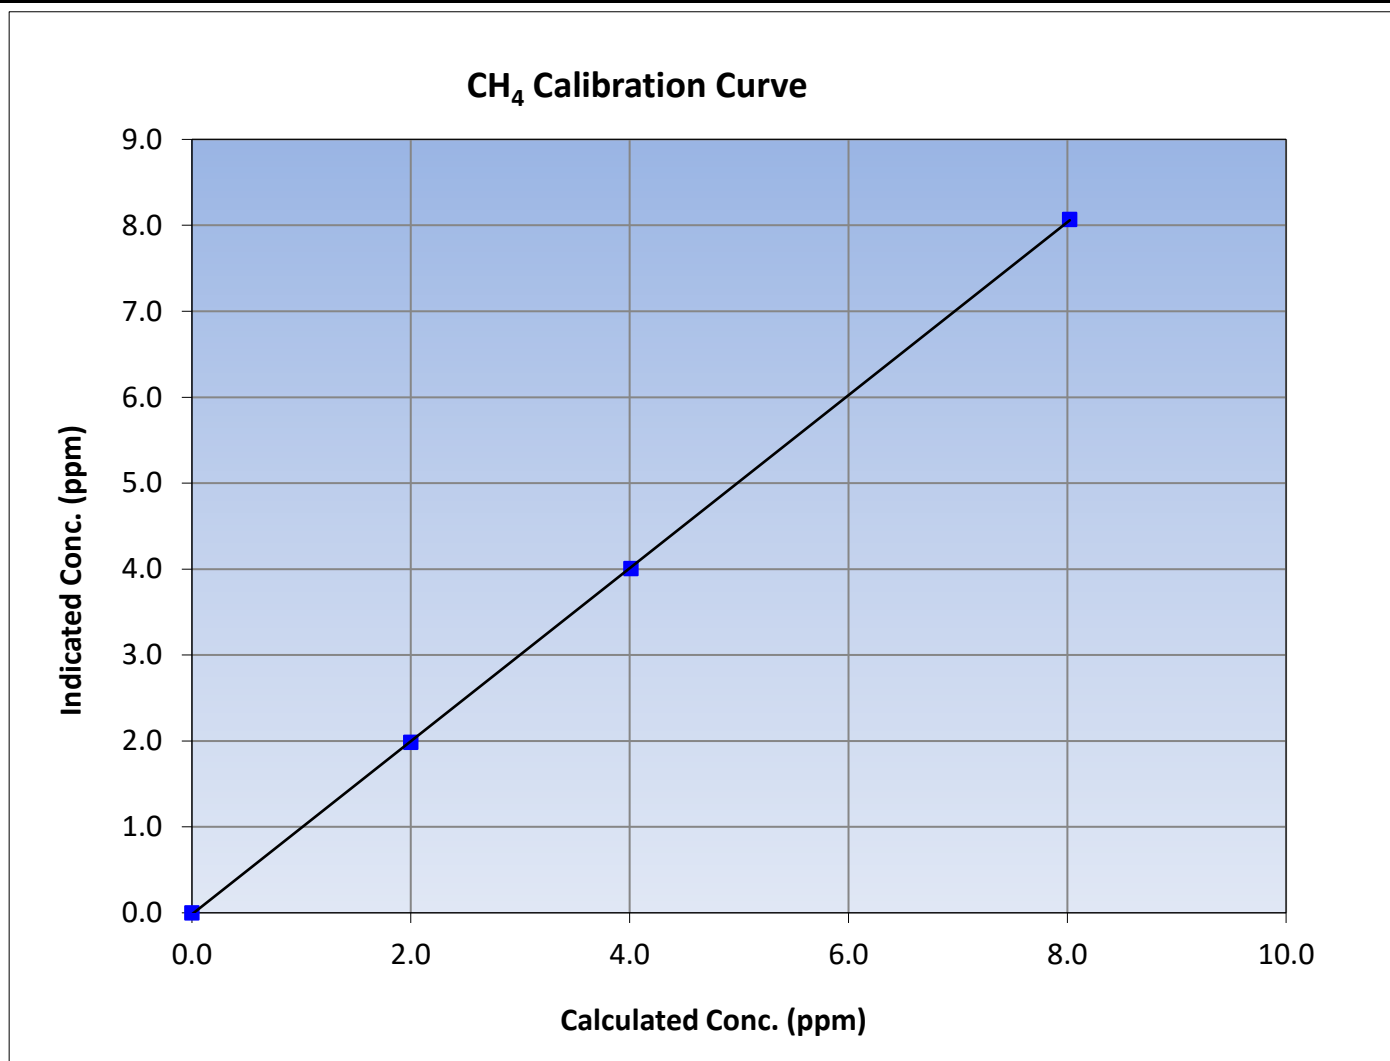



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-06-2022

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 5, 2022
Station Name:	Mildred Lake	Station Number:	AMS02
Start Time (MST):	11:03	End Time (MST):	13:49
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320038

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999999	≥ 0.995			
8.80	8.79	1.0004						
4.40	4.40	1.0004				Slope	0.999387	0.90 - 1.10
2.19	2.20	0.9975						
			Intercept	0.002541	± 0.5			

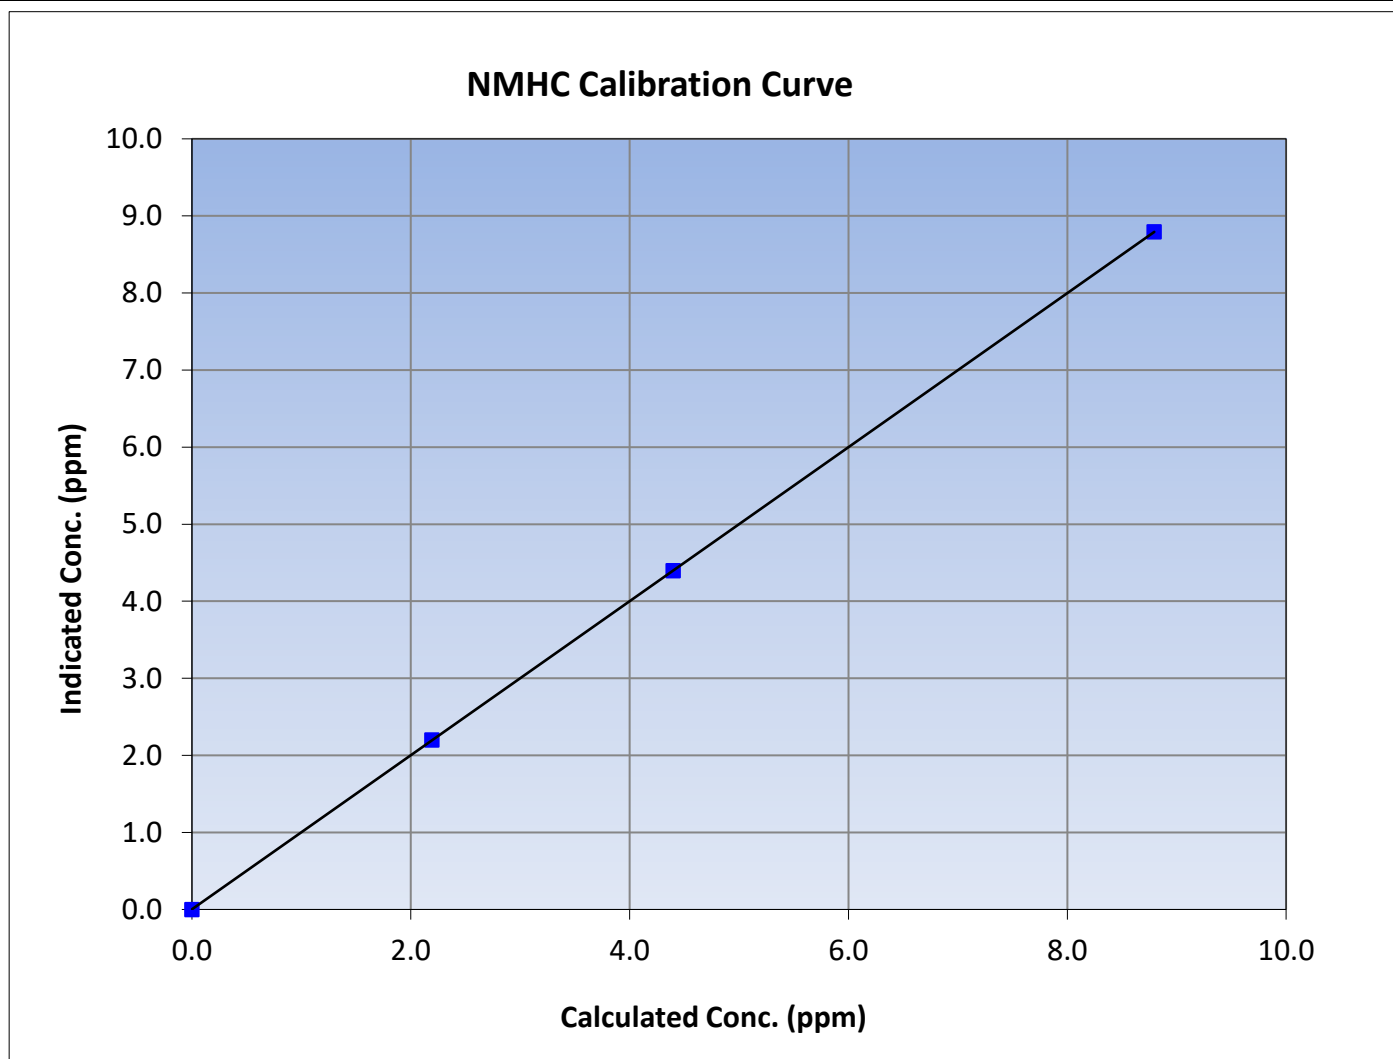

NMHC Calibration Plot

Date: January 3, 2023

Location: Mildred Lake

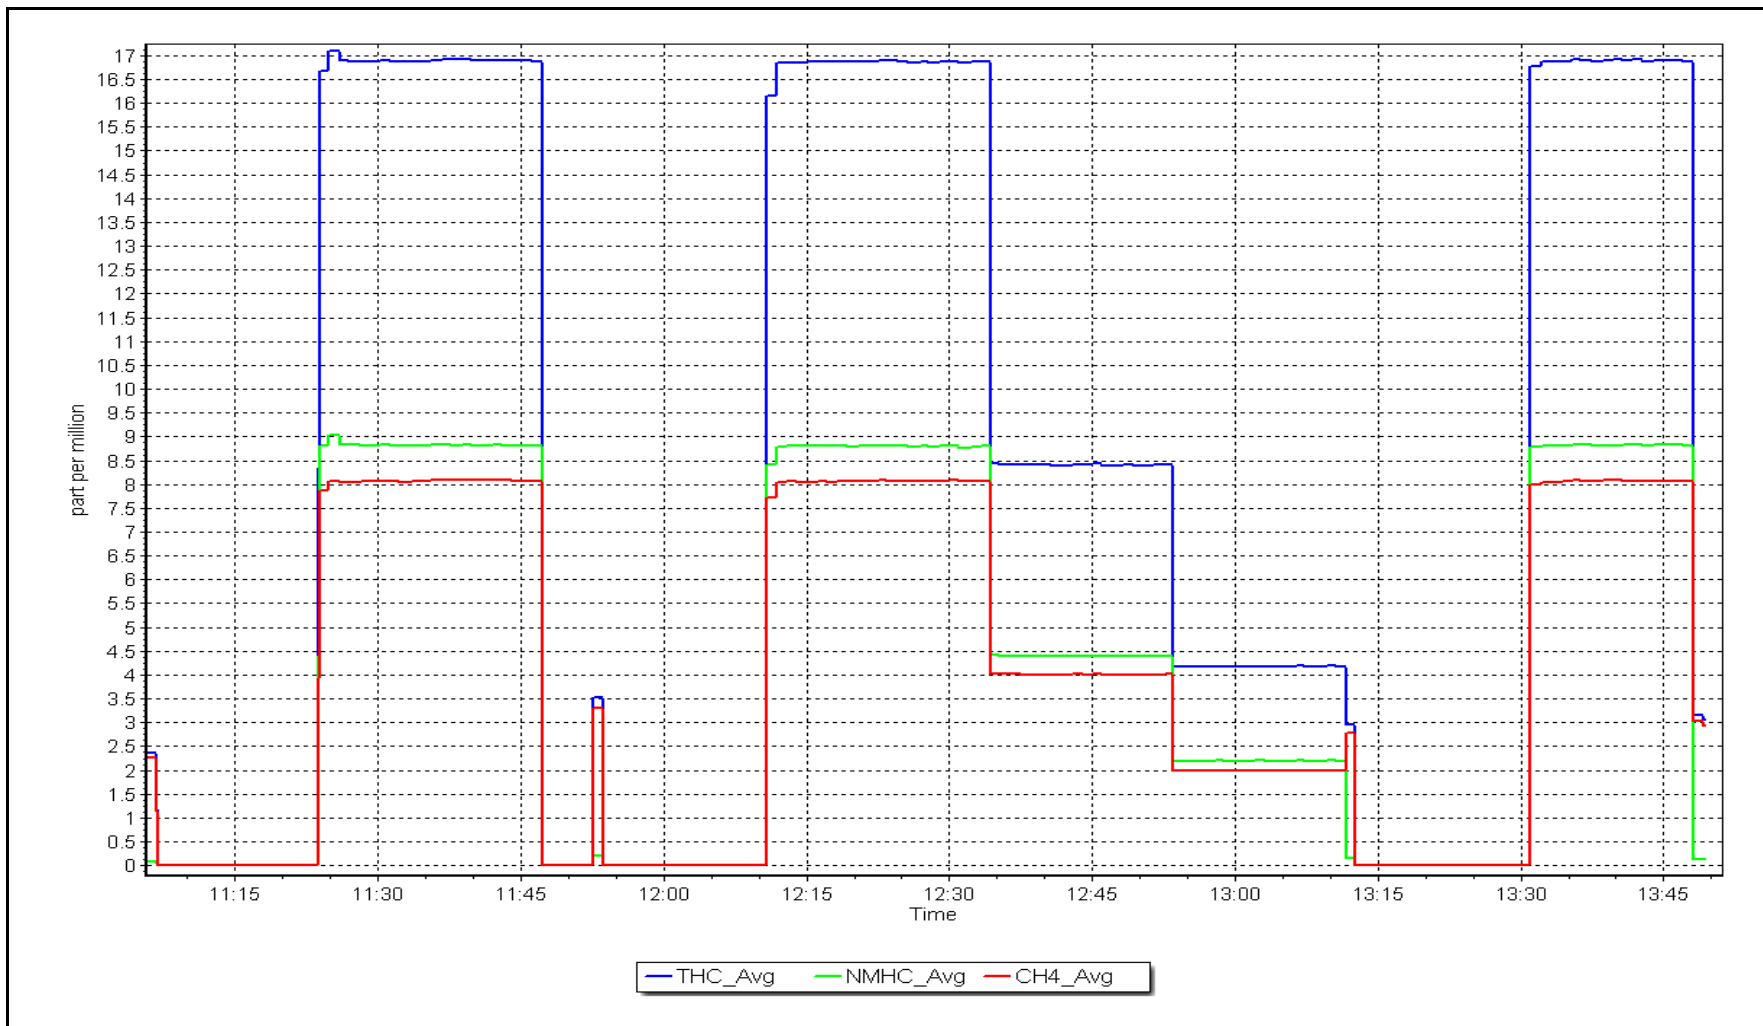



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS04 BUFFALO VIEWPOINT JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Buffalo Viewpoint	Station number:	AMS04
Calibration Date:	January 12, 2023	Last Cal Date:	December 13, 2022
Start time (MST):	10:40	End time (MST):	13:09
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	50.02	ppm	Cal Gas Exp Date:	September 9, 2028
Cal Gas Cylinder #:	CC470284			
Removed Cal Gas Conc:	50.02	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	2445
ZAG Make/Model:	API T701		Serial Number:	5611

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	JC1327300932
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.001942	0.998800	Backgd or Offset:	21.5	21.5
Calibration intercept:	0.880000	0.680000	Coeff or Slope:	0.869	0.869

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.4	----
as found span	4920	80.0	800.3	800.3	1.000
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.5	----
high point	4920	80.0	800.3	800.0	1.000
second point	4960	40.0	400.2	400.3	1.000
third point	4980	20.0	200.1	200.8	0.996
as left zero	5000	0.0	0.0	0.5	----
as left span	4920	80.0	800.3	800.5	1.000
Average Correction Factor					0.999

Baseline Corr As found:	799.90	Previous response	802.75	*% change	-0.4%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: No Maintenance or adjustments done.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 13, 2022
Station Name:	Buffalo Viewpoint	Station Number:	AMS04
Start Time (MST):	7:45	End Time (MST):	13:09
Analyzer make:	Thermo 43i	Analyzer serial #:	JC1327300932

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.5	----	Correlation Coefficient	1.000000	≥0.995
800.3	800.0	1.0004			
400.2	400.3	0.9997	Slope	0.998800	0.90 - 1.10
200.1	200.8	0.9964			
			Intercept	0.680000	+/-30

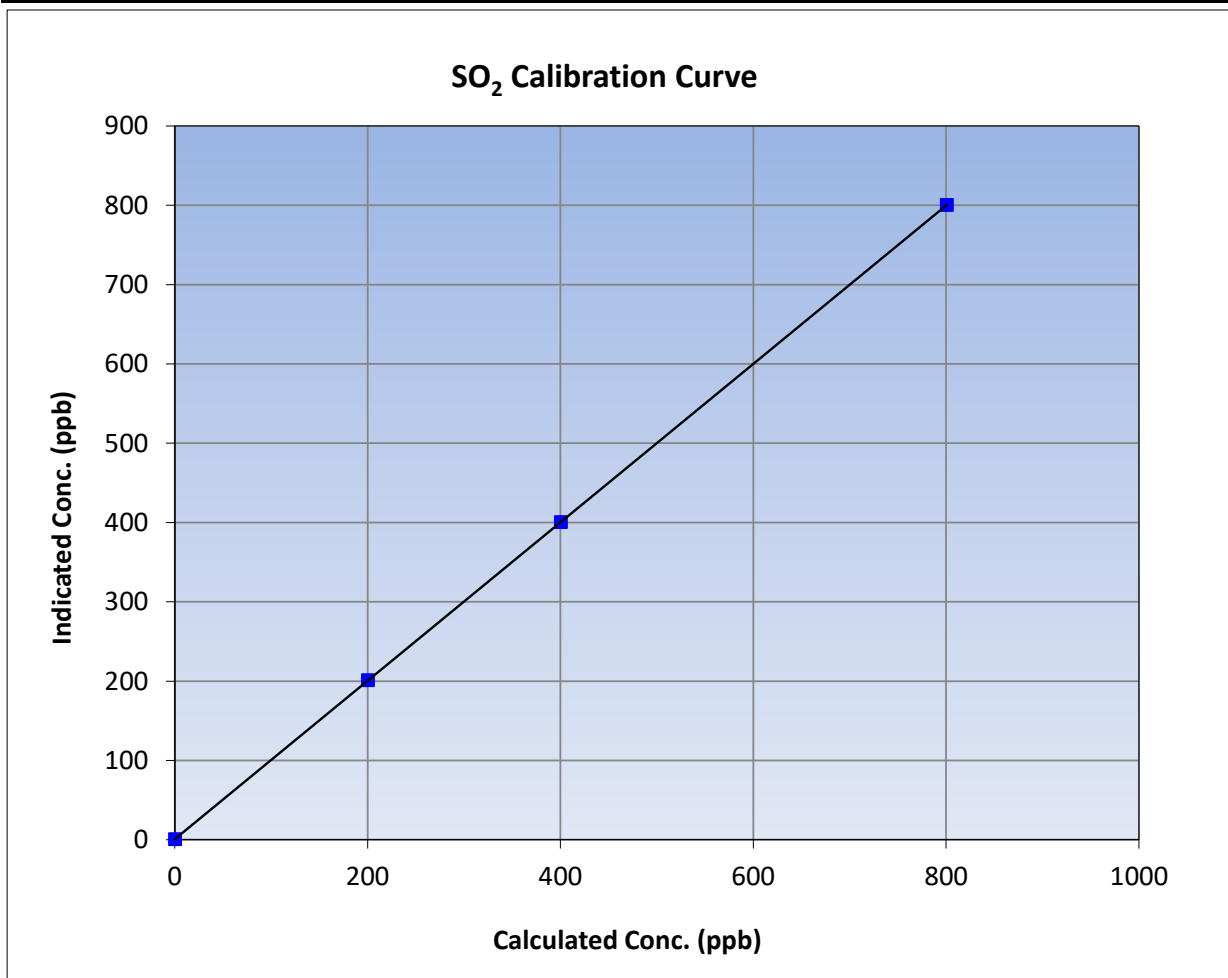

SO2 Calibration Plot

Date: January 12, 2023

Location: Buffalo Viewpoint

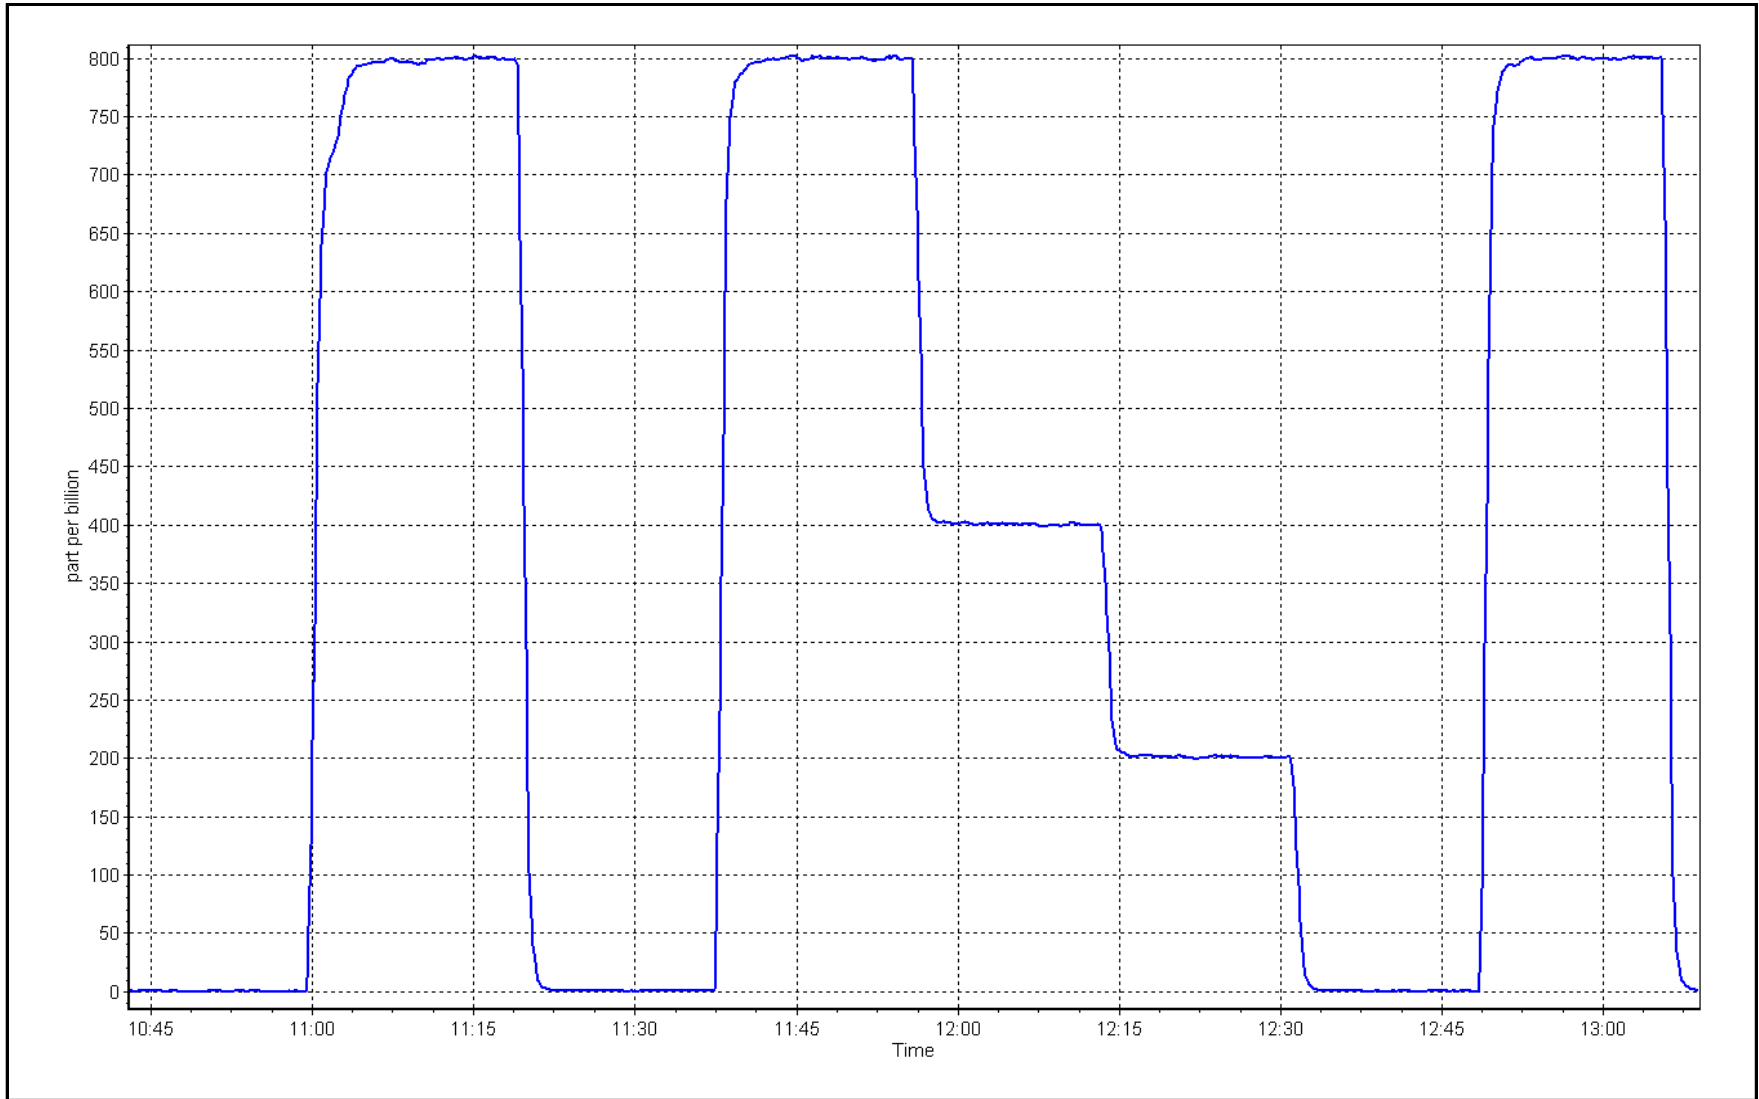



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Buffalo Viewpoint Station number: AMS04
 Calibration Date: January 16, 2023 Last Cal Date: December 8, 2022
 Start time (MST): 7:25 End time (MST): 13:09
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.42 ppm Cal Gas Exp Date: January 4, 2025
 Cal Gas Cylinder #: CC345266
 Removed Cal Gas Conc: 5.42 ppm Rem Gas Exp Date: January 4, 2025
 Removed Gas Cyl #: CC345266 Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 3060
 ZAG Make/Model: API T701H Serial Number: 362

Analyzer Information

Analyzer make: Thermo 450i Analyzer serial #: 1336160094
 Converter make: NA Converter serial #: NA
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	1.003620	1.000770	Backgd or Offset: 17.9	20.1
Calibration intercept:	-0.197849	0.002271	Coeff or Slope: 1.074	1.119

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.2	----
as found span	4926	74.1	80.3	81.5	0.988
as found 2nd point	4963	37.0	40.1	40.6	0.993
as found 3rd point	4982	18.5	20.1	20.5	0.988
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	-0.1	----
high point	4926	74.1	80.3	80.3	1.000
second point	4963	37.0	40.1	40.3	0.995
third point	4982	18.5	20.1	20.1	0.998
as left zero	5000	0.0	0.0	-0.2	----
as left span	4926	74.1	80.3	80.5	0.998
SO2 Scrubber Check	4920	80.0	800.0	-0.2	----
Date of last scrubber change:				Ave Corr Factor	0.998
Date of last converter efficiency test:				efficiency	

Baseline Corr As found: 81.3 Prev response: 80.42 *% change: 1.1%
 Baseline Corr 2nd AF pt: 40.4 AF Slope: 1.011872 AF Intercept: 0.162360
 Baseline Corr 3rd AF pt: 20.3 AF Correlation: 0.999992

** = > +/-5% change initiates investigation*

Notes: Sox scrubber failed. Sox scrubber replaced. Pump replaced. Sox scrubber checked after the calibrator zero. Span adjusted.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 8, 2022
Station Name:	Buffalo Viewpoint	Station Number:	AMS04
Start Time (MST):	7:25	End Time (MST):	13:09
Analyzer make:	Thermo 450i	Analyzer serial #:	1336160094

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	-0.1	----	Correlation Coefficient	0.999988	
80.3	80.3	1.0003			≥0.995
40.1	40.3	0.9952	Slope	1.000770	
20.1	20.1	0.9976			0.90 - 1.10
			Intercept	0.002271	+/-3

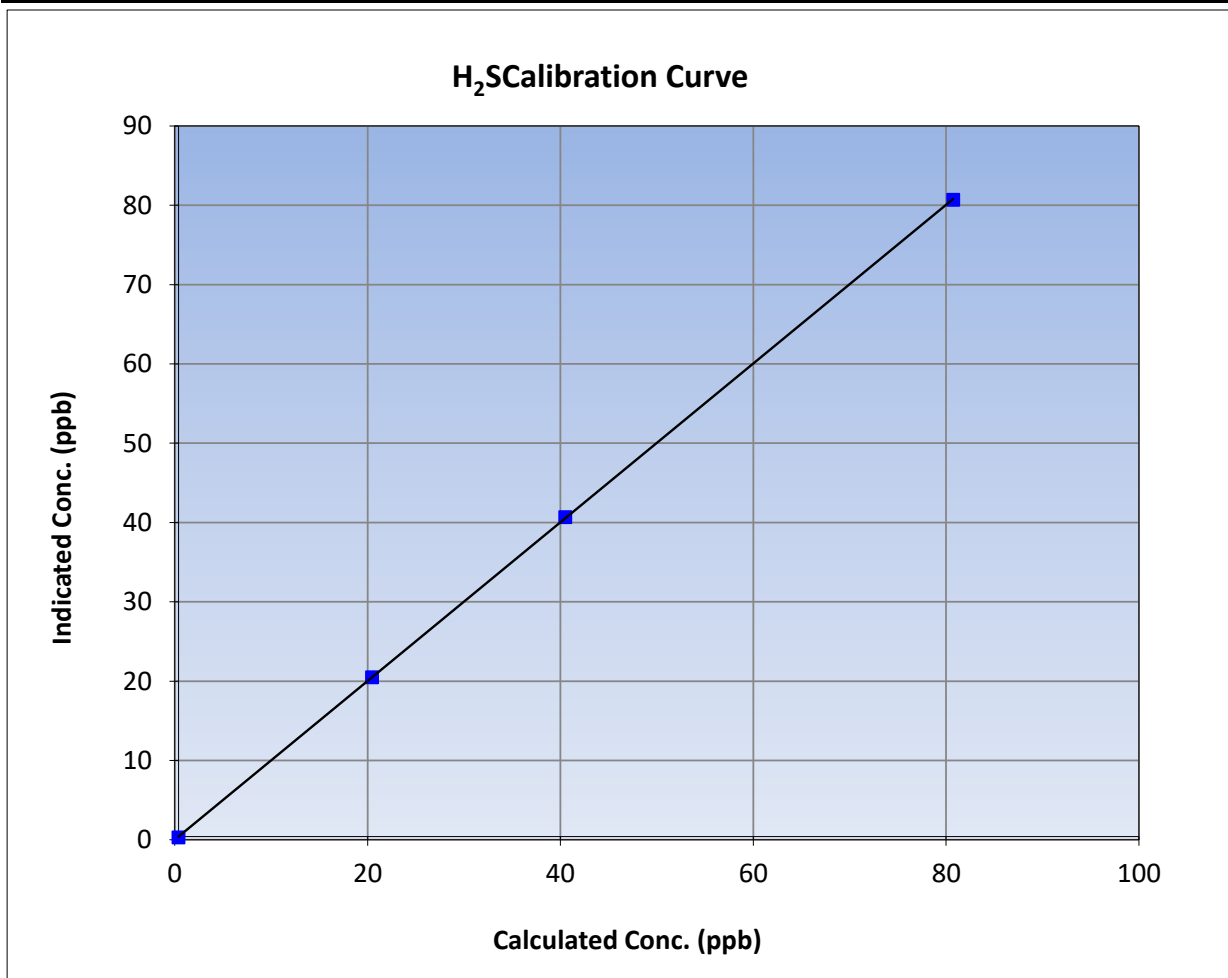

H₂S Calibration Plot

Date: January 16, 2023

Location: Buffalo Viewpoint

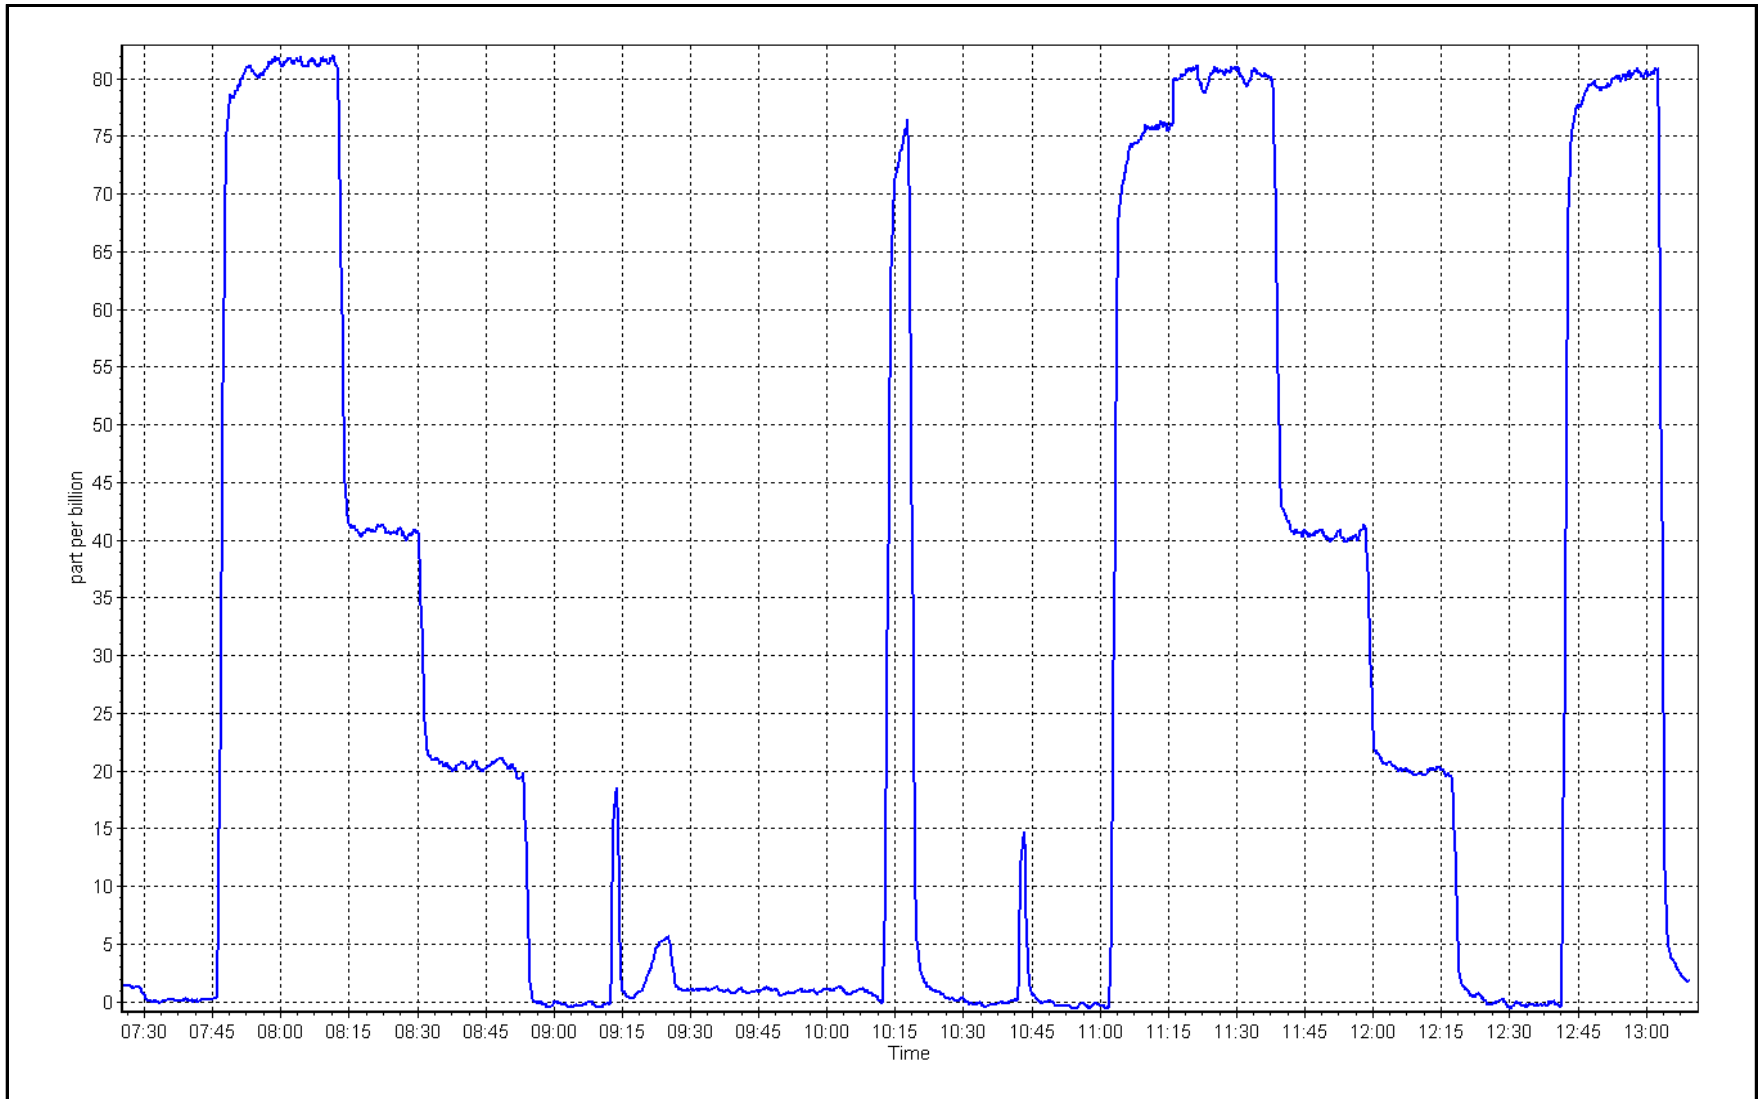



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Buffalo Viewpoint	Station number:	AMS04
Calibration Date:	January 12, 2023	Last Cal Date:	December 12, 2022
Start time (MST):	10:40	End time (MST):	13:10
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC470284	Cal Gas Expiry Date:	September 9, 2028
CH ₄ Cal Gas Conc.	497.8 ppm	CH ₄ Equiv Conc.	1062.9 ppm
C ₃ H ₈ Cal Gas Conc.	205.5 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	497.8 ppm	CH ₄ Equiv Conc.	1062.9 ppm
Removed C ₃ H ₈ Conc.	205.5 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	2445
ZAG make/model:	API T701	Serial Number:	362

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1426262594
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	3.070E-04	3.070E-04	NMHC SP Ratio:	6.120E-05
CH ₄ Retention time:	13.6	13.6	NMHC Peak Area:	147690
				147690

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.0	17.01	17.21	0.988
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.0	17.01	17.09	0.995
second point	4960	40.0	8.50	8.38	1.015
third point	4980	20.0	4.25	4.18	1.017
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.0	17.01	17.04	0.998

Average Correction Factor				1.009
Baseline Corr AF:	17.21	Prev response	17.03	*% change 1.0%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	
as found span	4920	80.0	9.04	9.13	0.990
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.0	9.04	9.06	0.998
second point	4960	40.0	4.52	4.49	1.007
third point	4980	20.0	2.26	2.26	1.000
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.0	9.04	9.02	1.002
Average Correction Factor					1.002
Baseline Corr AF:	9.13	Prev response	9.03	*% change	1.1%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.0	7.96	8.08	0.986
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.0	7.96	8.04	0.991
second point	4960	40.0	3.98	3.89	1.024
third point	4980	20.0	1.99	1.92	1.037
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.0	7.96	8.02	0.993
Average Correction Factor					1.017
Baseline Corr AF:	8.08	Prev response	7.99	*% change	1.1%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	1.005447	1.005648
THC Cal Offset:	-0.066000	-0.070000
CH ₄ Cal Slope:	1.011020	1.011450
CH ₄ Cal Offset:	-0.058000	-0.062000
NMHC Cal Slope:	0.999400	1.001675
NMHC Cal Offset:	-0.006000	-0.010000

Notes: No maintenance or adjustments done.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 12, 2022
Station Name:	Buffalo Viewpoint	Station Number:	AMS04
Start Time (MST):	10:40	End Time (MST):	13:10
Analyzer make:	Thermo 55i	Analyzer serial #:	1426262594

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999881	≥ 0.995			
17.01	17.09	0.9951						
8.50	8.38	1.0147				Slope	1.005648	0.90 - 1.10
4.25	4.18	1.0172						
			Intercept	-0.070000	± 0.5			

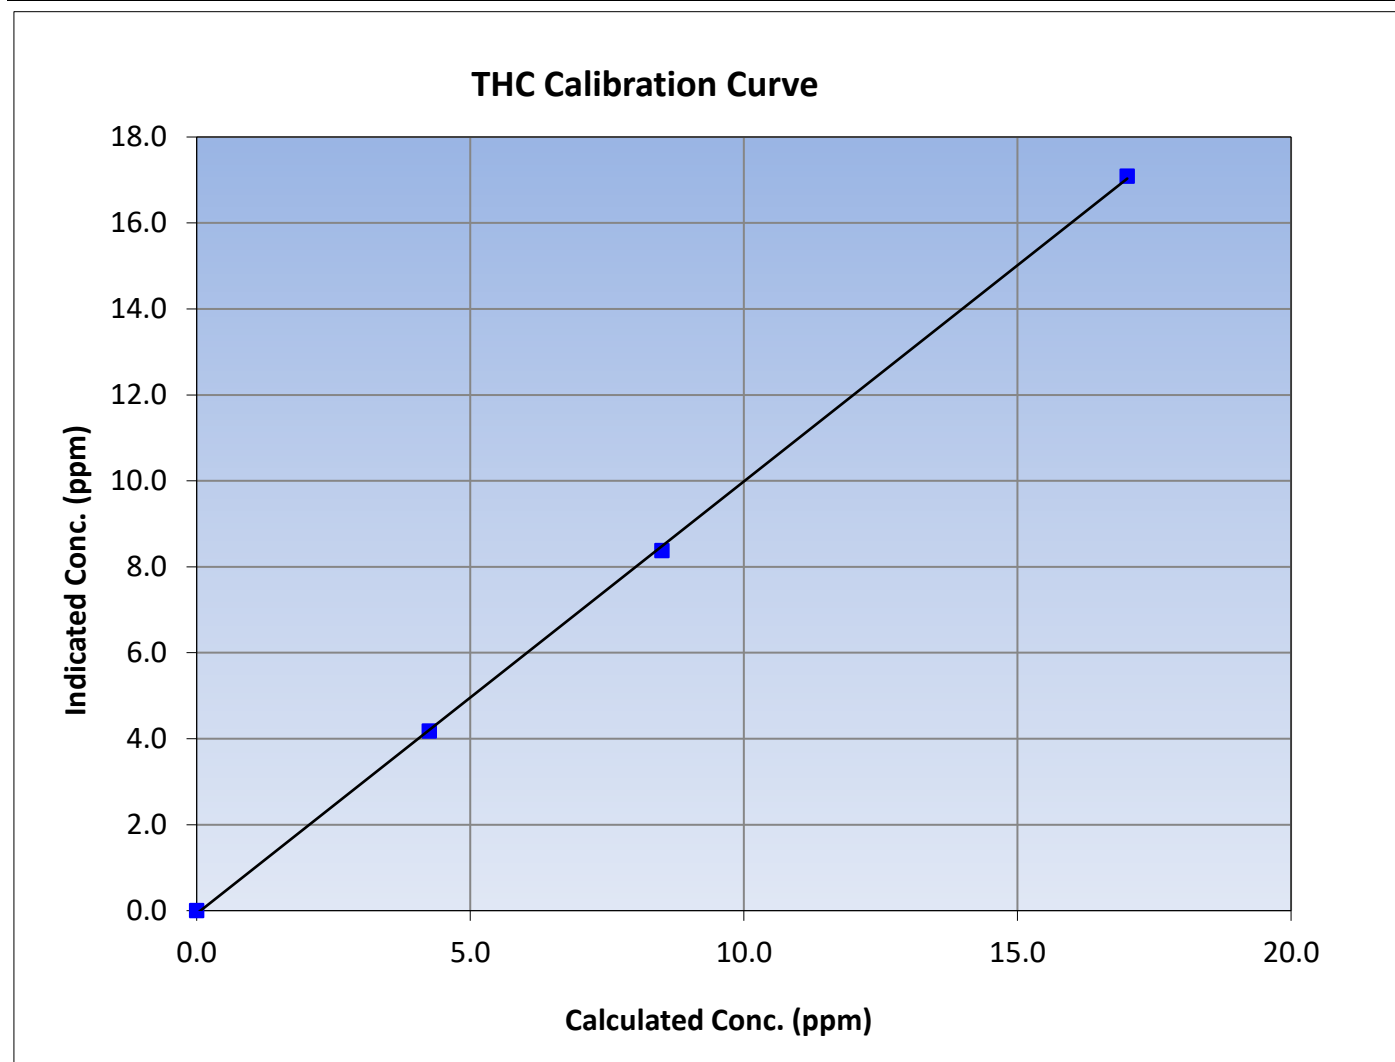



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 12, 2022
Station Name:	Buffalo Viewpoint	Station Number:	AMS04
Start Time (MST):	10:40	End Time (MST):	13:10
Analyzer make:	Thermo 55i	Analyzer serial #:	1426262594

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999641	≥ 0.995
7.96	8.04	0.9906			
3.98	3.89	1.0238			
1.99	1.92	1.0371			
			Slope	1.011450	0.90 - 1.10
			Intercept	-0.062000	+/-0.5

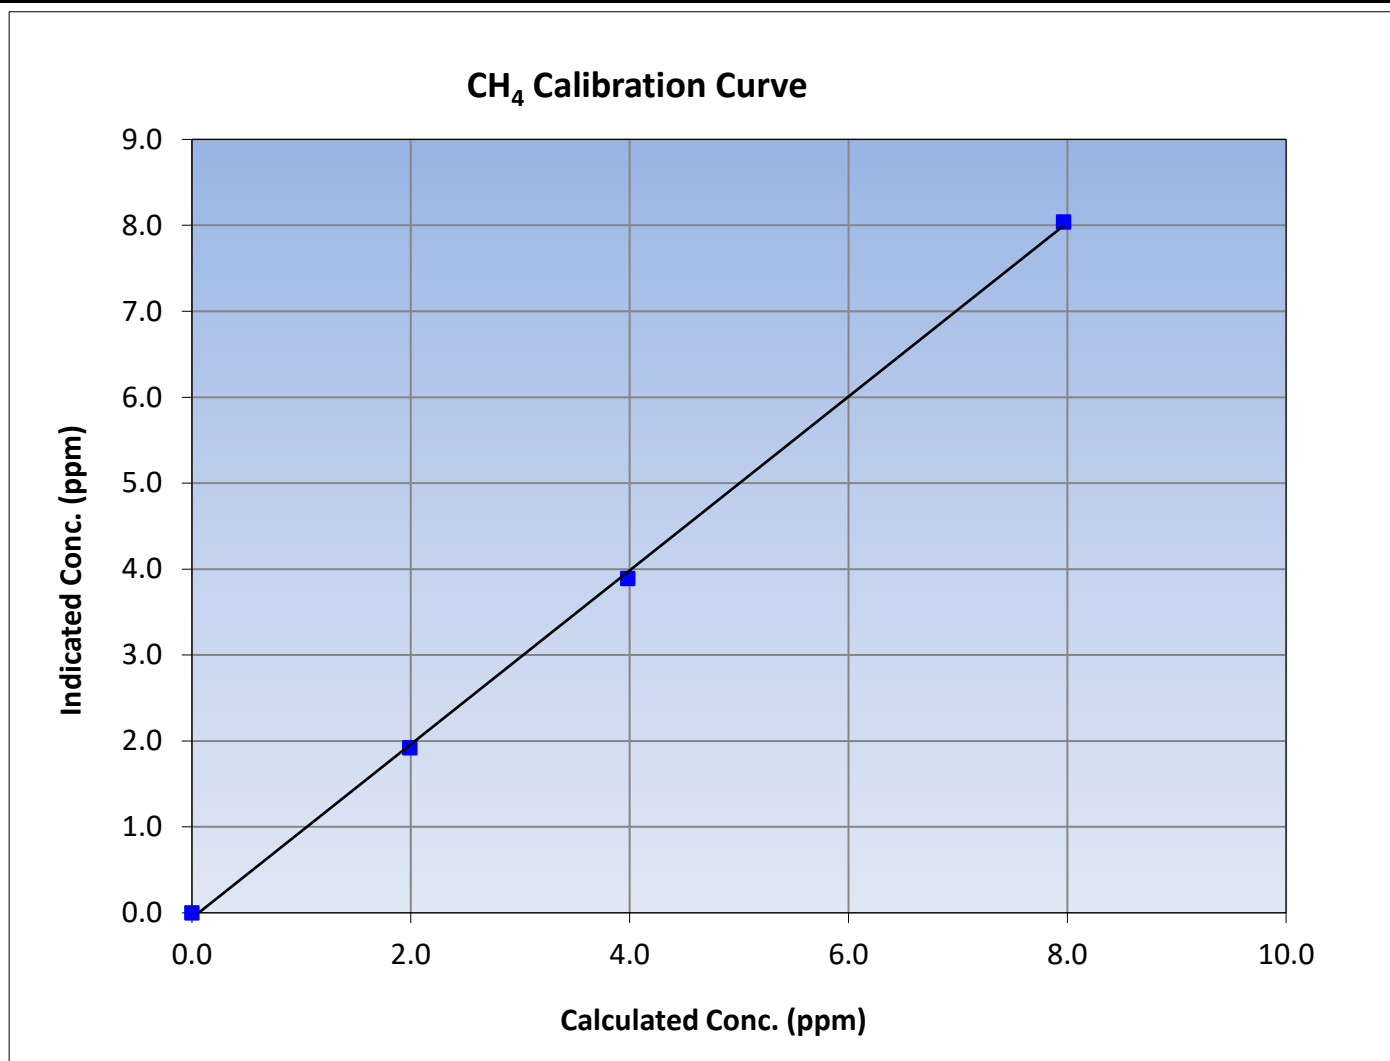



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 12, 2022
Station Name:	Buffalo Viewpoint	Station Number:	AMS04
Start Time (MST):	10:40	End Time (MST):	13:10
Analyzer make:	Thermo 55i	Analyzer serial #:	1426262594

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999975	≥ 0.995			
9.04	9.06	0.9980						
4.52	4.49	1.0069				Slope	1.001675	0.90 - 1.10
2.26	2.26	1.0002						
			Intercept	-0.010000	± 0.5			

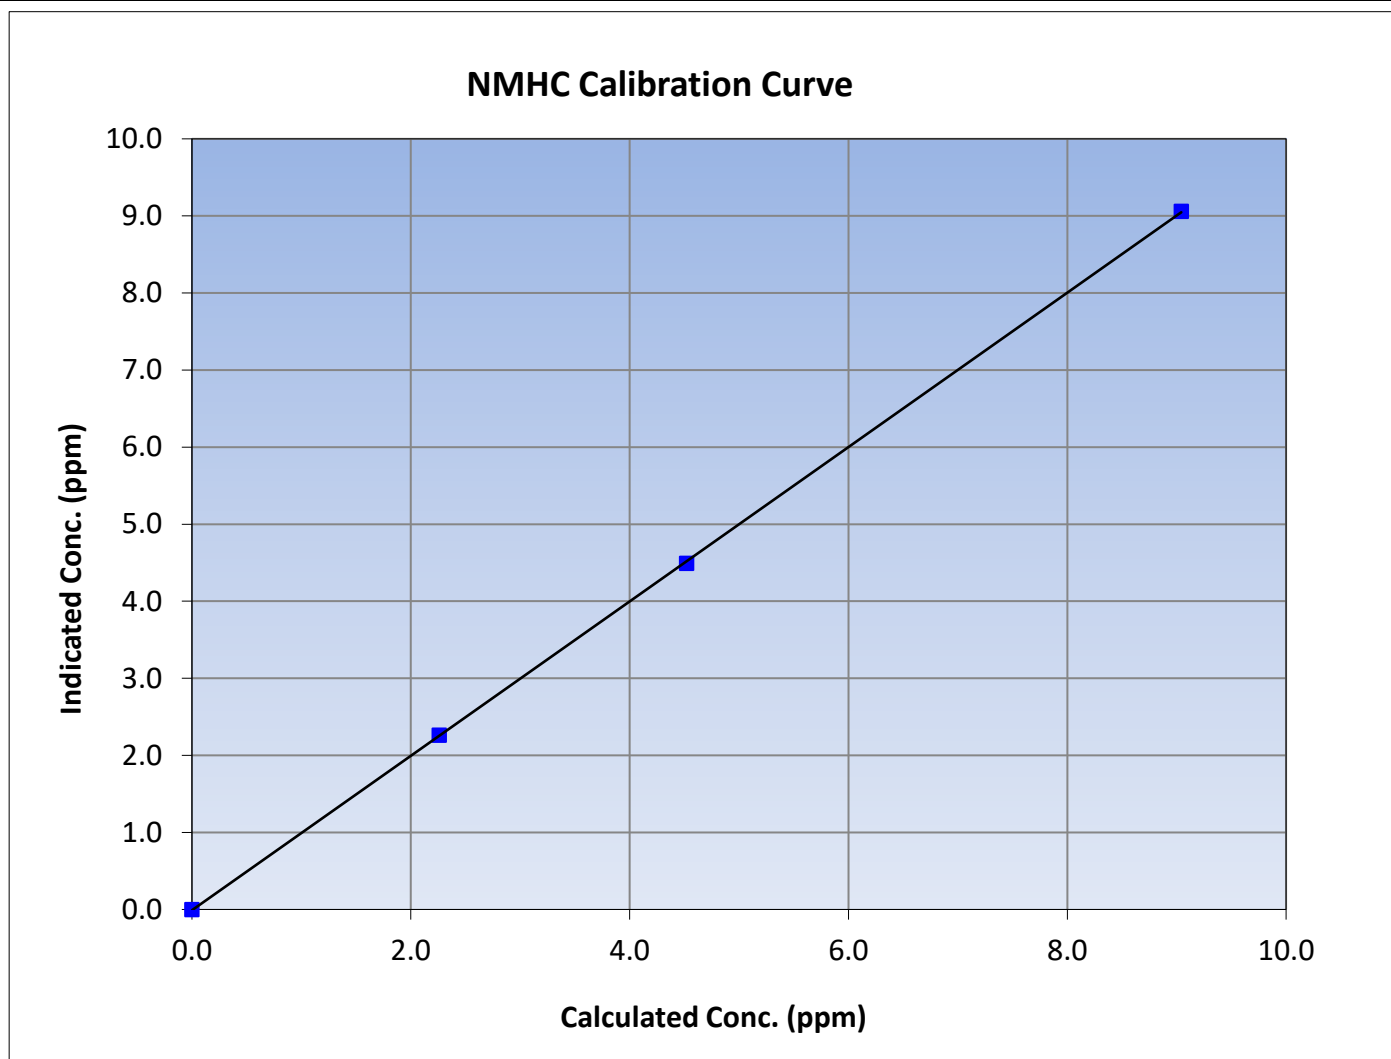

NMHC Calibration Plot

Date: January 12, 2023

Location: Buffalo Viewpoint

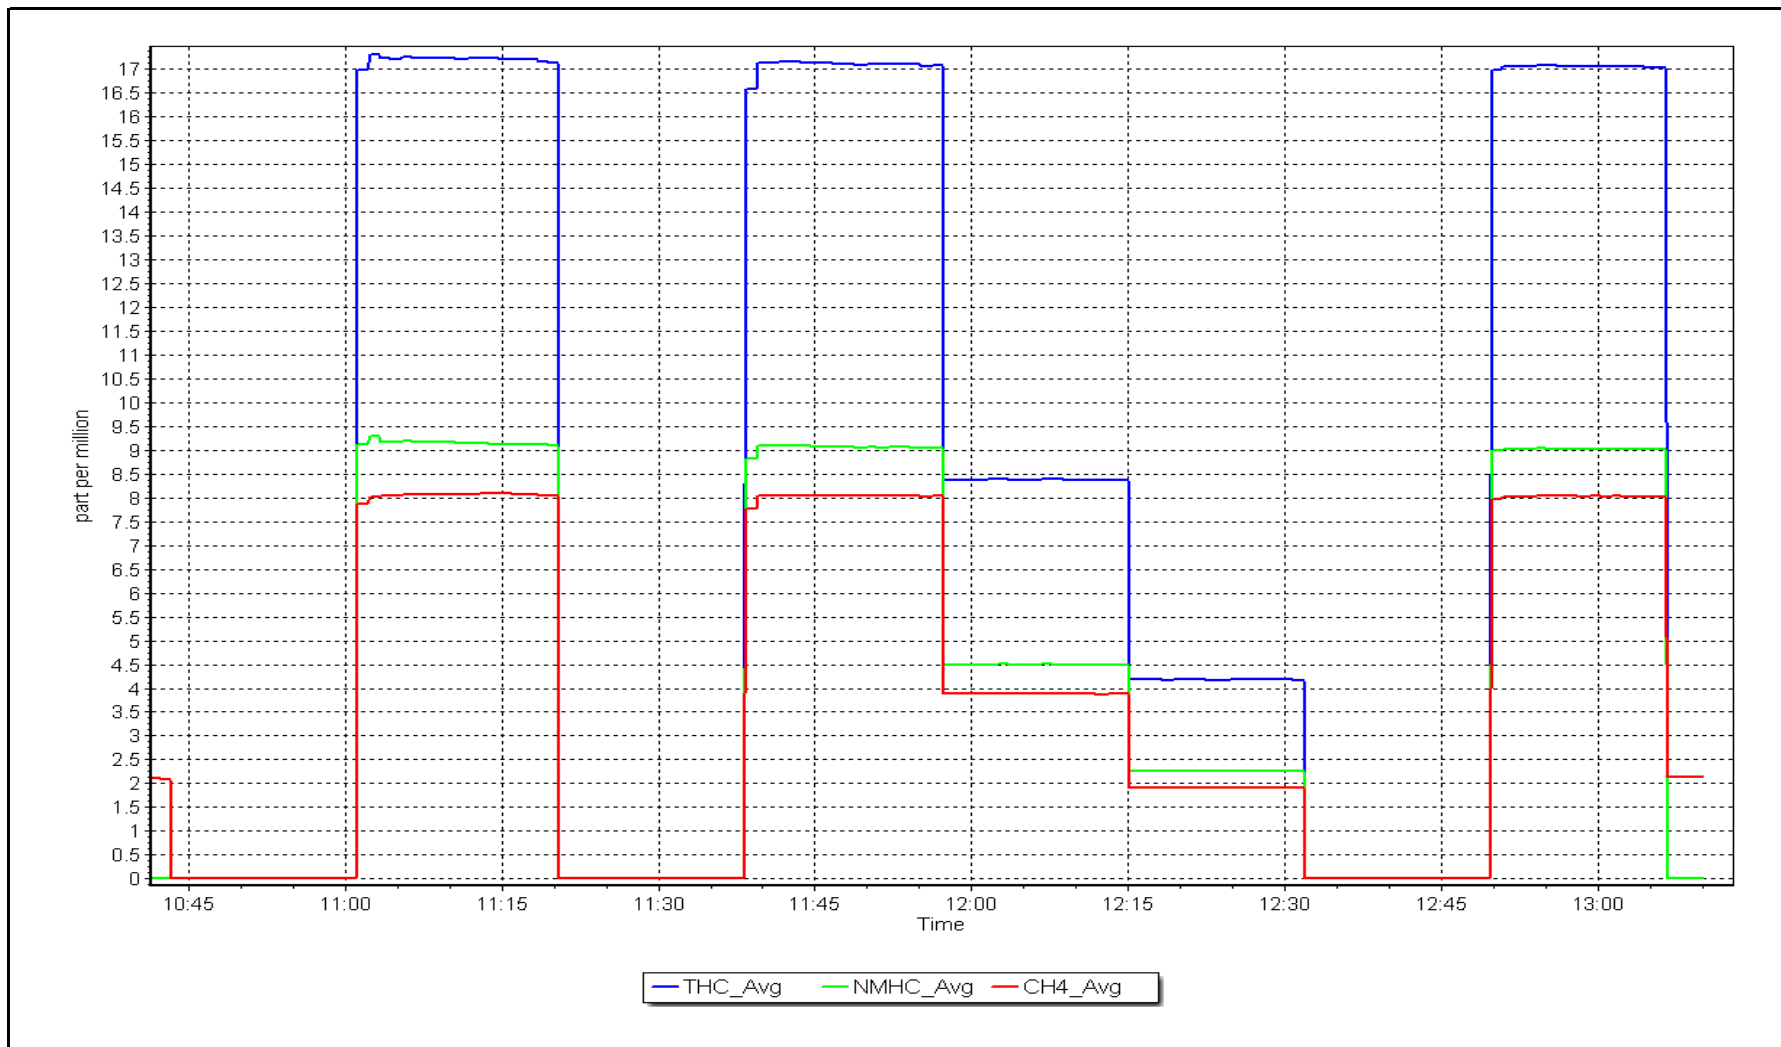



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Buffalo Viewpoint
Calibration Date: January 13, 2023
Start time (MST): 7:12
Reason: Routine
Station number: AMS04
Last Cal Date: December 1, 2022
End time (MST): 12:19

Calibration Standards

NO Gas Cylinder #: T36RH1F
NOX Cal Gas Conc: 51.16 ppm
Removed Cylinder #: NA
Removed Gas NOX Conc: 51.16 ppm
NOX gas Diff:
Calibrator Model: API T700
ZAG make/model: API T701
Cal Gas Expiry Date: August 18, 2023
NO Cal Gas Conc: 50.91 ppm
Removed Gas Exp Date: NA
Removed Gas NO Conc: 50.91 ppm
NO gas Diff:
Serial Number: 2445
Serial Number: 362

Analyzer Information

Analyzer make: API T200
NOX Range (ppb): 0 - 1000 ppb
Analyzer serial #: 723

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.149	1.204	NO bkgnd or offset:	-0.3	-0.3
NOX coeff or slope:	1.147	1.203	NOX bkgnd or offset:	-0.1	-0.1
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	6.8	6.8

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	0.999214	1.000402
NO _x Cal Offset:	0.407361	0.466890
NO Cal Slope:	0.999207	1.001422
NO Cal Offset:	-0.832949	-0.653871
NO ₂ Cal Slope:	0.995503	1.000220
NO ₂ Cal Offset:	1.627827	1.229528



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.7	0.0	0.7	----	----
as found span	4922	78.1	799.1	795.2	3.9	764.6	757.7	6.9	1.0451	1.0495
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.4	0.6	-0.2	----	----
high point	4922	78.1	799.1	795.2	3.9	800.1	796.2	3.9	0.9988	0.9987
second point	4961	39.1	400.1	398.1	2.0	400.0	397.7	2.4	1.0002	1.0010
third point	4981	19.5	199.5	198.5	1.0	200.6	196.7	3.9	0.9945	1.0093
as left zero	5000	0.0	0.0	0.0	0.0	1.4	1.4	0.0	----	----
as left span	4922	78.1	799.1	368.2	430.9	799.0	365.4	433.6	1.0001	1.0077
Average Correction Factor									0.9978	1.0030

Corrected As found	NO _x = 763.9 ppb	NO = 757.7 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -4.6%	
Previous Response	NO _x = 798.9 ppb	NO = 793.7 ppb		*Percent Change	NO = -4.8%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	794.0	367.0	430.9	431.7	0.9982	100.2%
2nd GPT point (200 ppb O3)	794.0	580.5	217.4	218.8	0.9936	100.6%
3rd GPT point (100 ppb O3)	794.0	687.9	110.0	113.1	0.9726	102.8%
Average Correction Factor					0.9881	101.2%

Notes: Pump and charcoal was changed recently. Diagnostics similar to last months. Span adjusted. No Maintenance done.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 1, 2022
Station Name:	Buffalo Viewpoint	Station Number:	AMS04
Start Time (MST):	7:12	End Time (MST):	12:19
Analyzer make:	API T200	Analyzer serial #:	723

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	0.4	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
799.1	800.1	0.9988		
400.1	400.0	1.0002		
199.5	200.6	0.9945		
			0.999998	
			1.000402	
			0.466890	

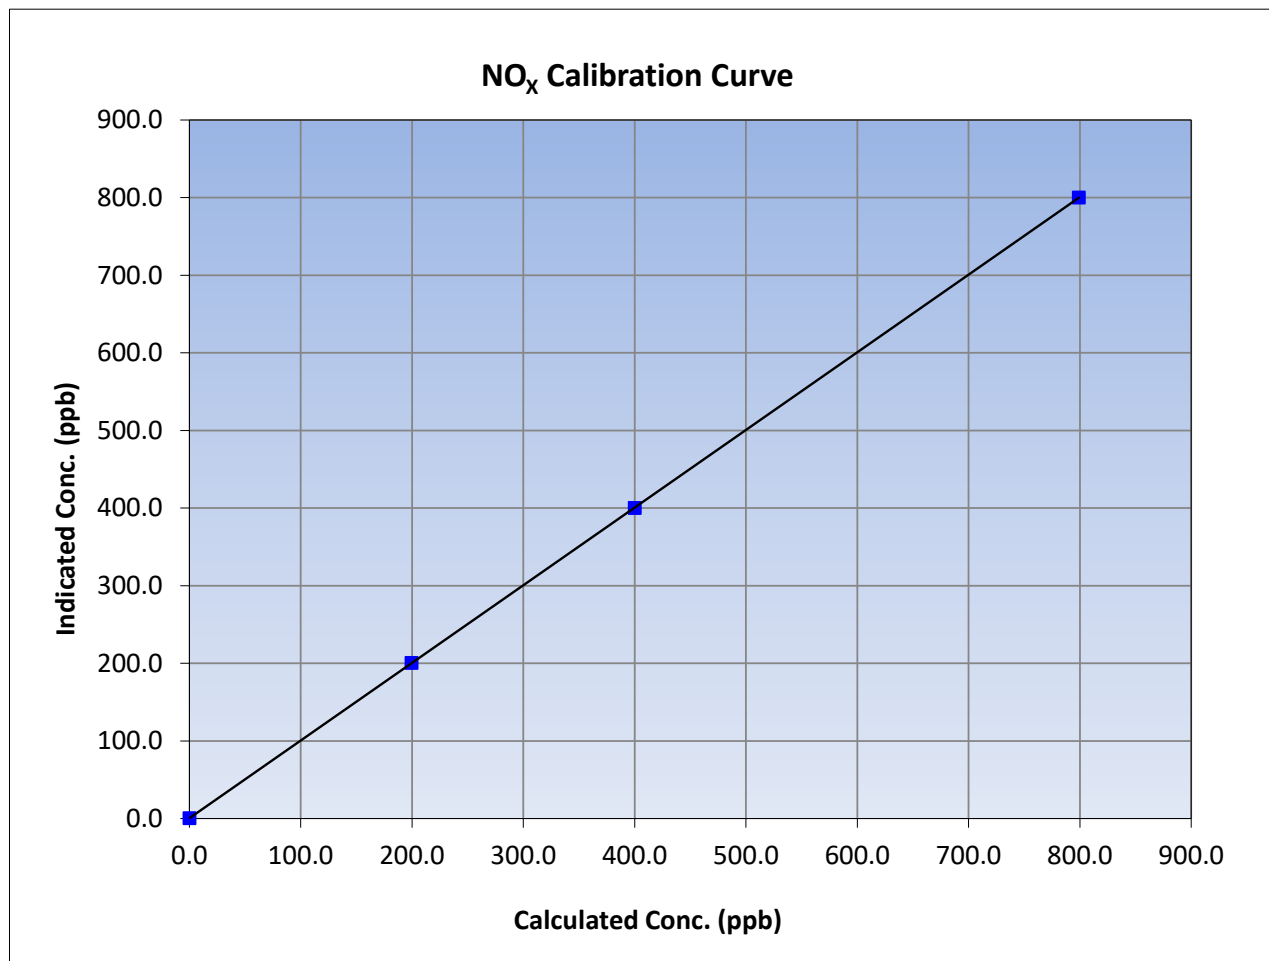



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 1, 2022
Station Name:	Buffalo Viewpoint	Station Number:	AMS04
Start Time (MST):	7:12	End Time (MST):	12:19
Analyzer make:	API T200	Analyzer serial #:	723

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.6	----	Correlation Coefficient	≥0.995	
795.2	796.2	0.9987			
398.1	397.7	1.0010			
198.5	196.7	1.0093			
			Slope	1.001422	0.90 - 1.10
			Intercept	-0.653871	+/-20

NO Calibration Curve

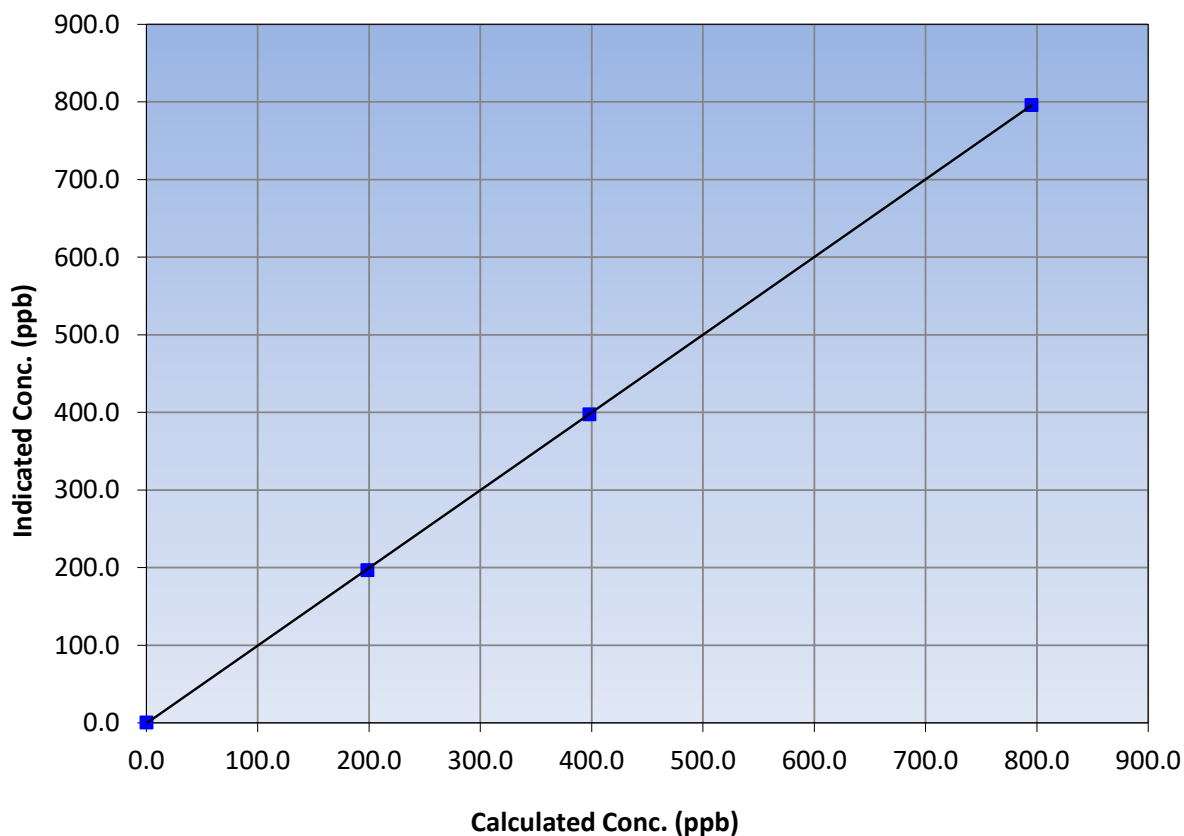



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 1, 2022
Station Name:	Buffalo Viewpoint	Station Number:	AMS04
Start Time (MST):	7:12	End Time (MST):	12:19
Analyzer make:	API T200	Analyzer serial #:	723

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	-0.2	----	Correlation Coefficient	0.999943	≥0.995
430.9	431.7	0.9982			
217.4	218.8	0.9936	Slope	1.000220	0.90 - 1.10
110.0	113.1	0.9726			
			Intercept	1.229528	+/-20

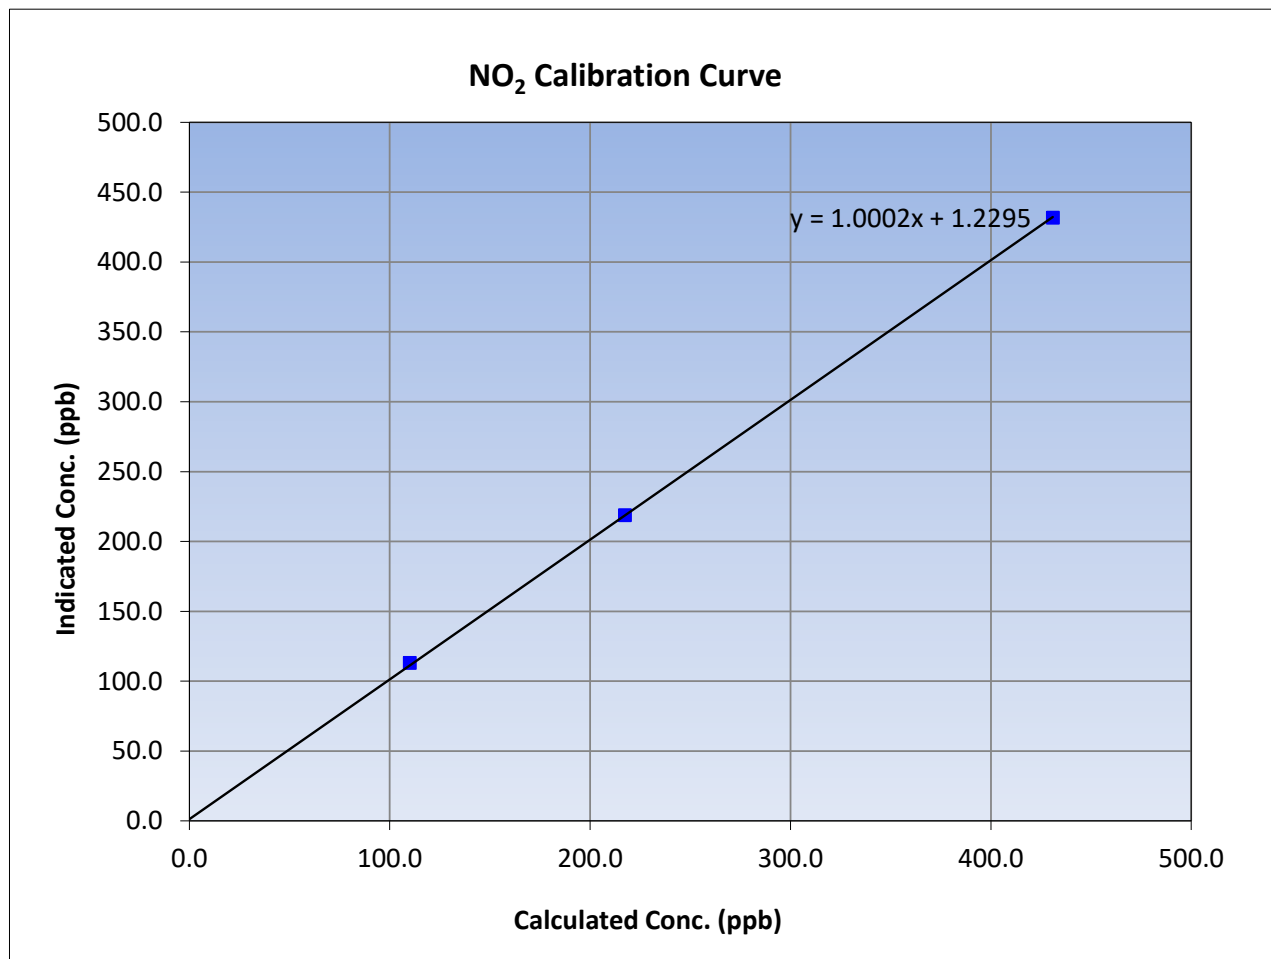

NO_x Calibration Plot

Date: January 13, 2023

Location: Buffalo Viewpoint

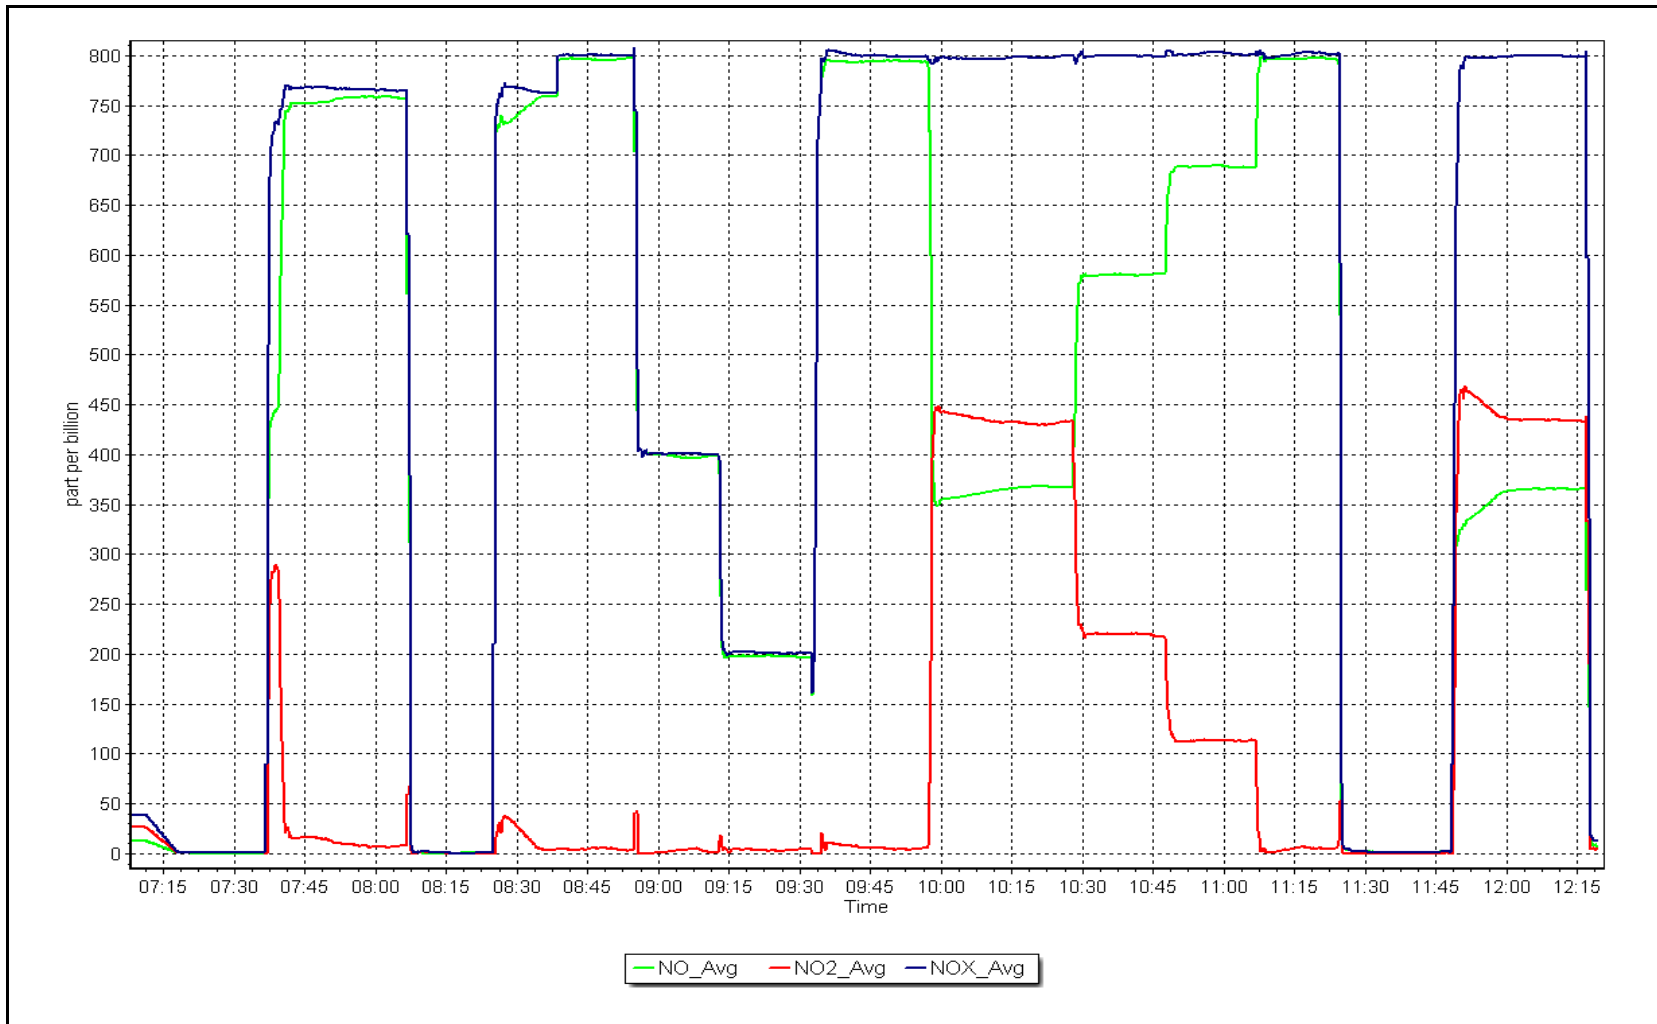



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Buffalo Viewpoint Station number: AMS04
 Calibration Date: January 12, 2023 Last Cal Date: December 13, 2022
 Start time (MST): 8:07 End time (MST): 10:46
 Reason: Routine

Calibration Standards

O3 generation mode: Photometer
 Calibrator Make/Model: API T700 Serial Number: 2445
 ZAG Make/Model: API T701 Serial Number: 362

Analyzer Information

Analyzer make: API T400 Analyzer serial #: 2961
 Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.993086	0.992571	Backgd or Offset:	-3.2	-3.3
Calibration intercept:	2.760000	2.700000	Coeff or Slope:	1.048	1.065

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.2	----
as found span	5000	1158.7	400.0	394.3	1.014
as found 2nd point					
as found 3rd point					
calibrator zero	5000	0.0	0.0	0.9	----
high point	5000	1160.3	400.0	399.0	1.003
second point	5000	919.0	200.0	201.6	0.992
third point	5000	787.5	100.0	104.1	0.961
as left zero	5000	0.0	0.0	0.5	----
as left span	5000	1159.5	400.0	399.6	1.001
Average Correction Factor					0.985

Baseline Corr As found:	394.1	Previous response	400.0	*% change	-1.5%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: No maintenance done. Span adjusted.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 13, 2022
Station Name:	Buffalo Viewpoint	Station Number:	AMS04
Start Time (MST):	8:07	End Time (MST):	10:46
Analyzer make:	API T400	Analyzer serial #:	2961

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.9	----	Correlation Coefficient	0.999901	
400.0	399.0	1.0025			≥0.995
200.0	201.6	0.9921	Slope	0.992571	
100.0	104.1	0.9606			0.90 - 1.10
			Intercept	2.700000	+/- 5

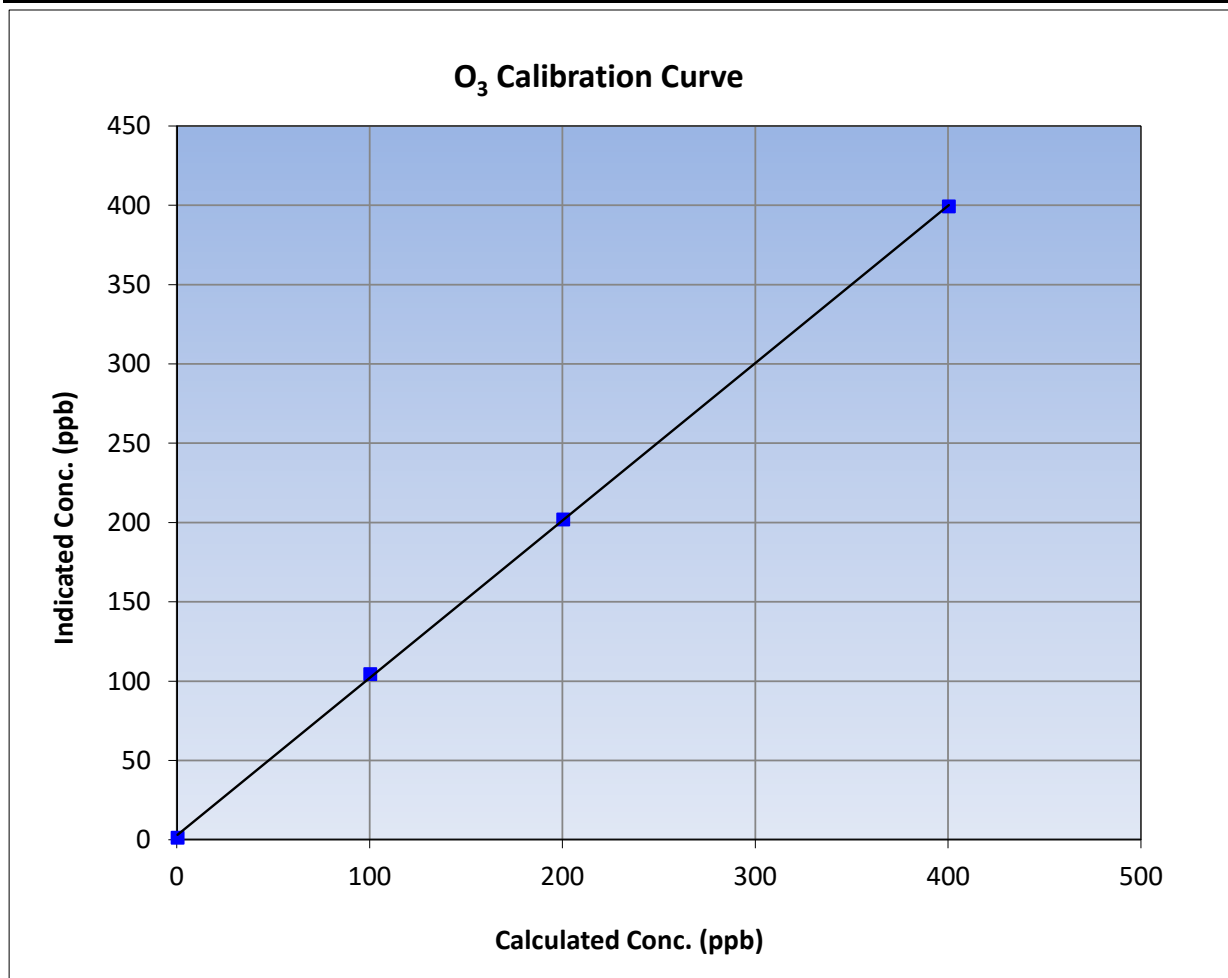

O₃ Calibration Plot

Date: January 12, 2023

Location: Buffalo Viewpoint

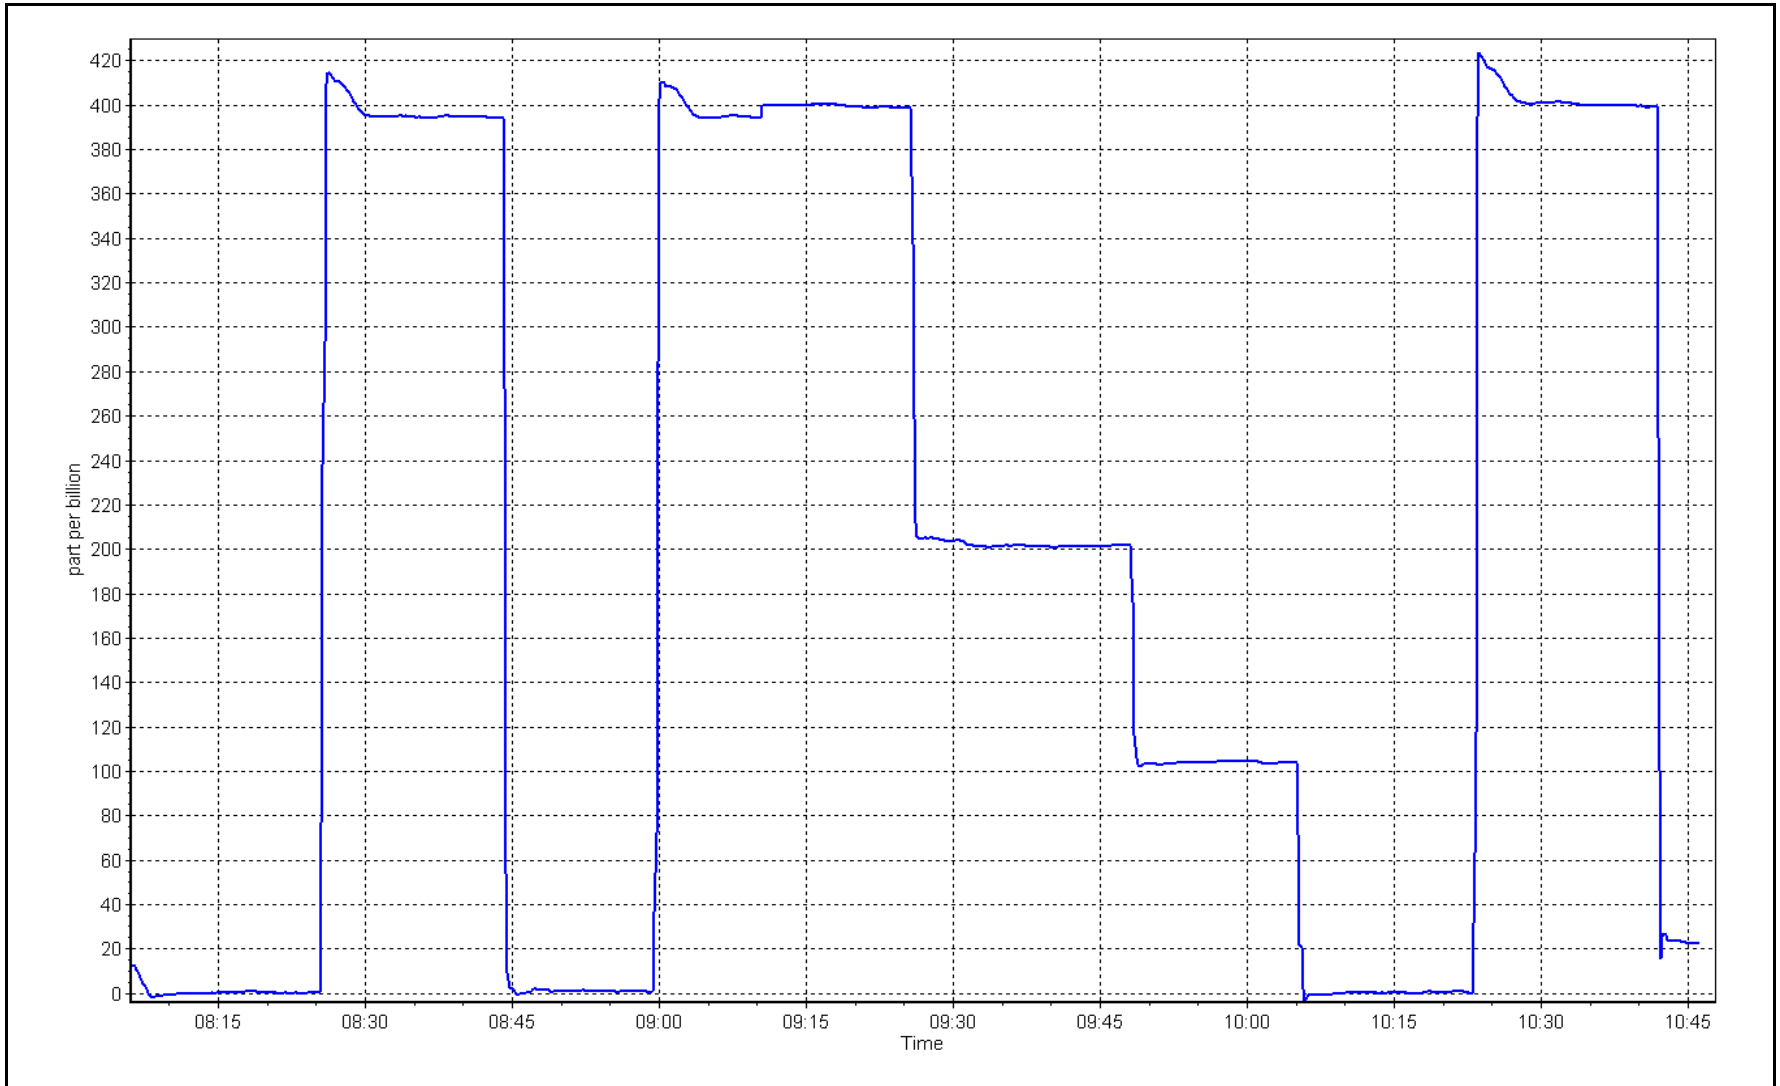



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Buffalo Viewpoint Station number: AMS 04
Calibration Date: January 16, 2023 Last Cal Date: December 13, 2022
Start time (MST): 9:35 End time (MST): 9:58

Analyzer Make: API T640 S/N: 844
Particulate Fraction: PM2.5

Flow Meter Make/Model: AliCat S/N: 228085
Temp/RH standard: AliCat S/N: 228085

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	<i>(Limits)</i>
T (°C)	-6.8	-6.6	-6.8	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	724.3	725.6	724.3	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5	4.60	5	<input checked="" type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 16, 2023 Last Cal Date: December 13, 2022
PM w/o HEPA: 60 PM w/ HEPA: 0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	<i>(Limits)</i>
PMT Peak Test		----		<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: December 13, 2022
Disposable Filter Changed: December 13, 2022

Annual Maintenance

Date Sample Tube Cleaned: September 15, 2022
Date RH/T Sensor Cleaned: September 15, 2022

Notes: Flow Adjusted. Inlet head cleaned.

Calibration by: Melissa Lemay



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

**AMS05
MANNIX
JANUARY 2023**

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Mannix	Station number:	AMS05
Calibration Date:	January 20, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	10:09	End time (MST):	14:55
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	50.02	ppm	Cal Gas Exp Date:	January 12, 2029
Cal Gas Cylinder #:	XC026809B			
Removed Cal Gas Conc:	50.02	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	621
ZAG Make/Model:	API T701H		Serial Number:	832

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	1008841399
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.999415	0.996673	Backgd or Offset:	8.9	8.9
Calibration intercept:	-0.560000	0.800000	Coeff or Slope:	0.914	0.914

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	-0.1	----
as found span	4920	80.0	800.3	797.7	1.003
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.2	----
high point	4920	80.0	800.3	797.5	1.004
second point	4960	40.0	400.2	401.9	0.996
third point	4980	20.0	200.1	199.5	1.003
as left zero	5000	0.0	0.0	0.2	----
as left span	4920	80.0	800.3	802.5	0.997
Average Correction Factor					1.001

Baseline Corr As found:	797.80	Previous response	799.29	*% change	-0.2%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. No adjustments made.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 2, 2022
Station Name:	Mannix	Station Number:	AMS05
Start Time (MST):	10:09	End Time (MST):	14:55
Analyzer make:	Thermo 43i	Analyzer serial #:	1008841399

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999980	≥0.995
800.3	797.5	1.0035			
400.2	401.9	0.9957	Slope	0.996673	0.90 - 1.10
200.1	199.5	1.0029			
			Intercept	0.800000	+/-30

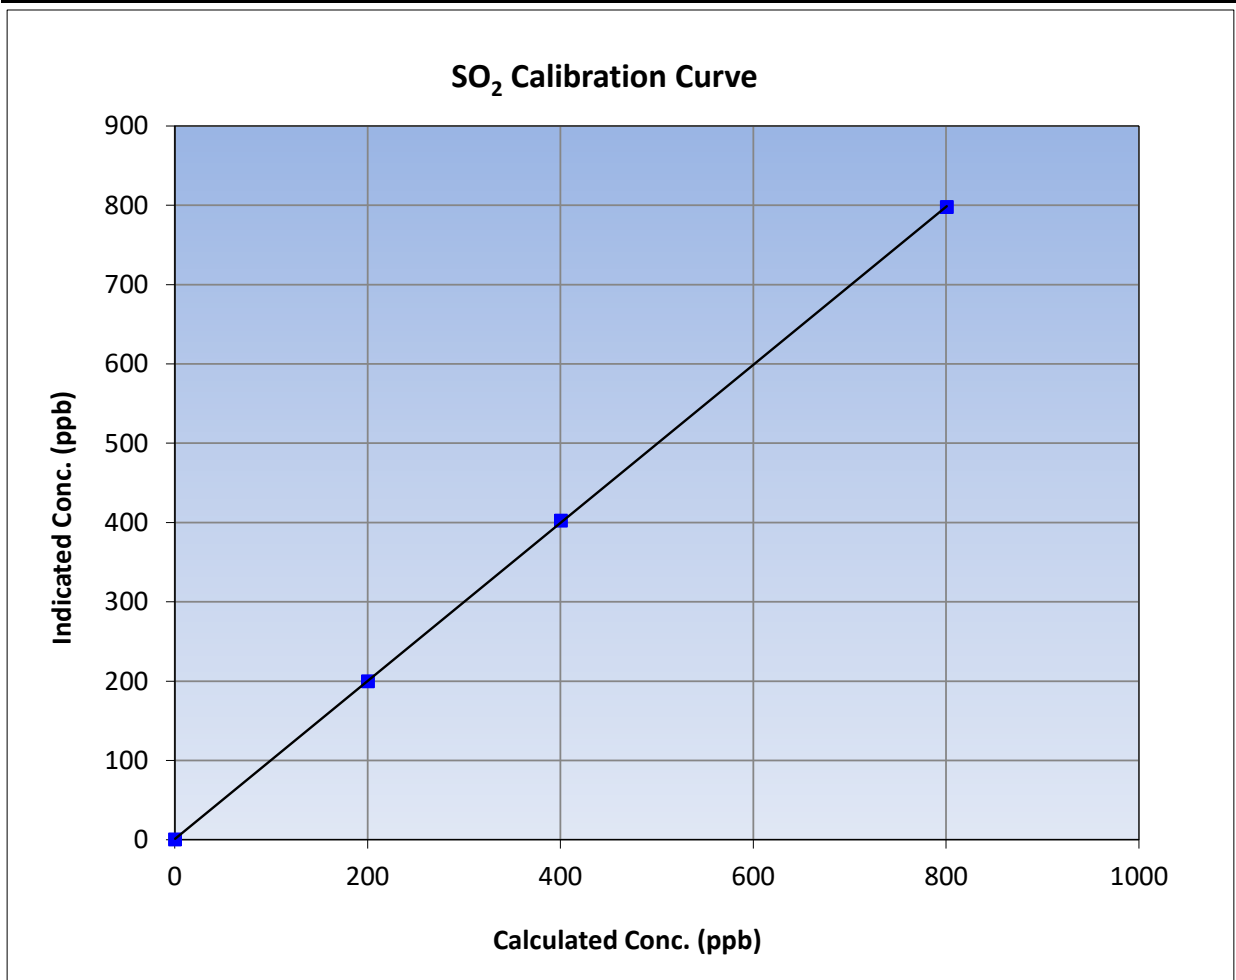

SO2 Calibration Plot

Date: January 20, 2023

Location: Mannix

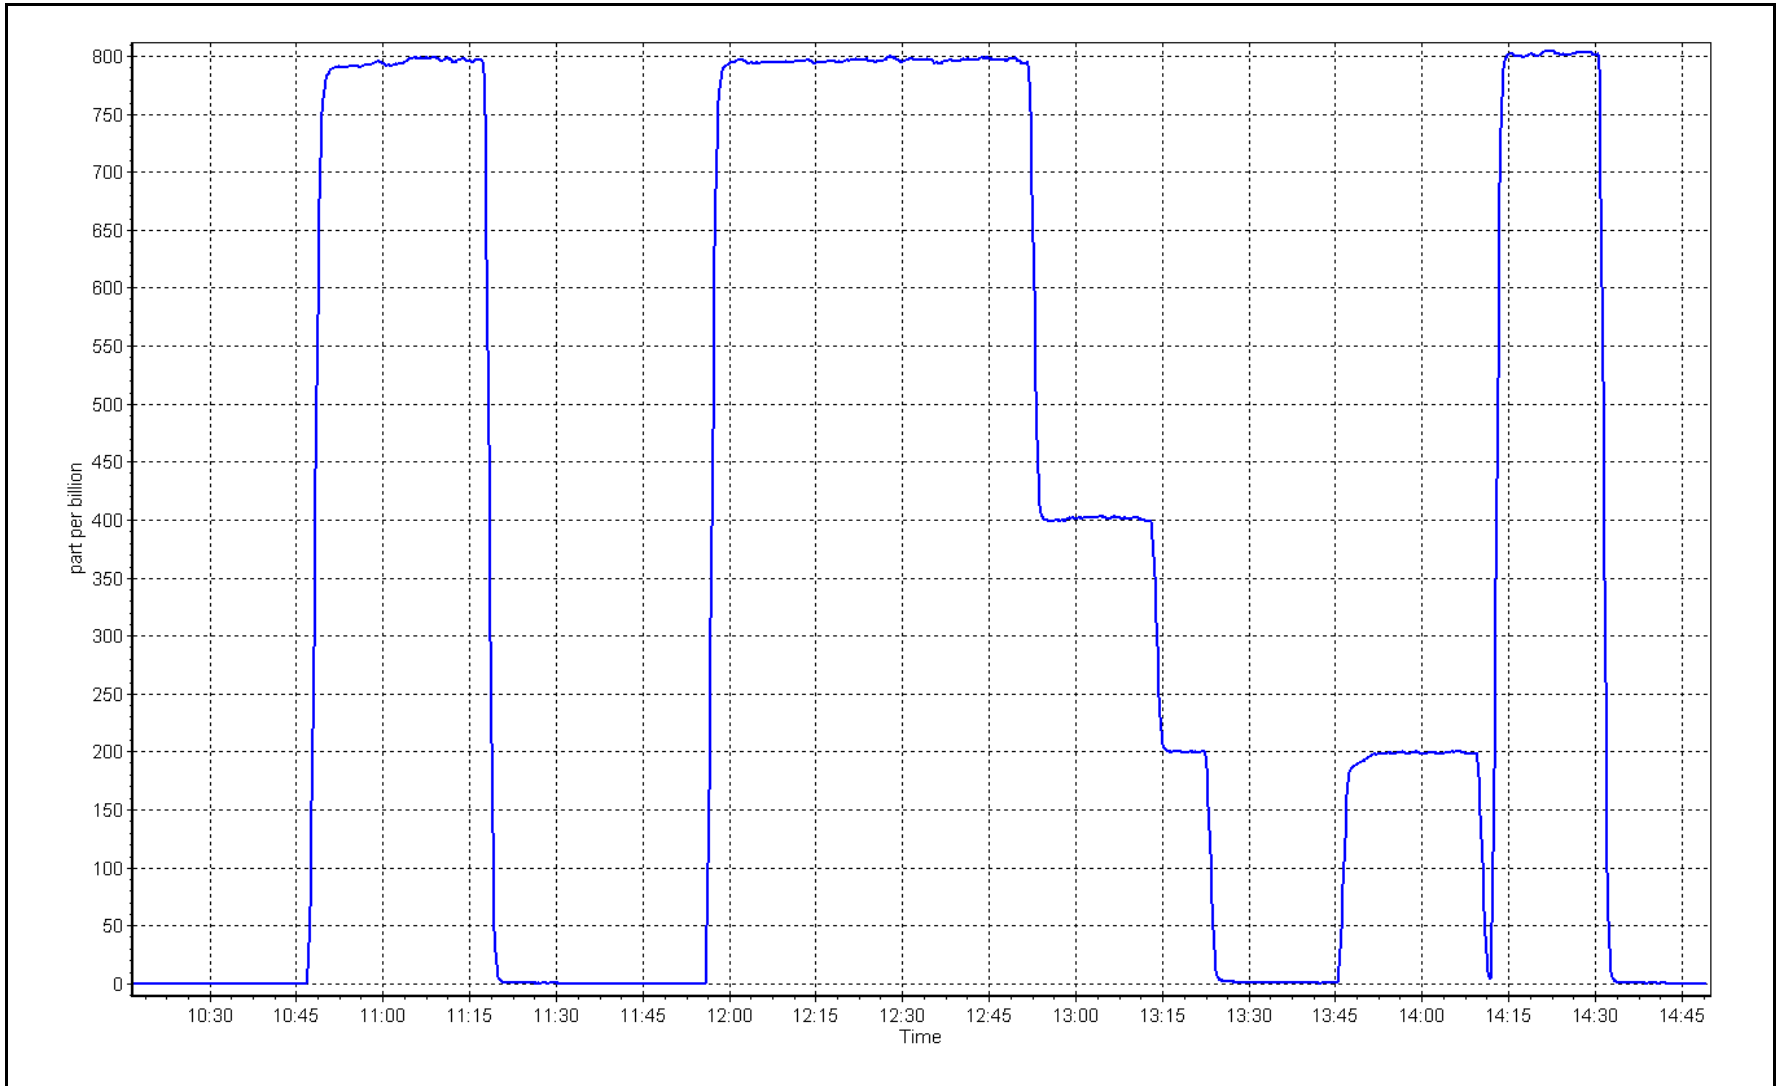



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name:	Mannix	Station number:	AMS05
Calibration Date:	January 3, 2023	Last Cal Date:	December 8, 2022
Start time (MST):	10:25	End time (MST):	15:15
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	4.92	ppm	Cal Gas Exp Date:	February 9, 2024
Cal Gas Cylinder #:	EY0002433			
Removed Cal Gas Conc:	4.92	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	1845
ZAG Make/Model:	API T701H		Serial Number:	832

Analyzer Information

Analyzer make:	Thermo 43iQTL	Analyzer serial #:	1203169745
Converter make:	Global	Converter serial #:	2022-196
Analyzer Range	0 - 100 ppb		

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.996760	0.998045	Backgd or Offset:	2.15
Calibration intercept:	0.460517	0.340531	Coeff or Slope:	0.846
				2.09
				0.822

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.2	----
as found span	4919	81.3	80.0	83.2	0.964
as found 2nd point	4960	40.7	40.0	42.1	0.956
as found 3rd point	4980	20.3	20.0	21.1	0.956
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.3	----
high point	4919	81.3	80.0	80.1	0.999
second point	4960	40.7	40.0	40.5	0.989
third point	4980	20.3	20.0	20.2	0.989
as left zero	5000	0.0	0.0	0.5	----
as left span	4919	81.3	80.0	78.8	1.015
SO2 Scrubber Check	4920	80.0	800.0	0.1	----
Date of last scrubber change:				Ave Corr Factor	0.992
Date of last converter efficiency test:					efficiency

Baseline Corr As found:	83.0	Prev response:	80.20	*% change:	3.4%
Baseline Corr 2nd AF pt:	41.9	AF Slope:	1.037326	AF Intercept:	0.340572
Baseline Corr 3rd AF pt:	20.9	AF Correlation:	0.999977		

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. Scrubber check completed after calibrator zero. Adjusted the span only.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 8, 2022
Station Name:	Mannix	Station Number:	AMS05
Start Time (MST):	10:25	End Time (MST):	15:15
Analyzer make:	Thermo 43iQTL	Analyzer serial #:	1203169745

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	0.999985	≥0.995
80.0	80.1	0.9987			
40.0	40.5	0.9887	Slope	0.998045	0.90 - 1.10
20.0	20.2	0.9888			
			Intercept	0.340531	+/-3

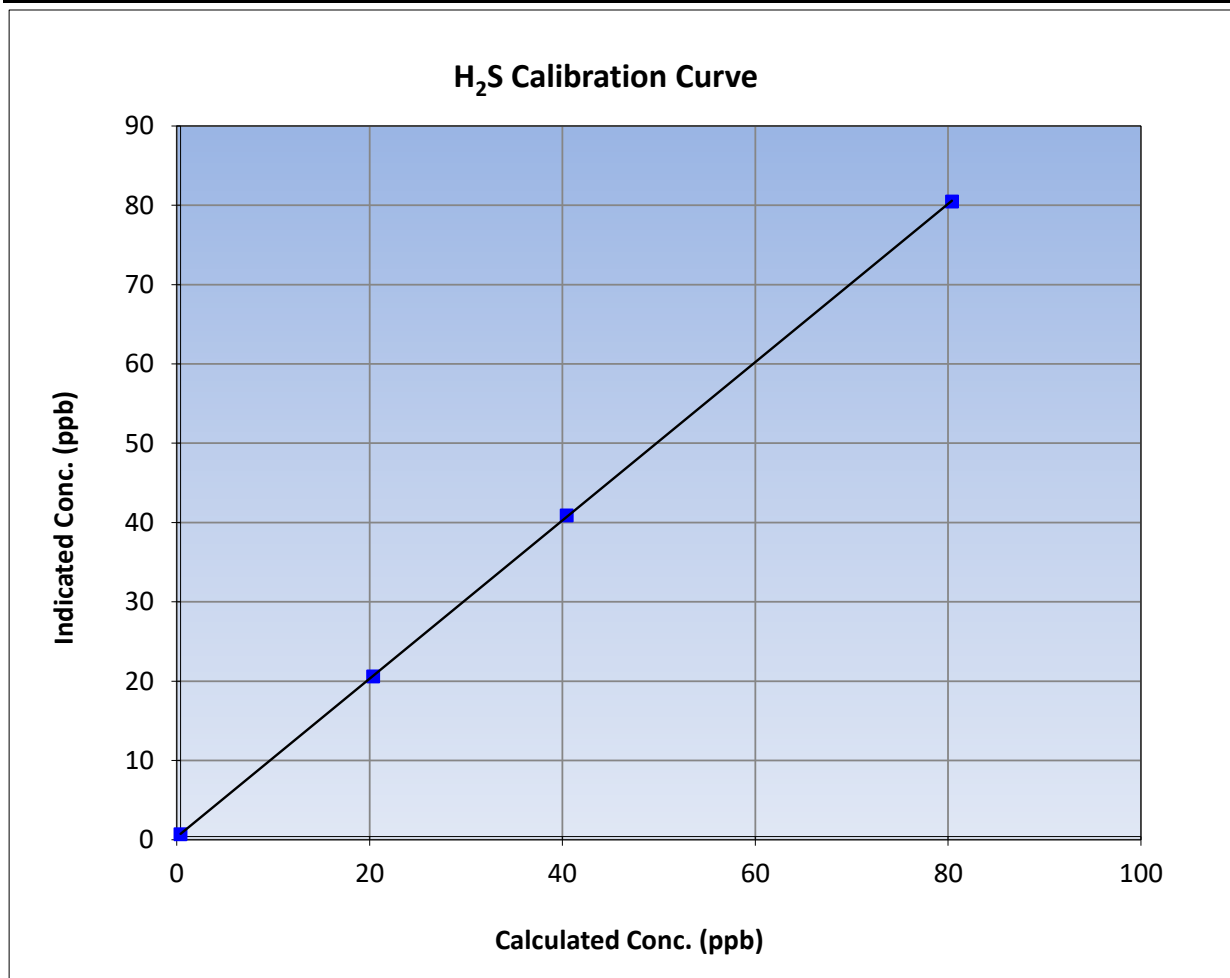

H₂S Calibration Plot

Date: January 3, 2023

Location: Mannix

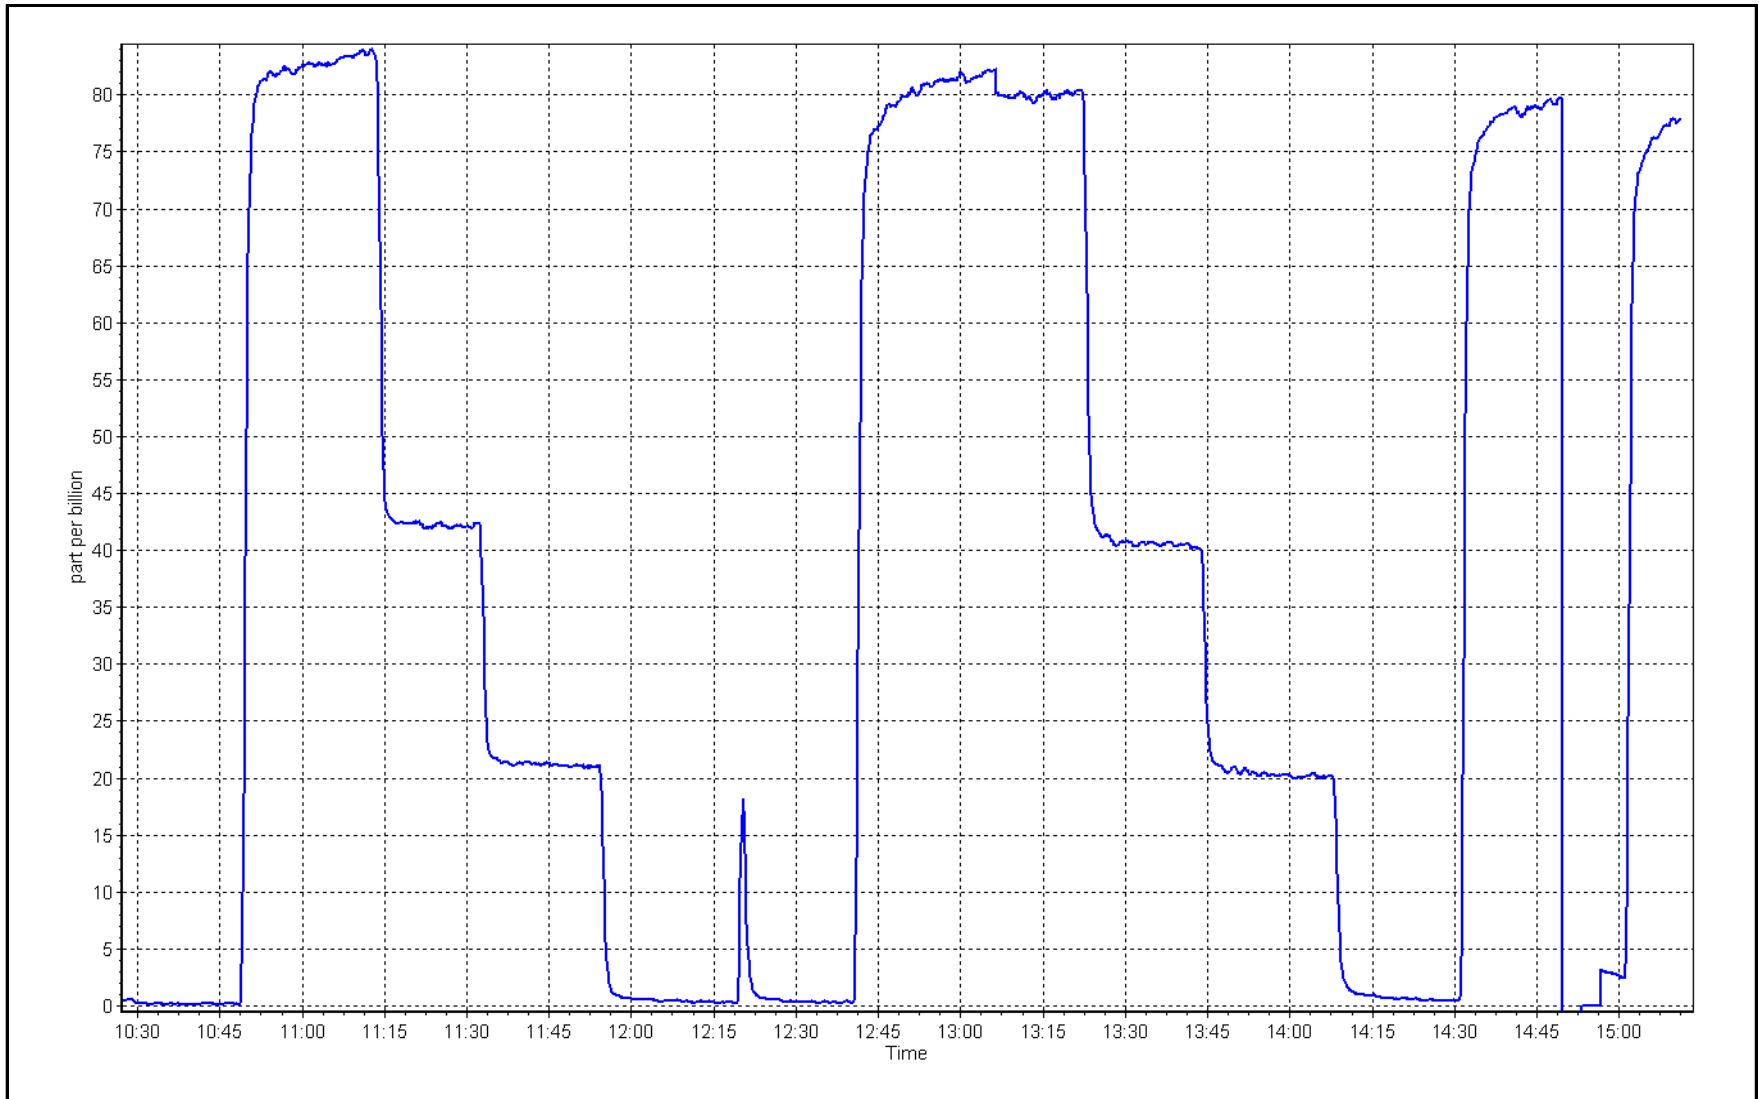



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Mannix	Station number:	AMS05
Calibration Date:	January 20, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	10:09	End time (MST):	14:55
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	XCO268098	Cal Gas Expiry Date:	January 12, 2029
CH ₄ Cal Gas Conc.	504.9 ppm	CH ₄ Equiv Conc.	1076.6 ppm
C ₃ H ₈ Cal Gas Conc.	207.9 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	
Removed CH ₄ Conc.	504.9 ppm	CH ₄ Equiv Conc.	1076.6 ppm
Removed C ₃ H ₈ Conc.	207.9 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	621
ZAG make/model:	API T701H	Serial Number:	832

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1152430011
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	2.64E-04	2.57E-04	NMHC SP Ratio:	4.73E-05
CH ₄ Retention time:	14.80	15.00	NMHC Peak Area:	193560
				207495

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.0	17.23	18.04	0.955
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.0	17.23	17.32	0.995
second point	4960	40.0	8.61	8.50	1.013
third point	4980	20.0	4.31	4.31	1.000
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.0	17.23	17.27	0.997

				Average Correction Factor	1.002
Baseline Corr AF:	18.04	Prev response	17.22	*% change	4.6%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4920	80	9.15	9.77	0.936
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4920	80	9.15	9.19	0.996
second point	4960	40	4.57	4.53	1.010
third point	4980	20	2.29	2.29	0.998
as left zero	5000	0	0.00	0.00	----
as left span	4920	80	9.15	9.17	0.997
Average Correction Factor					1.001
Baseline Corr AF:	9.77	Prev response	9.14	*% change	6.5%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.0	8.08	8.27	0.977
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.0	8.08	8.13	0.993
second point	4960	40.0	4.04	3.97	1.016
third point	4980	20.0	2.02	2.01	1.003
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.0	8.08	8.10	0.997
Average Correction Factor					1.004
Baseline Corr AF:	8.27	Prev response	8.08	*% change	2.3%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
THC Cal Slope:	1.000481	1.004873
THC Cal Offset:	-0.017000	-0.040600
CH ₄ Cal Slope:	1.000509	1.006140
CH ₄ Cal Offset:	-0.005600	-0.026000
NMHC Cal Slope:	1.000444	1.003542
NMHC Cal Offset:	-0.011600	-0.015000

Notes: Investigated high span; zero air generator failed during calibration, and most likely caused the unstable response. Re-pressurized the generator and adjusted station temperature to obtain a better response. Inlet filter changed. Captured a new zero chromatogram, and adjusted the span.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 2, 2022
Station Name:	Mannix	Station Number:	AMS05
Start Time (MST):	10:09	End Time (MST):	14:55
Analyzer make:	Thermo 55i	Analyzer serial #:	1152430011

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999896	≥ 0.995			
17.23	17.32	0.9946						
8.61	8.50	1.0129				Slope	1.004873	0.90 - 1.10
4.31	4.31	0.9999						
			Intercept	-0.040600	± 0.5			

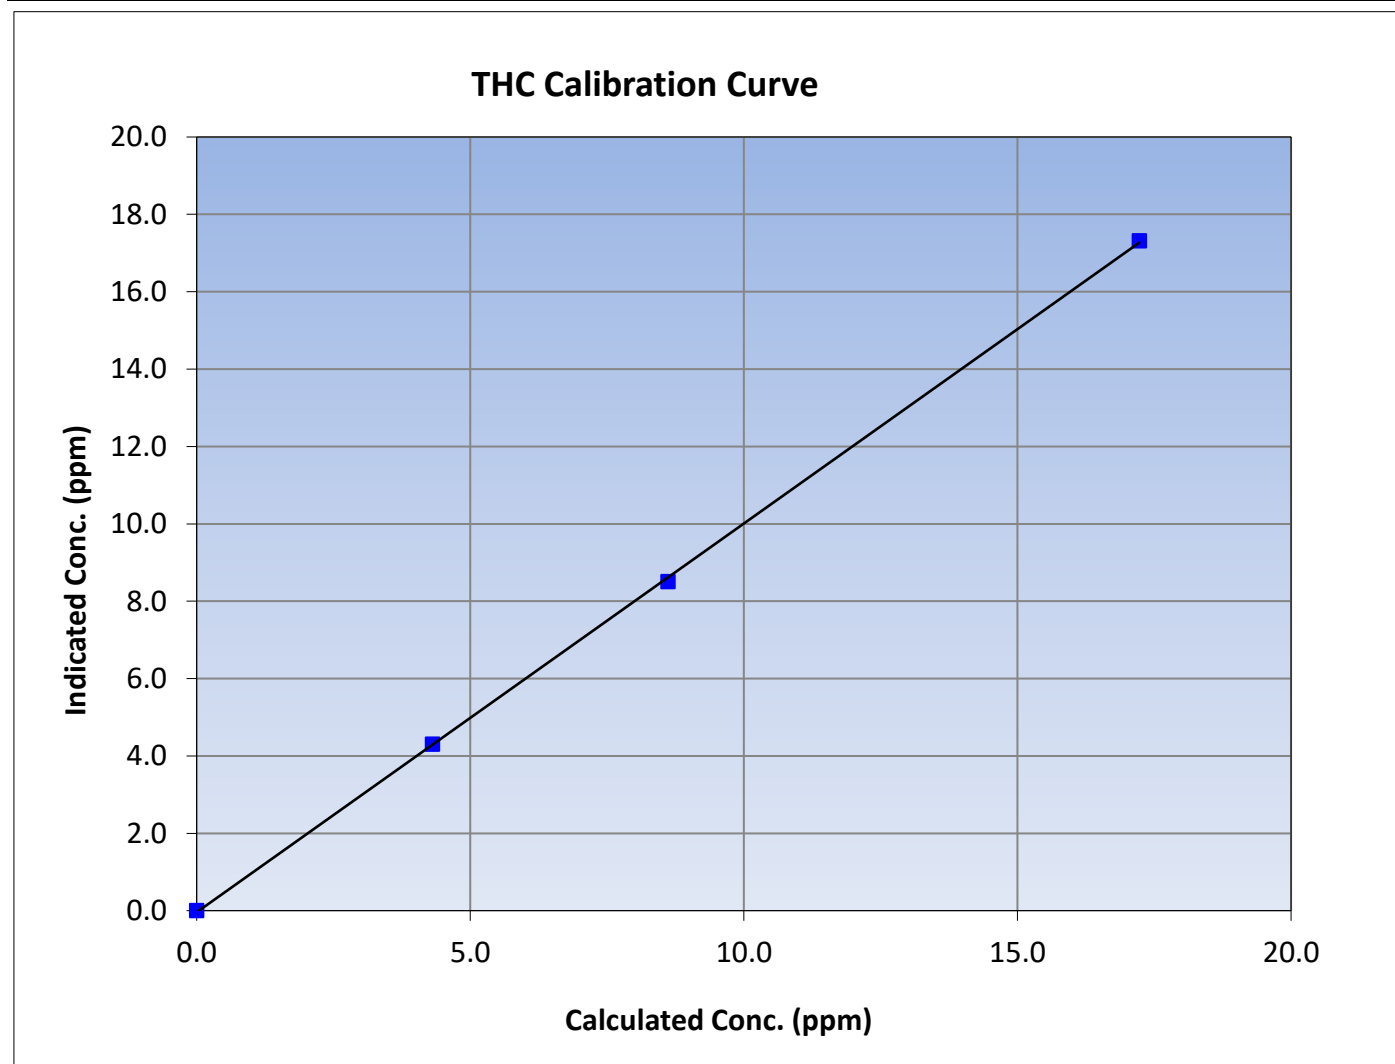



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 2, 2022
Station Name:	Mannix	Station Number:	AMS05
Start Time (MST):	10:09	End Time (MST):	14:55
Analyzer make:	Thermo 55i	Analyzer serial #:	1152430011

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999841	≥0.995
8.08	8.13	0.9934			
4.04	3.97	1.0164			
2.02	2.01	1.0028			
			Slope	1.006140	0.90 - 1.10
			Intercept	-0.026000	+/-0.5

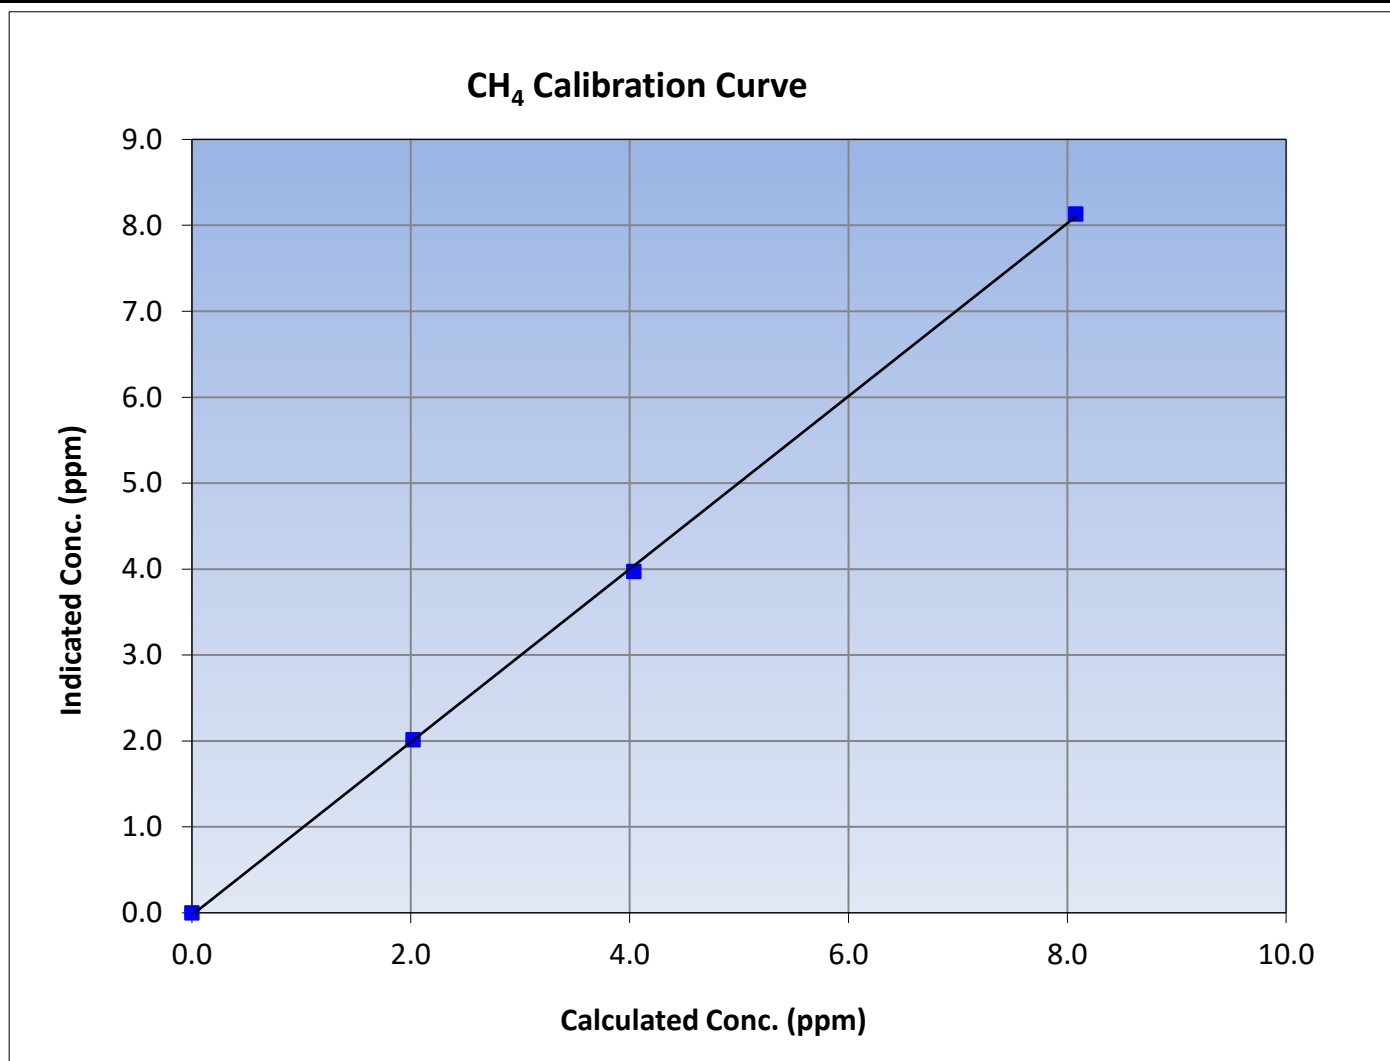



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 2, 2022
Station Name:	Mannix	Station Number:	AMS05
Start Time (MST):	10:09	End Time (MST):	14:55
Analyzer make:	Thermo 55i	Analyzer serial #:	1152430011

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999932	≥ 0.995			
9.15	9.19	0.9958						
4.57	4.53	1.0103				Slope	1.003542	0.90 - 1.10
2.29	2.29	0.9978						
			Intercept	-0.015000	± 0.5			

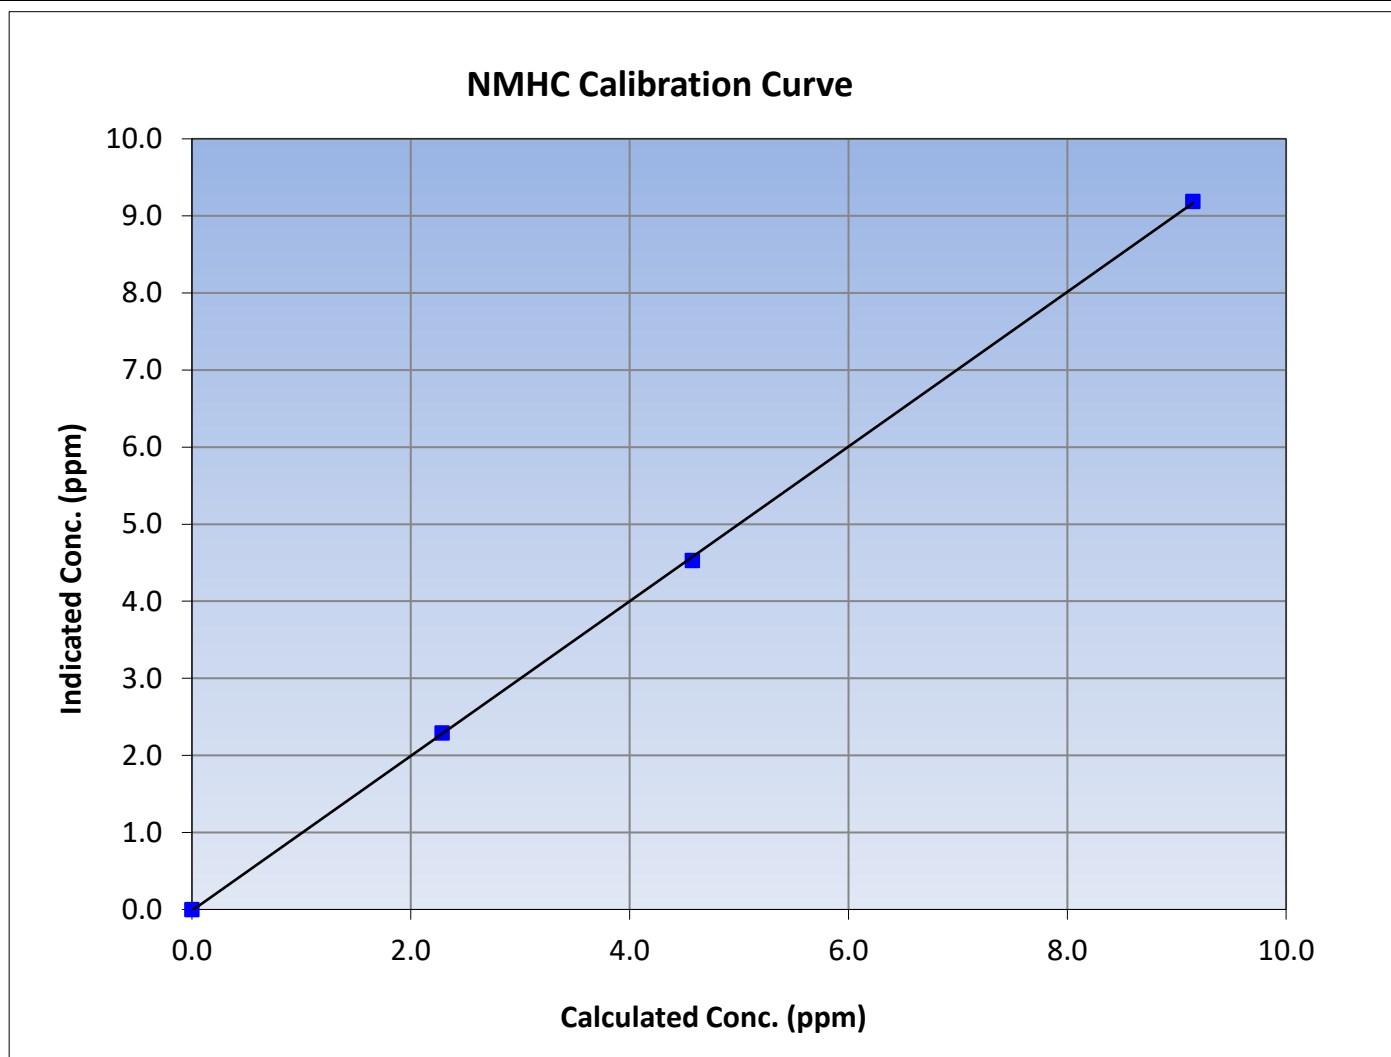

NMHC Calibration Plot

Date: January 20, 2023

Location: Mannix

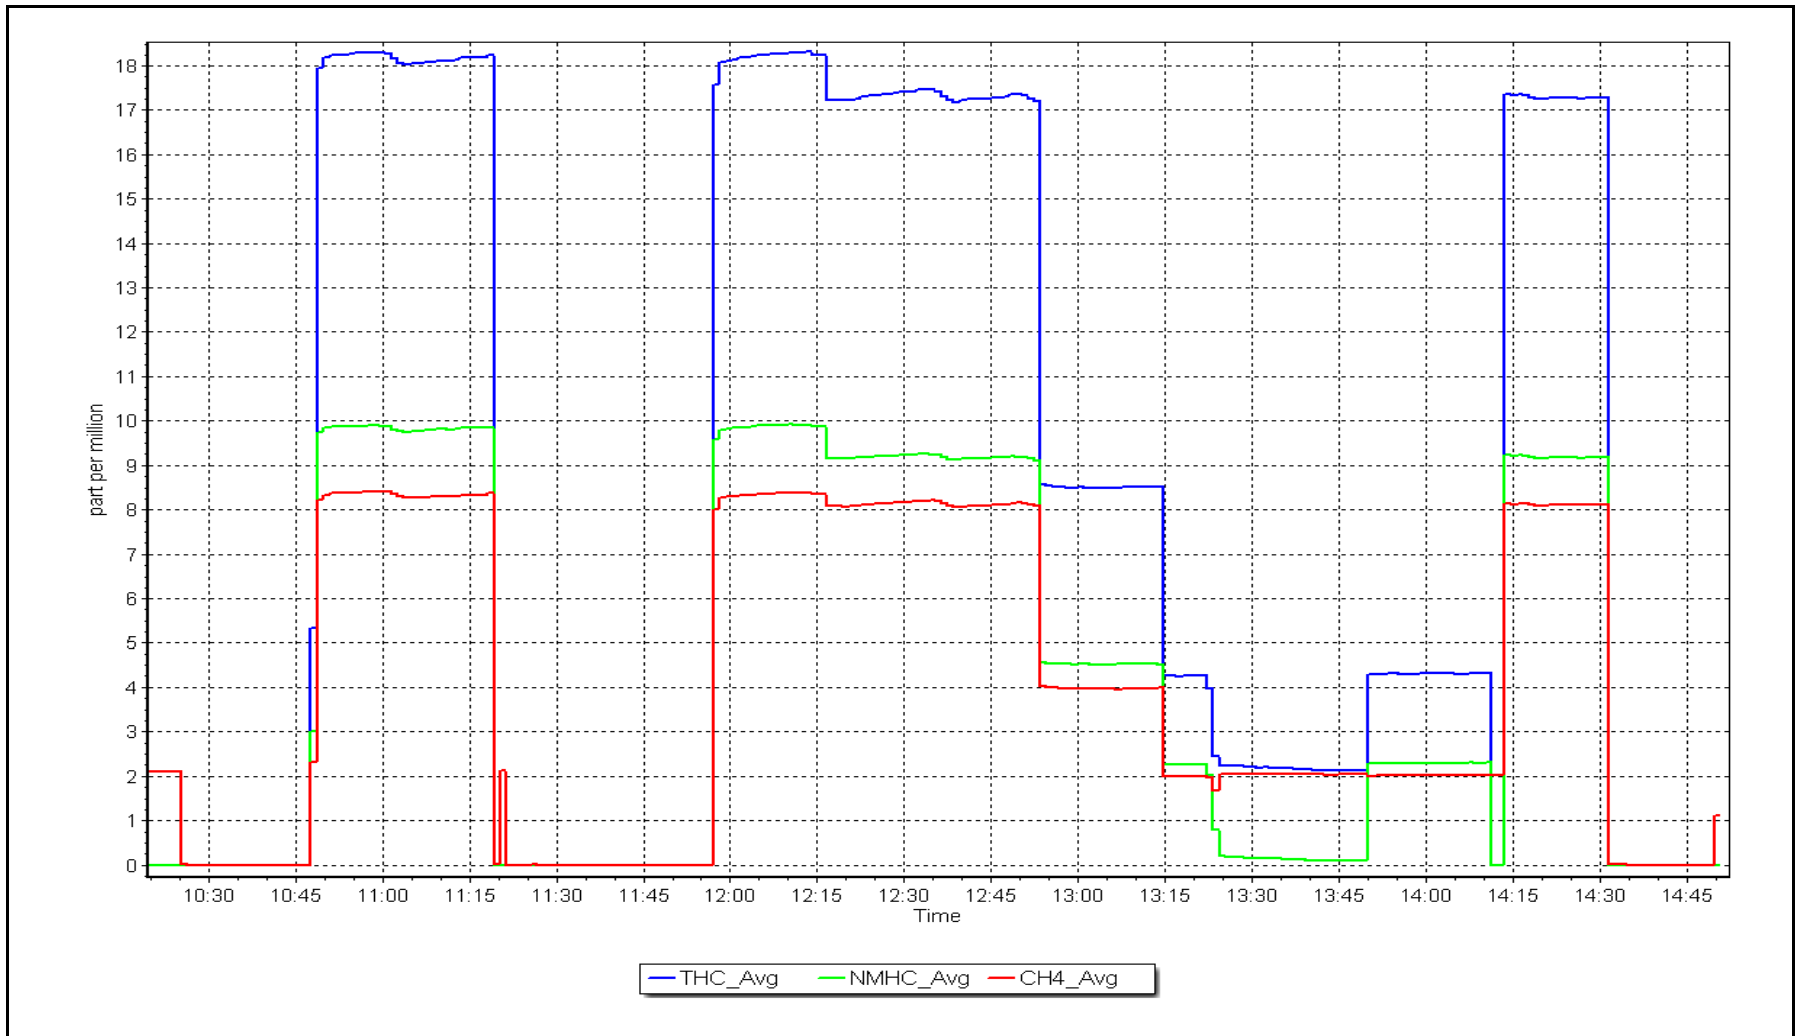



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS06
PATRICIA MCINNES
JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

August 30, 2023

Revision 01



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Patricia McInnes	Station number:	AMS06
Calibration Date:	January 9, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	10:14	End time (MST):	13:09
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.78	ppm	Cal Gas Exp Date:	September 9, 2024
Cal Gas Cylinder #:	AAL070632			
Removed Cal Gas Conc:	49.78	ppm	Rem Gas Exp Date:	N/A
Removed Gas Cyl #:	N/A		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	689
ZAG Make/Model:	API T701		Serial Number:	3566

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	1160290013
Analyzer Range:	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.992599	0.992084	Backgd or Offset:	17.2	17.2
Calibration intercept:	1.461745	1.741680	Coeff or Slope:	0.907	0.907

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	-0.3	----
as found span	4920	80.3	799.5	792.2	1.009
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.0	----
high point	4920	80.3	799.5	794.1	1.007
second point	4960	40.2	400.2	399.4	1.002
third point	4980	20.1	200.1	202.2	0.990
as left zero	5000	0.0	0.0	-0.1	----
as left span	4920	80.3	799.5	796.5	1.004
Average Correction Factor					1.000

Baseline Corr As found:	792.50	Previous response	795.01	*% change	-0.3%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds. No adjustments made.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 9, 2023	Previous Calibration:	December 2, 2022
Station Name:	Patricia McInnes	Station Number:	AMS06
Start Time (MST):	10:14	End Time (MST):	13:09
Analyzer make:	Thermo 43i	Analyzer serial #:	1160290013

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	0.999978	≥0.995
799.5	794.1	1.0068			
400.2	399.4	1.0021	Slope	0.992084	0.90 - 1.10
200.1	202.2	0.9897			
			Intercept	1.741680	+/-30

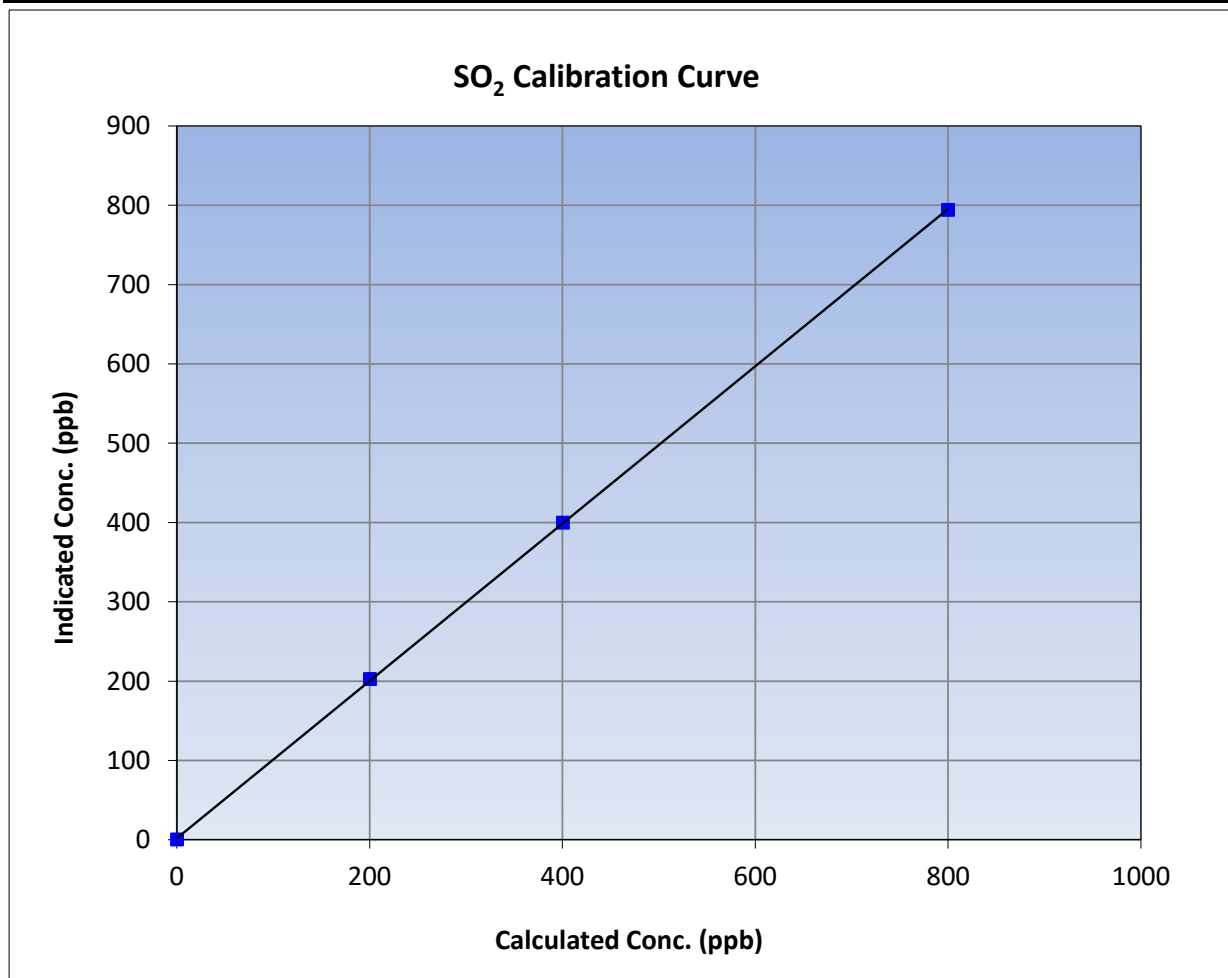

SO2 Calibration Plot

Date: January 9, 2023

Location: Patricia McInnes

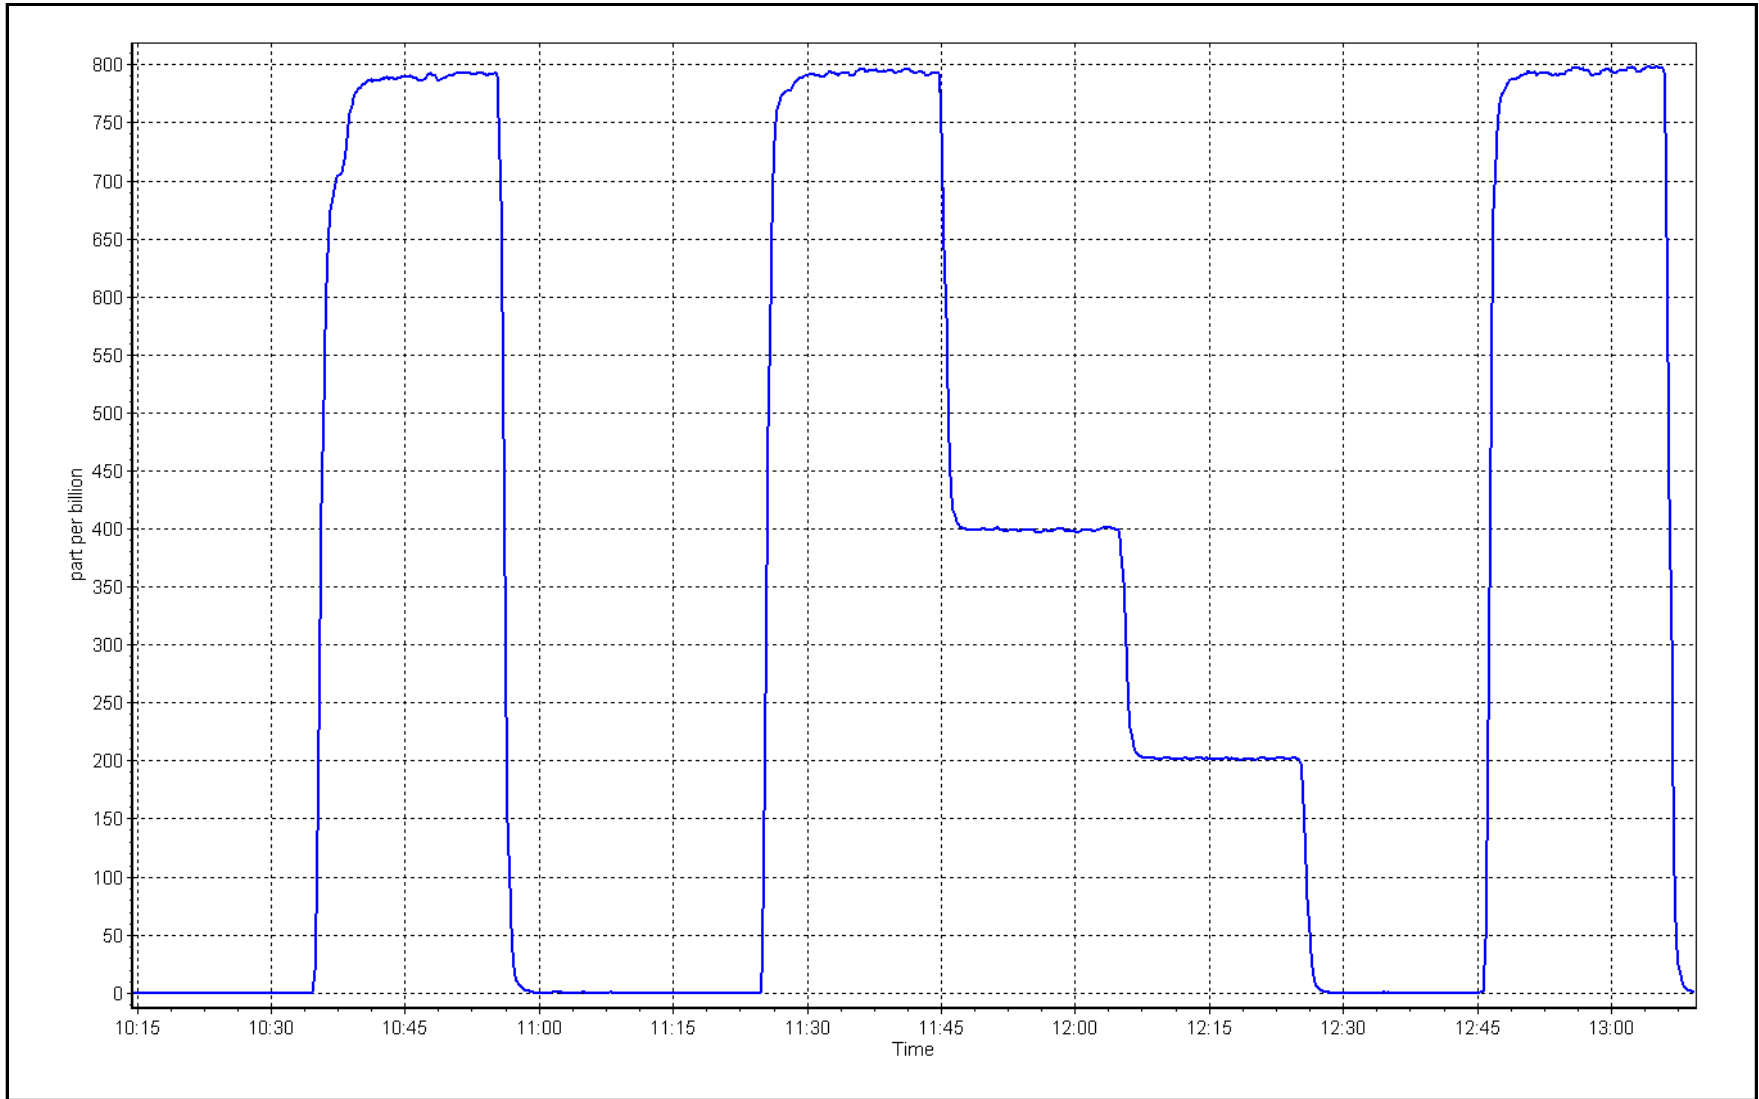



Wood Buffalo Environmental Association

H2S Calibration Report

Version-11-2021

Station Information

Station Name: Patricia McInnes Station number: AMS 06
 Calibration Date: January 3, 2023 Last Cal Date: December 12, 2022
 Start time (MST): 12:00 End time (MST): 14:36
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.38 ppm Cal Gas Exp Date: March 2, 2023
 Cal Gas Cylinder #: EY0000809
 Removed Cal Gas Conc: 5.38 ppm Rem Gas Exp Date: N/A
 Removed Gas Cyl #: N/A Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 3566
 ZAG Make/Model: API T701 H Serial Number: 689

Analyzer Information

Analyzer make: Thermo 43i TLE Analyzer serial #: 1218153358
 Converter make: Global G150 Converter serial #: 2022-195
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.992920	0.997488	Backgd or Offset: 1.97	1.97
Calibration intercept:	0.677080	0.117191	Coeff or Slope: 1.155	1.155

H2S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0		----
as found span	4926	74.3	79.9		
as found 2nd point	4963	37.2	40.0		
as found 3rd point	4981	18.6	20.0		
new cylinder response					

H2S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.0	----
high point	4926	74.3	79.9	79.8	1.002
second point	4963	37.2	40.0	40.1	0.998
third point	4981	18.6	20.0	20.2	0.991
as left zero	5000	0.0	0.0	-0.1	----
as left span	4926	74.3	79.9	79.2	1.009
SO2 Scrubber Check	4920	80.3	803.0	0.1	----
Date of last scrubber change:	December 20, 2021			Ave Corr Factor	0.997
Date of last converter efficiency test:	efficiency				

Baseline Corr As found: NA Prev response: 80.05 *% change: NA
 Baseline Corr 2nd AF pt: NA AF Slope: NA AF Intercept: NA
 Baseline Corr 3rd AF pt: NA AF Correlation: NA

* = > +/-5% change initiates investigation

Notes: No as founds due to the converter not working. Replaced the converter. Adjusted both zero and span. Ran a SO2 scrubber check after the calibrator zero.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

H2S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 12, 2022
Station Name:	Patricia McInnes	Station Number:	AMS 06
Start Time (MST):	12:00	End Time (MST):	14:36
Analyzer make:	Thermo 43i TLE	Analyzer serial #:	1218153358

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	0.999990	≥0.995
79.9	79.8	1.0018			
40.0	40.1	0.9981	Slope	0.997488	0.90 - 1.10
20.0	20.2	0.9909			
			Intercept	0.117191	+/-3

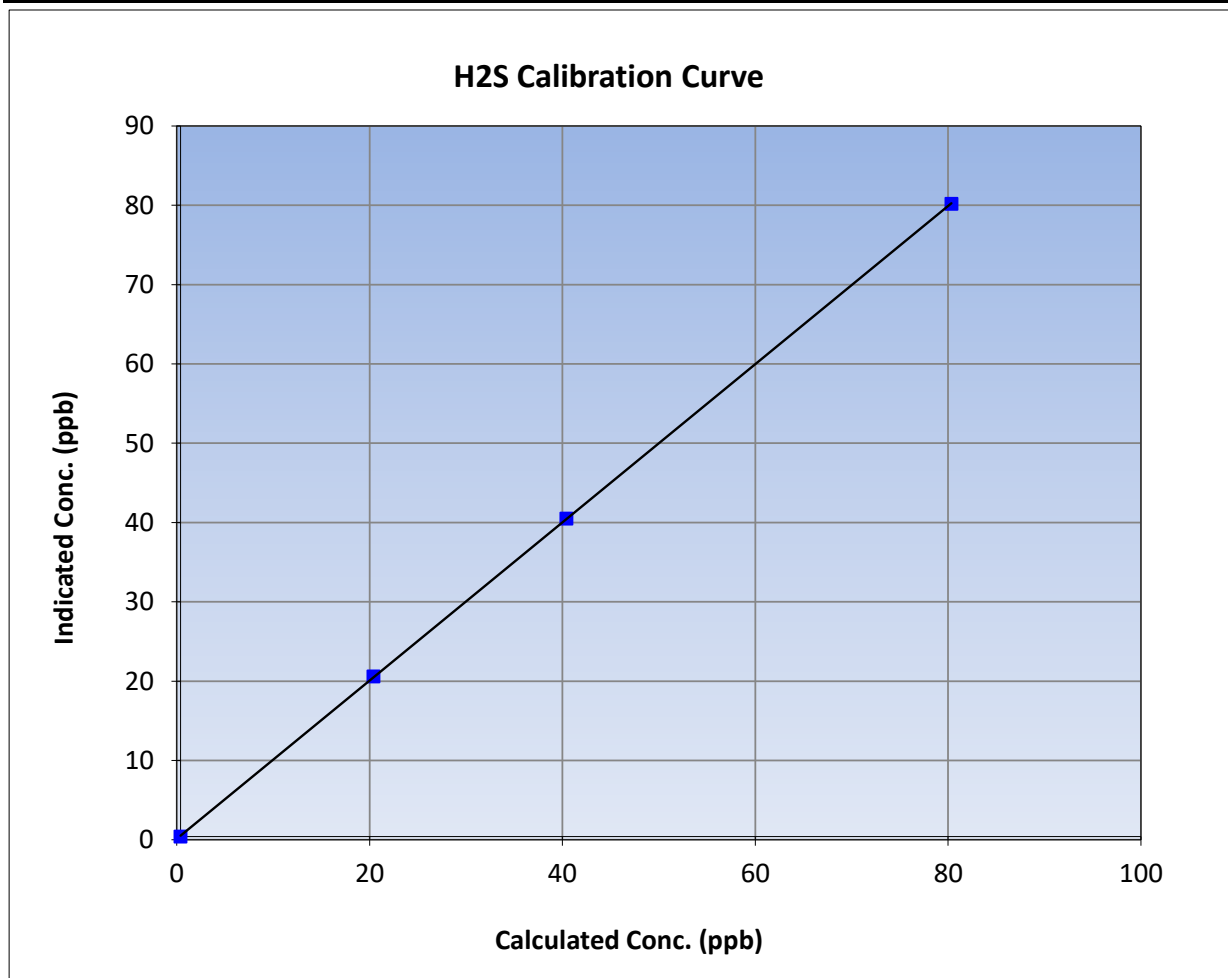

H2S Calibration Plot

Date: January 3, 2023

Location: Patricia McInnes

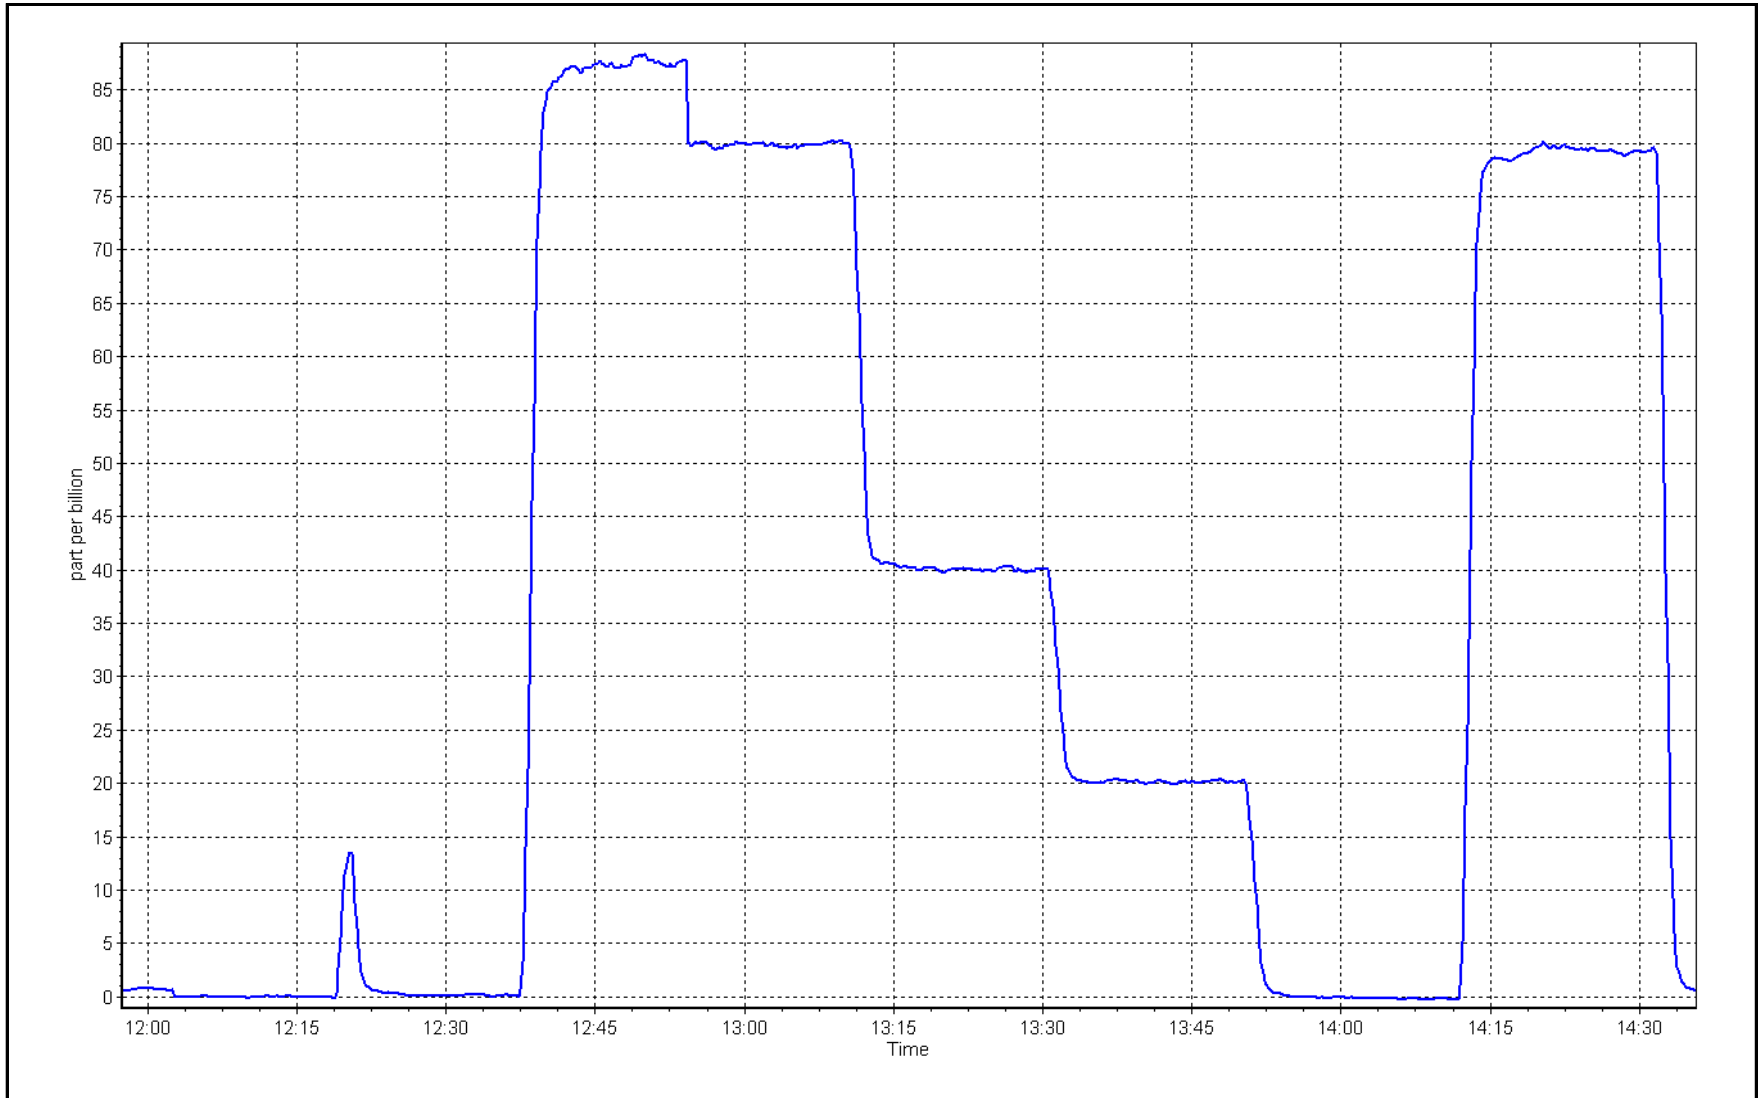



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Patricia McInnes	Station number:	AMS06
Calibration Date:	January 9, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	10:14	End time (MST):	13:09
Reason:	Cylinder Change N2 cylinder change		

Calibration Standards

Gas Cert Reference:	AAL070632	Cal Gas Expiry Date:	September 9, 2024
CH4 Cal Gas Conc.	501.6 ppm	CH4 Equiv Conc.	1066.2 ppm
C3H8 Cal Gas Conc.	205.3 ppm		
Removed Gas Ref.	N/A	Removed Gas Expiry:	N/A
Removed CH4 Conc.	501.6 ppm	CH4 Equiv Conc.	1066.2 ppm
Removed C3H8 Conc.	205.3 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	689
ZAG make/model:	API T701	Serial Number:	3566

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1180320037
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH4 Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH4 SP Ratio:	3.19E-04	3.19E-04	NMHC SP Ratio:	5.63E-05
CH4 Retention time:	13.8	13.8	NMHC Peak Area:	161210

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.3	17.12	17.04	1.005
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.3	17.12	17.14	0.999
second point	4960	40.2	8.57	8.53	1.004
third point	4980	20.1	4.29	4.29	0.998
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.3	17.12	17.01	1.007

Average Correction Factor	1.001
---------------------------	-------

Baseline Corr AF:	17.04	Prev response	17.14	*% change	-0.6%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF Limit= 0.95-1.05
as found zero	5000	0	0.00	0.00	----
as found span	4920	80.3	9.07	9.01	1.006
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4920	80.3	9.07	9.07	0.999
second point	4960	40.2	4.54	4.52	1.004
third point	4980	20.1	2.27	2.27	0.999
as left zero	5000	0	0.00	0.00	----
as left span	4920	80.3	9.07	8.98	1.010
Average Correction Factor					1.001
Baseline Corr AF:	9.01	Prev response	9.08	*% change	-0.7%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF Limit= 0.95-1.05
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.3	8.06	8.03	1.004
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.3	8.06	8.07	0.998
second point	4960	40.2	4.03	4.01	1.005
third point	4980	20.1	2.02	2.02	0.998
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.3	8.06	8.03	1.003
Average Correction Factor					1.000
Baseline Corr AF:	8.03	Prev response	8.06	*% change	-0.5%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
THC Cal Slope:	1.000220	1.000499
THC Cal Offset:	0.011138	-0.007453
CH ₄ Cal Slope:	1.000512	1.001107
CH ₄ Cal Offset:	0.003196	-0.004401
NMHC Cal Slope:	1.000100	1.000174
NMHC Cal Offset:	0.008141	-0.003652

Notes: Changed the inlet filter and the N₂ cylinder after as founds. No adjustments made.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 9, 2023	Previous Calibration:	December 2, 2022
Station Name:	Patricia McInnes	Station Number:	AMS06
Start Time (MST):	10:14	End Time (MST):	13:09
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320037

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999990	≥ 0.995			
17.12	17.14	0.9991						
8.57	8.53	1.0045				Slope	1.000499	0.90 - 1.10
4.29	4.29	0.9981						
			Intercept	-0.007453	± 0.5			

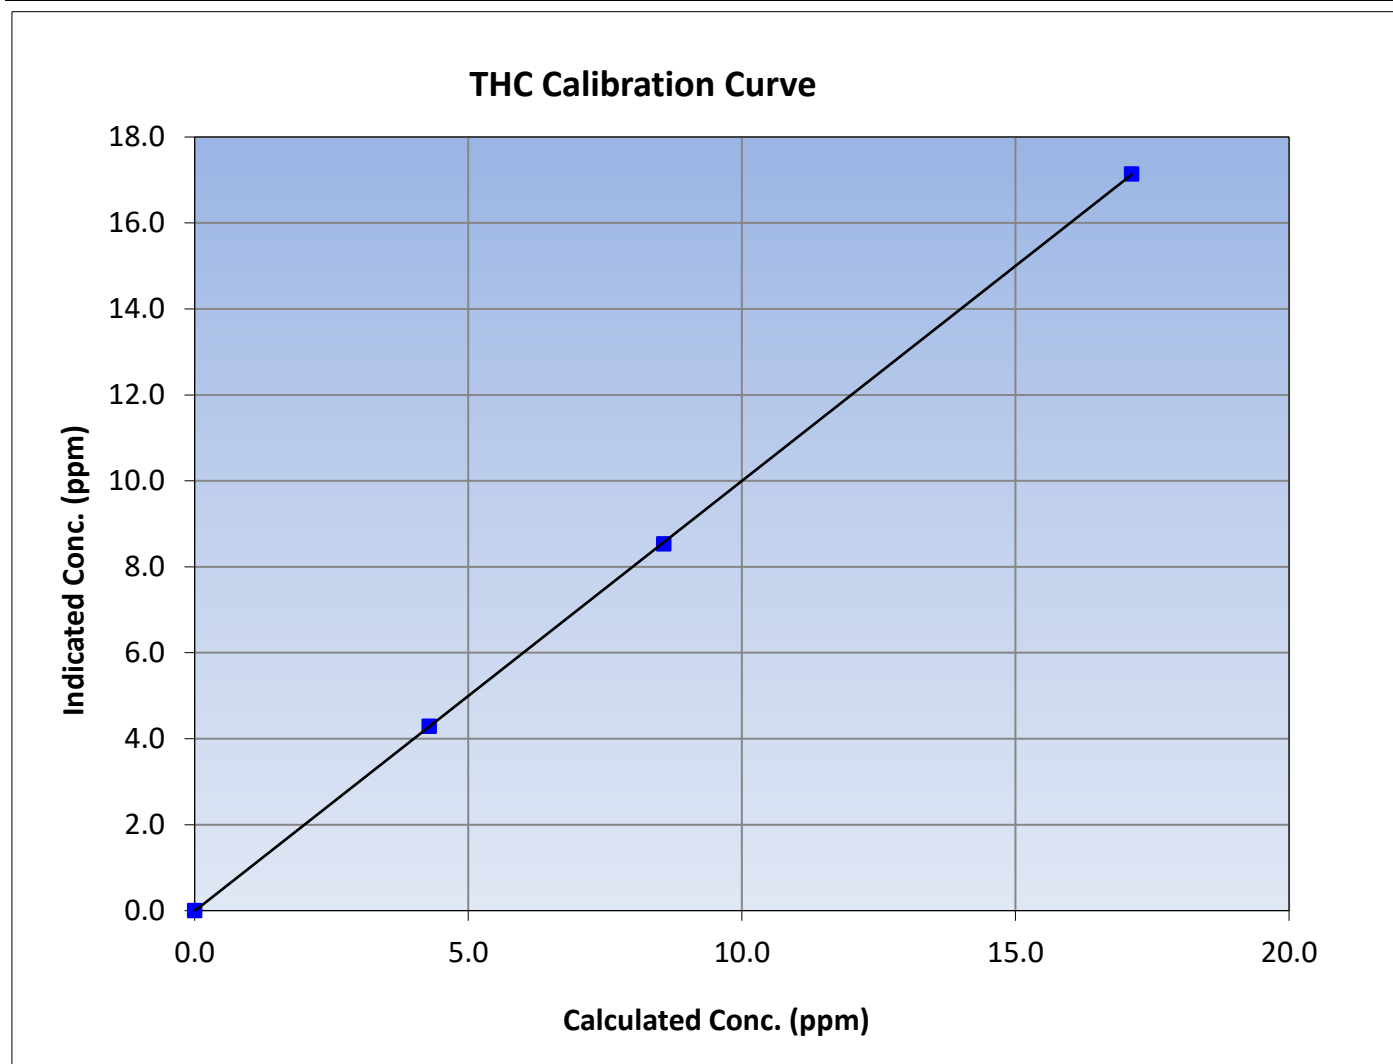



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 9, 2023	Previous Calibration:	December 2, 2022
Station Name:	Patricia McInnes	Station Number:	AMS06
Start Time (MST):	10:14	End Time (MST):	13:09
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320037

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999986	≥0.995			
8.06	8.07	0.9985						
4.03	4.01	1.0047				Slope	1.001107	0.90 - 1.10
2.02	2.02	0.9977						
			Intercept	-0.004401	+/-0.5			

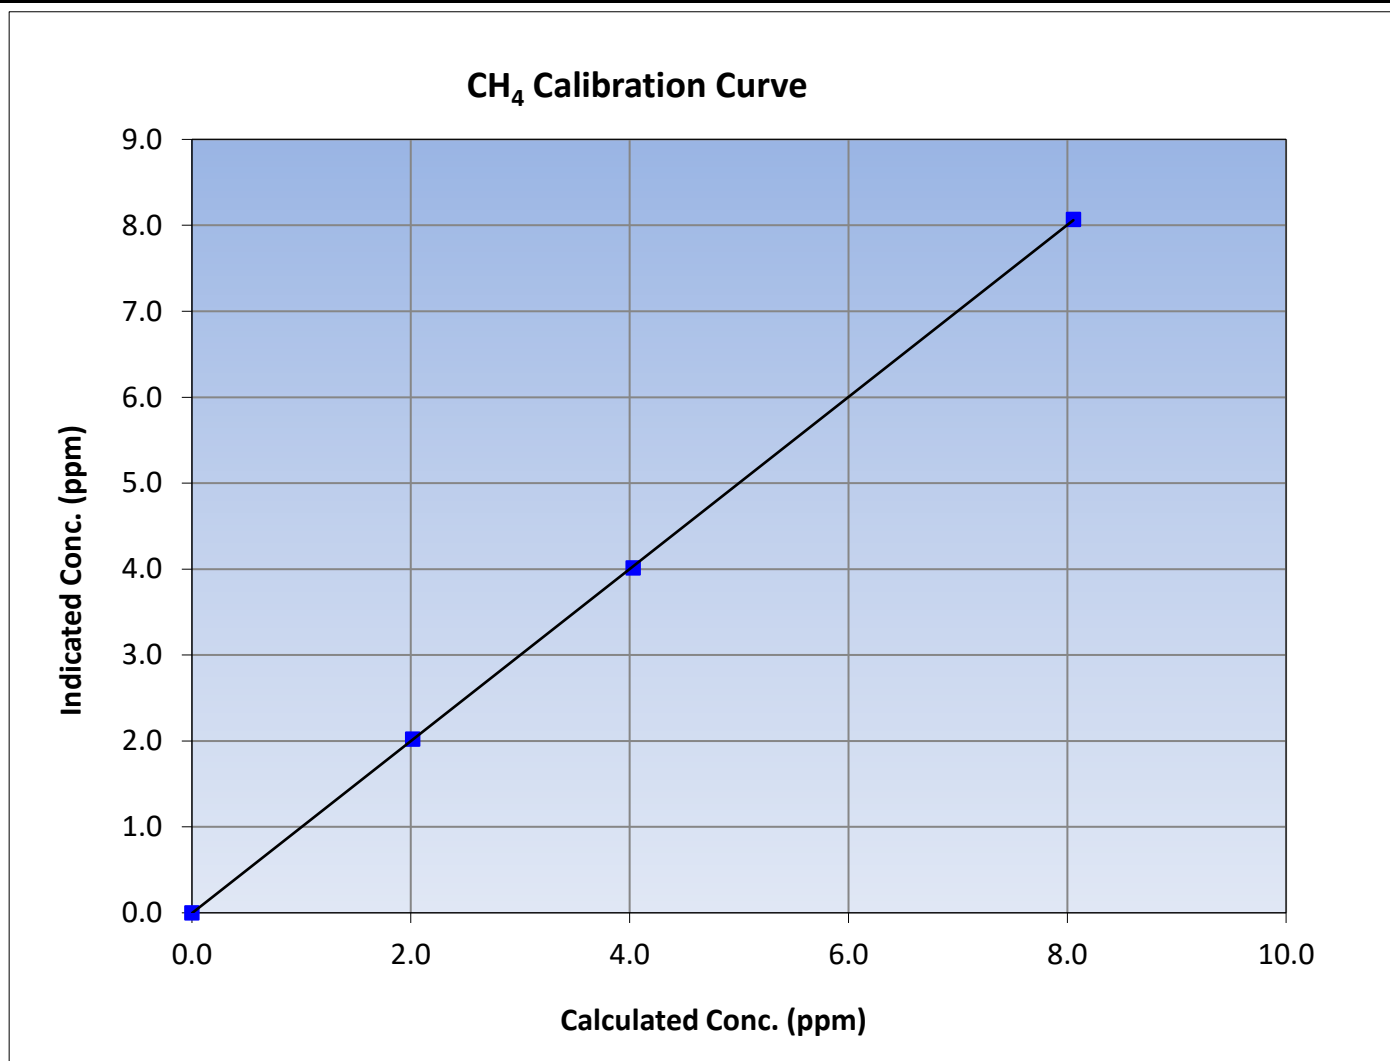



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 9, 2023	Previous Calibration:	December 2, 2022
Station Name:	Patricia McInnes	Station Number:	AMS06
Start Time (MST):	10:14	End Time (MST):	13:09
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320037

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999991	≥ 0.995			
9.07	9.07	0.9995						
4.54	4.52	1.0045				Slope	1.000174	0.90 - 1.10
2.27	2.27	0.9985						
			Intercept	-0.003652	± 0.5			

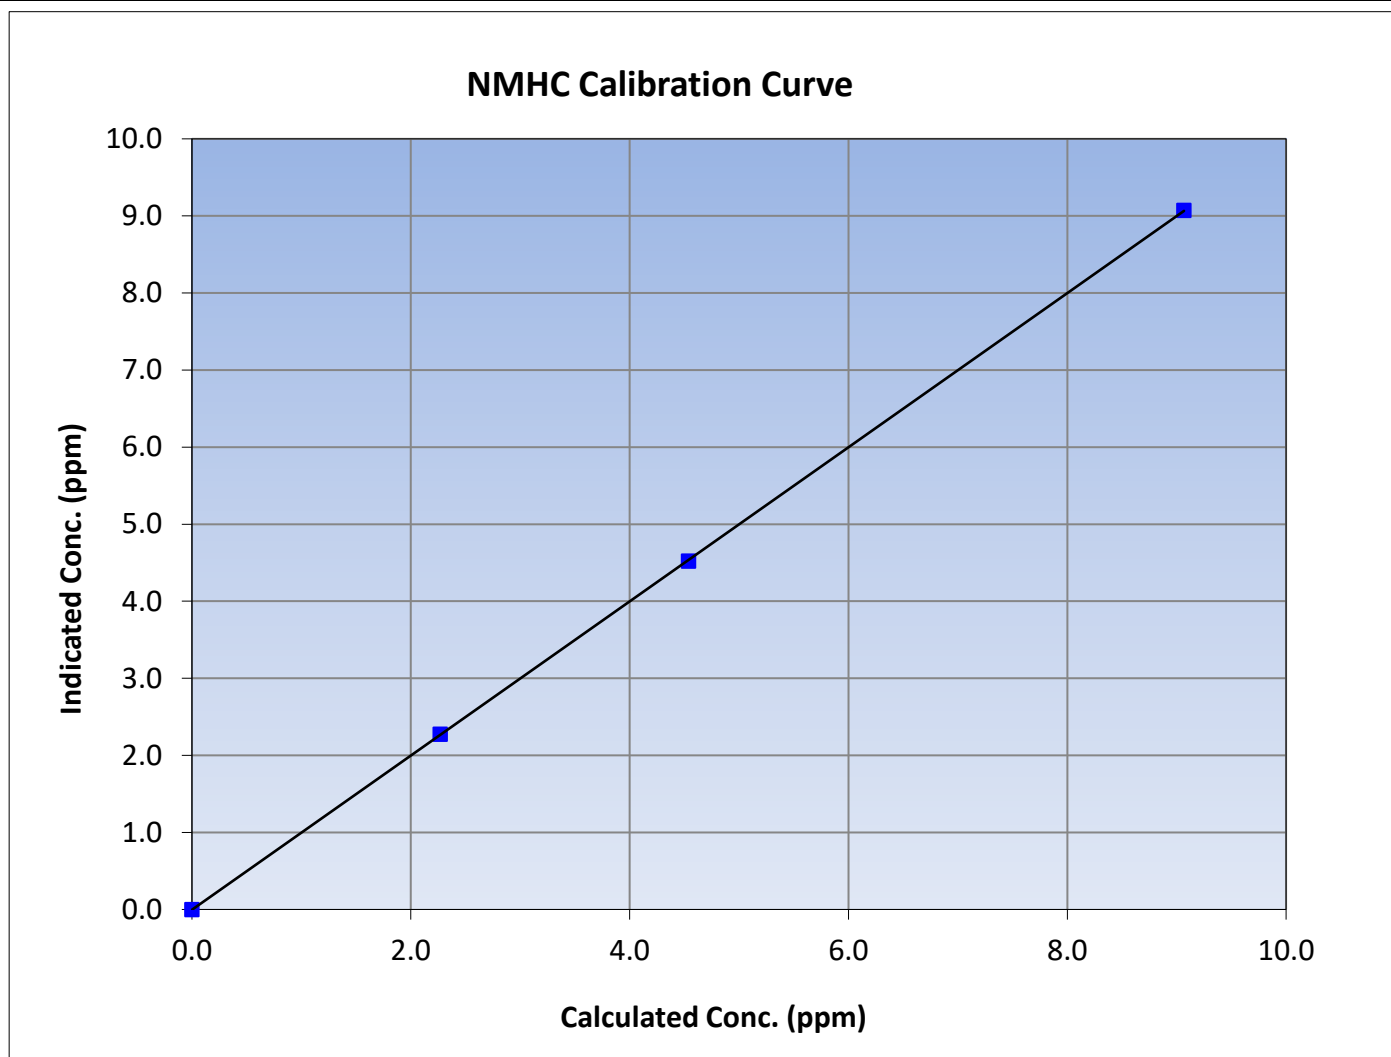

NMHC Calibration Plot

Date: January 9, 2023

Location: Patricia McInnes

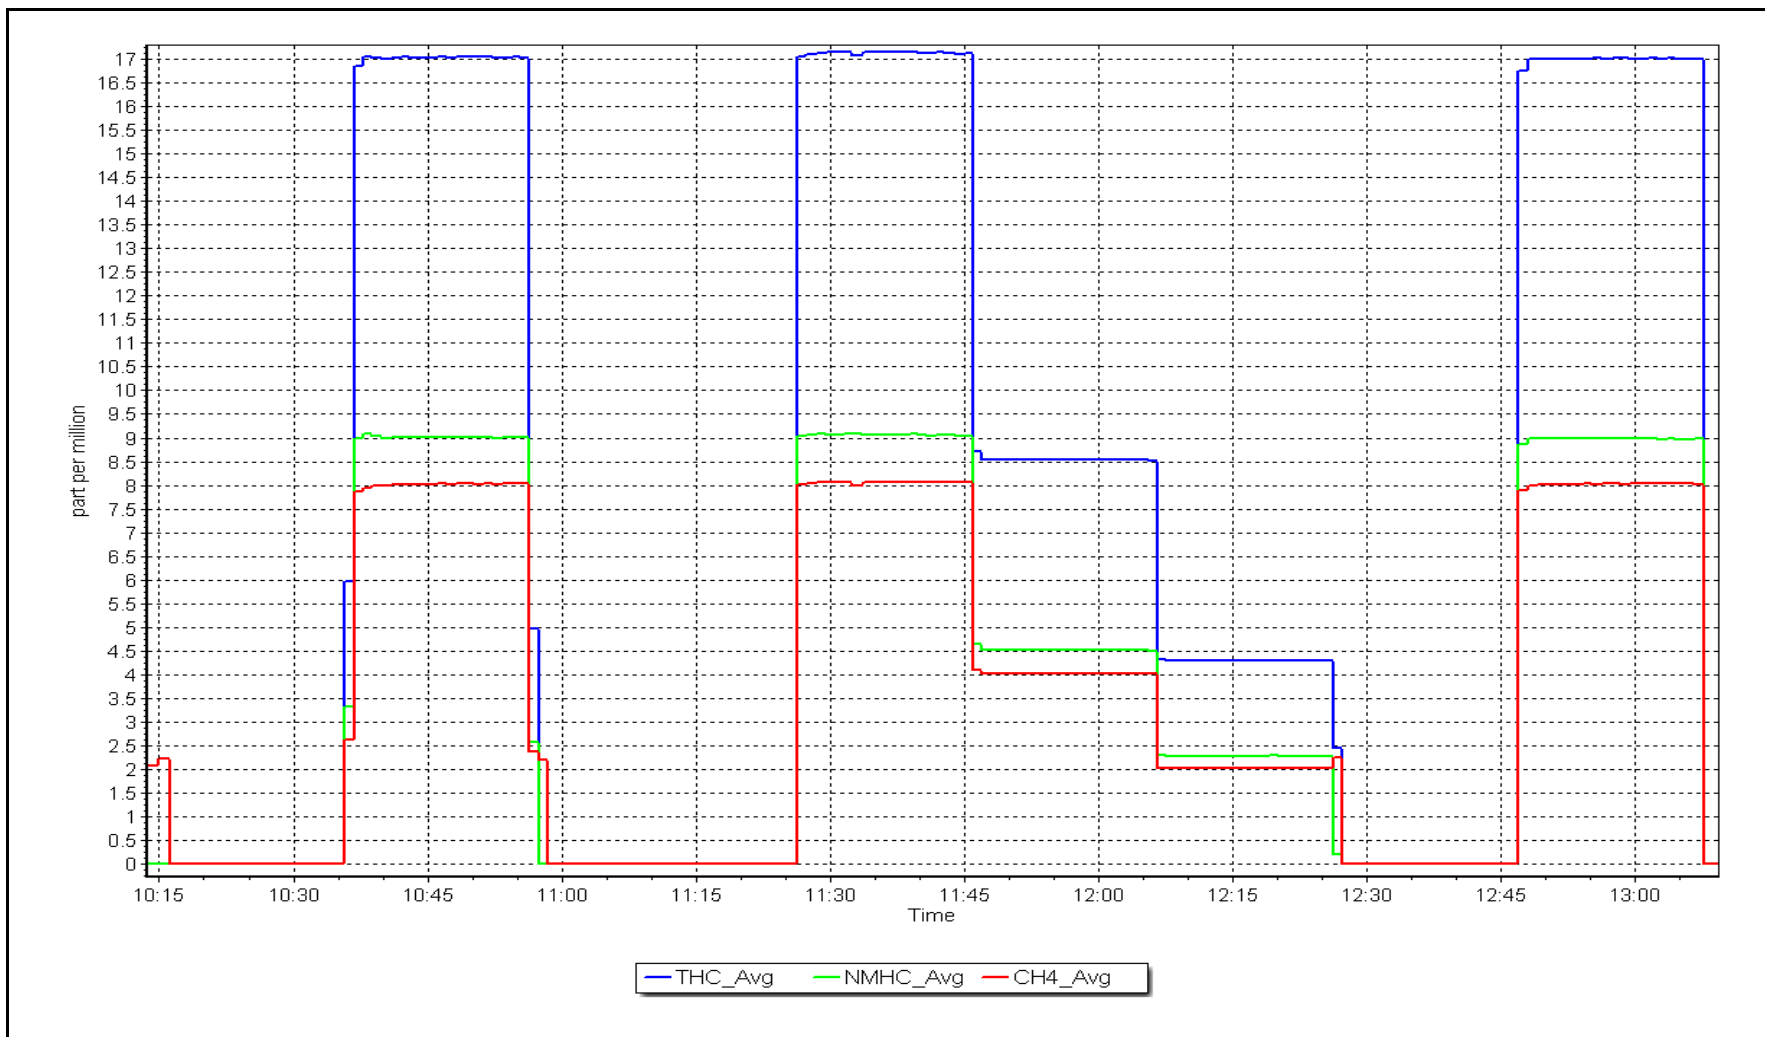



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Patricia McInnes
Calibration Date: January 5, 2023
Start time (MST): 10:11
Reason: Routine
Station number: AMS06
Last Cal Date: December 1, 2022
End time (MST): 14:44

Calibration Standards

NO Gas Cylinder #: T26D9MR
NOX Cal Gas Conc: 52.51 ppm
Removed Cylinder #: N/A
Removed Gas NOX Conc: 52.51 ppm
NOX gas Diff:
Calibrator Model: Teledyne API T700
ZAG make/model: Teledyne API T701
Cal Gas Expiry Date: August 18, 2023
NO Cal Gas Conc: 51.98 ppm
Removed Gas Exp Date: N/A
Removed Gas NO Conc: 51.98 ppm
NO gas Diff:
Serial Number: 3566
Serial Number: 689

Analyzer Information

Analyzer make: Thermo 42i
NOX Range (ppb): 0 - 1000 ppb
Analyzer serial #: 1172750022

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	0.818	0.818	NO bkgnd or offset:	3.2	3.2
NOX coeff or slope:	0.996	0.996	NOX bkgnd or offset:	3.8	3.8
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	156.3	154.2

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.000673	1.000715
NO _x Cal Offset:	2.819985	2.680164
NO Cal Slope:	1.000413	0.999284
NO Cal Offset:	1.780160	1.700041
NO ₂ Cal Slope:	1.002852	1.007019
NO ₂ Cal Offset:	0.310120	0.124373



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.1	0.2	-0.2	----	----
as found span	4923	76.9	807.6	799.5	8.2	812.0	799.6	12.4	0.9946	0.9998
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.2	0.3	-0.1	----	----
high point	4923	76.9	807.6	799.5	8.2	809.7	799.9	9.9	0.9974	0.9994
second point	4962	38.5	404.3	400.2	4.1	408.3	402.3	6.0	0.9903	0.9949
third point	4981	19.2	201.6	199.6	2.0	207.1	202.6	4.5	0.9736	0.9852
as left zero	5000	0.0	0.0	0.0	0.0	0.0	0.2	-0.2	----	----
as left span	4923	76.9	807.6	388.0	419.7	807.4	387.2	420.4	1.0003	1.0019
Average Correction Factor									0.9871	0.9932

Corrected As found	NO _x = 811.9 ppb	NO = 799.4 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = 0.1%	
Previous Response	NO _x = 811.0 ppb	NO = 801.6 ppb		*Percent Change	NO = -0.3%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO ₂)						
as found GPT point (200 ppb NO ₂)						
as found GPT point (100 ppb NO ₂)						
1st GPT point (400 ppb O ₃)	797.7	386.2	419.7	422.6	0.9930	100.7%
2nd GPT point (200 ppb O ₃)	797.7	590.9	215.0	216.7	0.9919	100.8%
3rd GPT point (100 ppb O ₃)	797.7	692.7	113.2	114.3	0.9900	101.0%
Average Correction Factor					0.9916	100.8%

Notes: Changed the inlet filter after as founds. No adjustments made.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 5, 2023	Previous Calibration:	December 1, 2022
Station Name:	Patricia McInnes	Station Number:	AMS06
Start Time (MST):	10:11	End Time (MST):	14:44
Analyzer make:	Thermo 42i	Analyzer serial #:	1172750022

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.2	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
807.6	809.7	0.9974		
404.3	408.3	0.9903		
201.6	207.1	0.9736		
			0.999957	
			1.000715	
			2.680164	

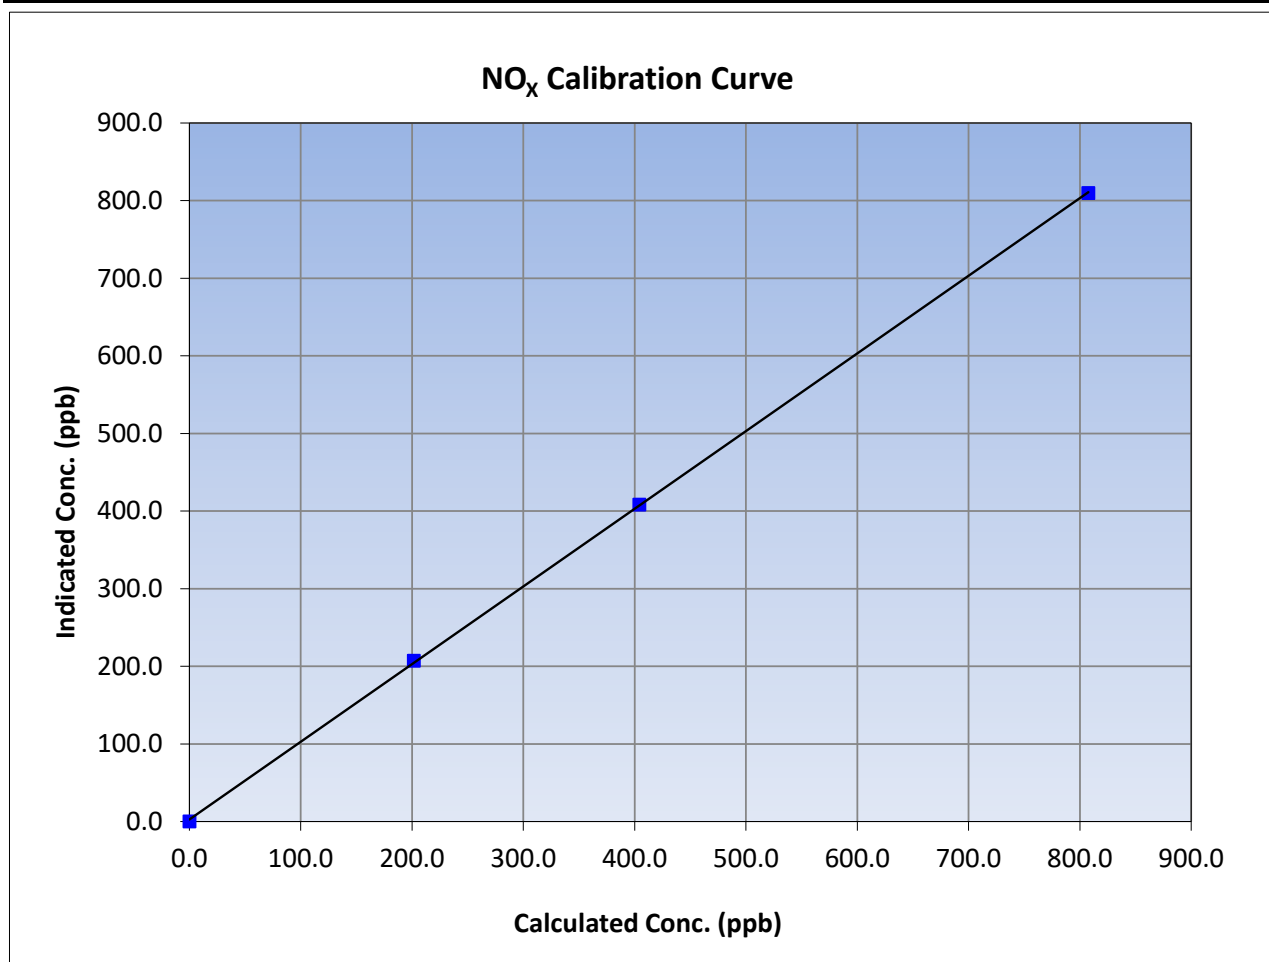



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 5, 2023	Previous Calibration:	December 1, 2022
Station Name:	Patricia McInnes	Station Number:	AMS06
Start Time (MST):	10:11	End Time (MST):	14:44
Analyzer make:	Thermo 42i	Analyzer serial #:	1172750022

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	≥0.995	
799.5	799.9	0.9994			
400.2	402.3	0.9949			
199.6	202.6	0.9852			
			Slope	0.999284	0.90 - 1.10
			Intercept	1.700041	+/-20

NO Calibration Curve

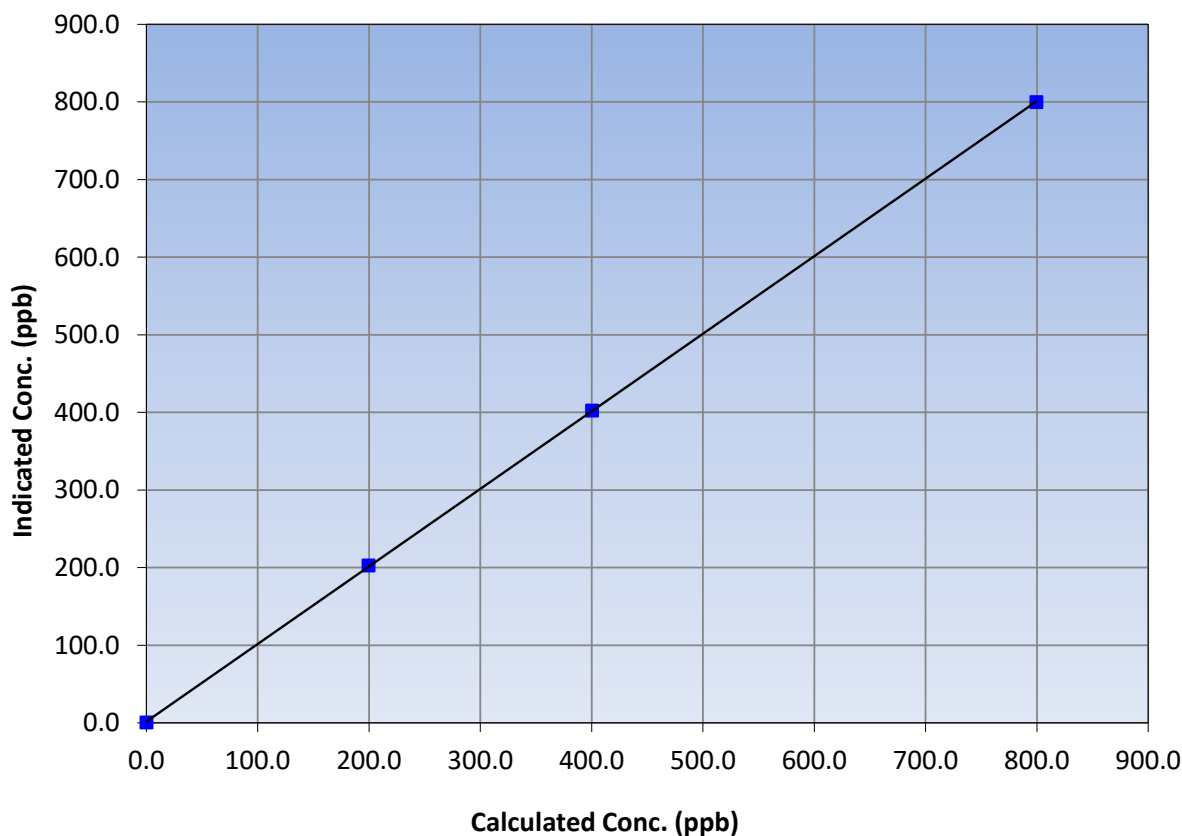



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 5, 2023	Previous Calibration:	December 1, 2022
Station Name:	Patricia McInnes	Station Number:	AMS06
Start Time (MST):	10:11	End Time (MST):	14:44
Analyzer make:	Thermo 42i	Analyzer serial #:	1172750022

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	-0.1	----	Correlation Coefficient	≥0.995	
419.7	422.6	0.9930			
215.0	216.7	0.9919			
113.2	114.3	0.9900			
			Slope	1.007019	0.90 - 1.10
			Intercept	0.124373	+/-20


NO₂ Calibration Curve

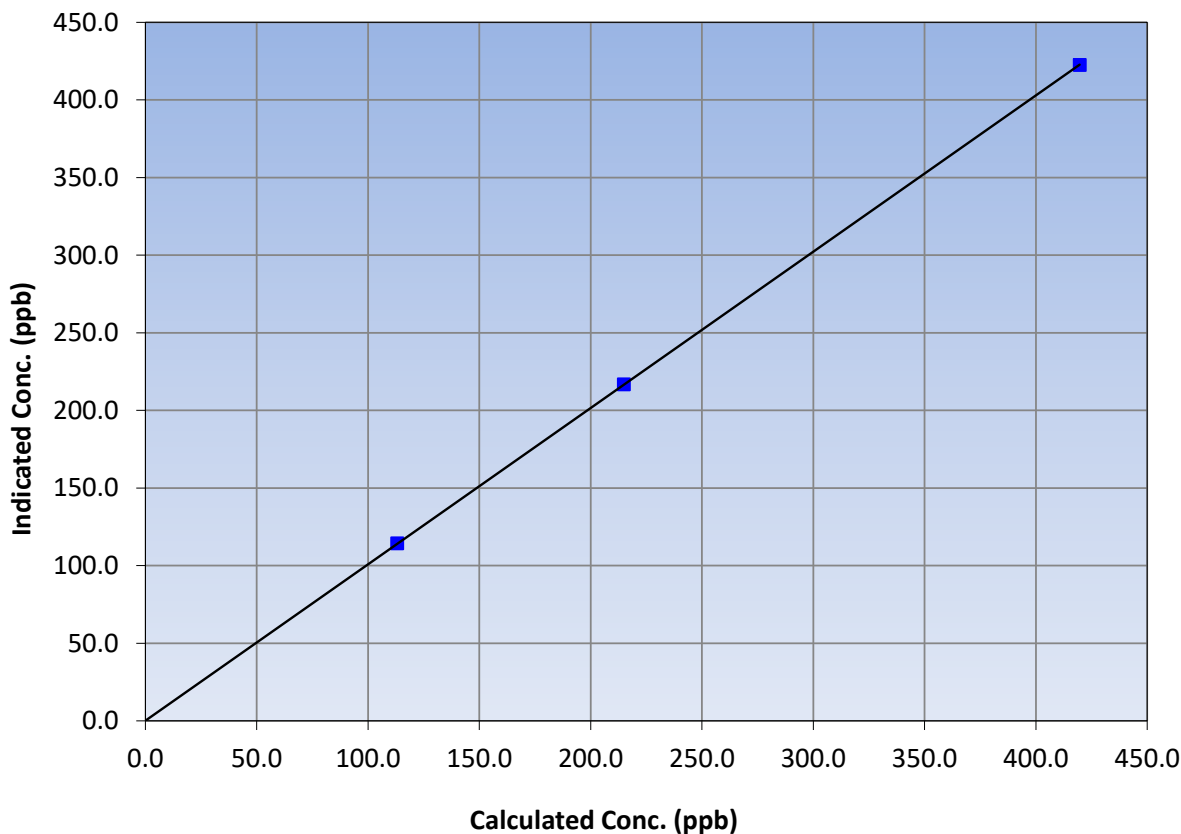

NO_x Calibration Plot

Date: January 5, 2023

Location: Patricia McInnes

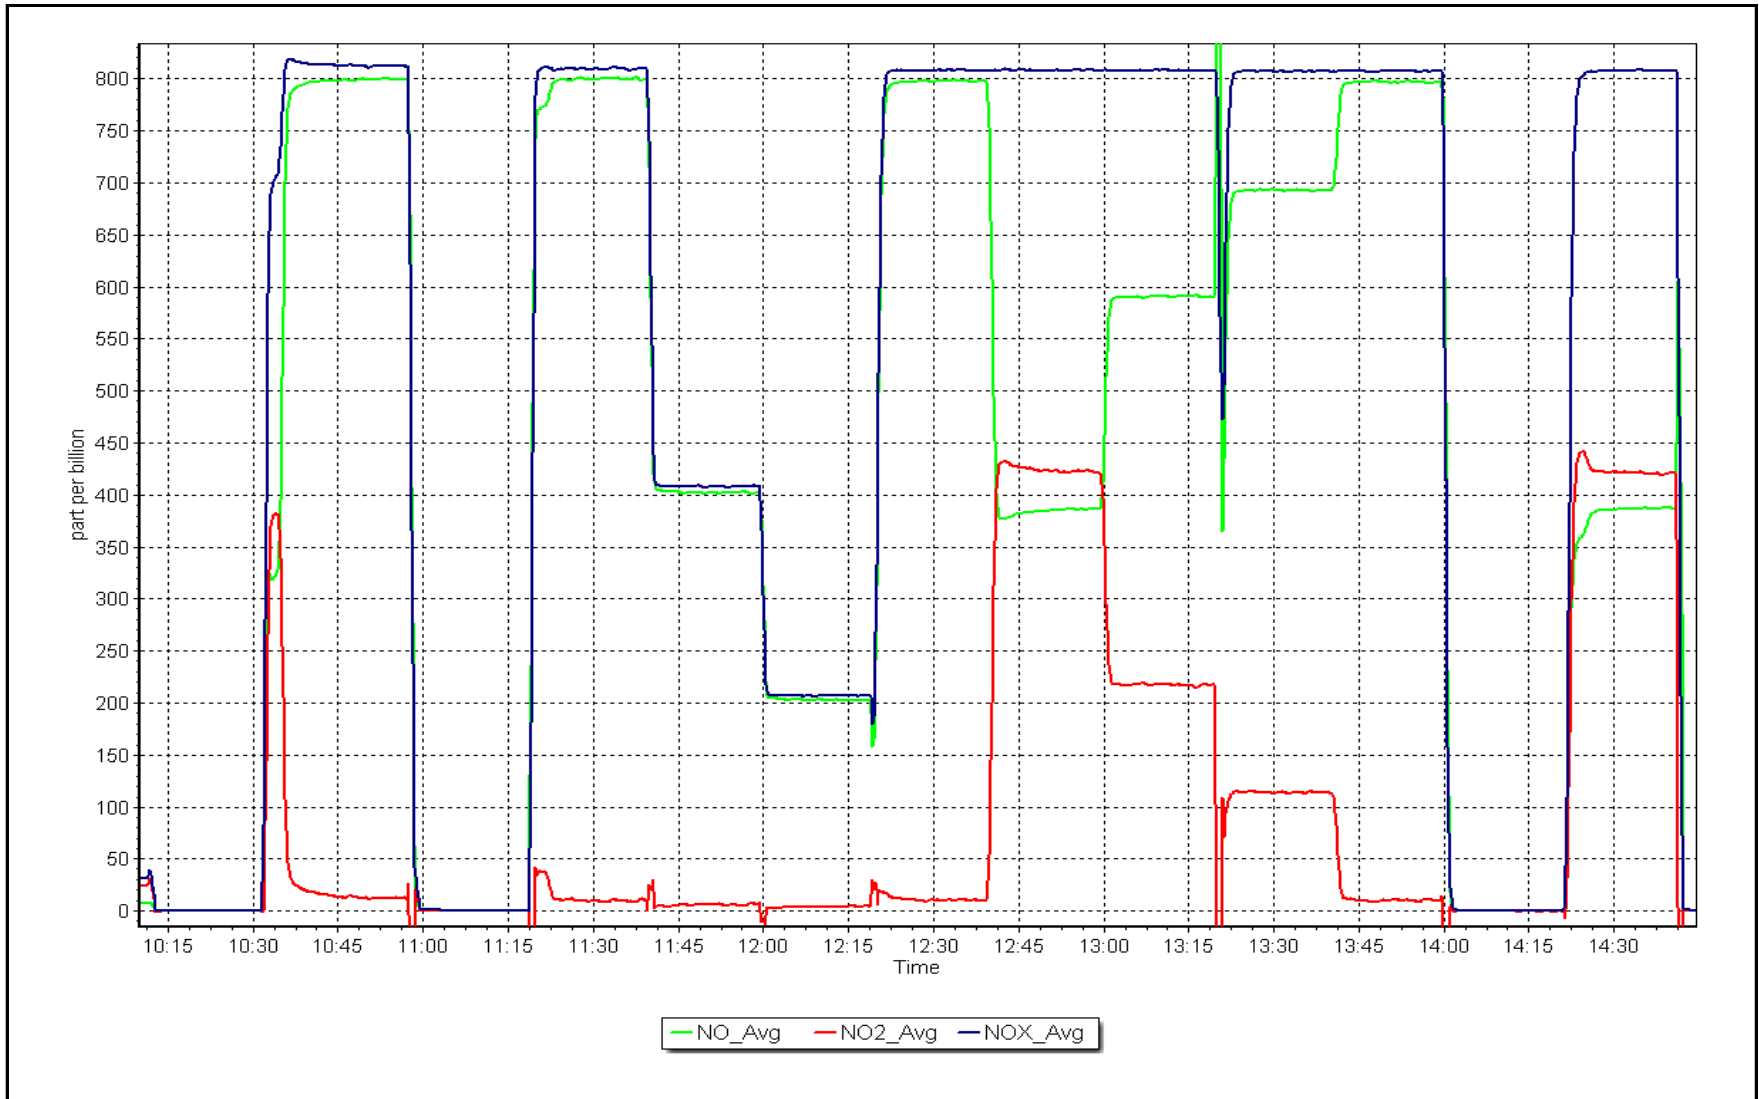



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Patricia McInnes Station number: AMS06
 Calibration Date: January 12, 2023 Last Cal Date: December 2, 2022
 Start time (MST): 9:55 End time (MST): 13:23
 Reason: Routine

Calibration Standards

O3 generation mode: Photometer
 Calibrator Make/Model: API T700 Serial Number: 3566
 ZAG Make/Model: API T701H Serial Number: 689

Analyzer Information

Analyzer make: Thermo 49i Analyzer serial #: 1300156234
 Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.007000	1.004914	Backgd or Offset:	-1.2	-1.2
Calibration intercept:	1.200000	1.440000	Coeff or Slope:	1.019	1.019

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	800.0	0.0	0.6	----
as found span	5000	1303.0	400.0	402.6	0.994
as found 2nd point					
as found 3rd point					
calibrator zero	5000	800.0	0.0	0.5	----
high point	5000	1303.0	400.0	402.9	0.993
second point	5000	966.5	200.0	203.0	0.985
third point	5000	794.3	100.0	102.8	0.973
as left zero	5000	800.0	0.0	0.4	----
as left span	5000	1303.0	400.0	404.2	0.990
Average Correction Factor					0.984

Baseline Corr As found:	402.0	Previous response	404.0	*% change	-0.5%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds. No adjustments made.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 2, 2022
Station Name:	Patricia McInnes	Station Number:	AMS06
Start Time (MST):	9:55	End Time (MST):	13:23
Analyzer make:	Thermo 49i	Analyzer serial #:	1300156234

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.5	----	Correlation Coefficient	0.999975	
400.0	402.9	0.9928			≥0.995
200.0	203.0	0.9852	Slope	1.004914	
100.0	102.8	0.9728			0.90 - 1.10
			Intercept	1.440000	+/- 5

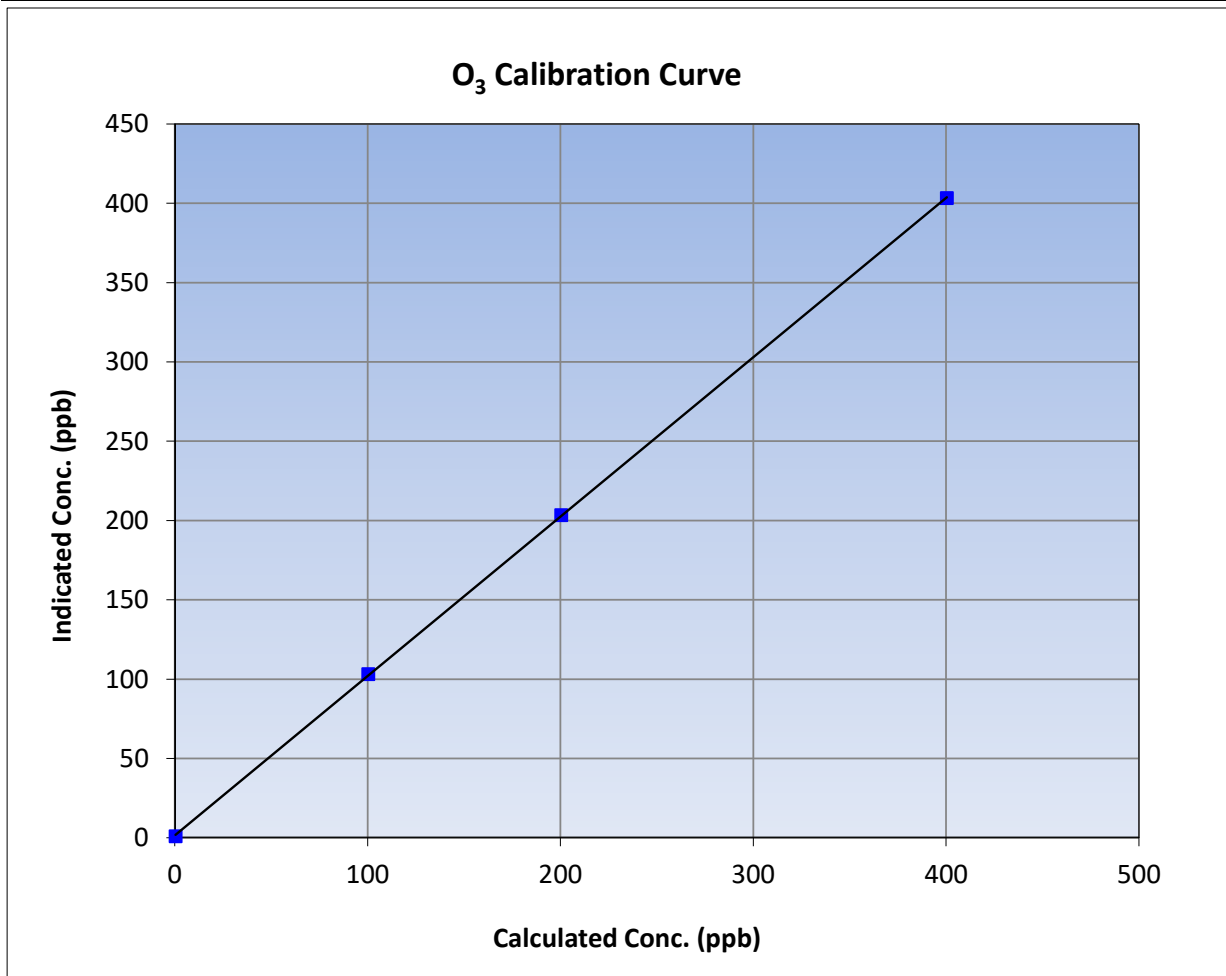

O₃ Calibration Plot

Date: January 12, 2023

Location: Patricia McInnes

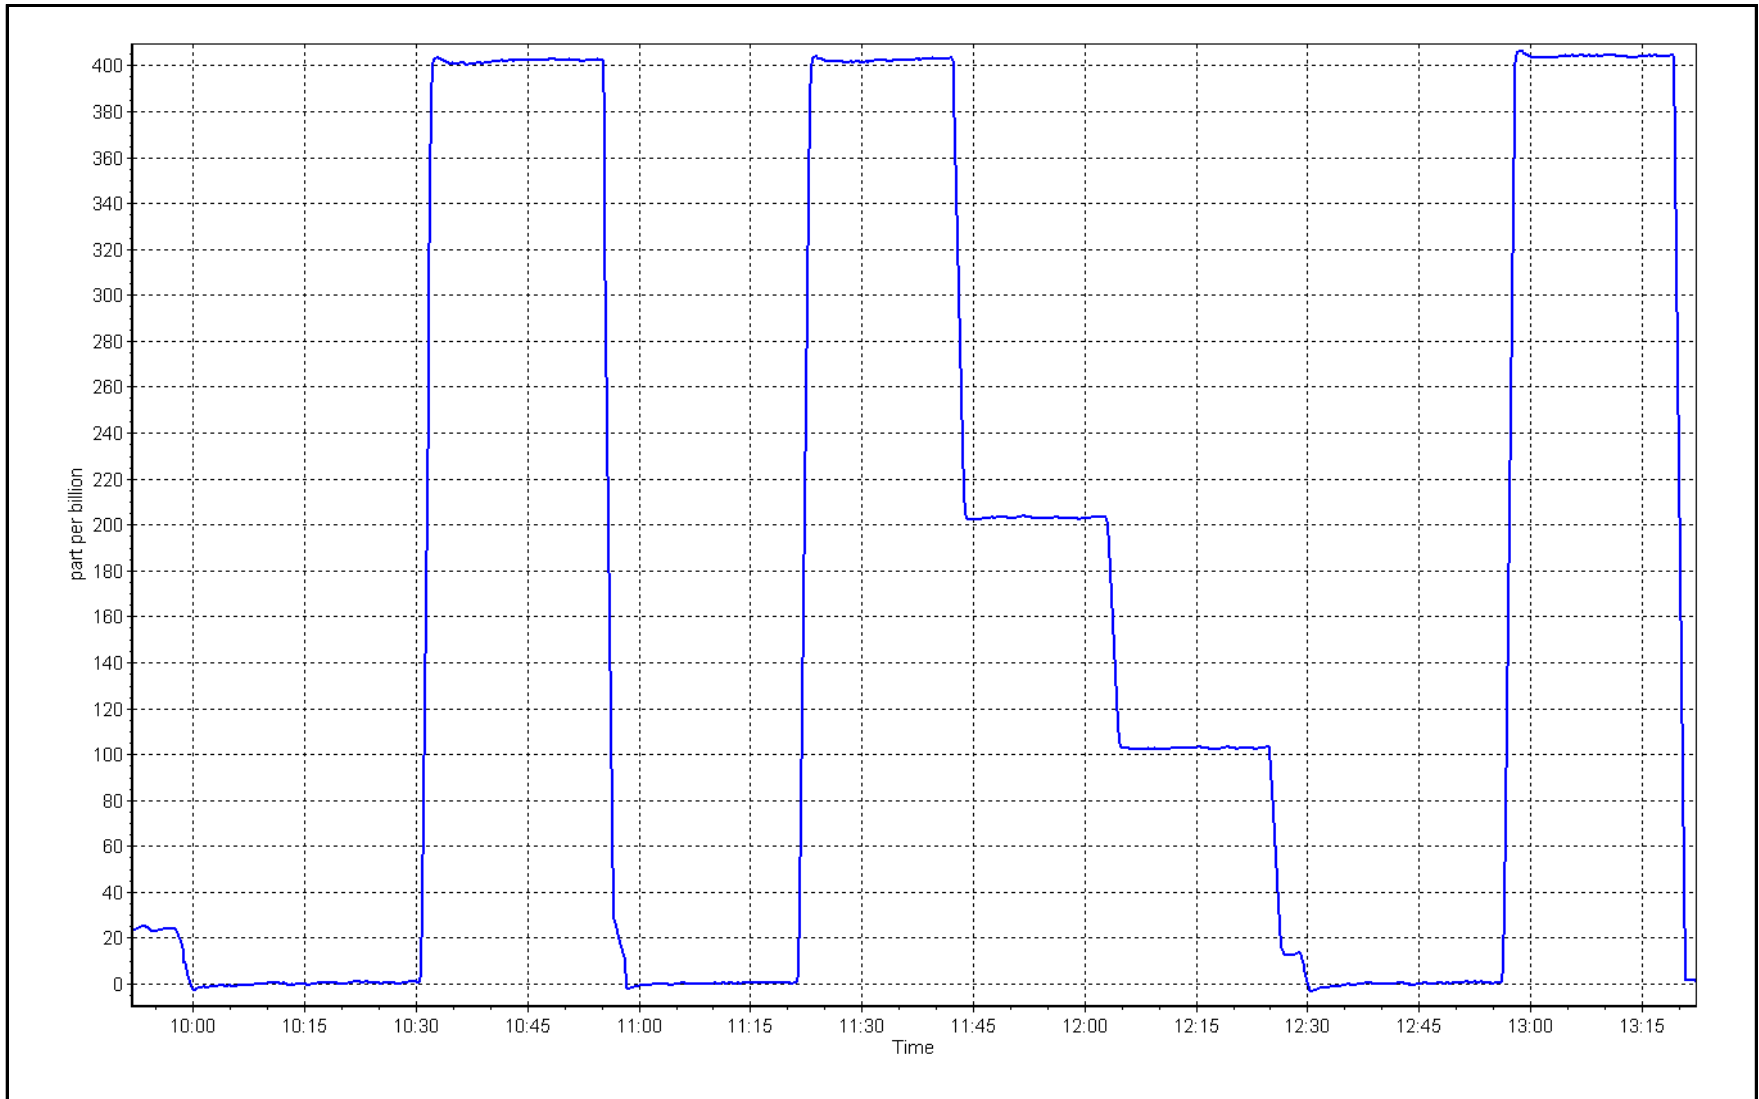



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Patricia McInnes Station number: AMS 06
Calibration Date: January 9, 2023 Last Cal Date: December 12, 2022
Start time (MST): 14:07 End time (MST): 15:05

Analyzer Make: API T640 S/N: 766
Particulate Fraction: PM2.5

Flow Meter Make/Model: Delta Cal S/N: 628
Temp/RH standard: Delta Cal S/N: 628

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-8.6	-7.3	-8.6	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	720.4	718	720.4	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	4.98	5.16	4.98	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 9, 2023 Last Cal Date: December 12, 2022
PM w/o HEPA: 18.5 PM w/ HEPA: 0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test	10.9	10.9	10.9	<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: January 9, 2023
Disposable Filter Changed: January 9, 2023

Annual Maintenance

Date Sample Tube Cleaned: August 28, 2020
Date RH/T Sensor Cleaned: August 28, 2020

Notes: PMT Peak test completed. Leak check passed. No adjustments made.

Calibration by: Max Farrell



Wood Buffalo Environmental Association

TN - NO_x - NH₃ Calibration Report

Version-11-2021

Station Information

Station Name:	Patricia McInnes	Station number:	AMS 06
NOX Cal Date:	January 11, 2023	Last Cal Date:	December 6, 2022
Start time (MST):	9:30	End time (MST):	13:41
NH3 Cal Date:	January 11, 2023	Last Cal Date:	December 6, 2022
Start time (MST):	13:41	End time (MST):	15:29
Reason:	Routine		

Calibration Standards

NOX Cal Gas Conc:	52.51	ppm	NO Gas Cylinder #:	T26D9MR
NO Cal Gas Conc:	51.98	ppm	NO Cal Gas Expiry:	August 18, 2023
Removed NOX Conc:	52.51	ppm	Removed Cylinder #:	N/A
Removed NO Conc:	51.98	ppm	Removed cyl Expiry:	N/A
NOX gas Diff:			NO gas Diff:	
NH3 Cal Gas Conc:	73.9	ppm	NH3 Gas Cylinder #:	CC430800
			NH3 Cal Gas Expiry:	January 7, 2023
Removed NH3 Conc:	73.9	ppm	Removed Cylinder #:	
NH3 gas Diff:			Removed cyl Expiry:	
Calibrator Model:	API T700		Serial Number:	3566
ZAG make/model:	API T701		Serial Number:	689

Analyzer Information

Analyzer model:	API T201	Analyzer serial #:	152
Converter model:	API T501	Converter serial #:	147
NH3 Range (ppb):	0 - 2000 ppb	Reaction cell Press:	5.70
NOX Range (ppb):	0 - 1000 ppb	Sample Flow:	531

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coefficient:	0.823	0.839	TN coefficient:	0.823	0.843
NOX coefficient:	0.823	0.840	NO bkgrnd:	-0.1	-0.1
NO2 coefficient:	1.000	1.000	NOX bkgrnd:	0.0	0.0
NH3 coefficient:	0.951	0.951	TN bkgrnd:	0.0	0.0

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	0.994035	0.996497
NO _x Cal Offset:	2.840711	1.220653
NO Cal Slope:	0.997954	1.002531
NO Cal Offset:	1.640234	-0.260924
NO ₂ Cal Slope:	0.996702	1.003819
NO ₂ Cal Offset:	-1.098676	1.157200
NH3 Cal Slope:	1.007009	0.998364
NH3 Cal Offset:	8.369635	7.107284
TN Cal Slope:	1.011540	1.003901
TN Cal Offset:	8.804361	5.611013



Wood Buffalo Environmental Association

TN - NOX - NH₃ Calibration Report

Version-11-2021

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated TN concentration (ppb) (Cc)	Calculated NOX concentration (ppb) (Cc)	Calculated NH3 concentration (ppb) (Cc)	Indicated TN concentration (ppb) (Ic)	Indicated NOX concentration (ppb) (Ic)	Indicated NH3 concentration (ppb) (Ic)	TN Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NH3 Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-1.1	-1.5	0.4	----	----
as found NO	4923	76.9	807.6	807.6	----	789.9	786.8	3.1	1.022	----
calibrator zero	5000	0.0	0.0	0.0	0.0	-0.2	-1.6	1.4	----	----
high NO point	4923	76.9	807.6	807.6	----	807.9	804.9	3.0	1.000	----
NO/O3 point	4923	76.9	807.6	807.6	----	811.2	802.5	8.7	0.996	----
as found NH3	3415	85.3	1801.0	----	1801.0	1810.5	----	1802.2	0.995	0.999
new NH3 cyl rp							----			
first NH3	3415	85.3	1801.0	----	1801.0	1810.5	----	1802.2	0.995	0.999
second NH3	3453	47.4	1000.8	----	1000.8	1012.8	----	1008.4	0.988	0.992
third NH3	3476	23.7	500.4	----	500.4	514.5	----	513.3	0.973	0.975
Average Correction Factor									0.9976	0.9889

Corrected As found TN = 791 ppb NO_x = 788.3 ppb NH3 = 1801.8 ppb

Previous Response TN = 825.7 ppb NO_x = 805.6 ppb NH3 = 1822.0 ppb

NH3 Previous Converter Efficiency = 95.1%

NH3 Current Converter Efficiency = 95.1%

*Percent Change TN = -4.4%

*Percent Change NO_x = -2.2%

*Percent Change NH3 = -1.1%

* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

NO_x - NO - NO₂ Calibration Report

Version-11-2021

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated TN concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated TN concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-1.5	-1.7	-1.1	----	----
as found span	4923	76.9	807.6	799.5	807.6	786.8	780.7	789.9	1.0264	1.0240
new NO cyl rp										
calibrator zero	5000	0.0	0.0	0.0	0.0	-1.6	-1.2	-0.2	----	----
high point	4923	76.9	807.6	799.5	807.6	804.9	800.3	807.9	1.0034	0.9989
second point	4962	38.5	404.3	400.2	404.3	404.6	402.8	406.5	0.9993	0.9937
third point	4981	19.2	201.6	199.6	201.6	205.6	199.9	206.3	0.9807	0.9985
Average Correction Factor									0.9945	0.9970

Baseline Corr As fnd TN = 791 ppb NO_x = 788.3 ppb NO = 782.4 ppb *Percent Change TN = -4.4%

Previous Response TN = 825.7 ppb NO_x = 805.6 ppb NO = 799.5 ppb *Percent Change NO_x = -2.2%

*Percent Change NO = -2.2%

* = > +/-5% change initiates investigation

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found zero	----	----	0.0	0.2	----	----
calibration zero	----	----	0.0	-0.4	----	----
1st GPT point (400 ppb O3)	792.5	385.7	415.0	416.7	0.9958	100.4%
2nd GPT point (200 ppb O3)	792.5	589.1	211.6	214.8	0.9849	101.5%
3rd GPT point (100 ppb O3)	792.5	689.6	111.1	113.9	0.9750	102.6%
Average Correction Factor					0.9852	101.5%

Notes:

Changed the inlet filter after as founds. Adjusted the NO_x span only.

Calibration Performed By:

Max Farrell



Wood Buffalo Environmental Association

TN Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 6, 2022
Station Name:	Patricia McInnes	Station Number:	AMS 06
Start Time (MST):	9:30	End Time (MST):	13:41
Analyzer make:	API T201	Analyzer serial #:	152

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>
0.0	-0.2	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
1801.0	1810.5	0.9948		
1000.8	1012.8	0.9882		
500.4	514.5	0.9726		

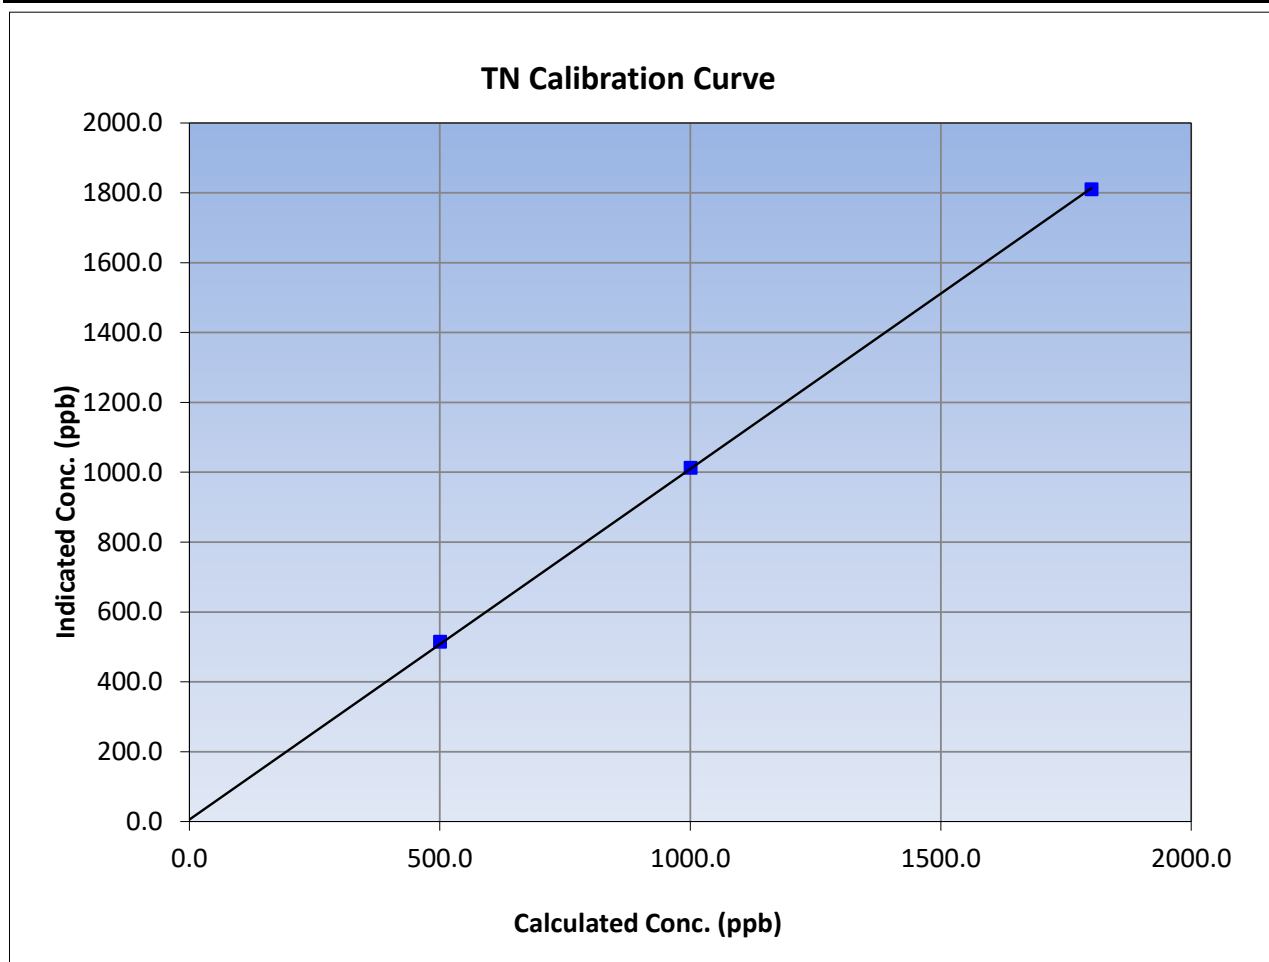



Wood Buffalo Environmental Association

NH₃ Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 6, 2022
Station Name:	Patricia McInnes	Station Number:	AMS 06
Start Time (MST):	9:30	End Time (MST):	13:41
Analyzer make:	API T201	Analyzer serial #:	152

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	1.4	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
1801.0	1802.2	0.9994		
1000.8	1008.4	0.9925		
500.4	513.3	0.9749		

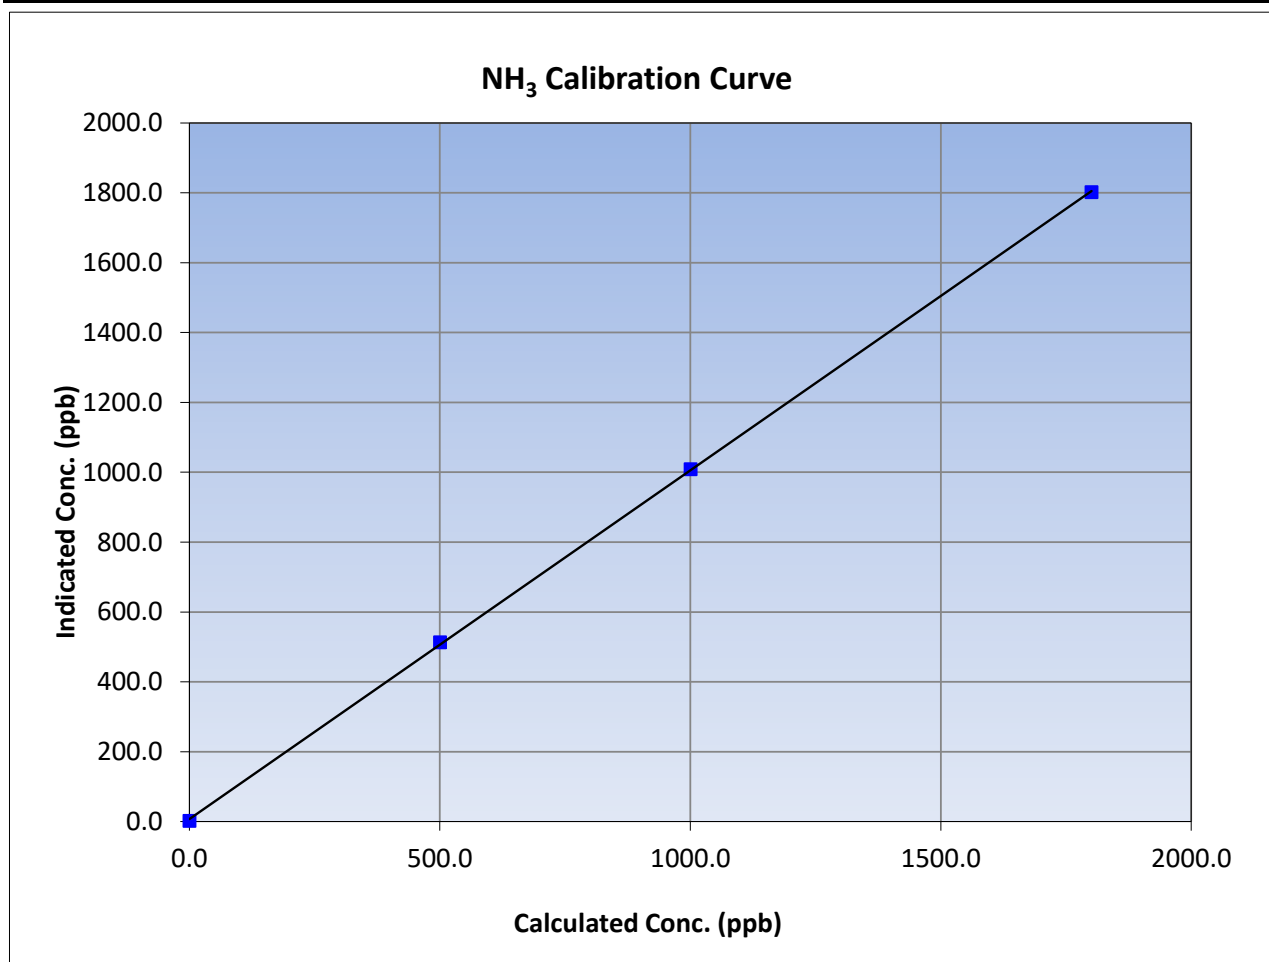



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 6, 2022
Station Name:	Patricia McInnes	Station Number:	AMS 06
Start Time (MST):	9:30	End Time (MST):	13:41
Analyzer make:	API T201	Analyzer serial #:	152

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	-1.6	----	Correlation Coefficient	≥0.995	
807.6	804.9	1.0034			
404.3	404.6	0.9993			
201.6	205.6	0.9807			
			Slope	0.996497	0.90 - 1.10
			Intercept	1.220653	+/-20

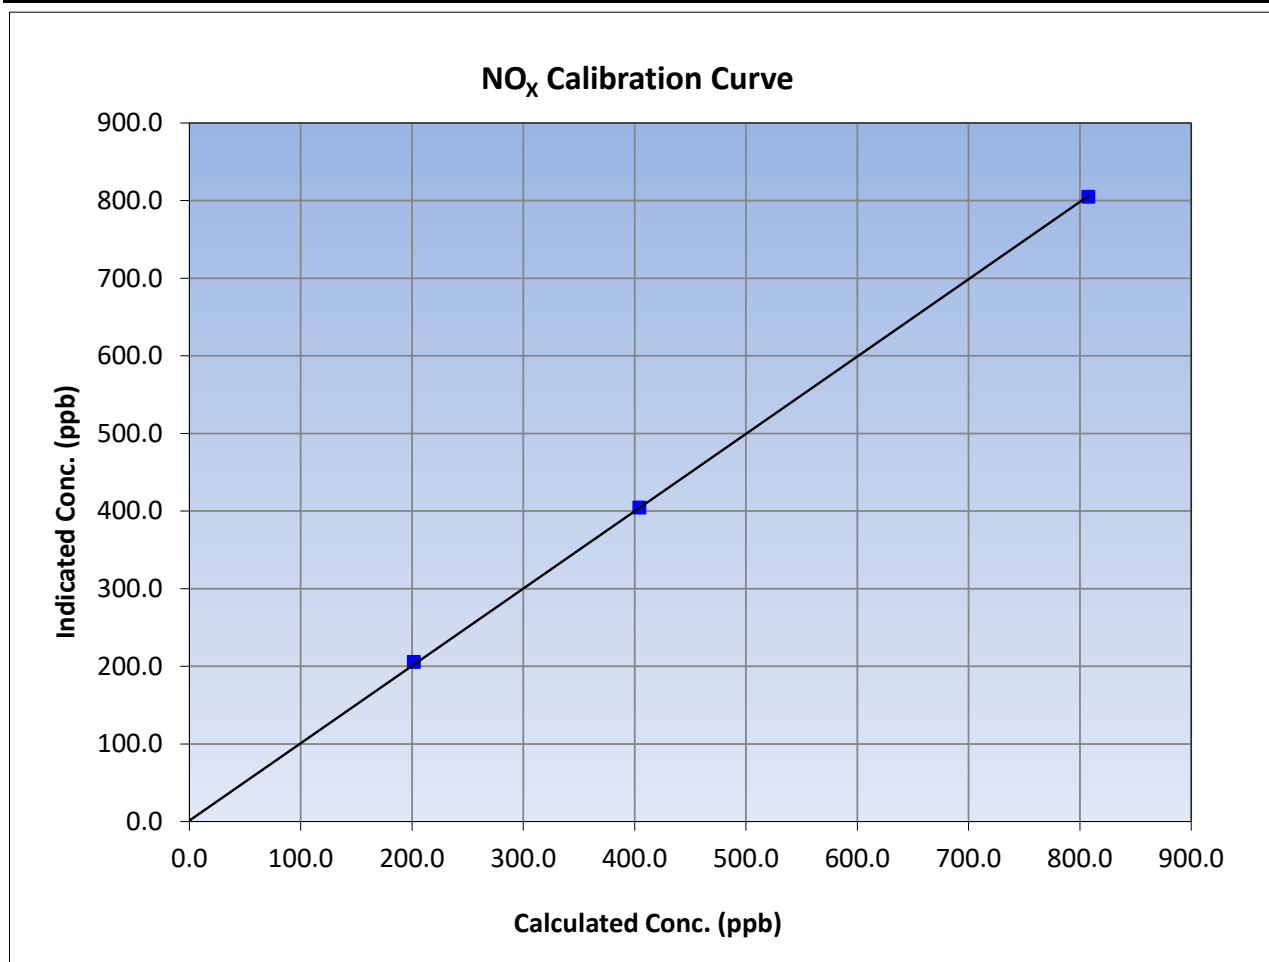



Wood Buffalo Environmental Association

NO Calibration Summary

Version-11-2021


Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 6, 2022
Station Name:	Patricia McInnes	Station Number:	AMS 06
Start Time (MST):	9:30	End Time (MST):	13:41
Analyzer make:	API T201	Analyzer serial #:	152

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	-1.2	----	Correlation Coefficient	≥0.995	
799.5	800.3	0.9989			
400.2	402.8	0.9937			
199.6	199.9	0.9985			
			Slope	1.002531	0.90 - 1.10
			Intercept	-0.260924	+/-20

NO Calibration Curve

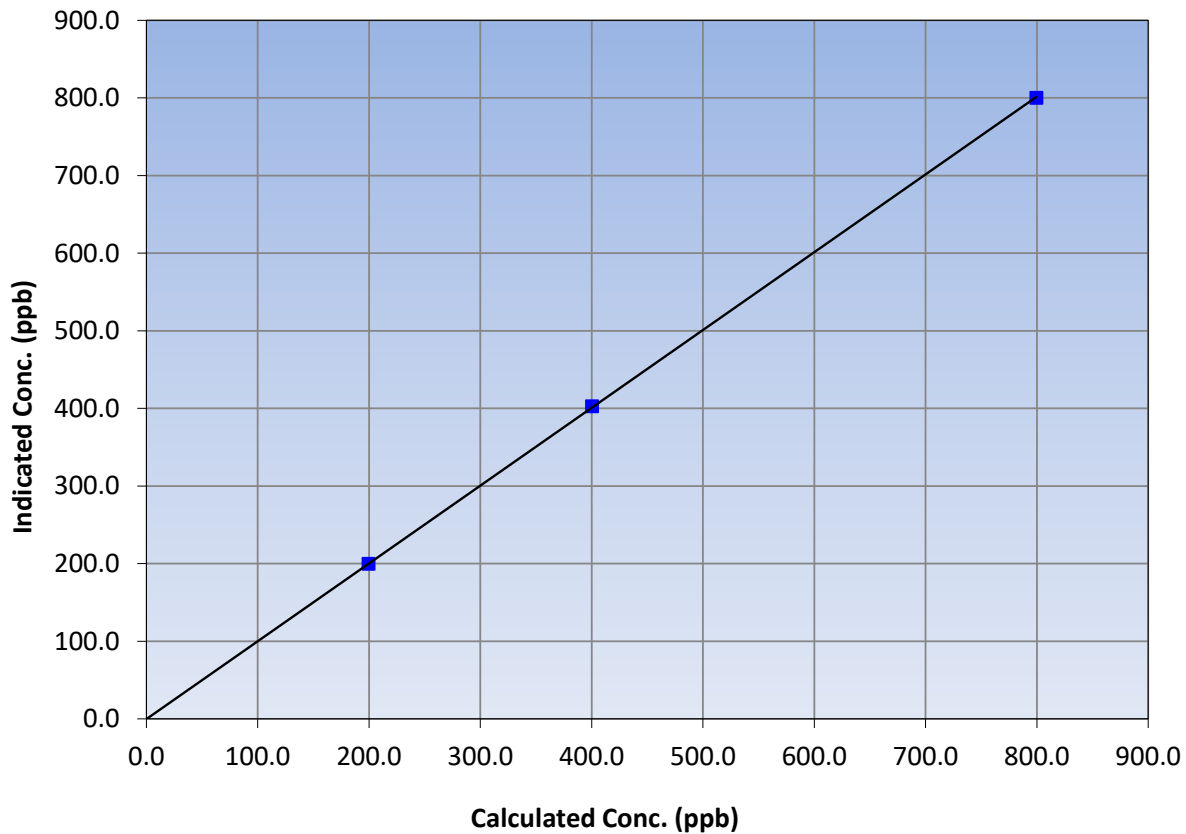



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 6, 2022
Station Name:	Patricia McInnes	Station Number:	AMS 06
Start Time (MST):	9:30	End Time (MST):	13:41
Analyzer make:	API T201	Analyzer serial #:	152

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	-0.4	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
415.0	416.7	0.9958		
211.6	214.8	0.9849		
111.1	113.9	0.9750		

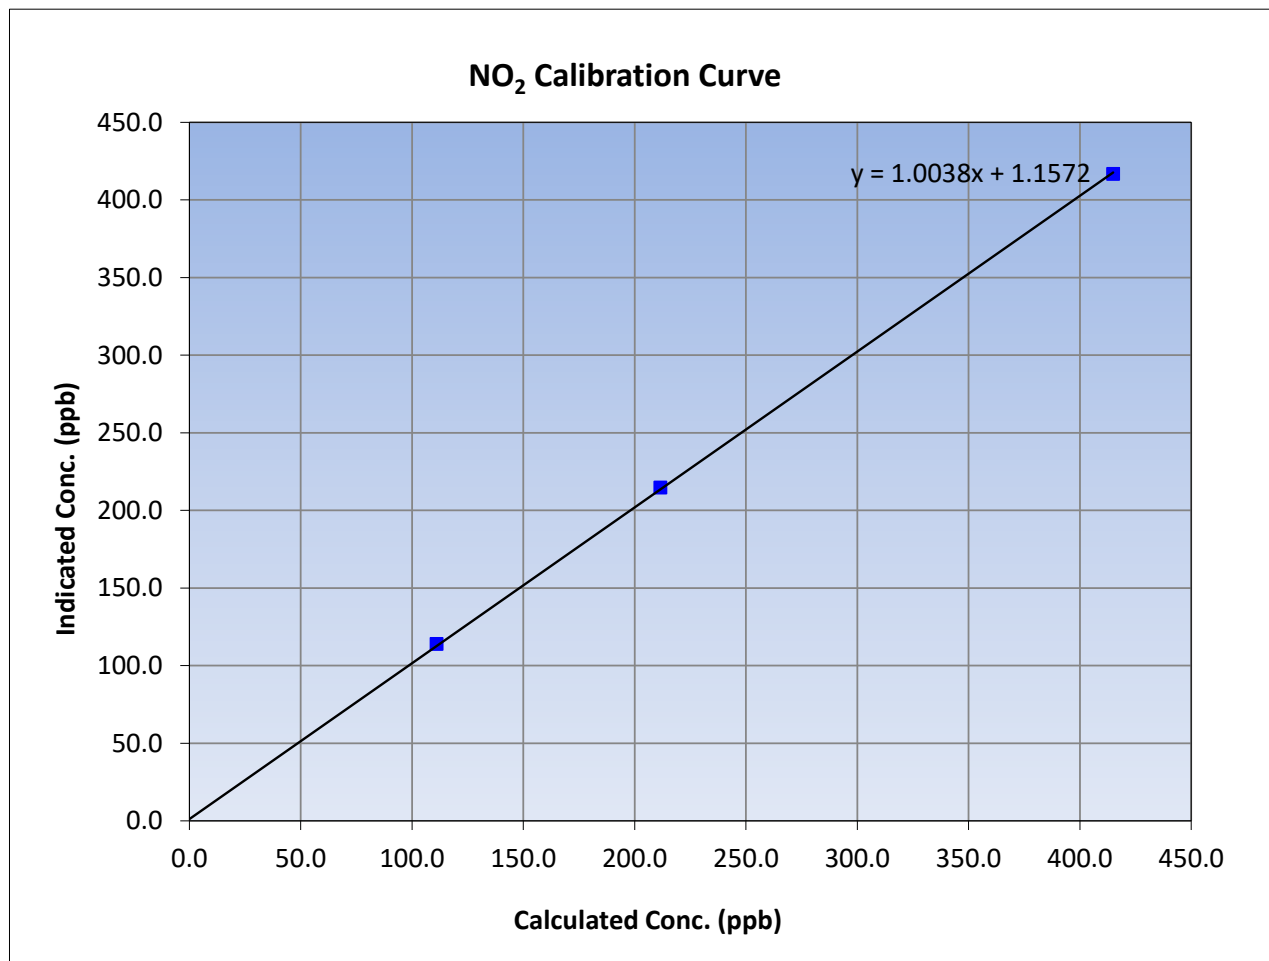

NO_x Calibration Plot

Date: January 11, 2023


Location: Patricia McInnes

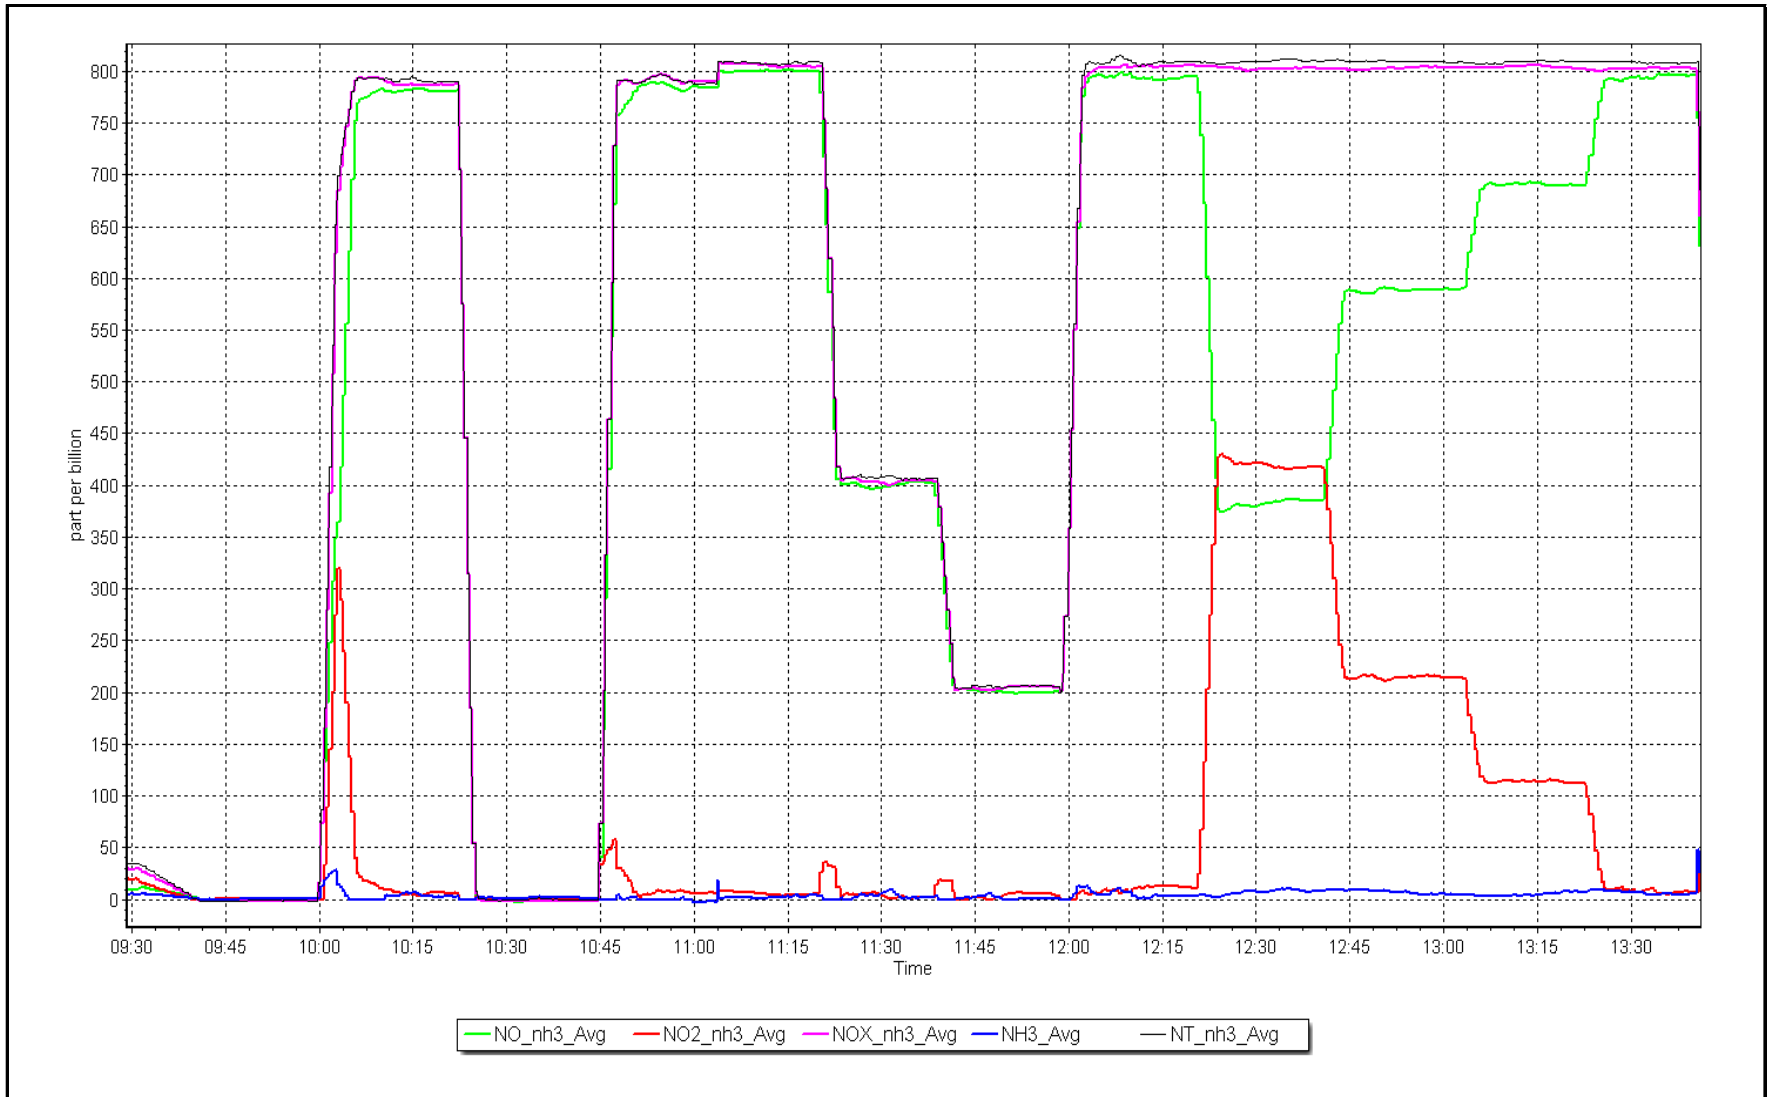

NH₃ Calibration Plot

Date: January 11, 2023

Location: Patricia McInnes

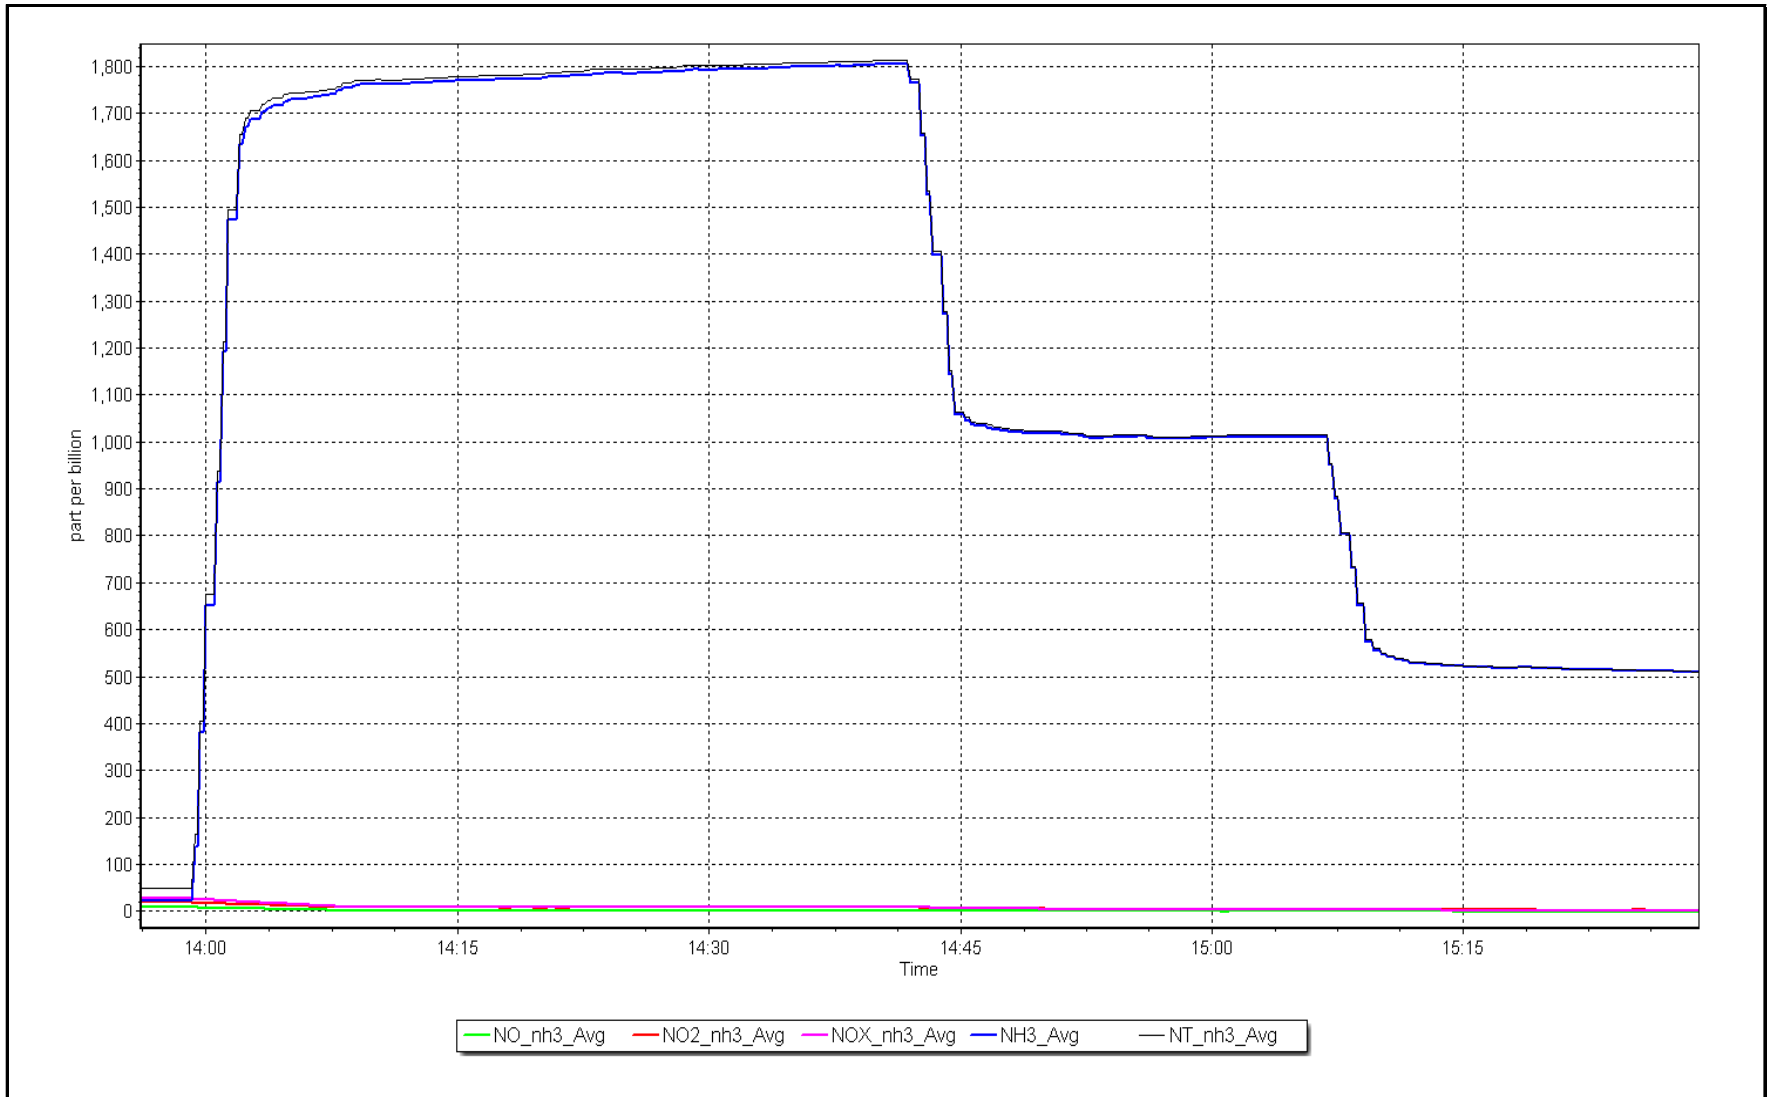



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS07 ATHABASCA VALLEY JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Athabasca Valley	Station number:	AMS07
Calibration Date:	January 16, 2023	Last Cal Date:	December 5, 2022
Start time (MST):	11:20	End time (MST):	14:05
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	50.52	ppm	Cal Gas Exp Date:	December 29, 2028
Cal Gas Cylinder #:	CC282115			
Removed Cal Gas Conc:	50.52	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	3805
ZAG Make/Model:	API 701H		Serial Number:	198

Analyzer Information

Analyzer make:	Thermo 43i-LTE	Analyzer serial #:	1507864683
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.996995	0.997038	Backgd or Offset:	2.68	2.71
Calibration intercept:	1.923766	1.683589	Coeff or Slope:	0.857	0.857

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	-0.1	----
as found span	4921	79.3	801.2	797.1	1.005
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.1	----
high point	4921	79.3	801.2	799.1	1.003
second point	4960	39.6	400.2	403.3	0.992
third point	4980	19.8	200.1	201.5	0.993
as left zero	5000	0.0	0.0	0.1	----
as left span	4921	79.2	800.2	799.9	1.000
Average Correction Factor					0.996

Baseline Corr As found:	797.20	Previous response	800.71	*% change	-0.4%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: No adjustments required.

Calibration Performed By: Denny Ray Estador



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 5, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	11:20	End Time (MST):	14:05
Analyzer make:	Thermo 43i-LTE	Analyzer serial #:	1507864683

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.1	----	Correlation Coefficient	0.999967	≥0.995
801.2	799.1	1.0026			
400.2	403.3	0.9922	Slope	0.997038	0.90 - 1.10
200.1	201.5	0.9929			
			Intercept	1.683589	+/-30

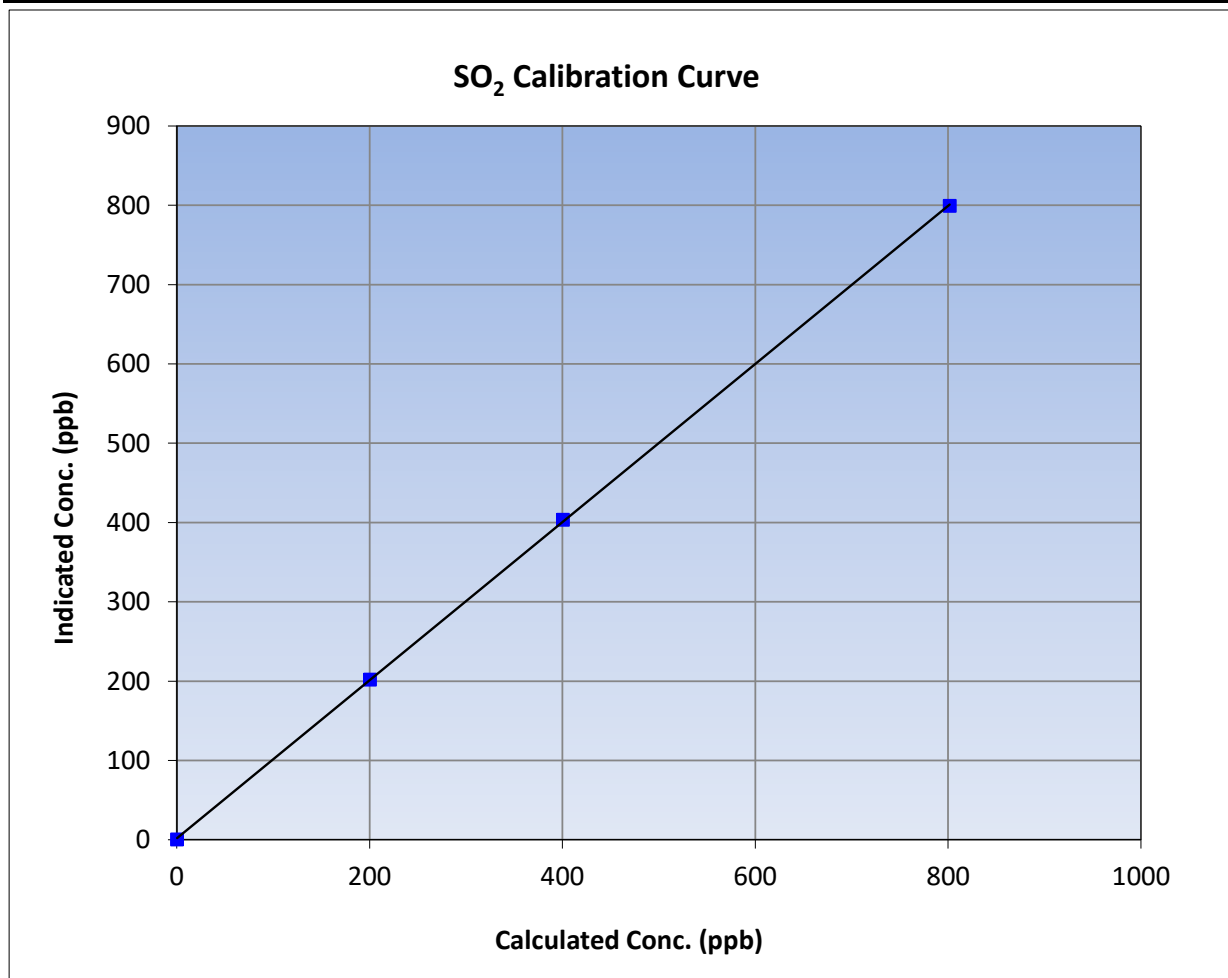

SO2 Calibration Plot

Date: January 16, 2023

Location: Athabasca Valley

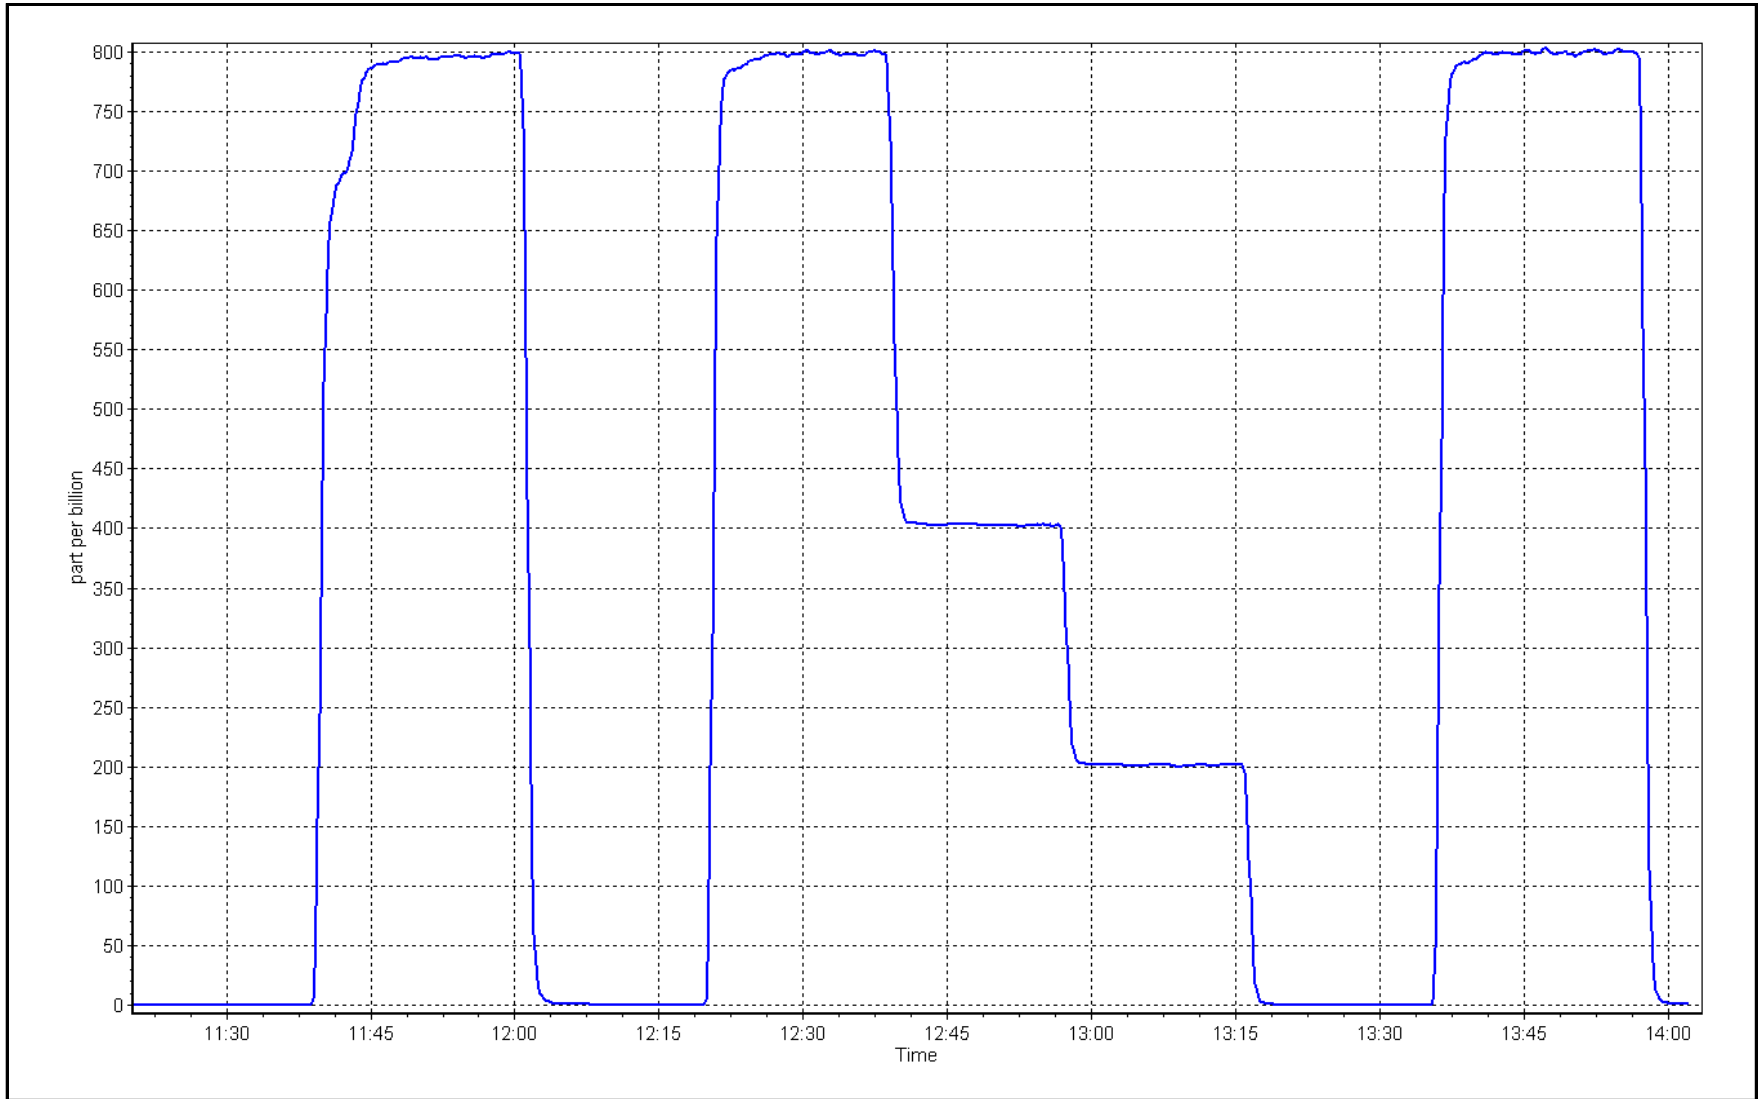



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name: Athabasca Valley Station number: AMS07
 Calibration Date: January 17, 2023 Last Cal Date: December 13, 2022
 Start time (MST): 7:00 End time (MST): 10:57
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 4.94 ppm Cal Gas Exp Date: February 9, 2024
 Cal Gas Cylinder #: EY0002277
 Removed Cal Gas Conc: 4.94 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 3805
 ZAG Make/Model: API T701H Serial Number: 198

Analyzer Information

Analyzer make: Thermo 43i LTE Analyzer serial #: 1180540018
 Converter make: CDN-101 Converter serial #: 551
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.993768	0.987815	Backgd or Offset:	2.18
Calibration intercept:	-0.078405	0.181600	Coeff or Slope:	0.834

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	-0.1	----
as found span	4918	81.6	80.6	80.1	1.005
as found 2nd point	4959	40.8	40.3	40.1	1.003
as found 3rd point	4980	20.4	20.2	19.7	1.018
new cylinder response					

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.0	----
high point	4918	81.6	80.6	79.7	1.012
second point	4959	40.8	40.3	40.2	1.003
third point	4980	20.4	20.2	20.2	0.998
as left zero	5000	0.0	0.0	0.7	----
as left span	4918	81.6	80.6	78.3	1.030
SO2 Scrubber Check	4921	79.2	800.2	0.3	----
Date of last scrubber change:	25-Feb-22			Ave Corr Factor	1.004
Date of last converter efficiency test:	April 22, 2022			98.5% efficiency	

Baseline Corr As found: 80.2 Prev response: 80.05 *% change: 0.2%
 Baseline Corr 2nd AF pt: 40.2 AF Slope: 0.995894 AF Intercept: -0.178398
 Baseline Corr 3rd AF pt: 19.8 AF Correlation: 0.999983

* = > +/-5% change initiates investigation

Notes: Sox scrubber checked after the calibrator zero. No maintenance or adjustments done.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 13, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	7:00	End Time (MST):	10:57
Analyzer make:	CDN-101	Analyzer serial #:	551

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	0.999971	
80.6	79.7	1.0116			≥0.995
40.3	40.2	1.0028	Slope	0.987815	
20.2	20.2	0.9977			0.90 - 1.10
			Intercept	0.181600	+/-3

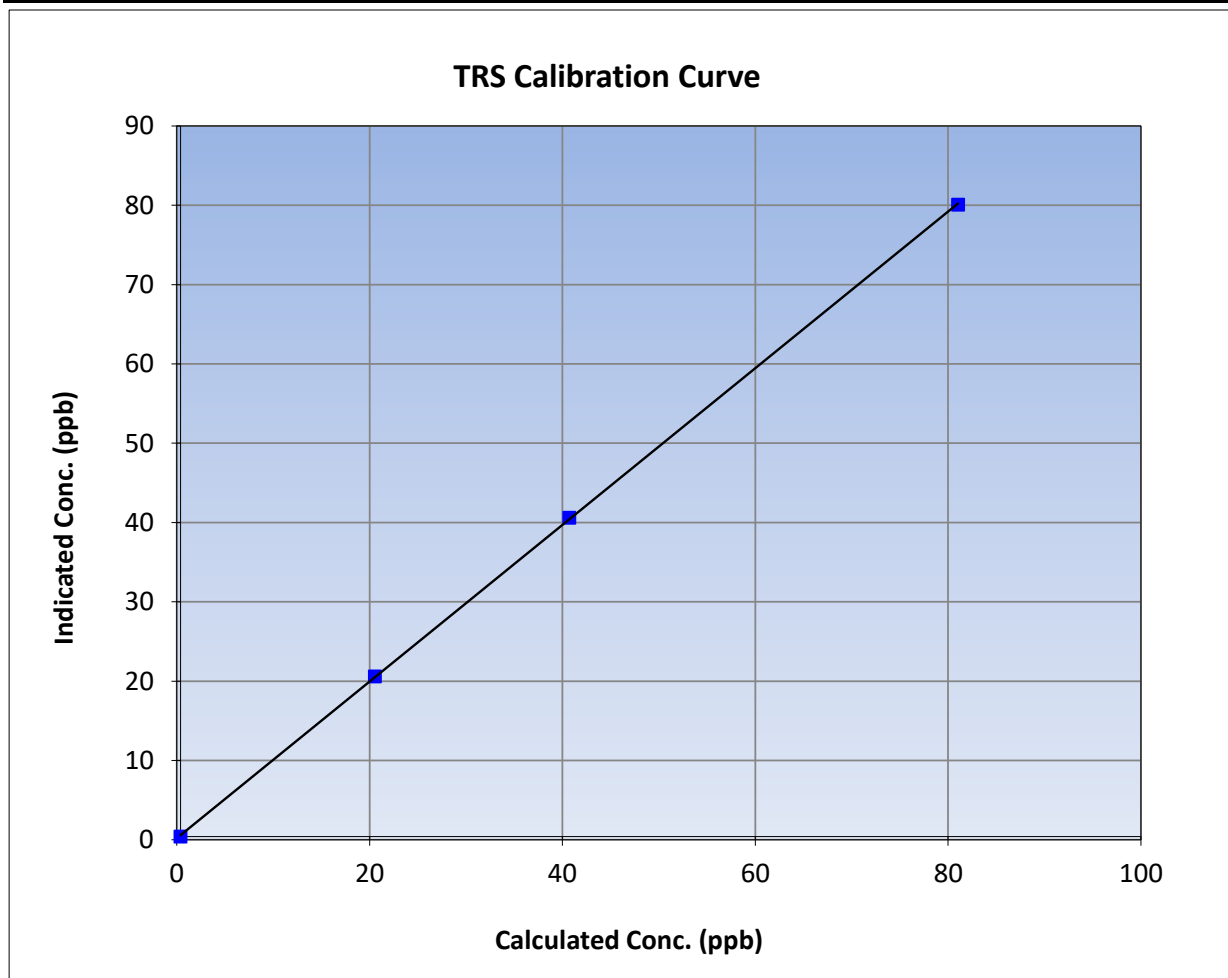

TRS Calibration Plot

Date: January 17, 2023

Location: Athabasca Valley

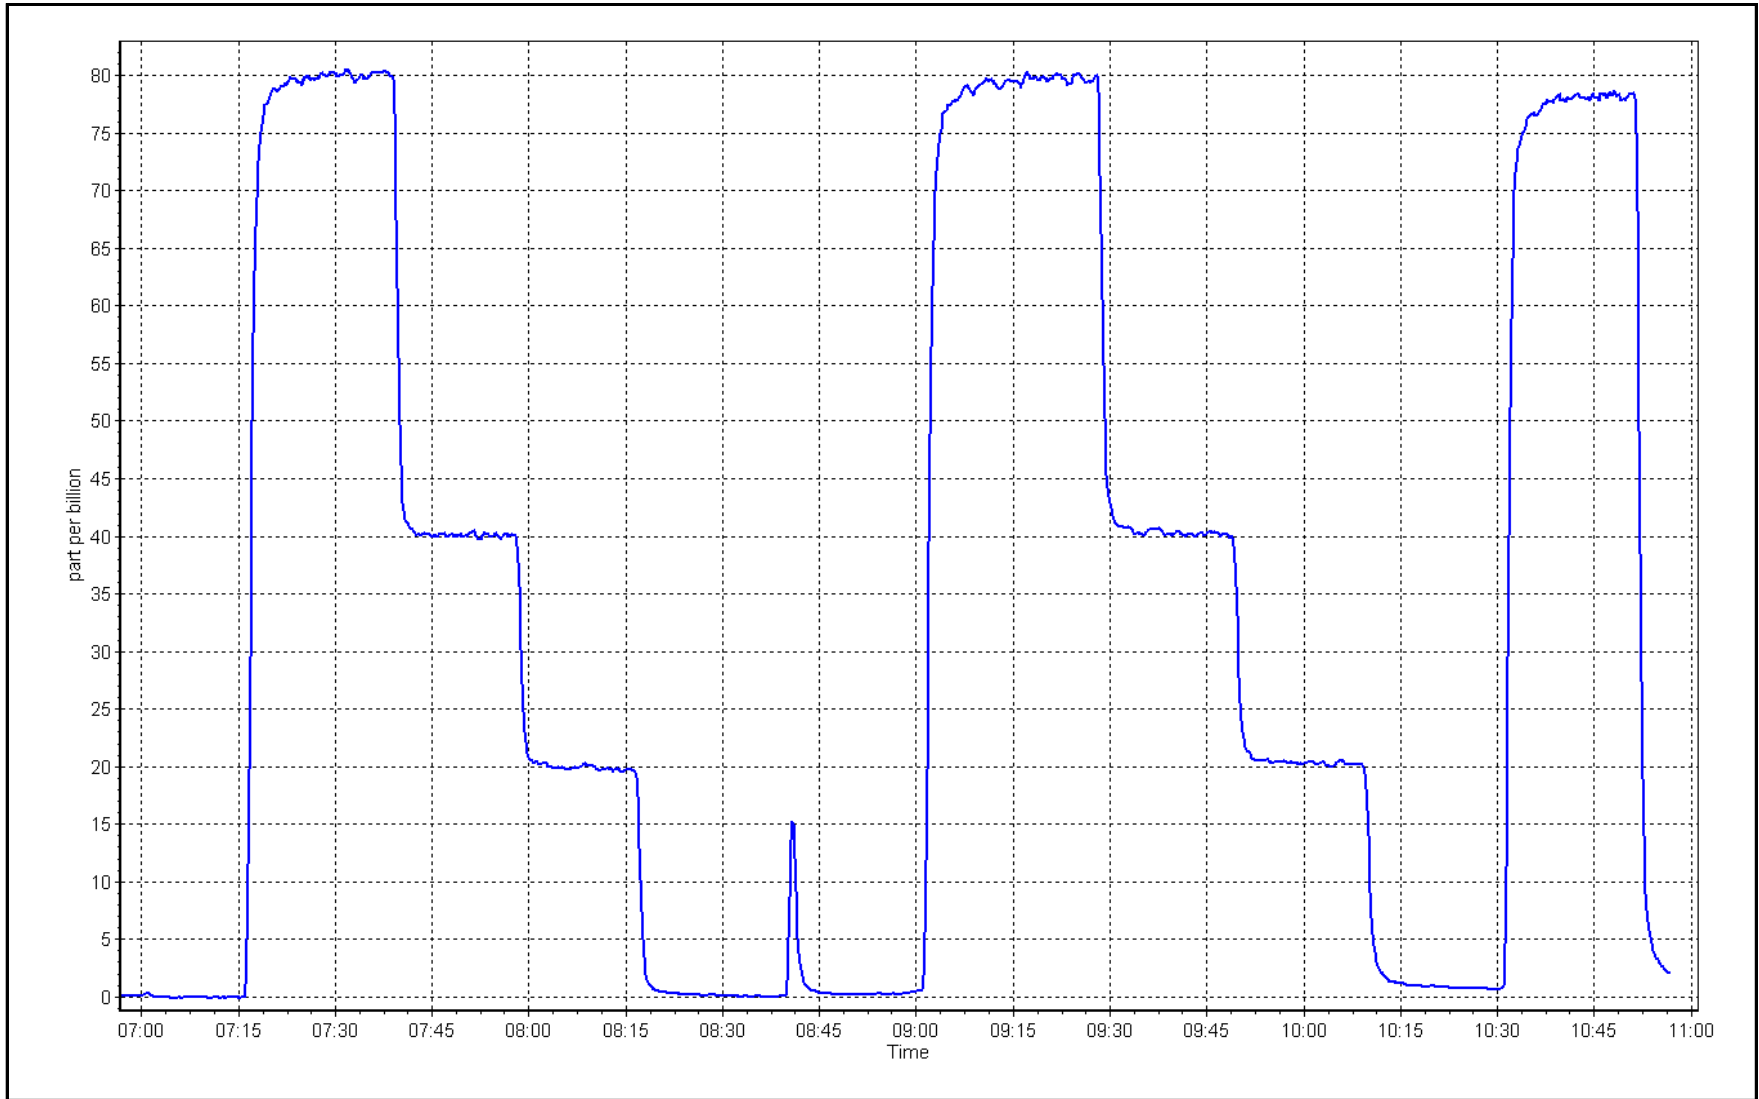



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Athabasca Valley	Station number:	AMS07
Calibration Date:	January 16, 2023	Last Cal Date:	December 5, 2022
Start time (MST):	11:20	End time (MST):	14:05
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC282115	Cal Gas Expiry Date:	December 29, 2028
CH ₄ Cal Gas Conc.	501.2 ppm	CH ₄ Equiv Conc.	1075.1 ppm
C ₃ H ₈ Cal Gas Conc.	208.7 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	501.2 ppm	CH ₄ Equiv Conc.	1075.1 ppm
Removed C ₃ H ₈ Conc.	208.7 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	3805
ZAG make/model:	API 701H	Serial Number:	198

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1317958219
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	0.000270	0.000270	NMHC SP Ratio: 4.42E-05	4.42E-05
CH ₄ Retention time:	13.4	13.4	NMHC Peak Area: 205840	205840

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4921	79.3	17.05	16.96	1.005
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4921	79.3	17.05	16.97	1.005
second point	4960	39.6	8.52	8.48	1.004
third point	4980	19.8	4.26	4.26	1.000
as left zero	5000	0.0	0.00	0.00	----
as left span	4921	79.2	17.03	16.97	1.003

Average Correction Factor				1.003
Baseline Corr AF:	16.96	Prev response	17.04	*% change -0.5%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4921	79.3	9.10	9.02	1.009
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4921	79.3	9.10	9.04	1.007
second point	4960	39.6	4.55	4.52	1.007
third point	4980	19.8	2.27	2.27	1.000
as left zero	5000	0.0	0.00	0.00	----
as left span	4921	79.2	9.09	9.03	1.007
Average Correction Factor					1.005
Baseline Corr AF:	9.02	Prev response	9.10	*% change	-0.8%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4921	79.3	7.95	7.94	1.001
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4921	79.3	7.95	7.94	1.002
second point	4960	39.6	3.97	3.97	1.001
third point	4980	19.8	1.98	1.99	0.999
as left zero	5000	0.0	0.00	0.00	----
as left span	4921	79.2	7.94	7.95	0.999
Average Correction Factor					1.001
Baseline Corr AF:	7.94	Prev response	7.94	*% change	0.0%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	0.998506	0.994820
THC Cal Offset:	0.011691	0.009674
CH ₄ Cal Slope:	0.999047	0.998255
CH ₄ Cal Offset:	0.000012	0.002012
NMHC Cal Slope:	0.998021	0.992058
NMHC Cal Offset:	0.012480	0.007463

Notes: No adjustments required.

Calibration Performed By: Denny Ray Estador



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 5, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	11:20	End Time (MST):	14:05
Analyzer make:	Thermo 55i	Analyzer serial #:	1317958219

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999998	≥ 0.995			
17.05	16.97	1.0048						
8.52	8.48	1.0042				Slope	0.994820	0.90 - 1.10
4.26	4.26	0.9997						
			Intercept	0.009674	± 0.5			

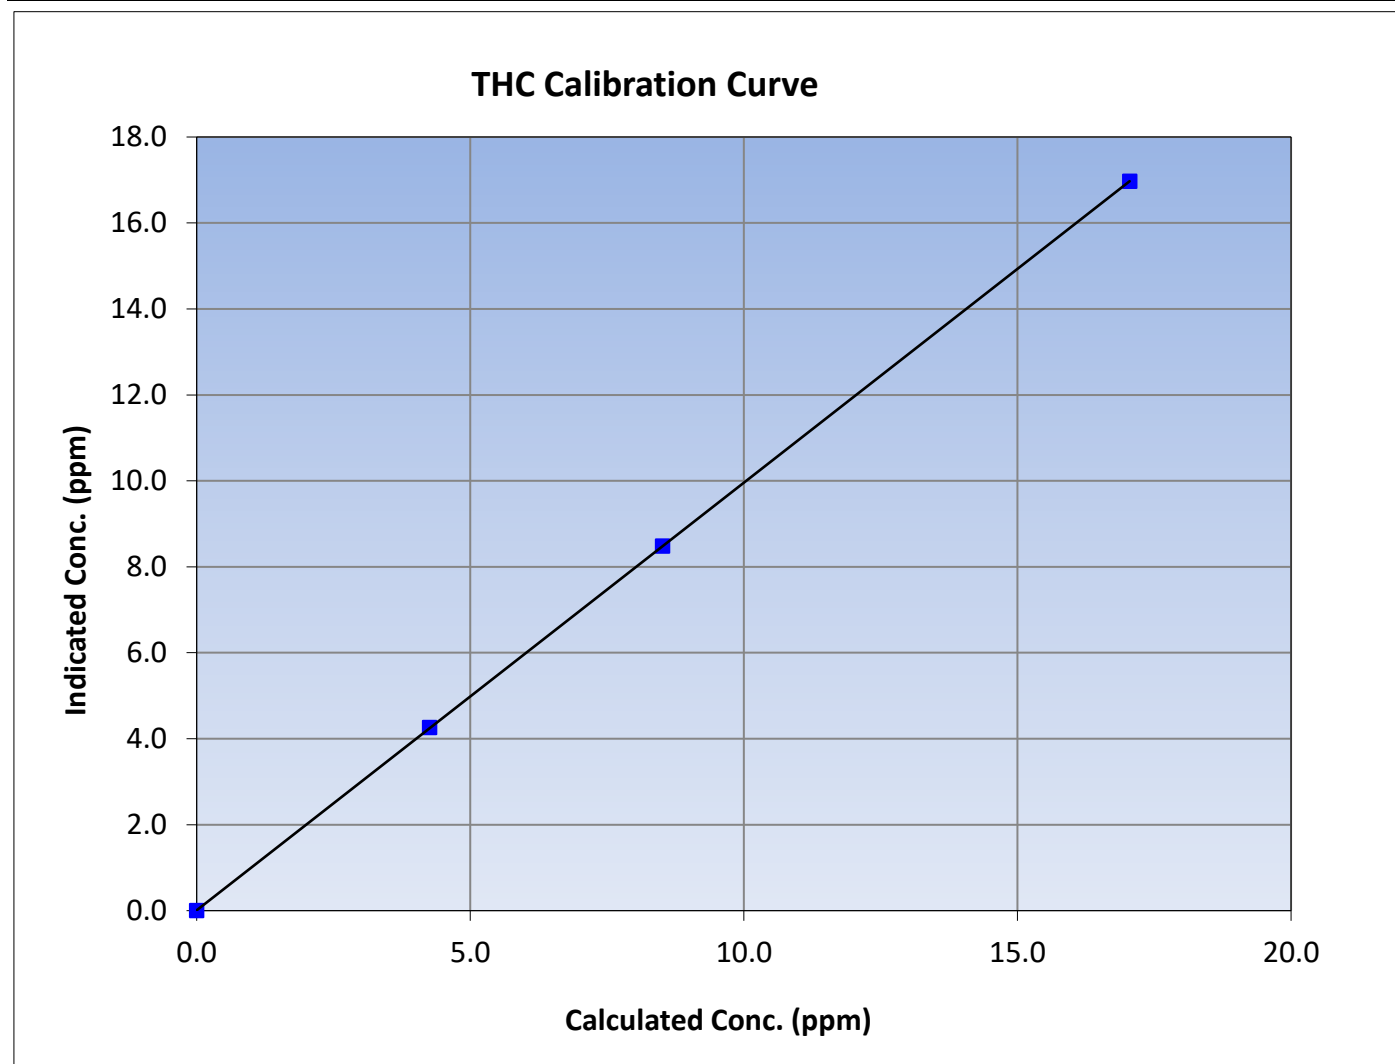



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 5, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	11:20	End Time (MST):	14:05
Analyzer make:	Thermo 55i	Analyzer serial #:	1317958219

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	1.000000	≥ 0.995			
7.95	7.94	1.0016						
3.97	3.97	1.0012				Slope	0.998255	0.90 - 1.10
1.98	1.99	0.9994						
			Intercept	0.002012	± 0.5			

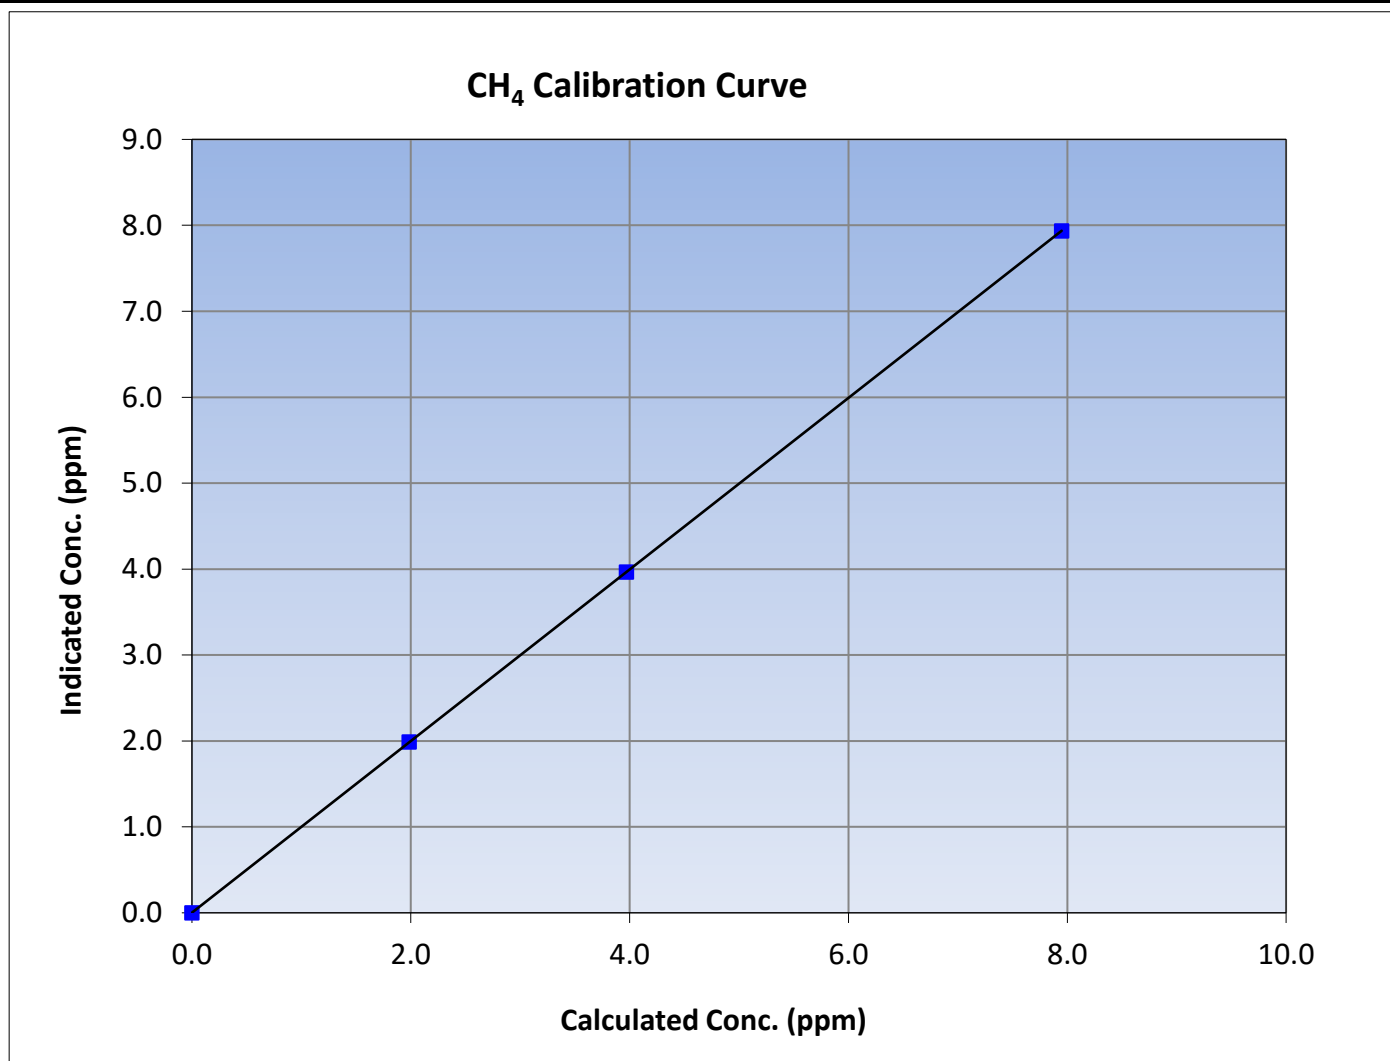



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 5, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	11:20	End Time (MST):	14:05
Analyzer make:	Thermo 55i	Analyzer serial #:	1317958219

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999996	≥ 0.995			
9.10	9.04	1.0074						
4.55	4.52	1.0066				Slope	0.992058	0.90 - 1.10
2.27	2.27	0.9999						
			Intercept	0.007463	± 0.5			

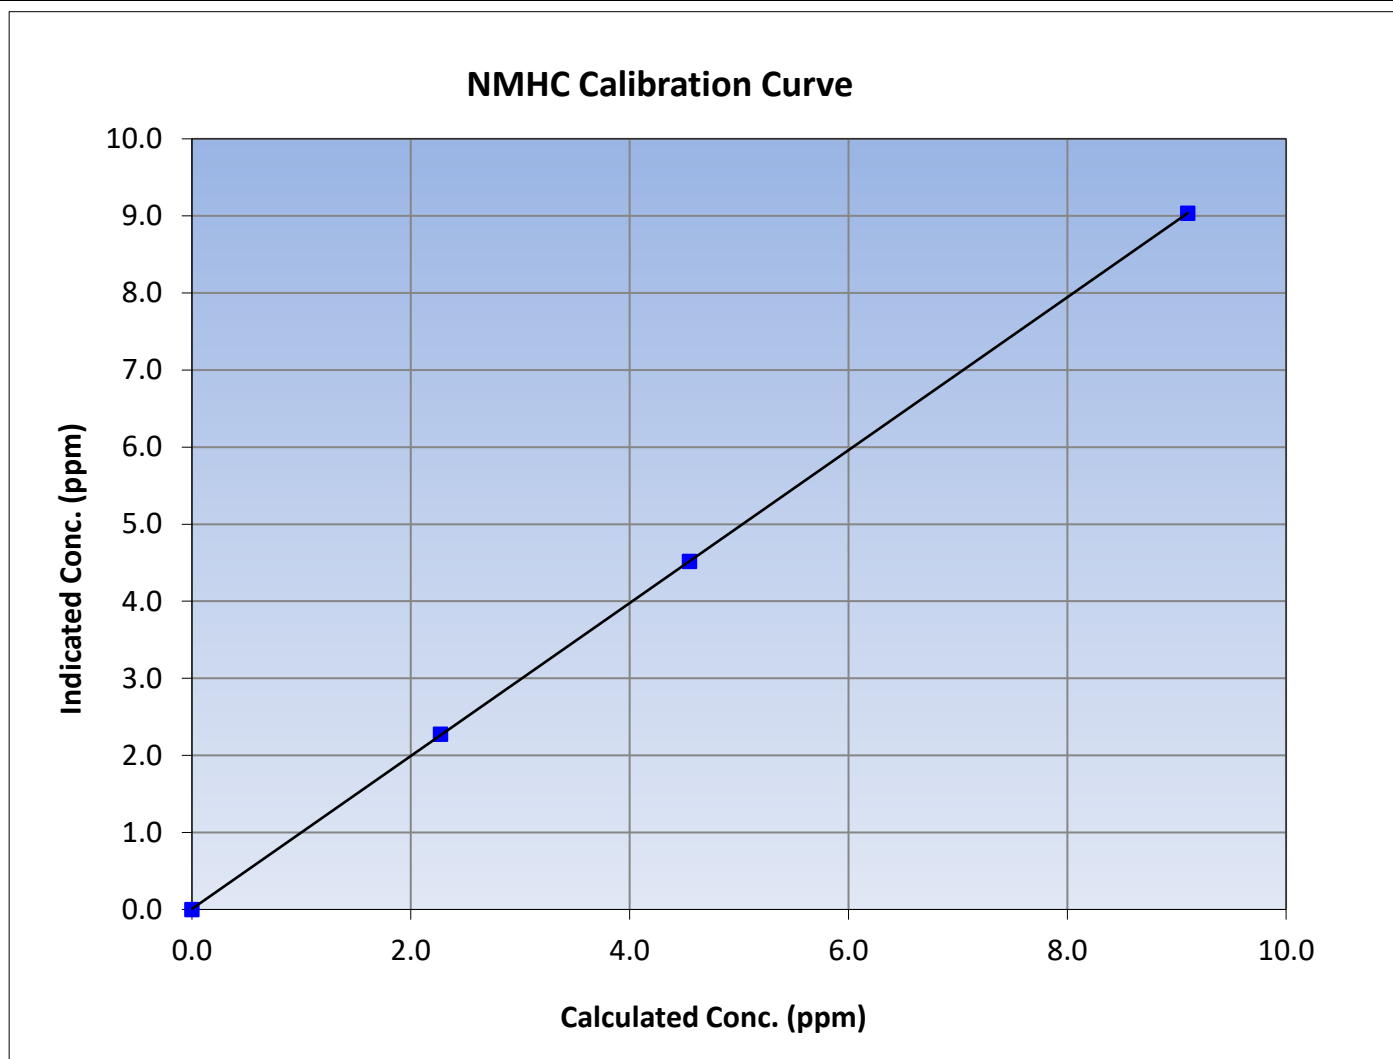

NMHC Calibration Plot

Date: January 16, 2023

Location: Athabasca Valley

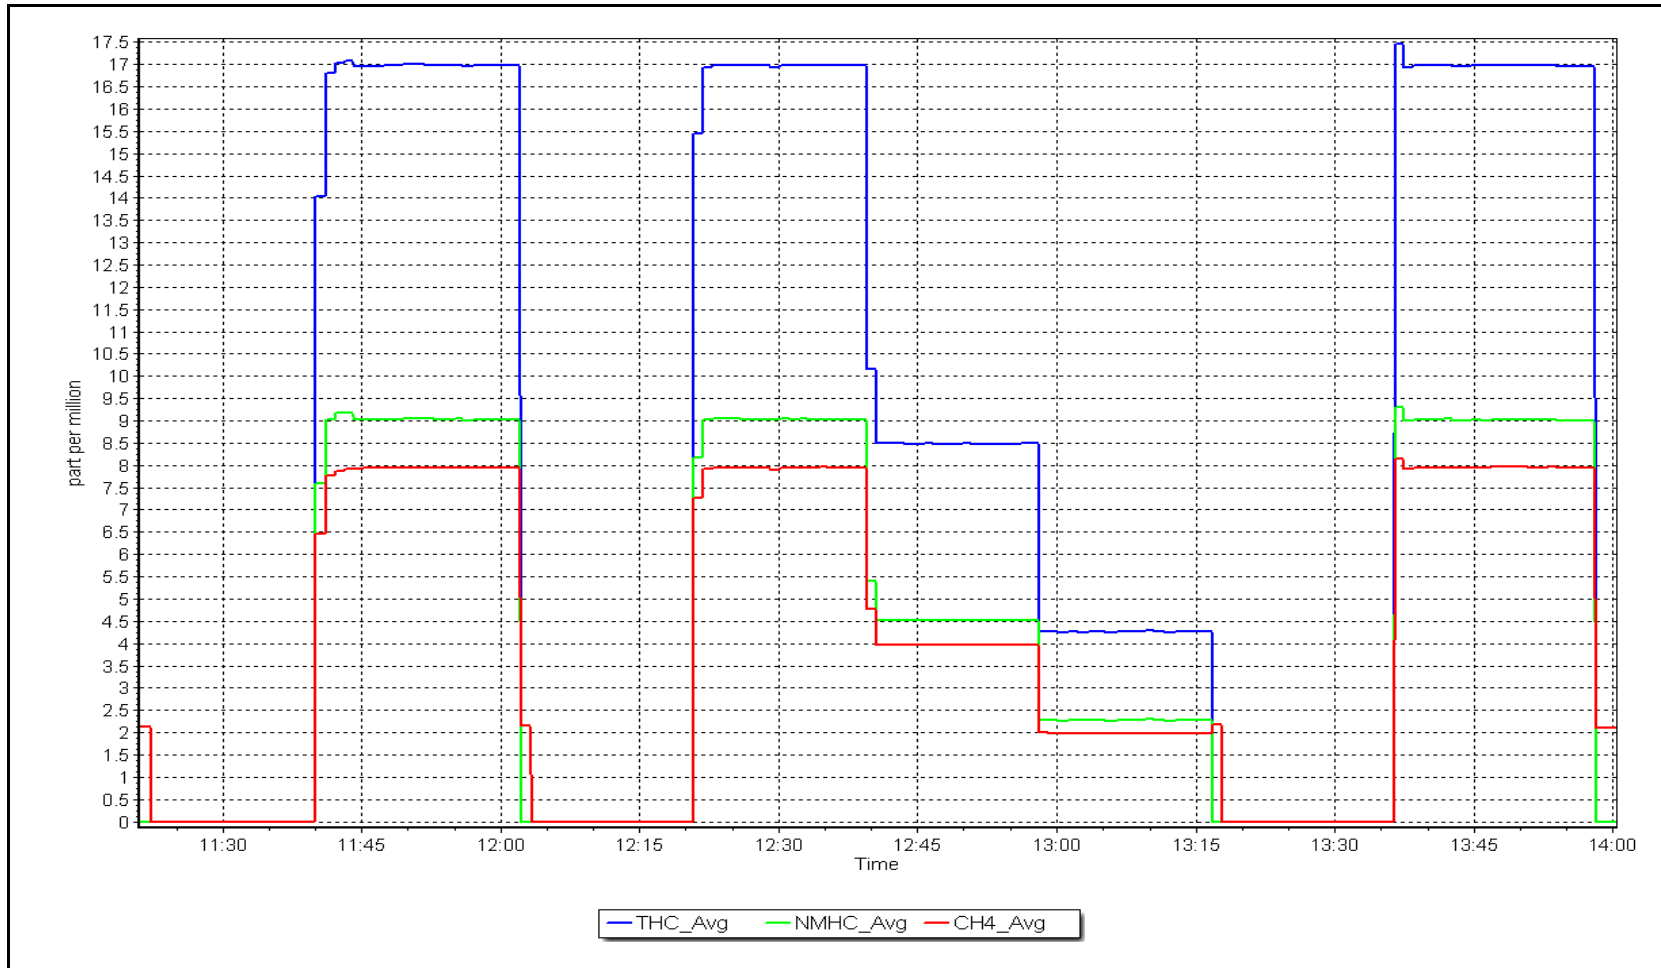



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Athabasca Valley Station number: AMS07
Calibration Date: January 19, 2023 Last Cal Date: December 12, 2022
Start time (MST): 7:10 End time (MST): 11:48
Reason: Routine

Calibration Standards

NO Gas Cylinder #: T2Y1KA4 Cal Gas Expiry Date: November 30, 2023
NO_x Cal Gas Conc: 50.92 ppm NO Cal Gas Conc: 49.92 ppm
Removed Cylinder #: NA Removed Gas Exp Date: NA
Removed Gas NO_x Conc: 50.92 ppm Removed Gas NO Conc: 49.92 ppm
NO_x gas Diff: NO gas Diff:
Calibrator Model: API T700 Serial Number: 3805
ZAG make/model: API T701H Serial Number: 198

Analyzer Information

Analyzer make: Thermo 42i Analyzer serial #: 1160120024
NO_x Range (ppb): 0 - 1000 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.048	1.048	NO bkgnd or offset:	7.3	7.3
NO _x coeff or slope:	0.995	0.995	NO _x bkgnd or offset:	7.5	7.5
NO ₂ coeff or slope:	1.000	1.000	Reaction cell Press:	198.8	198.8

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.003211	0.991445
NO _x Cal Offset:	1.159557	1.137226
NO Cal Slope:	1.003486	0.991156
NO Cal Offset:	0.775567	0.993235
NO ₂ Cal Slope:	1.001755	1.002806
NO ₂ Cal Offset:	0.287731	0.326300



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.0	0.0	0.1	----	----
as found span	4920	80.2	816.7	800.7	16.0	810.1	793.2	16.8	1.0082	1.0094
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.1	0.1	0.1	----	----
high point	4920	80.2	816.7	800.7	16.0	810.0	793.8	16.2	1.0083	1.0087
second point	4960	40.1	408.4	400.4	8.0	407.6	399.3	8.3	1.0019	1.0026
third point	4980	20.0	203.7	199.7	4.0	203.4	199.1	4.4	1.0014	1.0029
as left zero	5000	0.0	0.0	0.0	0.0	0.0	0.0	0.0	----	----
as left span	4920	80.2	816.7	401.2	415.5	816.5	394.8	421.6	1.0003	1.0162
Average Correction Factor									1.0039	1.0047

Corrected As found	NO _x = 810.1 ppb	NO = 793.2 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -1.3%	
Previous Response	NO _x = 820.5 ppb	NO = 804.3 ppb		*Percent Change	NO = -1.4%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO ₂)						
as found GPT point (200 ppb NO ₂)						
as found GPT point (100 ppb NO ₂)						
1st GPT point (400 ppb O ₃)	792.0	392.5	415.5	416.9	0.9967	100.3%
2nd GPT point (200 ppb O ₃)	792.0	597.8	210.2	211.3	0.9950	100.5%
3rd GPT point (100 ppb O ₃)	792.0	693.8	114.2	115.1	0.9925	100.8%
Average Correction Factor					0.9947	100.5%

Notes:

No maintenance or adjustments done.

Calibration Performed By:

Melissa Lemay



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 12, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	7:10	End Time (MST):	11:48
Analyzer make:	Thermo 42i	Analyzer serial #:	1160120024

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
816.7	810.0	1.0083		
408.4	407.6	1.0019		
203.7	203.4	1.0014		
			0.999988	
			0.991445	
			1.137226	

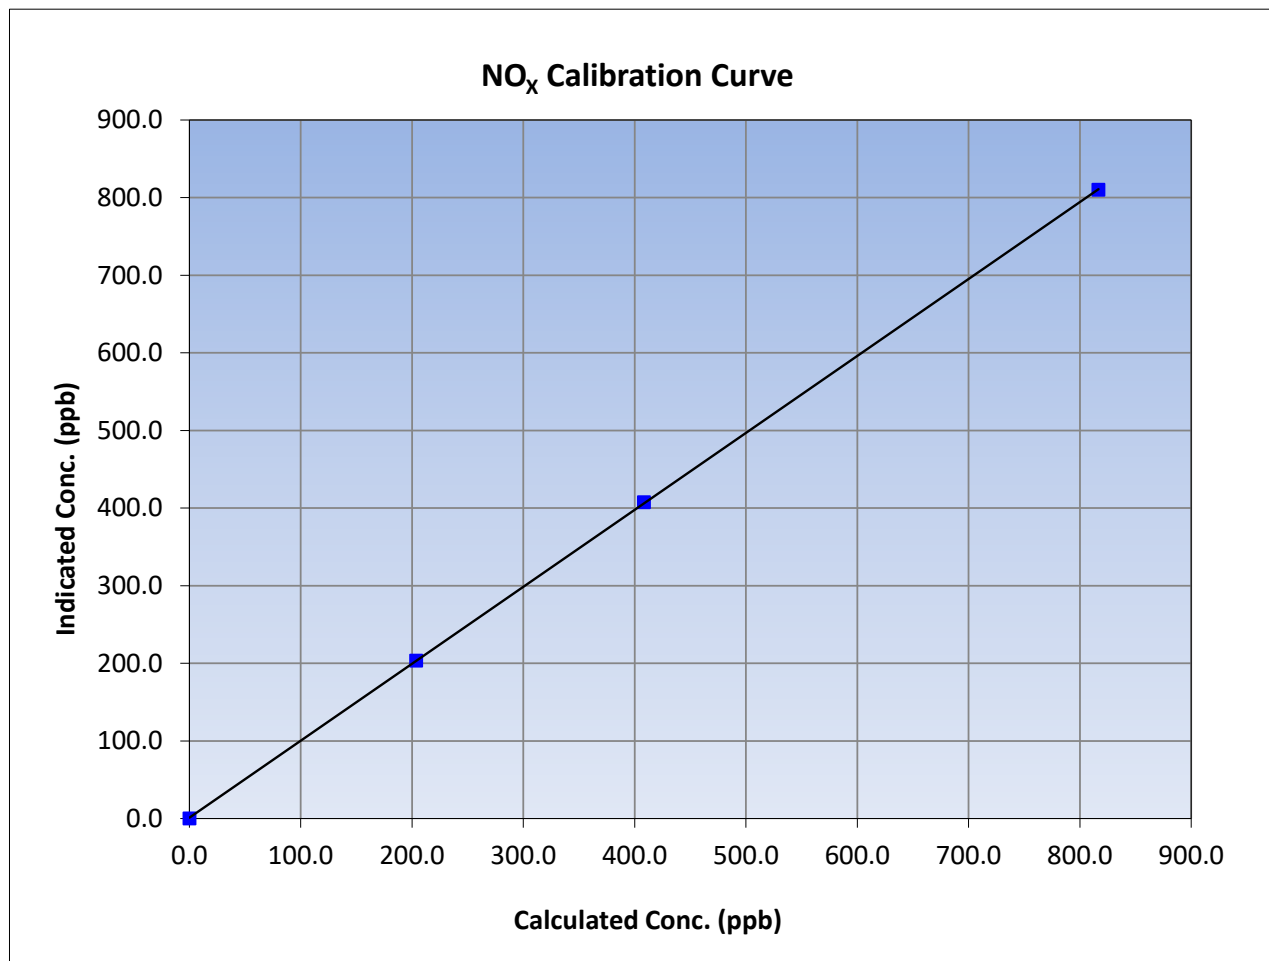



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 12, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	7:10	End Time (MST):	11:48
Analyzer make:	Thermo 42i	Analyzer serial #:	1160120024

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.1	----	Correlation Coefficient	≥0.995	
800.7	793.8	1.0087			
400.4	399.3	1.0026			
199.7	199.1	1.0029			
			Slope	0.991156	0.90 - 1.10
			Intercept	0.993235	+/-20

NO Calibration Curve

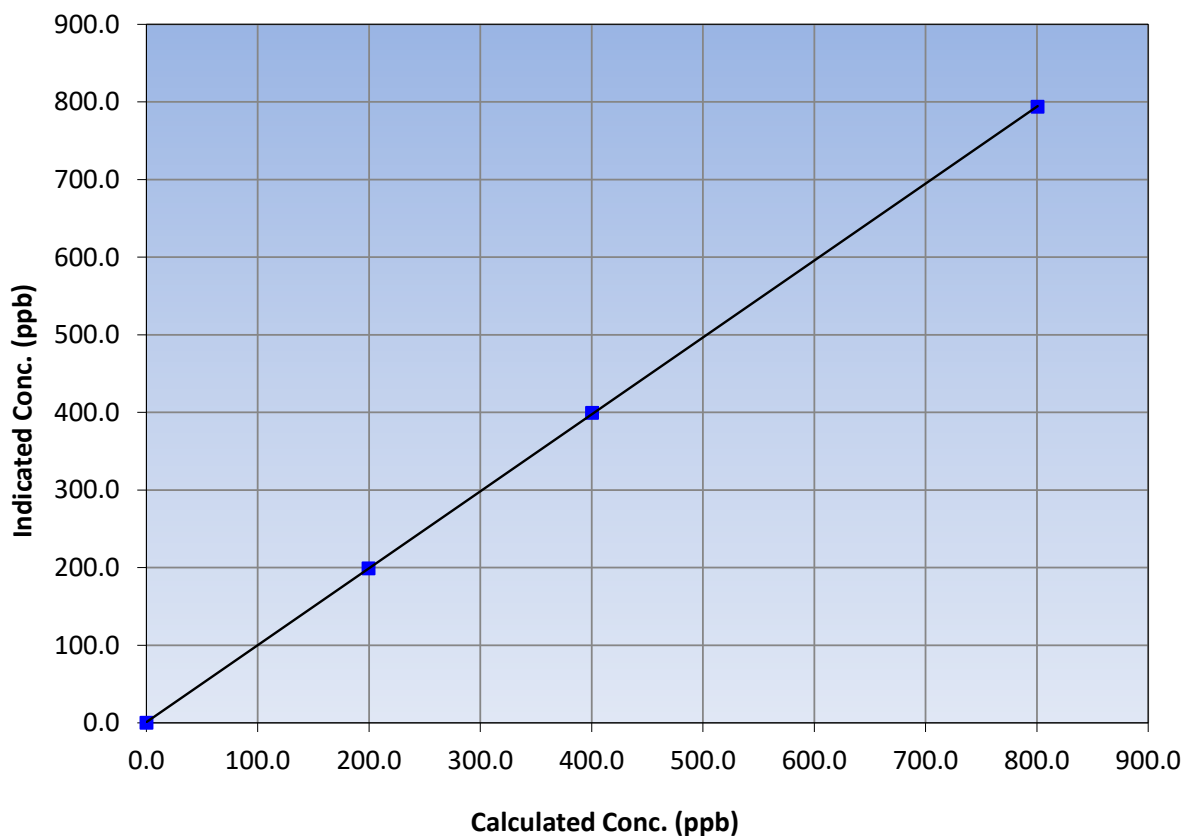



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 12, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	7:10	End Time (MST):	11:48
Analyzer make:	Thermo 42i	Analyzer serial #:	1160120024

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.1	----	Correlation Coefficient	≥0.995	
415.5	416.9	0.9967			
210.2	211.3	0.9950			
114.2	115.1	0.9925			
			Slope	1.002806	0.90 - 1.10
			Intercept	0.326300	+/-20


NO₂ Calibration Curve

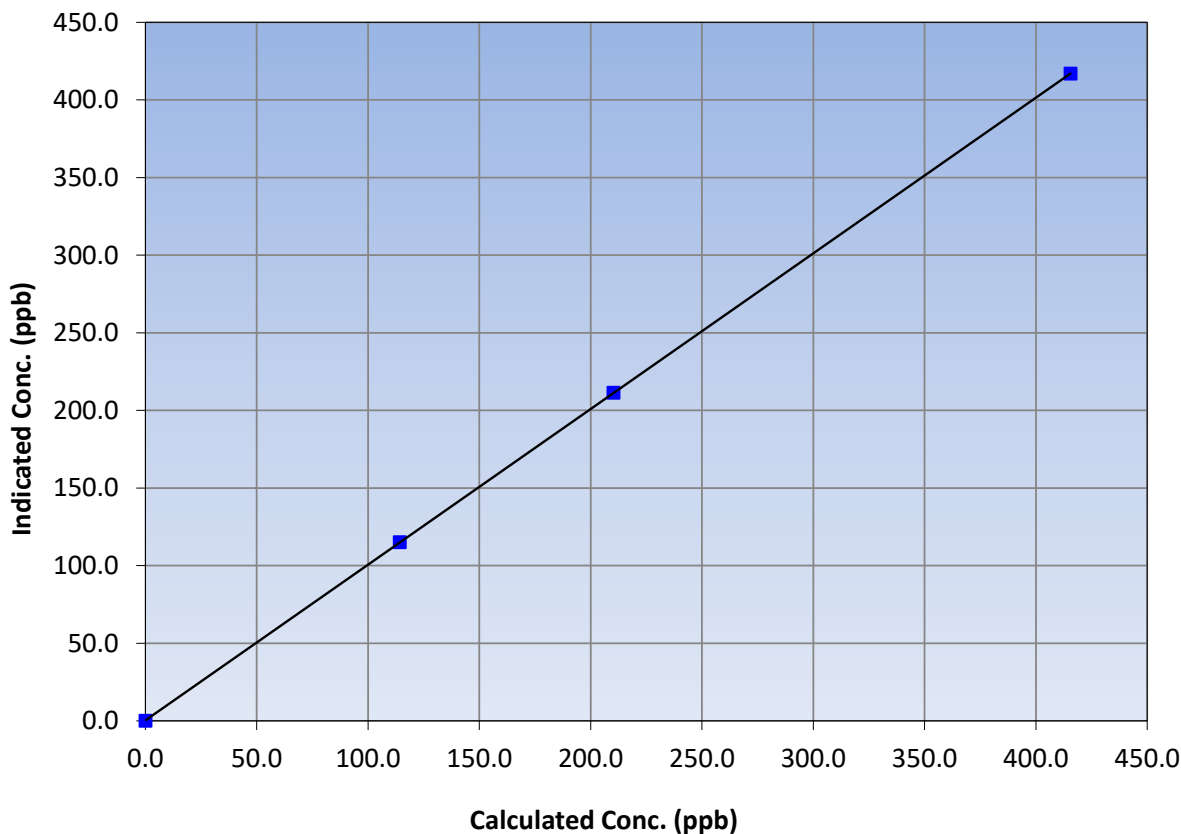

NO_x Calibration Plot

Date: January 19, 2023

Location: Athabasca Valley

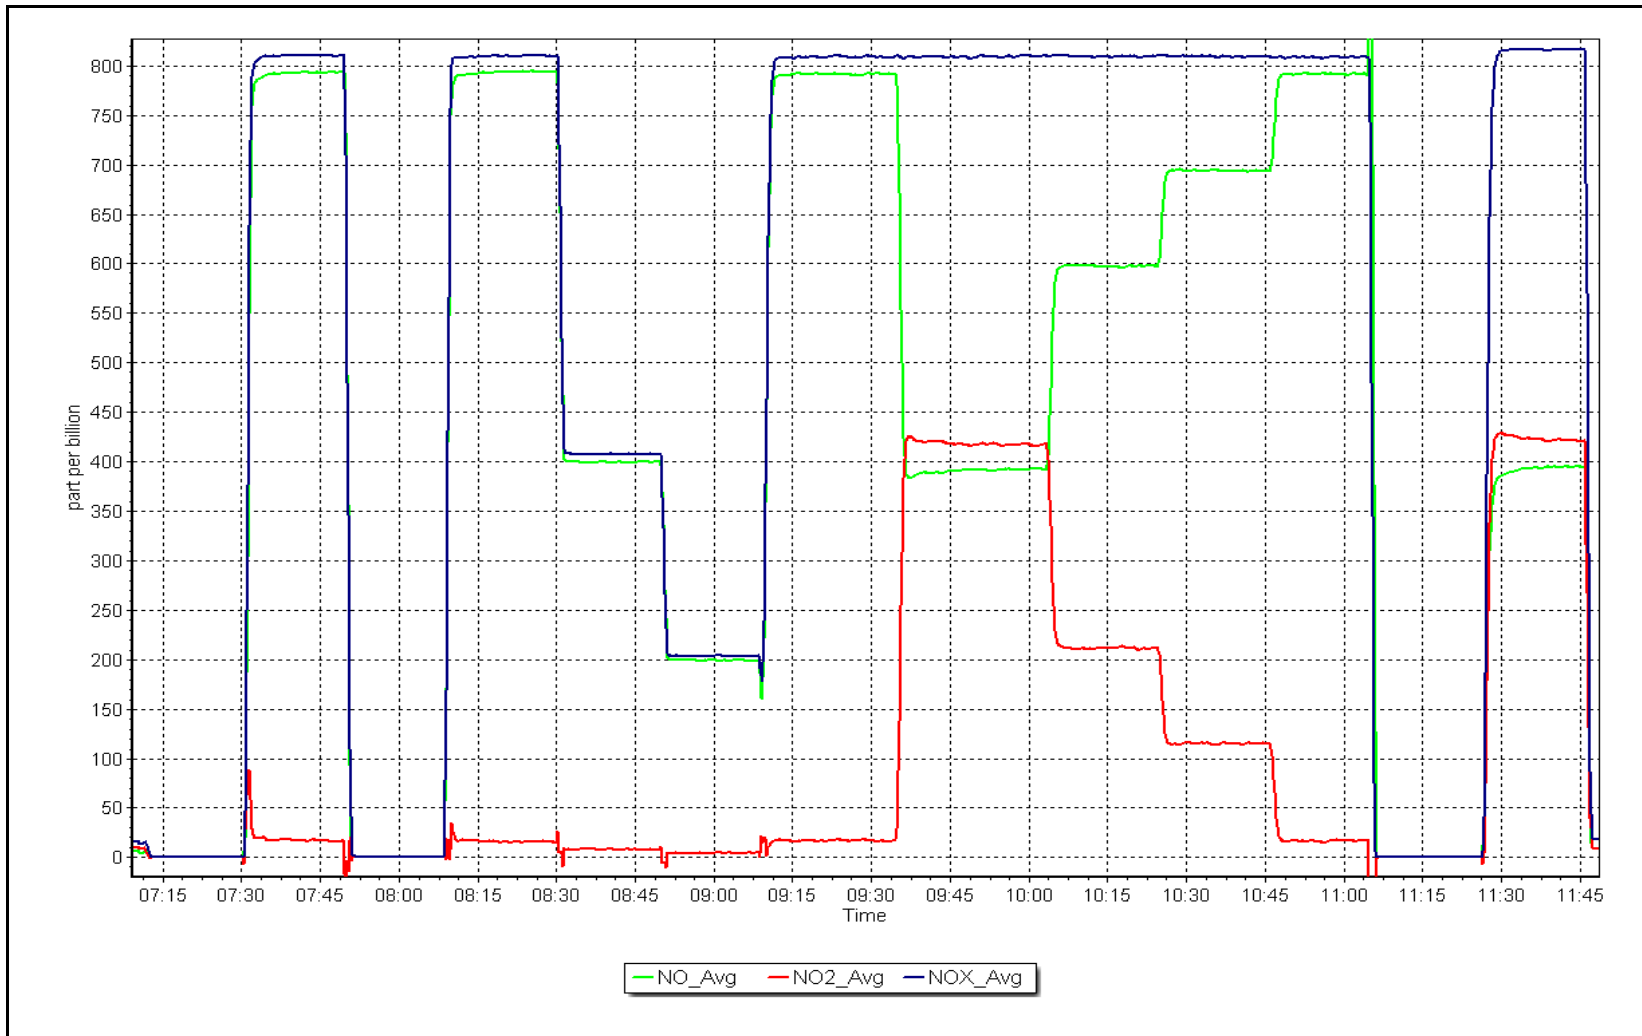



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Athabasca Valley Station number: AMS07
 Calibration Date: January 20, 2023 Last Cal Date: December 6, 2022
 Start time (MST): 10:28 End time (MST): 13:37
 Reason: Routine

Calibration Standards

O3 generation mode: Photometer
 Calibrator Make/Model: T700 Serial Number: 3805
 ZAG Make/Model: T701H Serial Number: 198

Analyzer Information

Analyzer make: Thermo 49i Analyzer serial #: 1507964700
 Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.997143	0.995429	Backgd or Offset:	-0.5	-0.6
Calibration intercept:	1.100000	1.500000	Coeff or Slope:	1.070	1.102

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	-0.1	----
as found span	5000	1374.8	400.0	391.6	1.021
as found 2nd point					
as found 3rd point					
calibrator zero	5000	0.0	0.0	0.5	----
high point	5000	1374.3	400.0	399.0	1.003
second point	5000	1017.7	200.0	201.6	0.992
third point	5000	840.4	100.0	101.7	0.983
as left zero	5000	0.0	0.0	0.0	----
as left span	5000	1373.6	400.0	403.5	0.991
Average Correction Factor					0.993

Baseline Corr As found:	391.7	Previous response	400.0	*% change	-2.1%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: No Maintenance done. Span adjusted.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 6, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	10:28	End Time (MST):	13:37
Analyzer make:	Thermo 49i	Analyzer serial #:	1507964700

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.5	----	Correlation Coefficient	0.999966	≥0.995
400.0	399.0	1.0025			
200.0	201.6	0.9921	Slope	0.995429	0.90 - 1.10
100.0	101.7	0.9833			
			Intercept	1.500000	+/- 5

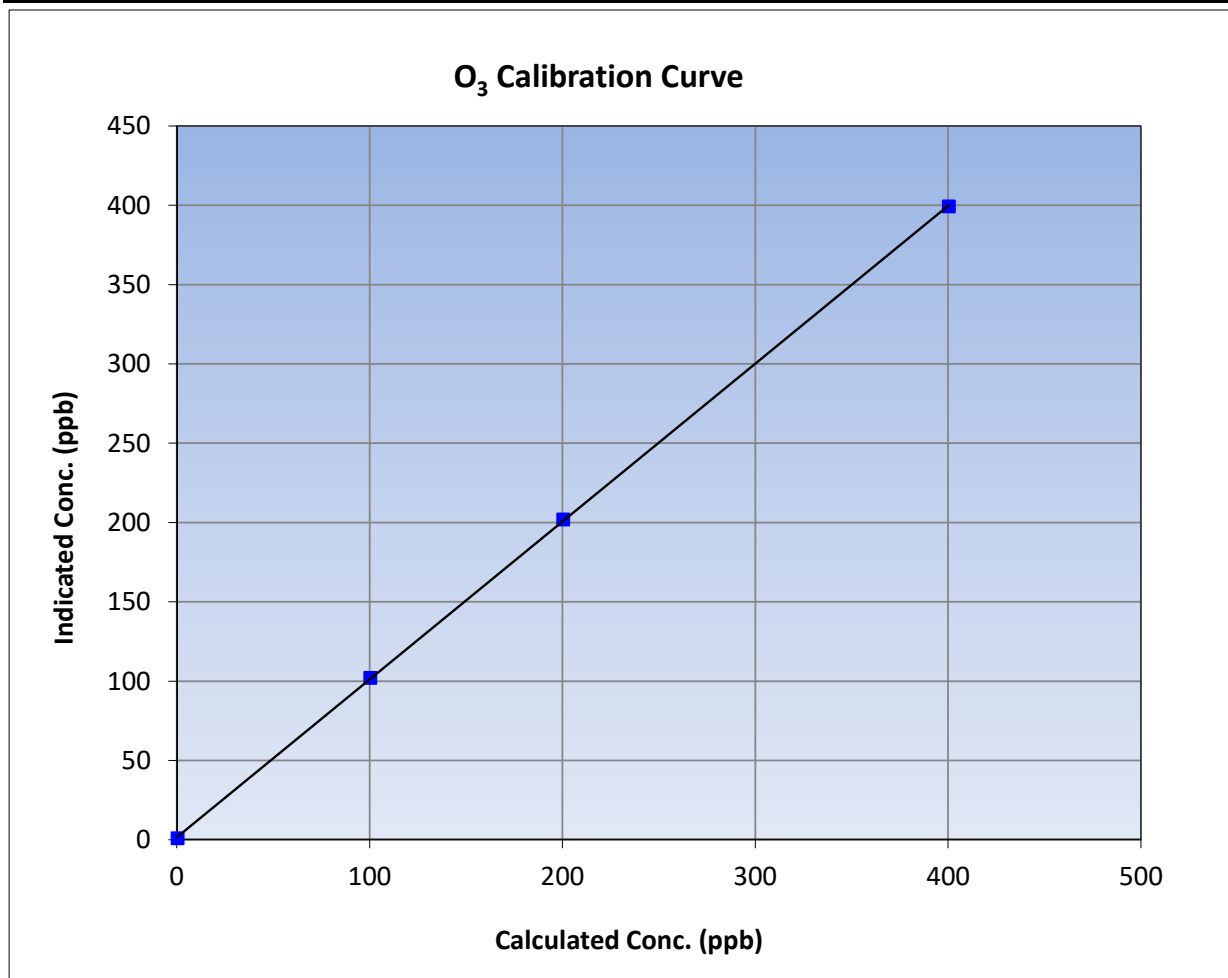

O₃ Calibration Plot

Date: January 20, 2023

Location: Athabasca Valley

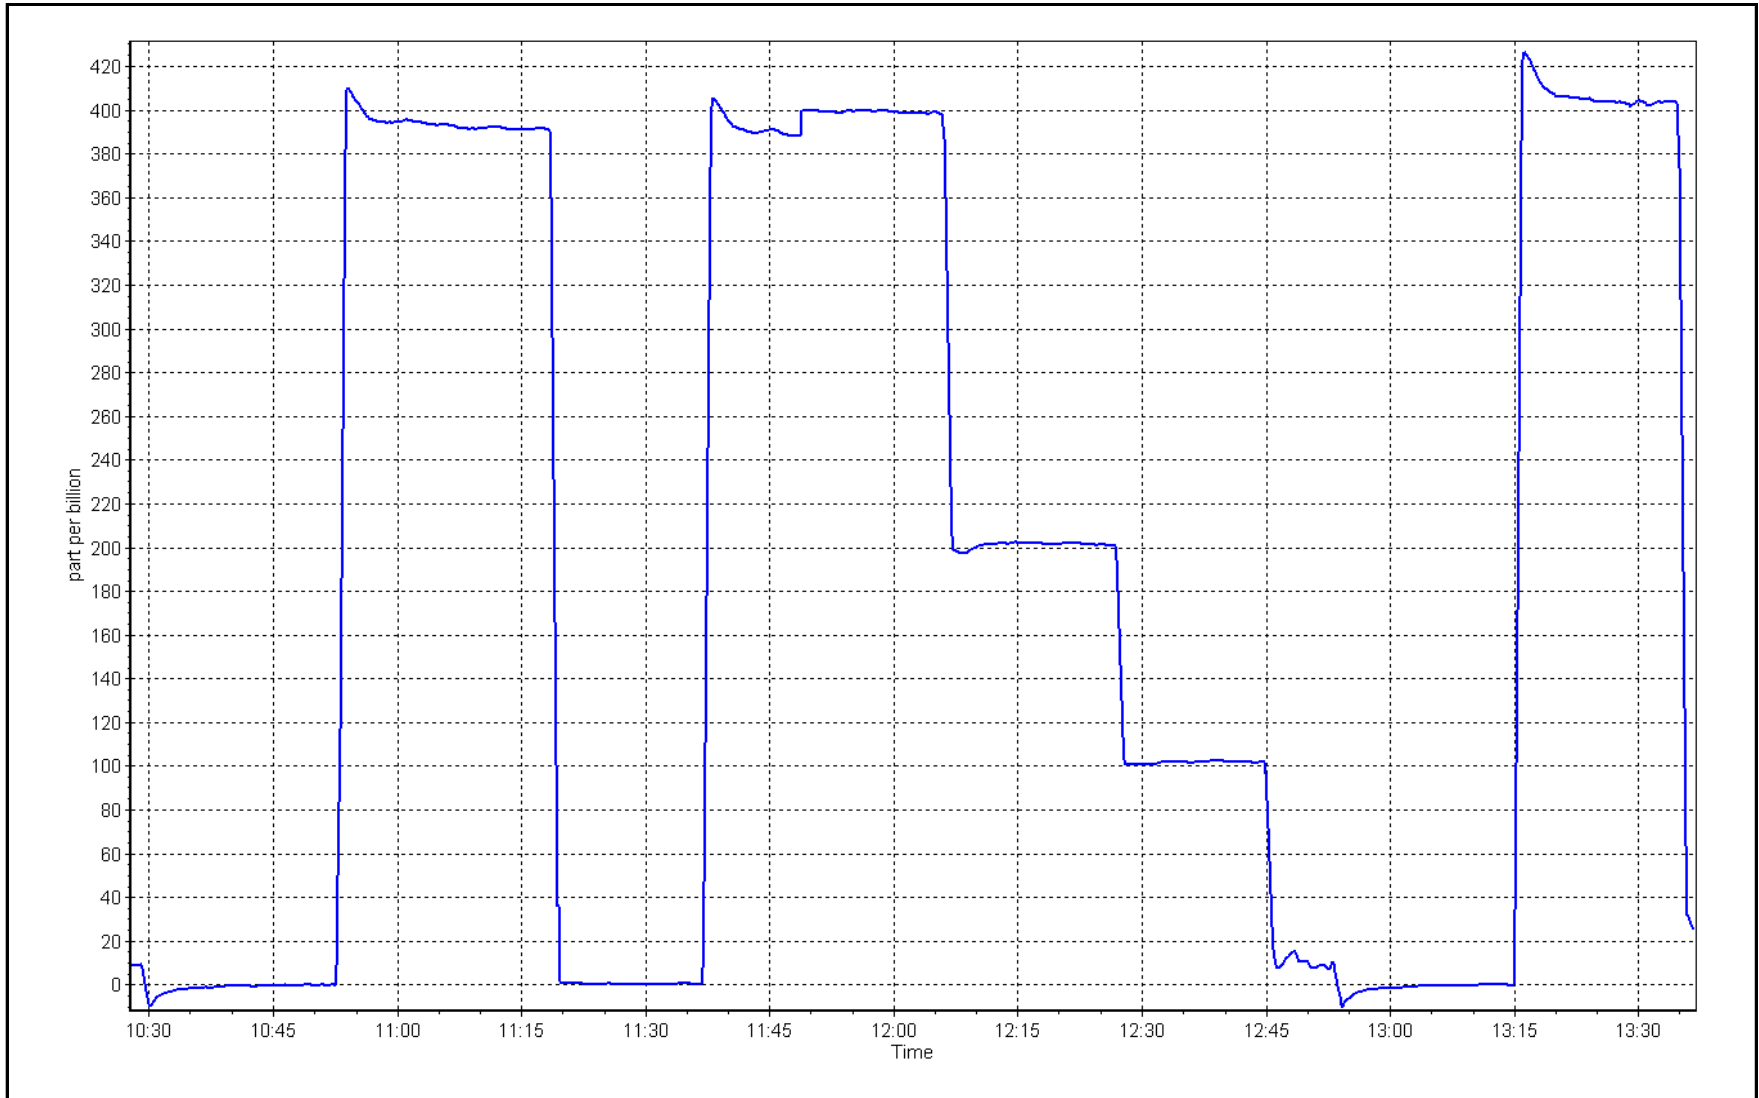



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Athabasca Valley Station number: AMS 07
Calibration Date: January 19, 2023 Last Cal Date: December 5, 2022
Start time (MST): 11:51 End time (MST): 12:29

Analyzer Make: API T640 S/N: 326
Particulate Fraction: PM2.5

Flow Meter Make/Model: Alicat FP-25BT S/N: 388753
Temp/RH standard: Alicat FP-25BT S/N: 388753

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-6.0	-6.1	-6.0	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	733.1	735.2	733.1	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5.00	5.08	5.00	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 19, 2023 December 5, 2022
PM w/o HEPA: 11.2 PM w/ HEPA: 0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test				<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: December 5, 2022
Disposable Filter Changed: December 5, 2022

Annual Maintenance

Date Sample Tube Cleaned: December 5, 2022
Date RH/T Sensor Cleaned: December 5, 2022

Notes: No adjustments done. Inlet Head cleaned.

Calibration by: Melissa Lemay



Wood Buffalo Environmental Association

CO Calibration Report

Version-01-2020

Station Information

Station Name:	Athabasca Valley	Station number:	AMS07
Calibration Date:	January 20, 2023	Last Cal Date:	December 14, 2022
Start time (MST):	7:05	End time (MST):	9:52
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	3,000	ppm	Cal Gas Exp Date:	December 12, 2026
Cal Gas Cylinder #:	LL66942			
Removed Cal Gas Conc:	3,000	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	3805
ZAG Make/Model:	API 700H		Serial Number:	198

Analyzer Information

Analyzer make:	Thermo 48i-LTE	Analyzer serial #:	1408761381
Analyzer Range:	0 - 50 ppm		

	Start	Finish		Start	Finish
Calibration slope:	0.999858	0.999713	Backgd or Offset:	3.341	3.600
Calibration intercept:	0.074542	0.044565	Coeff or Slope:	1.079	1.079

CO Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	----
as found span	4933	66.7	40.0	40.4	0.991
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.0	----
high point	4933	66.7	40.0	40.0	1.001
second point	4967	33.3	20.0	20.1	0.992
third point	4983	16.7	10.0	10.0	0.998
as left zero	5000	0.0	0.0	0.0	----
as left span	4933	66.7	40.0	40.0	1.001
Average Correction Factor					0.997

Baseline Corr As found:	40.38	Prev response:	40.09	*% change:	0.7%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: No Maintenance done. Zero adjusted.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

CO Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 14, 2022
Station Name:	Athabasca Valley	Station Number:	AMS07
Start Time (MST):	7:05	End Time (MST):	9:52
Analyzer make:	Thermo 48i-LTE	Analyzer serial #:	1408761381

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	0.999977	≥0.995
40.0	40.0	1.0006			
20.0	20.1	0.9920	Slope	0.999713	0.90 - 1.10
10.0	10.0	0.9981			
			Intercept	0.044565	+/-1.5

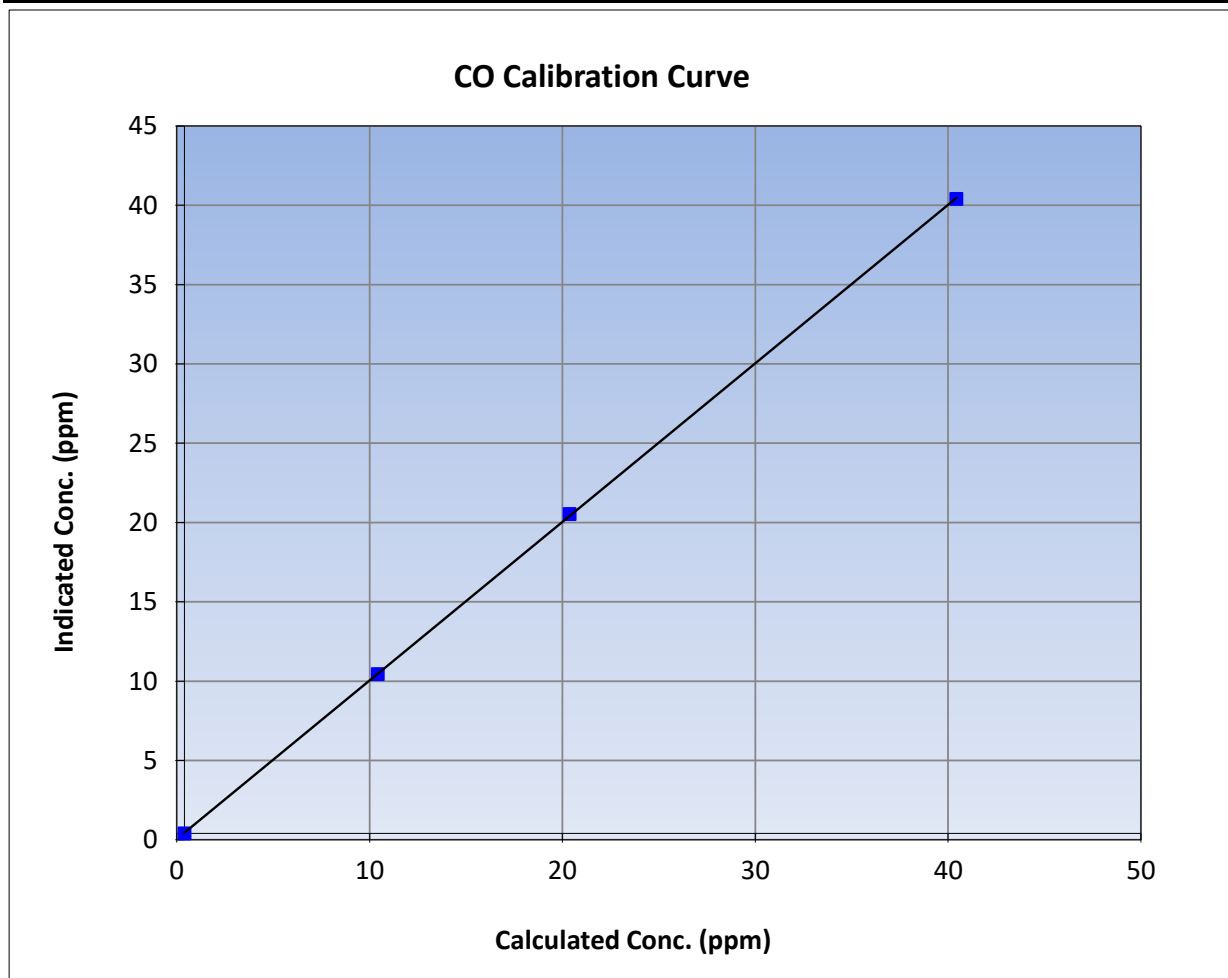

CO Calibration Plot

Date: January 20, 2023

Location: Athabasca Valley

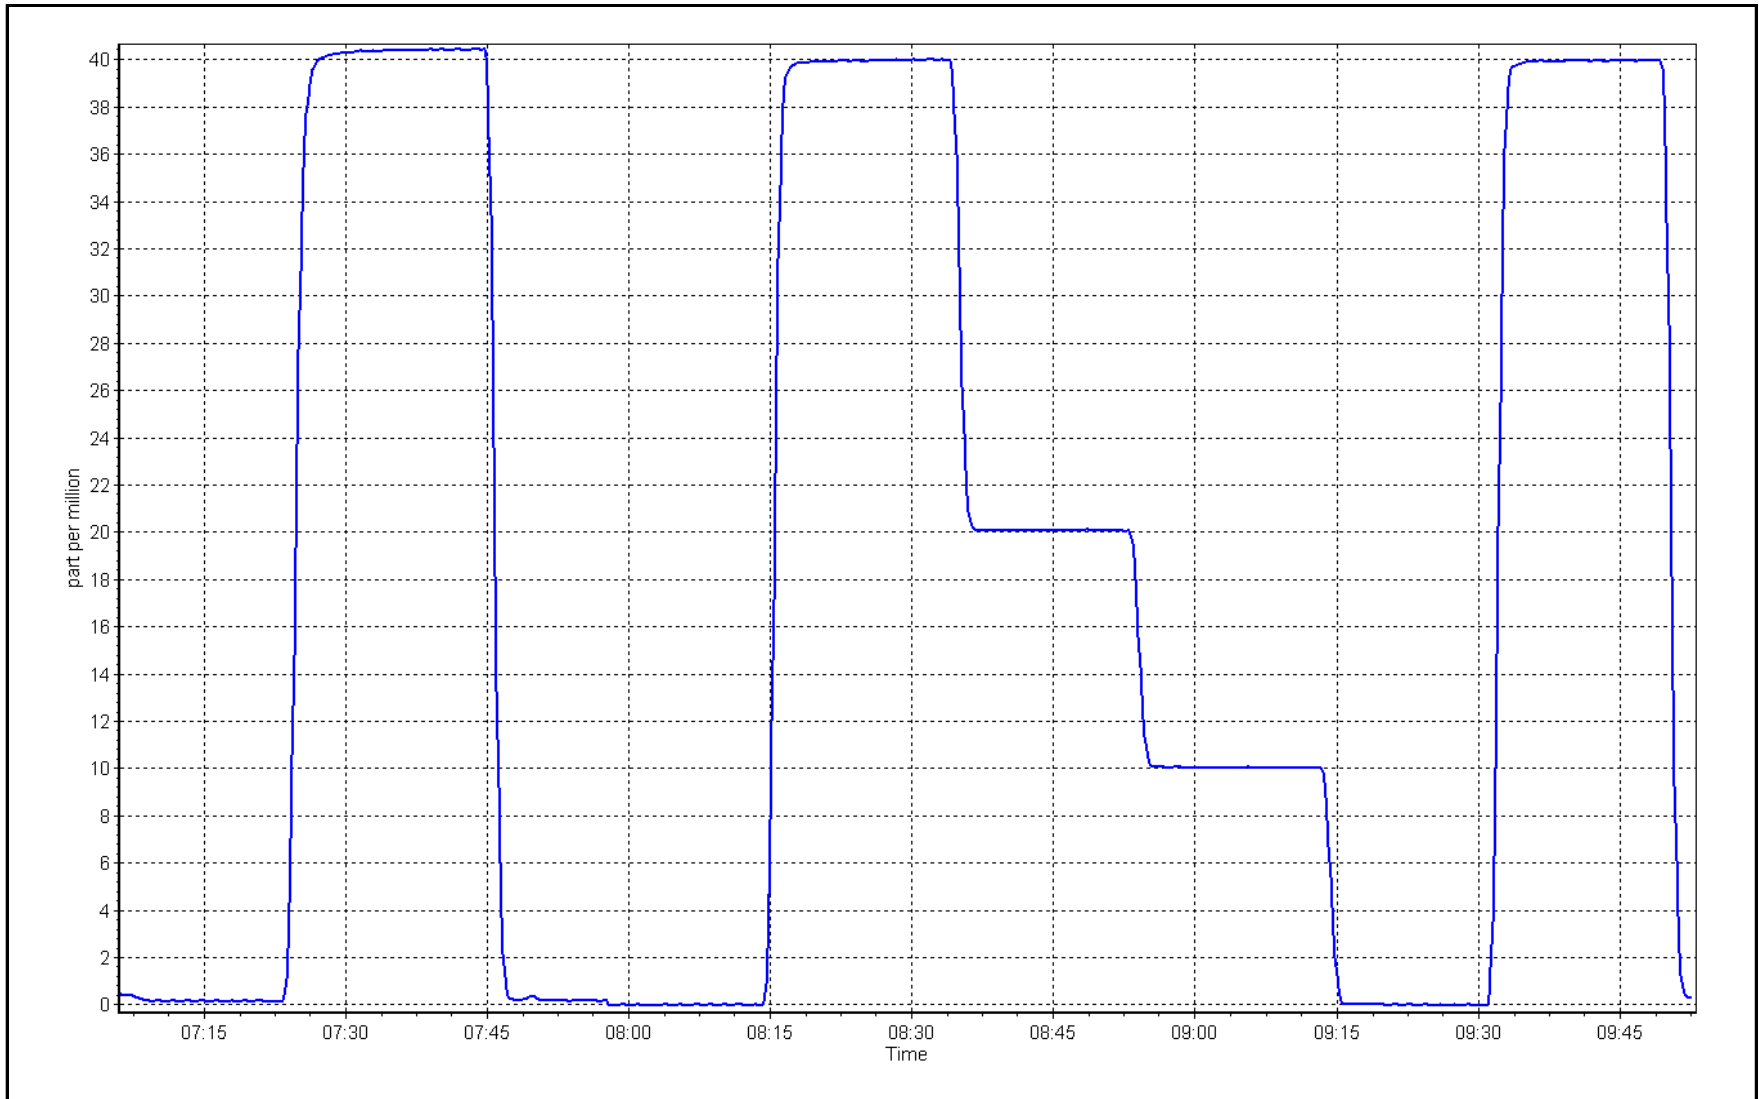



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS08 FORT CHIPEWYAN JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Fort Chipewyan	Station number:	AMS08
Calibration Date:	January 11, 2023	Last Cal Date:	December 6, 2022
Start time (MST):	12:19	End time (MST):	3:08 PM
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.84	ppm	Cal Gas Exp Date:	January 6, 2030
Cal Gas Cylinder #:	CC196697			
Removed Cal Gas Conc:	49.84	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	3252
ZAG Make/Model:	Teledyne API T701		Serial Number:	260

Analyzer Information

Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1136451241
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.999374	1.000787	Backgd or Offset:	1.31	1.32
Calibration intercept:	0.136257	0.415954	Coeff or Slope:	1.006	1.006

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4920	80.3	800.4	804.8	0.995
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.2	----
high point	4920	80.3	800.4	801.7	0.998
second point	4960	40.2	400.7	400.4	1.001
third point	4980	20.1	200.4	201.9	0.992
as left zero	5000	0.0	0.0	0.3	----
as left span	4920	80.3	800.4	806.4	0.993
Average Correction Factor					0.997

Baseline Corr As found:	804.70	Previous response	800.02	*% change	0.6%
-------------------------	--------	-------------------	--------	-----------	------

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. no adjustments needed

Calibration Performed By: Morgan Voyageur



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 6, 2022
Station Name:	Fort Chipewyan	Station Number:	AMS08
Start Time (MST):	12:19	End Time (MST):	15:08
Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1136451241

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999994	≥0.995
800.4	801.7	0.9984			
400.7	400.4	1.0007	Slope	1.000787	0.90 - 1.10
200.4	201.9	0.9923			
			Intercept	0.415954	+/-30

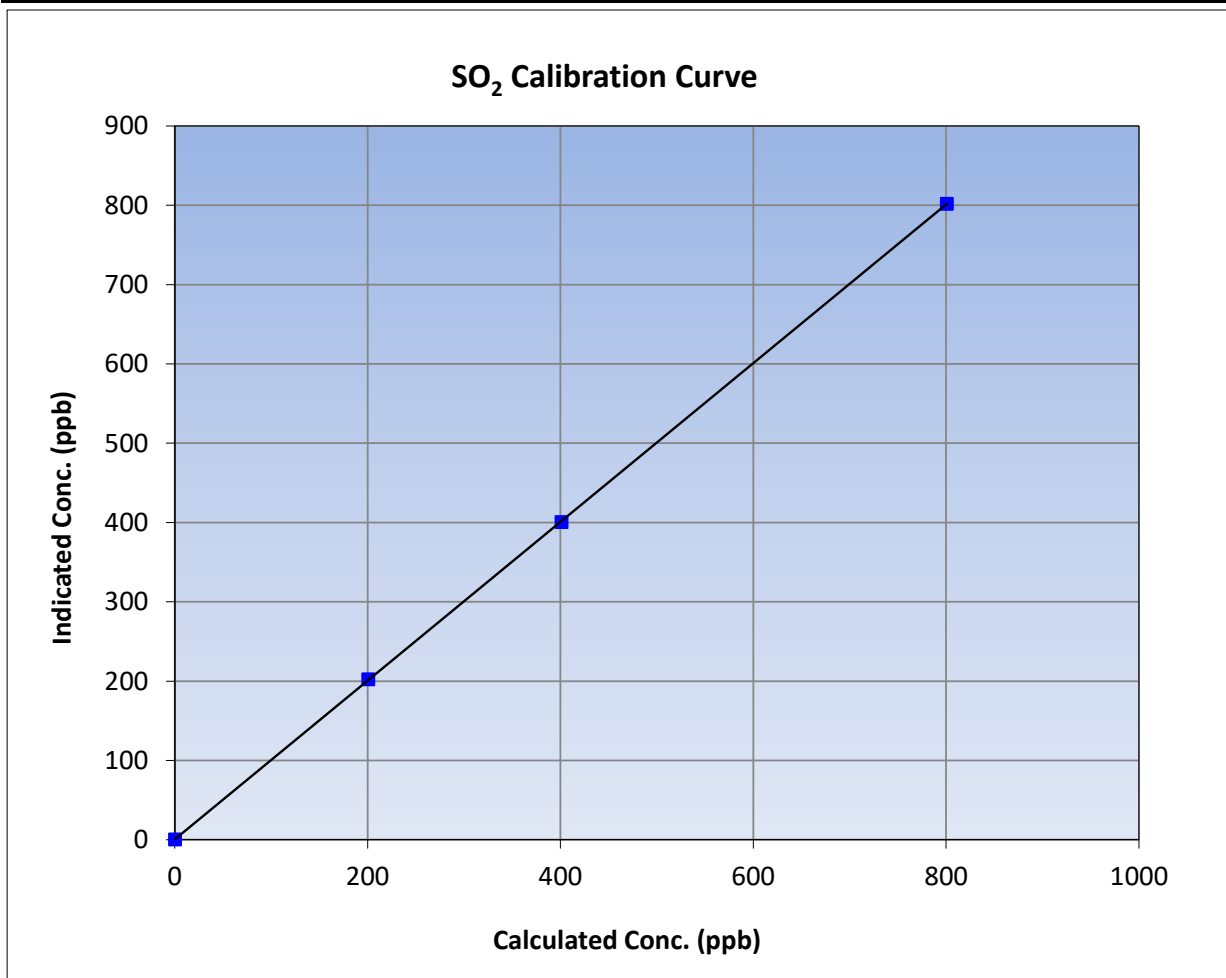

SO2 Calibration Plot

Date: January 11, 2023

Location: Fort Chipewyan

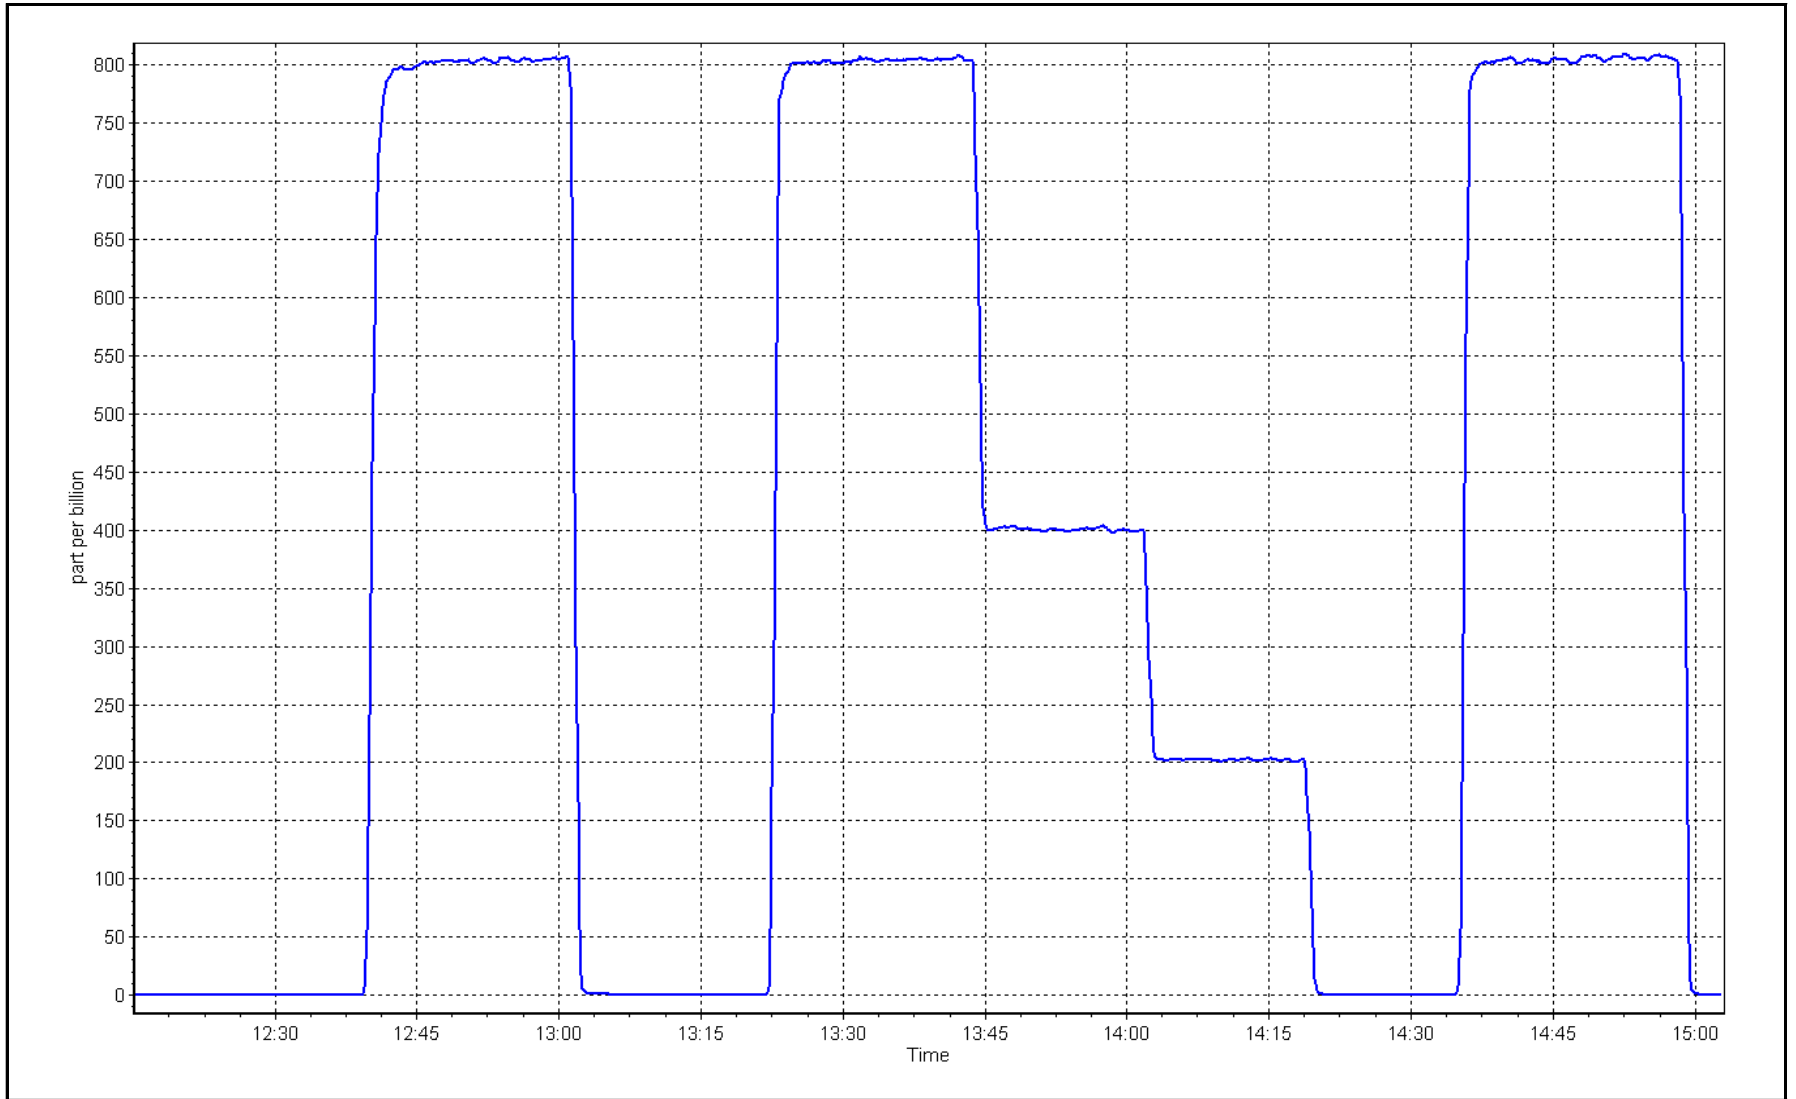



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name: Fort Chipewyan Station number: AMS08
 Calibration Date: January 11, 2023 Last Cal Date: December 5, 2022
 Start time (MST): 8:20 End time (MST): 12:05
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 4.97 ppm Cal Gas Exp Date: February 9, 2024
 Cal Gas Cylinder #: EY0002276
 Removed Cal Gas Conc: 4.97 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: Teledyne API T700 Serial Number: 3252
 ZAG Make/Model: Teledyne API T701 Serial Number: 260

Analyzer Information

Analyzer make: Thermo 43iQ-TL Analyzer serial #: 1203169744
 Converter make: CDN-101 Converter serial #: 14639
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.001428	0.999140	Backgd or Offset:	1.42	1.42
Calibration intercept:	-0.261248	0.018799	Coeff or Slope:	0.743	0.743

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	-0.1	----
as found span	4920	80.5	80.0	80.1	0.998
as found 2nd point	4960	40.2	40.0	39.9	0.999
as found 3rd point	4980	20.1	20.0	19.7	1.009
new cylinder response					

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.0	----
high point	4920	80.5	80.0	79.9	1.001
second point	4960	40.2	40.0	40.1	0.996
third point	4980	20.1	20.0	19.9	1.004
as left zero	5000	0.0	0.0	0.1	----
as left span	4920	80.5	80.0	80.1	0.999
SO2 Scrubber Check	4919.7	80.3	803.0	0.1	----
Date of last scrubber change:	March 7, 2022			Ave Corr Factor	1.001
Date of last converter efficiency test:	March 15, 2022			100.7% efficiency	

Baseline Corr As found: 80.2 Prev response: 79.86 *% change: 0.4%
 Baseline Corr 2nd AF pt: 40.0 AF Slope: 1.003284 AF Intercept: -0.201206
 Baseline Corr 3rd AF pt: 19.8 AF Correlation: 0.999991

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. Scrubber check completed after the calibrator zero. No adjustments

Calibration Performed By: Morgan Voyageur



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 5, 2022
Station Name:	Fort Chipewyan	Station Number:	AMS08
Start Time (MST):	8:20	End Time (MST):	12:05
Analyzer make:	Thermo 43iQ-TL	Analyzer serial #:	1203169744

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	0.999990	≥0.995
80.0	79.9	1.0014			
40.0	40.1	0.9964	Slope	0.999140	0.90 - 1.10
20.0	19.9	1.0040			
			Intercept	0.018799	+/-3

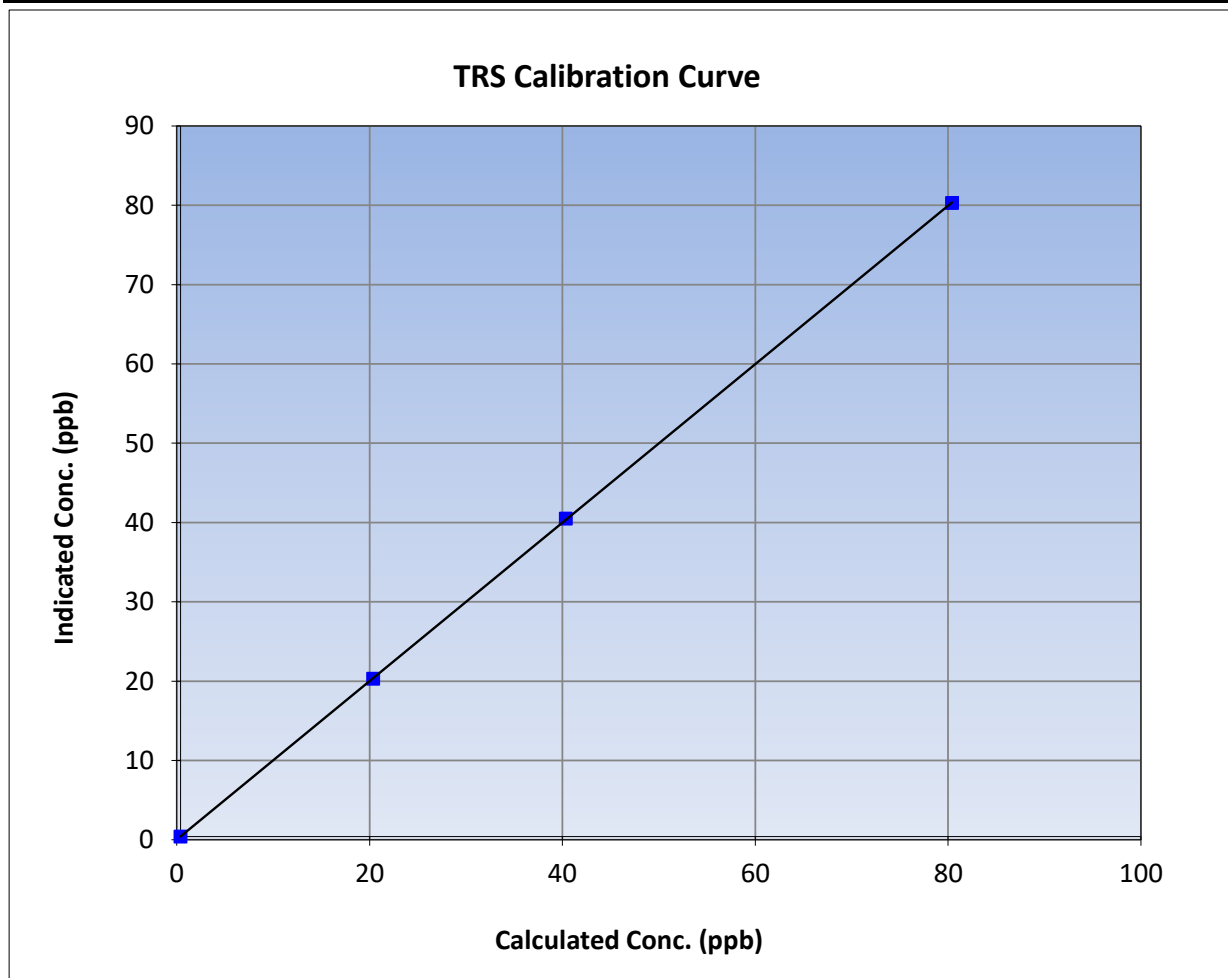

TRS Calibration Plot

Date: January 11, 2023

Location: Fort Chipewyan

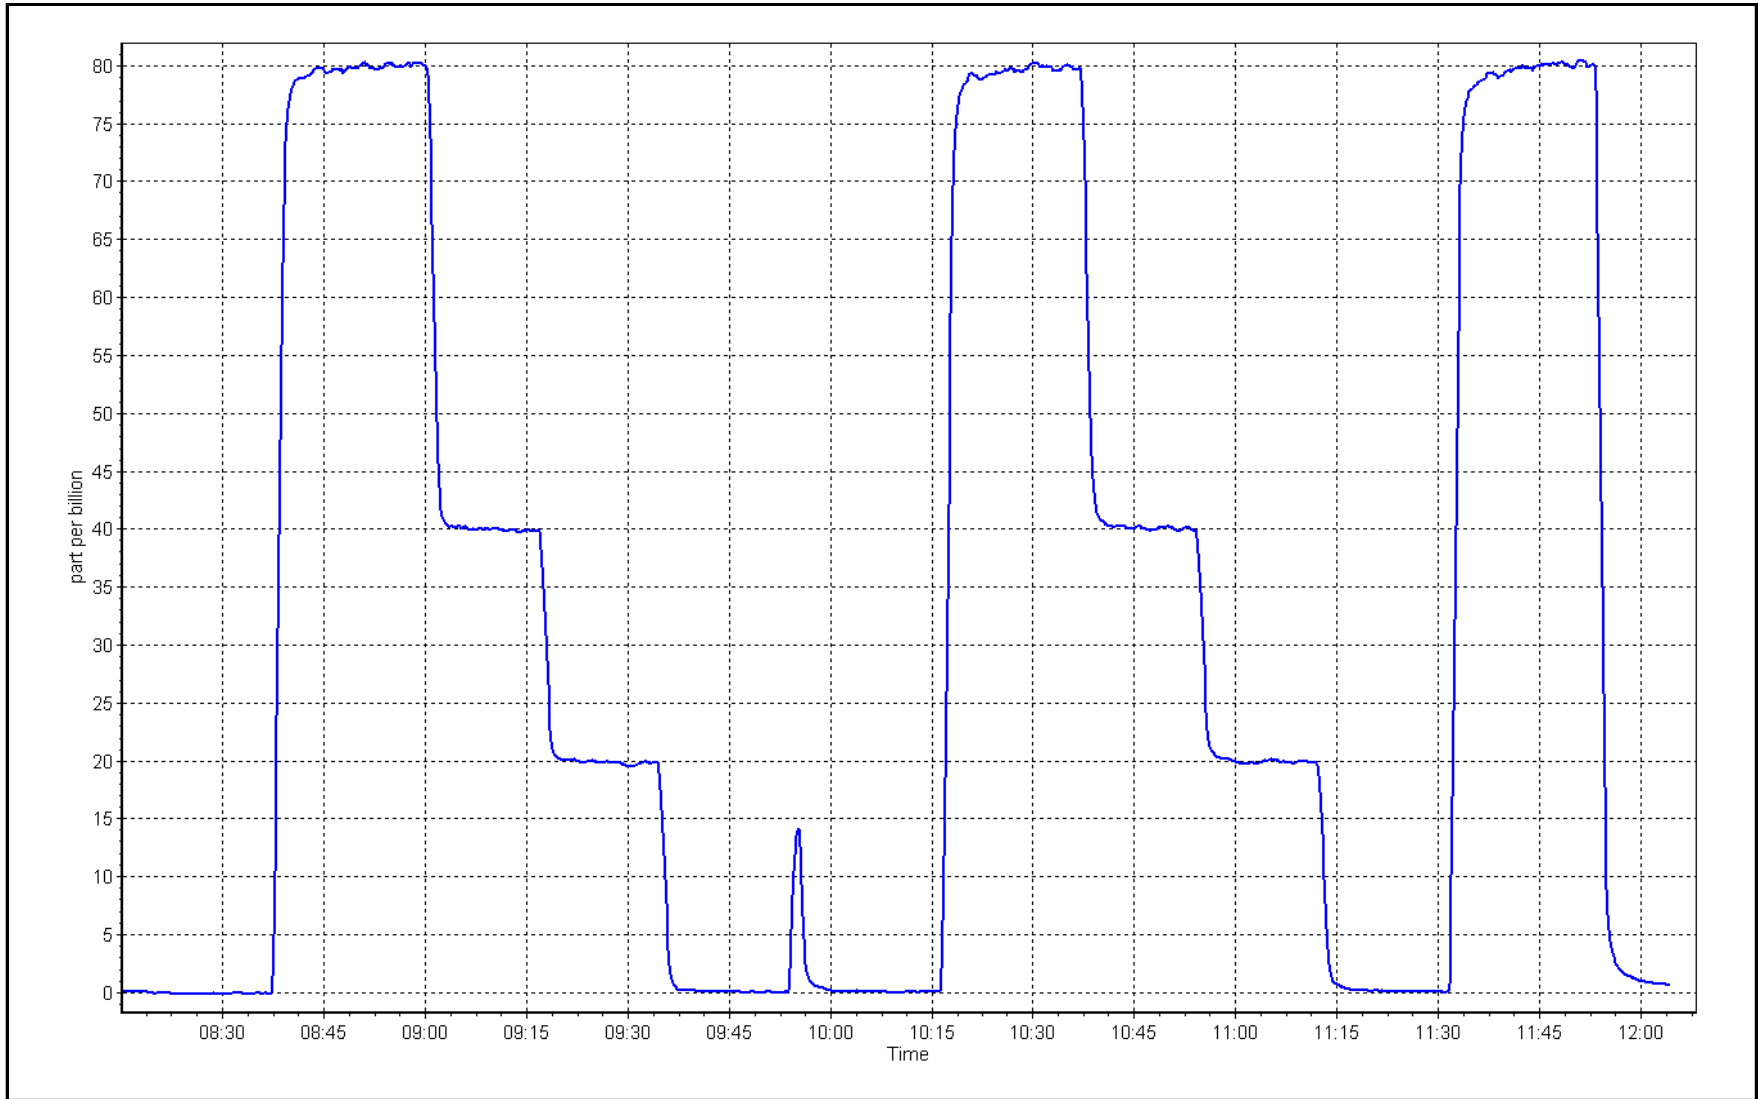



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Fort Chipewyan
Calibration Date: January 10, 2023
Start time (MST): 10:28
Reason: Routine
Station number: AMS08
Last Cal Date: December 5, 2022
End time (MST): 15:41

Calibration Standards

NO Gas Cylinder #: CC363447
NOX Cal Gas Conc: 48.80 ppm
Removed Cylinder #: NA
Removed Gas NOX Conc: 48.80 ppm
NOX gas Diff:
Calibrator Model: Teledyne API T700
ZAG make/model: Teledyne API T701H
Cal Gas Expiry Date: February 2, 2024
NO Cal Gas Conc: 48.80 ppm
Removed Gas Exp Date: NA
Removed Gas NO Conc: 48.80 ppm
NO gas Diff:
Serial Number: 3252
Serial Number: 260

Analyzer Information

Analyzer make: Thermo 42i
NOX Range (ppb): 0 - 1000 ppb
Analyzer serial #: 1426262592

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.819	1.844	NO bkgnd or offset:	6.8	6.9
NOX coeff or slope:	0.997	0.993	NOX bkgnd or offset:	6.8	6.9
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	252.6	252.6

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	0.998229	0.995345
NO _x Cal Offset:	-1.120000	0.840000
NO Cal Slope:	1.000300	0.998815
NO Cal Offset:	-2.120000	-0.200000
NO ₂ Cal Slope:	1.005217	0.991767
NO ₂ Cal Offset:	-0.633827	-0.832054



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.9	0.7	0.1	----	----
as found span	4918	82.0	800.3	800.3	0.0	794.0	787.9	6.8	1.0080	1.0158
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	1.0	0.9	0.1	----	----
high point	4918	82.0	800.3	800.3	0.0	797.7	800.0	-2.2	1.0033	1.0004
second point	4959	41.0	400.2	400.2	0.0	398.5	398.1	0.4	1.0042	1.0052
third point	4980	20.5	200.1	200.1	0.0	200.2	199.1	1.1	0.9994	1.0049
as left zero	5000	0.0	0.0	0.0	0.0	0.0	0.0	0.1	----	----
as left span	4918	82.0	800.3	412.1	388.2	800.5	412.4	388.3	0.9998	0.9993
Average Correction Factor									1.0023	1.0035

Corrected As found	NO _x = 793.1 ppb	NO = 787.2 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -0.6%	
Previous Response	NO _x = 797.8 ppb	NO = 798.4 ppb		*Percent Change	NO = -1.4%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	798.4	410.2	388.2	384.8	1.0088	99.1%
2nd GPT point (200 ppb O3)	798.4	603.7	194.7	191.3	1.0178	98.3%
3rd GPT point (100 ppb O3)	798.4	704.5	93.9	91.7	1.0240	97.7%
Average Correction Factor					1.0169	98.3%

Notes: Sample inlet filter changed after as founds. Adjusted the zero and span.

Calibration Performed By: Morgan Voyageur



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 5, 2022
Station Name:	Fort Chipewyan	Station Number:	AMS08
Start Time (MST):	10:28	End Time (MST):	15:41
Analyzer make:	Thermo 42i	Analyzer serial #:	1426262592

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	1.0	----	Correlation Coefficient Slope Intercept	0.999998 0.995345 0.840000	
800.3	797.7	1.0033			≥0.995
400.2	398.5	1.0042			0.90 - 1.10
200.1	200.2	0.9994			+/-20

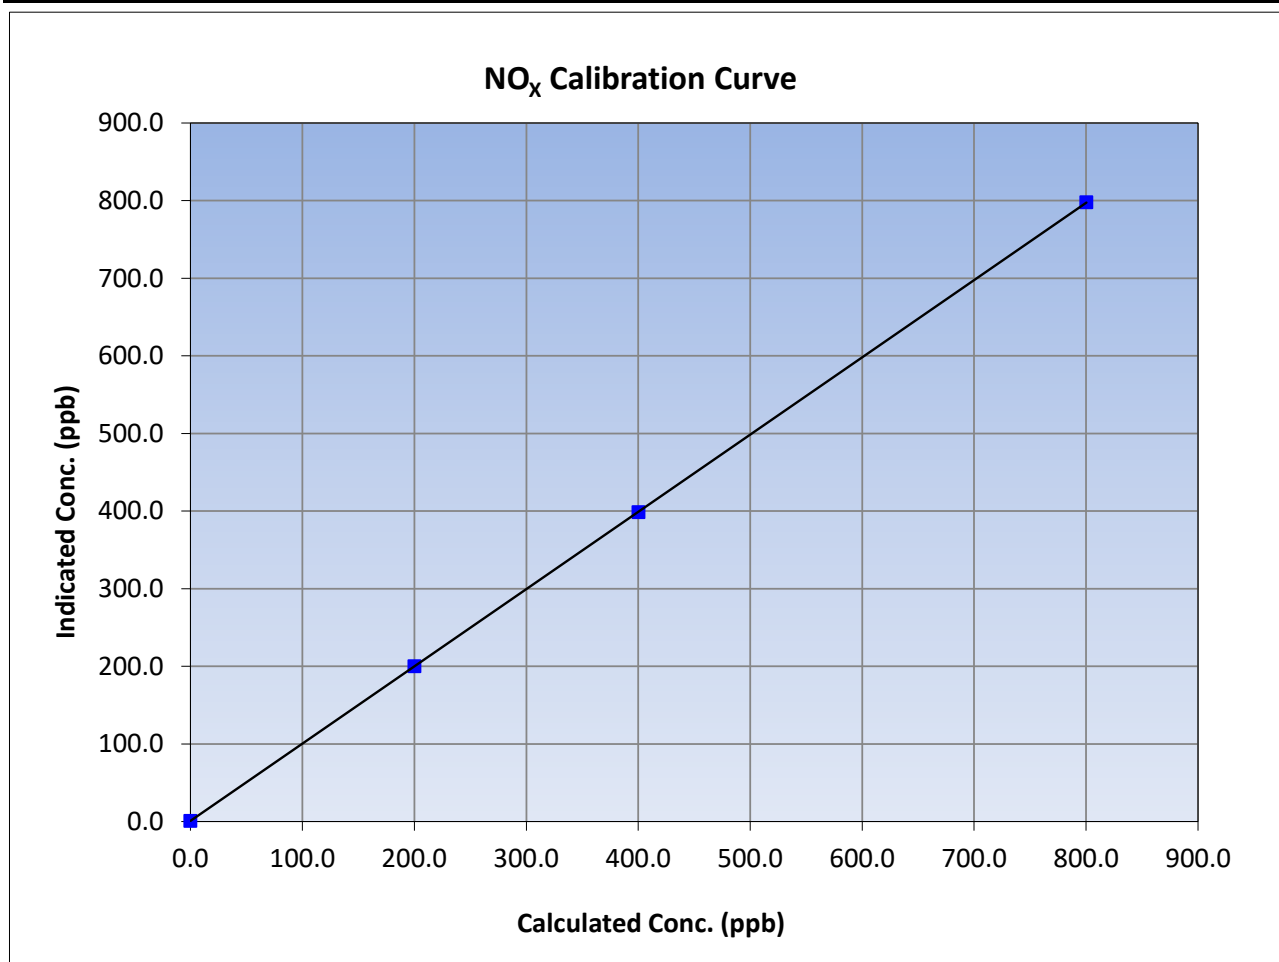



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 5, 2022
Station Name:	Fort Chipewyan	Station Number:	AMS08
Start Time (MST):	10:28	End Time (MST):	15:41
Analyzer make:	Thermo 42i	Analyzer serial #:	1426262592

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.9	----	Correlation Coefficient	≥0.995	
800.3	800.0	1.0004			
400.2	398.1	1.0052			
200.1	199.1	1.0049			
			Slope	0.998815	0.90 - 1.10
			Intercept	-0.200000	+/-20

NO Calibration Curve

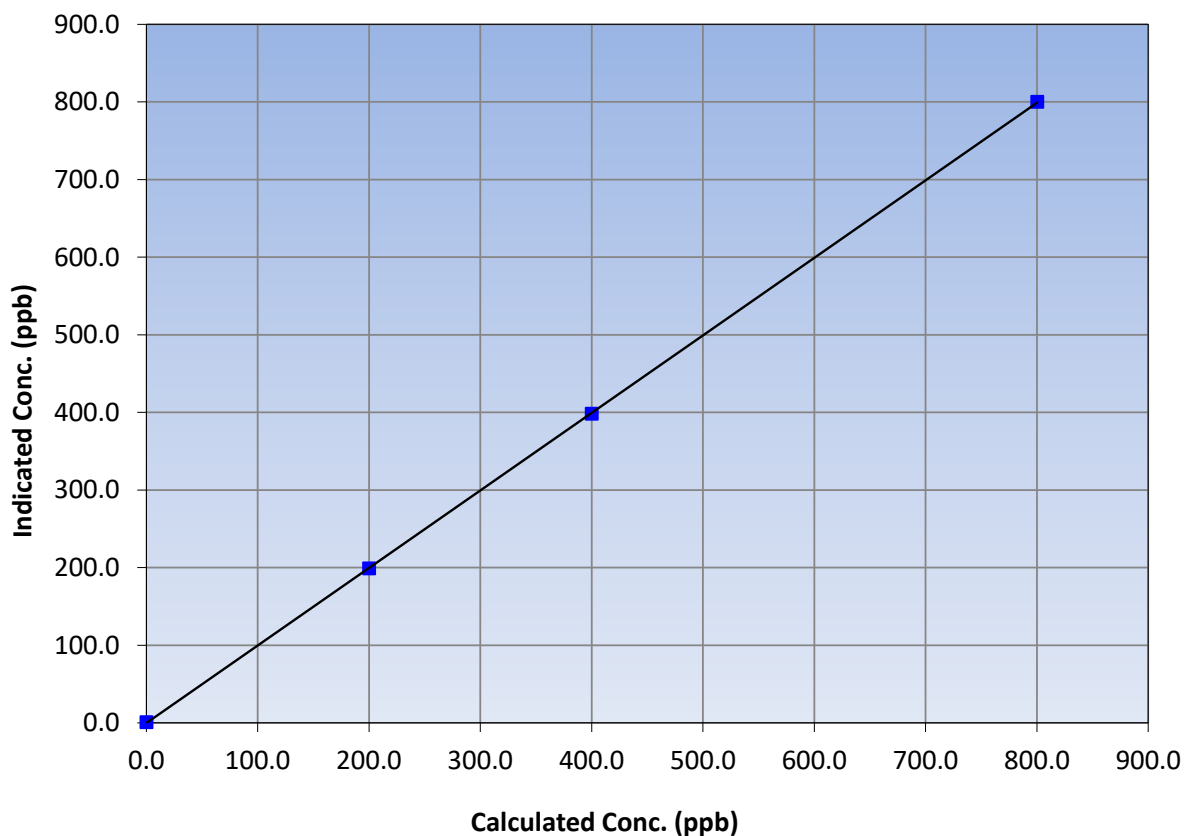



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 5, 2022
Station Name:	Fort Chipewyan	Station Number:	AMS08
Start Time (MST):	10:28	End Time (MST):	15:41
Analyzer make:	Thermo 42i	Analyzer serial #:	1426262592

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
388.2	384.8	1.0088		
194.7	191.3	1.0178		
93.9	91.7	1.0240		


NO₂ Calibration Curve

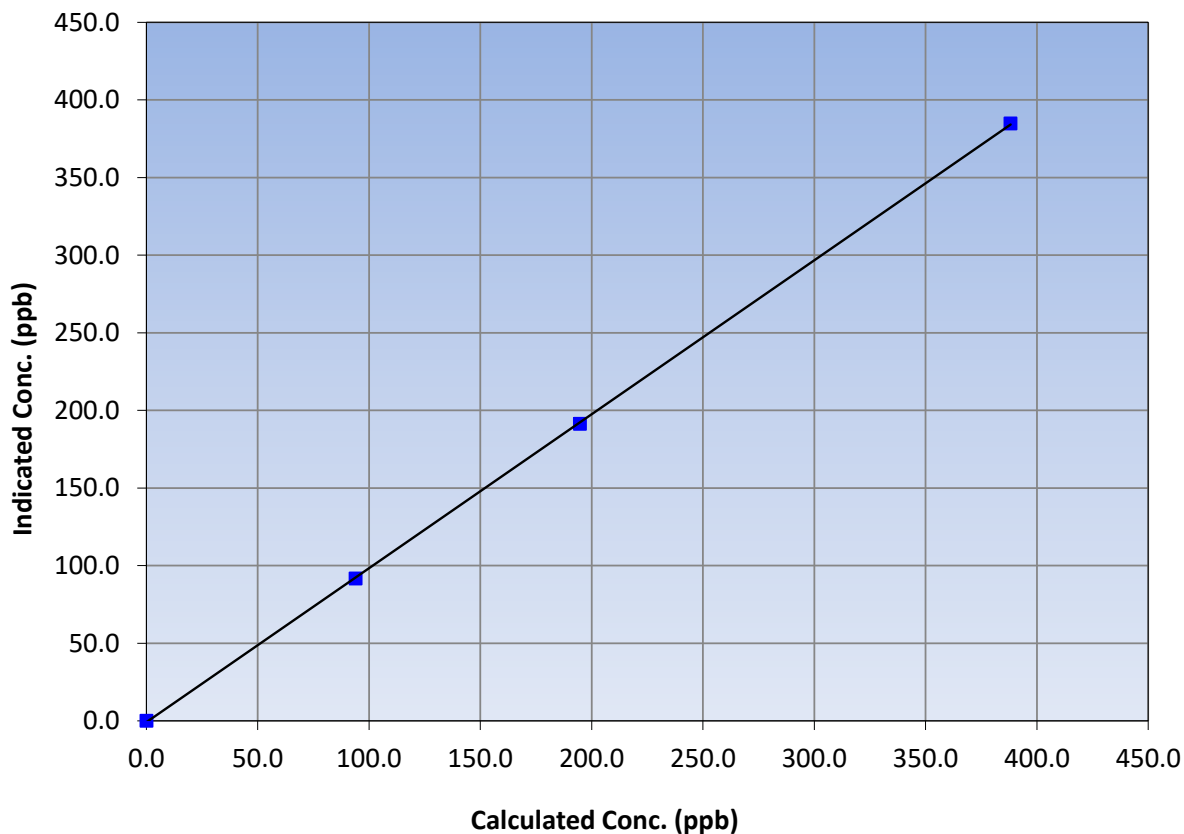

NO_x Calibration Plot

Date: January 10, 2023

Location: Fort Chipewyan

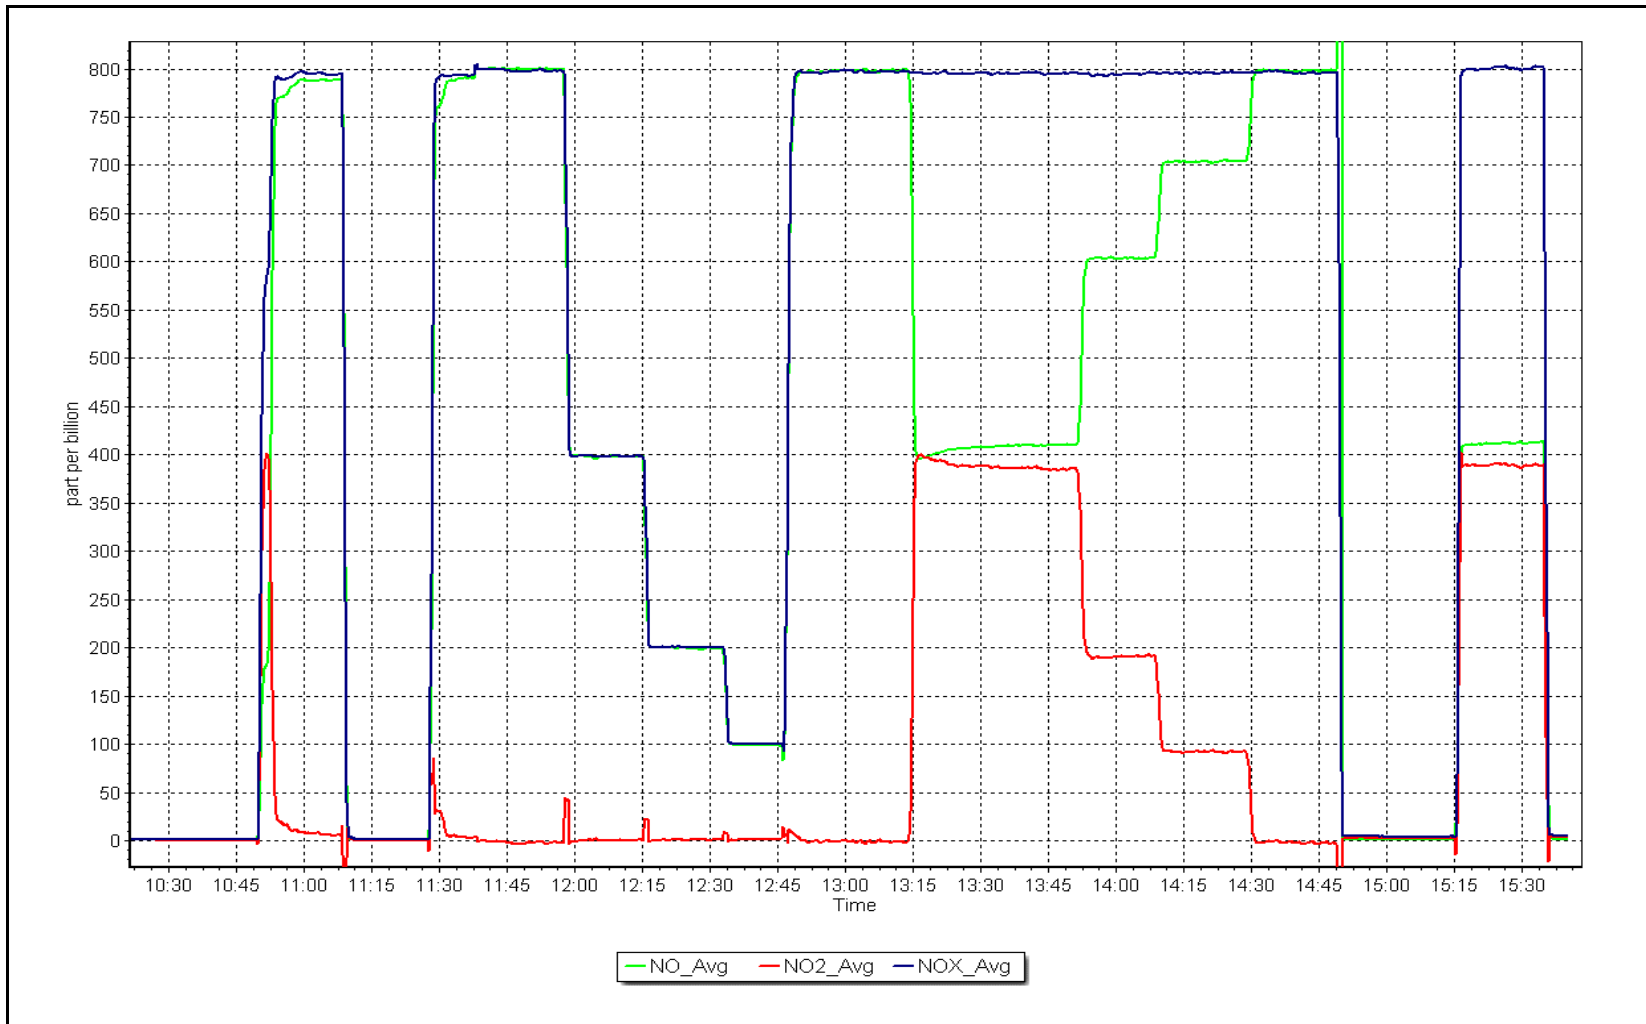



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Fort Chipewyan Station number: AMS08
 Calibration Date: January 10, 2023 Last Cal Date: December 6, 2022
 Start time (MST): 7:47 End time (MST): 10:23
 Reason: Routine

Calibration Standards

O3 generation mode: Photometer
 Calibrator Make/Model: Teledyne API T700 Serial Number: 3252
 ZAG Make/Model: Teledyne API T701 Serial Number: 260

Analyzer Information

Analyzer make: Teledyne API T400 Analyzer serial #: 3872
 Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.009714	1.011486	Backgd or Offset:	-2.0	-2.0
Calibration intercept:	-0.900000	-0.960000	Coeff or Slope:	1.036	1.036

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	NA	0.0	0.3	----
as found span	5000	963.6	400.0	404.6	0.989
as found 2nd point					
as found 3rd point					
calibrator zero	5000	NA	0.0	0.5	----
high point	5000	961.7	400.0	404.4	0.989
second point	5000	810.3	200.0	200.5	0.998
third point	5000	701.3	100.0	98.8	1.012
as left zero	5000	NA	0.0	0.1	----
as left span	5000	963.3	400.0	405.2	0.987
Average Correction Factor					1.000

Baseline Corr As found:	404.3	Previous response	403.0	*% change	0.3%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. No adjustments made.

Calibration Performed By: Morgan Voyageur



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 6, 2022
Station Name:	Fort Chipewyan	Station Number:	AMS08
Start Time (MST):	7:47	End Time (MST):	10:23
Analyzer make:	Teledyne API T400	Analyzer serial #:	3872

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.5	----	Correlation Coefficient	0.999940	≥0.995
400.0	404.4	0.9891			
200.0	200.5	0.9975	Slope	1.011486	0.90 - 1.10
100.0	98.8	1.0121			
			Intercept	-0.960000	+/- 5

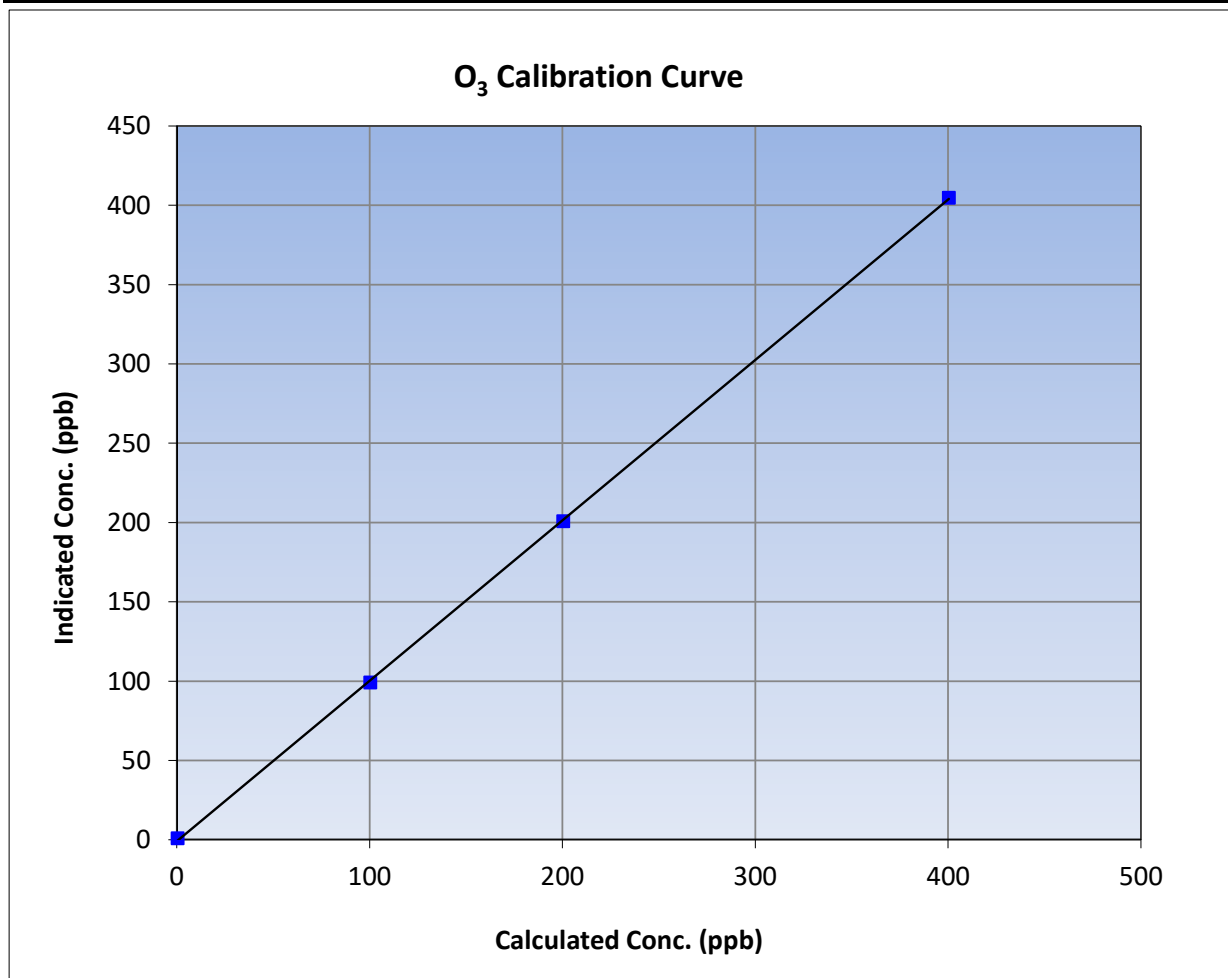

O₃ Calibration Plot

Date: January 10, 2023

Location: Fort Chipewyan

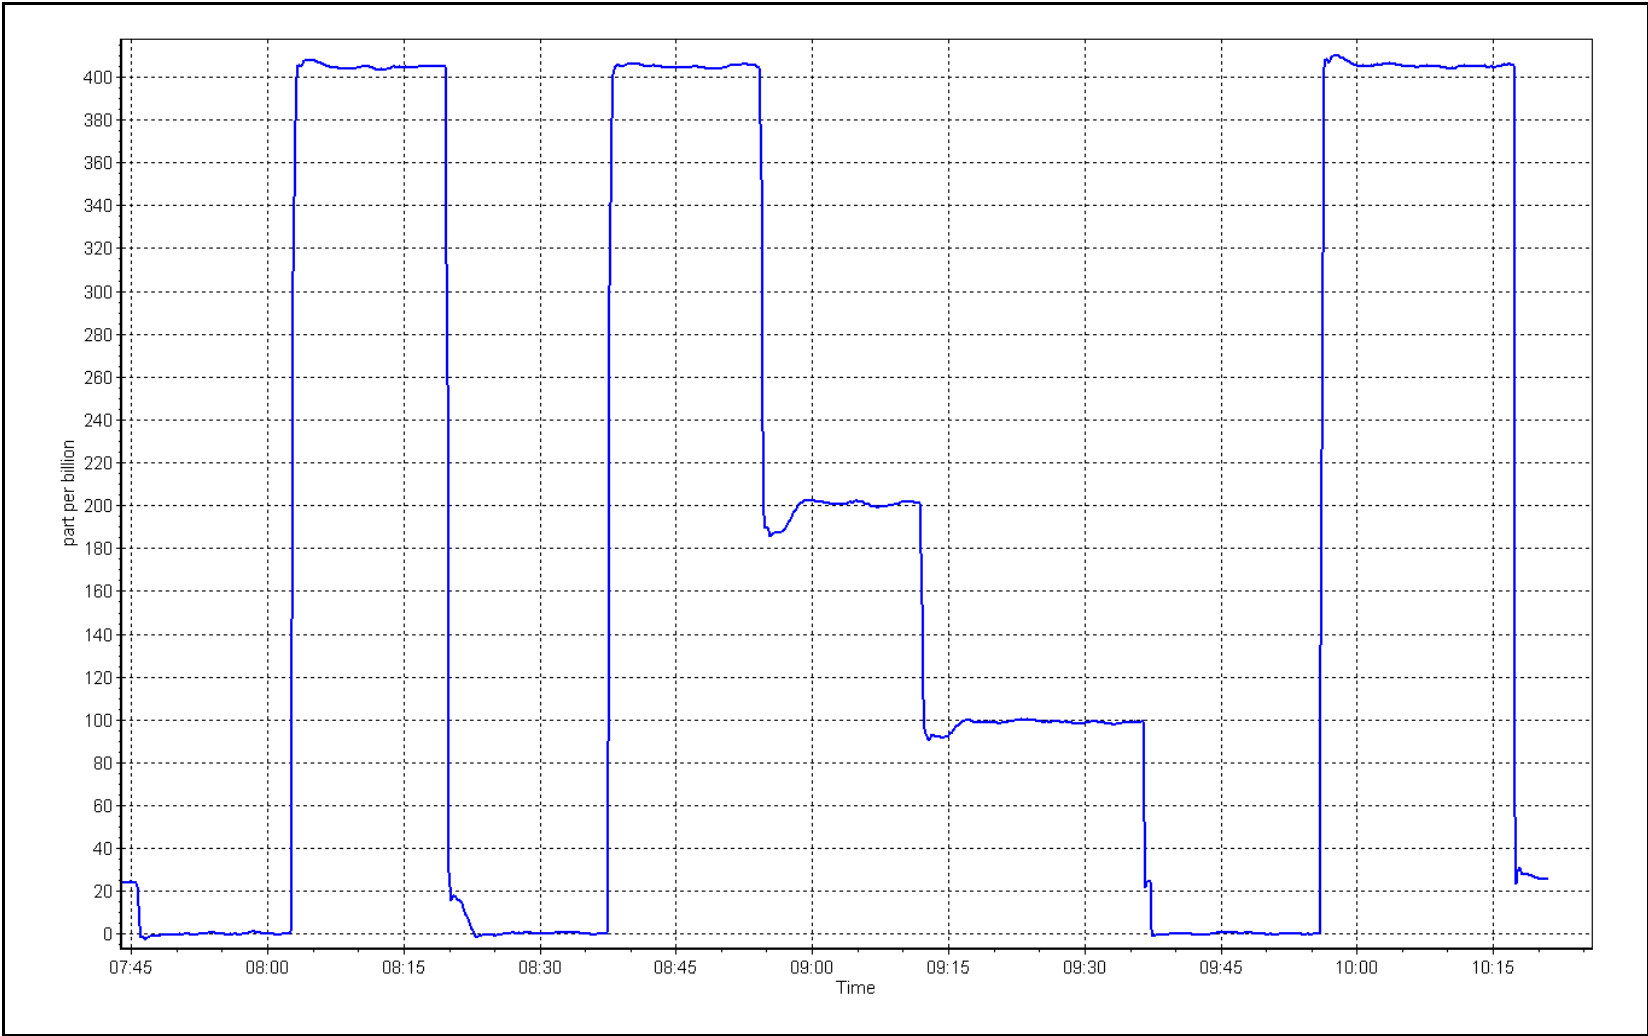

\



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Fort Chipewyan Station number: AMS 08
Calibration Date: January 11, 2023 Last Cal Date: December 5, 2022
Start time (MST): 10:55 End time (MST): 11:33

Analyzer Make: Teledyne API T640 S/N: 216
Particulate Fraction: PM2.5

Flow Meter Make/Model: Delta Cal S/N: 1212
Temp/RH standard: Delta Cal S/N: 1212

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-8.8	-8.8	-8.8	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	740.7	741.8	740.7	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5.05	4.99	5.05	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 11, 2023 Last Cal Date: December 5, 2022
PM w/o HEPA: 2.8 PM w/ HEPA: 0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test				<input type="checkbox"/>	11.1 +/- 0.5

Date Optical Chamber Cleaned: December 5, 2022
Disposable Filter Changed: December 5, 2022

Annual Maintenance

Date Sample Tube Cleaned: July 14, 2022
Date RH/T Sensor Cleaned: July 14, 2022

Notes:

No adjustments made.

Calibration by: Morgan Voyageur



Wood Buffalo Environmental Association

CO Calibration Report

Version-01-2020

Station Information

Station Name:	Fort Chipewyan	Station number:	AMS08
Calibration Date:	January 13, 2023	Last Cal Date:	December 6, 2022
Start time (MST):	10:03	End time (MST):	13:07
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	3,030	ppm	Cal Gas Exp Date:	December 1, 2028
Cal Gas Cylinder #:	ALM014846			
Removed Cal Gas Conc:	3,030	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	5272
ZAG Make/Model:	API T701H		Serial Number:	197

Analyzer Information

Analyzer make:	API T300	Analyzer serial #:	3505
Analyzer Range:	0 - 50 ppm		

	Start	Finish		Start	Finish
Calibration slope:	0.997591	0.995217	Backgd or Offset:	-0.013	-0.013
Calibration intercept:	-0.041052	0.070924	Coeff or Slope:	0.999	0.999

CO Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.05	----
as found span	4933	66.7	40.4	40.3	1.003
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.1	----
high point	4934	66.7	40.4	40.3	1.004
second point	4967	33.3	20.2	20.2	0.998
third point	4983	16.7	10.1	10.1	1.002
as left zero	5000	0.0	0.0	0.1	----
as left span	2960	40.0	40.4	40.2	1.005
Average Correction Factor					1.001

Baseline Corr As found:	40.26	Prev response:	40.28	*% change:	-0.1%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. No adjustments made.

Calibration Performed By: Matthew Courtoreille Morgan V



Wood Buffalo Environmental Association

CO Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 6, 2022
Station Name:	Fort Chipewyan	Station Number:	AMS08
Start Time (MST):	10:03	End Time (MST):	13:07
Analyzer make:	API T300	Analyzer serial #:	3505

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	0.1	----	Correlation Coefficient	0.999992
40.4	40.3	1.0036		
20.2	20.2	0.9980	Slope	0.995217
10.1	10.1	1.0020		
			Intercept	0.070924
				<i>+/-1.5</i>

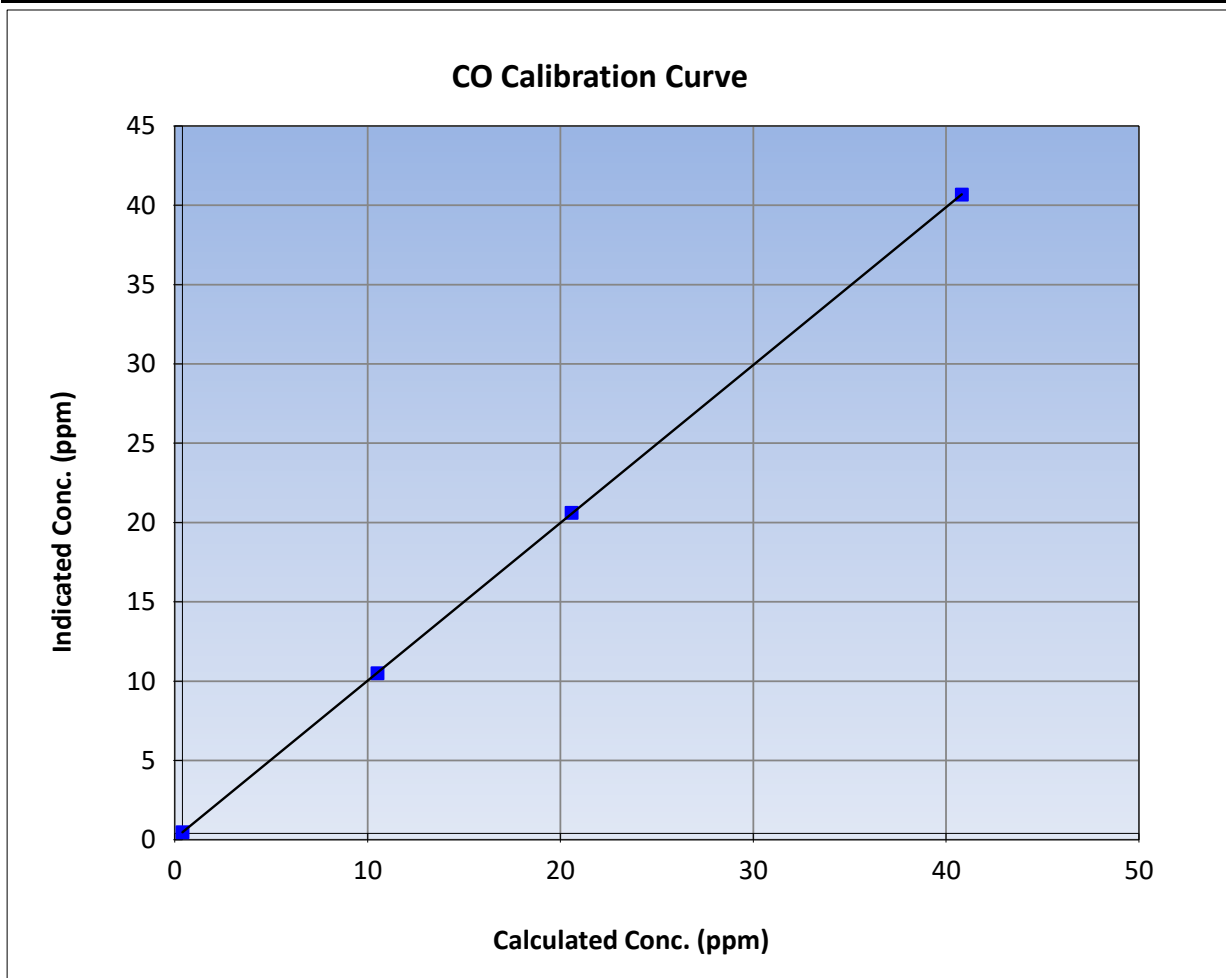

CO Calibration Plot

Date: January 13, 2023

Location: Fort Chipewyan

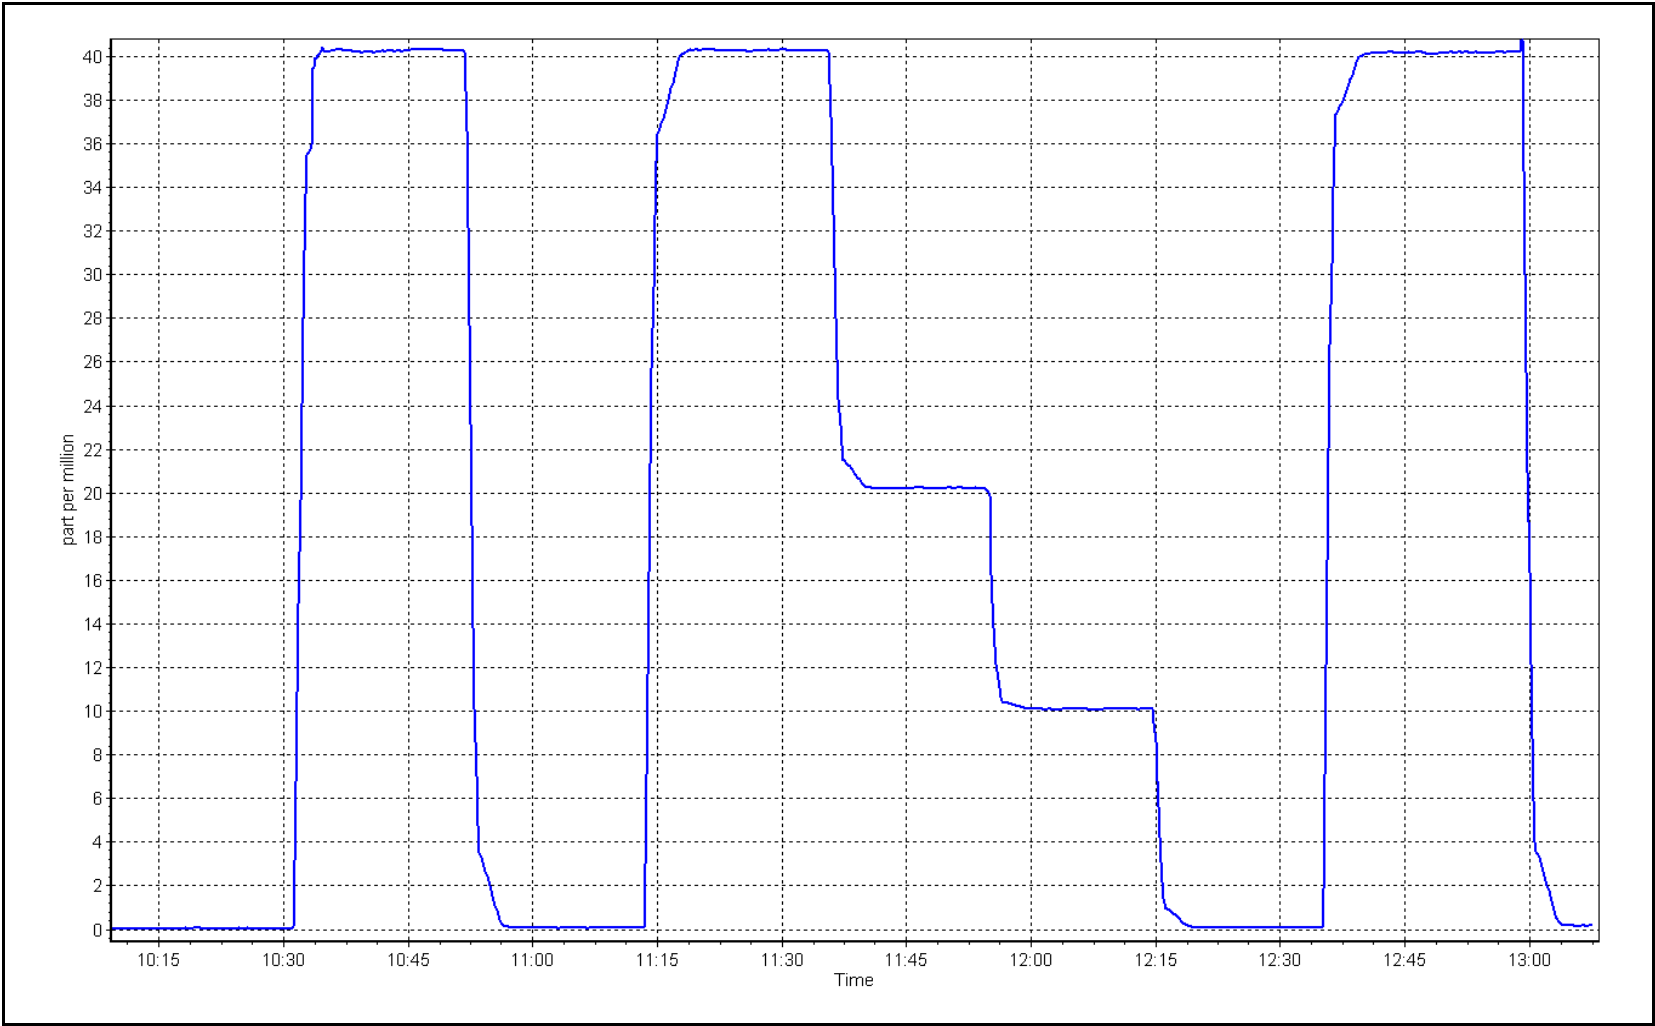



Wood Buffalo Environmental Association

CO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Fort Chipewyan	Station number:	AMS08
Calibration Date:	January 13, 2023	Last Cal Date:	December 6, 2022
Start time (MST):	13:11	End time (MST):	16:56
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	60,220	ppm	Cal Gas Exp Date:	December 1, 2028
Cal Gas Cylinder #:	ALM014846			
Removed Cal Gas Conc:	60,220	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	5272
N2 Gen Make/Model:	NG 5000		Serial Number:	771048318

Analyzer Information

Analyzer make: Teledyne API T360 Analyzer serial #: 289
 Analyzer Range 0 - 2,000 ppm

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.998681	0.998112	Backgd or Offset:	0.019	0.019
Calibration intercept:	-5.440000	-5.540000	Coeff or Slope:	1.007	1.011

CO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	3000	0.0	0.0	-0.2	----
as found span	2920	80.0	1605.9	1574.9	1.020
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	3000	0.0	0.0	0.1	----
high point	2920	80.0	1605.9	1604.1	1.001
second point	2960	40.0	802.9	781.1	1.028
third point	2980	20.0	401.5	397.5	1.010
as left zero	3000	0.0	0.0	-0.3	----
as left span	2960	40.0	802.9	778.5	1.031
Average Correction Factor					1.013

Baseline Corr As found:	1575.10	Prev response:	1598.31	*% change:	-1.5%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. Adjusted the span only.

Calibration Performed By: Matthew Courtoreille Morgan V



Wood Buffalo Environmental Association

CO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date	January 13, 2023	Previous Calibration	December 6, 2022
Station Name	Fort Chipewyan	Station Number	AMS08
Start Time (MST)	13:11	End Time (MST)	16:56
Analyzer make	Teledyne API T360	Analyzer serial #	289

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.1	----	Correlation Coefficient	0.999785	≥0.995
1605.9	1604.1	1.0011	Slope	0.998112	0.90 - 1.10
802.9	781.1	1.0280	Intercept	-5.540000	+/-20
401.5	397.5	1.0100			

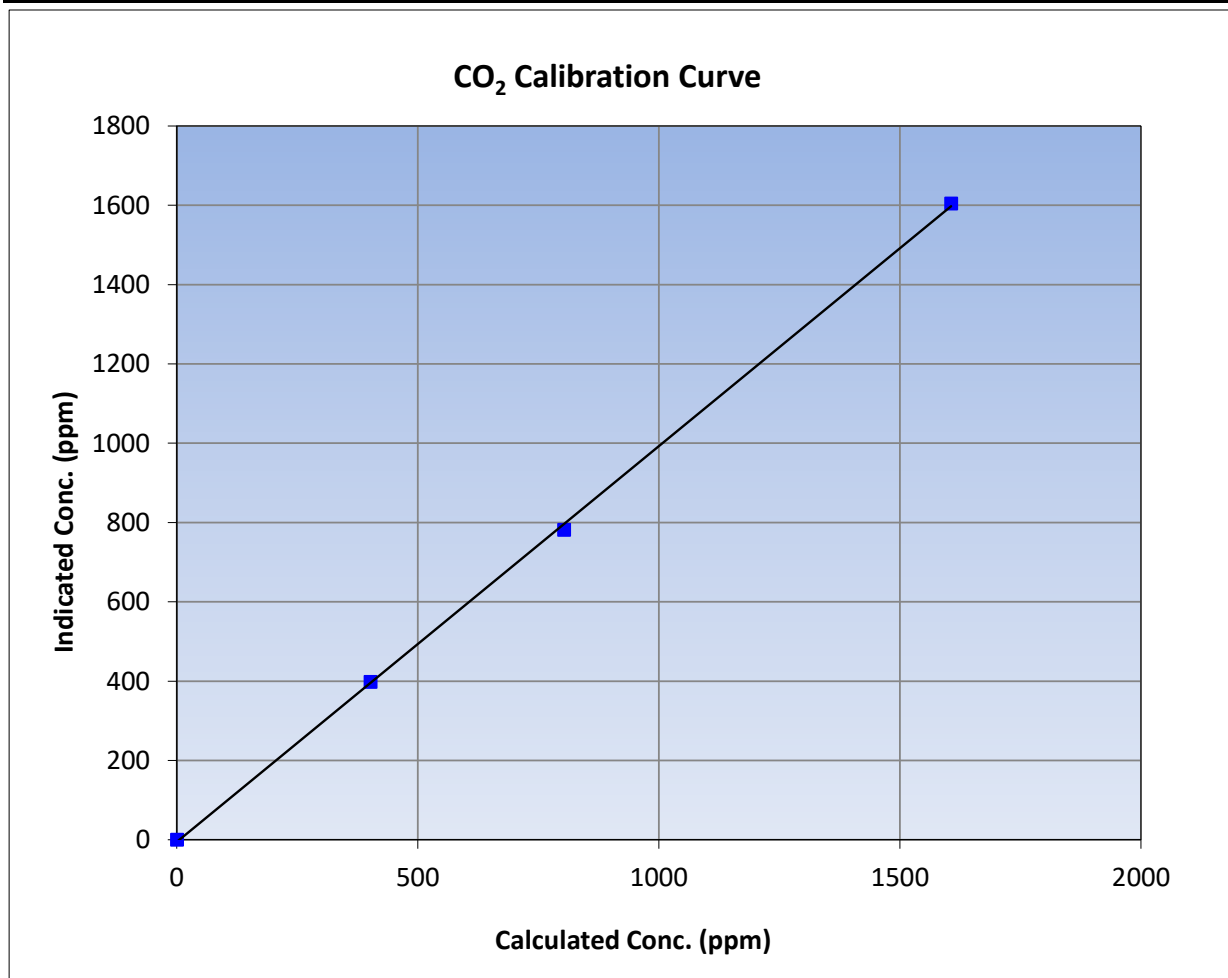

CO₂ Calibration Plot

Date: January 13, 2023

Location: Fort Chipewyan

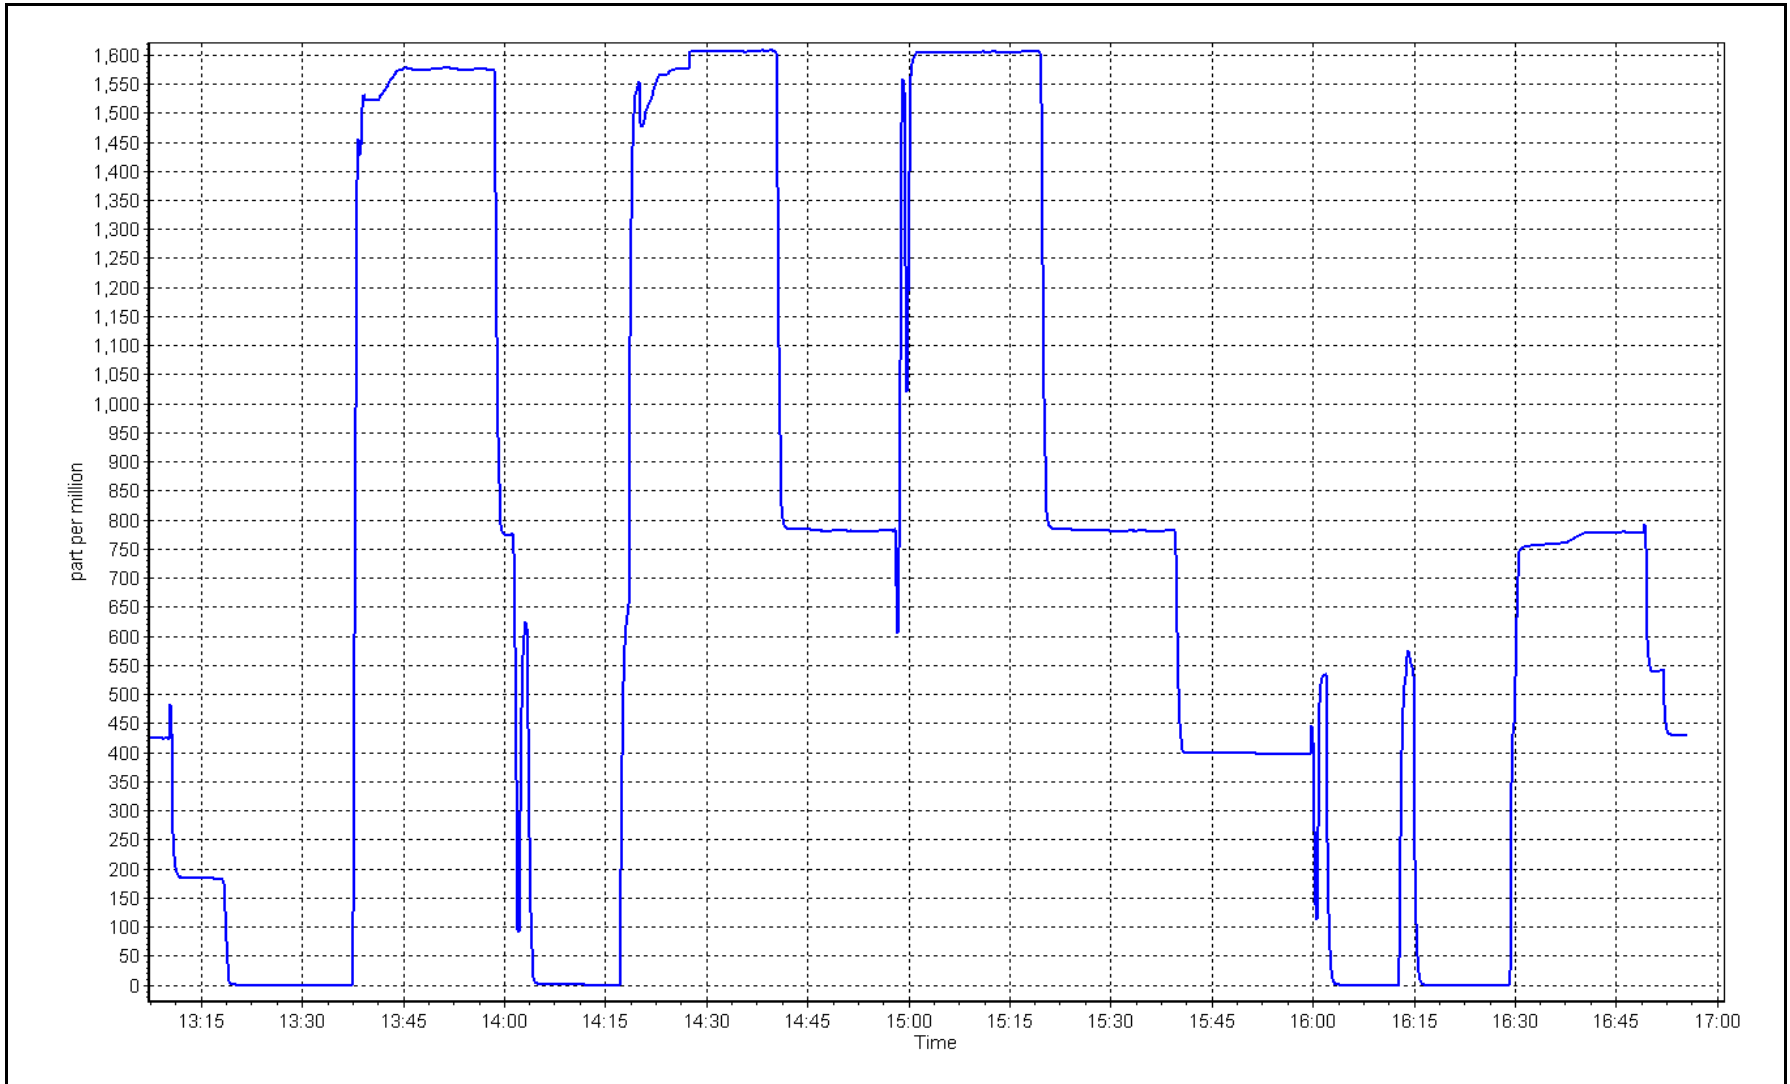



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS09 BARGE LANDING JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Barge Landing	Station number:	AMS09
Calibration Date:	January 13, 2023	Last Cal Date:	December 12, 2022
Start time (MST):	9:50	End time (MST):	13:51
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.96	ppm	Cal Gas Exp Date:	January 5, 2025
Cal Gas Cylinder #:	CC151285			
Removed Cal Gas Conc:	49.96	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	3812
ZAG Make/Model:	API T701		Serial Number:	4888

Analyzer Information

Analyzer make: Thermo 43i
 Analyzer Range 0 - 1000 ppb
 Analyzer serial #: 1118148498

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.997747	0.994624	Backgd or Offset:	9.6	9.8
Calibration intercept:	-0.329817	-0.310040	Coeff or Slope:	0.986	0.986

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.3	----
as found span	4919	80.2	801.5	796.3	1.007
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.3	----
high point	4919	80.2	801.5	797.5	1.005
second point	4959	40.1	400.8	397.0	1.009
third point	4980	20.0	199.8	198.5	1.007
as left zero	5000	0.0	0.0	0.3	----
as left span	4919	80.2	801.5	796.9	1.006
Average Correction Factor					1.007

Baseline Corr As found:	796.00	Previous response	799.35	*% change	-0.4%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed sample inlet filter after as founds. No adjustments made.

Calibration Performed By: Braiden Boutilier



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 12, 2022
Station Name:	Barge Landing	Station Number:	AMS09
Start Time (MST):	9:50	End Time (MST):	13:51
Analyzer make:	Thermo 43i	Analyzer serial #:	1118148498

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	0.999993	≥0.995
801.5	797.5	1.0050			
400.8	397.0	1.0094	Slope	0.994624	0.90 - 1.10
199.8	198.5	1.0068			
			Intercept	-0.310040	+/-30

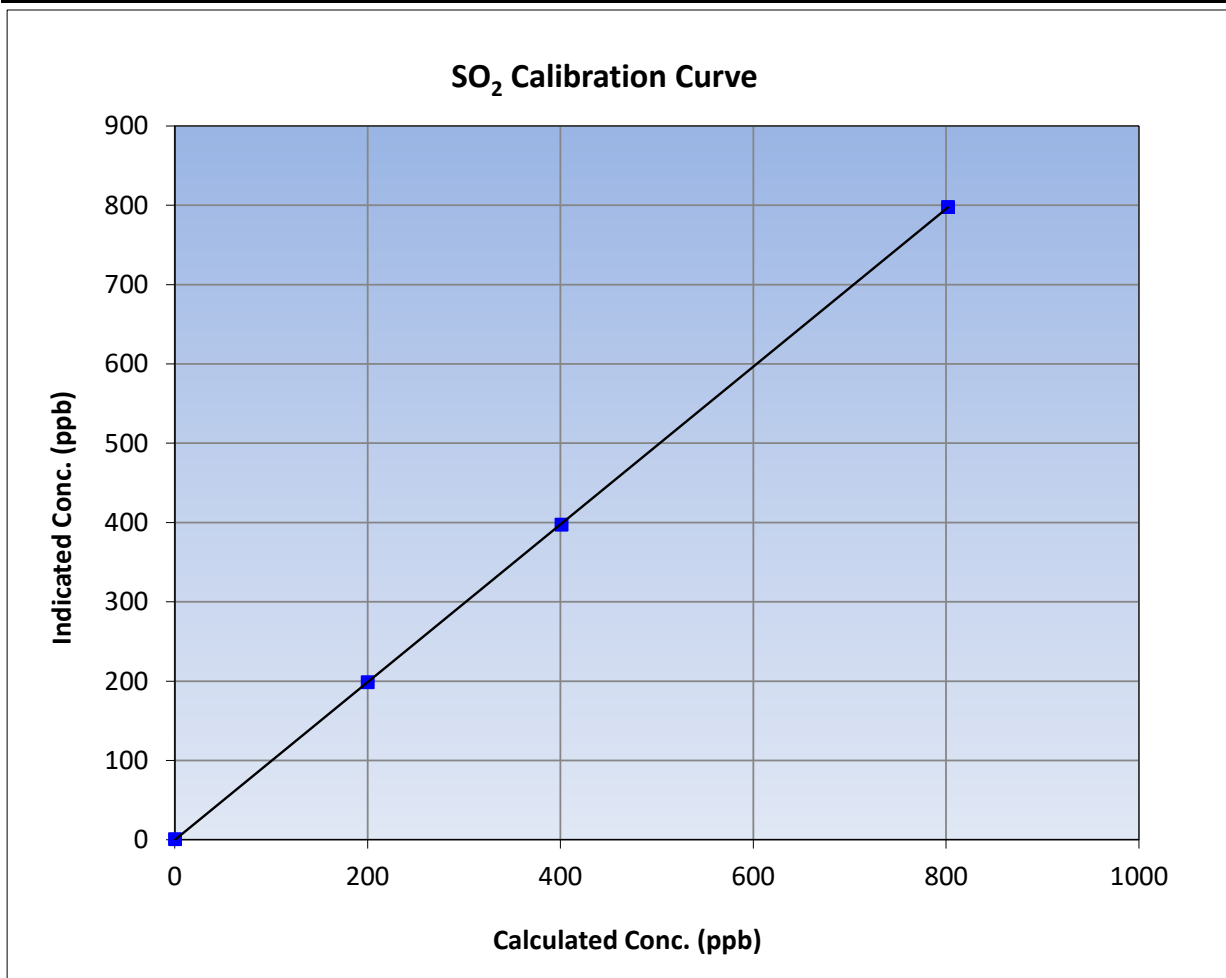

SO2 Calibration Plot

Date: January 13, 2023

Location: Barge Landing

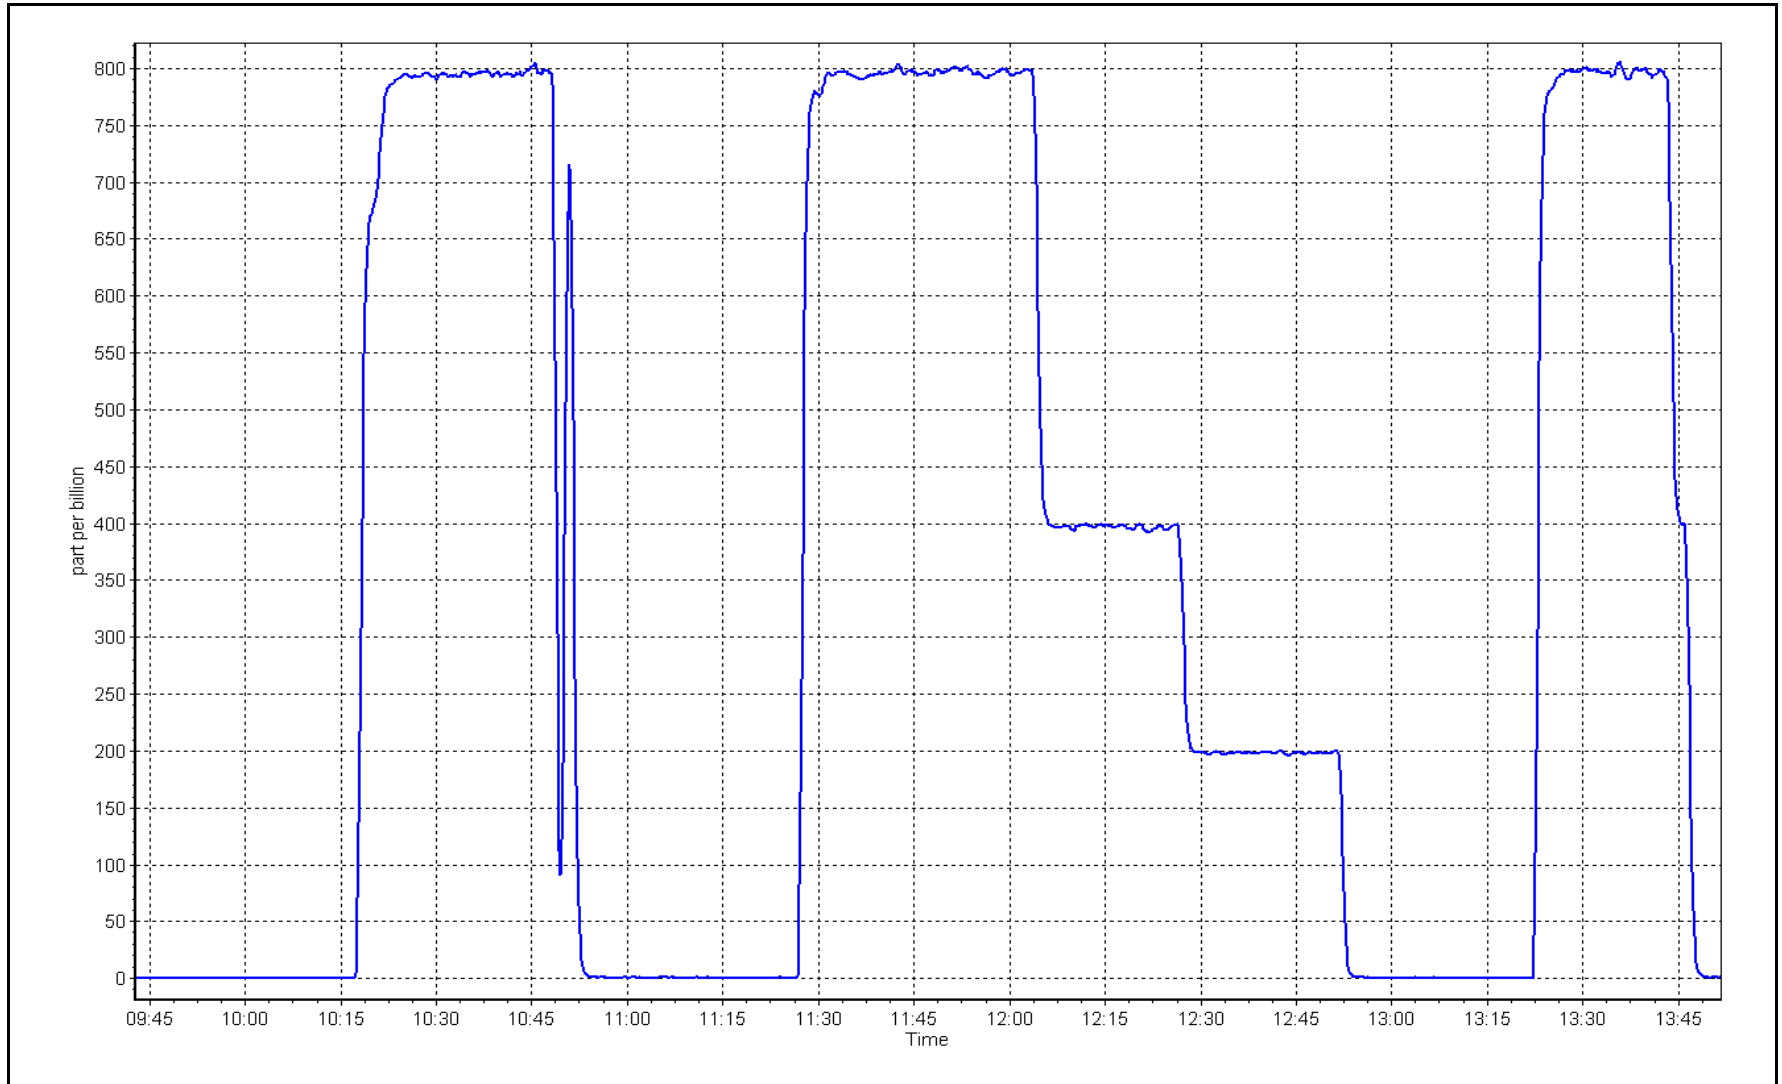



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name: Barge Landing Station number: AMS09
 Calibration Date: January 23, 2023 Last Cal Date: December 20, 2022
 Start time (MST): 11:31 End time (MST): 16:01
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 4.87 ppm Cal Gas Exp Date: September 2, 2024
 Cal Gas Cylinder #: EY0002346
 Removed Cal Gas Conc: 4.87 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 3812
 ZAG Make/Model: API T701 Serial Number: 4888

Analyzer Information

Analyzer make: Thermo 43i-TLE Analyzer serial #: 1331259320
 Converter make: CDN-101 Converter serial #: 519
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.999432	1.003148	Backgd or Offset: 2.46	2.52
Calibration intercept:	0.079028	-0.000990	Coeff or Slope: 1.084	1.091

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.0	----
as found span	4918	82.1	80.0	78.5	1.019
as found 2nd point	4959	41.1	40.0	39.4	1.016
as found 3rd point	4979	20.5	20.0	19.7	1.014
new cylinder response					

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.0	----
high point	4918	82.1	80.0	80.2	0.997
second point	4959	41.1	40.0	40.2	0.996
third point	4979	20.5	20.0	20.0	0.998
as left zero	5000	0.0	0.0	0.1	----
as left span	4918	82.1	80.0	80.4	0.995
SO2 Scrubber Check	4920	80.2	802.0	0.1	----
Date of last scrubber change:				Ave Corr Factor	0.997
Date of last converter efficiency test:				efficiency	

Baseline Corr As found: 78.5 Prev response: 80.00 *% change: -1.9%
 Baseline Corr 2nd AF pt: 39.4 AF Slope: 0.981427 AF Intercept: 0.059042
 Baseline Corr 3rd AF pt: 19.7 AF Correlation: 0.999997

* = > +/-5% change initiates investigation

Notes: Changed sample inlet filters after as founds. Small span adjustment made.

Calibration Performed By: Braiden Boutillier



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 23, 2023	Previous Calibration:	December 20, 2022
Station Name:	Barge Landing	Station Number:	AMS09
Start Time (MST):	11:31	End Time (MST):	16:01
Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1331259320

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.0	----	Correlation Coefficient	≥ 0.995
80.0	80.2	0.9971		
40.0	40.2	0.9958	Slope	0.90 - 1.10
20.0	20.0	0.9984		
			Intercept	+/-3

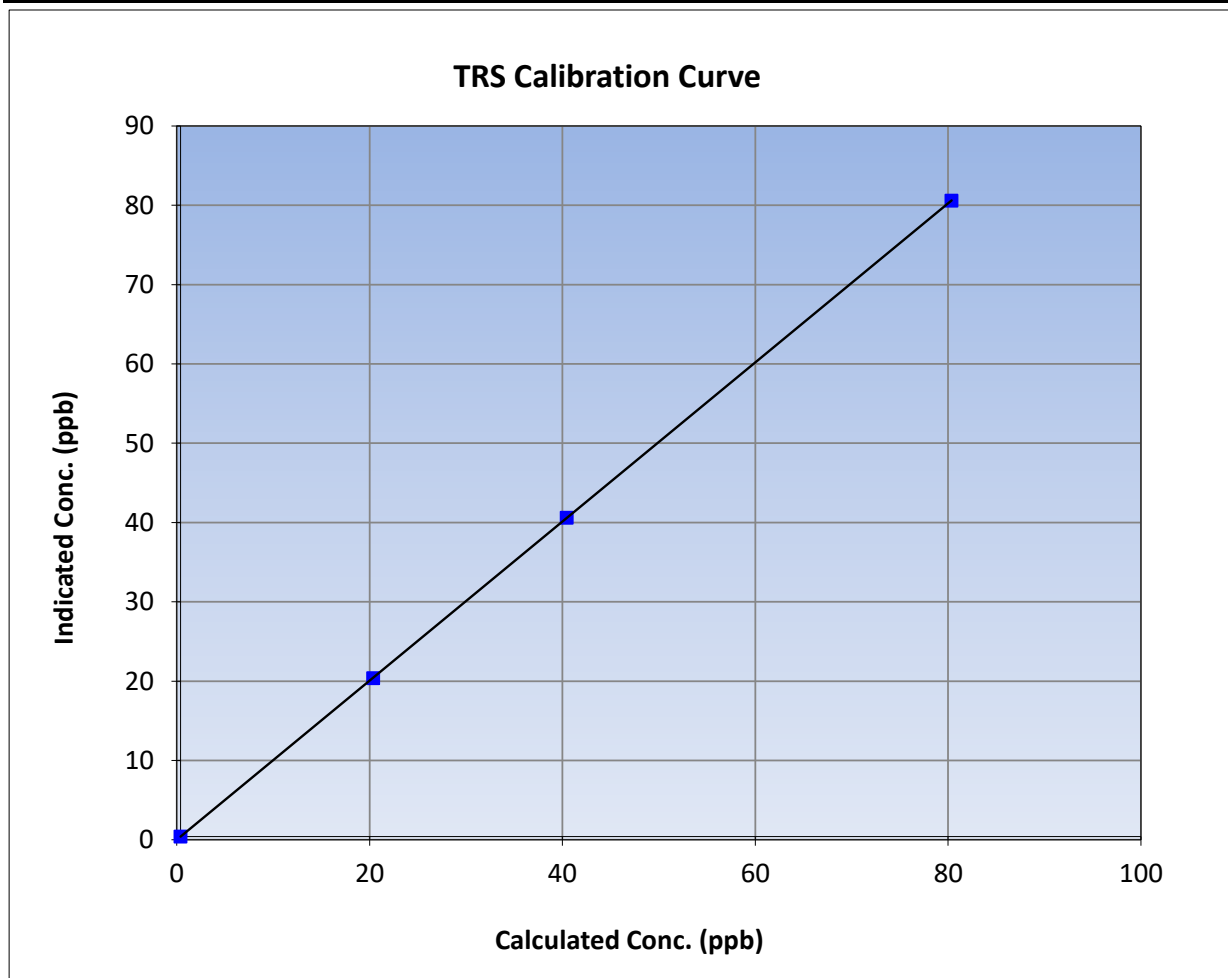

TRS Calibration Plot

Date: January 23, 2023

Location: Barge Landing

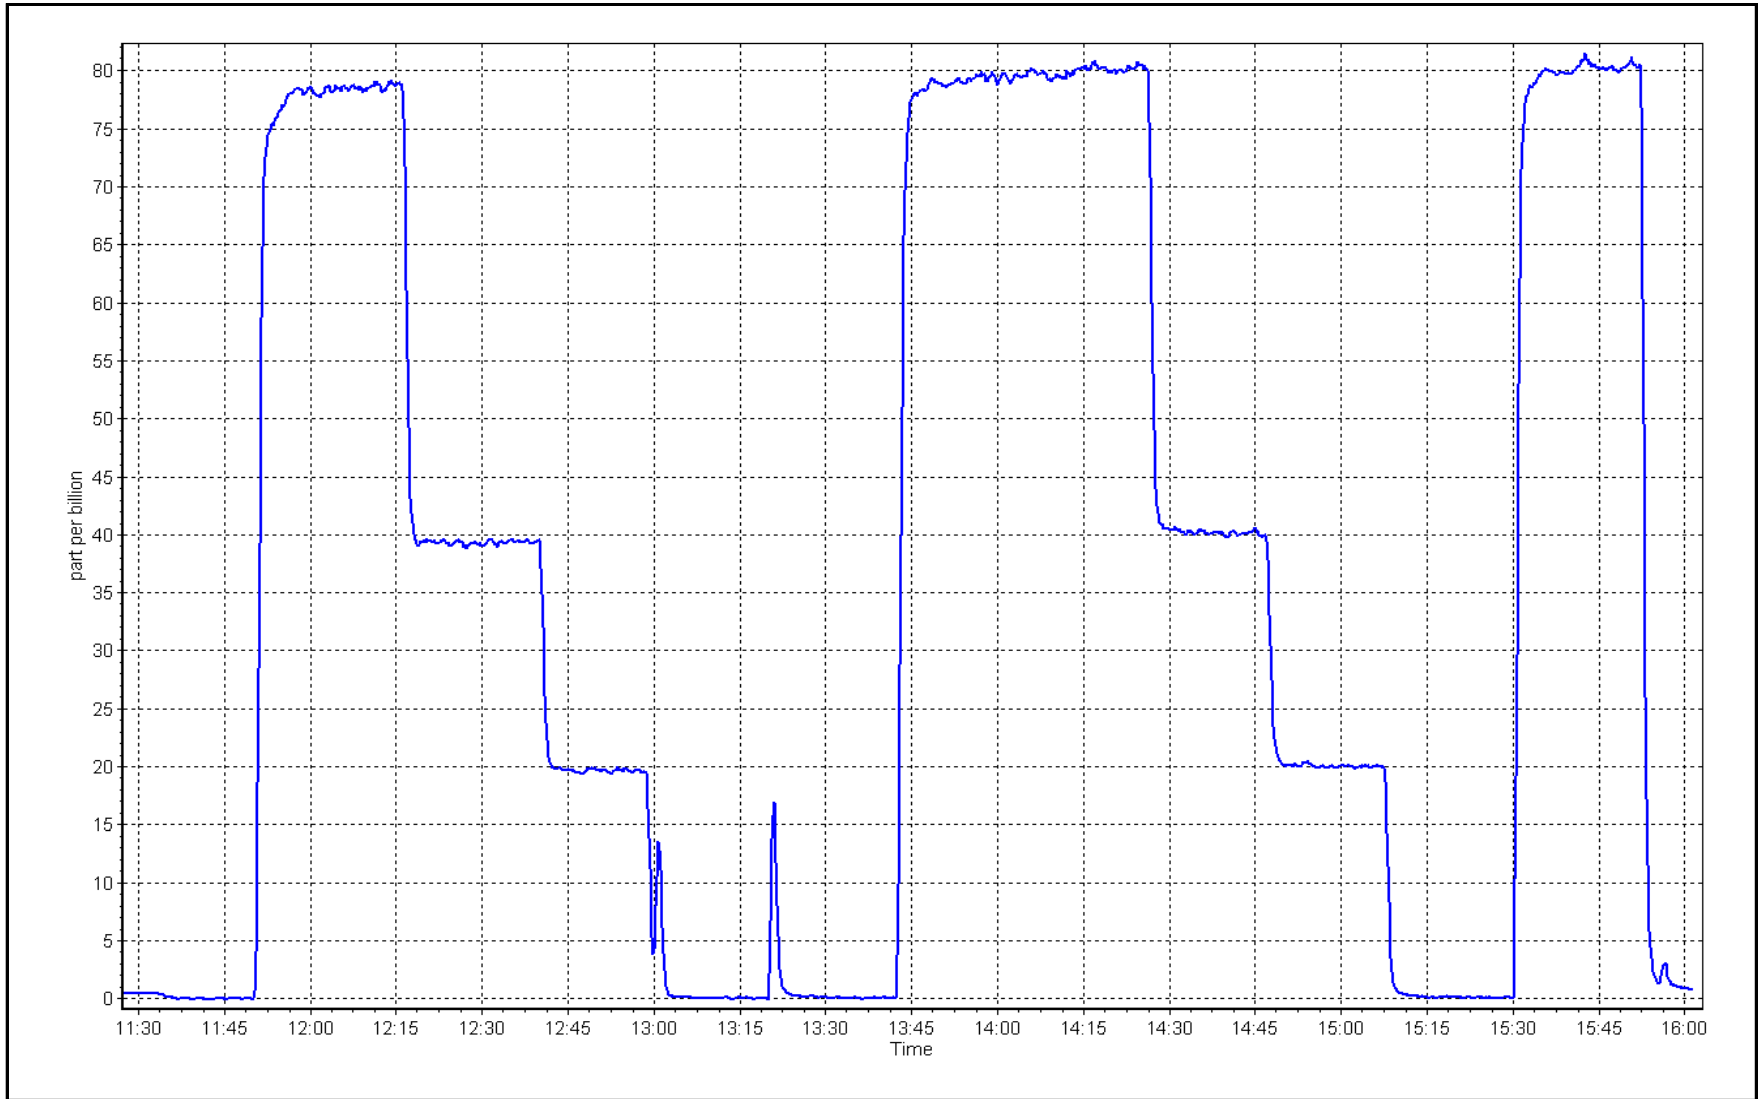



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Barge Landing	Station number:	AMS09
Calibration Date:	January 13, 2023	Last Cal Date:	December 13, 2022
Start time (MST):	9:50	End time (MST):	13:51
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC151285	Cal Gas Expiry Date:	January 5, 2025
CH ₄ Cal Gas Conc.	497.6 ppm	CH ₄ Equiv Conc.	1067.1 ppm
C ₃ H ₈ Cal Gas Conc.	207.1 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	497.6 ppm	CH ₄ Equiv Conc.	1067.1 ppm
Removed C ₃ H ₈ Conc.	207.1 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	3812
ZAG make/model:	API T701	Serial Number:	4888

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1170050131
THC Range (ppm):	0 - 100 ppm		
NMHC Range (ppm):	0 - 50 ppm	CH ₄ Range (ppm):	0 - 50 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	1.96E-04	1.99E-04	NMHC SP Ratio:	4.31E-05
CH ₄ Retention time:	12.00	12.2	NMHC Peak Area:	212118
				213327

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4919	80.2	17.12	17.03	1.005
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4919	80.2	17.12	17.15	0.998
second point	4960	40.1	8.56	8.45	1.013
third point	4980	20.0	4.27	4.19	1.019
as left zero	5000	0.0	0.00	0.00	----
as left span	4919	80.2	17.12	17.05	1.004

Average Correction Factor				1.010
Baseline Corr AF:	17.03	Prev response	17.02	*% change 0.1%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.0	----
as found span	4919	80.2	9.14	9.21	0.992
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4919	80.2	9.14	9.17	0.996
second point	4960	40.1	4.57	4.54	1.007
third point	4980	20	2.28	2.25	1.013
as left zero	5000	0	0.00	0.00	----
as left span	4919	80.2	9.14	9.13	1.001
Average Correction Factor					1.005
Baseline Corr AF:	9.21	Prev response	9.16	*% change	0.6%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4919	80.2	7.98	7.81	1.022
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4919	80.2	7.98	7.98	1.000
second point	4960	40.1	3.99	3.91	1.021
third point	4980	20.0	1.99	1.94	1.025
as left zero	5000	0.0	0.00	0.00	----
as left span	4919	80.2	7.98	7.92	1.008
Average Correction Factor					1.016
Baseline Corr AF:	7.81	Prev response	7.86	*% change	-0.6%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	0.995340	1.002709
THC Cal Offset:	-0.022383	-0.059558
CH ₄ Cal Slope:	0.985022	1.000454
CH ₄ Cal Offset:	-0.004175	-0.035549
NMHC Cal Slope:	1.004429	1.004517
NMHC Cal Offset:	-0.018008	-0.024610

Notes: Changed sample inlet filter after as founds. Adjusted span.

Calibration Performed By: Braiden Boutillier



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 13, 2022
Station Name:	Barge Landing	Station Number:	AMS09
Start Time (MST):	9:50	End Time (MST):	13:51
Analyzer make:	Thermo 55i	Analyzer serial #:	1170050131

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999928	≥ 0.995
17.12	17.15	0.9982			
8.56	8.45	1.0128			
4.27	4.19	1.0190			
			Slope	1.002709	0.90 - 1.10
			Intercept	-0.059558	+/-0.5

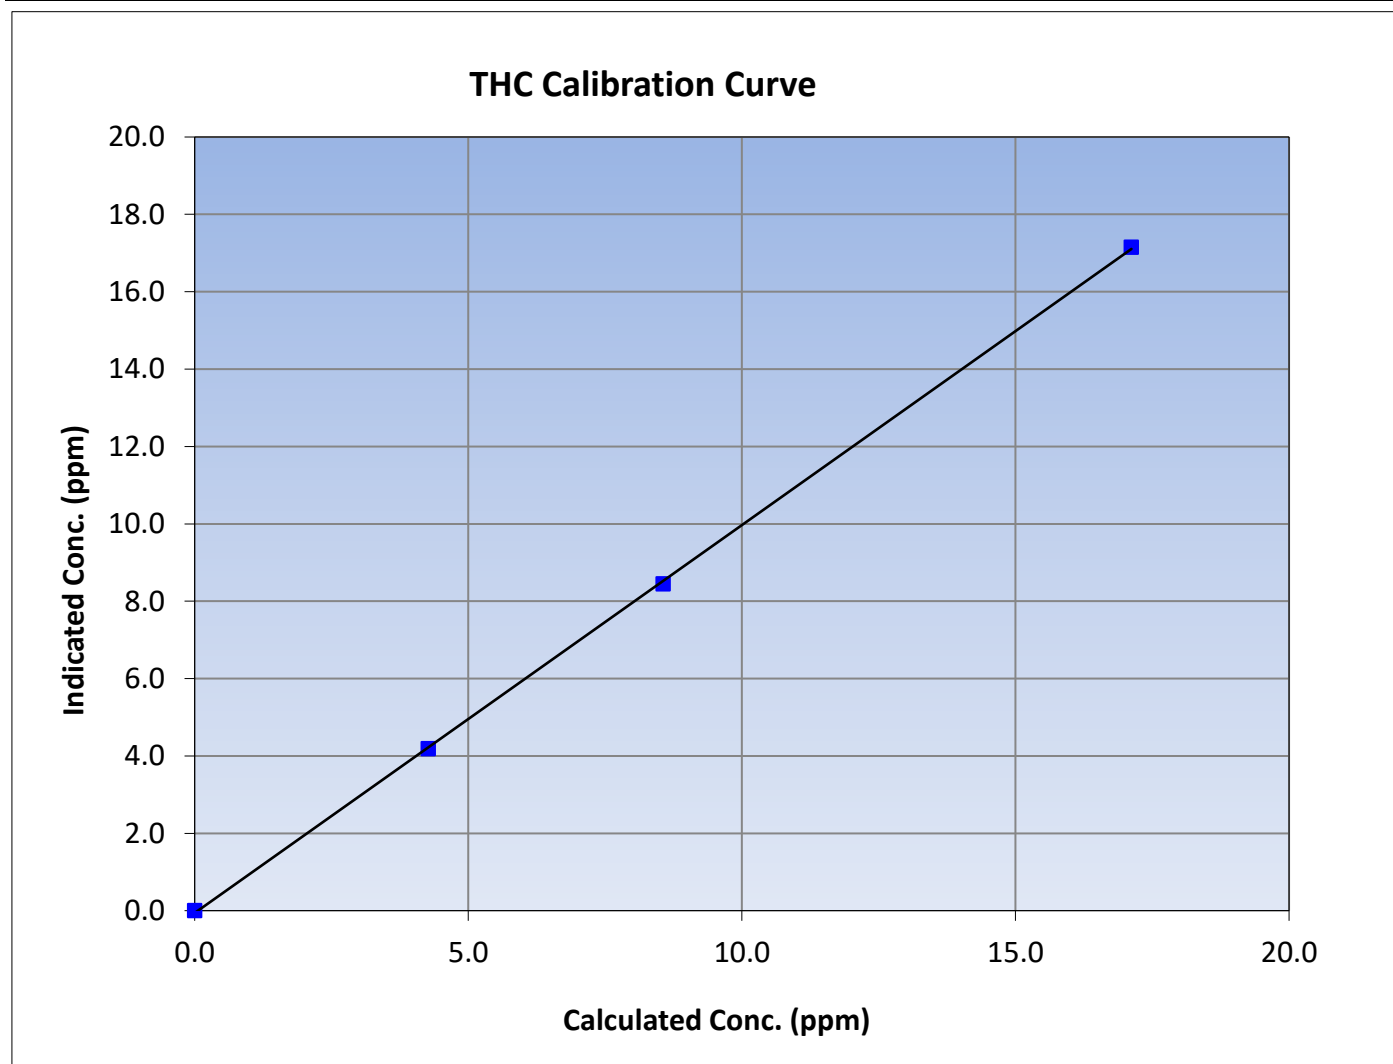



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 13, 2022
Station Name:	Barge Landing	Station Number:	AMS09
Start Time (MST):	9:50	End Time (MST):	13:51
Analyzer make:	Thermo 55i	Analyzer serial #:	1170050131

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999866	≥ 0.995
7.98	7.98	1.0005			
3.99	3.91	1.0212			
1.99	1.94	1.0255			
			Slope	1.000454	0.90 - 1.10
			Intercept	-0.035549	+/-0.5

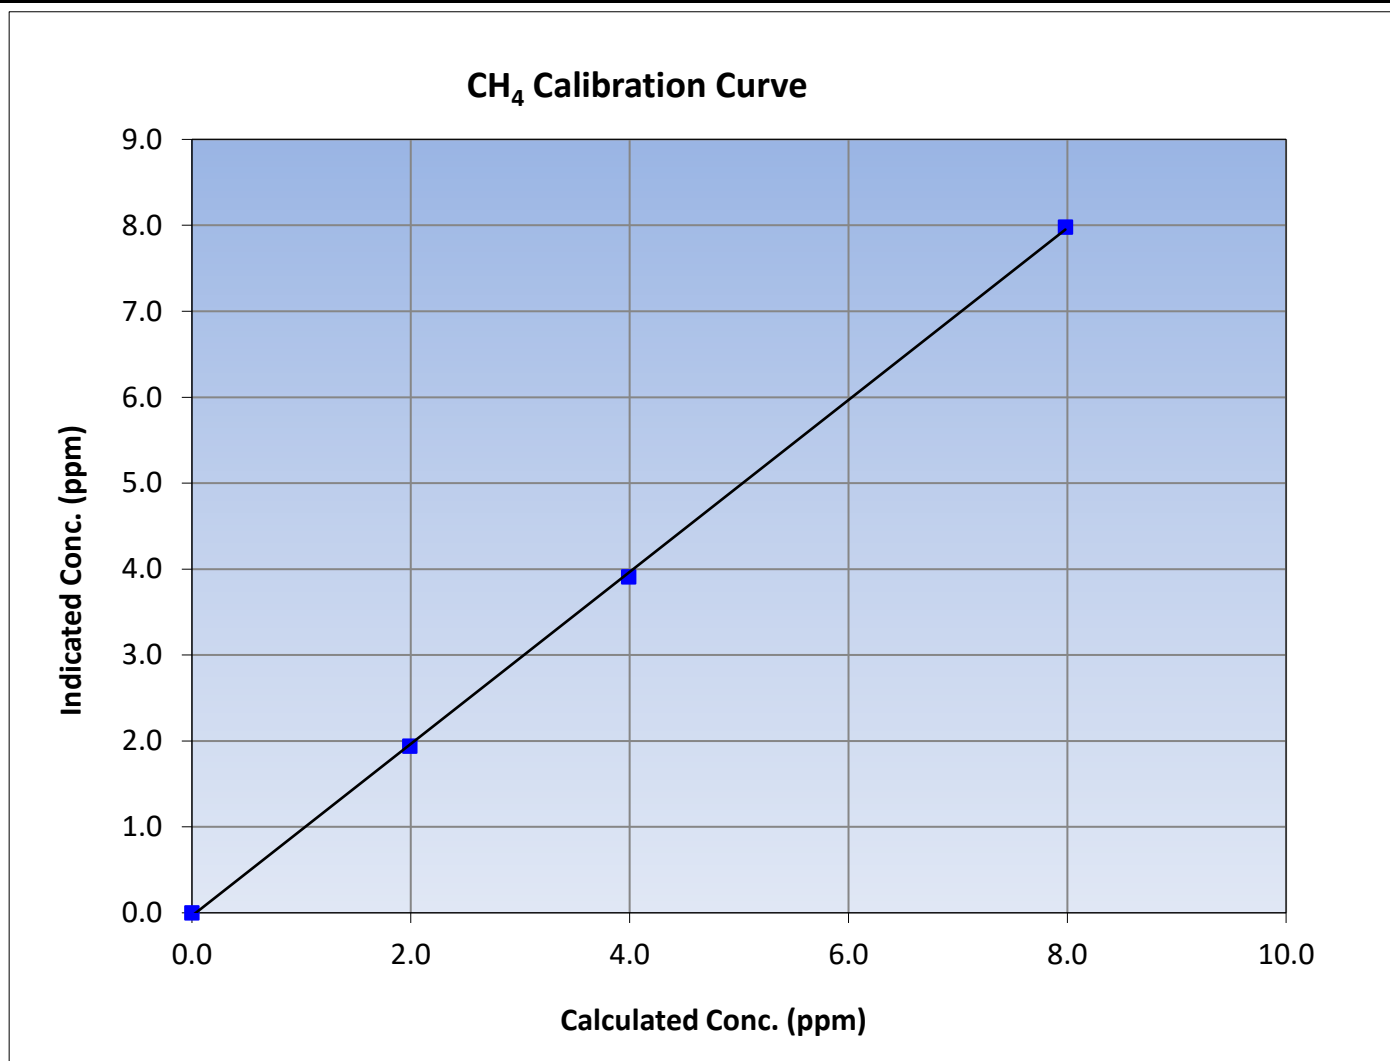



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 13, 2022
Station Name:	Barge Landing	Station Number:	AMS09
Start Time (MST):	9:50	End Time (MST):	13:51
Analyzer make:	Thermo 55i	Analyzer serial #:	1170050131

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999961	≥ 0.995			
9.14	9.17	0.9964						
4.57	4.54	1.0065				Slope	1.004517	0.90 - 1.10
2.28	2.25	1.0134						
			Intercept	-0.024610	± 0.5			

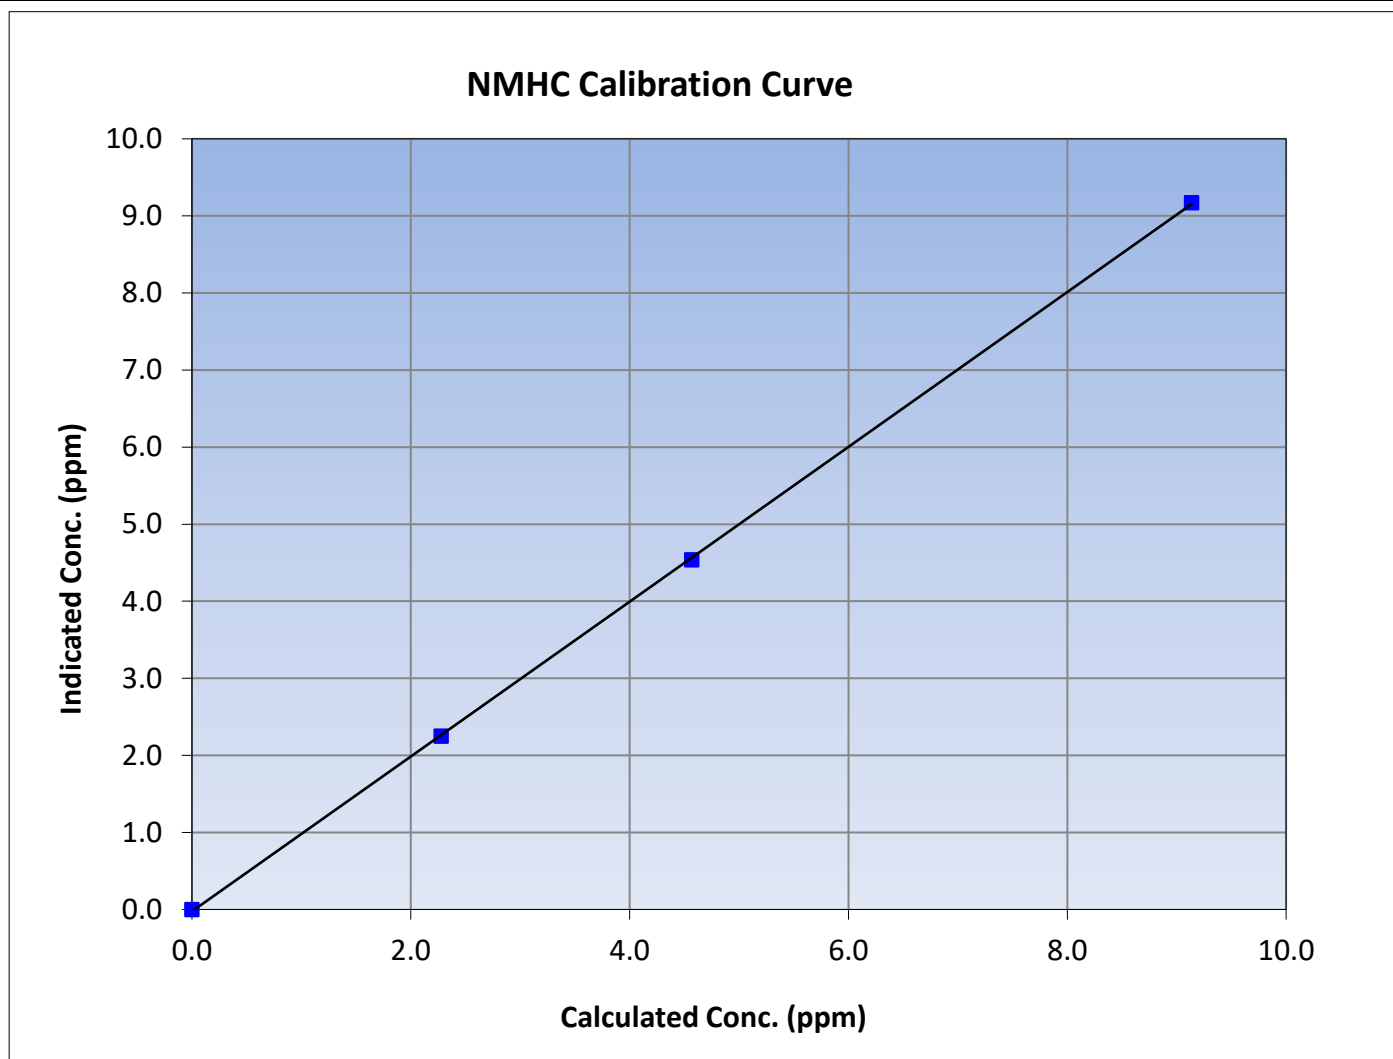

NMHC Calibration Plot

Date: January 13, 2023

Location: Barge Landing

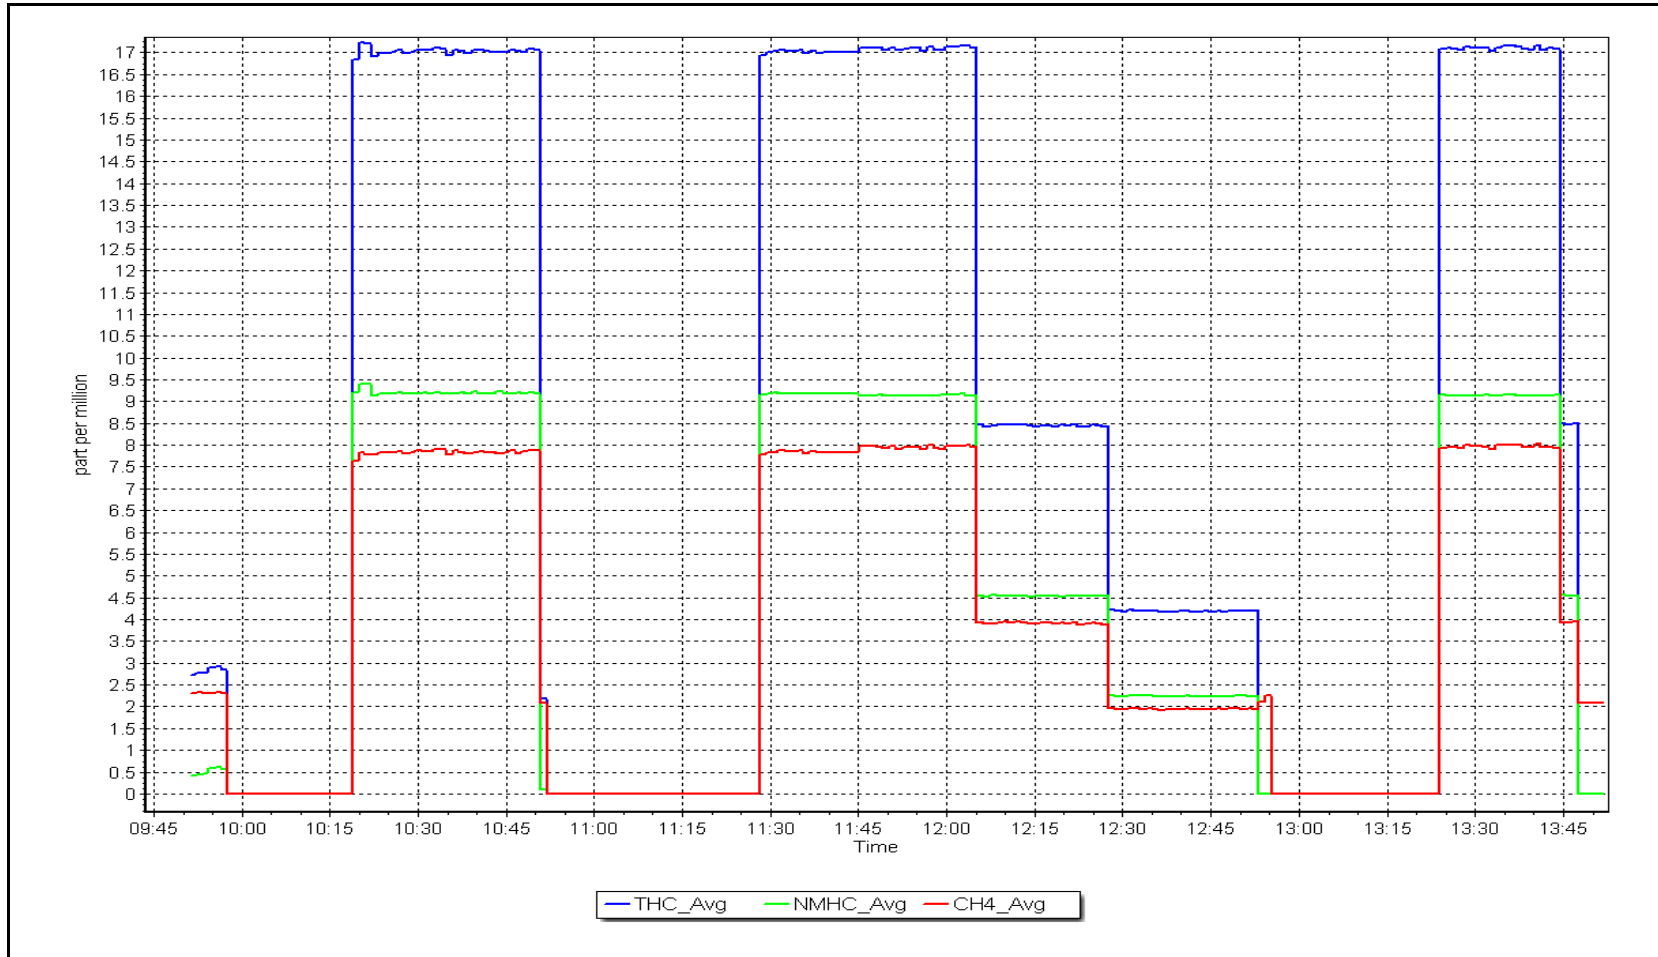



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Barge Landing
Calibration Date: January 20, 2023
Start time (MST): 10:52
Reason: Routine
Station number: AMS09
Last Cal Date: December 22, 2022
End time (MST): 15:46

Calibration Standards

NO Gas Cylinder #: DT0036634
NOX Cal Gas Conc: 50.00 ppm
Removed Cylinder #: NA
Removed Gas NOX Conc: 50.00 ppm
NOX gas Diff:
Calibrator Model: API T700
ZAG make/model: API T701
Cal Gas Expiry Date: January 28, 2024
NO Cal Gas Conc: 49.70 ppm
Removed Gas Exp Date: NA
Removed Gas NO Conc: 49.70 ppm
NO gas Diff:
Serial Number: 3812
Serial Number: 4888

Analyzer Information

Analyzer make: Thermo 42i
NOX Range (ppb): 0 - 1000 ppb

Analyzer serial #: 1426262593

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.164	1.182	NO bkgnd or offset:	10.4	10.6
NOX coeff or slope:	0.997	0.996	NOX bkgnd or offset:	10.5	10.6
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	178.6	172.5

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.020387	0.998369
NO _x Cal Offset:	0.452747	0.728922
NO Cal Slope:	1.019892	0.997899
NO Cal Offset:	-0.569015	-0.272767
NO ₂ Cal Slope:	1.003188	1.000917
NO ₂ Cal Offset:	-0.637715	0.473394



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-0.1	-0.1	0.0	----	----
as found span	4919	80.5	805.1	800.3	4.8	795.8	787.6	8.2	1.012	1.016
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.1	0.1	0.0	----	----
high point	4919	80.5	805.1	800.3	4.8	804.0	798.3	5.8	1.001	1.002
second point	4959	40.2	402.1	399.7	2.4	403.0	398.9	4.1	0.998	1.002
third point	4979	20.1	201.0	199.8	1.2	201.7	198.4	3.3	0.997	1.007
as left zero	5000	0.0	0.0	0.0	0.0	0.1	0.1	0.1	----	----
as left span	4919	80.5	805.1	447.7	357.4	803.0	445.1	357.8	1.003	1.006
Average Correction Factor									0.999	1.004

Corrected As found	NO _x = 795.9 ppb	NO = 787.7 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -3.3%	
Previous Response	NO _x = 821.9 ppb	NO = 815.6 ppb		*Percent Change	NO = -3.5%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO ₂)						
as found GPT point (200 ppb NO ₂)						
as found GPT point (100 ppb NO ₂)						
1st GPT point (400 ppb O ₃)	796.5	443.9	357.4	357.9	0.999	100.1%
2nd GPT point (200 ppb O ₃)	796.5	667.4	133.9	135.5	0.988	101.2%
3rd GPT point (100 ppb O ₃)	796.5	731.1	70.2	70.6	0.995	100.5%
Average Correction Factor					0.994	100.6%

Notes: Sample inlet filter changed after as founds. Adjusted span.

Calibration Performed By: Braiden Boutilier



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 22, 2022
Station Name:	Barge Landing	Station Number:	AMS09
Start Time (MST):	10:52	End Time (MST):	15:46
Analyzer make:	Thermo 42i	Analyzer serial #:	1426262593

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.1	----	Correlation Coefficient	≥0.995	
805.1	804.0	1.0013			
402.1	403.0	0.9977			
201.0	201.7	0.9967			
			Slope	0.998369	0.90 - 1.10
			Intercept	0.728922	+/-20

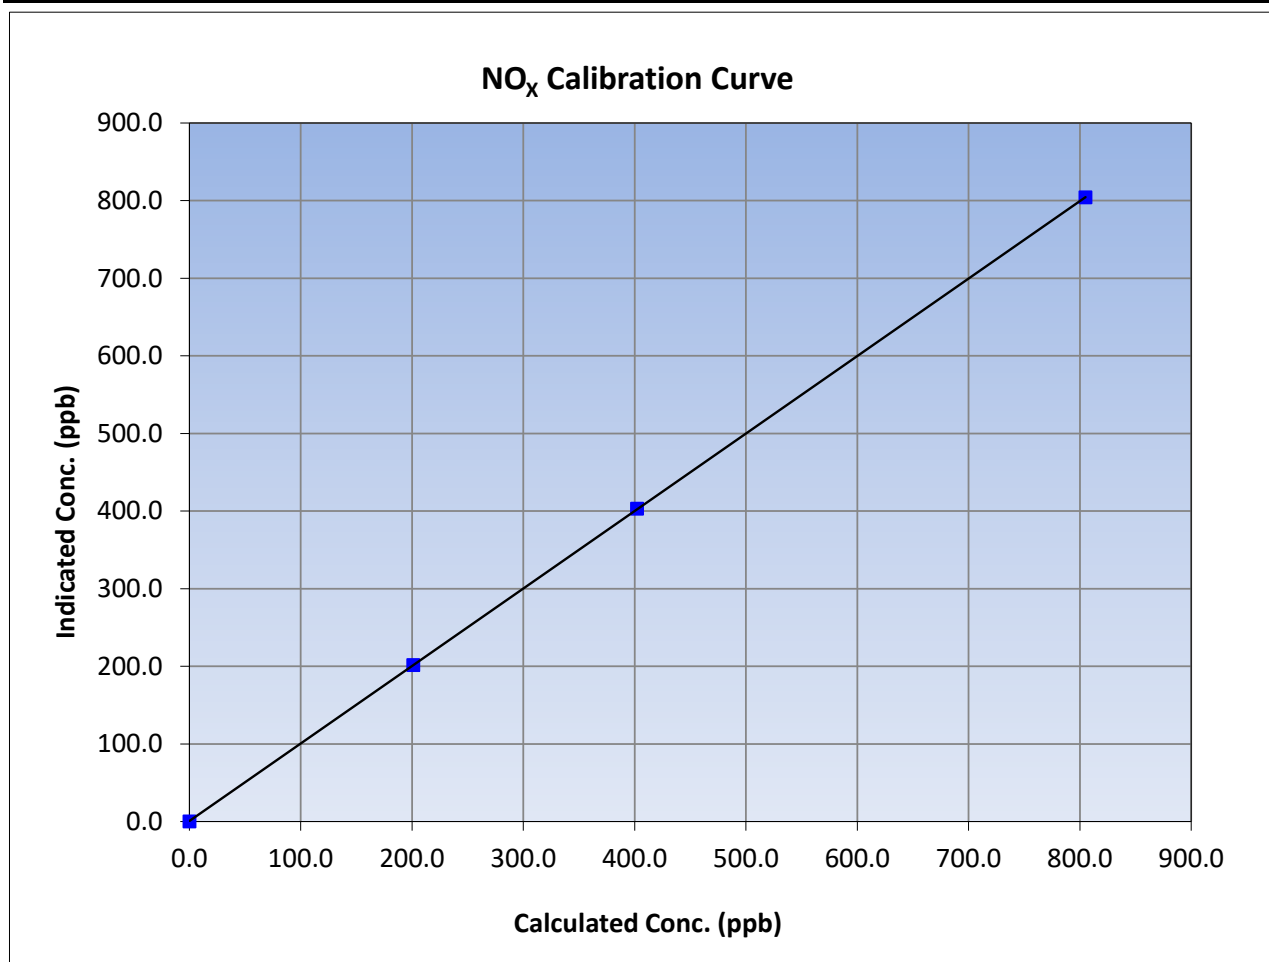



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 22, 2022
Station Name:	Barge Landing	Station Number:	AMS09
Start Time (MST):	10:52	End Time (MST):	15:46
Analyzer make:	Thermo 42i	Analyzer serial #:	1426262593

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.1	----	Correlation Coefficient	≥0.995	
800.3	798.3	1.0024			
399.7	398.9	1.0019			
199.8	198.4	1.0072			
			Slope	0.997899	0.90 - 1.10
			Intercept	-0.272767	+/-20

NO Calibration Curve

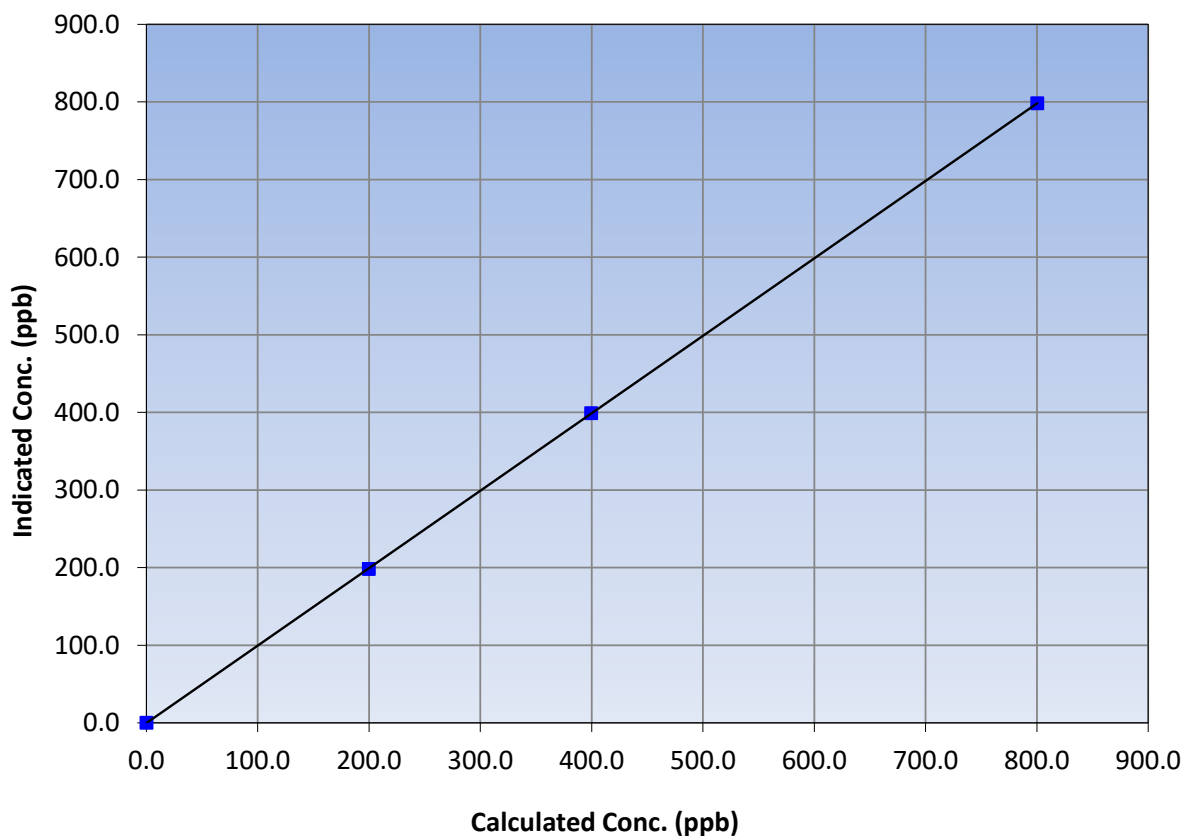



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 22, 2022
Station Name:	Barge Landing	Station Number:	AMS09
Start Time (MST):	10:52	End Time (MST):	15:46
Analyzer make:	Thermo 42i	Analyzer serial #:	1426262593

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		Limits
0.0	0.0	----	Correlation Coefficient	0.999982	≥0.995
357.4	357.9	0.9987			
133.9	135.5	0.9884			
70.2	70.6	0.9948			
			Slope	1.000917	0.90 - 1.10
			Intercept	0.473394	+/-20

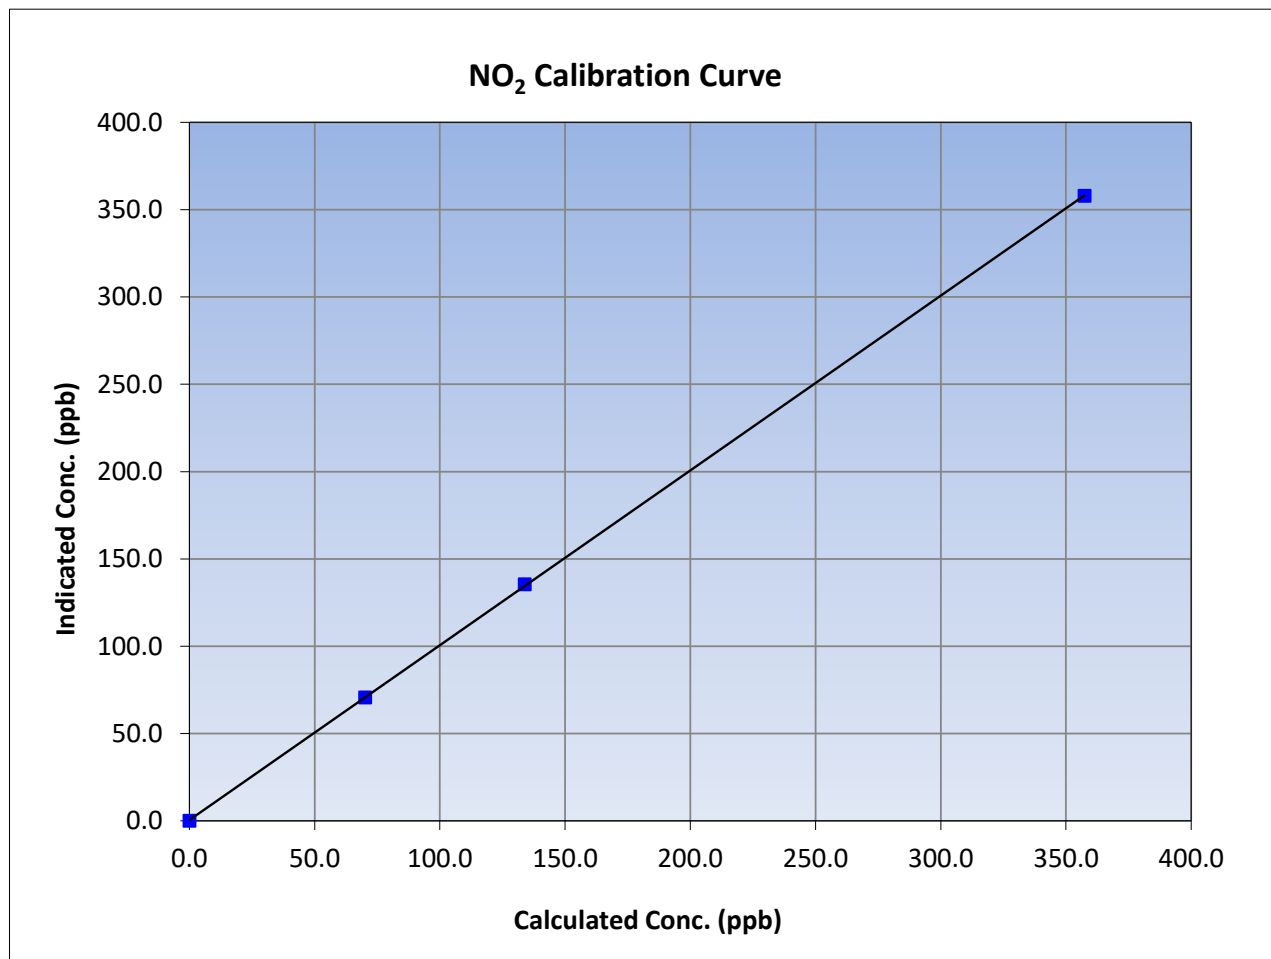

NO_x Calibration Plot

Date: January 20, 2023

Location: Barge Landing

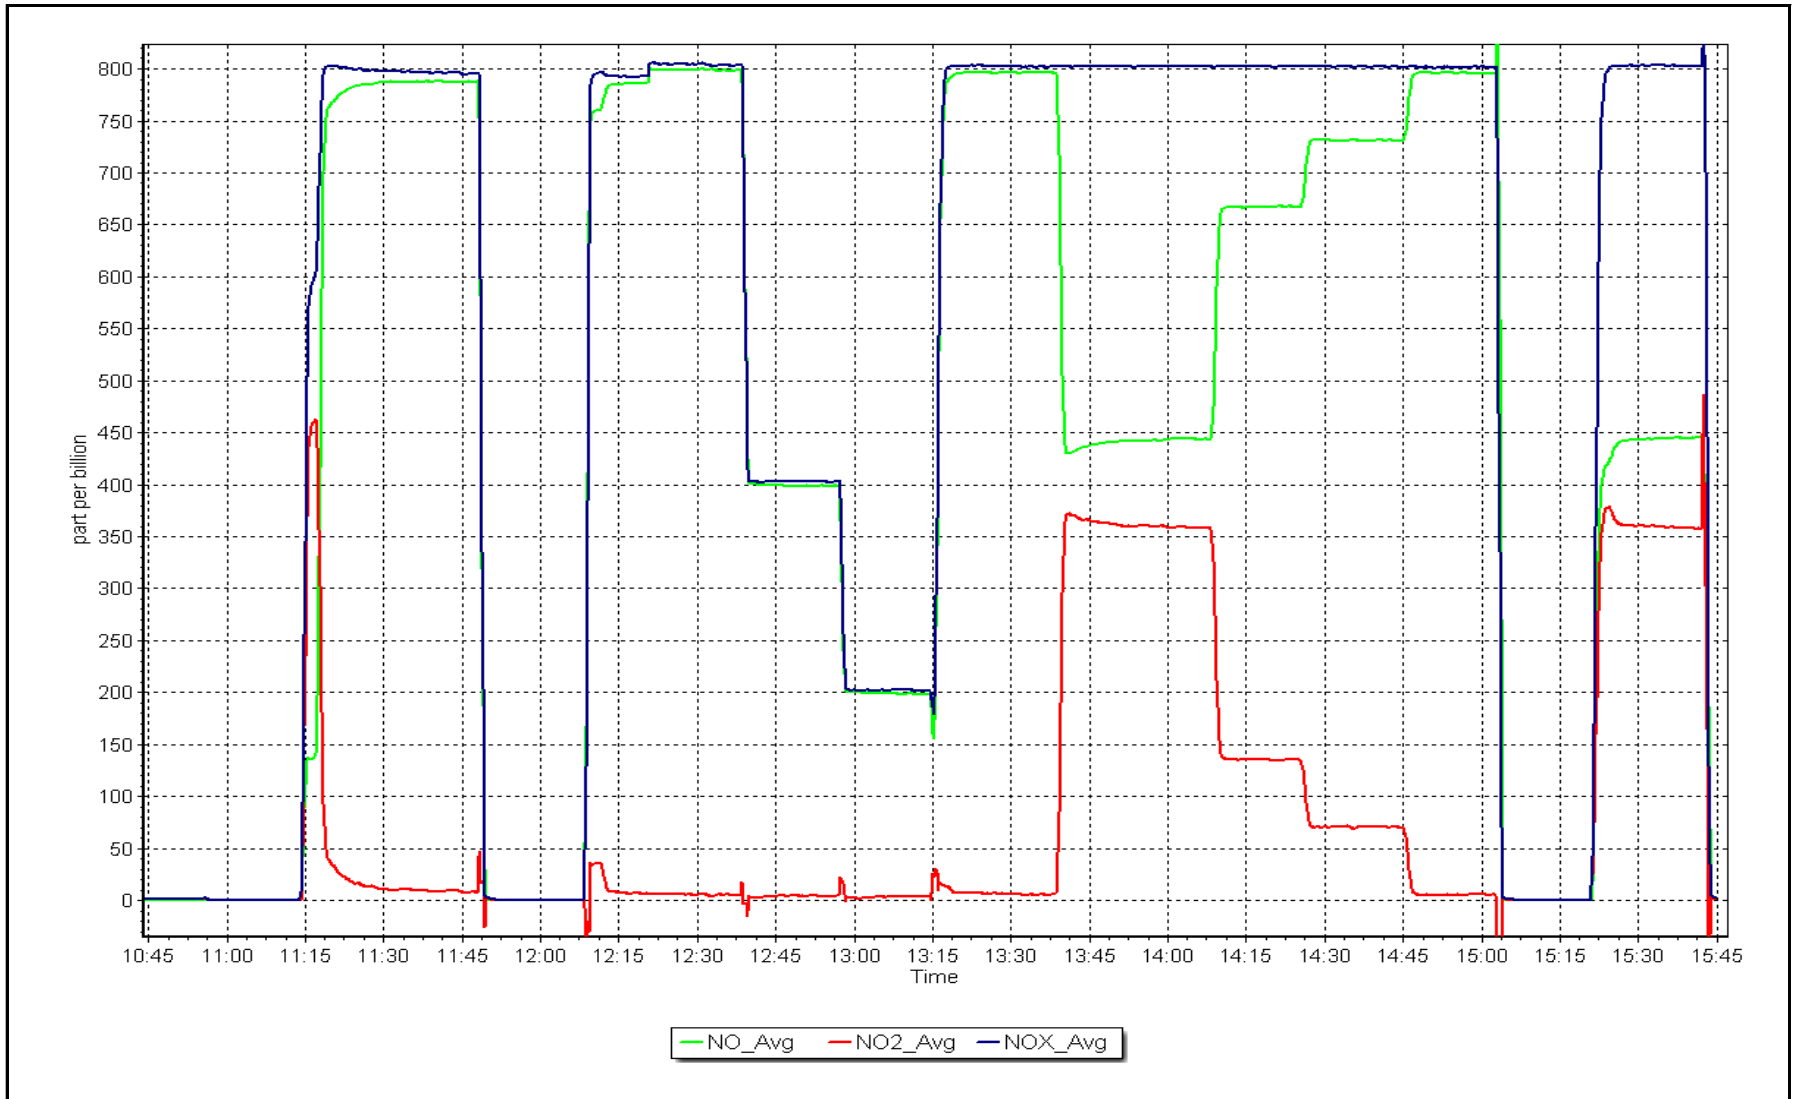



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Barge Landing Station number: AMS 09
 Calibration Date: January 27, 2023 Last Cal Date: December 22, 2022
 Start time (MST): 13:59 End time (MST): 14:19

Analyzer Make: API T640 S/N: 321
 Particulate Fraction: PM2.5

Flow Meter Make/Model: Delta Cal S/N: 1102
 Temp/RH standard: Delta Cal S/N: 1102

Monthly Calibration Test

Parameter	As found	Measured	As left	Adjusted	(Limits)
T (°C)	-16.7	-16.6	-16.7	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	743.1	742.4	743.1	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5.01	5.17	5.01	<input type="checkbox"/>	+/- 0.25 LPM
Leak Test:	Date of check: <u>January 27, 2023</u>	Last Cal Date: <u>December 22, 2022</u>			
	PM w/o HEPA: <u>15.9</u>	PM w/ HEPA: <u>0.0</u>			

Inlet cleaning : Inlet Head

Quarterly Calibration Test

Parameter	As found	Measured	As left	Adjusted	(Limits)
PMT Peak Test				<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: _____
 Disposable Filter Changed: _____

Annual Maintenance

Date Sample Tube Cleaned: November 15, 2022
 Date RH/T Sensor Cleaned: November 15, 2022

Notes: Monthly checks showing no issues. No adjustments needed.

Calibration by: Ryan Power



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS11 LOWER CAMP JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Lower Camp	Station number:	AMS11
Calibration Date:	January 20, 2023	Last Cal Date:	December 7, 2022
Start time (MST):	10:58	End time (MST):	14:05
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.25	ppm	Cal Gas Exp Date:	February 23, 2025
Cal Gas Cylinder #:	CC2216			
Removed Cal Gas Conc:	49.25	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	3807
ZAG Make/Model:	Teledyne API T701		Serial Number:	196

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	100841398
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.987356	0.996844	Backgd or Offset:	14.0	14.2
Calibration intercept:	-0.949290	-0.548951	Coeff or Slope:	1.039	1.051

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.3	----
as found span	4919	81.3	800.8	787.1	1.017
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.3	----
high point	4919	81.3	800.8	798.4	1.003
second point	4959	40.7	400.9	397.8	1.008
third point	4980	20.3	199.9	198.5	1.007
as left zero	5000	0.0	0.0	0.1	----
as left span	4919	81.3	800.8	797.9	1.004
Average Correction Factor					1.006

Baseline Corr As found:	786.80	Previous response	789.68	*% change	-0.4%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed sample inlet filter after as founds. Adjusted the span only.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 7, 2022
Station Name:	Lower Camp	Station Number:	AMS11
Start Time (MST):	10:58	End Time (MST):	14:05
Analyzer make:	Thermo 43i	Analyzer serial #:	100841398

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.3	----	Correlation Coefficient	0.999991	
800.8	798.4	1.0030			≥0.995
400.9	397.8	1.0078	Slope	0.996844	
199.9	198.5	1.0073			0.90 - 1.10
			Intercept	-0.548951	+/-30

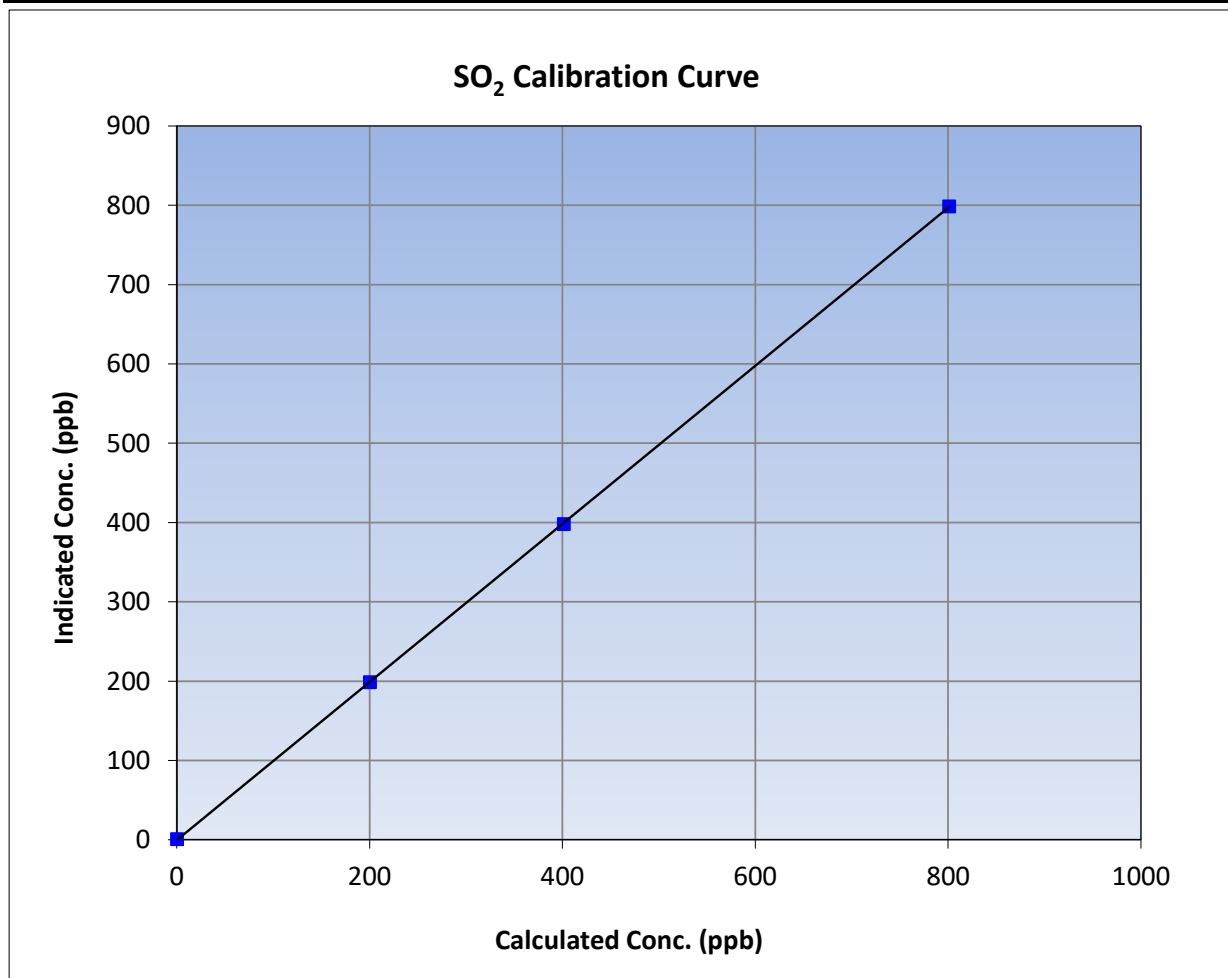

SO2 Calibration Plot

Date: January 20, 2023

Location: Lower Camp

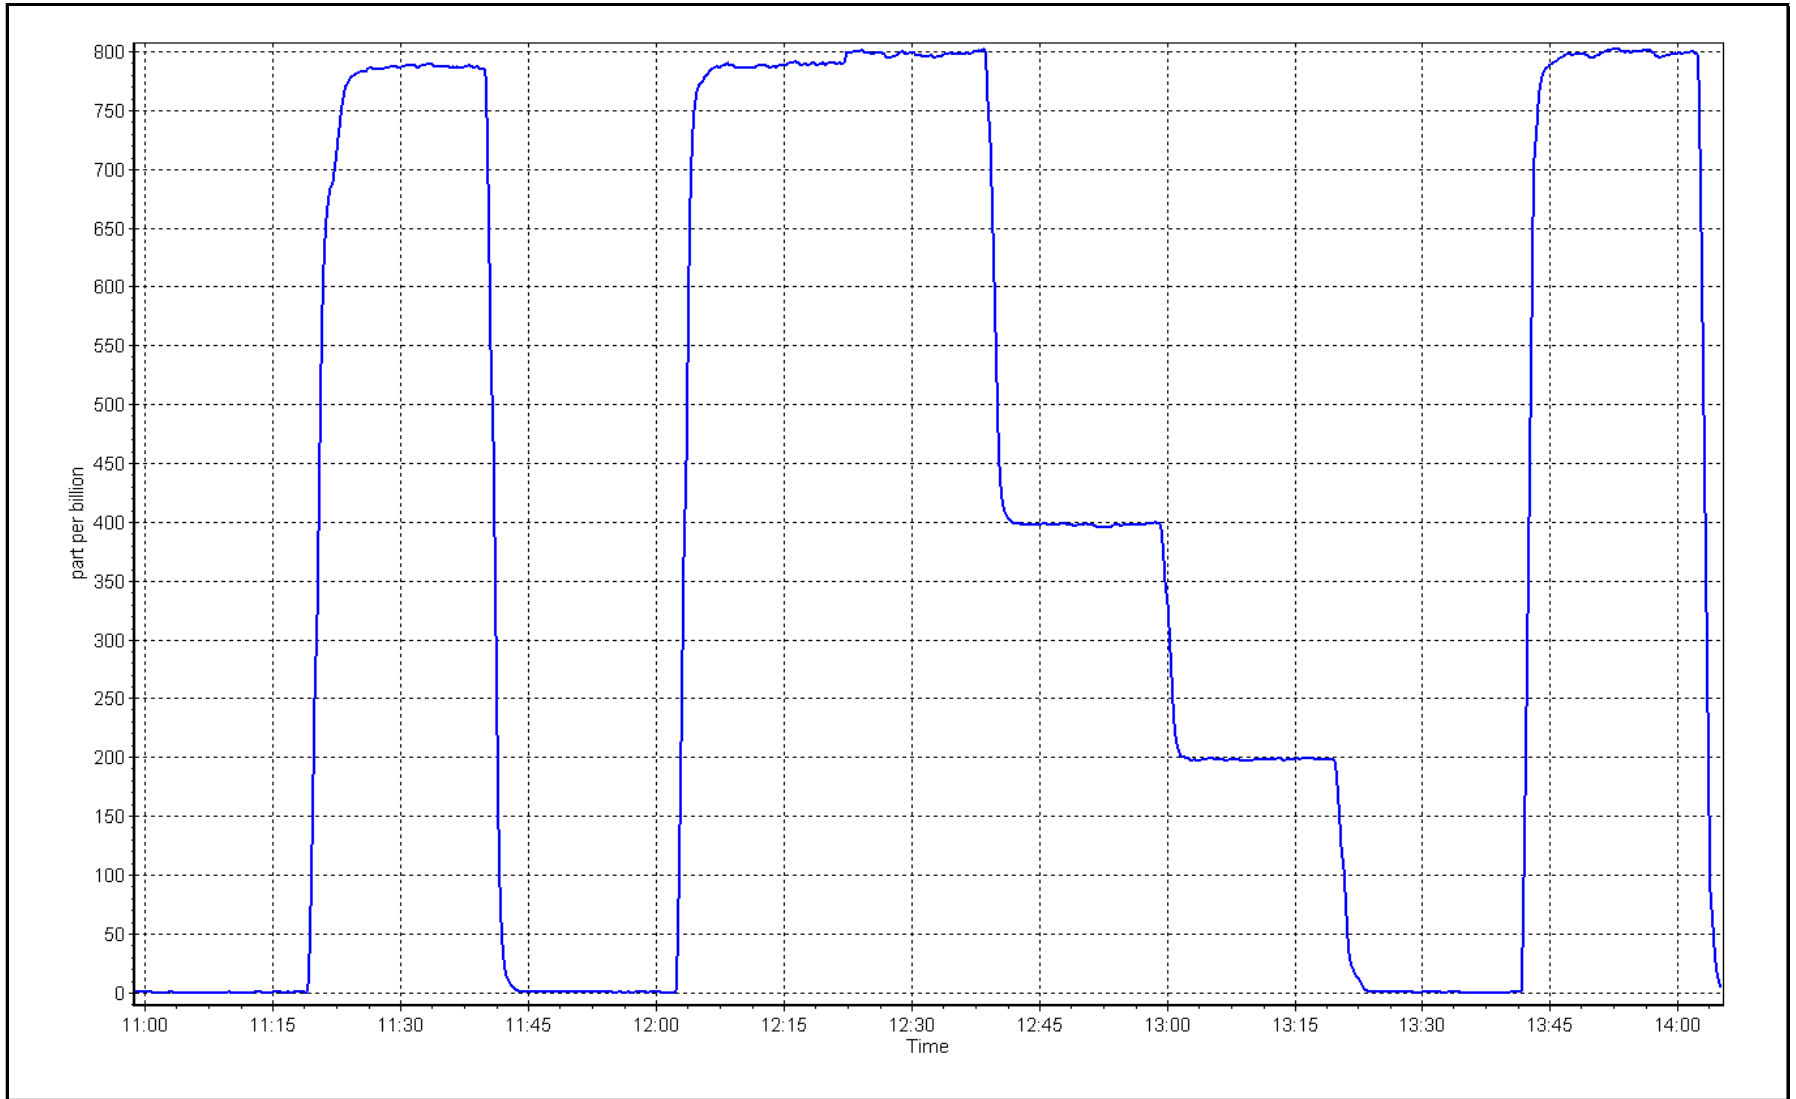



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Lower Camp Station number: AMS11
 Calibration Date: January 19, 2023 Last Cal Date: December 12, 2022
 Start time (MST): 10:52 End time (MST): 14:35
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.429 ppm Cal Gas Exp Date: January 4, 2025
 Cal Gas Cylinder #: CC501097
 Removed Cal Gas Conc: 5.429 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 3807
 ZAG Make/Model: API T701H Serial Number: 196

Analyzer Information

Analyzer make: Thermo 450iQ Analyzer serial #: CM20080003
 Converter make: NA Converter serial #: NA
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.988178	1.000040	Backgd or Offset: 13.9	13.9
Calibration intercept:	0.595542	0.055163	Coeff or Slope: 1.043	1.043

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4926	73.6	79.9	80.5	0.994
as found 2nd point	4963	36.8	40.0	40.1	0.999
as found 3rd point	4982	18.6	20.2	20.1	1.010
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.2	----
high point	4926	73.6	79.9	80.1	0.998
second point	4963	36.8	40.0	39.8	1.004
third point	4982	18.6	20.2	20.2	1.000
as left zero	5000	0.0	0.0	0.0	----
as left span	4926	73.6	79.9	79.8	1.002
SO2 Scrubber Check	4919	81.1	811.0	0.0	----
Date of last scrubber change:				Ave Corr Factor	1.000
Date of last converter efficiency test:				efficiency	

Baseline Corr As found: 80.4 Prev response: 79.57 *% change: 1.0%
 Baseline Corr 2nd AF pt: 40.0 AF Slope: 1.007046 AF Intercept: -0.065171
 Baseline Corr 3rd AF pt: 20.0 AF Correlation: 0.999981

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds. Completed a SO2 scrubber check after calibrator zero. No adjustments made.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 12, 2022
Station Name:	Lower Camp	Station Number:	AMS11
Start Time (MST):	10:52	End Time (MST):	14:35
Analyzer make:	Thermo 450iQ	Analyzer serial #:	CM20080003

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999976	≥0.995
79.9	80.1	0.9978			
40.0	39.8	1.0040	Slope	1.000040	0.90 - 1.10
20.2	20.2	0.9997			
			Intercept	0.055163	+/-3

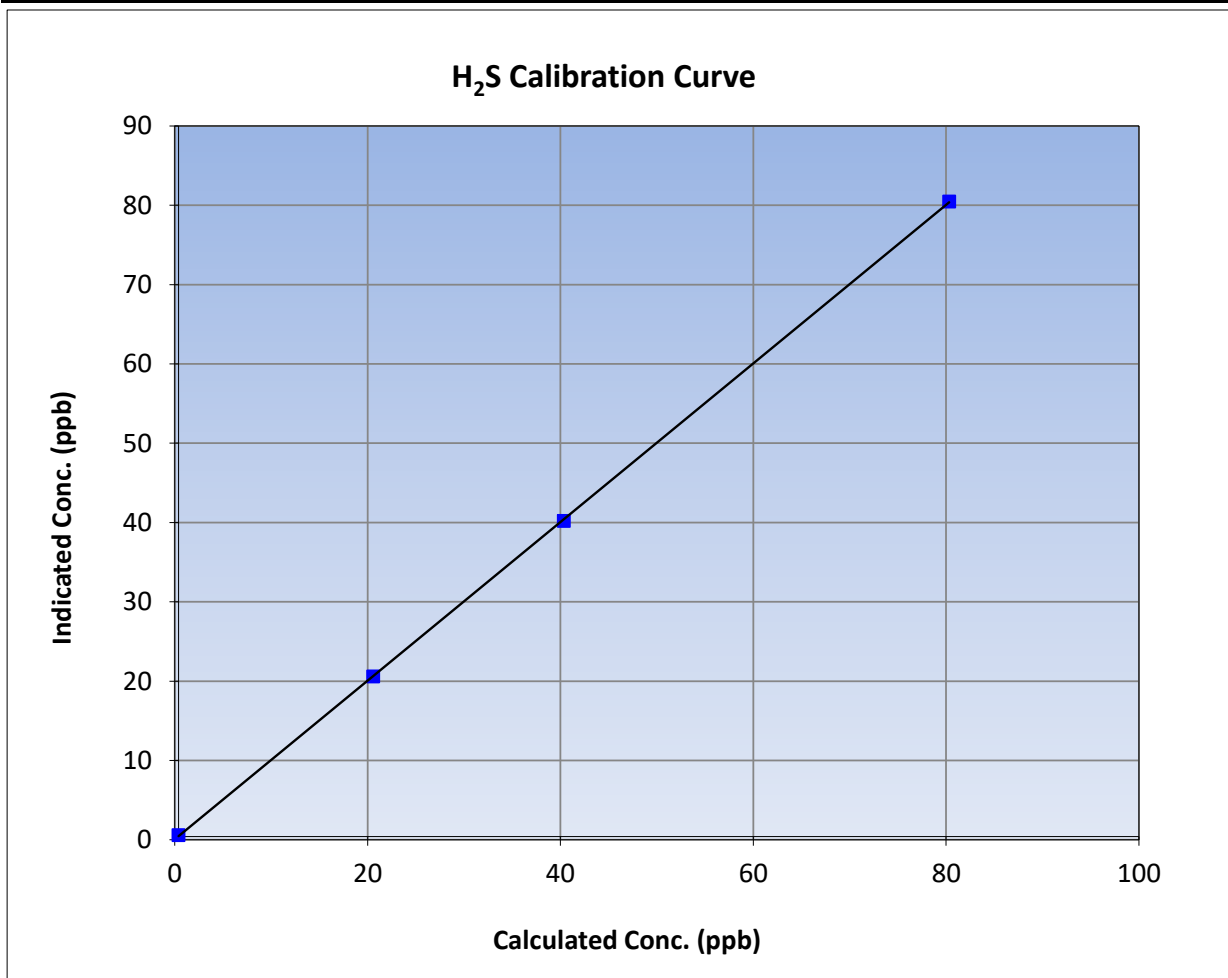

H₂S Calibration Plot

Date: January 19, 2023

Location: Lower Camp

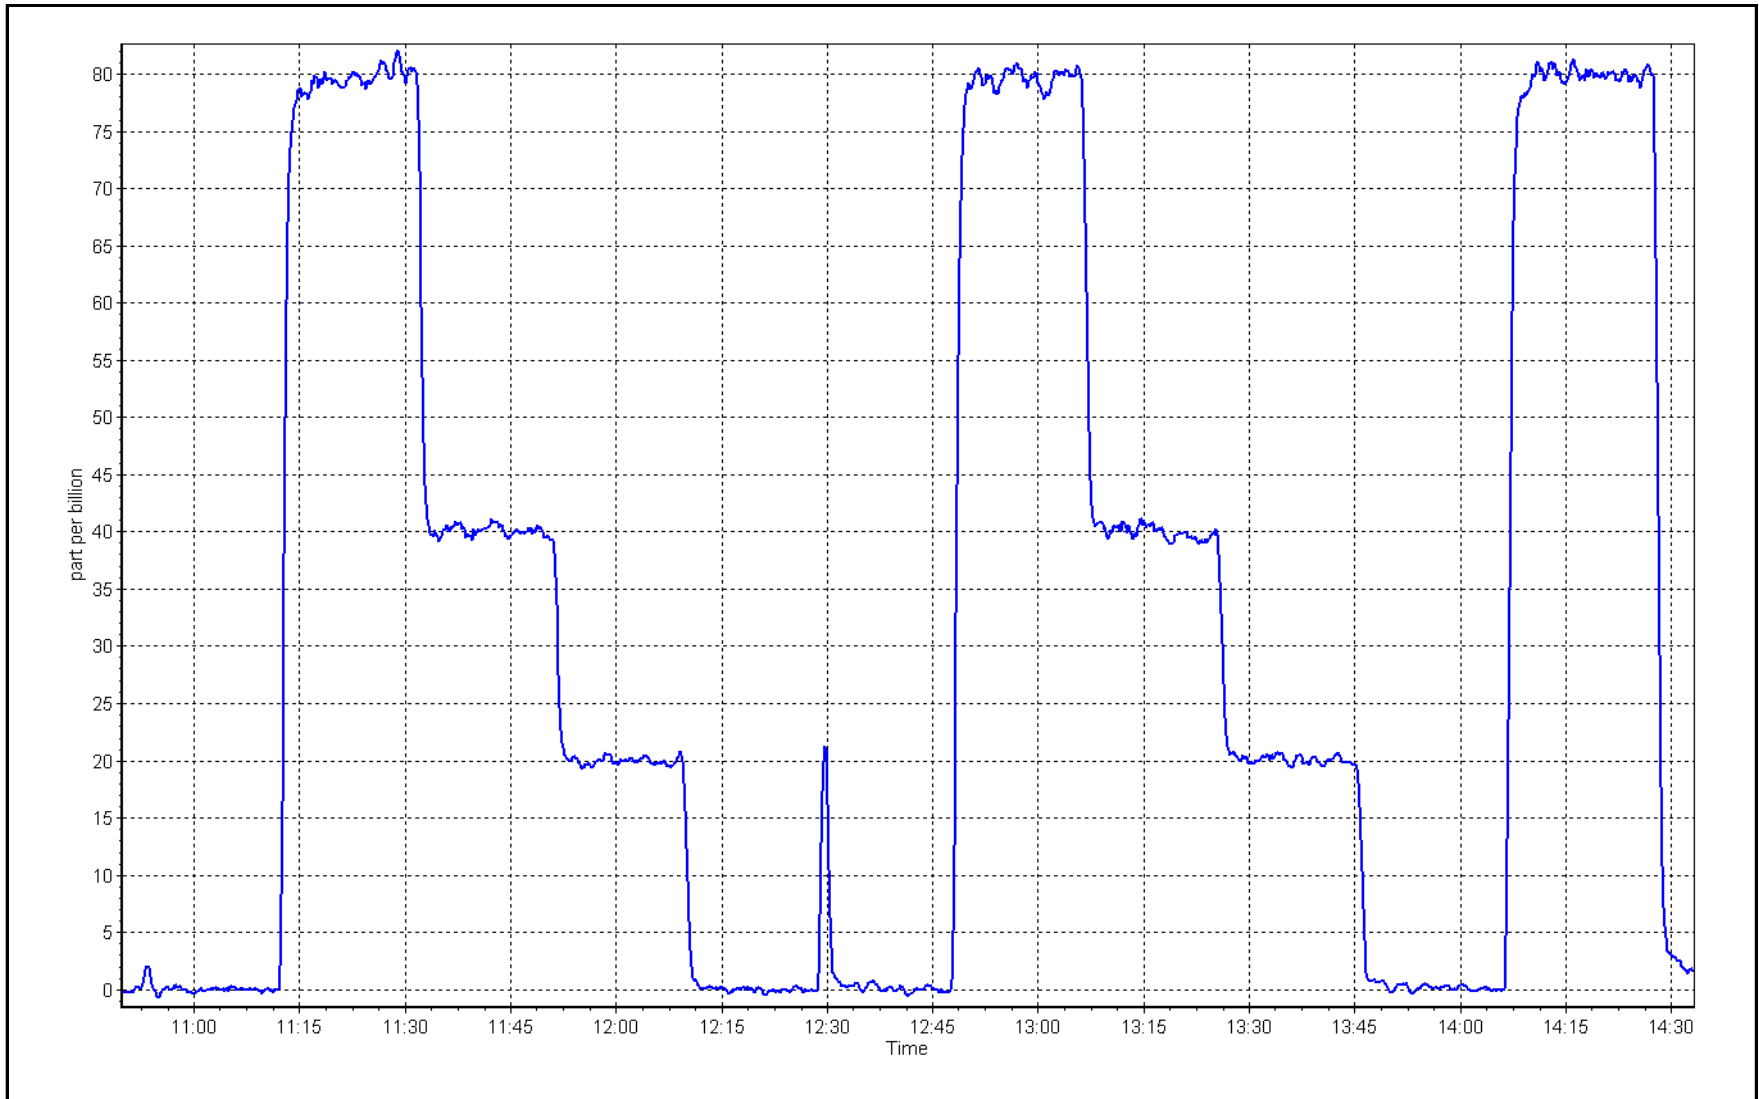



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Lower Camp	Station number:	AMS11
Calibration Date:	January 20, 2023	Last Cal Date:	December 7, 2022
Start time (MST):	10:58	End time (MST):	14:07
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC2216	Cal Gas Expiry Date:	February 23, 2025
CH ₄ Cal Gas Conc.	502.0 ppm	CH ₄ Equiv Conc.	1067.1 ppm
C ₃ H ₈ Cal Gas Conc.	205.5 ppm		
Removed Gas Cert:		Removed Gas Expiry:	
Removed CH ₄ Conc.	502.0 ppm	CH ₄ Equiv Conc.	1067.1 ppm
Removed C ₃ H ₈ Conc.	205.5 ppm		
Diff between cyl (CH ₄):		Diff between cyl (THC):	
Calibrator Model:	API T700	Diff between cyl (NM):	
ZAG make/model:	API T701	Serial Number:	3807
		Serial Number:	196

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1505164381
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	3.09E-04	3.09E-04	NMHC SP Ratio:	5.97E-05
CH ₄ Retention time:	14.0	14.0	NMHC Peak Area:	153551

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4919	81.3	17.35	17.42	0.996
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4919	81.3	17.35	17.42	0.996
second point	4959	40.7	8.69	8.66	1.003
third point	4980	20.3	4.33	4.32	1.003
as left zero	5000	0.0	0.00	0.00	----
as left span	4919	81.3	17.35	17.50	0.991

Average Correction Factor				1.001
Baseline Corr AF:	17.42	Prev response	17.28	*% change 0.8%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4919	81.3	9.19	9.21	0.997
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4919	81.3	9.19	9.20	0.999
second point	4959	40.7	4.60	4.58	1.004
third point	4980	20.3	2.29	2.29	1.003
as left zero	5000	0.0	0.00	0.00	----
as left span	4919	81.3	9.19	9.26	0.993
Average Correction Factor					1.002
Baseline Corr AF:	9.21	Prev response	9.12	*% change	1.1%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4919	81.3	8.16	8.21	0.995
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4919	81.3	8.16	8.22	0.993
second point	4959	40.7	4.09	4.08	1.003
third point	4980	20.3	2.04	2.03	1.003
as left zero	5000	0.0	0.00	0.00	----
as left span	4919	81.3	8.16	8.25	0.990
Average Correction Factor					0.999
Baseline Corr AF:	8.21	Prev response	8.16	*% change	0.5%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	0.996778	1.004292
THC Cal Offset:	-0.017186	-0.024989
CH ₄ Cal Slope:	1.001133	1.007657
CH ₄ Cal Offset:	-0.009686	-0.016486
NMHC Cal Slope:	0.992847	1.001092
NMHC Cal Offset:	-0.007499	-0.007903

Notes: Changed sample inlet filter after as founds. No adjustments made.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 7, 2022
Station Name:	Lower Camp	Station Number:	AMS11
Start Time (MST):	10:58	End Time (MST):	14:07
Analyzer make:	Thermo 55i	Analyzer serial #:	1505164381

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999983	≥ 0.995			
17.35	17.42	0.9959						
8.69	8.66	1.0033				Slope	1.004292	0.90 - 1.10
4.33	4.32	1.0028						
			Intercept	-0.024989	± 0.5			

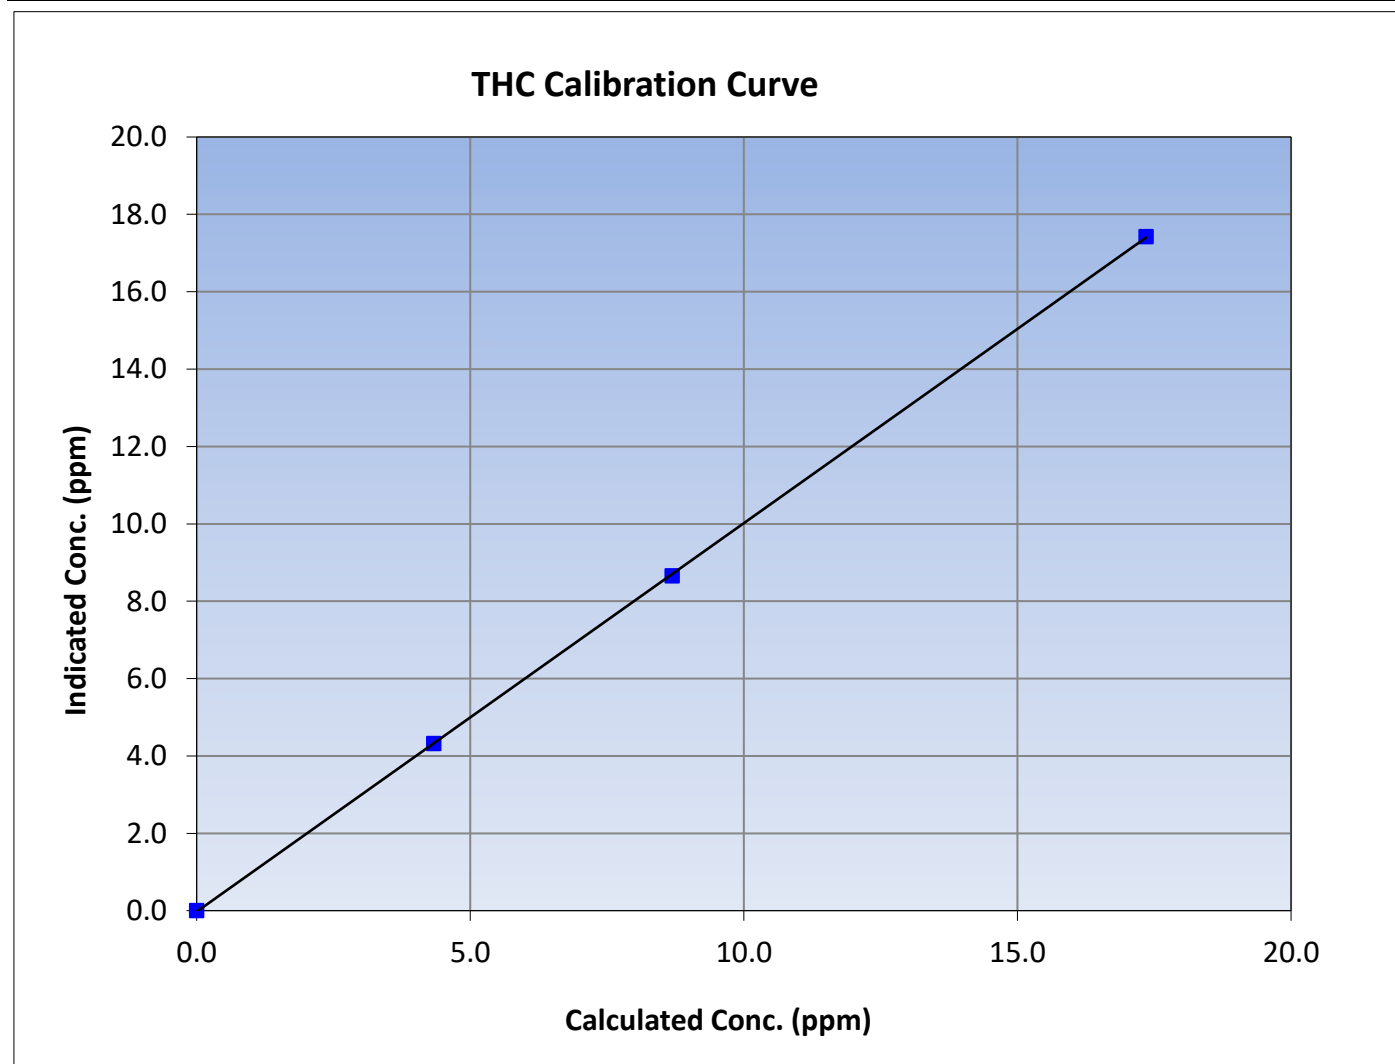



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 7, 2022
Station Name:	Lower Camp	Station Number:	AMS11
Start Time (MST):	10:58	End Time (MST):	14:07
Analyzer make:	Thermo 55i	Analyzer serial #:	1505164381

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999969	≥0.995
8.16	8.22	0.9927			
4.09	4.08	1.0026			
2.04	2.03	1.0030			
			Slope	1.007657	0.90 - 1.10
			Intercept	-0.016486	+/-0.5

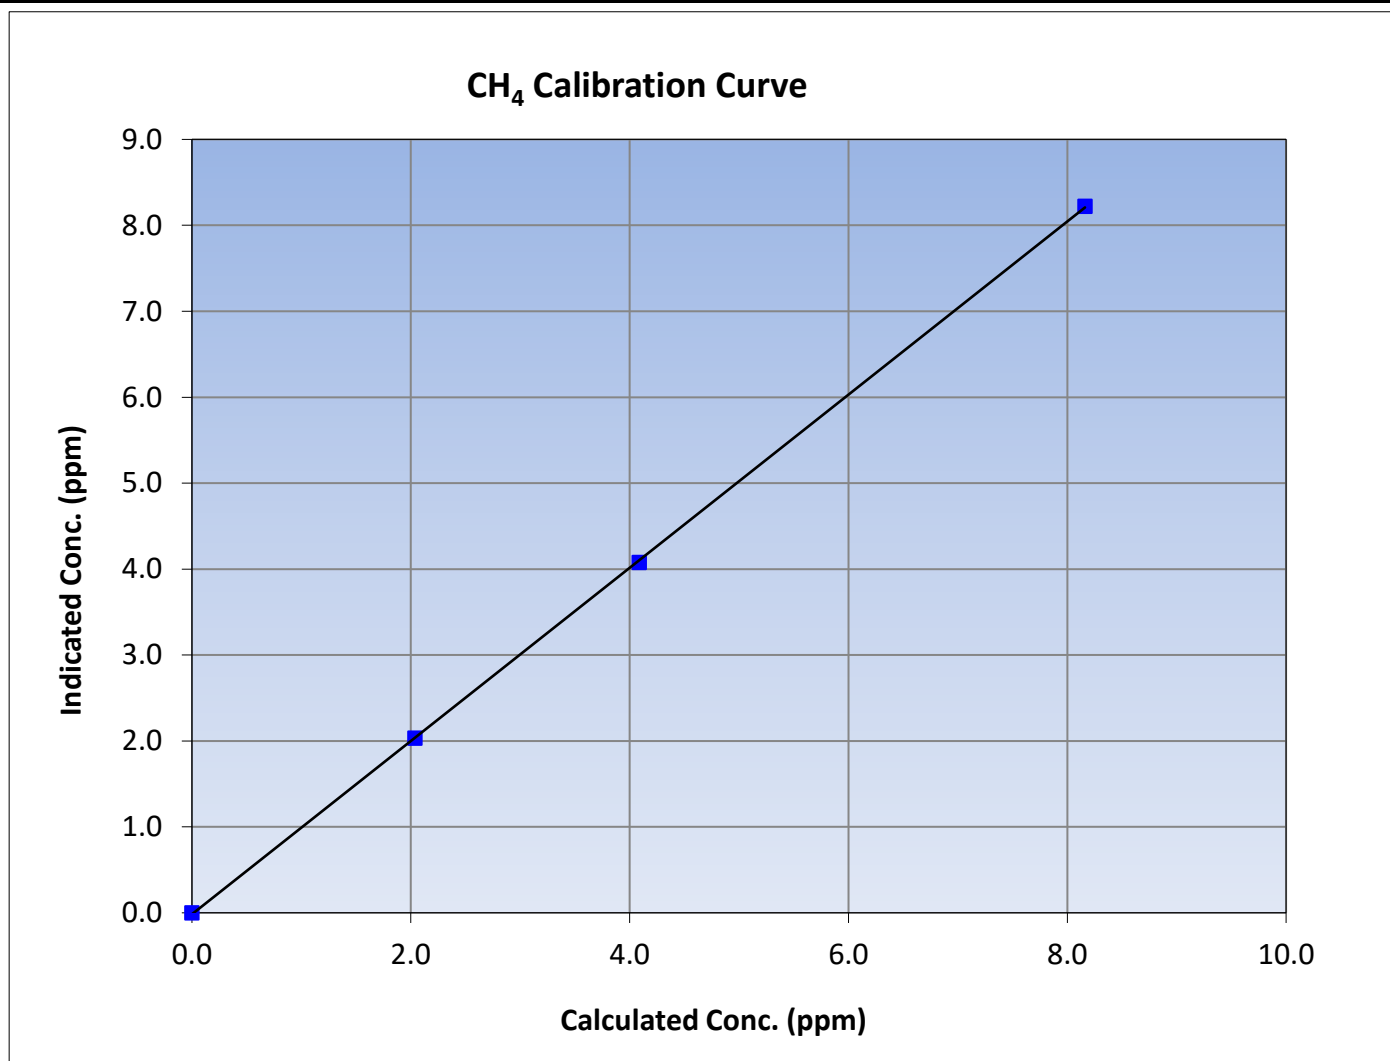



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 7, 2022
Station Name:	Lower Camp	Station Number:	AMS11
Start Time (MST):	10:58	End Time (MST):	14:07
Analyzer make:	Thermo 55i	Analyzer serial #:	1505164381

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999993	≥ 0.995
9.19	9.20	0.9990			
4.60	4.58	1.0038	Slope	1.001092	0.90 - 1.10
2.29	2.29	1.0027			
			Intercept	-0.007903	± 0.5

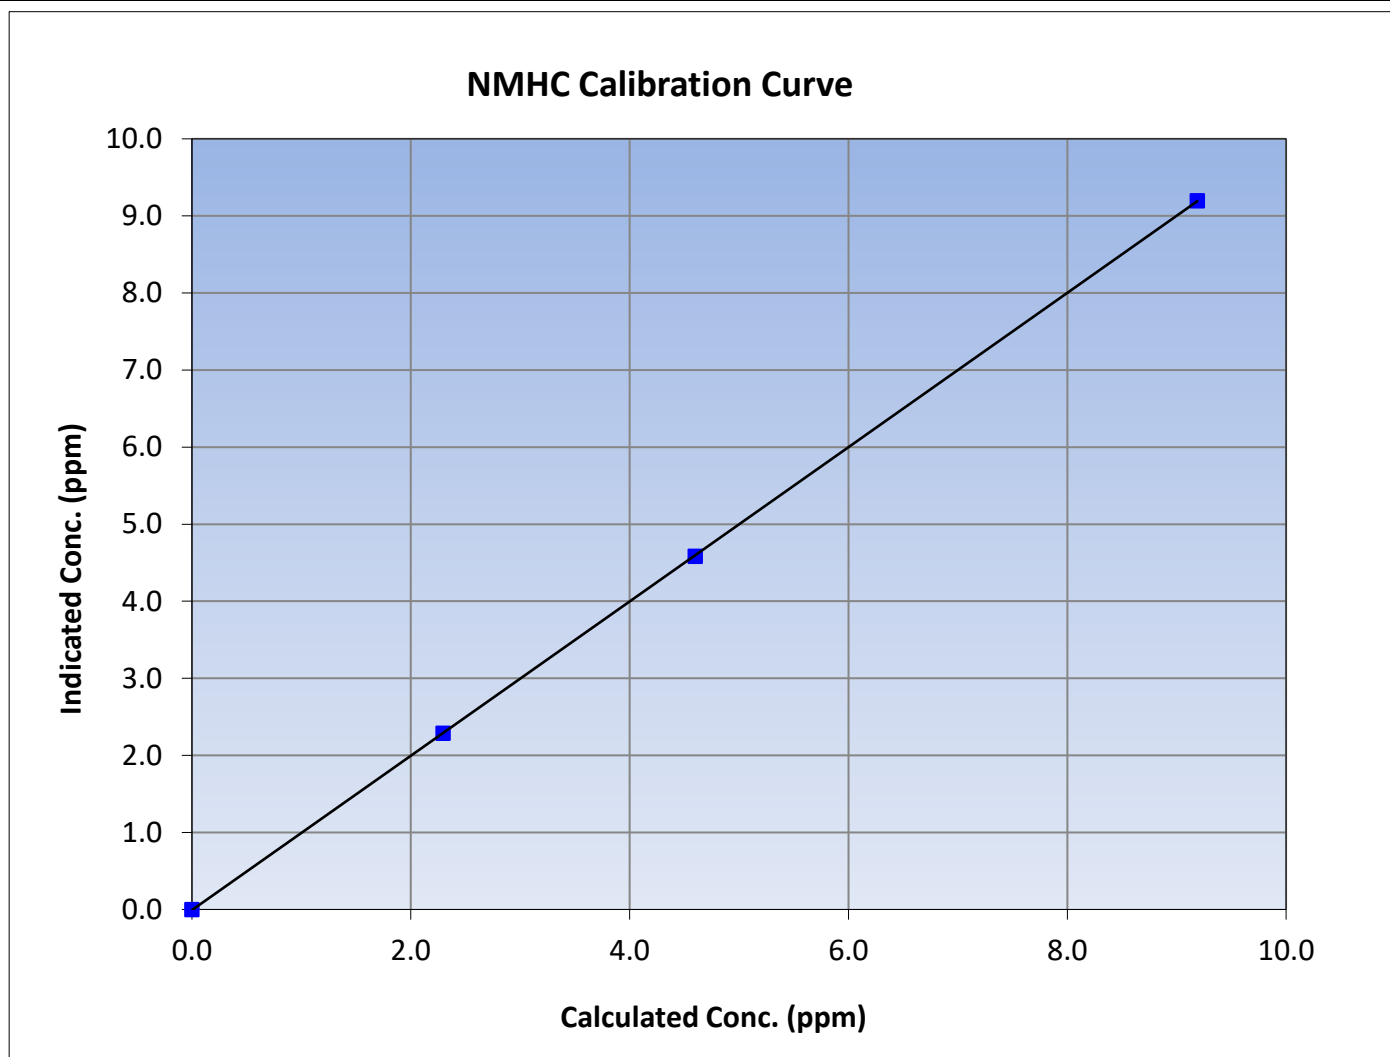

NMHC Calibration Plot

Date: January 20, 2023

Location: Lower Camp

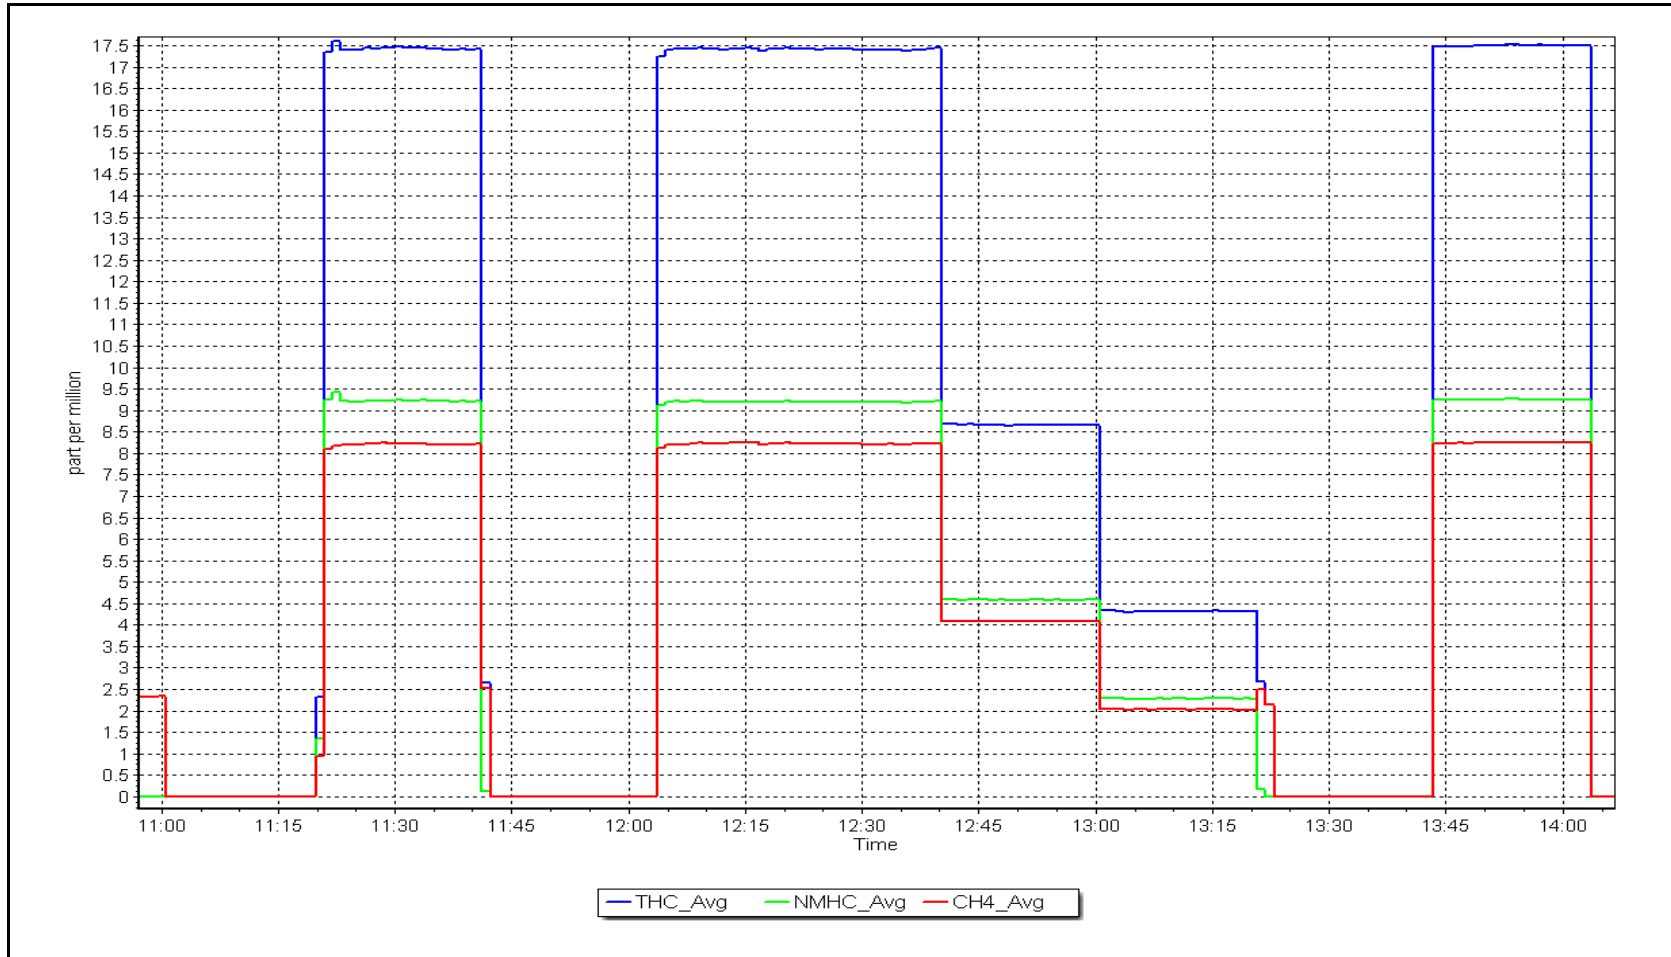



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS13 FORT MCKAY SOUTH JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Fort McKay South	Station number:	AMS13
Calibration Date:	January 16, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	10:30	End time (MST):	13:37
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	50.55	ppm	Cal Gas Exp Date:	December 29, 2028
Cal Gas Cylinder #:	CC260812			
Removed Cal Gas Conc:	50.55	ppm	Rem Gas Exp Date:	N/A
Removed Gas Cyl #:	N/A		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	2448
ZAG Make/Model:	API 701		Serial Number:	1117

Analyzer Information

Analyzer make:	API T100	Analyzer serial #:	599
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.006001	1.003886	Backgd or Offset:	77.0	79.7
Calibration intercept:	-3.218258	-3.178199	Coeff or Slope:	0.741	0.733

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.7	----
as found span	4921	79.1	799.7	807.4	0.990
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	-0.2	----
high point	4921	79.1	799.7	801.0	0.998
second point	4961	39.5	399.3	396.5	1.007
third point	4980	19.8	200.2	194.6	1.029
as left zero	5000	0.0	0.0	-0.4	----
as left span	4921	79.1	799.7	800.7	0.999
Average Correction Factor					1.011

Baseline Corr As found:	806.70	Previous response	801.27	*% change	0.7%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds. Adjusted zero and span.

Calibration Performed By: Sean Bala



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 2, 2022
Station Name:	Fort McKay South	Station Number:	AMS13
Start Time (MST):	10:30	End Time (MST):	13:37
Analyzer make:	API T100	Analyzer serial #:	599

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	-0.2	----	Correlation Coefficient	0.999937	≥0.995
799.7	801.0	0.9984			
399.3	396.5	1.0071	Slope	1.003886	0.90 - 1.10
200.2	194.6	1.0287			
			Intercept	-3.178199	+/-30

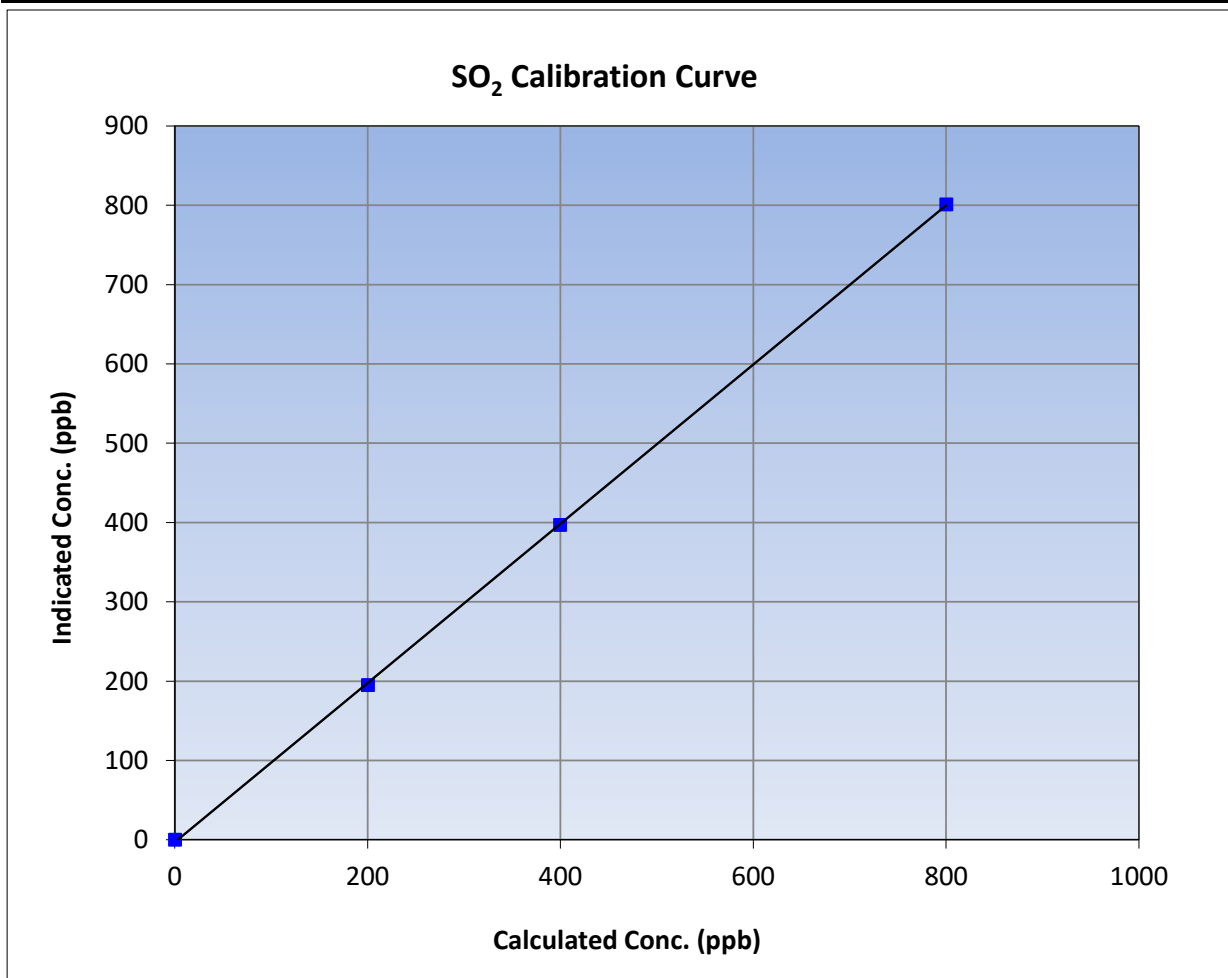

SO2 Calibration Plot

Date: January 16, 2023

Location: Fort McKay South

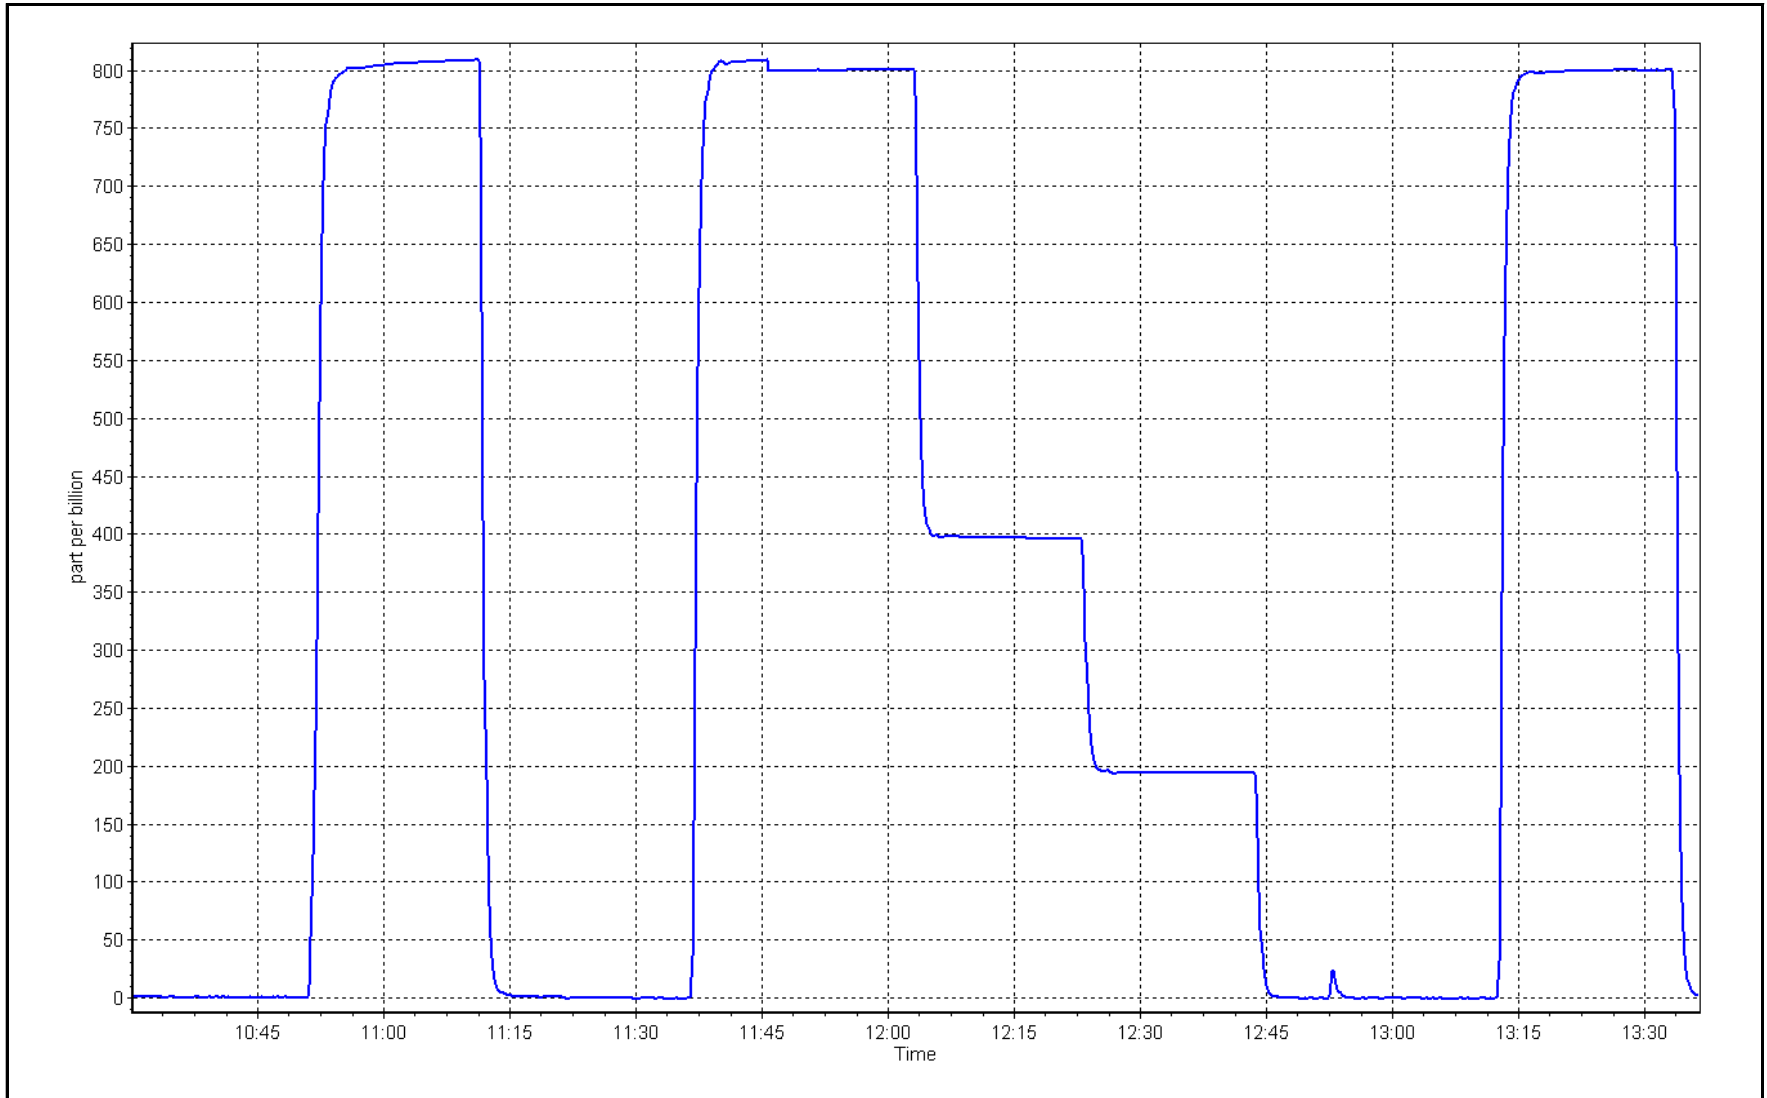



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name:	Fort McKay South	Station number:	AMS13
Calibration Date:	January 17, 2023	Last Cal Date:	December 13, 2022
Start time (MST):	9:27	End time (MST):	14:37
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	5.34	ppm	Cal Gas Exp Date:	January 4, 2025
Cal Gas Cylinder #:	CC500241			
Removed Cal Gas Conc:	5.32	ppm	Rem Gas Exp Date:	March 2, 2023
Removed Gas Cyl #:	EY0001990		Diff between cyl:	-4.1%
Calibrator Make/Model:	Teledyne API T700		Serial Number:	2448
ZAG Make/Model:	Teledyne API 701		Serial Number:	1117

Analyzer Information

Analyzer make:	Thermo 43i TLE	Analyzer serial #:	1180540017
Converter make:	CDN-101	Converter serial #:	521
Analyzer Range	0 - 100 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.001418	0.999228	Backgd or Offset:	3.55	3.69
Calibration intercept:	-0.062130	-0.042157	Coeff or Slope:	1.080	1.120

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4925	75.5	80.3	80.2	1.003
as found 2nd point	4962	37.7	40.1	39.8	1.010
as found 3rd point	4981	18.9	20.1	19.6	1.031
new cylinder response	4925	75.5	80.6	77.3	1.043

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.2	----
high point	4925	75.5	80.6	80.6	1.000
second point	4962	37.7	40.3	40.2	1.002
third point	4981	18.9	20.2	19.8	1.019
as left zero	5000	0.0	0.0	0.3	----
as left span	4925	75.5	80.6	80.4	1.003
SO2 Scrubber Check	4921	79.1	791.0	0.0	----

Date of last scrubber change:	20-Mar-20	Ave Corr Factor	1.007
Date of last converter efficiency test:	NA	efficiency	

Baseline Corr As found:	80.1	Prev response:	80.38	*% change:	-0.3%
Baseline Corr 2nd AF pt:	39.7	AF Slope:	0.999144	AF Intercept:	-0.182203
Baseline Corr 3rd AF pt:	19.5	AF Correlation:	0.999943		

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds and changed the cylinder as well. Completed a SO2 scrubber check after calibrator zero. Adjusted span only.

Calibration Performed By: Sean Bala



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 13, 2022
Station Name:	Fort McKay South	Station Number:	AMS13
Start Time (MST):	9:27	End Time (MST):	13:36
Analyzer make:	Thermo 43i TLE	Analyzer serial #:	1180540017

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999951	
80.6	80.6	1.0003			≥0.995
40.3	40.2	1.0016	Slope	0.999228	
20.2	19.8	1.0195			0.90 - 1.10
			Intercept	-0.042157	+/-3

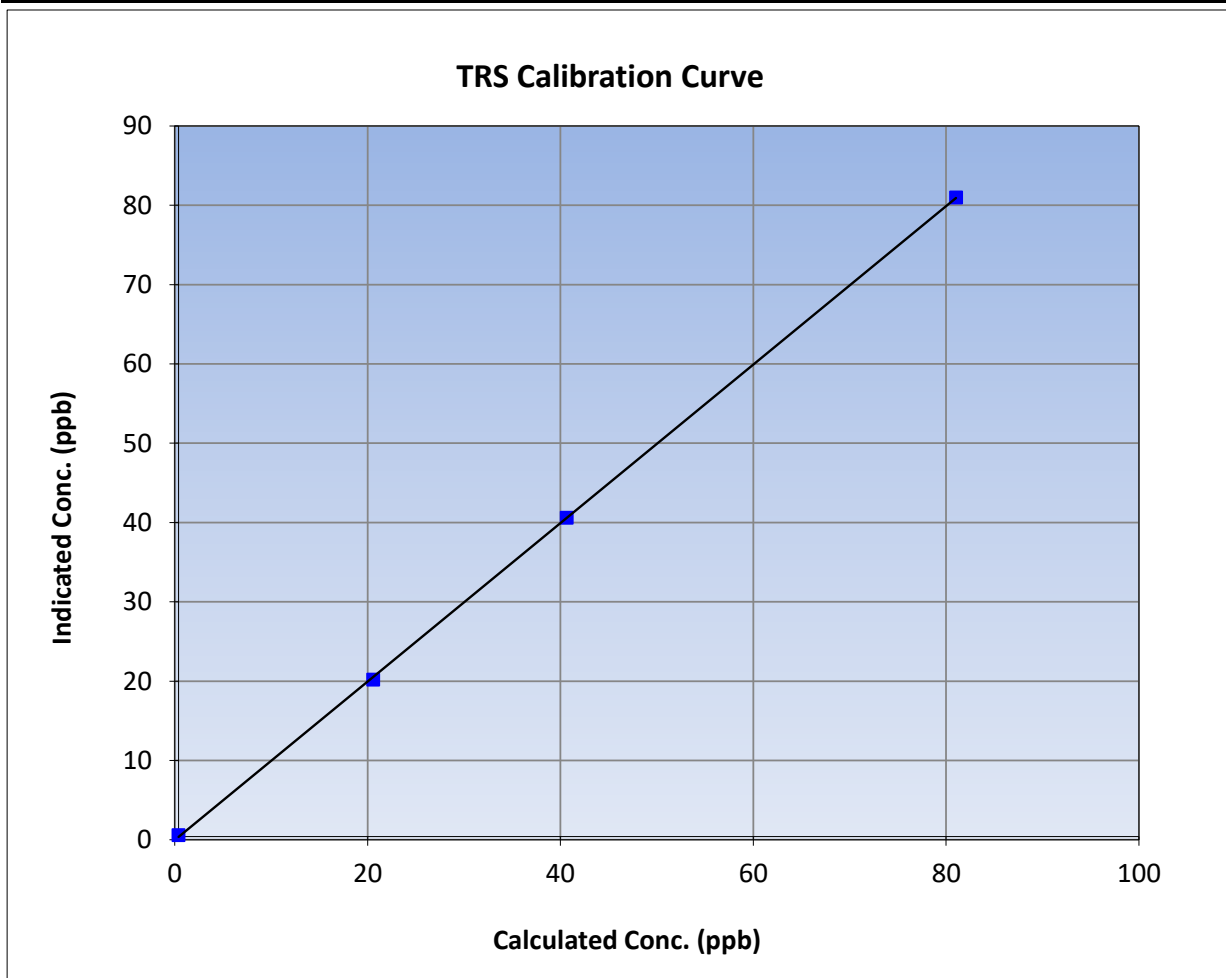

TRS Calibration Plot

Date: January 17, 2023

Location: Fort McKay South

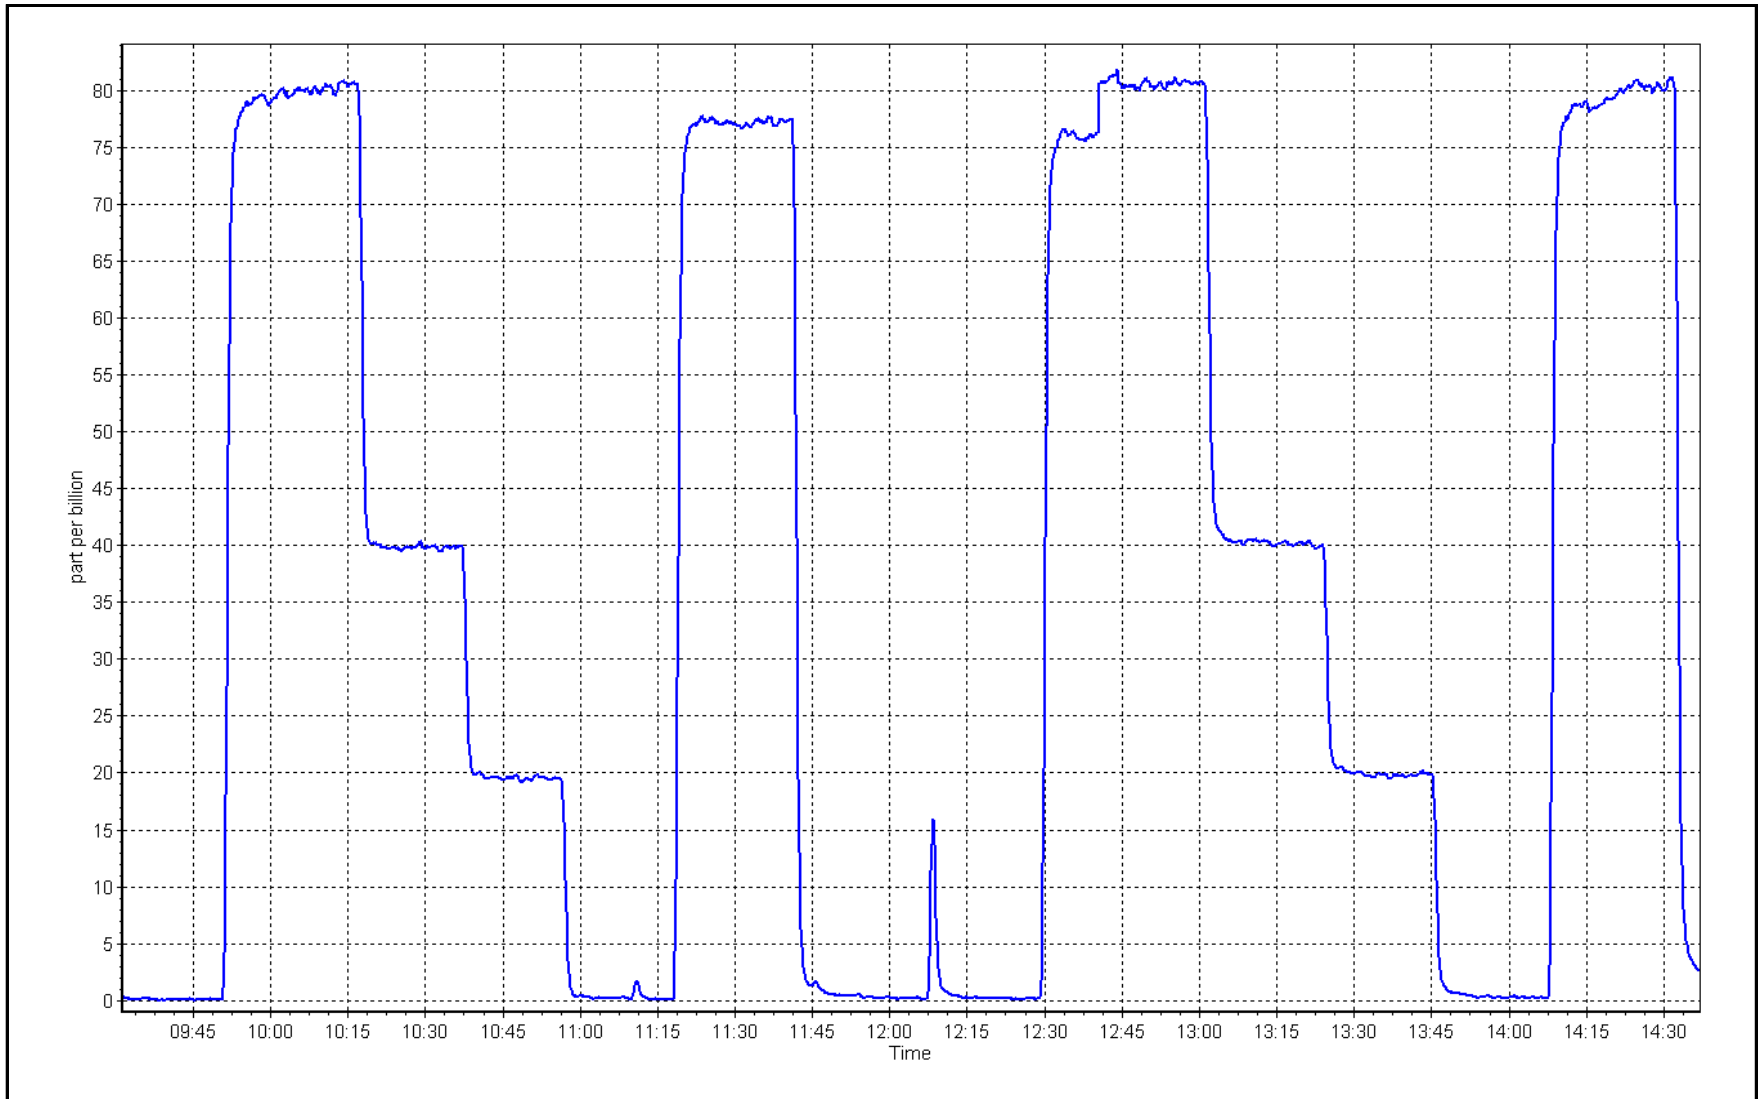



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Fort McKay South	Station number:	AMS13
Calibration Date:	January 16, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	10:30	End time (MST):	13:37
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC260812	Cal Gas Expiry Date:	December 29, 2028
CH ₄ Cal Gas Conc.	503.6 ppm	CH ₄ Equiv Conc.	1077.5 ppm
C ₃ H ₈ Cal Gas Conc.	208.7 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	503.6 ppm	CH ₄ Equiv Conc.	1077.5 ppm
Removed C ₃ H ₈ Conc.	208.7 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	2448
ZAG make/model:	API 701	Serial Number:	1117

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1152430012
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	2.38E-04	2.38E-04	NMHC SP Ratio:	4.69E-05
CH ₄ Retention time:	12.0	12.0	NMHC Peak Area:	193414
				191456

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4921	79.1	17.05	16.99	1.003
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4921	79.1	17.05	17.06	0.999
second point	4961	39.5	8.51	8.37	1.017
third point	4980	19.8	4.27	4.24	1.007
as left zero	5000	0.0	0.00	0.00	----
as left span	4921	79.1	17.05	17.10	0.997
Average Correction Factor					1.008
Baseline Corr AF:	16.99	Prev response	16.99	*% change	0.0%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4921	79.1	9.08	9.02	1.006
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4921	79.1	9.08	9.09	0.998
second point	4961	39.5	4.53	4.49	1.010
third point	4980	19.8	2.27	2.28	0.999
as left zero	5000	0	0.00	0.00	----
as left span	4921	79.1	9.08	9.12	0.996
Average Correction Factor					1.003
Baseline Corr AF:	9.02	Prev response	9.05	*% change	-0.4%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4921	79.1	7.97	7.97	1.000
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4921	79.1	7.97	7.97	1.000
second point	4961	39.5	3.98	3.89	1.024
third point	4980	19.8	1.99	1.96	1.016
as left zero	5000	0.0	0.00	0.00	----
as left span	4921	79.1	7.97	7.99	0.998
Average Correction Factor					1.013
Baseline Corr AF:	7.97	Prev response	7.94	*% change	0.3%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
THC Cal Slope:	1.002563	1.000765
THC Cal Offset:	-0.096578	-0.043424
CH ₄ Cal Slope:	1.003387	1.000366
CH ₄ Cal Offset:	-0.054594	-0.031817
NMHC Cal Slope:	1.001929	1.001015
NMHC Cal Offset:	-0.042585	-0.011206

Notes: Changed the inlet filter after as founds. Adjusted span only.

Calibration Performed By: Sean Bala



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 2, 2022
Station Name:	Fort McKay South	Station Number:	AMS13
Start Time (MST):	10:30	End Time (MST):	13:37
Analyzer make:	Thermo 55i	Analyzer serial #:	1152430012

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999908	≥ 0.995			
17.05	17.06	0.9990						
8.51	8.37	1.0166				Slope	1.000765	0.90 - 1.10
4.27	4.24	1.0071						
			Intercept	-0.043424	± 0.5			

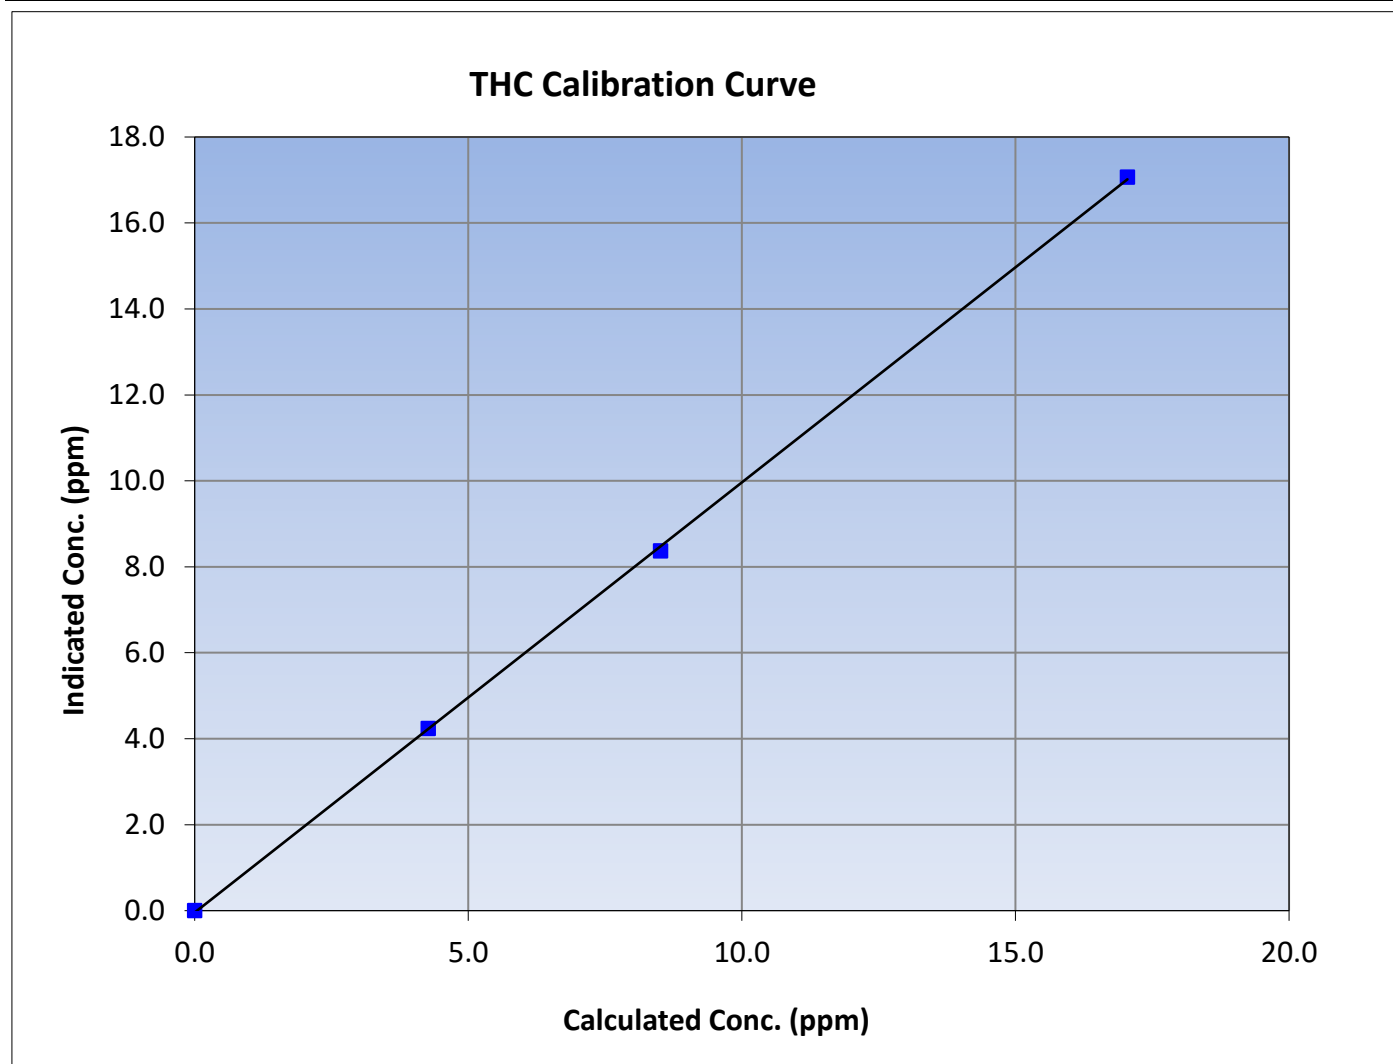



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 2, 2022
Station Name:	Fort McKay South	Station Number:	AMS13
Start Time (MST):	10:30	End Time (MST):	13:37
Analyzer make:	Thermo 55i	Analyzer serial #:	1152430012

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999833	≥0.995
7.97	7.97	0.9997			
3.98	3.89	1.0237			
1.99	1.96	1.0165			
			Slope	1.000366	0.90 - 1.10
			Intercept	-0.031817	+/-0.5

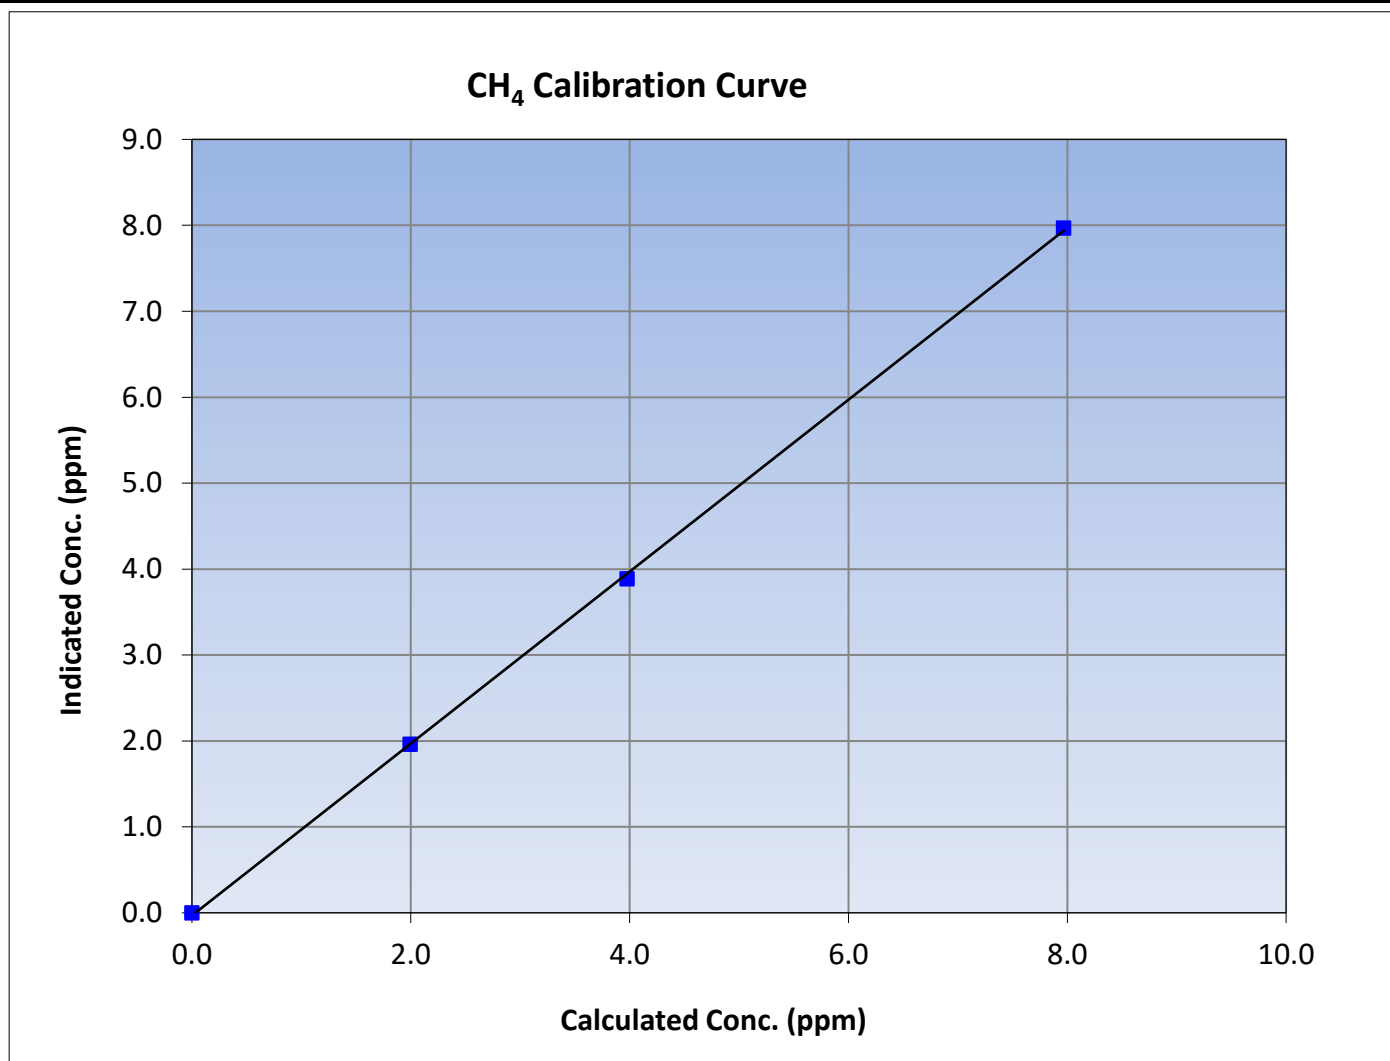



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 2, 2022
Station Name:	Fort McKay South	Station Number:	AMS13
Start Time (MST):	10:30	End Time (MST):	13:37
Analyzer make:	Thermo 55i	Analyzer serial #:	1152430012

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999955	≥ 0.995			
9.08	9.09	0.9984						
4.53	4.49	1.0102				Slope	1.001015	0.90 - 1.10
2.27	2.28	0.9990						
			Intercept	-0.011206	± 0.5			

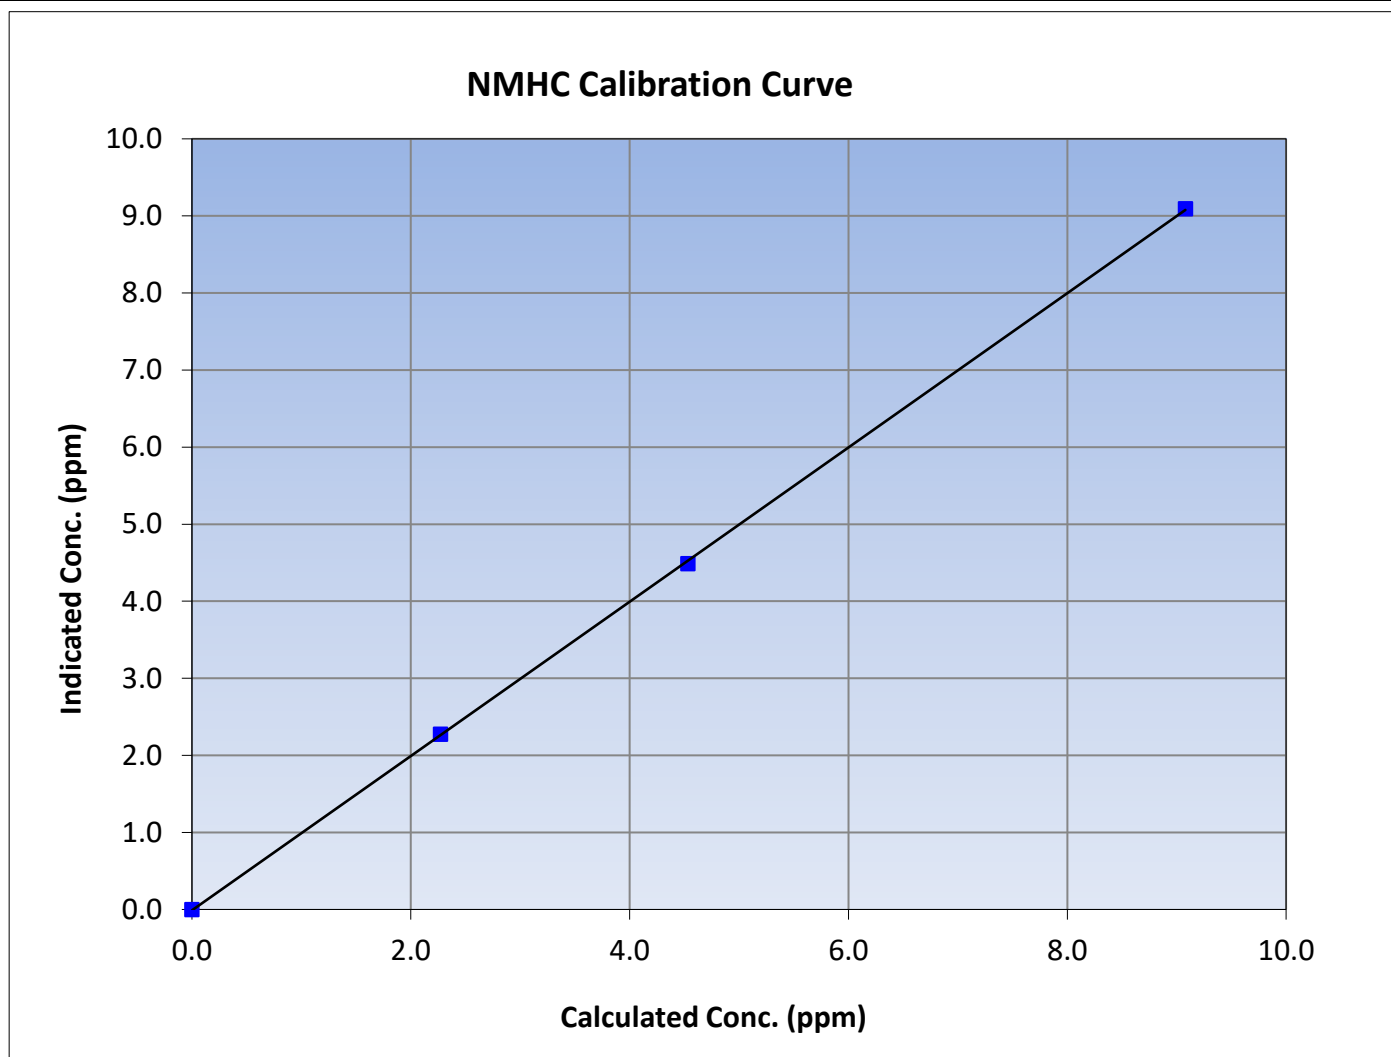

NMHC Calibration Plot

Date: January 16, 2023

Location: Fort McKay South

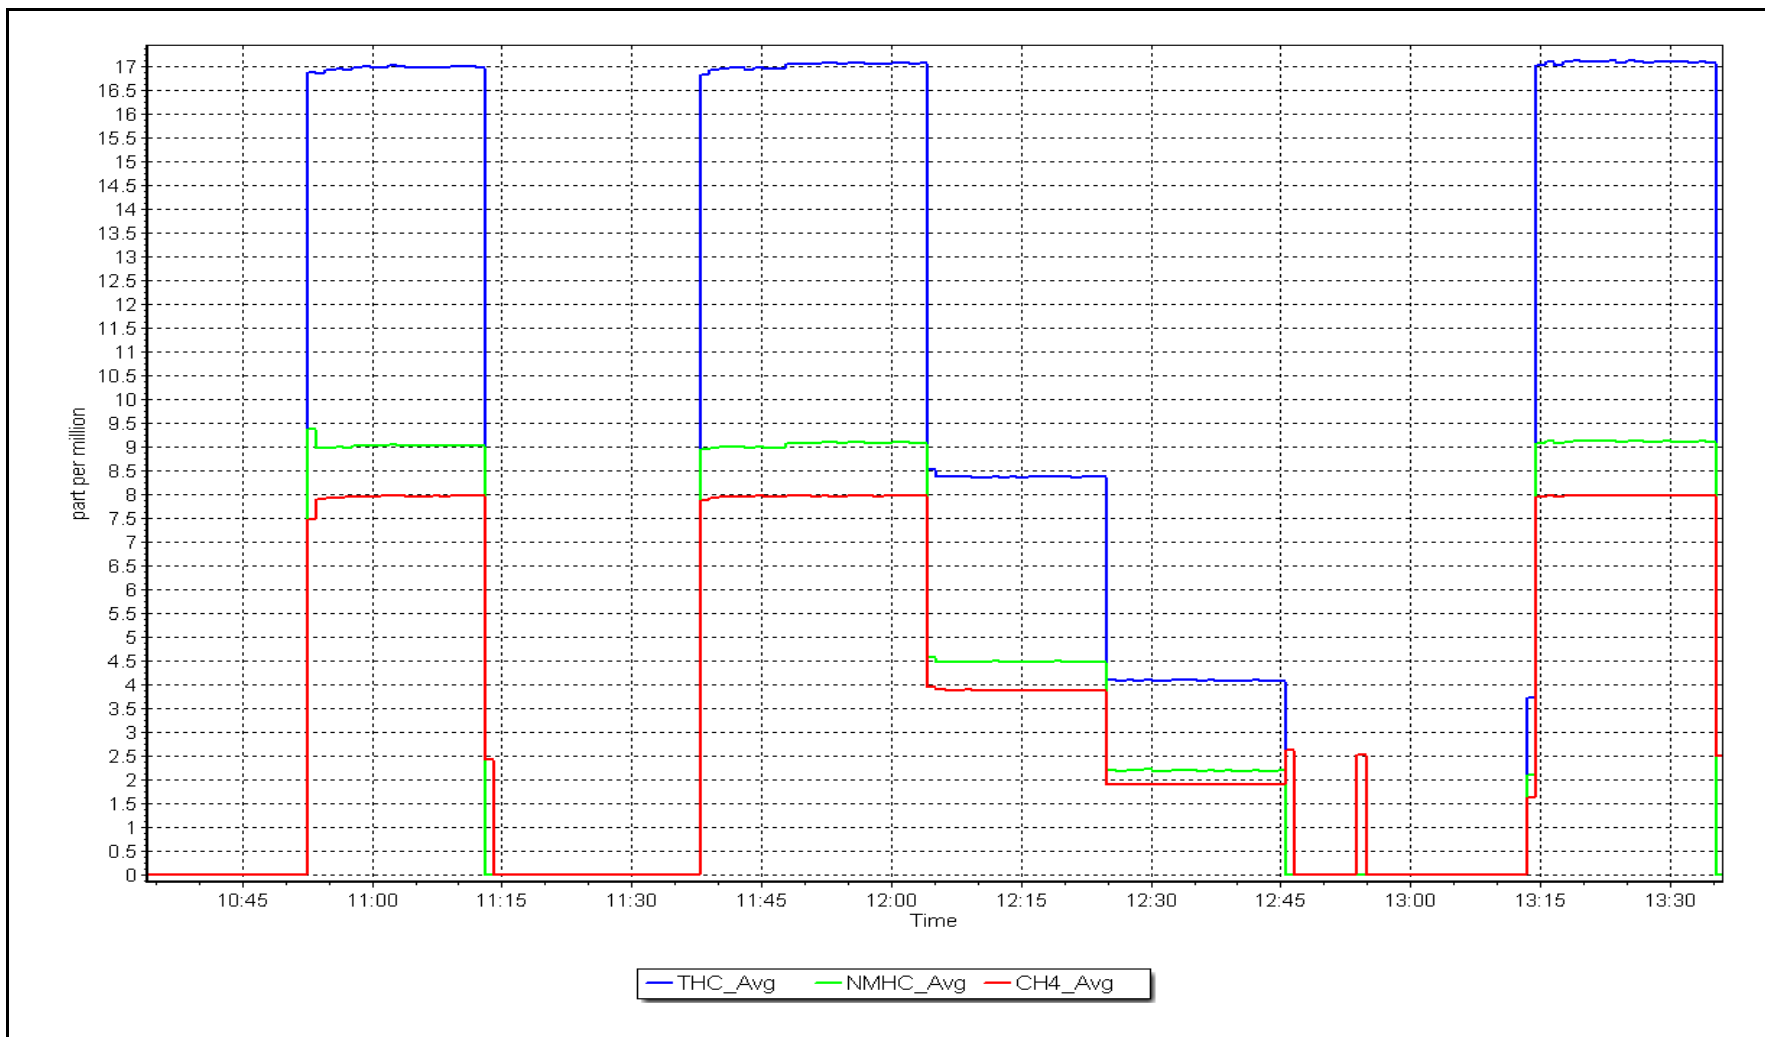



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Fort McKay South
Calibration Date: January 19, 2023
Start time (MST): 9:27
Reason: Routine
Station number: AMS 13
Last Cal Date: December 6, 2022
End time (MST): 13:58

Calibration Standards

NO Gas Cylinder #: T2Y1P76
NOX Cal Gas Conc: 50.98 ppm
Removed Cylinder #: N/A
Removed Gas NOX Conc: 50.98 ppm
NOX gas Diff:
Calibrator Model: API T700
ZAG make/model: API T701
Cal Gas Expiry Date: December 11, 2023
NO Cal Gas Conc: 49.32 ppm
Removed Gas Exp Date: N/A
Removed Gas NO Conc: 49.32 ppm
NO gas Diff:
Serial Number: 2448
Serial Number: 1117

Analyzer Information

Analyzer make: Thermo 42i
NOX Range (ppb): 0 - 1000 ppb
Analyzer serial #: 1410661329

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.182	1.200	NO bkgnd or offset:	9.4	9.6
NOX coeff or slope:	0.991	0.992	NOX bkgnd or offset:	9.4	9.6
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	195.3	194.1

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.000035	0.999594
NO _x Cal Offset:	-2.551182	-2.291272
NO Cal Slope:	1.003791	1.002005
NO Cal Offset:	-3.305357	-3.105090
NO ₂ Cal Slope:	0.996580	1.006533
NO ₂ Cal Offset:	-1.621259	-0.433464



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-0.2	-0.2	0.1	----	----
as found span	4919	81.1	826.9	800.0	26.9	815.1	787.2	28.0	1.0145	1.0162
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	-0.1	-0.1	0.1	----	----
high point	4919	81.1	826.9	800.0	26.9	825.3	799.9	25.2	1.0019	1.0001
second point	4960	40.6	413.9	400.4	13.5	410.5	396.8	13.7	1.0083	1.0091
third point	4980	20.3	207.0	200.2	6.7	202.3	194.4	8.0	1.0231	1.0300
as left zero	5000	0.0	0.0	0.0	0.0	-0.1	-0.2	0.1	----	----
as left span	4919	81.1	826.9	386.3	440.6	834.0	389.4	444.6	0.9915	0.9919
Average Correction Factor									1.0111	1.0131

Corrected As found	NO _x = 815.3 ppb	NO = 787.4 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -1.1%
Previous Response	NO _x = 824.4 ppb	NO = 799.7 ppb		*Percent Change	NO = -1.6%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	792.8	379.1	440.6	443.2	0.9942	100.6%
2nd GPT point (200 ppb O3)	792.8	585.3	234.4	235.8	0.9942	100.6%
3rd GPT point (100 ppb O3)	792.8	689.6	130.1	129.6	1.0040	99.6%
Average Correction Factor					0.9975	100.3%

Notes: Changed the inlet filter after as founds. Used 2nd NO reference point due to drift. Adjusted span only.

Calibration Performed By: Sean Bala



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 6, 2022
Station Name:	Fort McKay South	Station Number:	AMS 13
Start Time (MST):	9:27	End Time (MST):	13:58
Analyzer make:	Thermo 42i	Analyzer serial #:	1410661329

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	-0.1	----	Correlation Coefficient	≥0.995	
826.9	825.3	1.0019			
413.9	410.5	1.0083			
207.0	202.3	1.0231			
			Slope	0.999594	0.90 - 1.10
			Intercept	-2.291272	+/-20

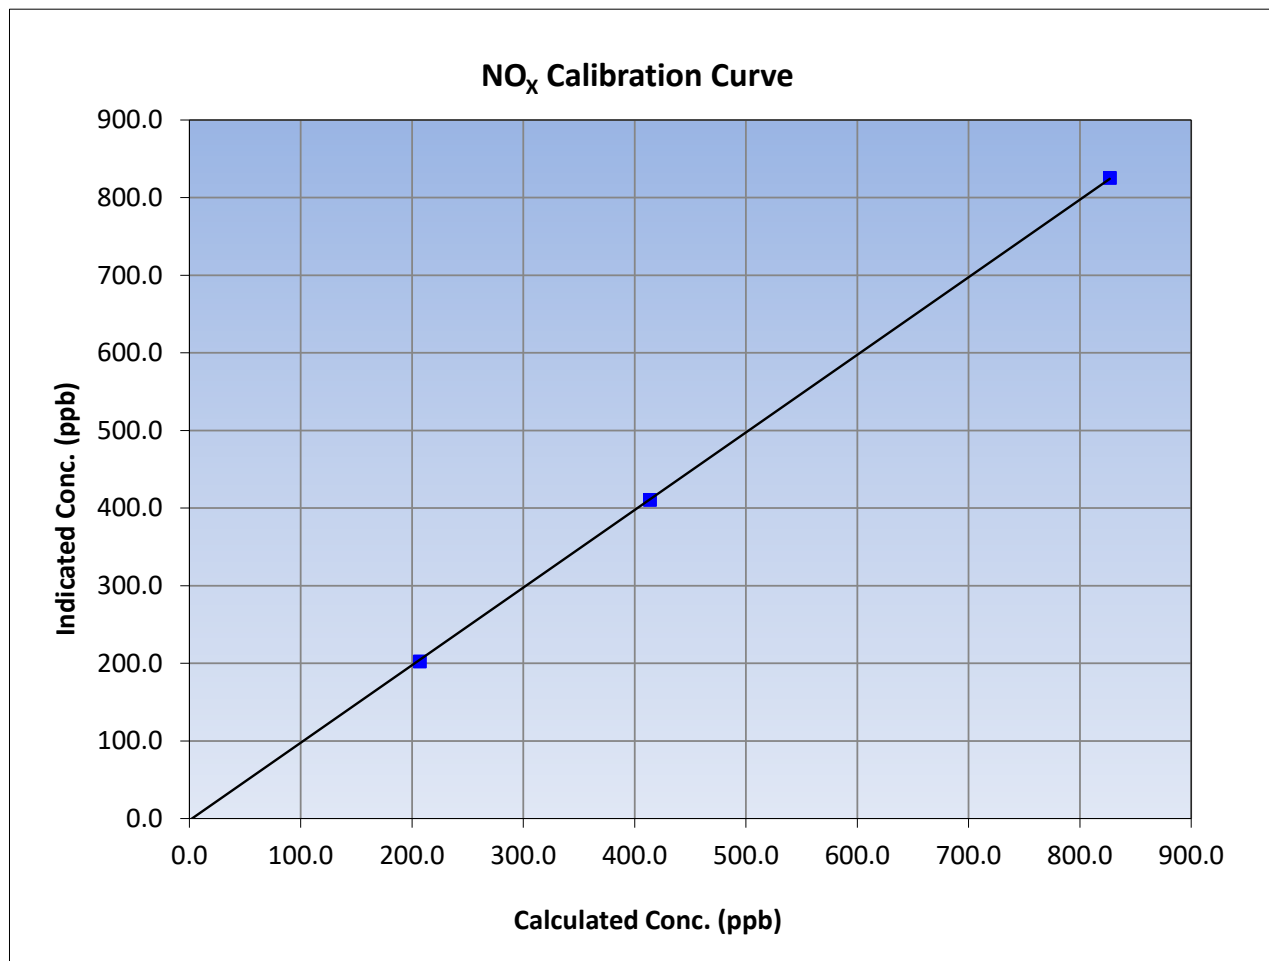



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 6, 2022
Station Name:	Fort McKay South	Station Number:	AMS 13
Start Time (MST):	9:27	End Time (MST):	13:58
Analyzer make:	Thermo 42i	Analyzer serial #:	1410661329

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	-0.1	----	Correlation Coefficient	0.999936	≥0.995
800.0	799.9	1.0001			
400.4	396.8	1.0091	Slope	1.002005	0.90 - 1.10
200.2	194.4	1.0300			
			Intercept	-3.105090	+/-20

NO Calibration Curve

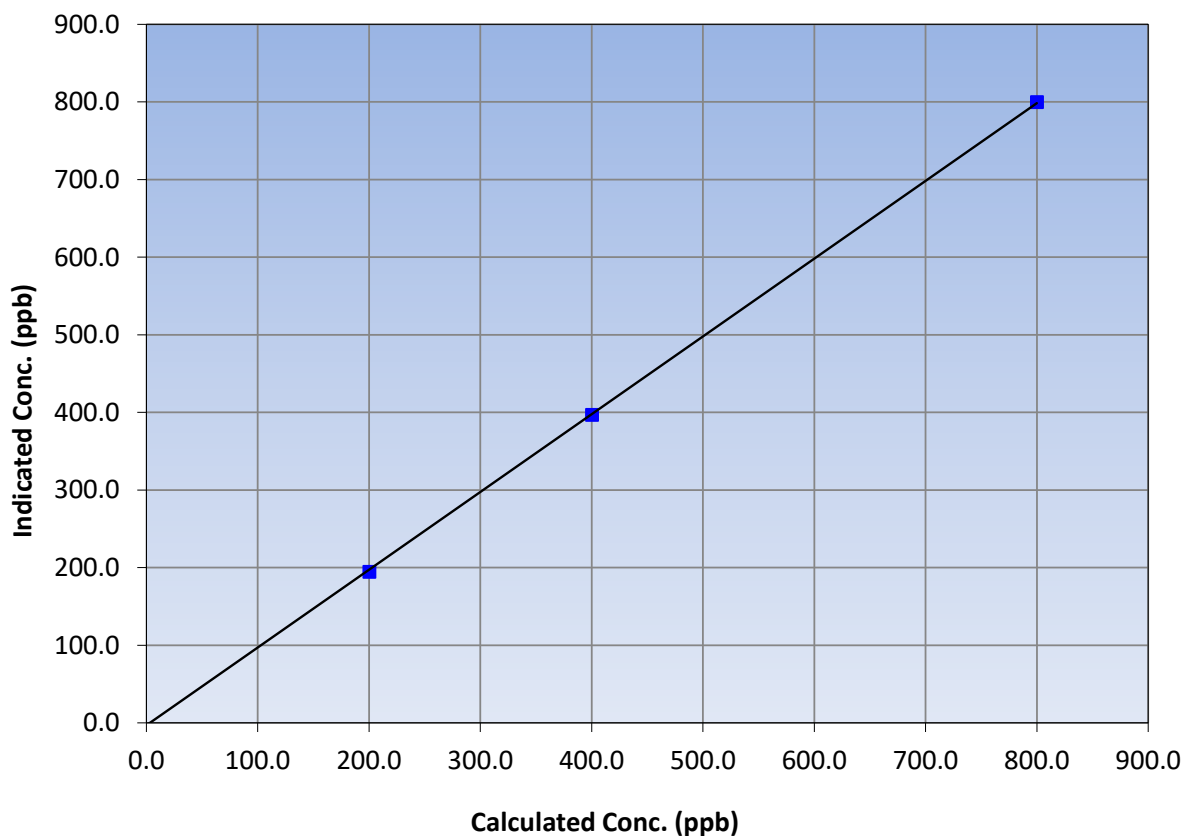



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 6, 2022
Station Name:	Fort McKay South	Station Number:	AMS 13
Start Time (MST):	9:27	End Time (MST):	13:58
Analyzer make:	Thermo 42i	Analyzer serial #:	1410661329

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
440.6	443.2	0.9942		
234.4	235.8	0.9942		
130.1	129.6	1.0040		
			0.999988	
			1.006533	
			-0.433464	


NO₂ Calibration Curve

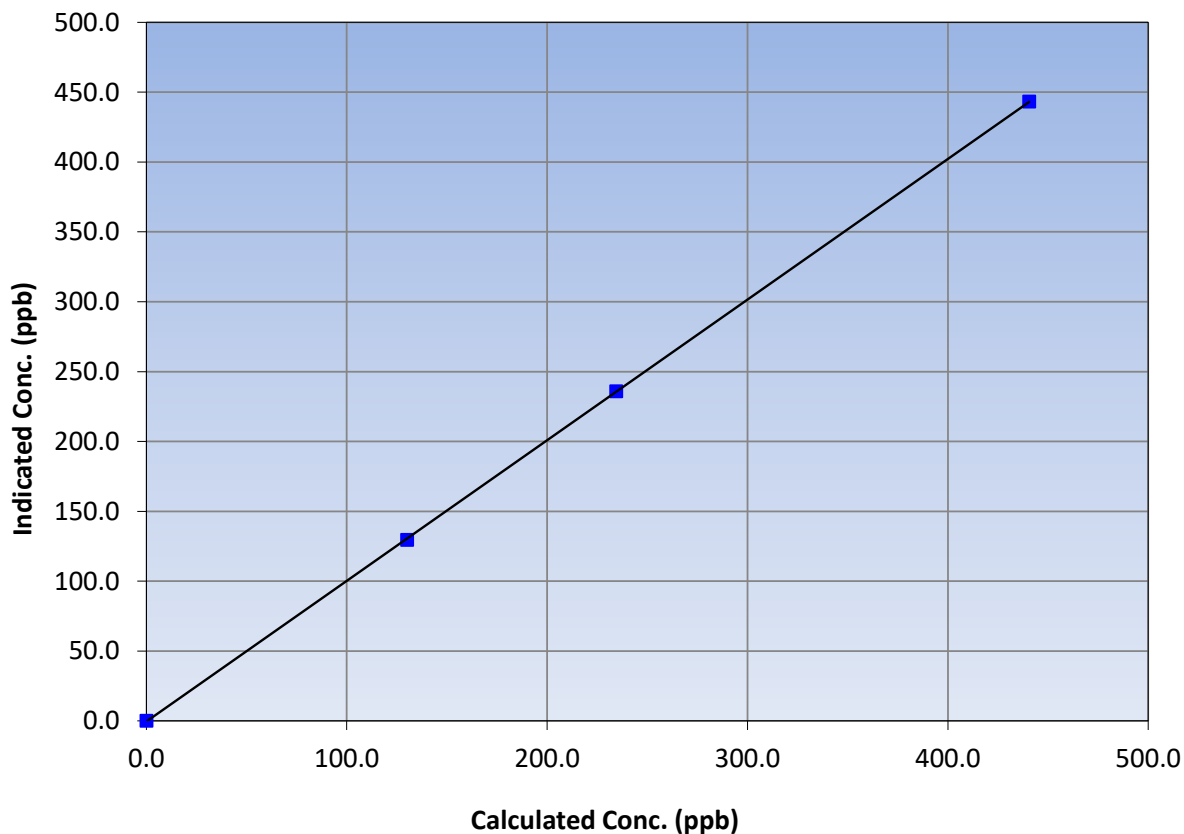

NO_x Calibration Plot

Date: January 19, 2023

Location: Fort McKay South

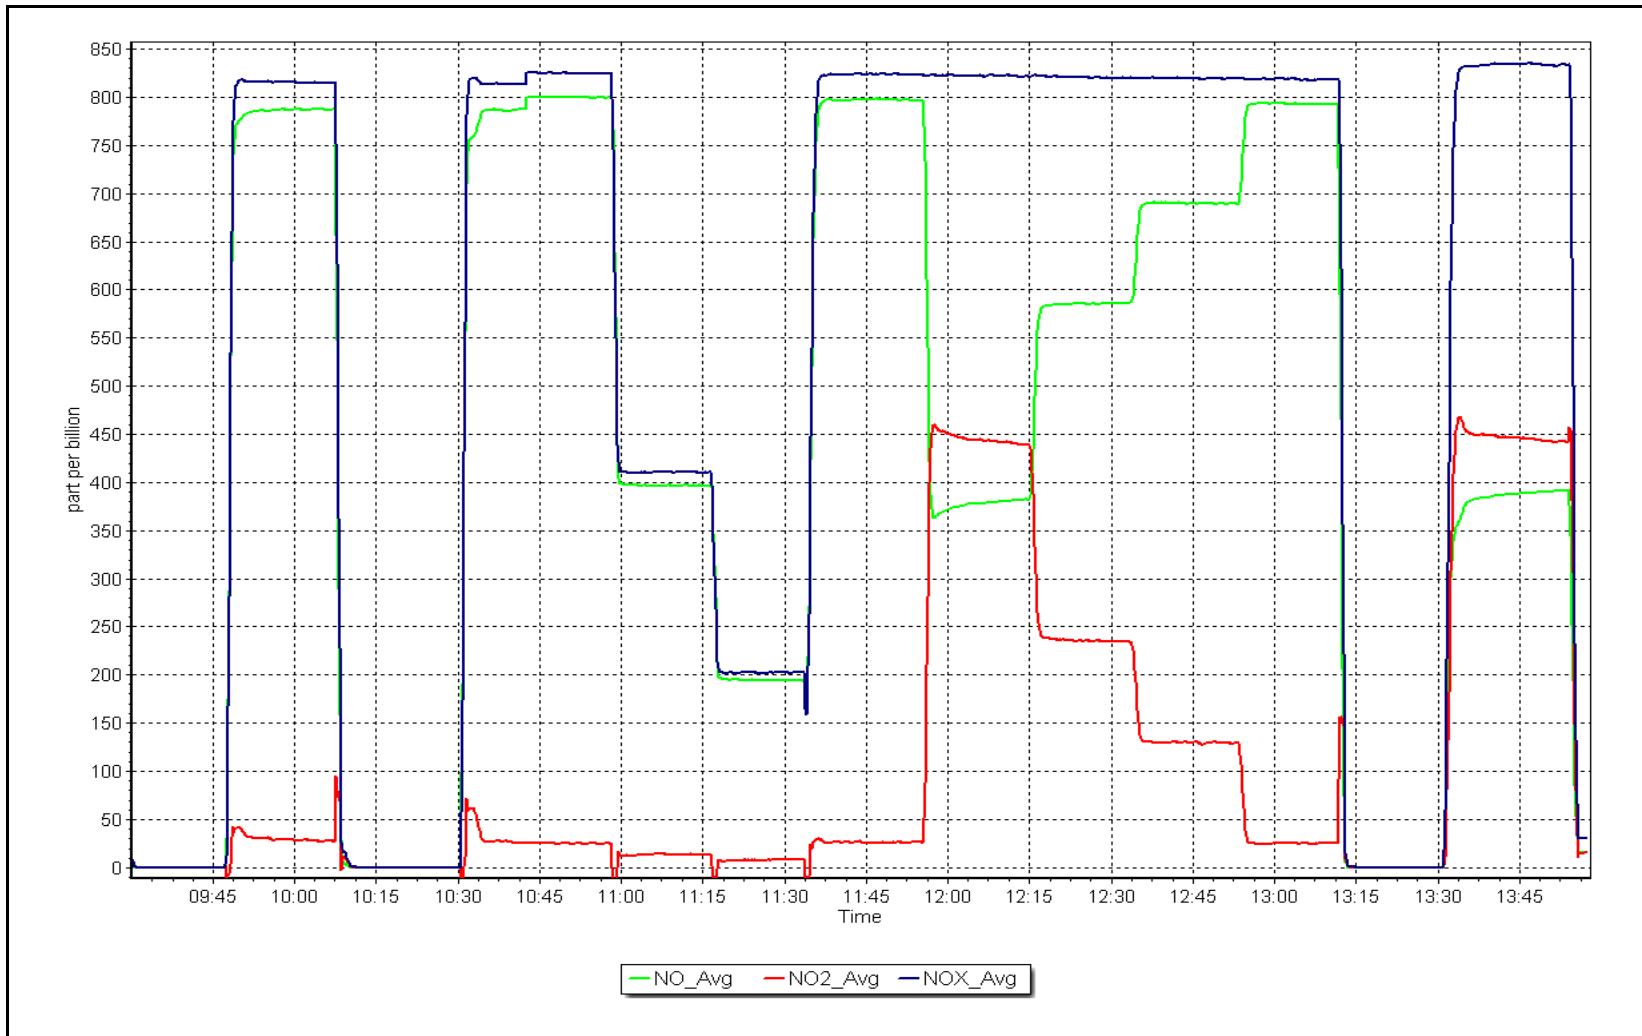



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Fort McKay South Station number: AMS13
 Calibration Date: January 18, 2023 Last Cal Date: December 1, 2022
 Start time (MST): 9:14 End time (MST): 12:25
 Reason: Routine

Calibration Standards

O3 generation mode: Photometer
 Calibrator Make/Model: Teledyne API T700 Serial Number: 2448
 ZAG Make/Model: Teledyne API T701 Serial Number: 1117

Analyzer Information

Analyzer make: Teledyne API T400 Analyzer serial #: 3871
 Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.000486	0.996143	Backgd or Offset:	2.7	2.7
Calibration intercept:	0.640000	1.300000	Coeff or Slope:	0.962	0.962

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	-0.1	----
as found span	5000	969.9	400.0	399.1	1.002
as found 2nd point					
as found 3rd point					
calibrator zero	5000	0.0	0.0	0.3	----
high point	5000	980.6	400.0	399.3	1.002
second point	5000	838.0	200.0	200.9	0.996
third point	5000	735.3	100.0	102.0	0.980
as left zero	5000	0.0	0.0	0.1	----
as left span	5000	979.1	400.0	401.8	0.996
Average Correction Factor					0.993

Baseline Corr As found:	399.2	Previous response	400.8	*% change	-0.4%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed inlet filter after as founds. No adjustment made.

Calibration Performed By: Sean Bala



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 18, 2023	Previous Calibration:	December 1, 2022
Station Name:	Fort McKay South	Station Number:	AMS13
Start Time (MST):	9:14	End Time (MST):	12:25
Analyzer make:	Teledyne API T400	Analyzer serial #:	3871

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	0.999971	≥0.995
400.0	399.3	1.0018			
200.0	200.9	0.9955	Slope	0.996143	0.90 - 1.10
100.0	102.0	0.9804			
			Intercept	1.300000	+/- 5

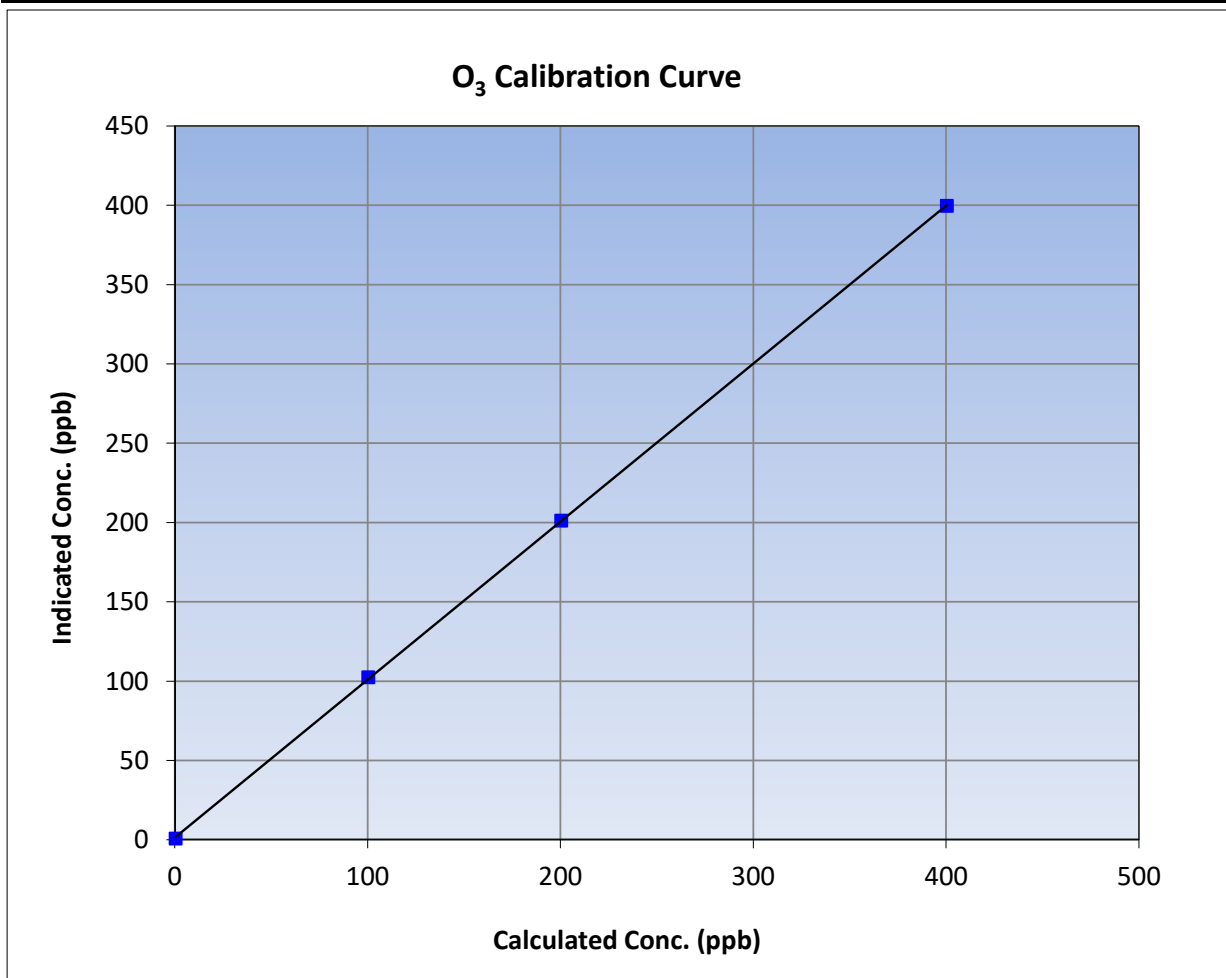

O₃ Calibration Plot

Date: January 18, 2023

Location: Fort McKay South

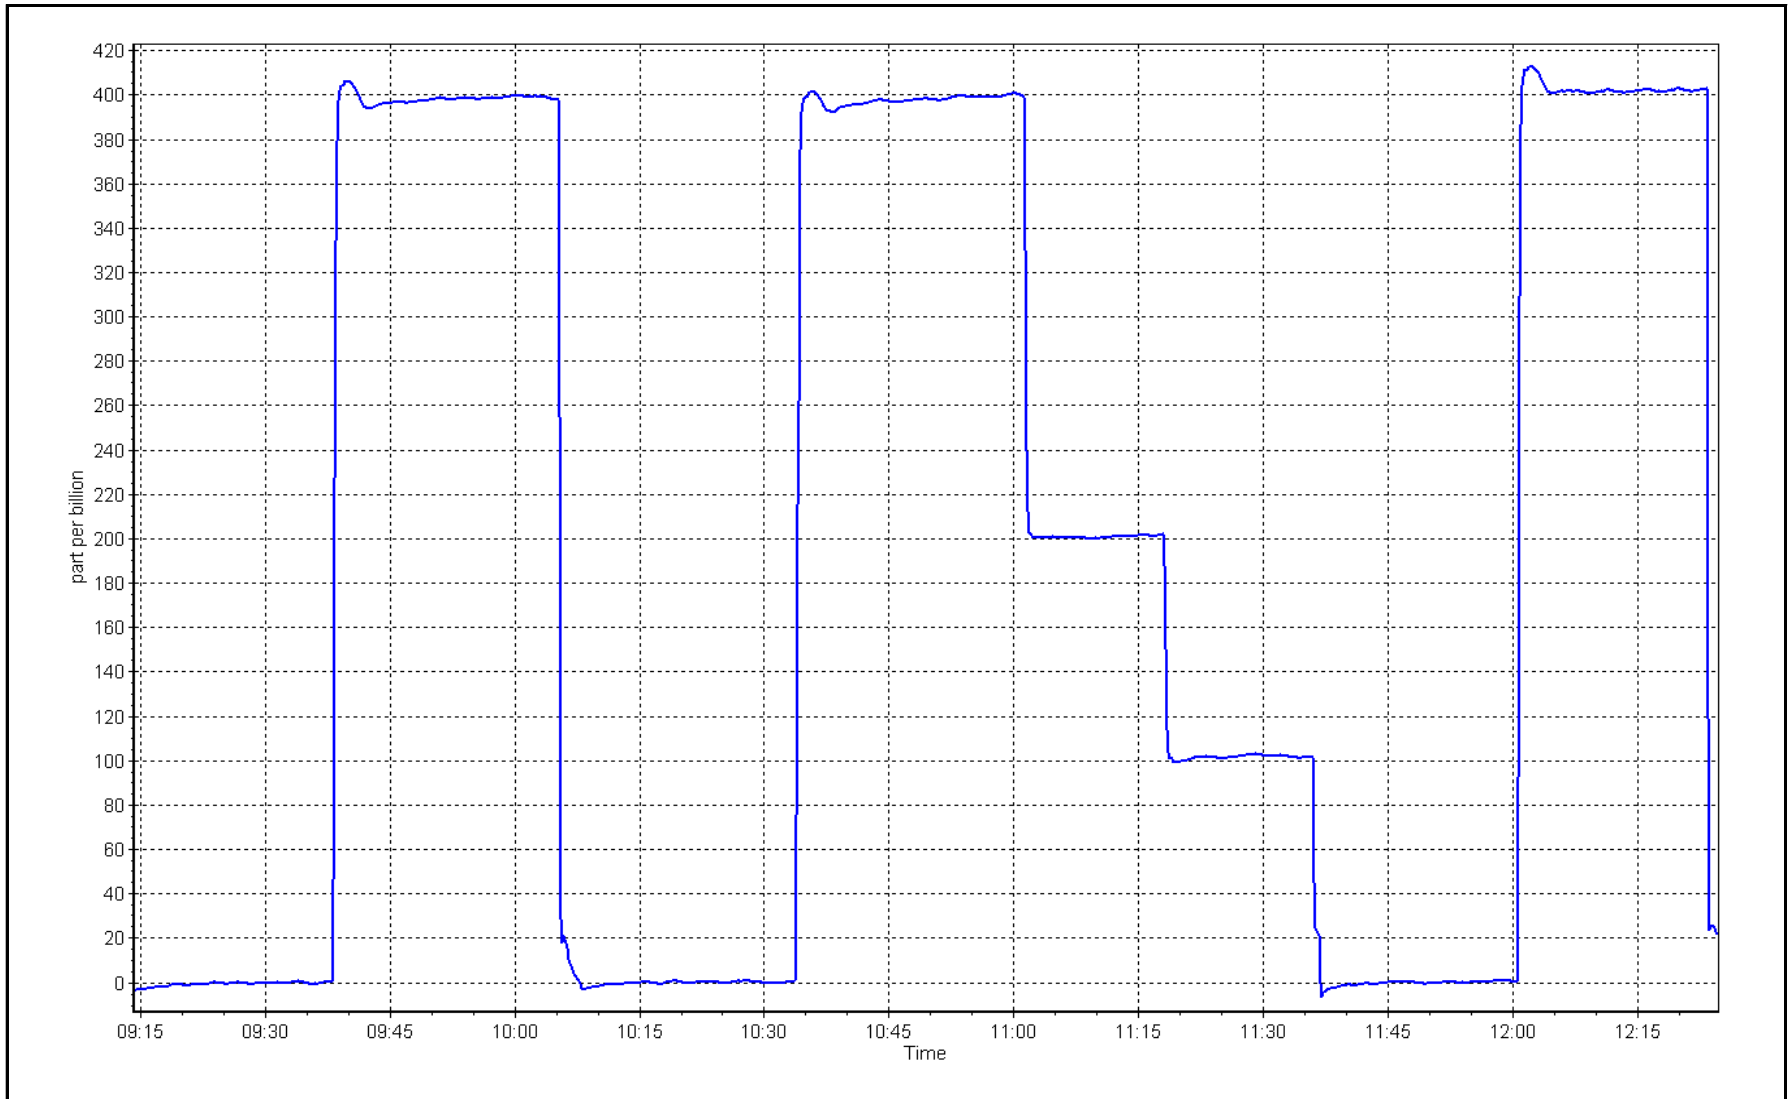



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Fort McKay South Station number: AMS 13
 Calibration Date: January 19, 2023 Last Cal Date: December 13, 2022
 Start time (MST): 10:49 End time (MST): 11:29

Analyzer Make: API T640 S/N: 319
 Particulate Fraction: PM2.5

Flow Meter Make/Model: Delta Cal S/N: 141229
 Temp/RH standard: Delta Cal S/N: 141229

Monthly Calibration Test

Parameter	As found	Measured	As left	Adjusted	(Limits)
T (°C)	-4.5	-4.7	-4.5	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	731.2	731.5	731.2	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	4.96	4.98	4.96	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 19, 2023 Last Cal Date: December 13, 2022
 PM w/o HEPA: 11.1 PM w/ HEPA: 0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

Parameter	As found	Measured	As left	Adjusted	(Limits)
PMT Peak Test				<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: December 13, 2022
 Disposable Filter Changed: December 13, 2022

Annual Maintenance

Date Sample Tube Cleaned: June 29, 2022
 Date RH/T Sensor Cleaned: June 29, 2022

Notes: No adjustment made. Leak check passed.

Calibration by: Sean Bala



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

**AMS14
ANZAC
JANUARY 2023**

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Anzac	Station number:	AMS 14
Calibration Date:	January 24, 2023	Last Cal Date:	December 6, 2022
Start time (MST):	7:30	End time (MST):	10:29
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.95	ppm	Cal Gas Exp Date:	January 5, 2025
Cal Gas Cylinder #:	CC279389			
Removed Cal Gas Conc:	49.95	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	5239
ZAG Make/Model:	API T701H		Serial Number:	357

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	0710321322
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.995082	0.998268	Backgd or Offset:	24.4	25.1
Calibration intercept:	-1.425034	-1.664595	Coeff or Slope:	0.784	0.795

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	-0.1	----
as found span	4920	80.1	800.2	787.4	1.016
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.2	----
high point	4920	80.1	800.2	798.0	1.003
second point	4960	40.0	399.6	396.5	1.008
third point	4980	20.0	199.8	195.8	1.020
as left zero	5000	0.0	0.0	0.2	----
as left span	4920	80.1	800.2	797.7	1.003
Average Correction Factor					1.010

Baseline Corr As found:	787.50	Previous response	794.82	*% change	-0.9%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: No maintenance done. Span adjusted.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 6, 2022
Station Name:	Anzac	Station Number:	AMS 14
Start Time (MST):	7:30	End Time (MST):	10:29
Analyzer make:	Thermo 43i	Analyzer serial #:	0710321322

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.2	----	Correlation Coefficient	0.999975	
800.2	798.0	1.0027			<i>≥0.995</i>
399.6	396.5	1.0078	Slope	0.998268	
199.8	195.8	1.0204			<i>0.90 - 1.10</i>
			Intercept	-1.664595	<i>+/-30</i>

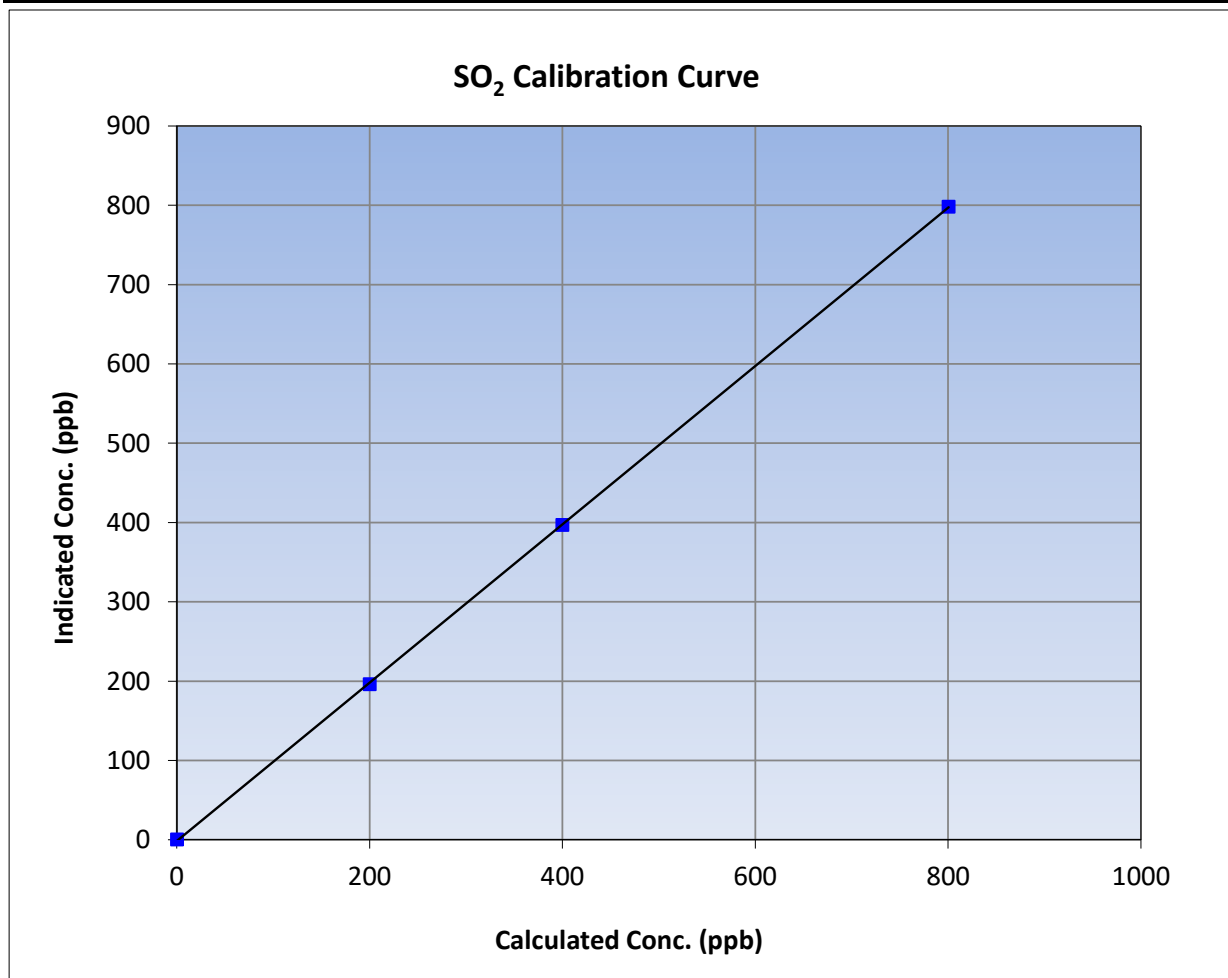

SO2 Calibration Plot

Date: January 24, 2023

Location: Anzac

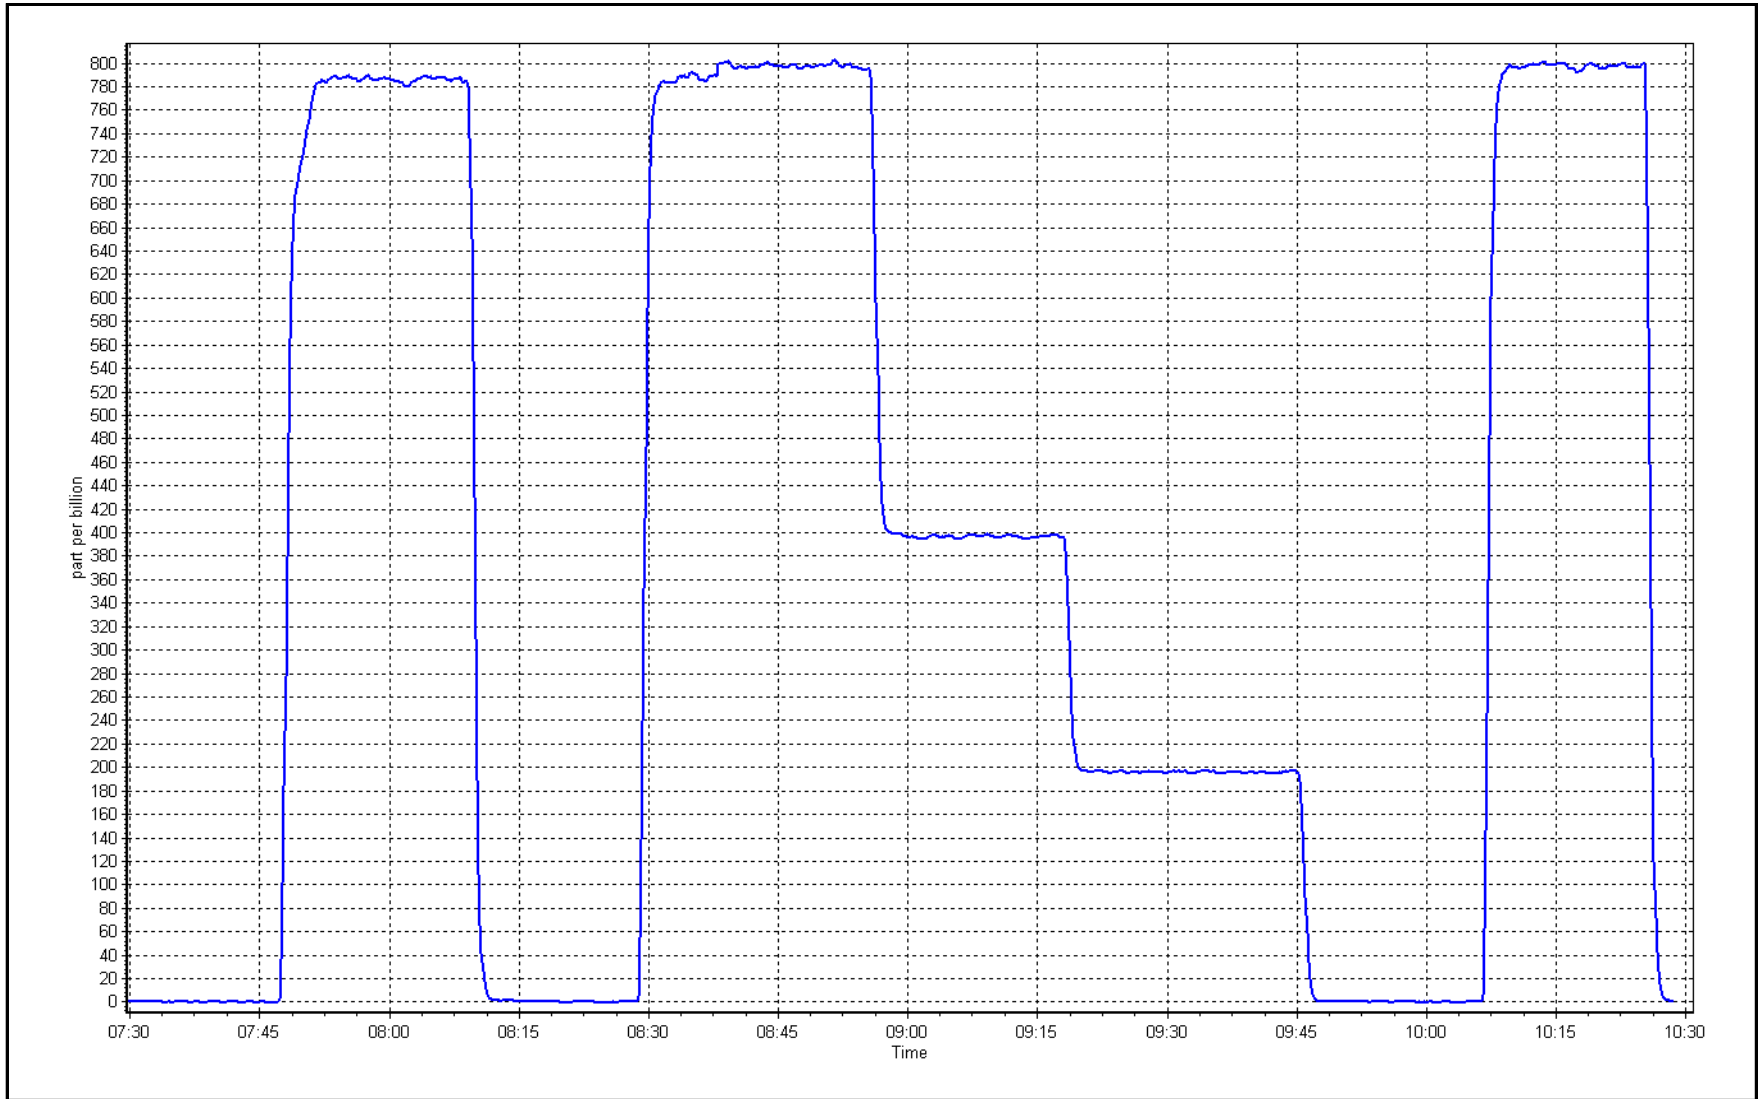



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name: Anzac Station number: AMS14
 Calibration Date: January 6, 2023 Last Cal Date: December 5, 2022
 Start time (MST): 7:45 End time (MST): 12:29
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.38 ppm Cal Gas Exp Date: February 3, 2023
 Cal Gas Cylinder #: EY0000859
 Removed Cal Gas Conc: 5.38 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 5252
 ZAG Make/Model: API 701H Serial Number: 357

Analyzer Information

Analyzer make: Thermo 43i-TLE Analyzer serial #: 1180540019
 Converter make: CD Nova CDN-101 Converter serial #: 503
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	1.002560	1.003842	Backgd or Offset:	5.61 5.54
Calibration intercept:	0.158711	0.038815	Coeff or Slope:	1.005 0.990

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.2	----
as found span	4925	74.3	80.0	81.4	0.985
as found 2nd point	4962	37.2	40.0	40.8	0.986
as found 3rd point	4981	18.6	20.0	20.0	1.011
new cylinder response					

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.3	----
high point	4925	74.3	80.0	80.4	0.995
second point	4962	37.2	40.0	40.2	0.996
third point	4981	18.6	20.0	19.8	1.011
as left zero	5000	0.0	0.0	0.4	----
as left span	4925	74.3	80.0	79.8	1.002
SO2 Scrubber Check	4920	80.0	800.0	0.0	----
Date of last scrubber change:				Ave Corr Factor	1.000
Date of last converter efficiency test:				efficiency	

Baseline Corr As found: 81.2 Prev response: 80.32 *% change: 1.1%
 Baseline Corr 2nd AF pt: 40.6 AF Slope: 1.017709 AF Intercept: -0.021532
 Baseline Corr 3rd AF pt: 19.8 AF Correlation: 0.999951

* = > +/-5% change initiates investigation

Notes: Scrubber checked after the calibrator zero. No maintenance done. Span adjusted.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 6, 2023	Previous Calibration:	December 5, 2022
Station Name:	Anzac	Station Number:	AMS14
Start Time (MST):	7:45	End Time (MST):	12:29
Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1180540019

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	0.999947	≥0.995
80.0	80.4	0.9945			
40.0	40.2	0.9959	Slope	1.003842	0.90 - 1.10
20.0	19.8	1.0109			
			Intercept	0.038815	+/-3

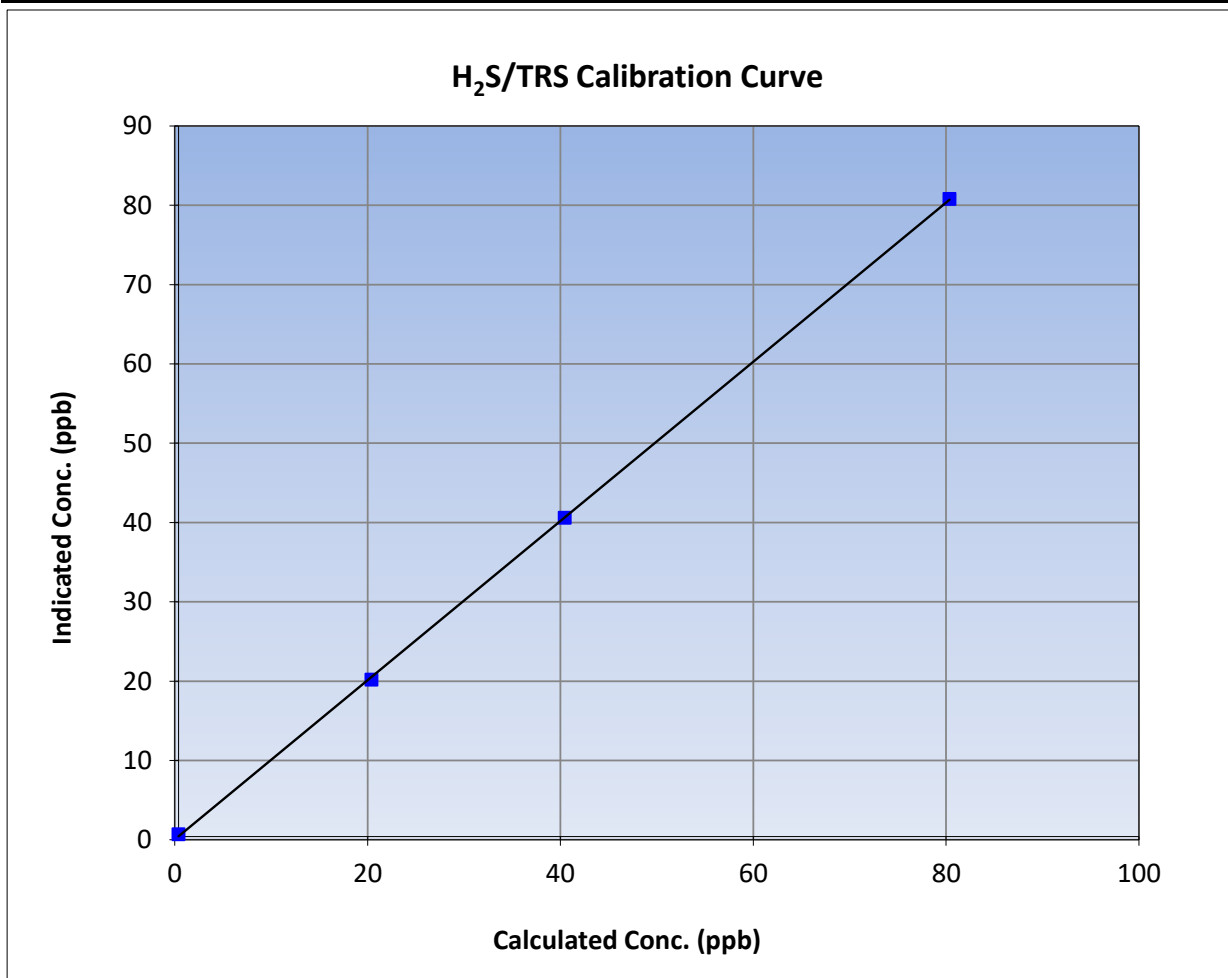

TRS Calibration Plot

Date: January 6, 2023

Location: Anzac

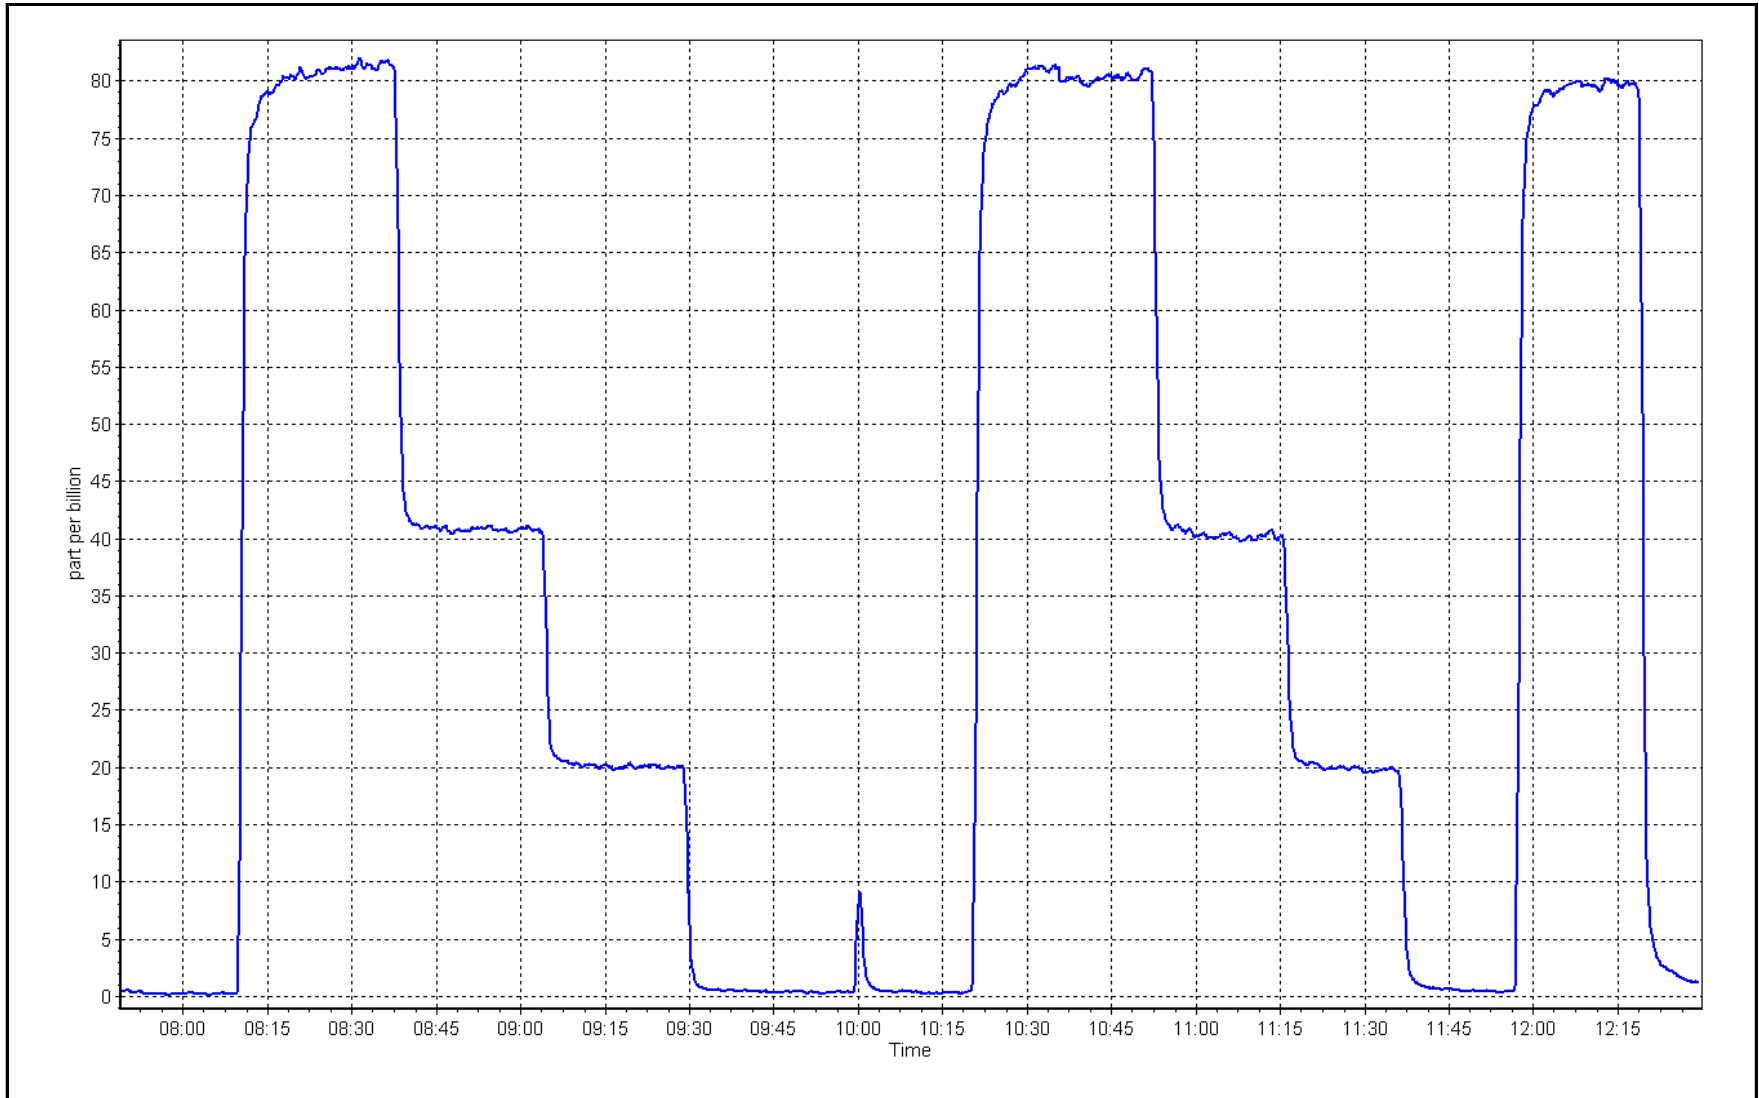



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Anzac	Station number:	AMS 14
Calibration Date:	January 23, 2023	Last Cal Date:	December 14, 2022
Start time (MST):	12:05	End time (MST):	15:15
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC279389	Cal Gas Expiry Date:	January 5, 2025
CH ₄ Cal Gas Conc.	499.3 ppm	CH ₄ Equiv Conc.	1068.8 ppm
C ₃ H ₈ Cal Gas Conc.	207.1 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	499.3 ppm	CH ₄ Equiv Conc.	1068.8 ppm
Removed C ₃ H ₈ Conc.	207.1 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	5252
ZAG make/model:	API 701H	Serial Number:	357

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1118148494
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	3.85E-04	3.85E-04	NMHC SP Ratio:	4.46E-05
CH ₄ Retention time:	12.00	12.00	NMHC Peak Area:	204554
				204554

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.1	17.12	17.17	0.997
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.1	17.12	17.13	1.000
second point	4960	40.0	8.55	8.57	0.998
third point	4980	20.0	4.28	4.25	1.007
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.1	17.12	17.17	0.997

Average Correction Factor				1.002
Baseline Corr AF:	17.17	Prev response	17.10	*% change 0.4%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.1	9.12	9.08	1.005
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.1	9.12	9.03	1.010
second point	4960	40.0	4.56	4.51	1.010
third point	4980	20.0	2.28	2.23	1.023
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.1	9.12	9.07	1.006
Average Correction Factor					1.014
Baseline Corr AF:	9.08	Prev response	9.12	*% change	-0.5%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.1	8.00	8.09	0.988
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.1	8.00	8.10	0.988
second point	4960	40.0	3.99	4.06	0.985
third point	4980	20.0	2.00	2.02	0.989
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.1	8.00	8.10	0.987
Average Correction Factor					0.987
Baseline Corr AF:	8.09	Prev response	7.98	*% change	1.4%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	0.998499	1.001116
THC Cal Offset:	0.004201	-0.010387
CH ₄ Cal Slope:	0.995993	1.012466
CH ₄ Cal Offset:	0.013958	0.001594
NMHC Cal Slope:	1.000697	0.991290
NMHC Cal Offset:	-0.009757	-0.011980

Notes:

N2 cylinder changed prior to calibration.

Calibration Performed By:

Denny Ray Estador



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 23, 2023	Previous Calibration:	December 14, 2022
Station Name:	Anzac	Station Number:	AMS 14
Start Time (MST):	12:05	End Time (MST):	15:15
Analyzer make:	Thermo 55i	Analyzer serial #:	1118148494

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999994	≥ 0.995			
17.12	17.13	0.9996						
8.55	8.57	0.9982				Slope	1.001116	0.90 - 1.10
4.28	4.25	1.0071						
			Intercept	-0.010387	± 0.5			

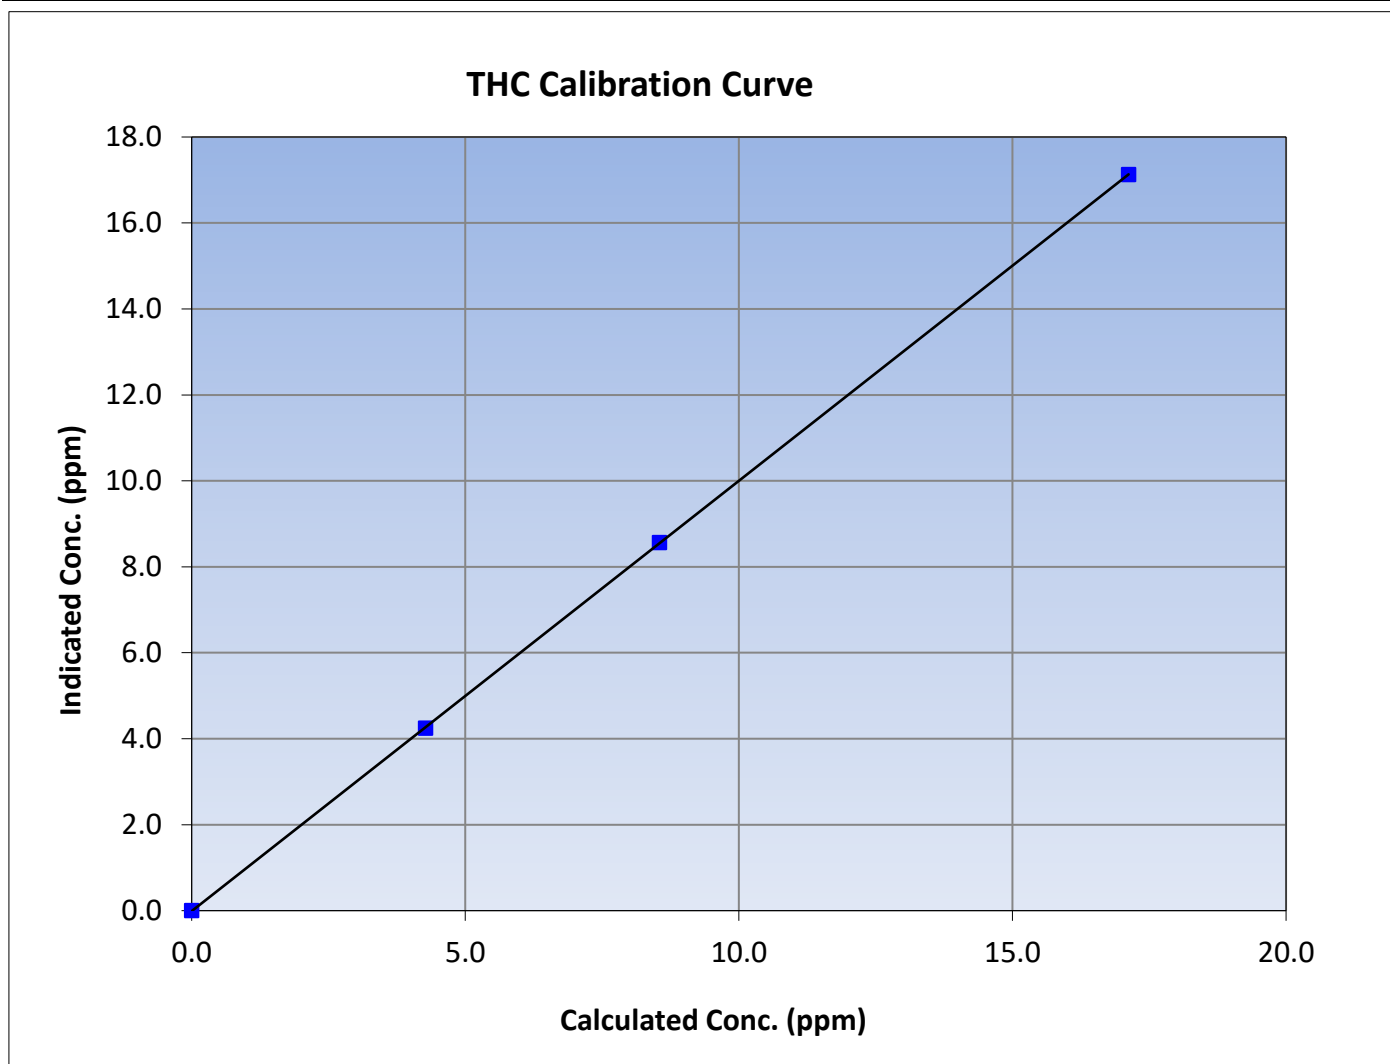



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 23, 2023	Previous Calibration:	December 14, 2022
Station Name:	Anzac	Station Number:	AMS 14
Start Time (MST):	12:05	End Time (MST):	15:15
Analyzer make:	Thermo 55i	Analyzer serial #:	1118148494

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999996	≥ 0.995
8.00	8.10	0.9880			
3.99	4.06	0.9848			
2.00	2.02	0.9892			
			Slope	1.012466	0.90 - 1.10
			Intercept	0.001594	+/-0.5

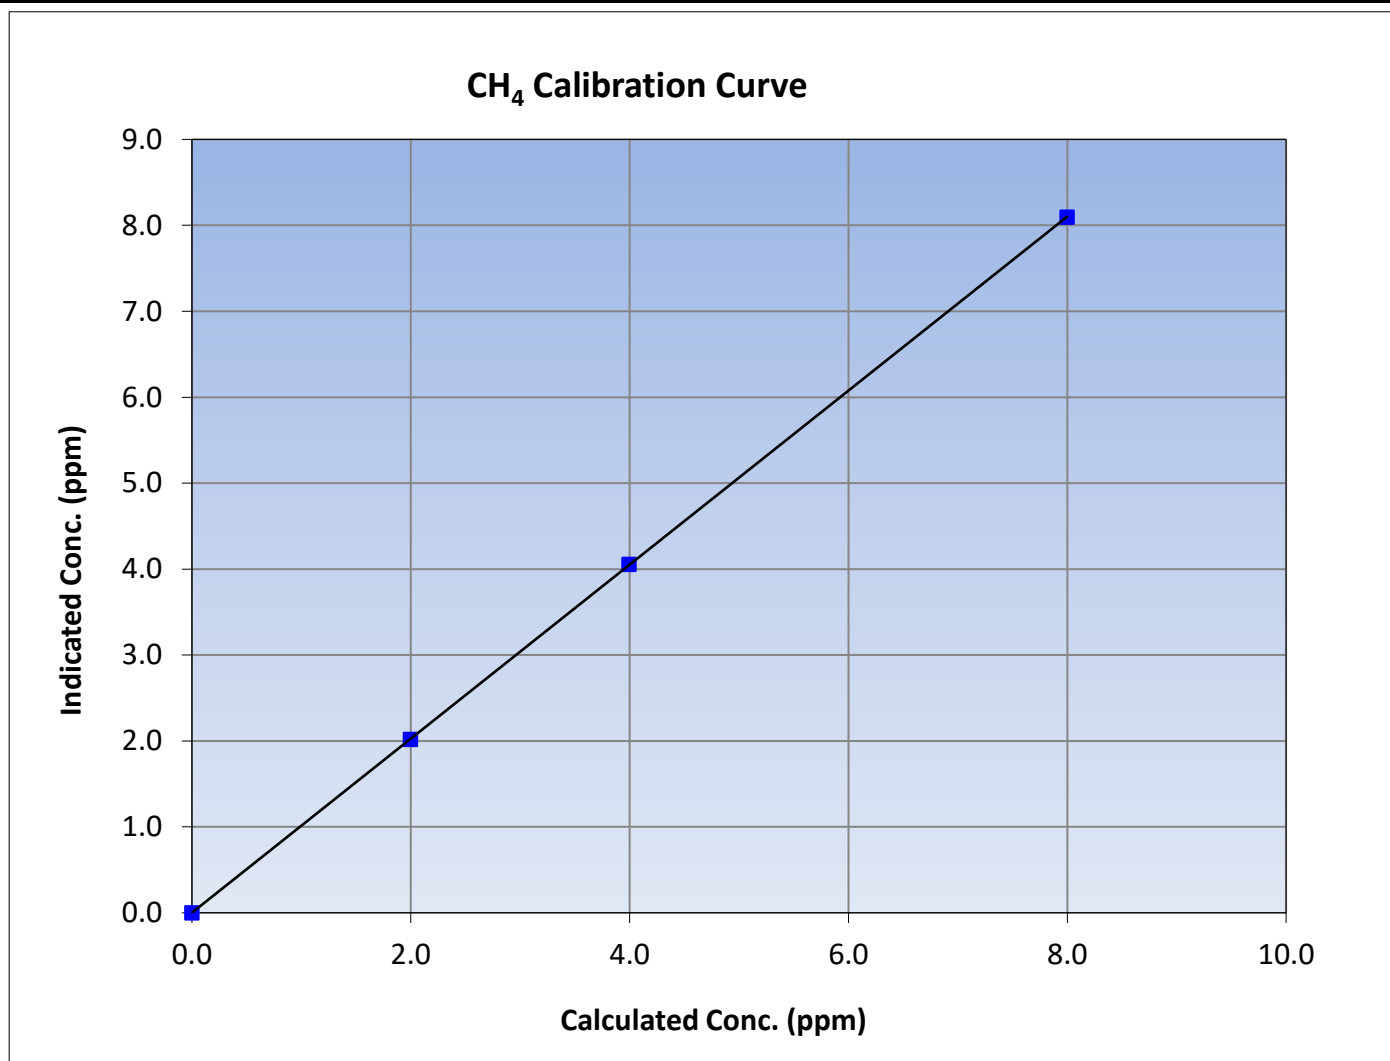



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 23, 2023	Previous Calibration:	December 14, 2022
Station Name:	Anzac	Station Number:	AMS 14
Start Time (MST):	12:05	End Time (MST):	15:15
Analyzer make:	Thermo 55i	Analyzer serial #:	1118148494

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999987	≥ 0.995			
9.12	9.03	1.0099						
4.56	4.51	1.0100				Slope	0.991290	0.90 - 1.10
2.28	2.23	1.0234						
			Intercept	-0.011980	± 0.5			

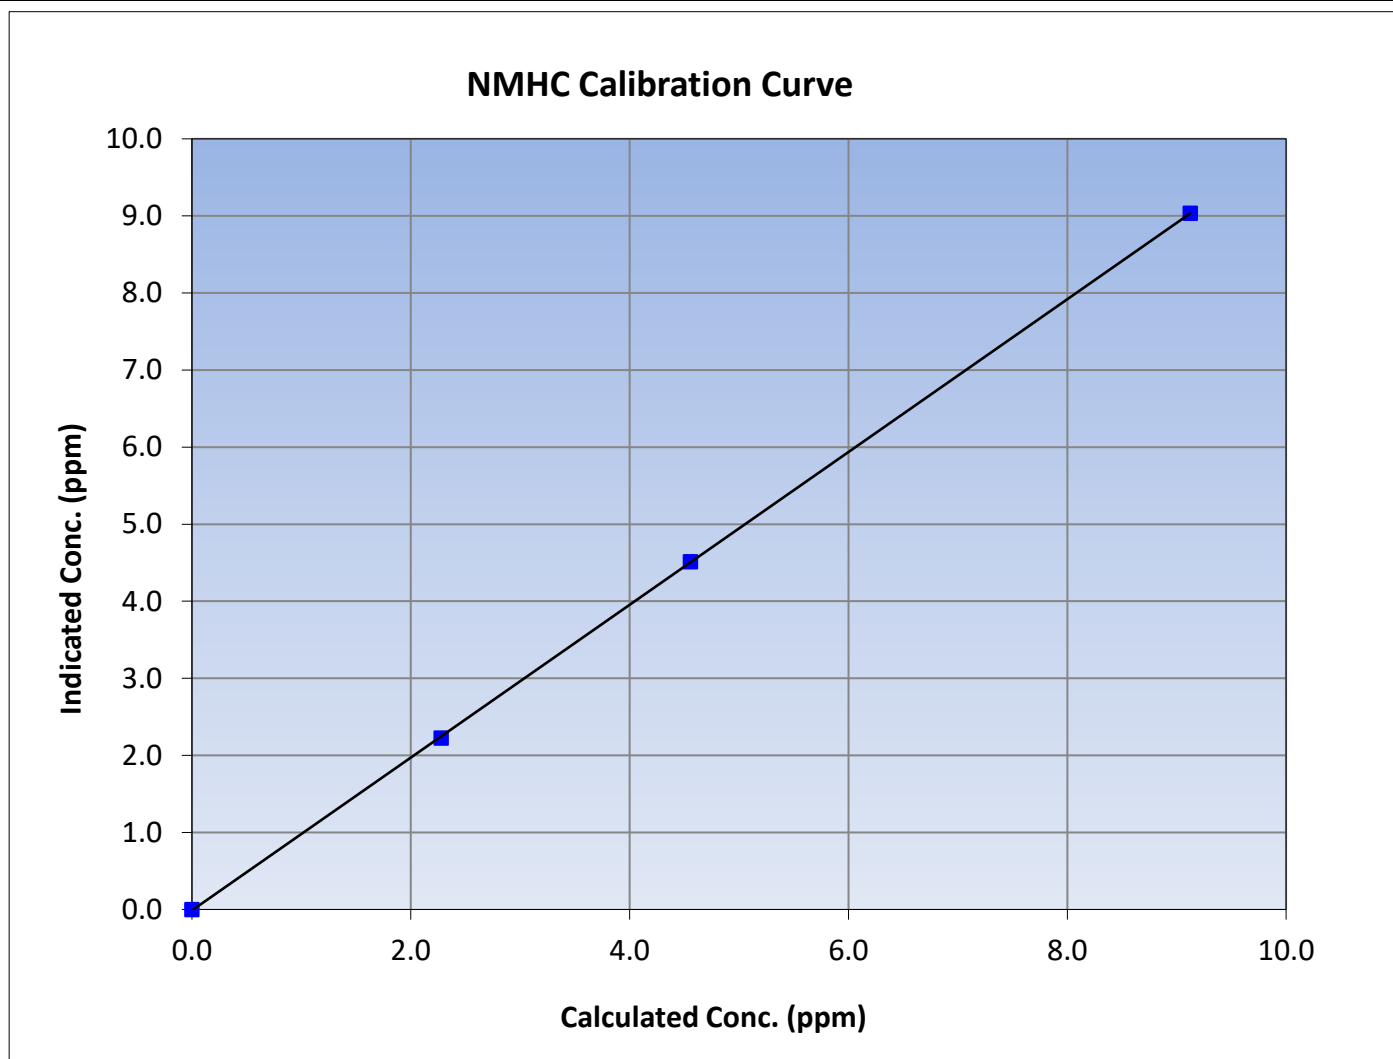

NMHC Calibration Plot

Date: January 23, 2023

Location: Anzac

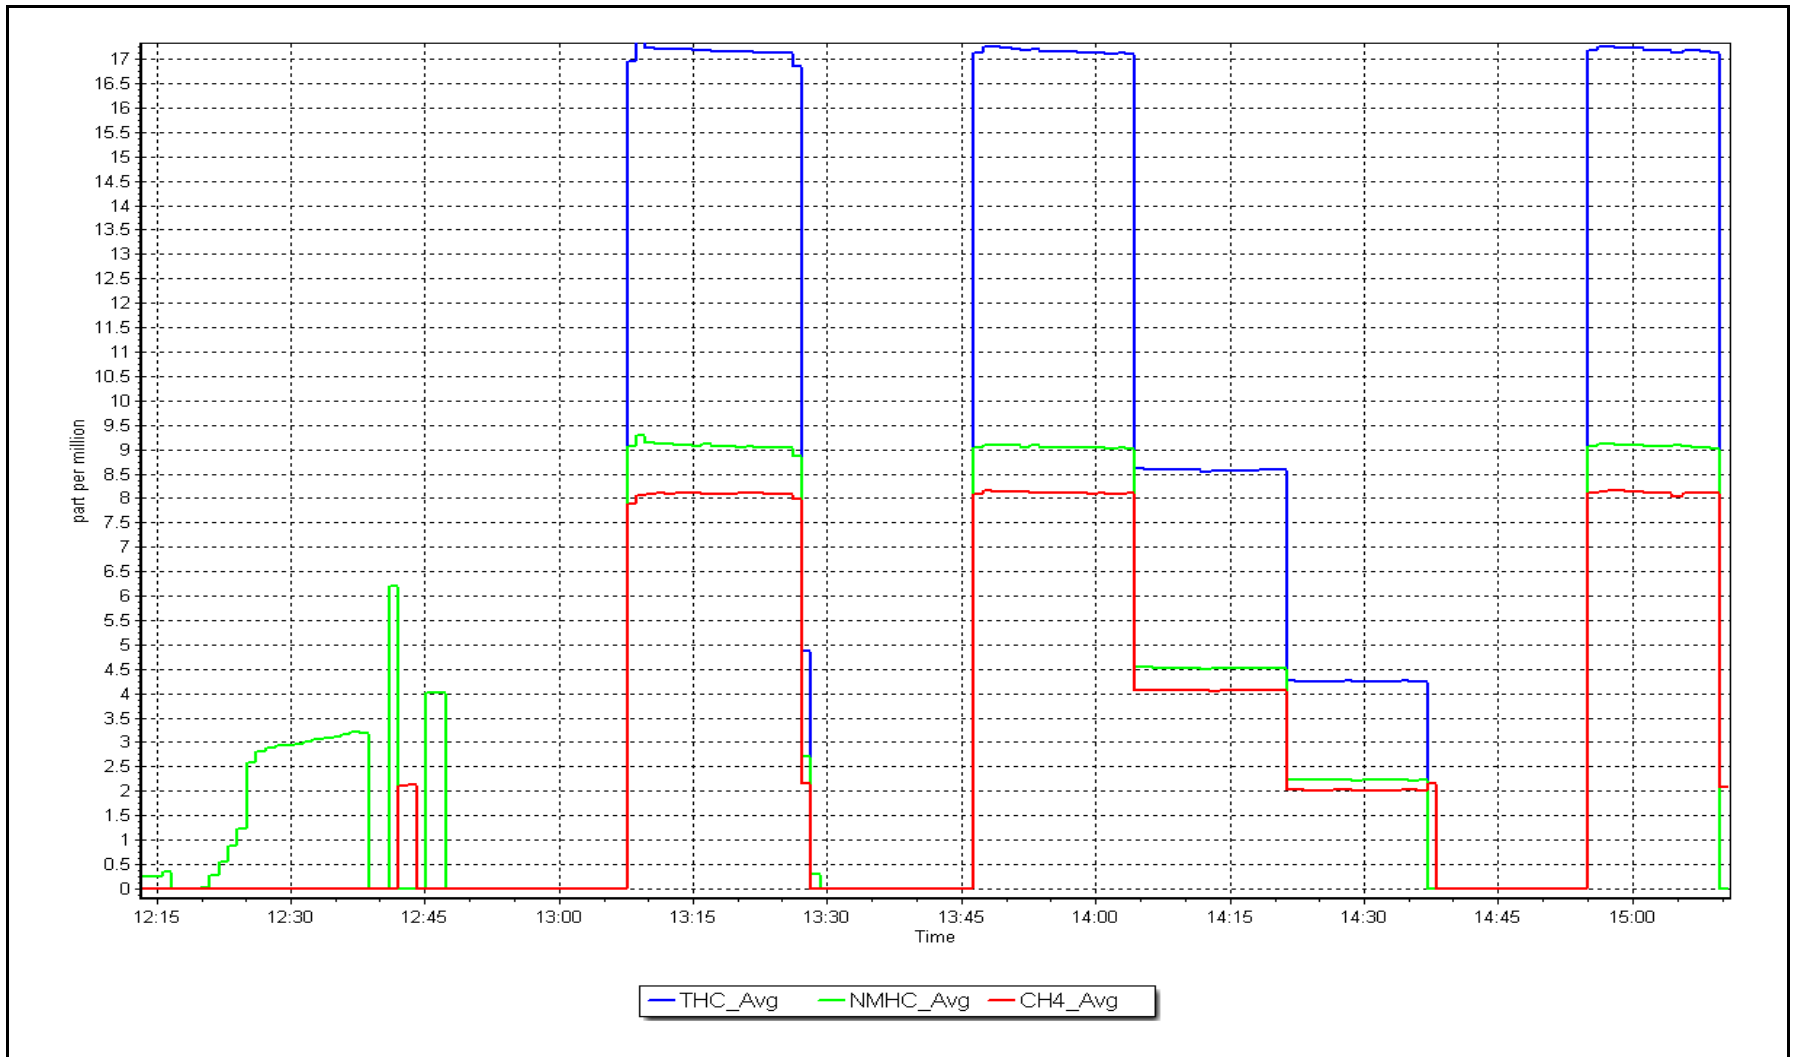



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Anzac	Station number:	AMS 14
Calibration Date:	January 31, 2023	Last Cal Date:	January 23, 2023
Start time (MST):	7:37	End time (MST):	8:52
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC279389	Cal Gas Expiry Date:	January 5, 2025
CH ₄ Cal Gas Conc.	499.3 ppm	CH ₄ Equiv Conc.	1068.8 ppm
C ₃ H ₈ Cal Gas Conc.	207.1 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	499.3 ppm	CH ₄ Equiv Conc.	1068.8 ppm
Removed C ₃ H ₈ Conc.	207.1 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	5252
ZAG make/model:	API 701H	Serial Number:	357

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1118148494
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	3.85E-04	3.85E-04	NMHC SP Ratio:	4.46E-05
CH ₄ Retention time:	12.00	12.00	NMHC Peak Area:	204554
				204554

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.1	17.12	17.09	1.002
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.1	17.12	17.02	1.006
second point					
third point					
as left zero					
as left span					

				Average Correction Factor	1.006
Baseline Corr AF:	17.09	Prev response	17.13	*% change	-0.2%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.1	9.12	9.06	1.007
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.1	9.12	9.04	1.009
second point					
third point					
as left zero					
as left span					
				Average Correction Factor	1.009
Baseline Corr AF:	9.06	Prev response	9.03	*% change	0.3%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.1	8.00	8.03	0.996
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.1	8.00	7.98	1.002
second point					
third point					
as left zero					
as left span					
				Average Correction Factor	1.002
Baseline Corr AF:	8.03	Prev response	8.10	*% change	-0.9%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	1.001116	0.994029
THC Cal Offset:	-0.010387	0.000000
CH ₄ Cal Slope:	1.012466	0.997671
CH ₄ Cal Offset:	0.001594	0.000000
NMHC Cal Slope:	0.991290	0.990836
NMHC Cal Offset:	-0.011980	0.000000


Notes: Hydrogen Cylinder change

Calibration Performed By: Melissa Lemay

NMHC Calibration Plot

Date: January 31, 2023

Location: Anzac

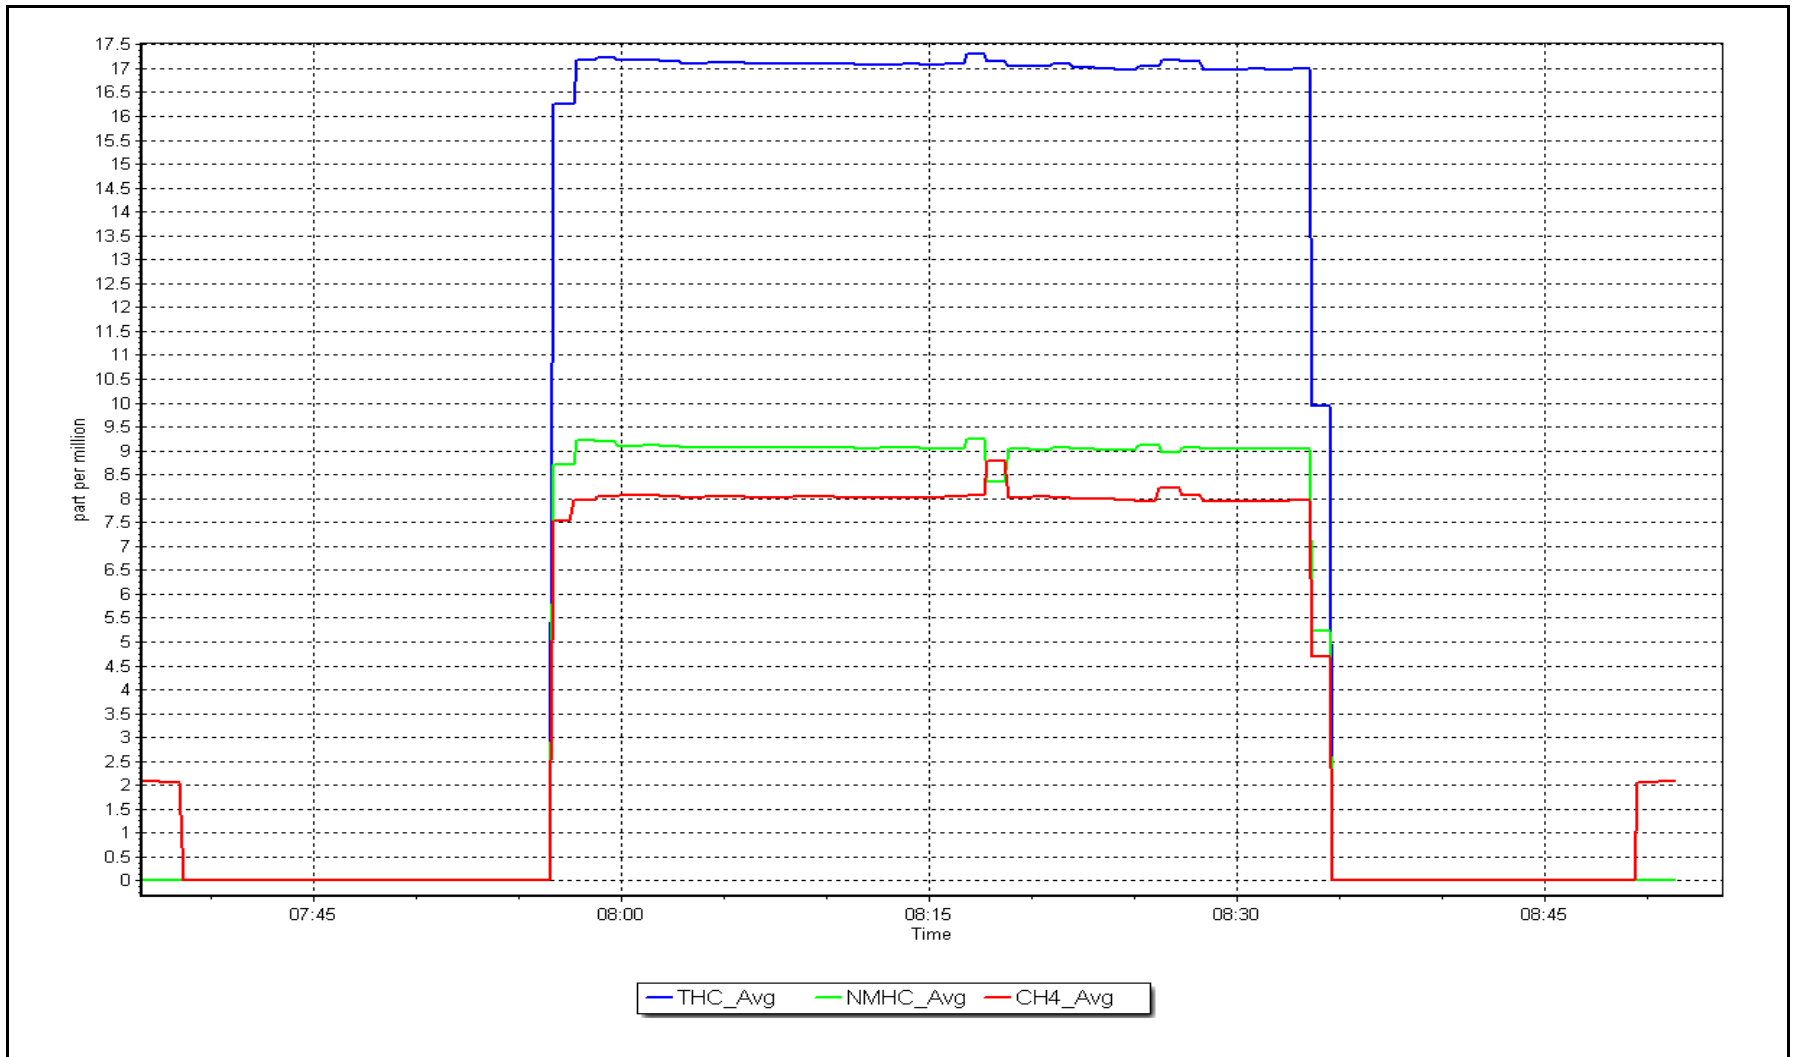



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Anzac Station number: AMS 14
Calibration Date: January 4, 2023 Last Cal Date: December 2, 2022
Start time (MST): 7:35 End time (MST): 12:31
Reason: Routine

Calibration Standards

NO Gas Cylinder #: T2Y1P8D Cal Gas Expiry Date: December 11, 2023
NOX Cal Gas Conc: 50.92 ppm NO Cal Gas Conc: 50.05 ppm
Removed Cylinder #: NA Removed Gas Exp Date: NA
Removed Gas NOX Conc: 50.92 ppm Removed Gas NO Conc: 50.05 ppm
NOX gas Diff: NO gas Diff:
Calibrator Model: Teledyne API T700 Serial Number: 5239
ZAG make/model: Teledyne API 701H Serial Number: 357

Analyzer Information

Analyzer make: Thermo 42i Analyzer serial #: 1426262592
NOX Range (ppb): 0 - 1000 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.361	1.361	NO bkgnd or offset:	3.7	3.7
NOX coeff or slope:	0.996	0.996	NOX bkgnd or offset:	3.7	3.7
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	161.8	163.3

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.002403	0.999876
NO _x Cal Offset:	-1.205267	-0.745750
NO Cal Slope:	1.003086	1.001401
NO Cal Offset:	-2.069261	-1.789671
NO ₂ Cal Slope:	1.000735	1.002246
NO ₂ Cal Offset:	0.178927	0.204305



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.0	-0.2	0.2	----	----
as found span	4921	78.6	800.5	786.8	13.7	800.8	785.7	15.1	0.9997	1.0015
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.1	0.2	-0.1	----	----
high point	4921	78.6	800.5	786.8	13.7	799.9	787.0	12.9	1.0008	0.9998
second point	4961	39.3	400.2	393.4	6.8	399.6	391.6	8.0	1.0015	1.0045
third point	4980	19.6	199.6	196.2	3.4	197.6	192.4	5.3	1.0102	1.0198
as left zero	5000	0.0	0.0	0.0	0.0	0.1	-0.1	0.2	----	----
as left span	4921	78.6	800.5	392.6	407.9	797.7	388.4	409.3	1.0035	1.0109
Average Correction Factor									1.0042	1.0080

Corrected As found	NO _x = 800.8 ppb	NO = 785.9 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -0.1%	
Previous Response	NO _x = 801.2 ppb	NO = 787.2 ppb		*Percent Change	NO = -0.2%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO ₂)						
as found GPT point (200 ppb NO ₂)						
as found GPT point (100 ppb NO ₂)						
1st GPT point (400 ppb O ₃)	781.8	387.6	407.9	408.9	0.9975	100.3%
2nd GPT point (200 ppb O ₃)	781.8	582.4	213.1	213.7	0.9971	100.3%
3rd GPT point (100 ppb O ₃)	781.8	681.5	114.0	114.9	0.9920	100.8%
Average Correction Factor					0.9955	100.5%

Notes:

No maintenance or adjustments done.

Melissa Lemay



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 2, 2022
Station Name:	Anzac	Station Number:	AMS 14
Start Time (MST):	7:35	End Time (MST):	12:31
Analyzer make:	Thermo 42i	Analyzer serial #:	1426262592

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
800.5	799.9	1.0008		
400.2	399.6	1.0015		
199.6	197.6	1.0102		

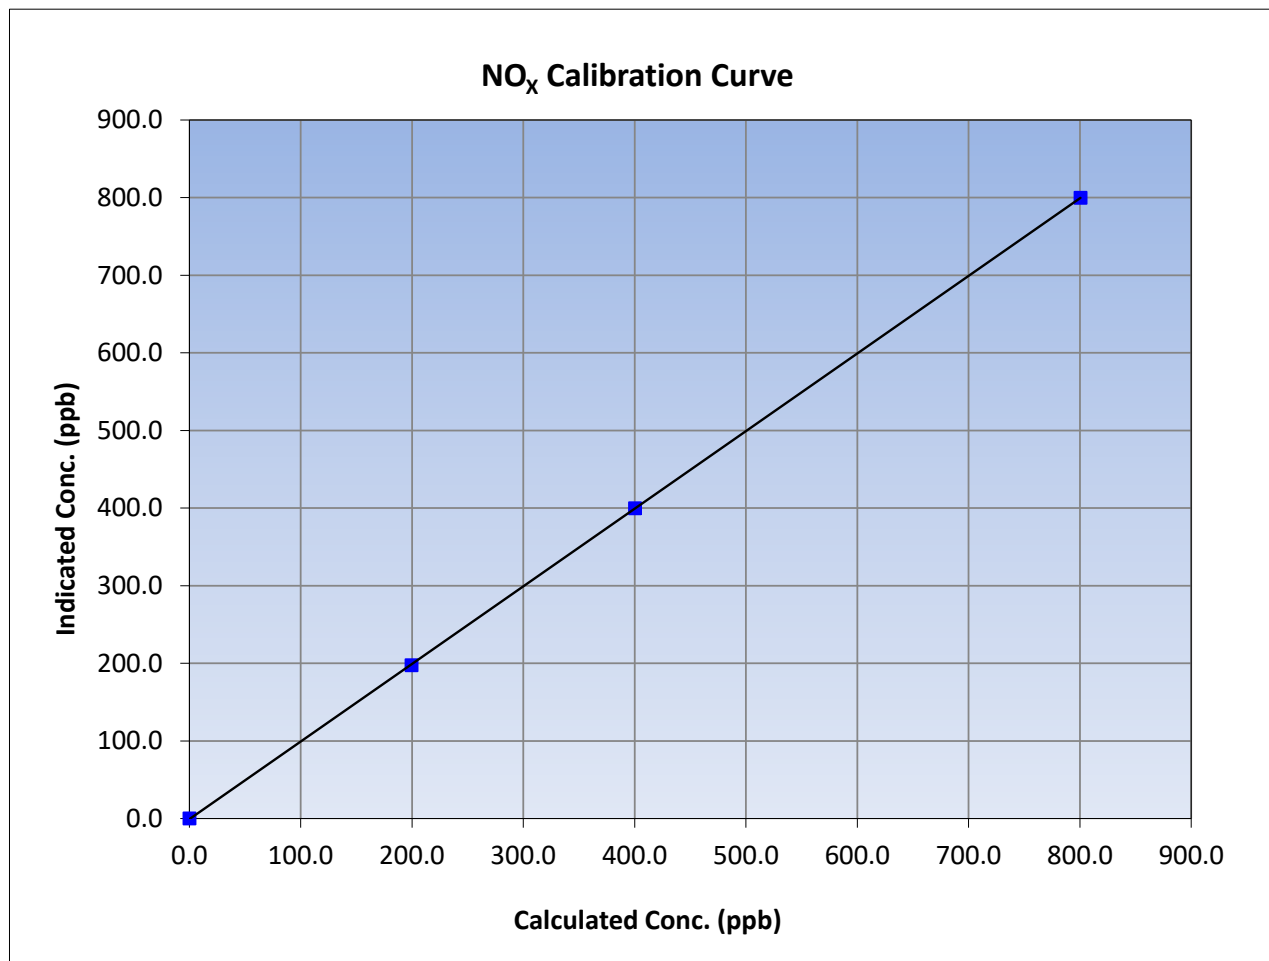



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 2, 2022
Station Name:	Anzac	Station Number:	AMS 14
Start Time (MST):	7:35	End Time (MST):	12:31
Analyzer make:	Thermo 42i	Analyzer serial #:	1426262592

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.2	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
786.8	787.0	0.9998		
393.4	391.6	1.0045		
196.2	192.4	1.0198		
			0.999970	
			1.001401	
			-1.789671	

NO Calibration Curve

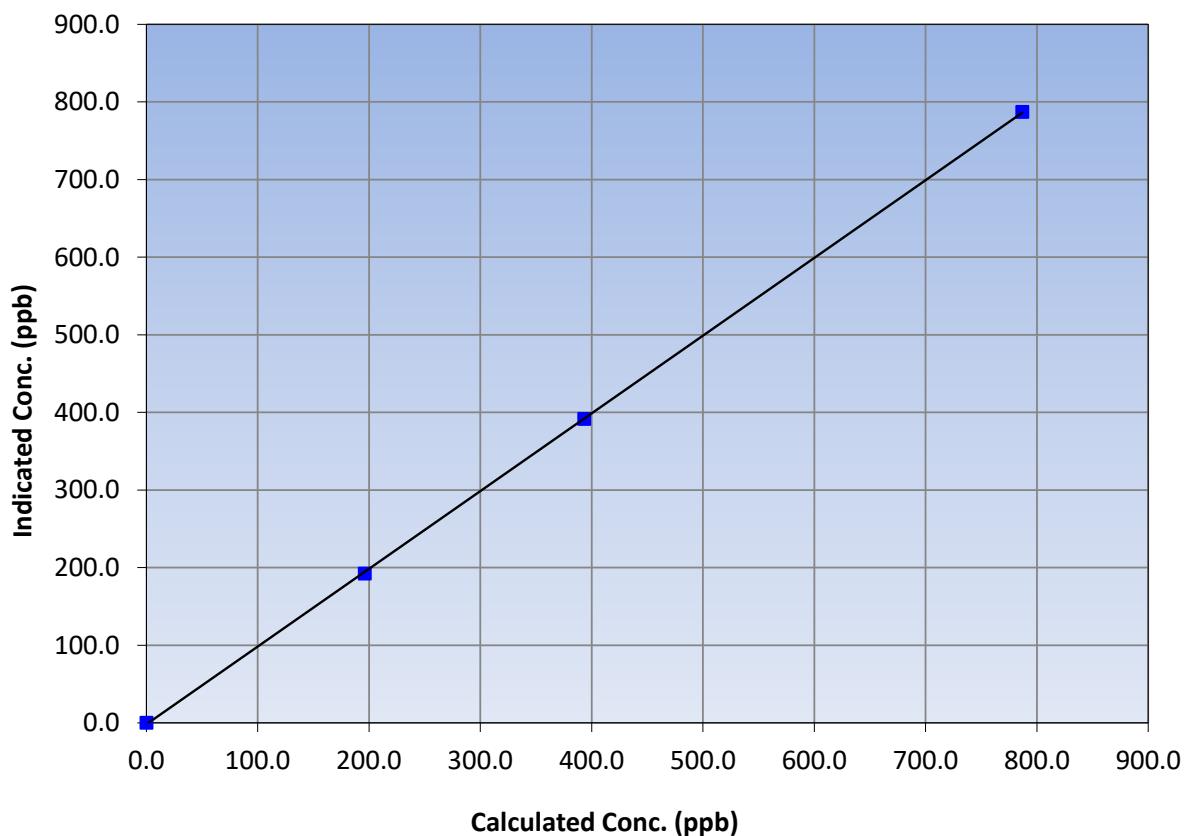



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 2, 2022
Station Name:	Anzac	Station Number:	AMS 14
Start Time (MST):	7:35	End Time (MST):	12:31
Analyzer make:	Thermo 42i	Analyzer serial #:	1426262592

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	-0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
407.9	408.9	0.9975		
213.1	213.7	0.9971		
114.0	114.9	0.9920		
			0.999996	
			1.002246	
			0.204305	


NO₂ Calibration Curve

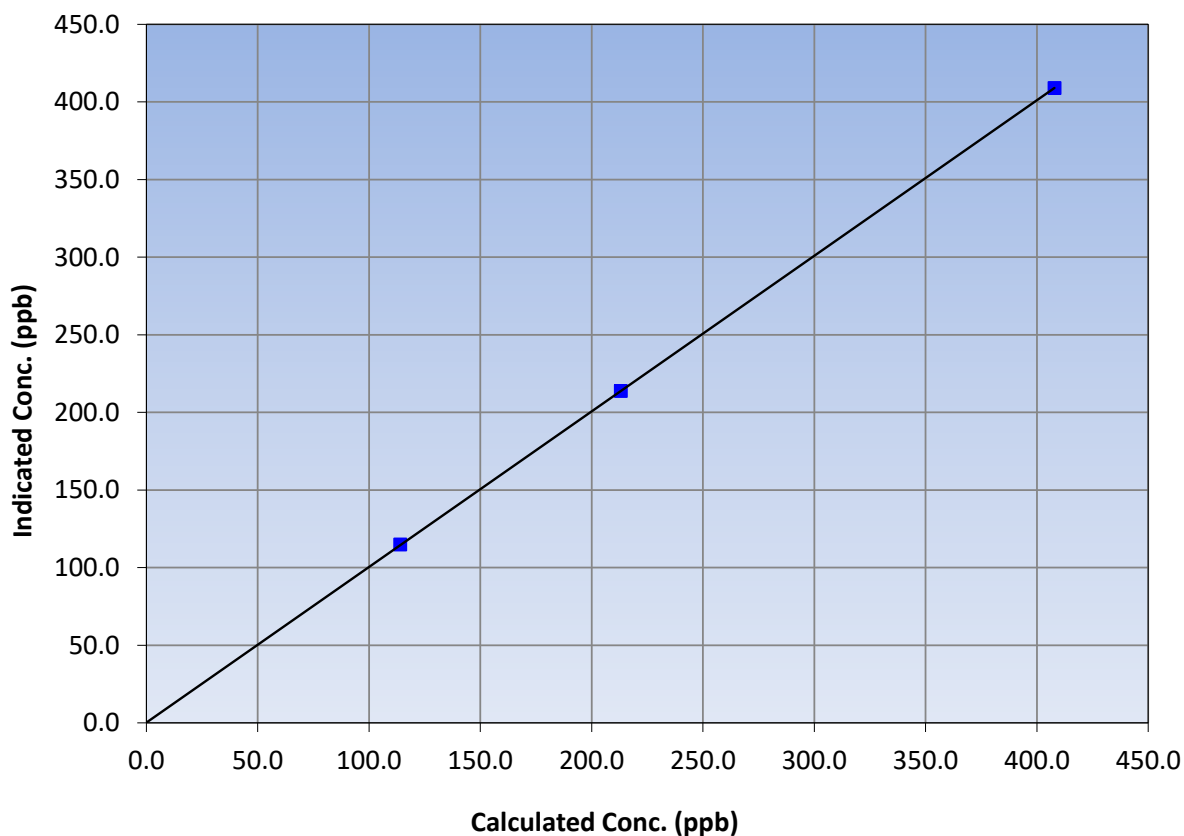

NO_x Calibration Plot

Date: January 4, 2023

Location: Anzac

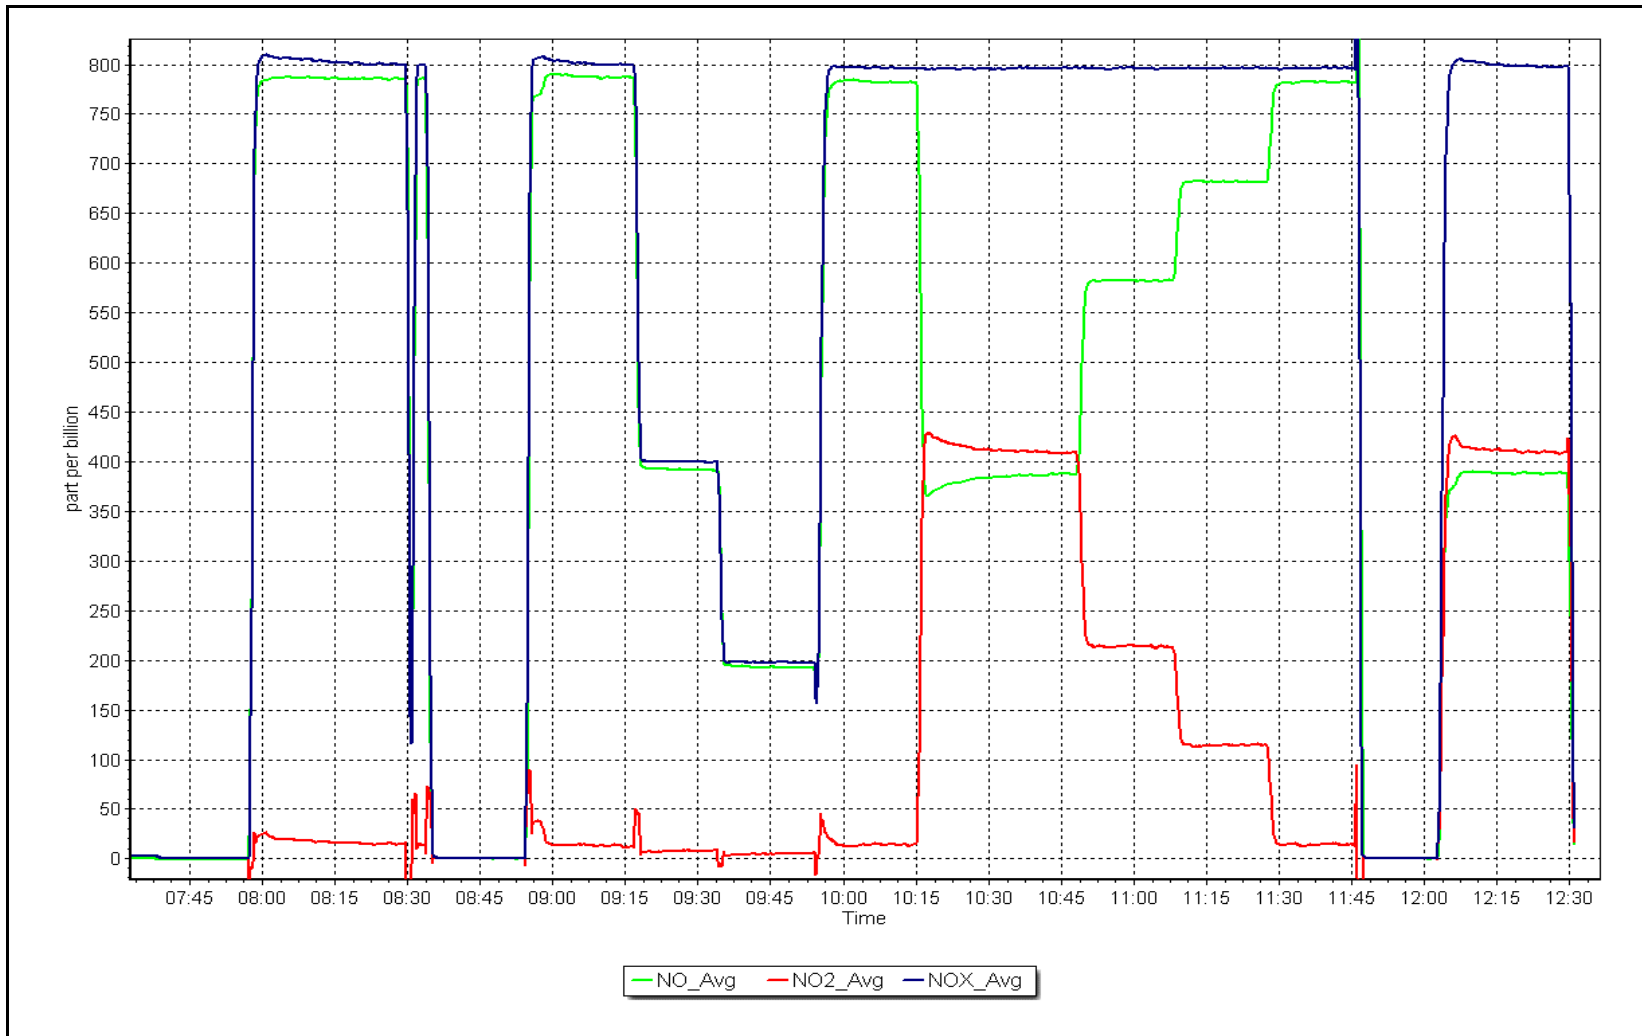



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Anzac Station number: AMS14
Calibration Date: January 24, 2023 Last Cal Date: December 14, 2022
Start time (MST): 10:29 End time (MST): 12:58
Reason: Routine

Calibration Standards

O3 generation mode: Photometer
Calibrator Make/Model: API T700 Serial Number: 5239
ZAG Make/Model: API 701H Serial Number: 357

Analyzer Information

Analyzer make: Thermo 49i Analyzer serial #: 1426262595
Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.993514	1.005686	Backgd or Offset:	2.8	2.7
Calibration intercept:	-1.440000	-1.420000	Coeff or Slope:	1.534	1.499

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	-1.2	----
as found span	5000	881.5	400.0	410.1	0.975
as found 2nd point					
as found 3rd point					
calibrator zero	5000	0.0	0.0	-1.8	----
high point	5000	882.6	400.0	400.7	0.998
second point	5000	766.8	200.0	199.8	1.001
third point	5000	669.6	100.0	99.6	1.004
as left zero	5000	0.0	0.0	-2.1	----
as left span	5000	924.8	400.0	400.4	0.999
Average Correction Factor					1.001

Baseline Corr As found:	411.3	Previous response	396.0	*% change	3.7%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: No maintenance done. Span adjusted.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 14, 2022
Station Name:	Anzac	Station Number:	AMS14
Start Time (MST):	10:29	End Time (MST):	12:58
Analyzer make:	Thermo 49i	Analyzer serial #:	1426262595

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	-1.8	----	Correlation Coefficient	0.999996	≥0.995
400.0	400.7	0.9983			
200.0	199.8	1.0010	Slope	1.005686	0.90 - 1.10
100.0	99.6	1.0040			
			Intercept	-1.420000	+/- 5

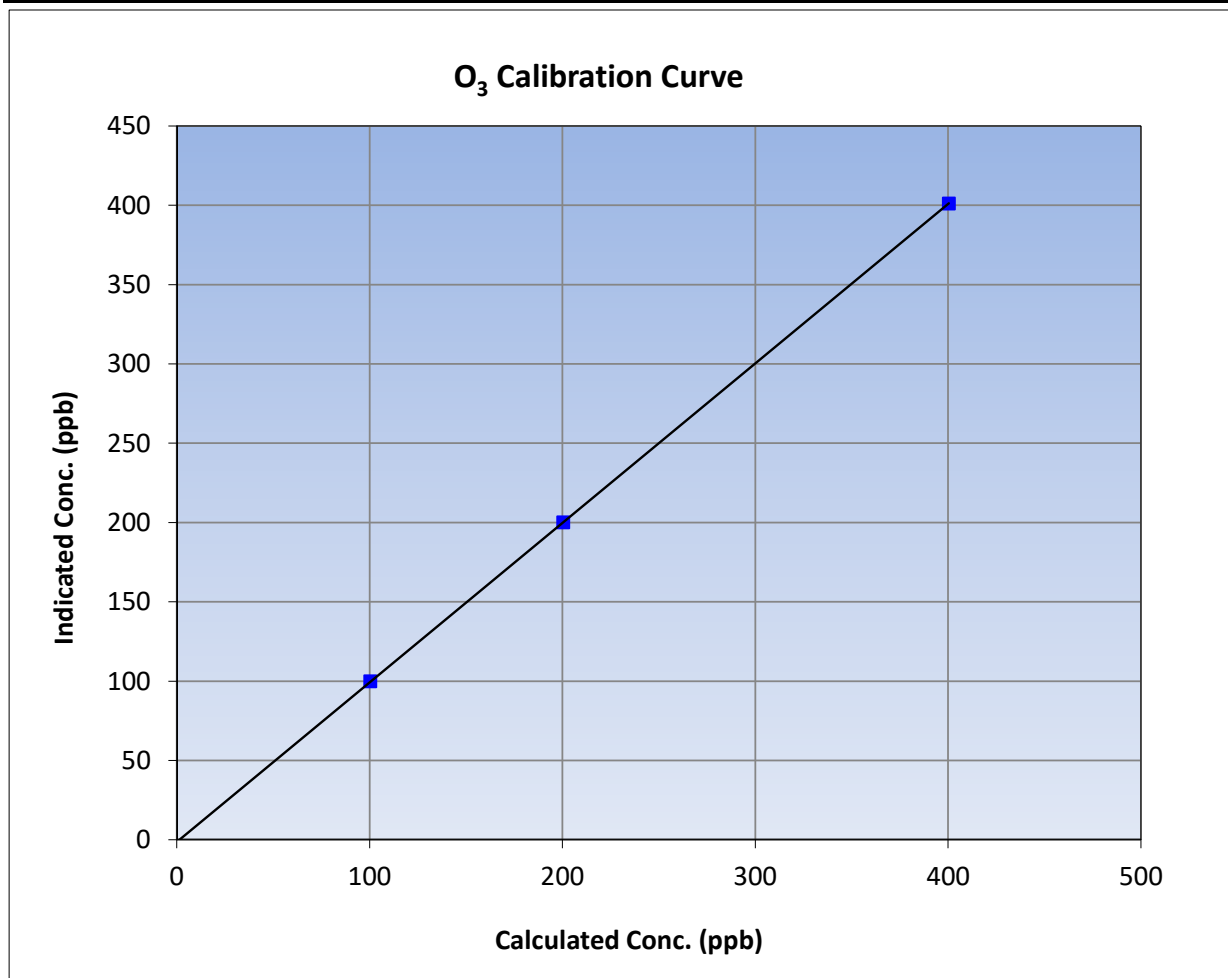

O₃ Calibration Plot

Date: January 24, 2023

Location: Anzac

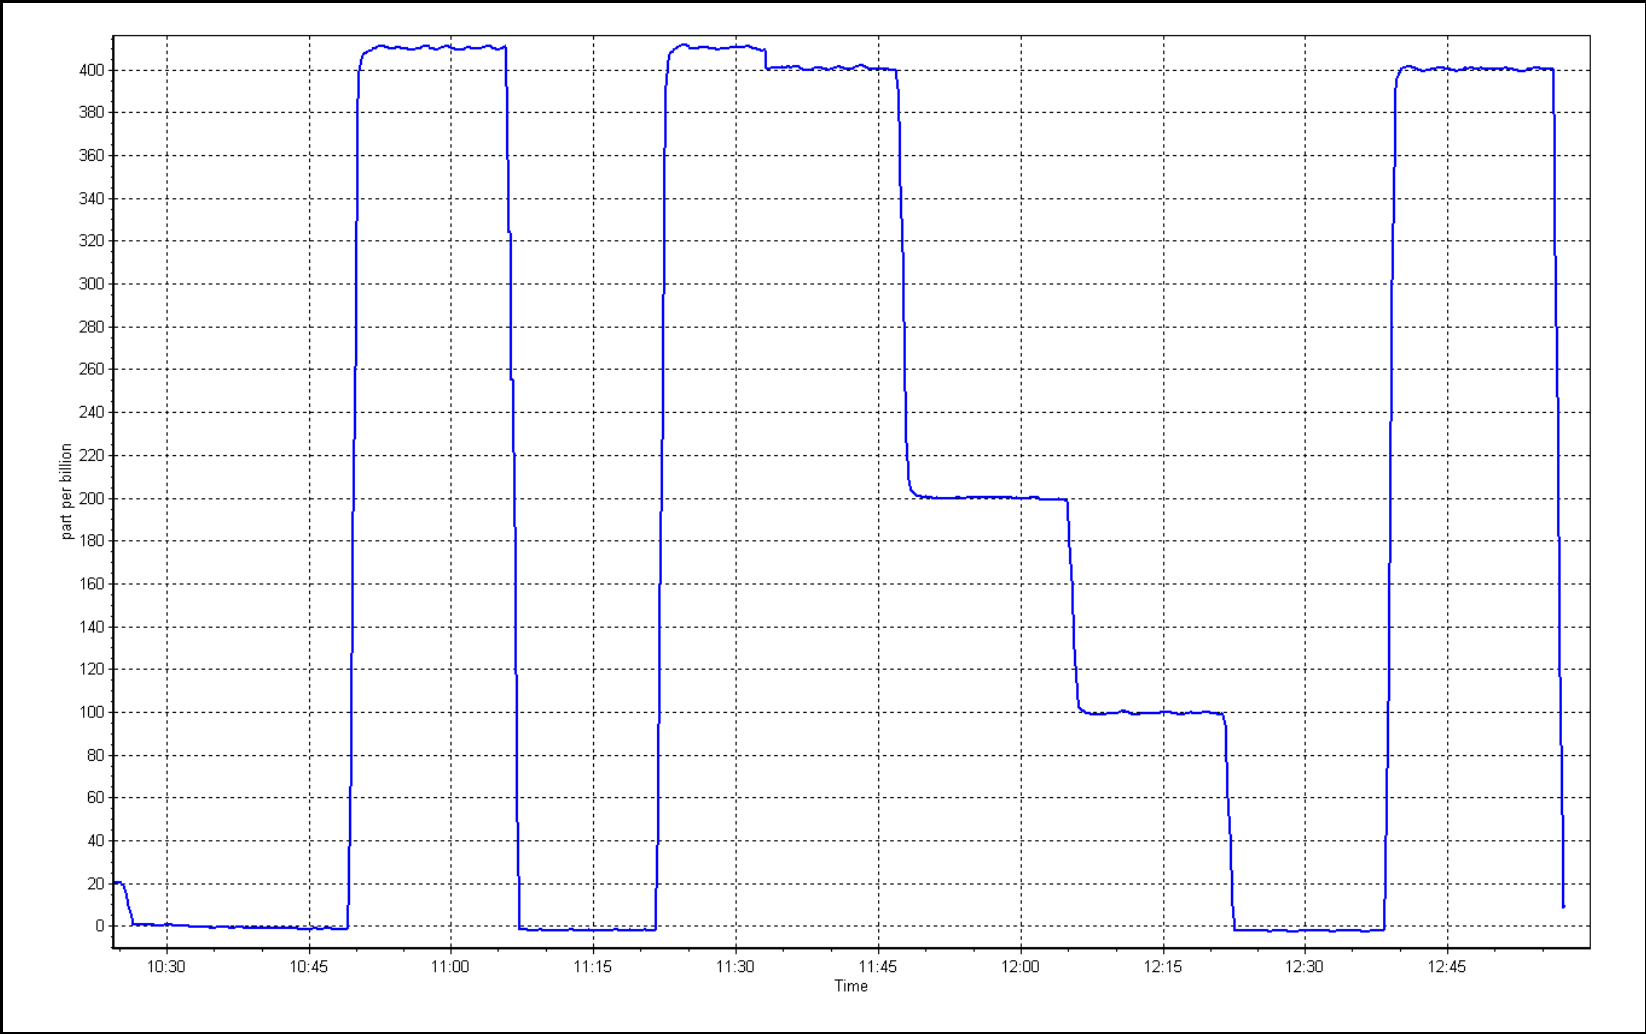



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Anzac Station number: AMS 14
Calibration Date: January 24, 2023 Last Cal Date: December 14, 2022
Start time (MST): 11:37 End time (MST): 12:01
Analyzer Make: API T640 S/N: 825
Particulate Fraction: PM2.5
Flow Meter Make/Model: Alicat FP-25 S/N: 388753
Temp/RH standard: Alicat FP-25 S/N: 388753

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-4.6	-4	-4.6	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	713.8	714.8	713.8	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5.00	5.1	5.00	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 24, 2023 Last Cal Date: December 14, 2022
PM w/o HEPA: 4.2 PM w/ HEPA: 0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test		---		<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: December 14, 2022
Disposable Filter Changed: December 14, 2022

Annual Maintenance

Date Sample Tube Cleaned: June 21, 2022
Date RH/T Sensor Cleaned: June 21, 2022

No adjustments done. Inlet Head cleaned.

Notes:

Calibration by: Melissa Lemay



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

**AMS17
WAPASU
JANUARY 2023**

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 7, 2022
Station Name:	Wapasu	Station Number:	AMS17
Start Time (MST):	10:56	End Time (MST):	13:48
Analyzer make:	Thermo 43i	Analyzer serial #:	1218153459

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.6	----	Correlation Coefficient	0.999969	
800.0	799.8	1.0002			≥0.995
400.0	396.7	1.0084	Slope	0.999825	
199.5	196.9	1.0133			0.90 - 1.10
			Intercept	-1.319798	+/-30

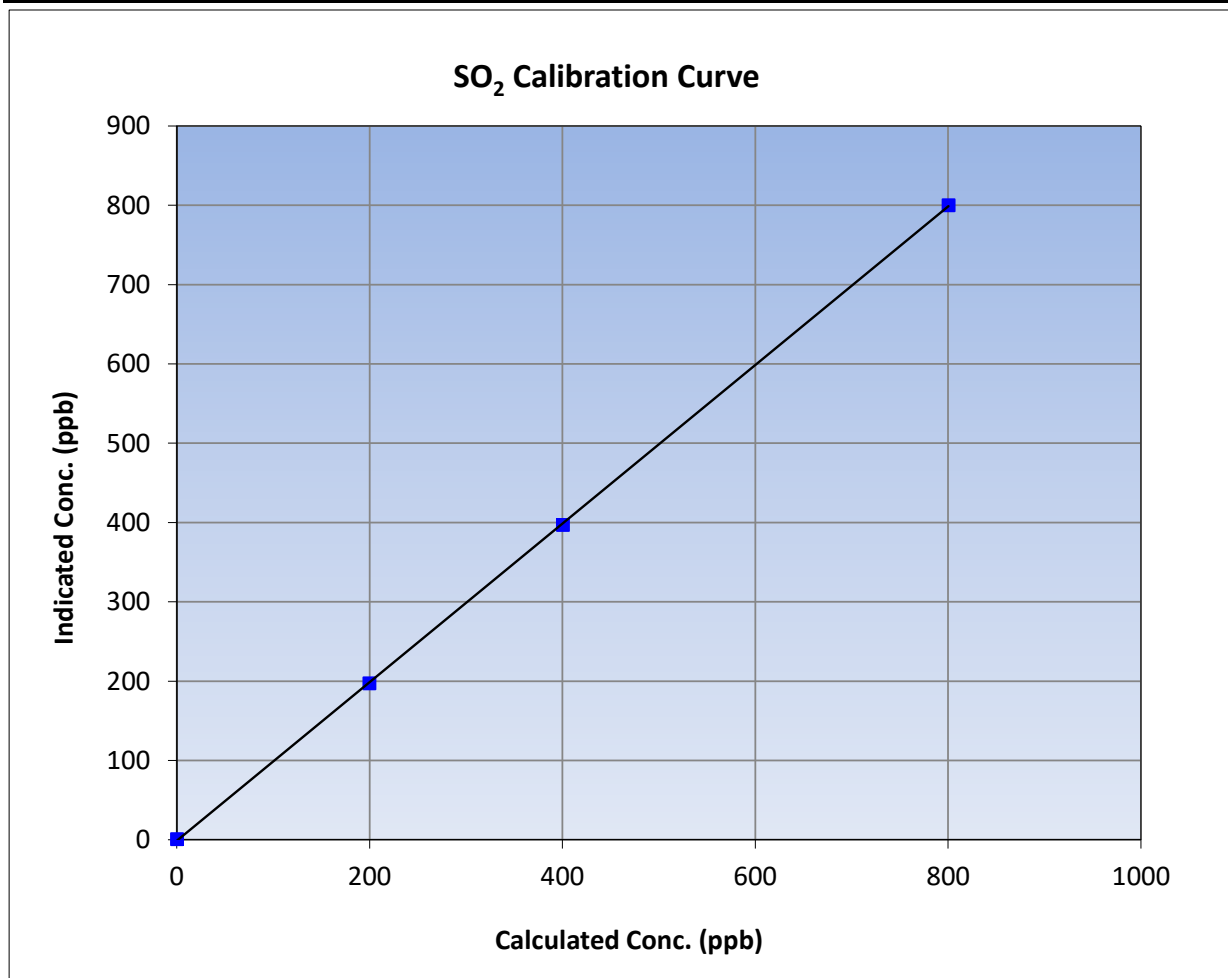

SO2 Calibration Plot

Date: January 10, 2023

Location: Wapasu

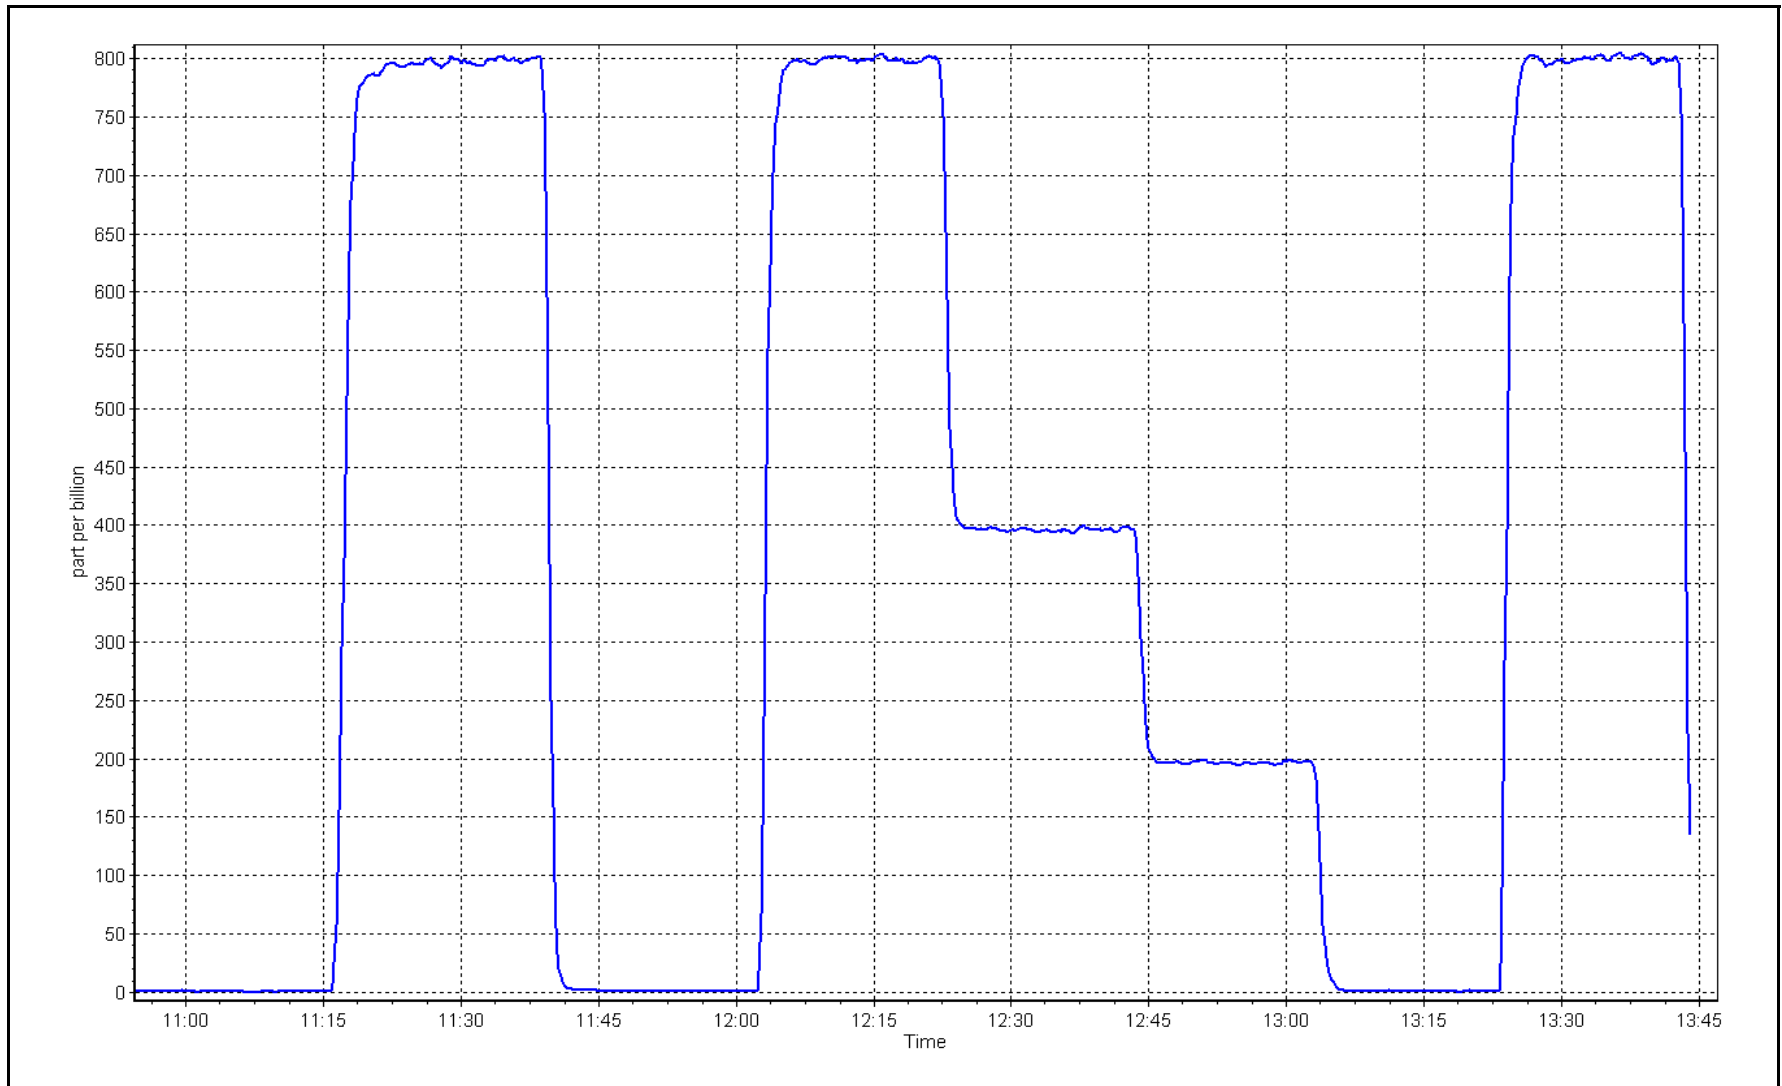



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name:	Wapasu	Station number:	AMS17
Calibration Date:	January 5, 2023	Last Cal Date:	December 14, 2022
Start time (MST):	10:23	End time (MST):	14:35
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	5.076	ppm	Cal Gas Exp Date:	September 16, 2024
Cal Gas Cylinder #:	CC511852			
Removed Cal Gas Conc:	5.076	ppm	Rem Gas Exp Date:	n/a
Removed Gas Cyl #:	n/a		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	2449
ZAG Make/Model:	API T701H		Serial Number:	359

Analyzer Information

Analyzer make:	Thermo 450i	Analyzer serial #:	1218153583
Converter make:	n/a	Converter serial #:	n/a
Analyzer Range	0 - 100 ppb		

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	1.004139	1.002282	Backgd or Offset:	12.8
Calibration intercept:	0.280806	0.320801	Coeff or Slope:	1.085

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.2	----
as found span	4921	78.8	80.0	80.1	1.001
as found 2nd point	4961	39.4	40.0	40.3	0.997
as found 3rd point	4980	19.7	20.0	20.1	1.005
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.3	----
high point	4921	78.8	80.0	80.5	0.994
second point	4961	39.4	40.0	40.4	0.990
third point	4980	19.7	20.0	20.4	0.980
as left zero	5000	0.0	0.0	0.7	----
as left span	4921	78.8	80.0	80.6	0.993
SO2 Scrubber Check	4921	79.4	800.0	-0.1	----
Date of last scrubber change:	n/a			Ave Corr Factor	0.988
Date of last converter efficiency test:	n/a				efficiency

Baseline Corr As found:	79.9	Prev response:	80.61	*% change:	-0.9%
Baseline Corr 2nd AF pt:	40.1	AF Slope:	0.999282	AF Intercept:	0.200806
Baseline Corr 3rd AF pt:	19.9	AF Correlation:	0.999992		

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. No adjustments made.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 5, 2023	Previous Calibration:	December 14, 2022
Station Name:	Wapasu	Station Number:	AMS17
Start Time (MST):	10:23	End Time (MST):	14:35
Analyzer make:	Thermo 450i	Analyzer serial #:	1218153583

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	1.000000	≥0.995
80.0	80.5	0.9938			
40.0	40.4	0.9900	Slope	1.002282	0.90 - 1.10
20.0	20.4	0.9804			
			Intercept	0.320801	+/-3

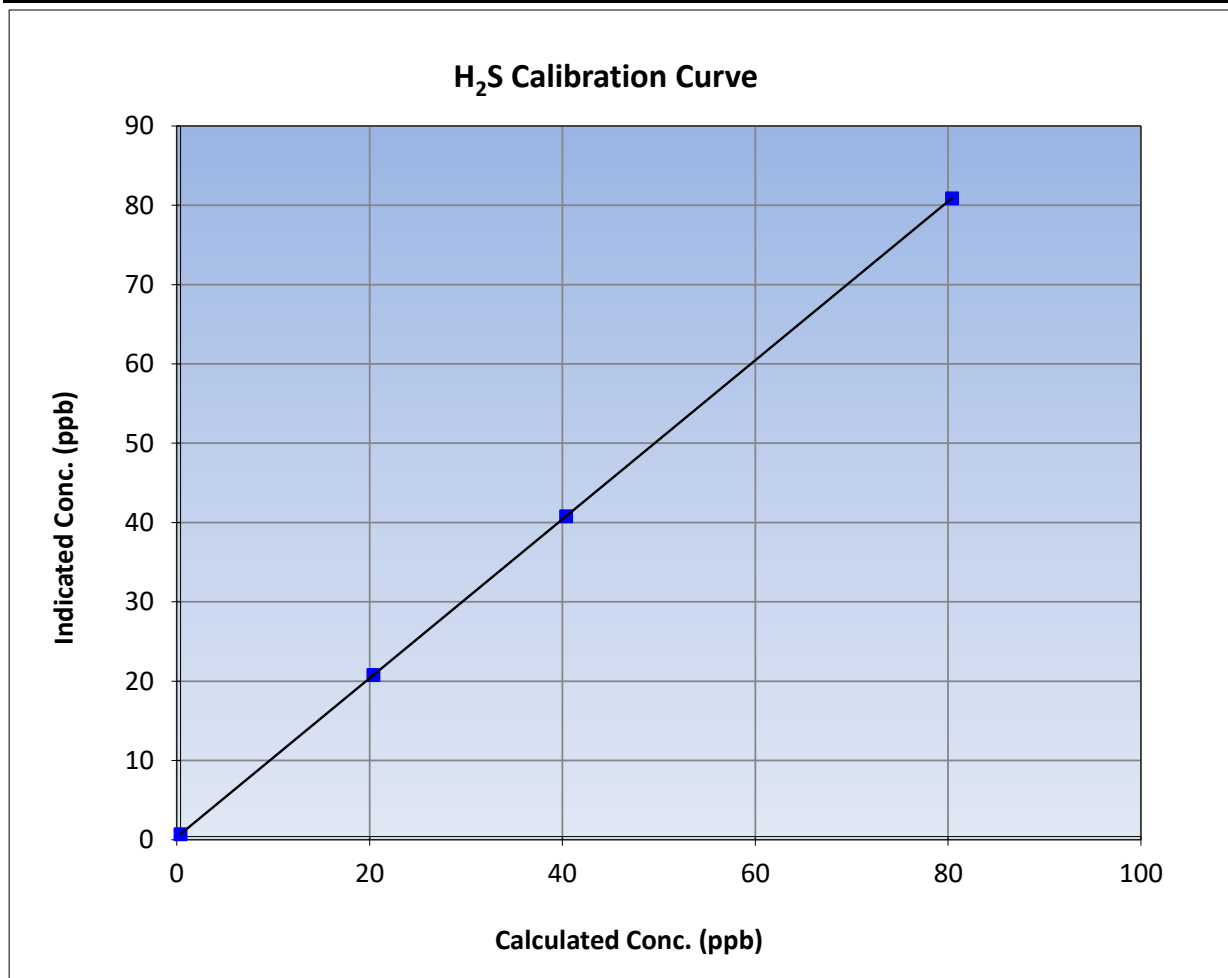

H₂S Calibration Plot

Date: January 5, 2023

Location: Wapasu

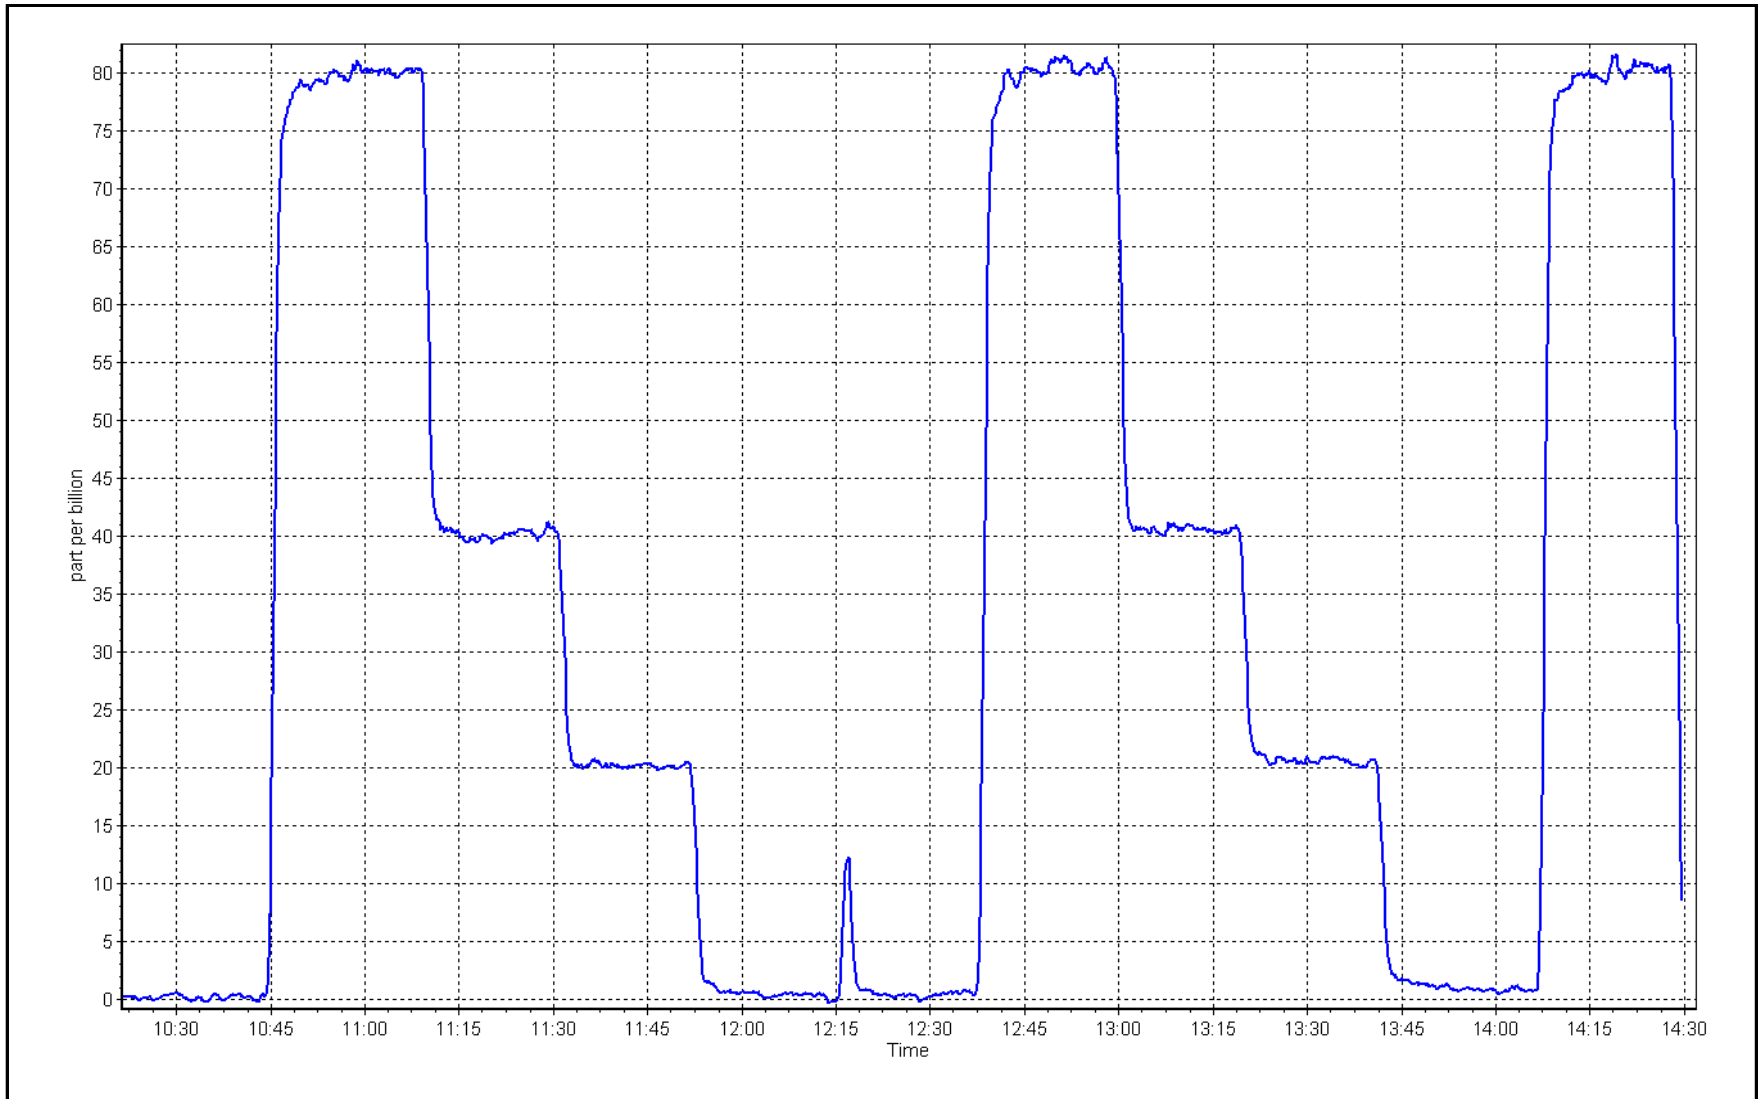



Wood Buffalo Environmental Association

THC Calibration Report

Version-01-2020

Station Information

Station Name:	Wapasu	Station number:	AMS17
Calibration Date:	January 10, 2023	Last Cal Date:	December 7, 2022
Start time (MST):	10:56	End time (MST):	13:48
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	ALM066507	Cal Gas Expiry Date:	January 12, 2029
CH4 Cal Gas Conc.	<u>503.5</u> ppm	CH4 Equiv Conc.	1076.3 ppm
C3H8 Cal Gas Conc.	<u>208.3</u> ppm		
Removed Gas Cert:	n/a	Removed Gas Expiry:	n/a
Removed CH4 Conc.	<u>503.5</u> ppm	CH4 Equiv Conc.	1076.3 ppm
Removed C3H8 Conc.	<u>208.3</u> ppm	Diff between cyl:	
Calibrator Make/Model:	API T700	Serial Number:	2449
ZAG Make/Model:	API 701H	Serial Number:	359

Analyzer Information

Analyzer make: Thermo 51i-LT Analyzer serial #: 1218153352
 Analyzer Range: 0 - 20 ppm

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.002399	1.003975	Background:	2.950	2.950
Calibration intercept:	-0.102337	0.033881	Coefficient:	4.292	4.292

THC Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated Concentration (ppm) (Cc)	Indicated Concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.03	----
as found span	4921	79.4	17.09	17.18	0.995
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.07	----
high point	4921	79.4	17.09	17.23	0.992
second point	4960	39.7	8.55	8.54	1.001
third point	4980	19.8	4.26	4.31	0.988
as left zero	5000	0.0	0.00	0.03	----
as left span	4920	79.4	17.09	17.24	0.992
Average Correction Factor					0.994
Baseline Corr As found:	17.14	Previous response	17.03	*% change	0.7%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. No adjustments made.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 7, 2022
Station Name:	Wapasu	Station Number:	AMS17
Start Time (MST):	10:56	End Time (MST):	13:48
Analyzer make:	Thermo 51i-LT	Analyzer serial #:	1218153352

Calibration Data


Calculated Concentration (ppm) (Cc)	Indicated Concentration (ppm) (lc)	Correction factor (Cc/lc)	Statistical Evaluation	<u>Limits</u>	
0.00	0.07	----	Correlation Coefficient	0.999947	
17.09	17.23	0.9919			≥0.995
8.55	8.54	1.0009	Slope	1.003975	
4.26	4.31	0.9880			0.90 - 1.10
			Intercept	0.033881	+/-1.5

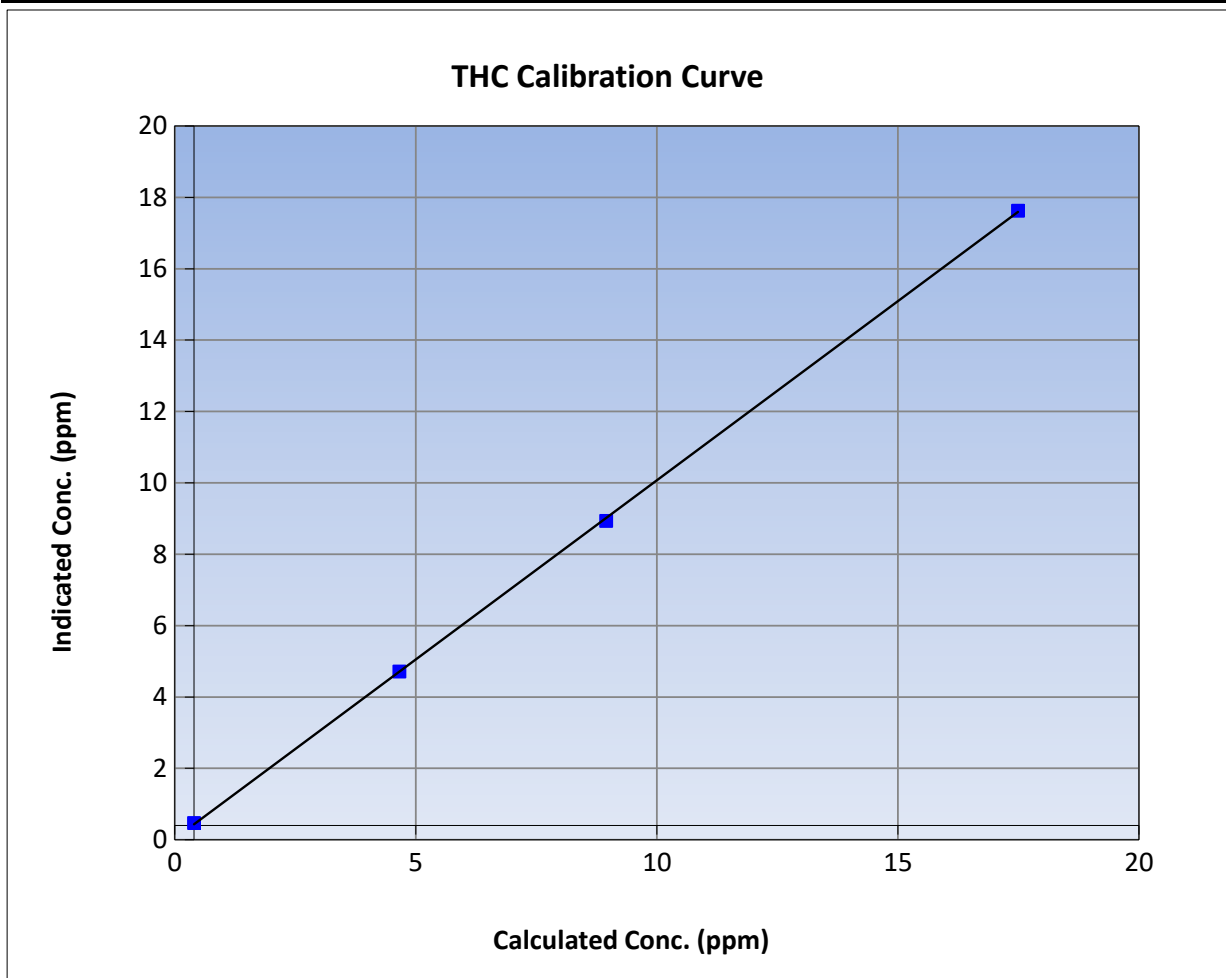

THC Calibration Plot

Date: January 10, 2023

Location: Wapasu

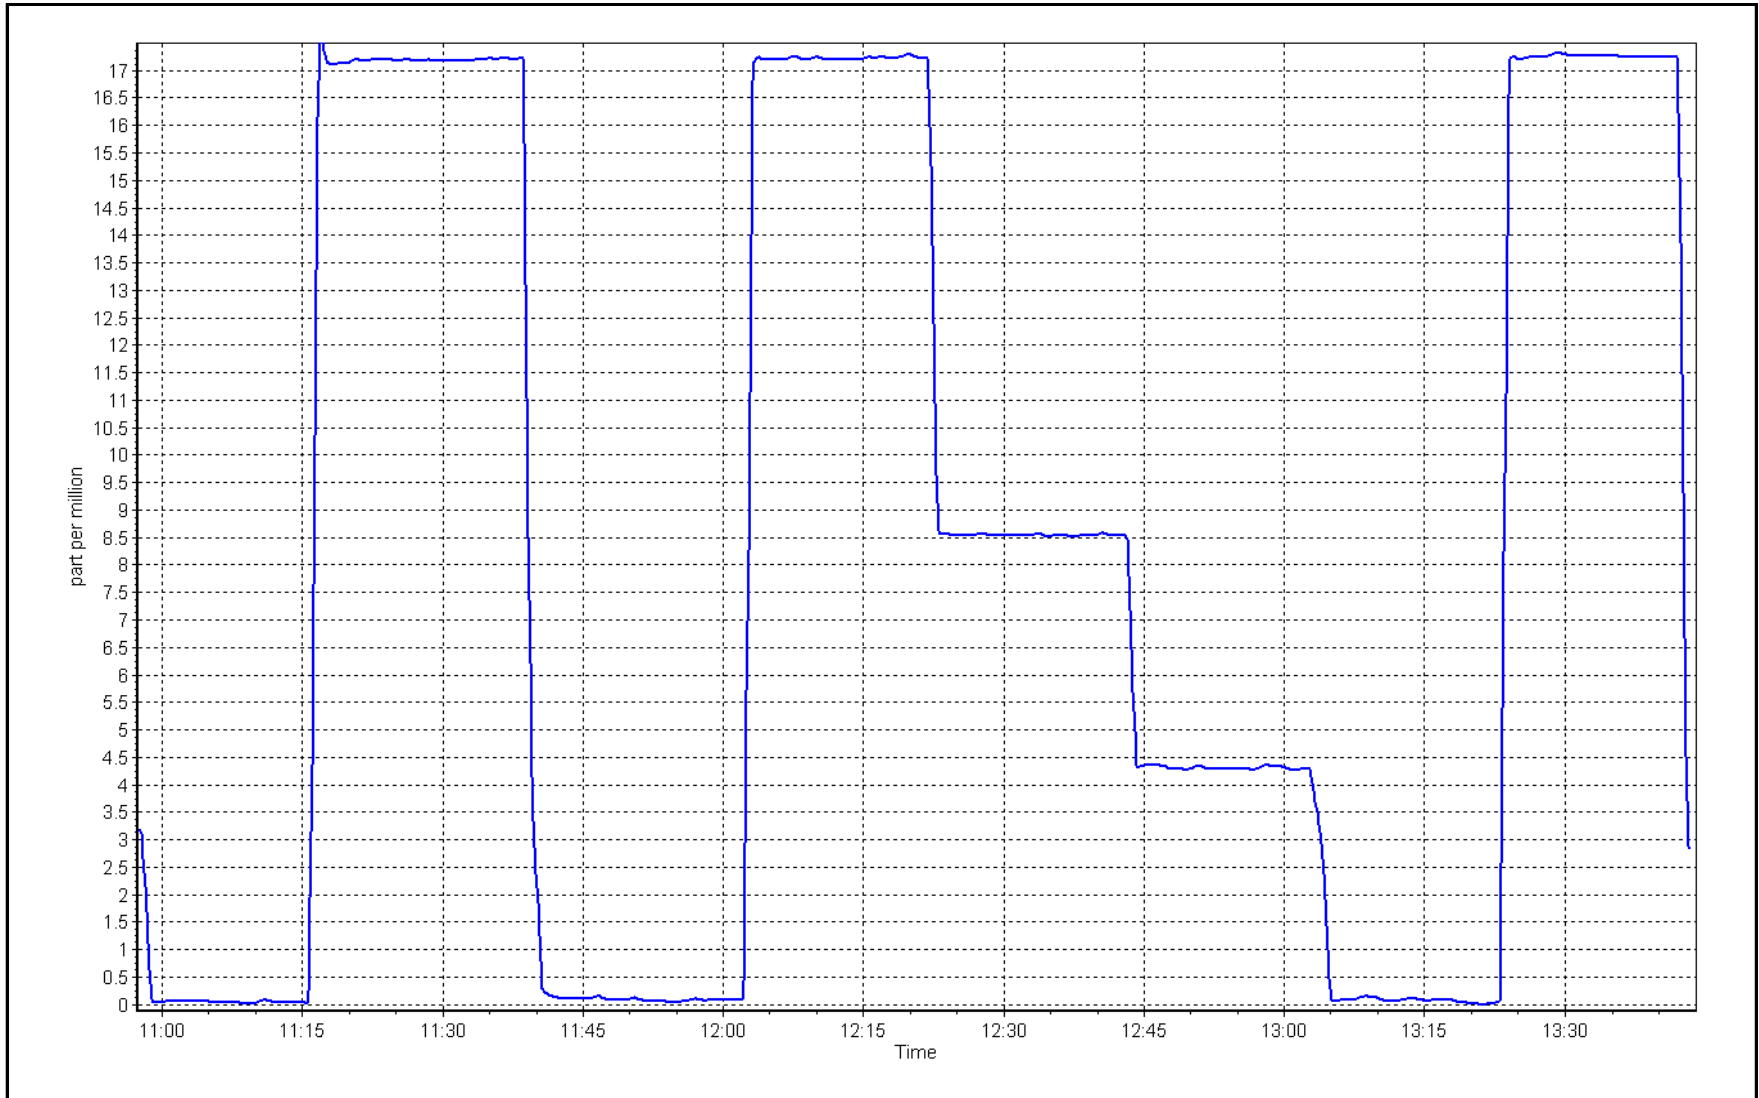



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Wapasu
Calibration Date: January 19, 2023
Start time (MST): 10:33
Reason: Routine
Station number: AMS17
Last Cal Date: December 8, 2022
End time (MST): 15:10

Calibration Standards

NO Gas Cylinder #: T375YK8
NOX Cal Gas Conc: 49.11 ppm
Removed Cylinder #: T375YK8
Removed Gas NOX Conc: 49.11 ppm
NOX gas Diff:
Calibrator Model: API T700
ZAG make/model: API T701H
Cal Gas Expiry Date: April 13, 2025
NO Cal Gas Conc: 48.07 ppm
Removed Gas Exp Date:
Removed Gas NO Conc: 48.07 ppm
NO gas Diff:
Serial Number: 2449
Serial Number: 359

Analyzer Information

Analyzer make: Teledyne API T200
NOX Range (ppb): 0 - 1000 ppb
Analyzer serial #: 833

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	0.820	0.820	NO bkgnd or offset:	0.1	0.1
NOX coeff or slope:	0.812	0.812	NOX bkgnd or offset:	-0.4	-0.4
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	4.3	4.4

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	0.999732	0.999578
NO _x Cal Offset:	-1.300000	-1.120000
NO Cal Slope:	1.000301	1.000973
NO Cal Offset:	-2.080000	-2.440000
NO ₂ Cal Slope:	0.992948	0.996862
NO ₂ Cal Offset:	-0.933811	-0.247483



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.3	-0.2	0.5	----	----
as found span	4917	83.2	817.2	799.9	17.3	812.5	794.7	17.9	1.0058	1.0065
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.3	0.0	0.3	----	----
high point	4917	83.2	817.2	799.9	17.3	816.4	799.9	16.4	1.0010	1.0000
second point	4958	41.6	408.6	399.9	8.7	406.7	395.3	11.4	1.0047	1.0117
third point	4979	20.8	204.3	200.0	4.3	201.6	196.2	5.4	1.0134	1.0192
as left zero	5000	0.0	0.0	0.0	0.0	0.5	0.2	0.3	----	----
as left span	4917	83.2	817.2	408.0	409.2	807.5	402.3	405.3	1.0120	1.0141
Average Correction Factor									1.0063	1.0103

Corrected As found	NO _x = 812.2 ppb	NO = 794.9 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -0.4%
Previous Response	NO _x = 815.7 ppb	NO = 798.0 ppb		*Percent Change	NO = -0.4%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	795.4	403.5	409.2	407.5	1.0042	99.6%
2nd GPT point (200 ppb O3)	795.4	595.6	217.1	217.3	0.9991	100.1%
3rd GPT point (100 ppb O3)	795.4	697.4	115.3	113.2	1.0186	98.2%
Average Correction Factor					1.0073	99.3%

Notes: Sample inlet filter changed after as founds. No adjustments made.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 8, 2022
Station Name:	Wapasu	Station Number:	AMS17
Start Time (MST):	10:33	End Time (MST):	15:10
Analyzer make:	Teledyne API T200	Analyzer serial #:	833

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.3	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
817.2	816.4	1.0010		
408.6	406.7	1.0047		
204.3	201.6	1.0134		

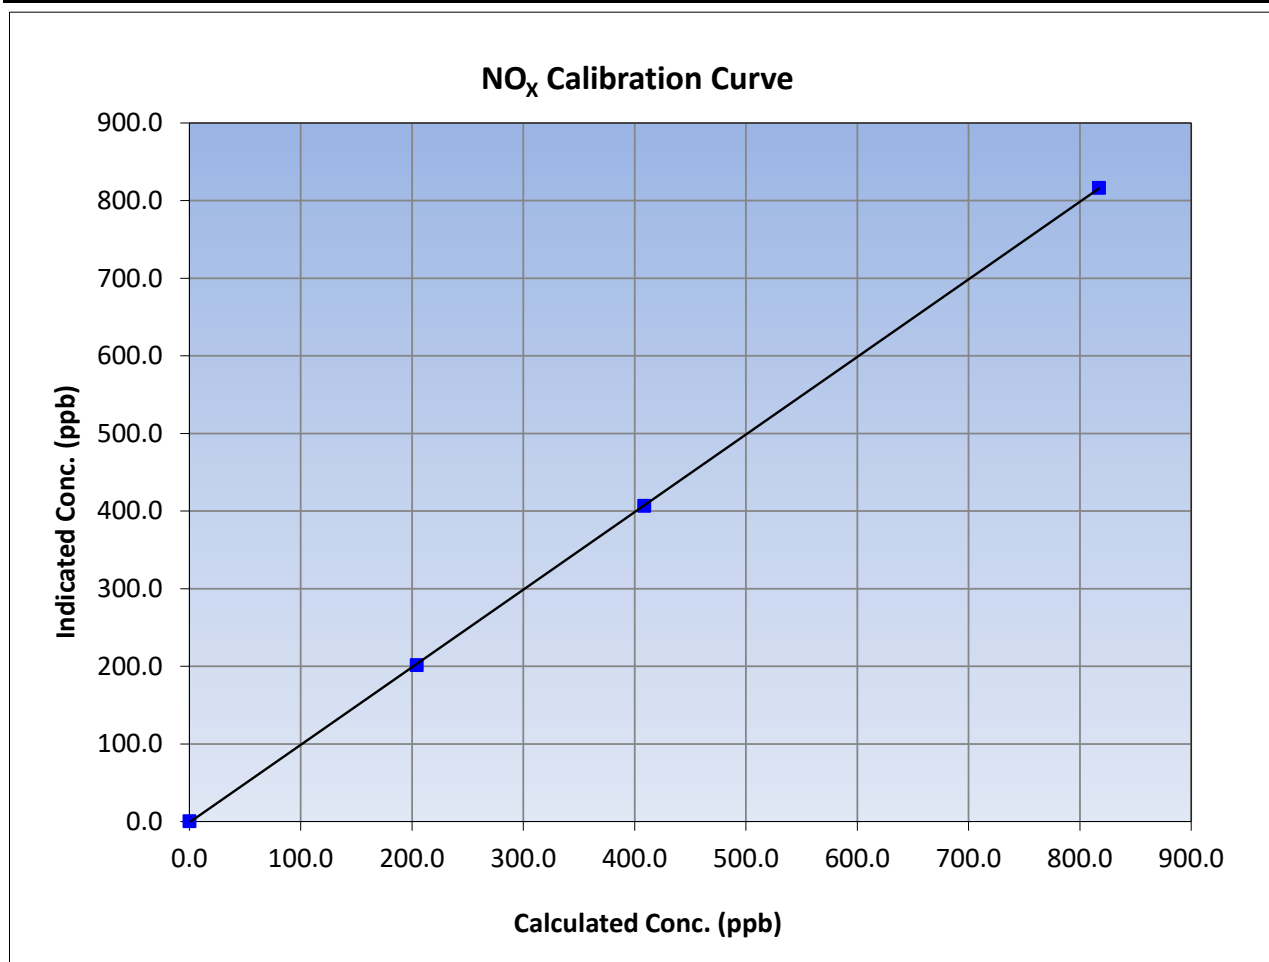



Wood Buffalo Environmental Association

NO Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 8, 2022
Station Name:	Wapasu	Station Number:	AMS17
Start Time (MST):	10:33	End Time (MST):	15:10
Analyzer make:	Teledyne API T200	Analyzer serial #:	833

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥ 0.995 0.90 - 1.10 +/-20
799.9	799.9	1.0000		
399.9	395.3	1.0117		
200.0	196.2	1.0192		

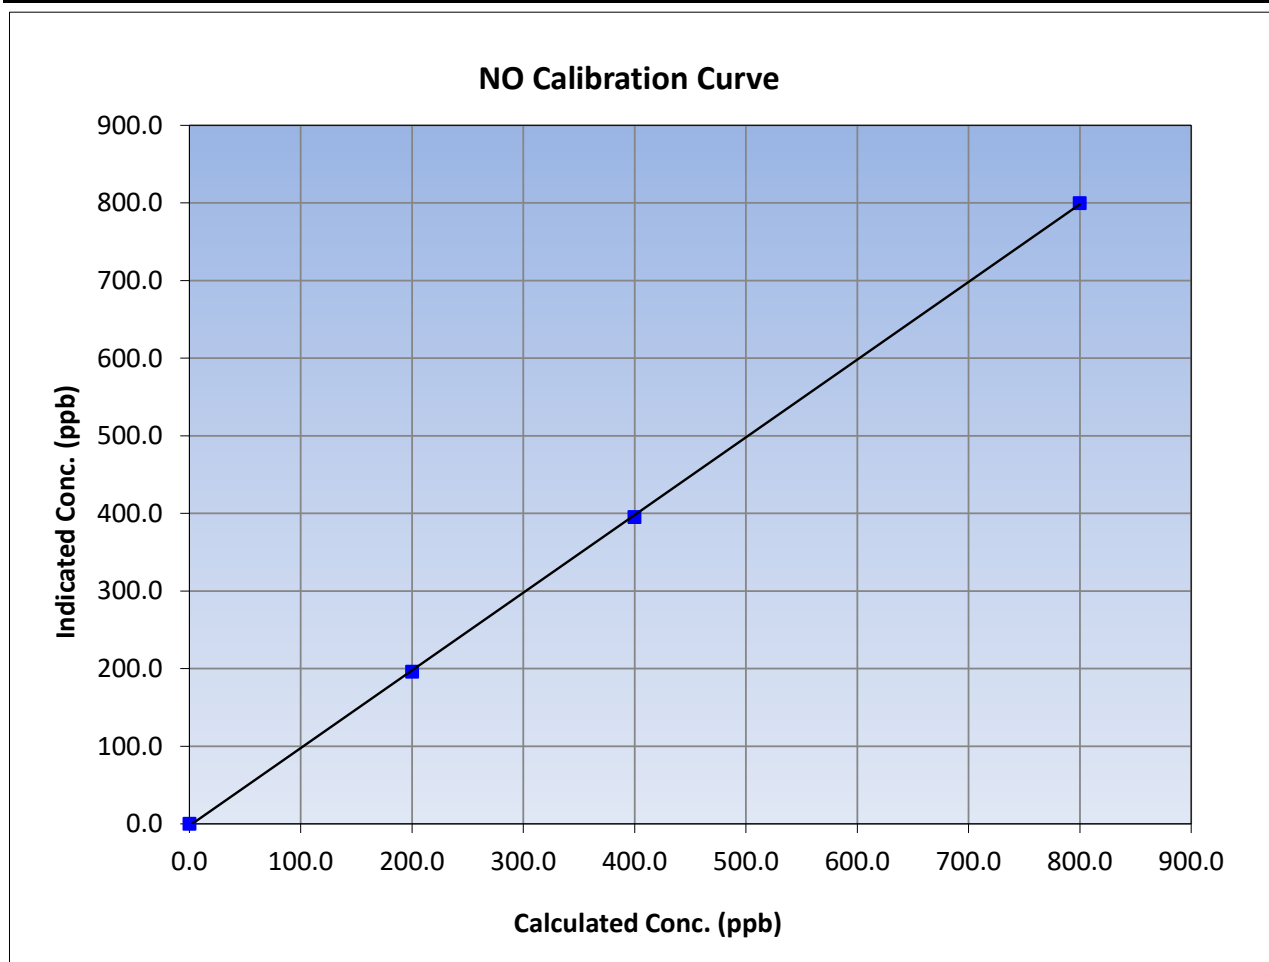



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 8, 2022
Station Name:	Wapasu	Station Number:	AMS17
Start Time (MST):	10:33	End Time (MST):	15:10
Analyzer make:	Teledyne API T200	Analyzer serial #:	833

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.3	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
409.2	407.5	1.0042		
217.1	217.3	0.9991		
115.3	113.2	1.0186		


NO₂ Calibration Curve

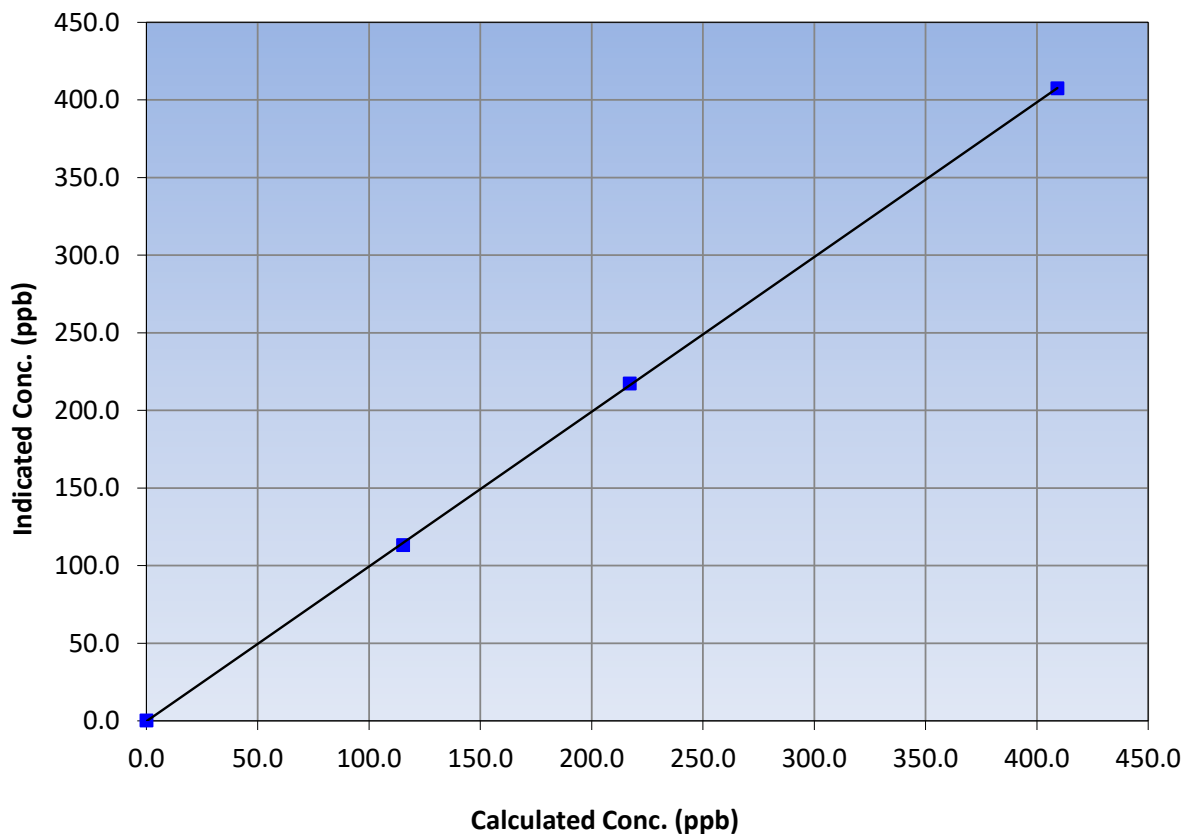

NO_x Calibration Plot

Date: January 19, 2023

Location: Wapasu

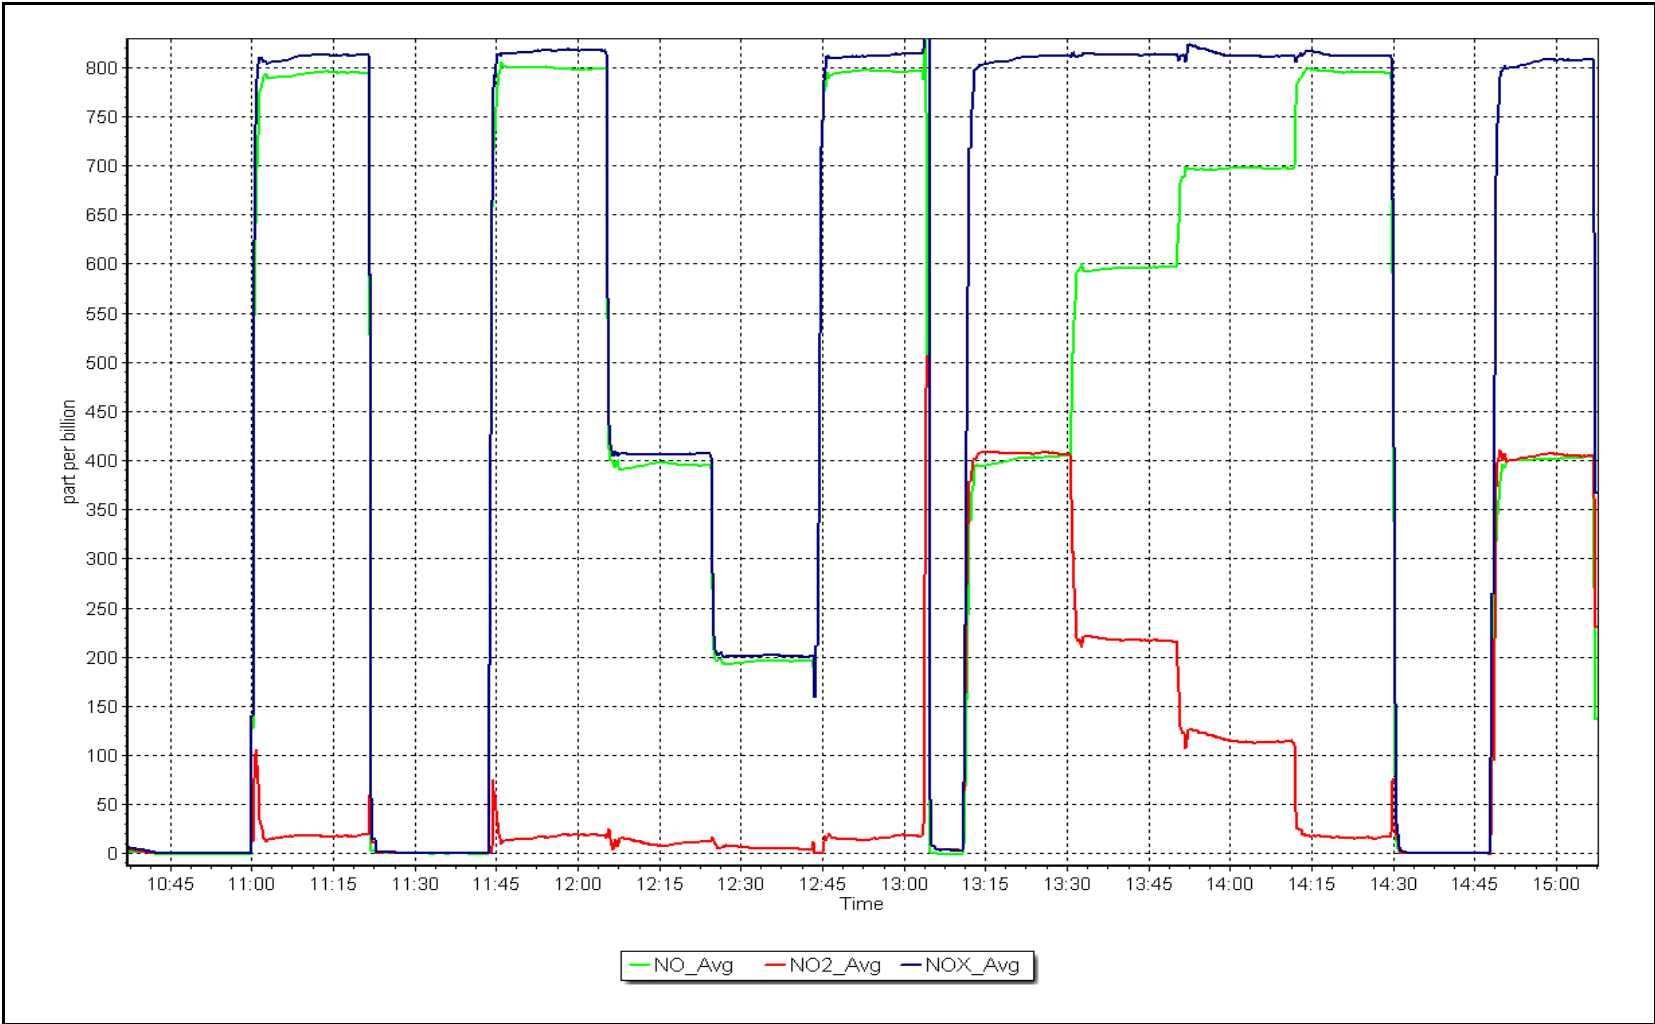



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Wapasu Station number: AMS17
 Calibration Date: January 4, 2023 Last Cal Date: December 15, 2022
 Start time (MST): 10:15 End time (MST): 13:05
 Reason: Routine

Calibration Standards

O3 generation mode: Photometer
 Calibrator Make/Model: API T700 Serial Number: 2449
 ZAG Make/Model: API T701H Serial Number: 359

Analyzer Information

Analyzer make: API T400 Analyzer serial #: 3870
 Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.005114	1.005486	Backgd or Offset:	-1.8	-1.8
Calibration intercept:	-0.320000	-0.360000	Coeff or Slope:	1.020	1.020

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	-0.1	----
as found span	5000	1077.3	400.0	402.7	0.993
as found 2nd point					
as found 3rd point					
calibrator zero	5000	0.0	0.0	0.2	----
high point	5000	1077.3	400.0	402.2	0.995
second point	5000	900.3	200.0	200.2	0.999
third point	5000	789.5	100.0	99.8	1.002
as left zero	5000	0.0	0.0	0.3	----
as left span	5000	1077.3	400.0	405.5	0.986
Average Correction Factor					0.999

Baseline Corr As found:	402.8	Previous response	401.7	*% change	0.3%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. No adjustments made.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 15, 2022
Station Name:	Wapasu	Station Number:	AMS17
Start Time (MST):	10:15	End Time (MST):	13:05
Analyzer make:	API T400	Analyzer serial #:	3870

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999990	
400.0	402.2	0.9945			≥0.995
200.0	200.2	0.9990	Slope	1.005486	
100.0	99.8	1.0020			0.90 - 1.10
			Intercept	-0.360000	+/- 5

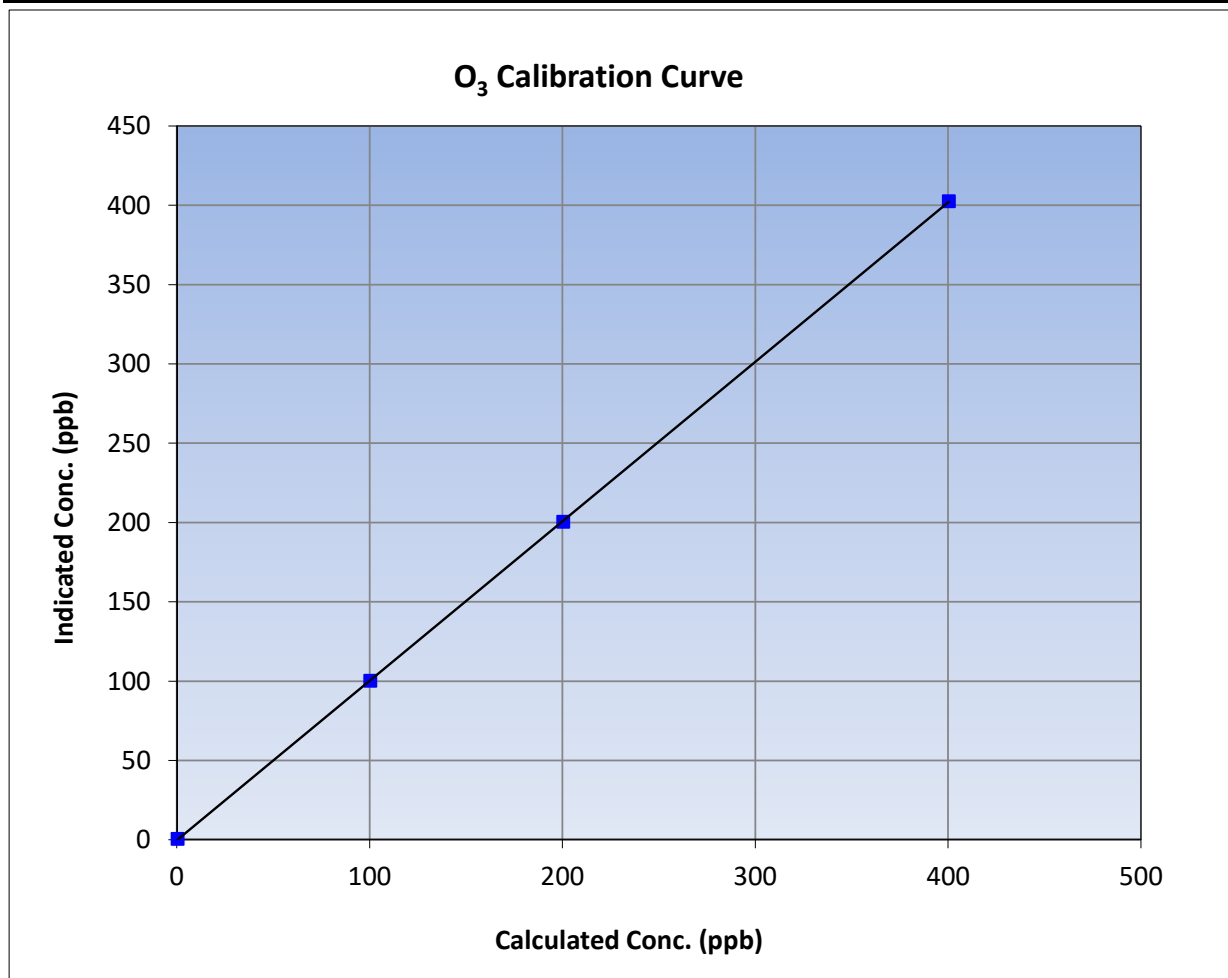

O₃ Calibration Plot

Date: January 4, 2023

Location: Wapasu

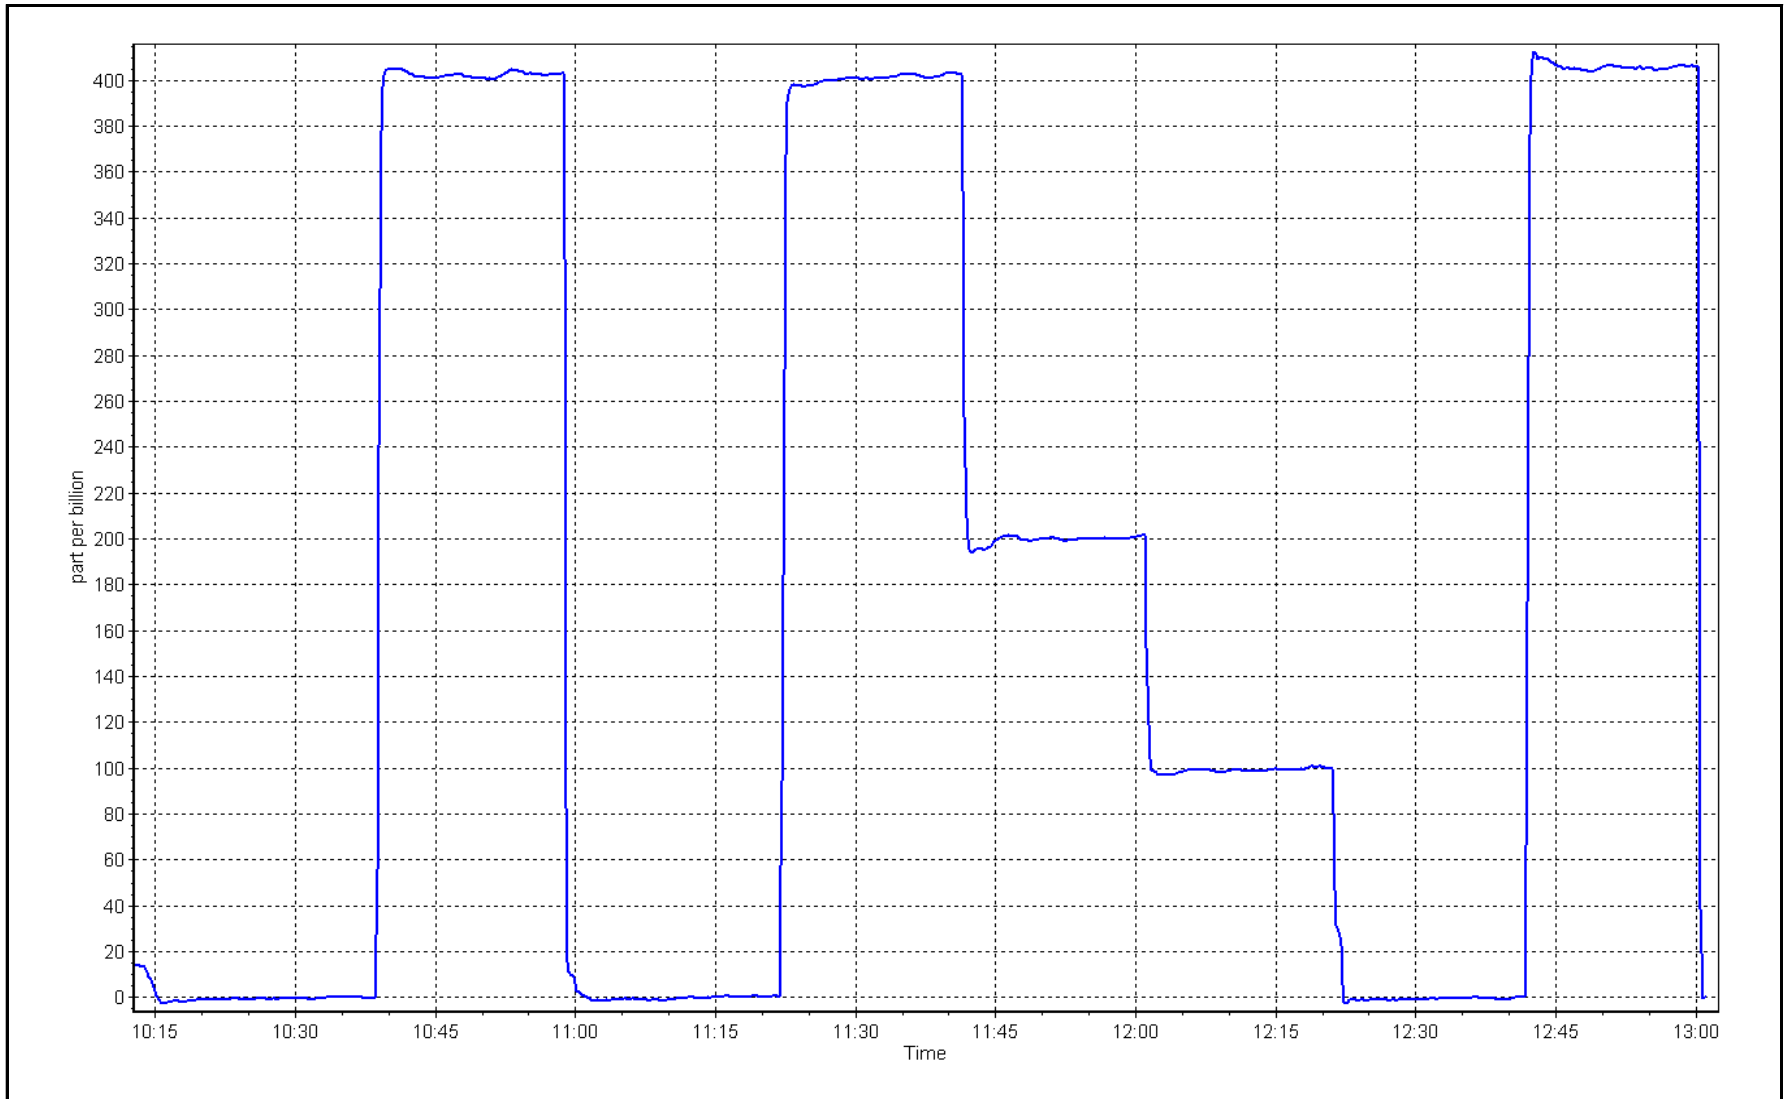



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Wapasu Station number: AMS 17
Calibration Date: January 19, 2023 Last Cal Date: December 15, 2022
Start time (MST): 11:29 End time (MST): 11:55

Analyzer Make: API T640 S/N: 1183
Particulate Fraction: PM2.5

Flow Meter Make/Model: Delta Cal S/N: 1102
Temp/RH standard: Delta Cal S/N: 1102

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-4.8	-4.7	-4.8	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	709.9	711.0	709.9	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5.01	5.05	5.01	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 19, 2023 Last Cal Date: December 15, 2022
PM w/o HEPA: 9.6 PM w/ HEPA: 0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test				<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: December 15, 2022
Disposable Filter Changed: December 15, 2022

Annual Maintenance

Date Sample Tube Cleaned: November 22, 2021
Date RH/T Sensor Cleaned: November 22, 2021

Notes: No adjustments made. Leak check passed.

Calibration by: Karan Pandit



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS18 STONY MOUNTAIN JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Stony Mountain	Station number:	AMS 18
Calibration Date:	January 16, 2023	Last Cal Date:	December 15, 2022
Start time (MST):	11:35	End time (MST):	14:42
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.40	ppm	Cal Gas Exp Date:	February 23, 2025
Cal Gas Cylinder #:	CC463851			
Removed Cal Gas Conc:	49.40	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	2658
ZAG Make/Model:	Teledyne API 701H		Serial Number:	360

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	JC1501301453
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.994979	1.003075	Backgd or Offset:	22.4	23.0
Calibration intercept:	-1.084581	-1.143339	Coeff or Slope:	0.807	0.817

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5009	0.0	0.0	-0.5	----
as found span	4919	81.0	800.3	788.7	1.015
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	-0.3	----
high point	4919	81.0	800.3	801.7	0.998
second point	4959	40.5	400.2	400.8	0.998
third point	4979	20.2	199.6	197.6	1.010
as left zero	5000	0.0	0.0	-0.3	----
as left span	4919	81.0	800.3	800.9	0.999
Average Correction Factor					1.002

Baseline Corr As found:	789.20	Previous response	795.18	*% change	-0.8%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. Adjusted the span only.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 15, 2022
Station Name:	Stony Mountain	Station Number:	AMS 18
Start Time (MST):	11:35	End Time (MST):	14:42
Analyzer make:	Thermo 43i	Analyzer serial #:	JC1501301453

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	-0.3	----	Correlation Coefficient	0.999991	
800.3	801.7	0.9982			≥0.995
400.2	400.8	0.9985	Slope	1.003075	
199.6	197.6	1.0102			0.90 - 1.10
			Intercept	-1.143339	+/-30

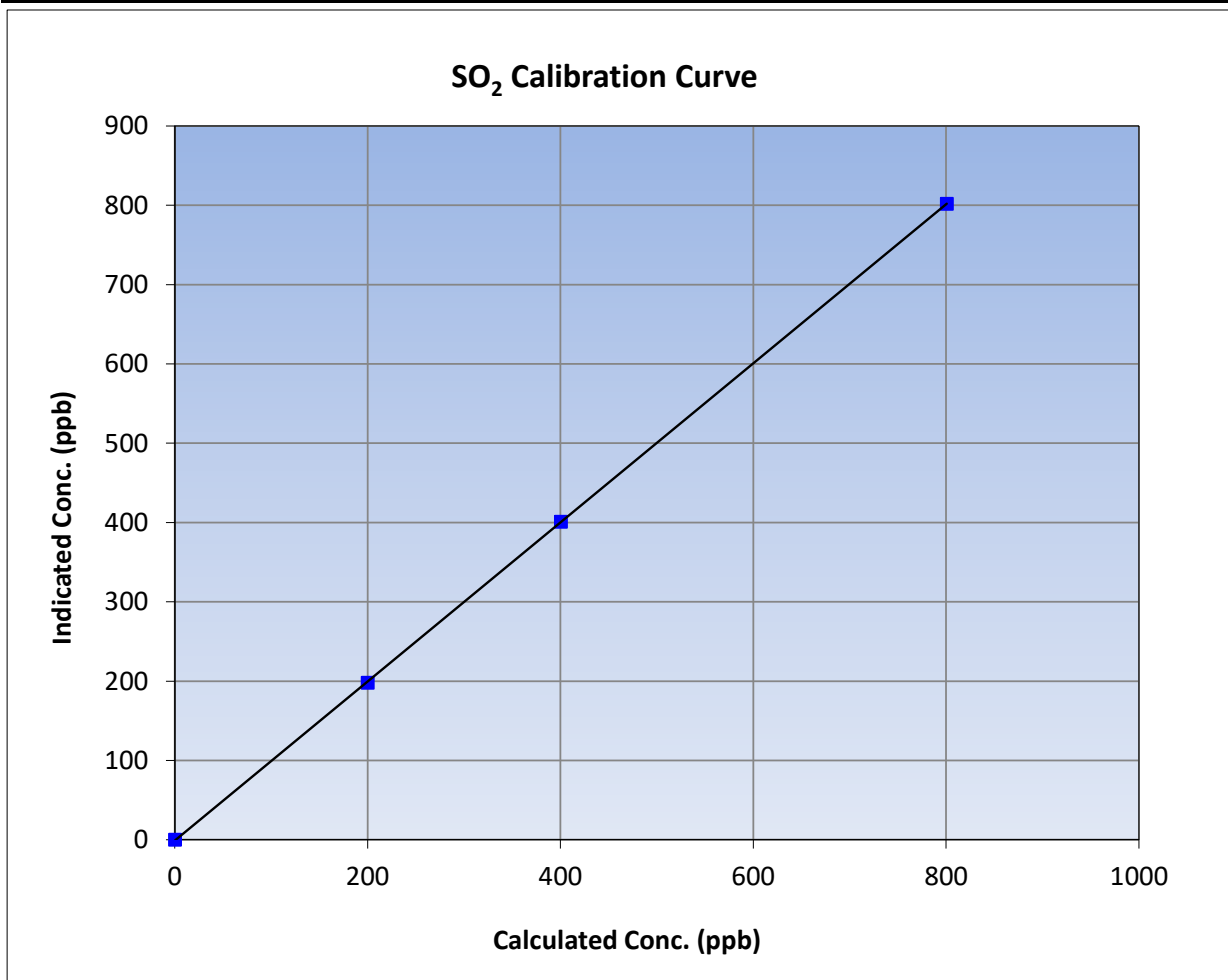

SO2 Calibration Plot

Date: January 16, 2023

Location: Stony Mountain

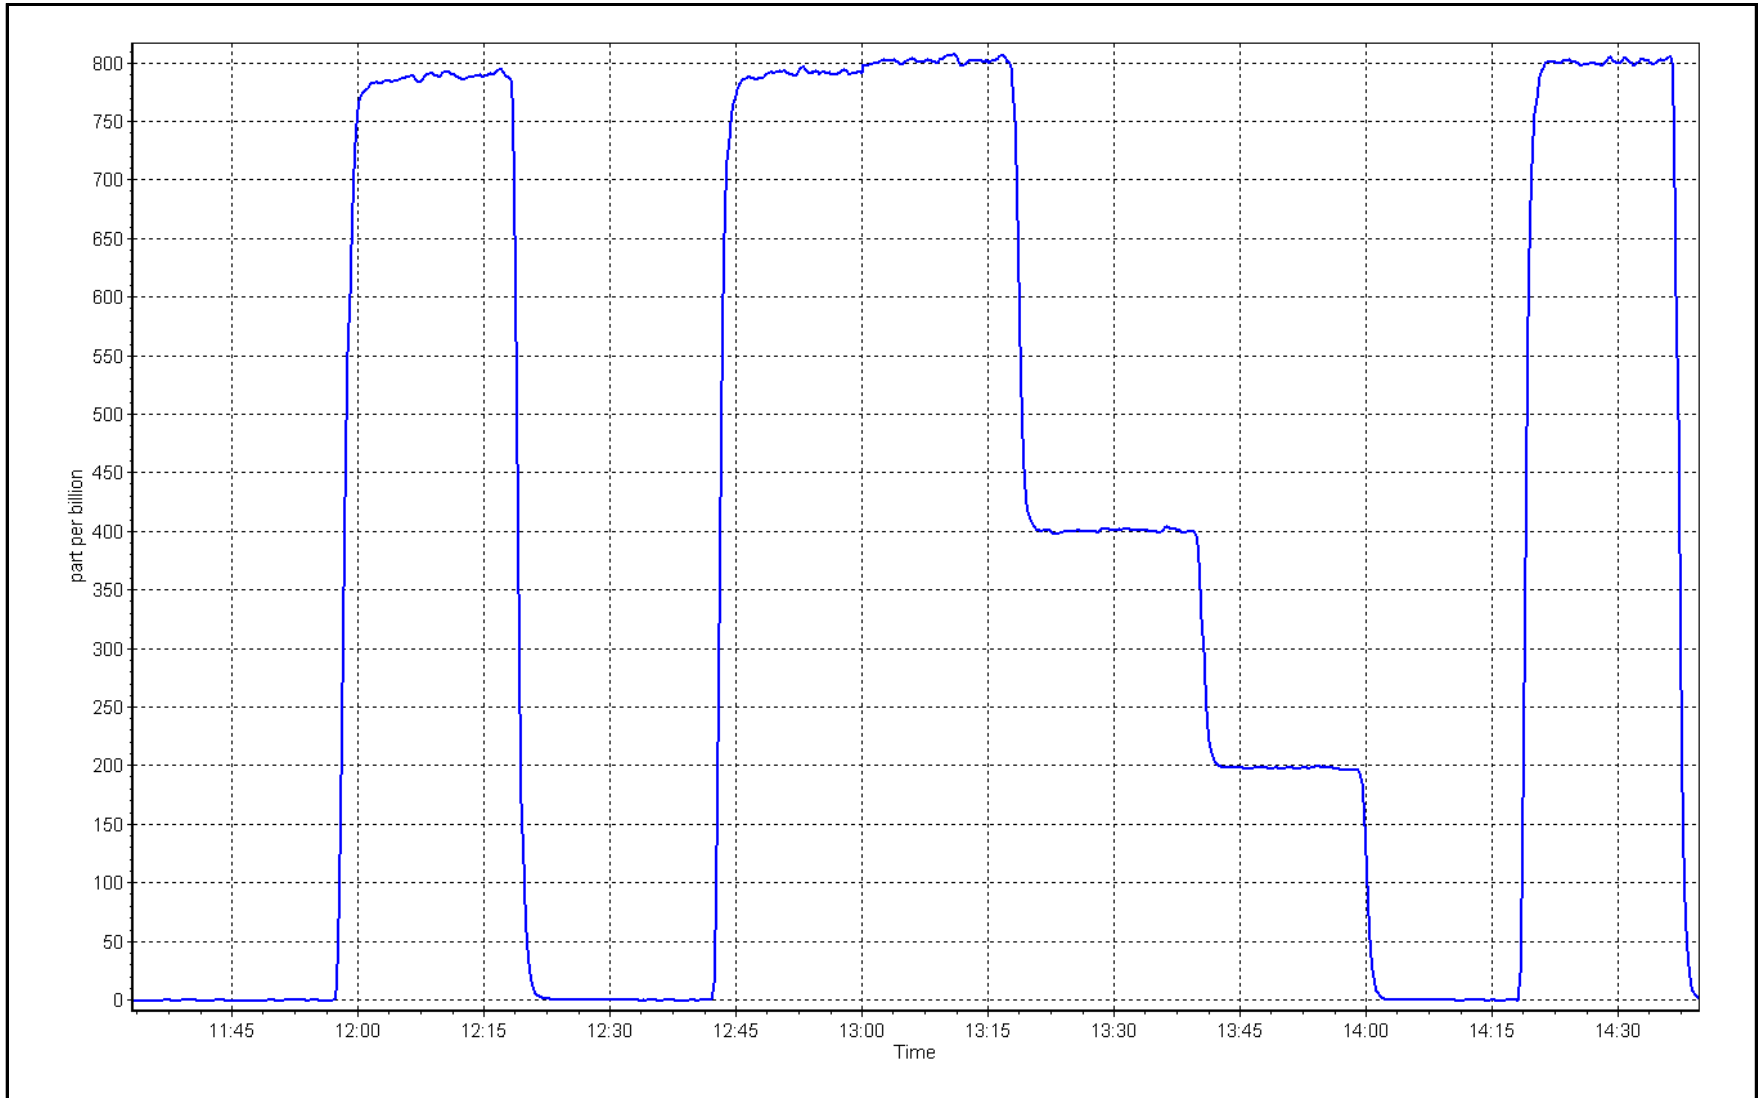



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name: Stony Mountain Station number: AMS18
 Calibration Date: January 18, 2023 Last Cal Date: December 14, 2022
 Start time (MST): 10:24 End time (MST): 14:43
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.479 ppm Cal Gas Exp Date: January 4, 2025
 Cal Gas Cylinder #: CC500395
 Removed Cal Gas Conc: 5.479 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: Teledyne API T700 Serial Number: 2658
 ZAG Make/Model: Teledyne API T701 Serial Number: 360

Analyzer Information

Analyzer make: Thermo 43i-TLE Analyzer serial #: 1218153359
 Converter make: CD Nova CDN-101 Converter serial #: 555
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.994298	0.989724	Backgd or Offset: 2.53	2.55
Calibration intercept:	0.241122	0.201244	Coeff or Slope: 1.129	1.129

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4927	73.0	80.0	78.4	1.022
as found 2nd point	4964	36.5	40.0	39.6	1.012
as found 3rd point	4983	18.3	20.0	19.7	1.023
new cylinder response					

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.2	----
high point	4927	73.0	80.0	79.3	1.009
second point	4964	36.5	40.0	40.0	1.000
third point	4983	18.3	20.0	19.9	1.007
as left zero	5000	0.0	0.0	0.2	----
as left span	4927	73.0	80.0	79.2	1.010
SO2 Scrubber Check	4923	77.1	771.0	0.0	----
Date of last scrubber change:	17-Dec-21			Ave Corr Factor	1.005
Date of last converter efficiency test:					efficiency

Baseline Corr As found: 78.3 Prev response: 79.78 *% change: -1.9%
 Baseline Corr 2nd AF pt: 39.5 AF Slope: 0.979436 AF Intercept: 0.161419
 Baseline Corr 3rd AF pt: 19.6 AF Correlation: 0.999971

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. Scrubber check completed after calibrator zero. No adjustments made.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 18, 2023	Previous Calibration:	December 14, 2022
Station Name:	Stony Mountain	Station Number:	AMS18
Start Time (MST):	10:24	End Time (MST):	14:43
Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1218153359

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999979	≥0.995
80.0	79.3	1.0087			
40.0	40.0	0.9998	Slope	0.989724	0.90 - 1.10
20.0	19.9	1.0074			
			Intercept	0.201244	+/-3

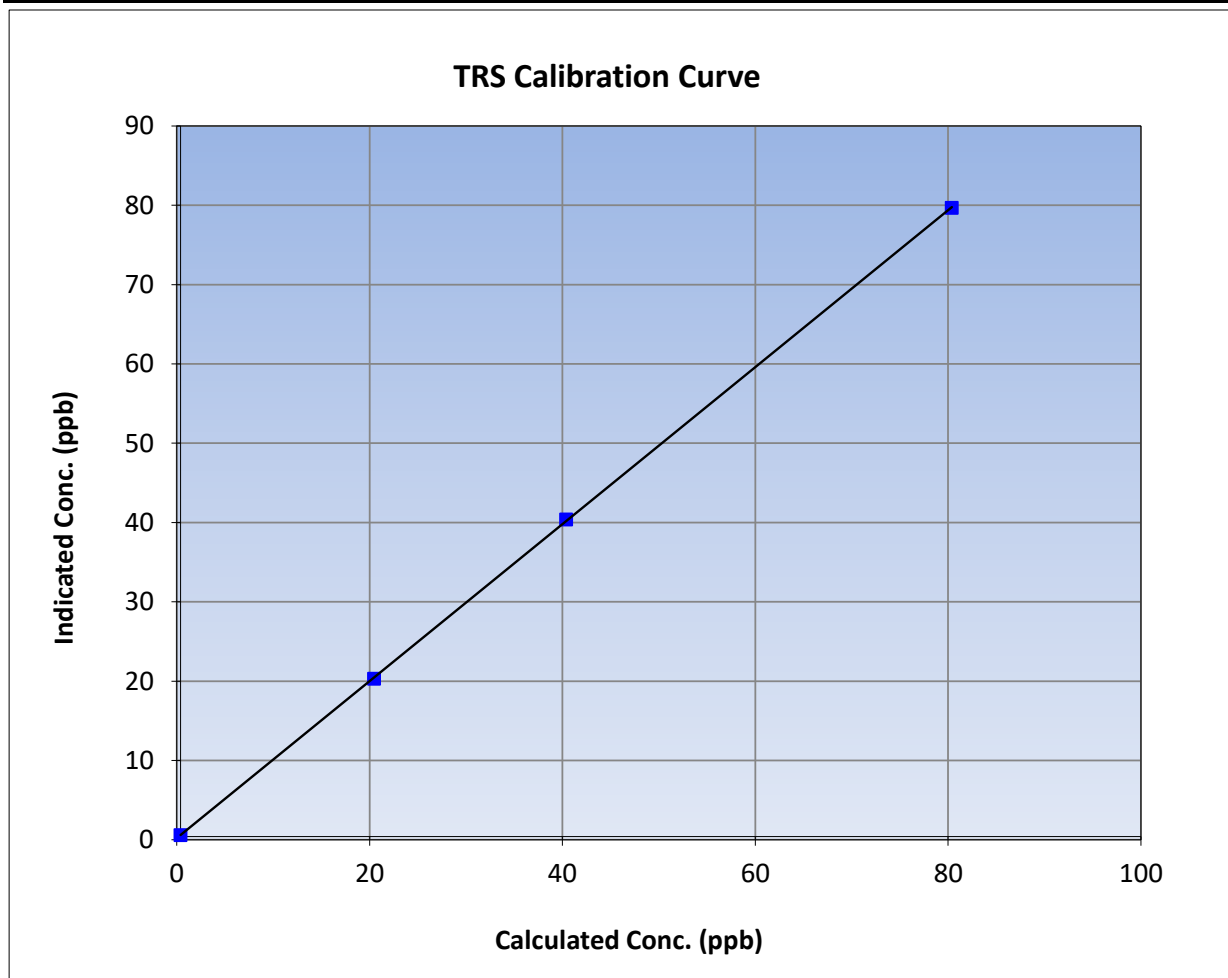

TRS Calibration Plot

Date: January 18, 2023

Location: Stony Mountain

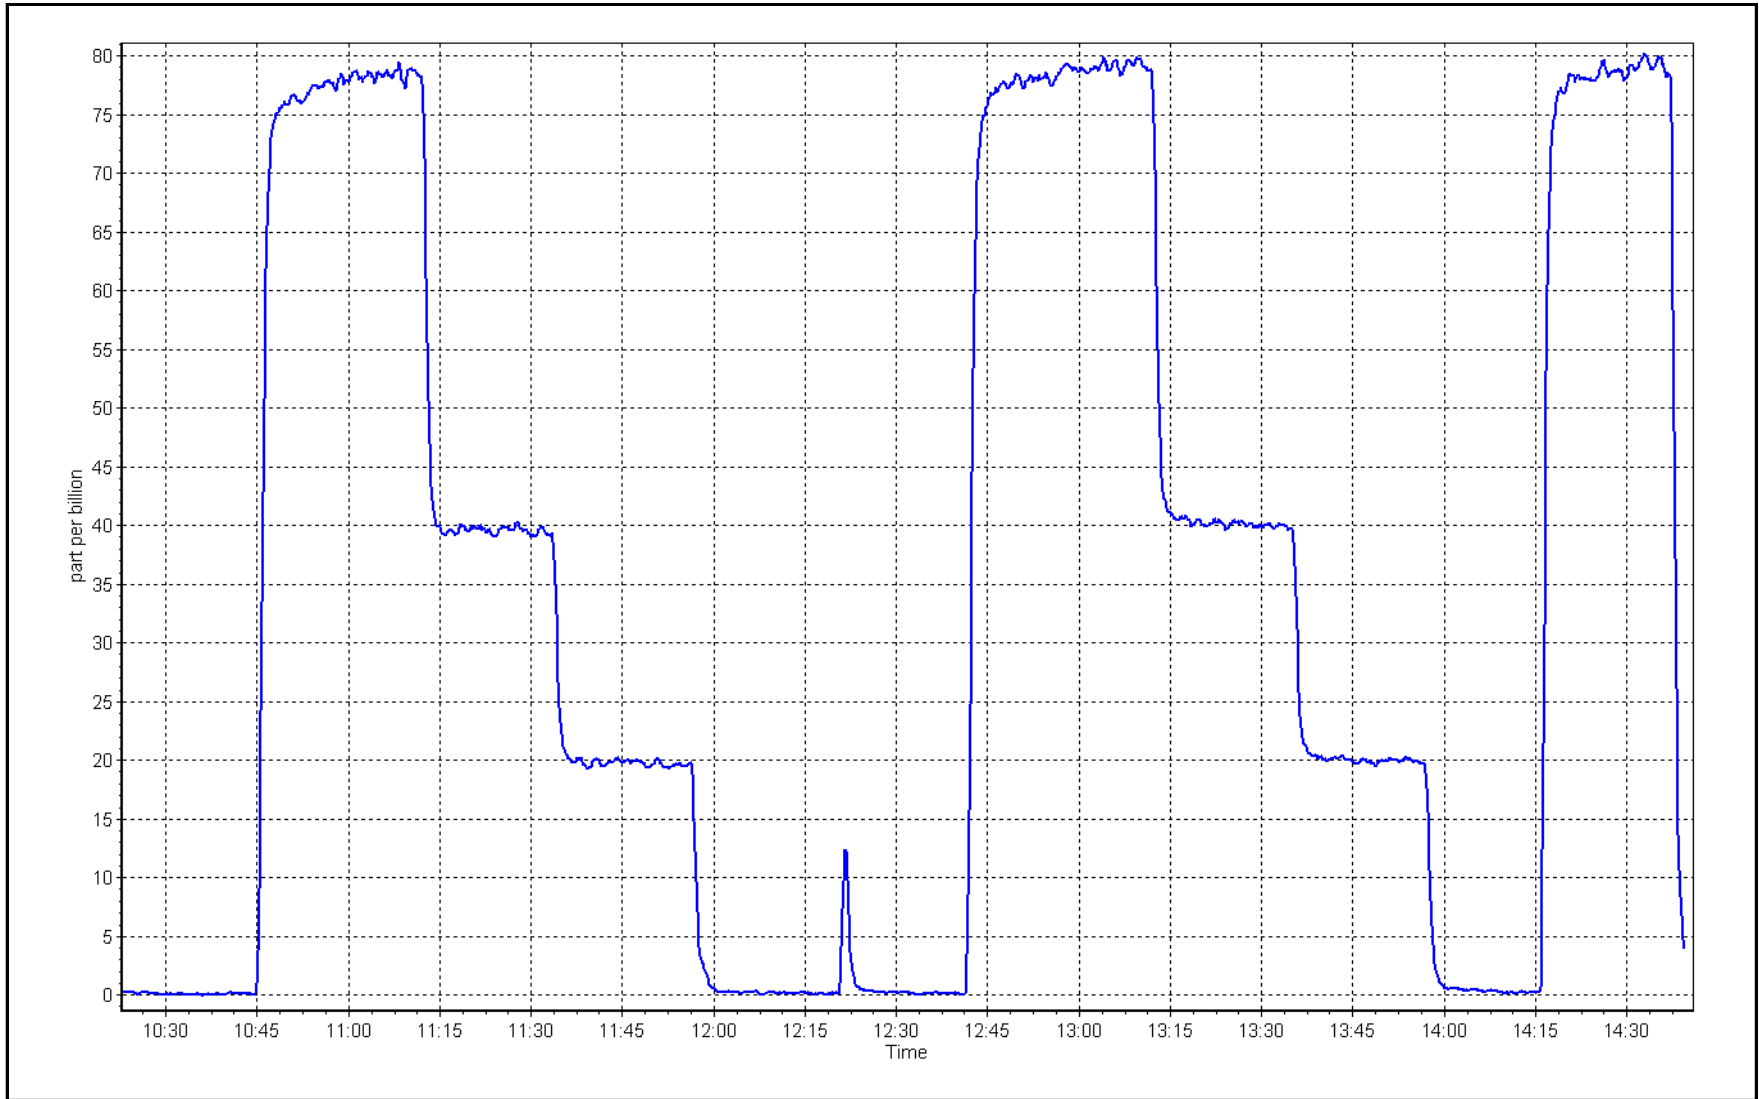



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Stony Mountain	Station number:	AMS 18
Calibration Date:	January 16, 2023	Last Cal Date:	December 15, 2022
Start time (MST):	11:35	End time (MST):	14:42
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC463851	Cal Gas Expiry Date:	February 23, 2025
CH ₄ Cal Gas Conc.	500.8 ppm	CH ₄ Equiv Conc.	1066.8 ppm
C ₃ H ₈ Cal Gas Conc.	205.8 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	500.8 ppm	CH ₄ Equiv Conc.	1066.8 ppm
Removed C ₃ H ₈ Conc.	205.8 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	Teledyne API T700	Serial Number:	2658
ZAG make/model:	Teledyne API T701H	Serial Number:	360

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1180320039
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	3.03E-04	3.06E-04	NMHC SP Ratio:	5.53E-05
CH ₄ Retention time:	14.60	14.60	NMHC Peak Area:	165923
				162130

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4919	81.0	17.28	16.99	1.017
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4919	81.0	17.28	17.25	1.002
second point	4959	40.5	8.64	8.61	1.004
third point	4979	20.2	4.31	4.29	1.005
as left zero	5000	0.0	0.00	0.00	----
as left span	4919	81.0	17.28	17.35	0.996

Average Correction Factor				1.004
Baseline Corr AF:	16.99	Prev response	17.31	*% change -1.9%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4919	81.0	9.17	8.94	1.026
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4919	81.0	9.17	9.14	1.003
second point	4959	40.5	4.58	4.58	1.002
third point	4979	20.2	2.29	2.29	0.999
as left zero	5000	0	0.00	0.00	----
as left span	4919	81	9.17	9.21	0.996
Average Correction Factor					1.001
Baseline Corr AF:	8.94	Prev response	9.17	*% change	-2.5%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4919	81.0	8.11	8.06	1.007
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4919	81.0	8.11	8.11	1.001
second point	4959	40.5	4.06	4.03	1.006
third point	4979	20.2	2.02	2.00	1.012
as left zero	5000	0.0	0.00	0.00	----
as left span	4919	81.0	8.11	8.14	0.996
Average Correction Factor					1.006
Baseline Corr AF:	8.06	Prev response	8.14	*% change	-1.1%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		<i>* = > +/-5% change initiates investigation</i>	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	1.001927	0.998211
THC Cal Offset:	-0.008379	-0.008790
CH ₄ Cal Slope:	1.005440	0.999750
CH ₄ Cal Offset:	-0.017403	-0.013212
NMHC Cal Slope:	0.998694	0.996638
NMHC Cal Offset:	0.009024	0.005021

Notes: Sample inlet filter changed after as founds. Adjusted the span only.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 15, 2022
Station Name:	Stony Mountain	Station Number:	AMS 18
Start Time (MST):	11:35	End Time (MST):	14:42
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320039

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999998	≥ 0.995
17.28	17.25	1.0019			
8.64	8.61	1.0040			
4.31	4.29	1.0050			
			Slope	0.998211	0.90 - 1.10
			Intercept	-0.008790	+/-0.5

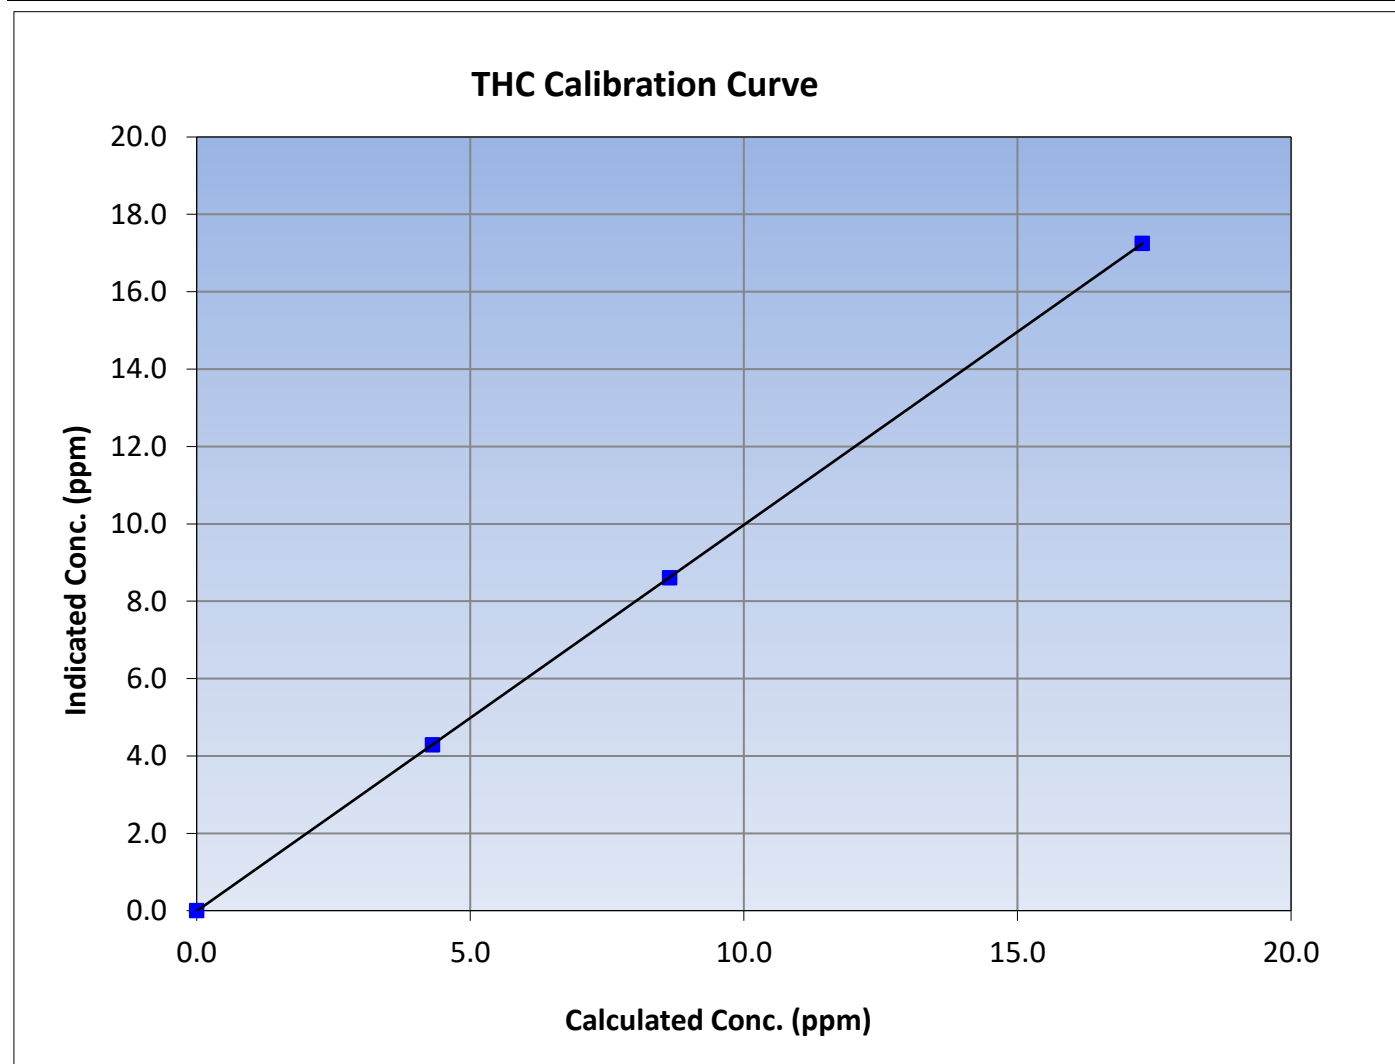



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 15, 2022
Station Name:	Stony Mountain	Station Number:	AMS 18
Start Time (MST):	11:35	End Time (MST):	14:42
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320039

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999987	≥ 0.995
8.11	8.11	1.0009			
4.06	4.03	1.0064			
2.02	2.00	1.0118			
			Slope	0.999750	0.90 - 1.10
			Intercept	-0.013212	+/-0.5

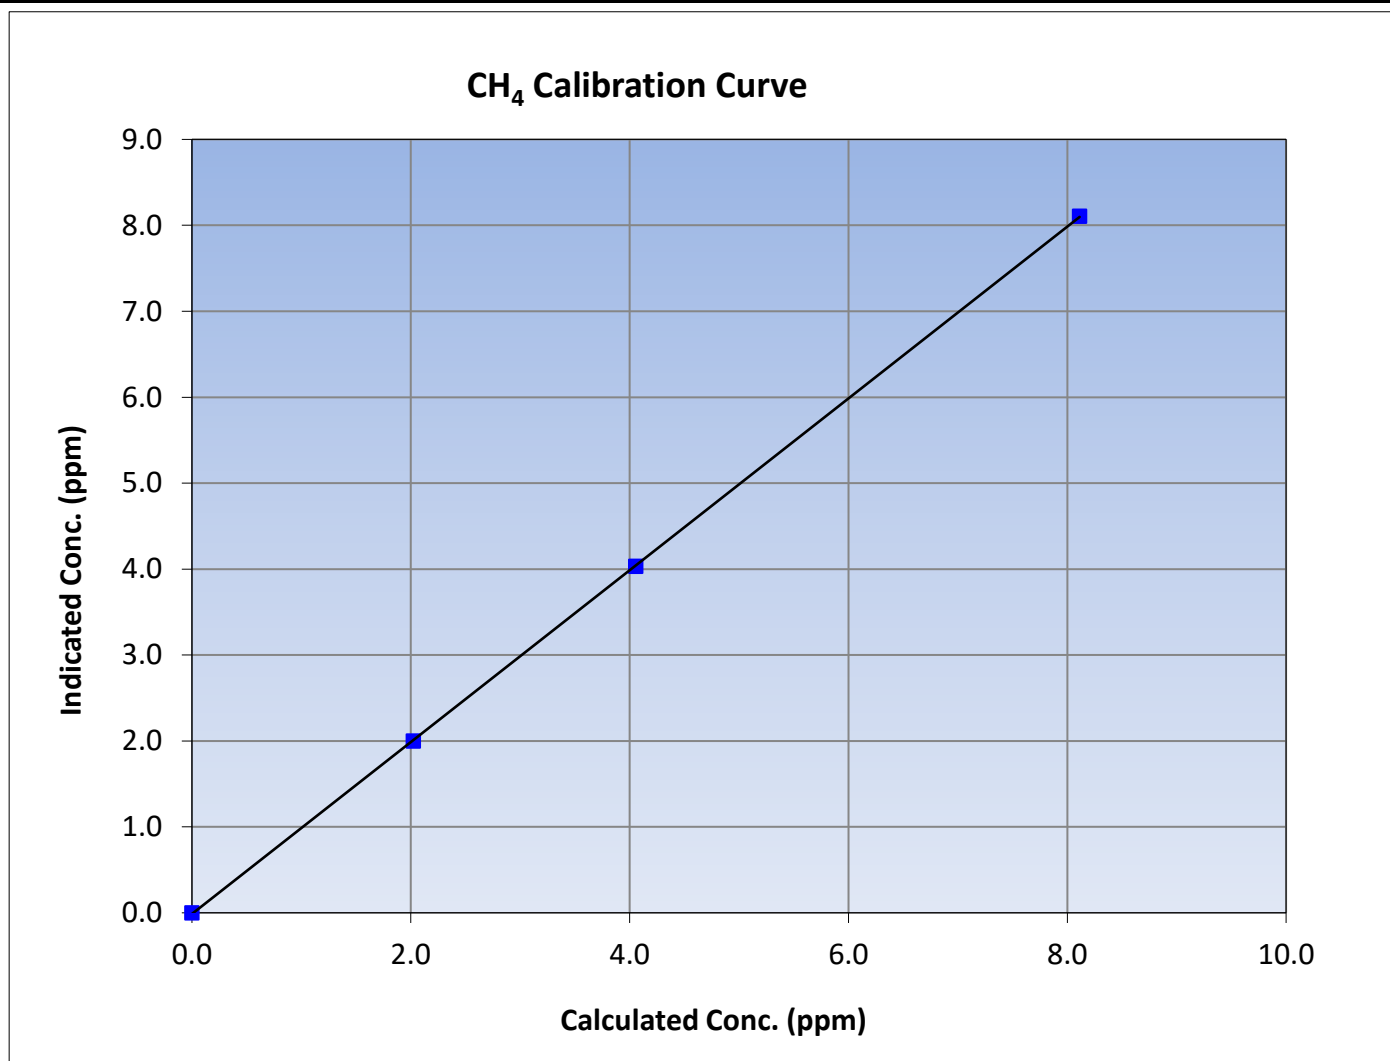



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 16, 2023	Previous Calibration:	December 15, 2022
Station Name:	Stony Mountain	Station Number:	AMS 18
Start Time (MST):	11:35	End Time (MST):	14:42
Analyzer make:	Thermo 55i	Analyzer serial #:	1180320039

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999999	≥ 0.995			
9.17	9.14	1.0031						
4.58	4.58	1.0017				Slope	0.996638	0.90 - 1.10
2.29	2.29	0.9990						
			Intercept	0.005021	± 0.5			

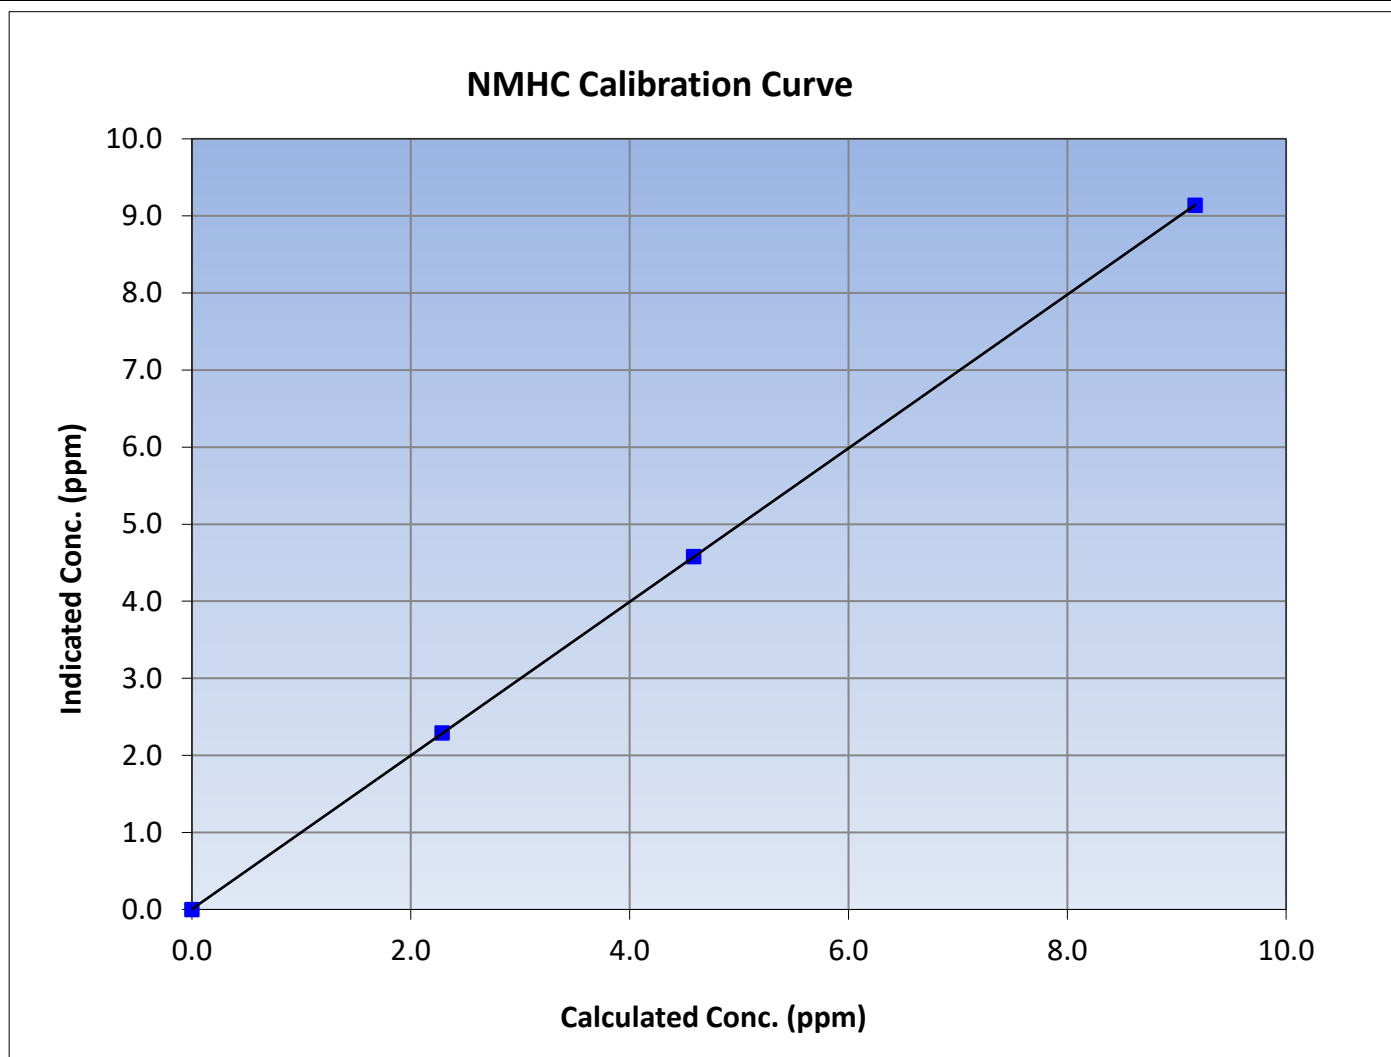

NMHC Calibration Plot

Date: January 16, 2023

Location: Stony Mountain

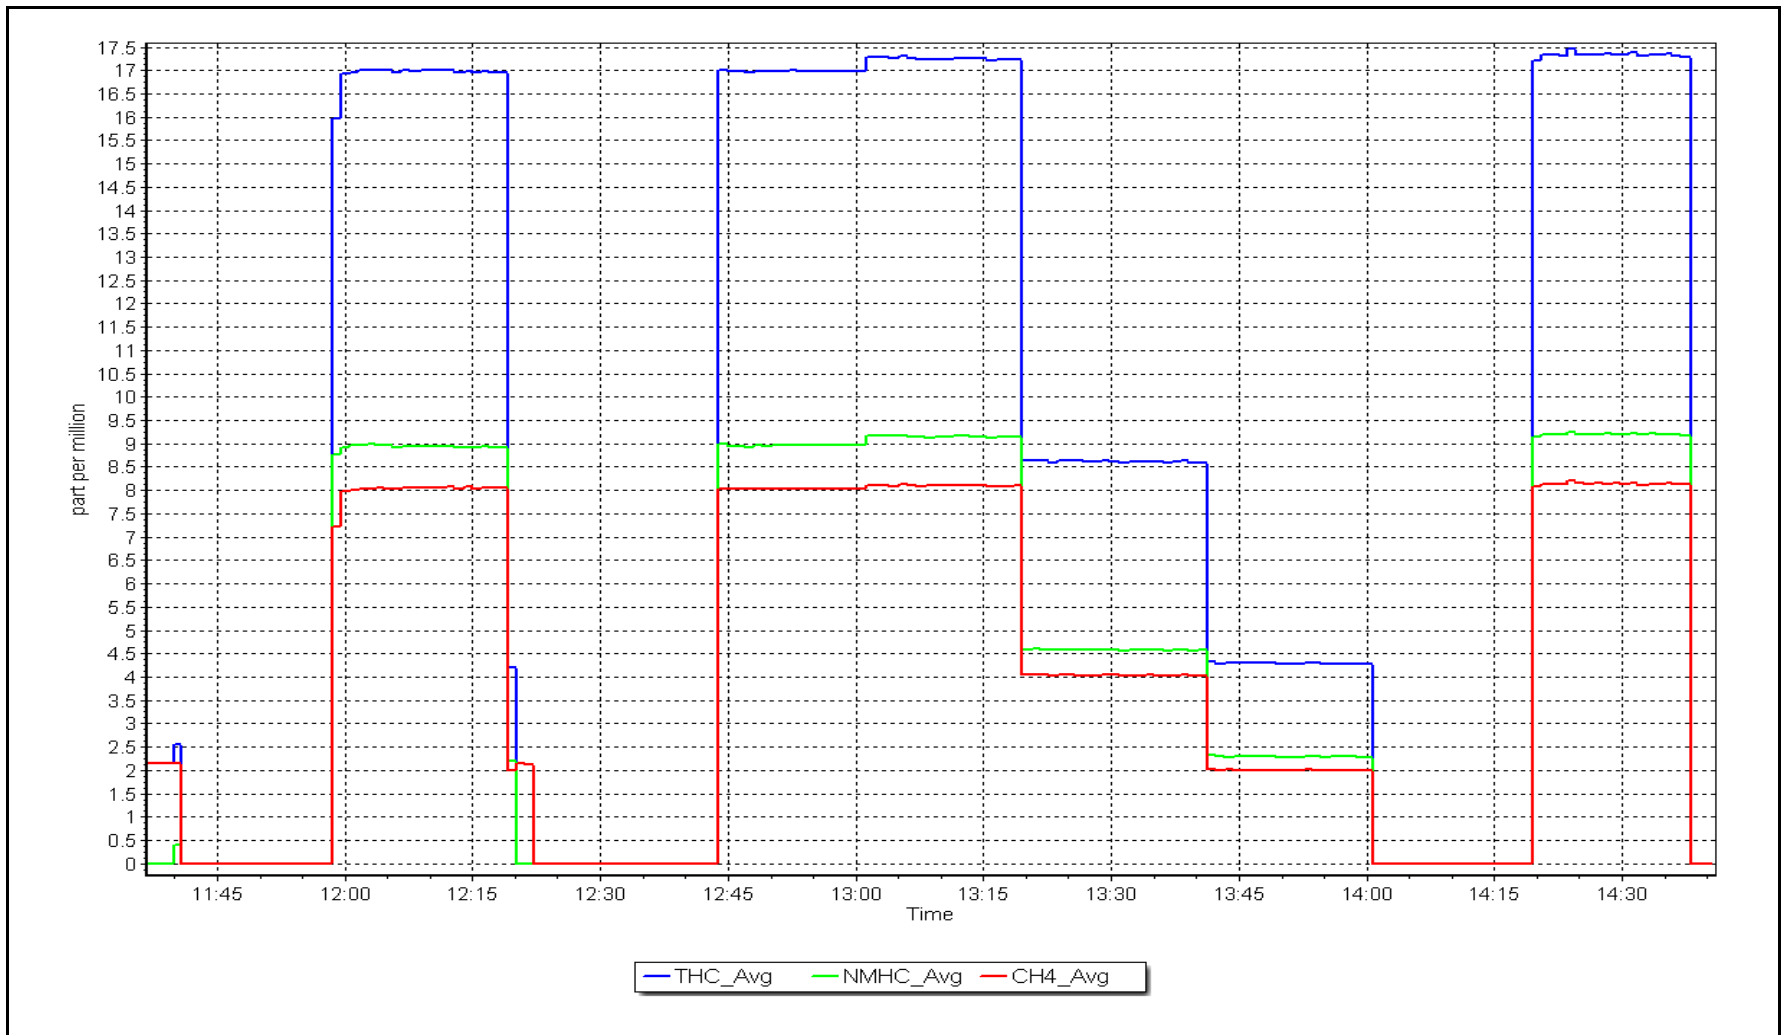



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Stony Mountain
Calibration Date: January 24, 2023
Start time (MST): 10:19
Reason: Cylinder Change
Station number: AMS 18
Last Cal Date: December 21, 2022
End time (MST): 15:58

Calibration Standards

NO Gas Cylinder #: T2XX7ME
NOX Cal Gas Conc: 50.48 ppm
Removed Cylinder #: T2Y1P5K
Removed Gas NOX Conc: 51.06 ppm
NOX gas Diff: -0.5%
Calibrator Model: Teledyne API T700
ZAG make/model: Teledyne API 701H
Cal Gas Expiry Date: January 14, 2024
NO Cal Gas Conc: 49.22 ppm
Removed Gas Exp Date: December 11, 2023
Removed Gas NO Conc: 50.35 ppm
NO gas Diff: -0.6%
Serial Number: 2658
Serial Number: 360

Analyzer Information

Analyzer make: Thermo 42i
NOX Range (ppb): 0 - 1000 ppb
Analyzer serial #: 1336160088

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.026	1.043	NO bkgnd or offset:	2.9	2.9
NOX coeff or slope:	0.990	0.987	NOX bkgnd or offset:	2.9	2.9
NO2 coeff or slope:	0.999	0.999	Reaction cell Press:	225.3	218.6

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.000898	1.000554
NO _x Cal Offset:	-0.096867	0.069933
NO Cal Slope:	1.001322	1.001394
NO Cal Offset:	-1.059867	-0.829546
NO ₂ Cal Slope:	0.997471	1.001873
NO ₂ Cal Offset:	0.297014	0.315702



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-0.1	-0.1	0.0	----	----
as found span	4921	79.4	810.8	799.5	11.3	804.0	790.1	13.9	1.0084	1.0119
as found 2nd										
as found 3rd										
new cyl resp	4919	81.3	820.8	800.3	20.5	809.7	786.2	23.4	1.0137	1.0179
calibrator zero	5000	0.0	0.0	0.0	0.0	0.1	0.0	0.1	----	----
high point	4919	81.3	820.8	800.3	20.5	821.2	801.0	20.2	0.9995	0.9991
second point	4959	40.7	410.9	400.7	10.3	411.5	399.9	11.6	0.9986	1.0019
third point	4980	20.3	204.9	199.8	5.1	204.9	198.5	6.4	1.0002	1.0067
as left zero	5000	0.0	0.0	0.0	0.0	0.2	0.0	0.2	----	----
as left span	4919	81.3	820.8	390.0	430.8	824.1	387.7	436.5	0.9959	1.0059
Average Correction Factor									0.9994	1.0026

Corrected As found	NO _x = 804.1 ppb	NO = 790.2 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -0.9%
Previous Response	NO _x = 811.4 ppb	NO = 799.5 ppb		*Percent Change	NO = -1.2%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	799.5	389.2	430.8	431.8	0.9977	100.2%
2nd GPT point (200 ppb O3)	799.5	585.7	234.3	235.1	0.9965	100.3%
3rd GPT point (100 ppb O3)	799.5	695.7	124.3	125.1	0.9935	100.7%
Average Correction Factor					0.9959	100.4%

Notes: Changed calibration gas cylinder after as founds. Sample inlet filter changed after new cylinder response. Adjusted the span only.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 21, 2022
Station Name:	Stony Mountain	Station Number:	AMS 18
Start Time (MST):	10:19	End Time (MST):	15:58
Analyzer make:	Thermo 42i	Analyzer serial #:	1336160088

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.1	----	Correlation Coefficient	≥0.995	
820.8	821.2	0.9995			
410.9	411.5	0.9986			
204.9	204.9	1.0002			
			Slope	1.000554	0.90 - 1.10
			Intercept	0.069933	+/-20

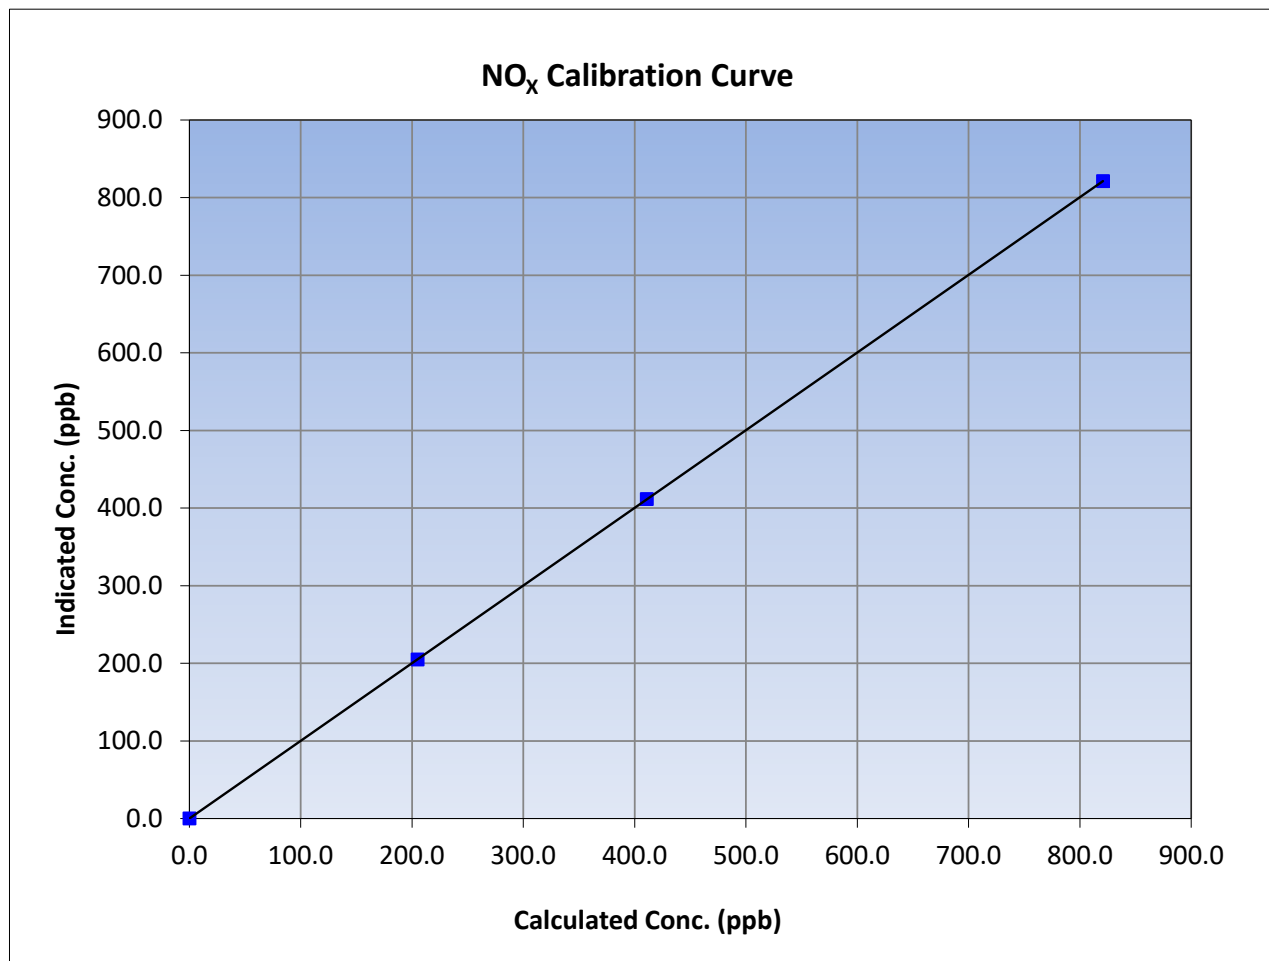



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 21, 2022
Station Name:	Stony Mountain	Station Number:	AMS 18
Start Time (MST):	10:19	End Time (MST):	15:58
Analyzer make:	Thermo 42i	Analyzer serial #:	1336160088

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20	
800.3	801.0	0.9991			0.999995
400.7	399.9	1.0019			1.001394
199.8	198.5	1.0067			-0.829546

NO Calibration Curve

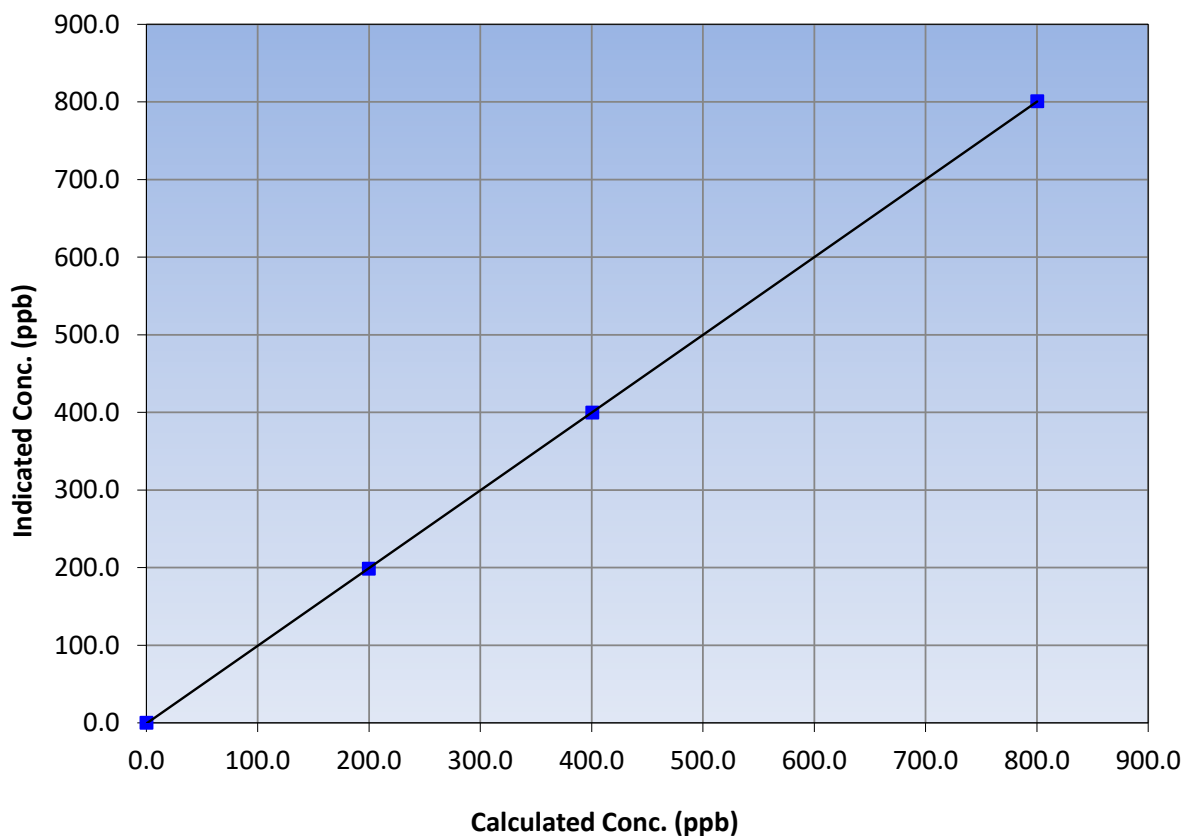



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 21, 2022
Station Name:	Stony Mountain	Station Number:	AMS 18
Start Time (MST):	10:19	End Time (MST):	15:58
Analyzer make:	Thermo 42i	Analyzer serial #:	1336160088

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.0	0.1	----	Correlation Coefficient	0.999999	≥0.995
430.8	431.8	0.9977			
234.3	235.1	0.9965			
124.3	125.1	0.9935			
			Slope	1.001873	0.90 - 1.10
			Intercept	0.315702	+/-20

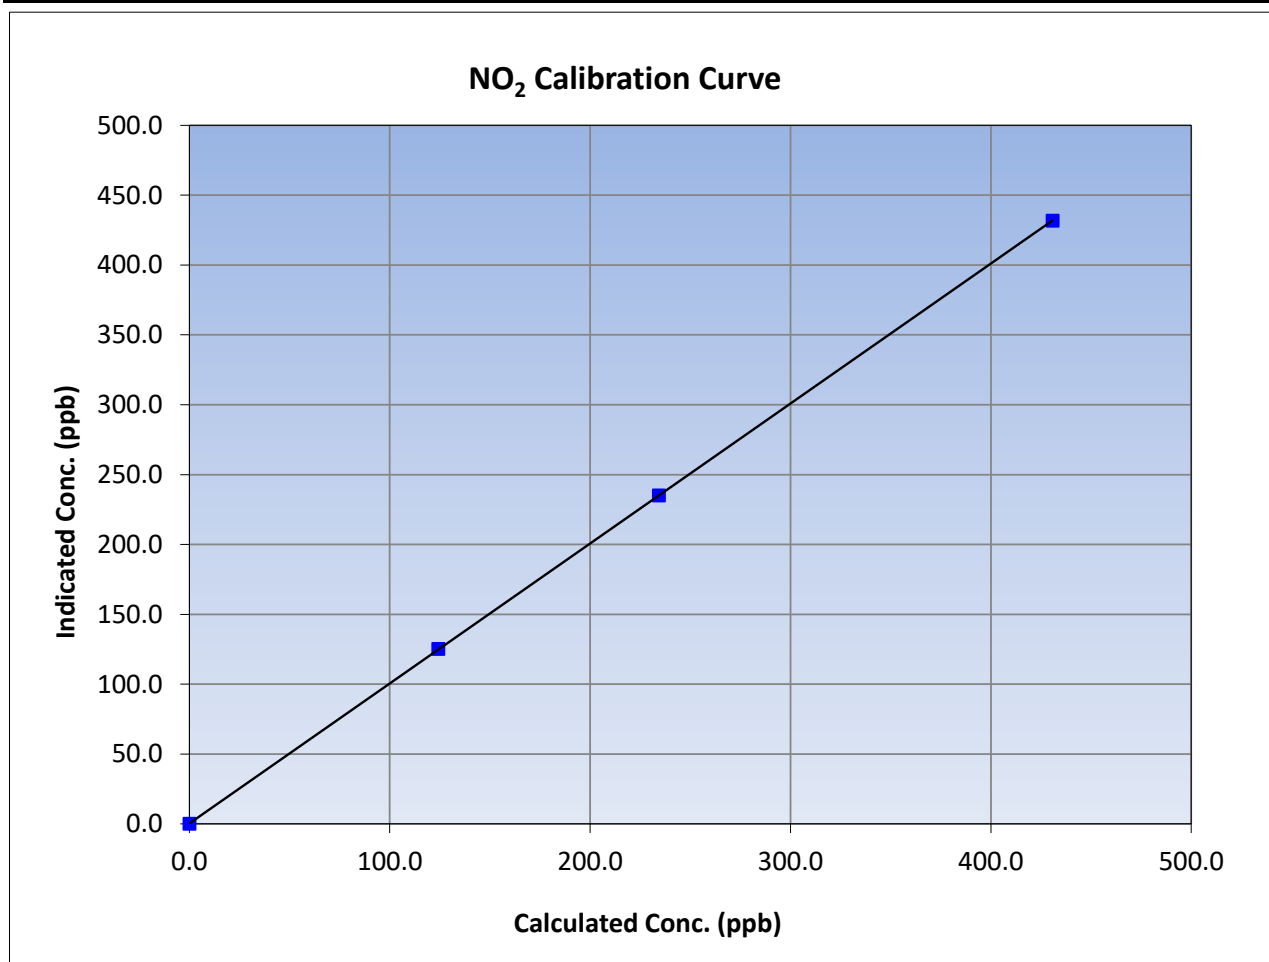

NO_x Calibration Plot

Date: January 24, 2023

Location: Stony Mountain

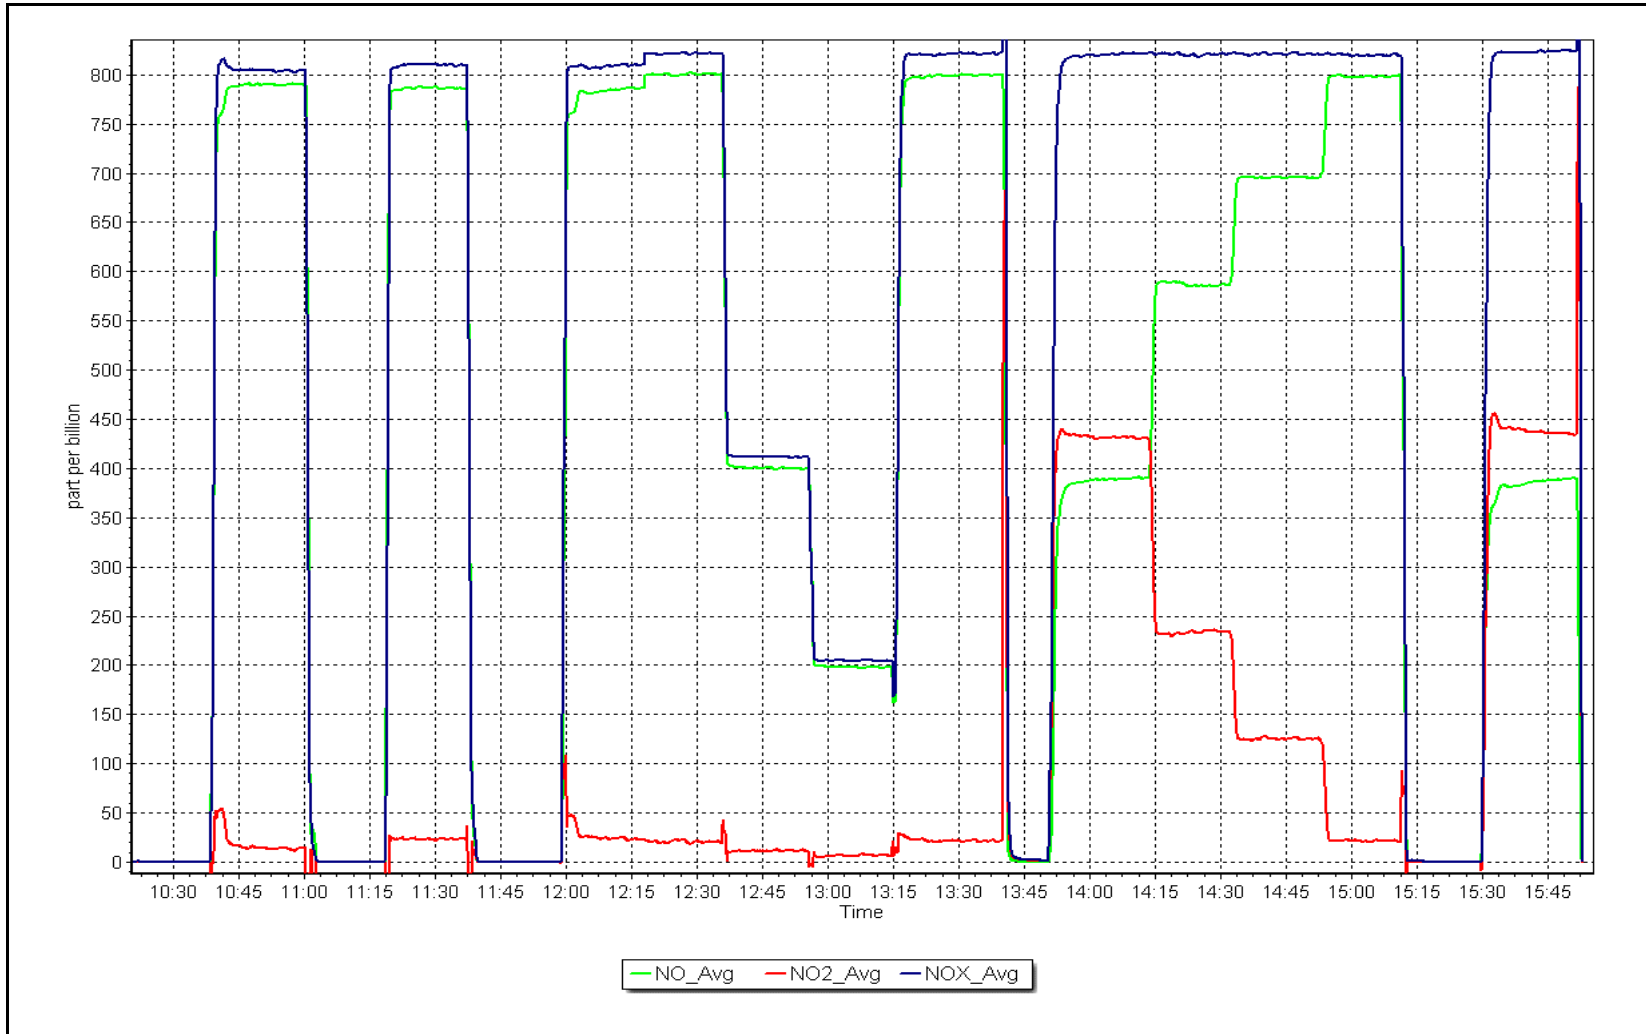



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Stony Mountain Station number: AMS18
 Calibration Date: January 9, 2023 Last Cal Date: December 1, 2022
 Start time (MST): 11:20 End time (MST): 14:20
 Reason: Routine

Calibration Standards

O3 generation mode: Photometer
 Calibrator Make/Model: Teledyne API T700 Serial Number: 2658
 ZAG Make/Model: Teledyne API T701H Serial Number: 360

Analyzer Information

Analyzer make: API T400 Analyzer serial #: 825
 Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.997743	0.993114	Backgd or Offset:	1.000	1.000
Calibration intercept:	-0.380000	-0.320000	Coeff or Slope:	0.976	0.976

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	800.0	0.0	-0.4	----
as found span	4888	1096.9	400.0	398.2	1.005
as found 2nd point					
as found 3rd point					
calibrator zero	5000	800.0	0.0	-0.2	----
high point	4888	1101.7	400.0	396.8	1.008
second point	4888	863.9	200.0	198.8	1.006
third point	4888	741.4	100.0	98.5	1.015
as left zero	5000	800.0	0.0	0.2	----
as left span	4812	1097.9	400.0	397.8	1.006
Average Correction Factor					1.010

Baseline Corr As found:	398.6	Previous response	398.7	*% change	0.0%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. No adjustments made.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 9, 2023	Previous Calibration:	December 1, 2022
Station Name:	Stony Mountain	Station Number:	AMS18
Start Time (MST):	11:20	End Time (MST):	14:20
Analyzer make:	API T400	Analyzer serial #:	825

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	-0.2	----	Correlation Coefficient	0.999994	≥0.995
400.0	396.8	1.0081			
200.0	198.8	1.0060	Slope	0.993114	0.90 - 1.10
100.0	98.5	1.0152			
			Intercept	-0.320000	+/- 5

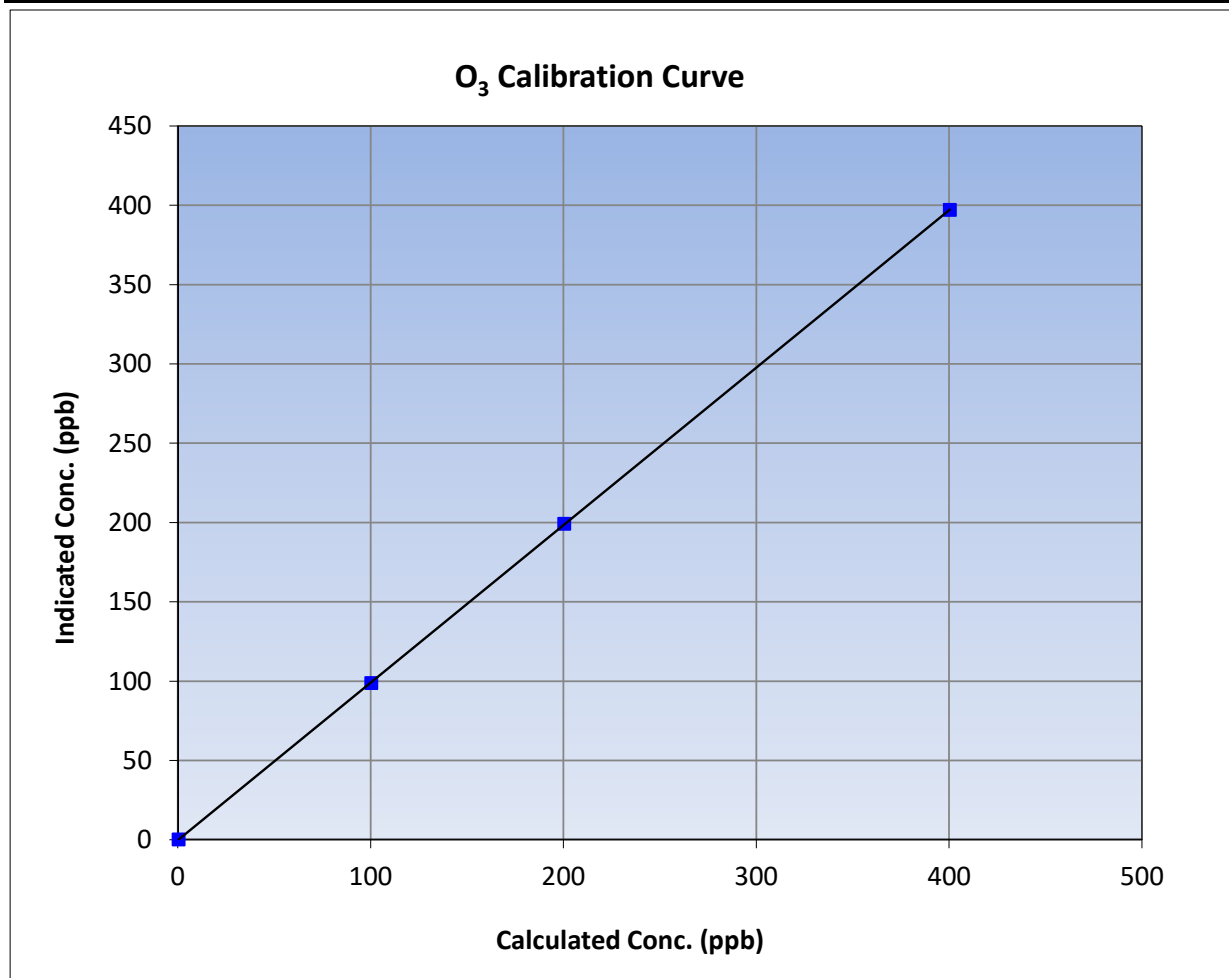

O₃ Calibration Plot

Date: January 9, 2023

Location: Stony Mountain

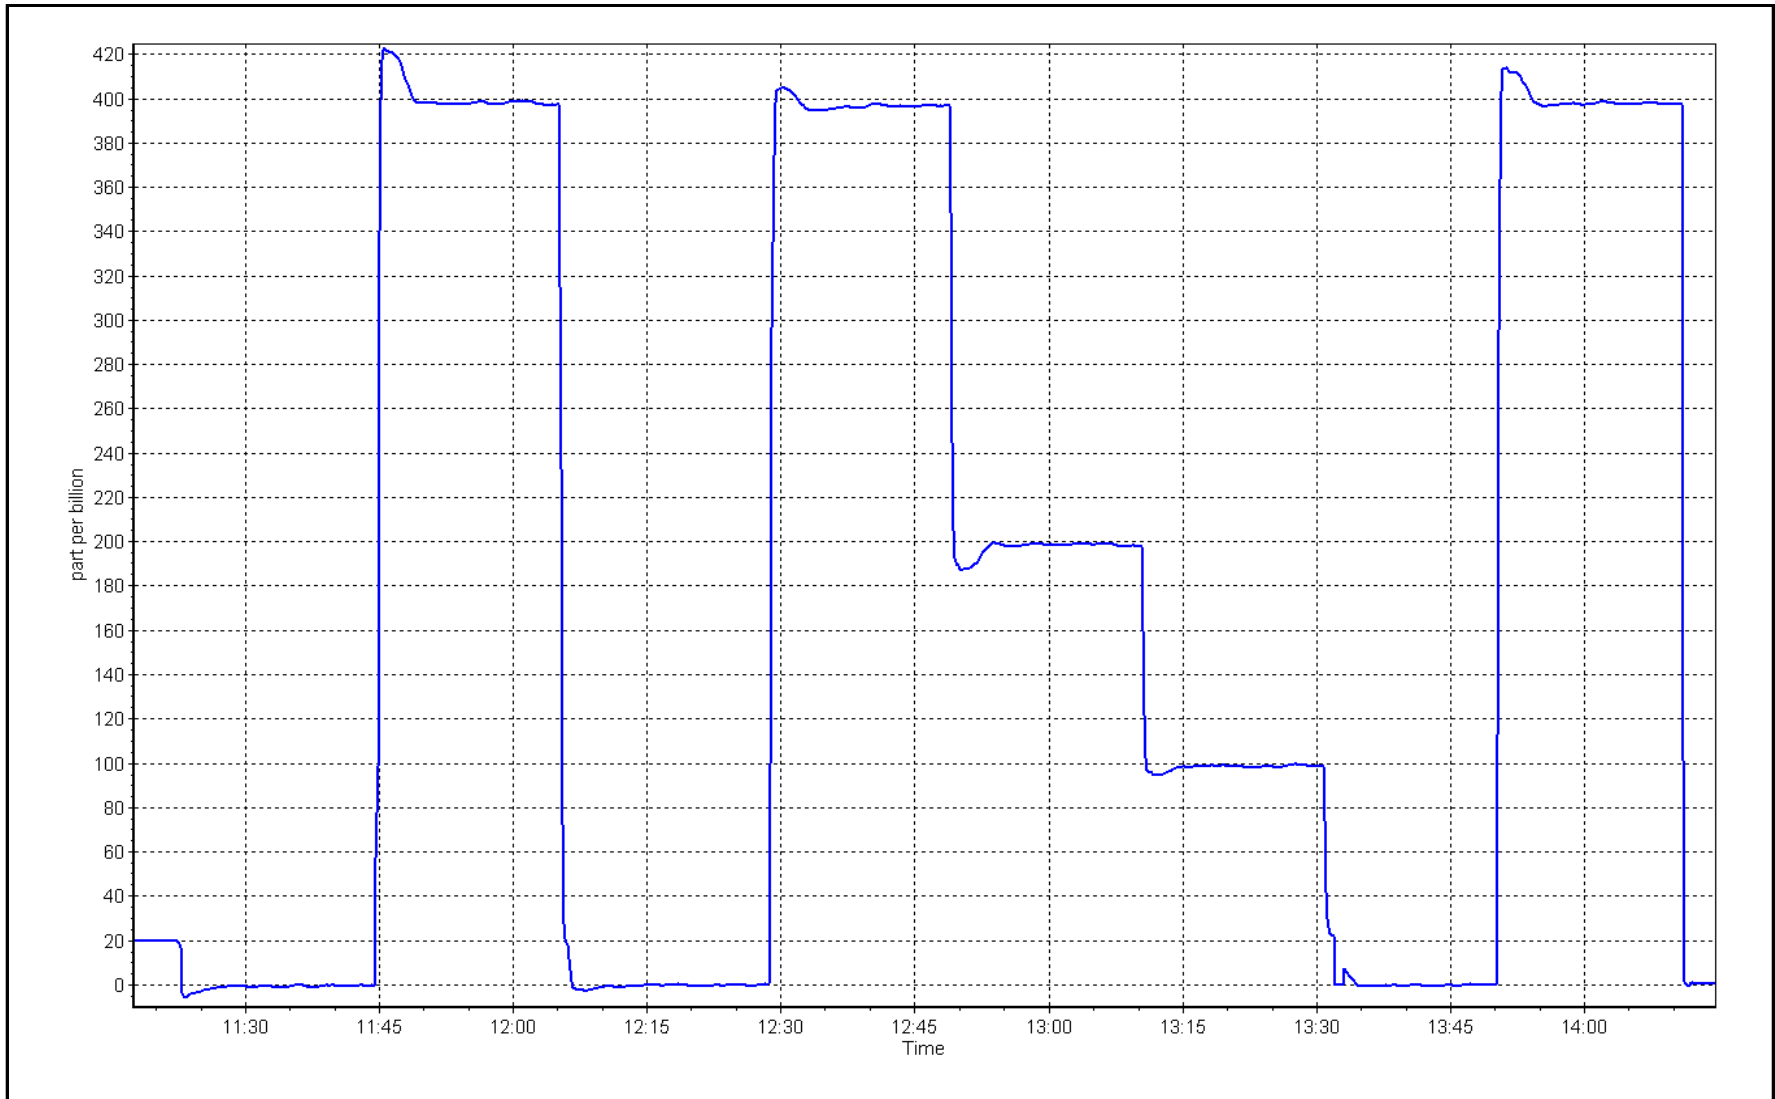



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Stony Mountain Station number: AMS 18
Calibration Date: January 24, 2023 Last Cal Date: December 14, 2022
Start time (MST): 12:20 End time (MST): 12:50

Analyzer Make: API T640 S/N: 1335
Particulate Fraction: PM2.5

Flow Meter Make/Model: DeltaCal S/N: 1102
Temp/RH standard: DeltaCal S/N: 1102

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-2.4	-2.1	-2.4	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	696.4	698.6	696.4	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5.01	4.95	5.01	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 24, 2023 Last Cal Date: December 14, 2022
PM w/o HEPA: 3.2 PM w/ HEPA: 0.0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test				<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: November 16, 2022
Disposable Filter Changed: November 16, 2022

Annual Maintenance

Date Sample Tube Cleaned: August 30, 2022
Date RH/T Sensor Cleaned: August 30, 2022

Notes: No adjustments made to temperature, pressure or flow. Leak check passed.

Calibration by: Karan Pandit



Wood Buffalo Environmental Association

CO Calibration Report

Version-01-2020

Station Information

Station Name:	Stony Mountain	Station number:	AMS 18
Calibration Date:	January 6, 2023	Last Cal Date:	December 12, 2022
Start time (MST):	10:46	End time (MST):	13:37
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	3,050	ppm	Cal Gas Exp Date:	December 1, 2028
Cal Gas Cylinder #:	ALM063503			
Removed Cal Gas Conc:	3,050	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	2658
ZAG Make/Model:	Teledyne API T701		Serial Number:	360

Analyzer Information

Analyzer make:	API T300	Analyzer serial #:	3504
Analyzer Range:	0 - 50 ppm		

	Start	Finish		Start	Finish
Calibration slope:	1.009187	1.018233	Backgd or Offset:	-0.009	-0.009
Calibration intercept:	0.095767	0.009764	Coeff or Slope:	0.910	0.916

CO Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4933	66.7	40.7	41.4	0.982
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.0	----
high point	4933	66.7	40.7	41.4	0.983
second point	4966	33.3	20.3	20.8	0.975
third point	4983	16.7	10.2	10.3	0.987
as left zero	3000	0.0	0.0	0.0	----
as left span	2960	40.0	40.7	41.6	0.979
Average Correction Factor					0.982

Baseline Corr As found:	41.29	Prev response:	41.16	*% change:	0.3%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. Adjusted the zero only.

Calibration Performed By: Karan Pandit



Wood Buffalo Environmental Association

CO Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 6, 2023	Previous Calibration:	December 12, 2022
Station Name:	Stony Mountain	Station Number:	AMS 18
Start Time (MST):	10:46	End Time (MST):	13:37
Analyzer make:	API T300	Analyzer serial #:	3504

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>
0.0	0.0	----	Correlation Coefficient	0.999973
40.7	41.4	0.9831		
20.3	20.8	0.9753	Slope	1.018233
10.2	10.3	0.9872		
			Intercept	0.009764
				± 1.5

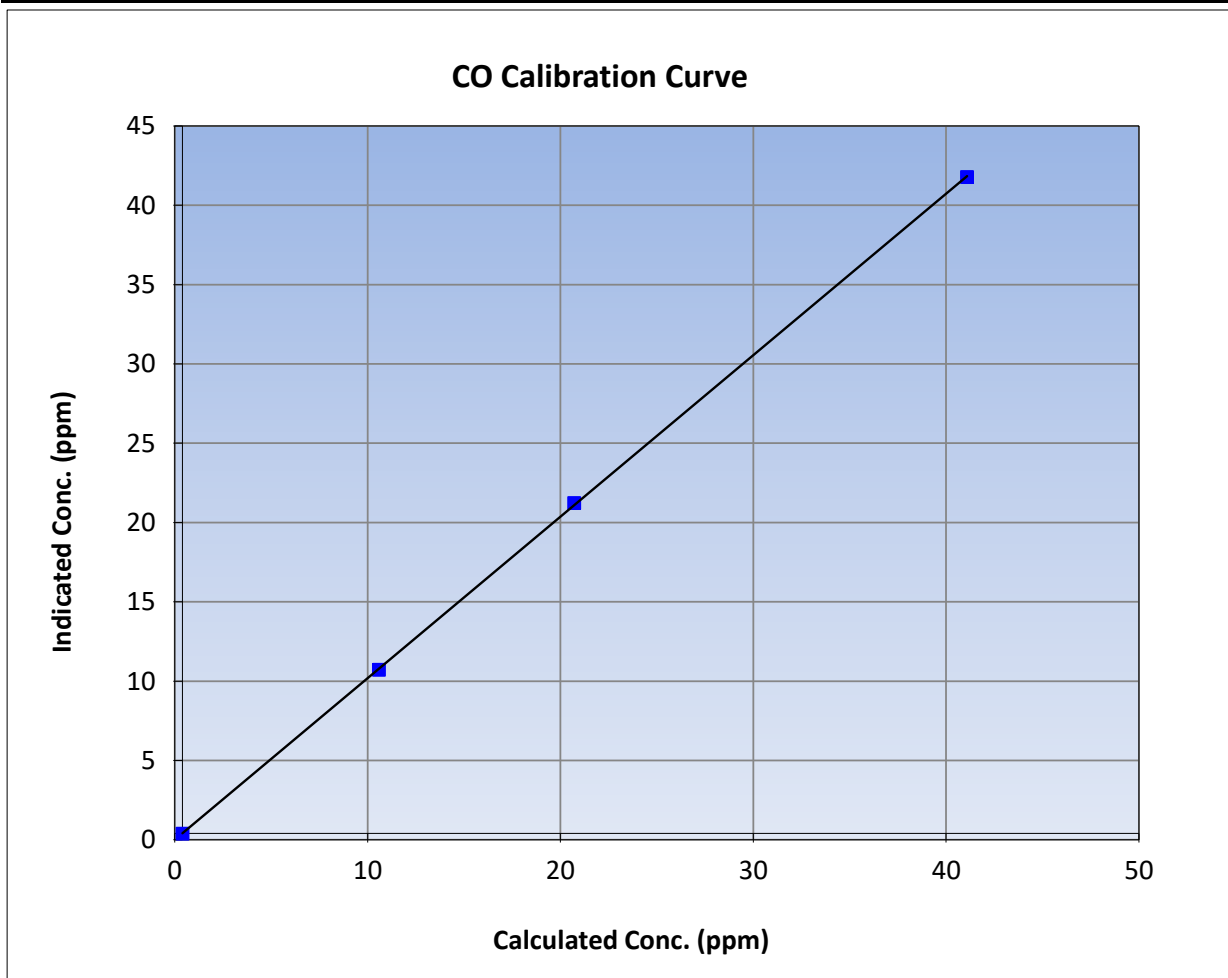

CO Calibration Plot

Date: January 6, 2023

Location: Stony Mountain

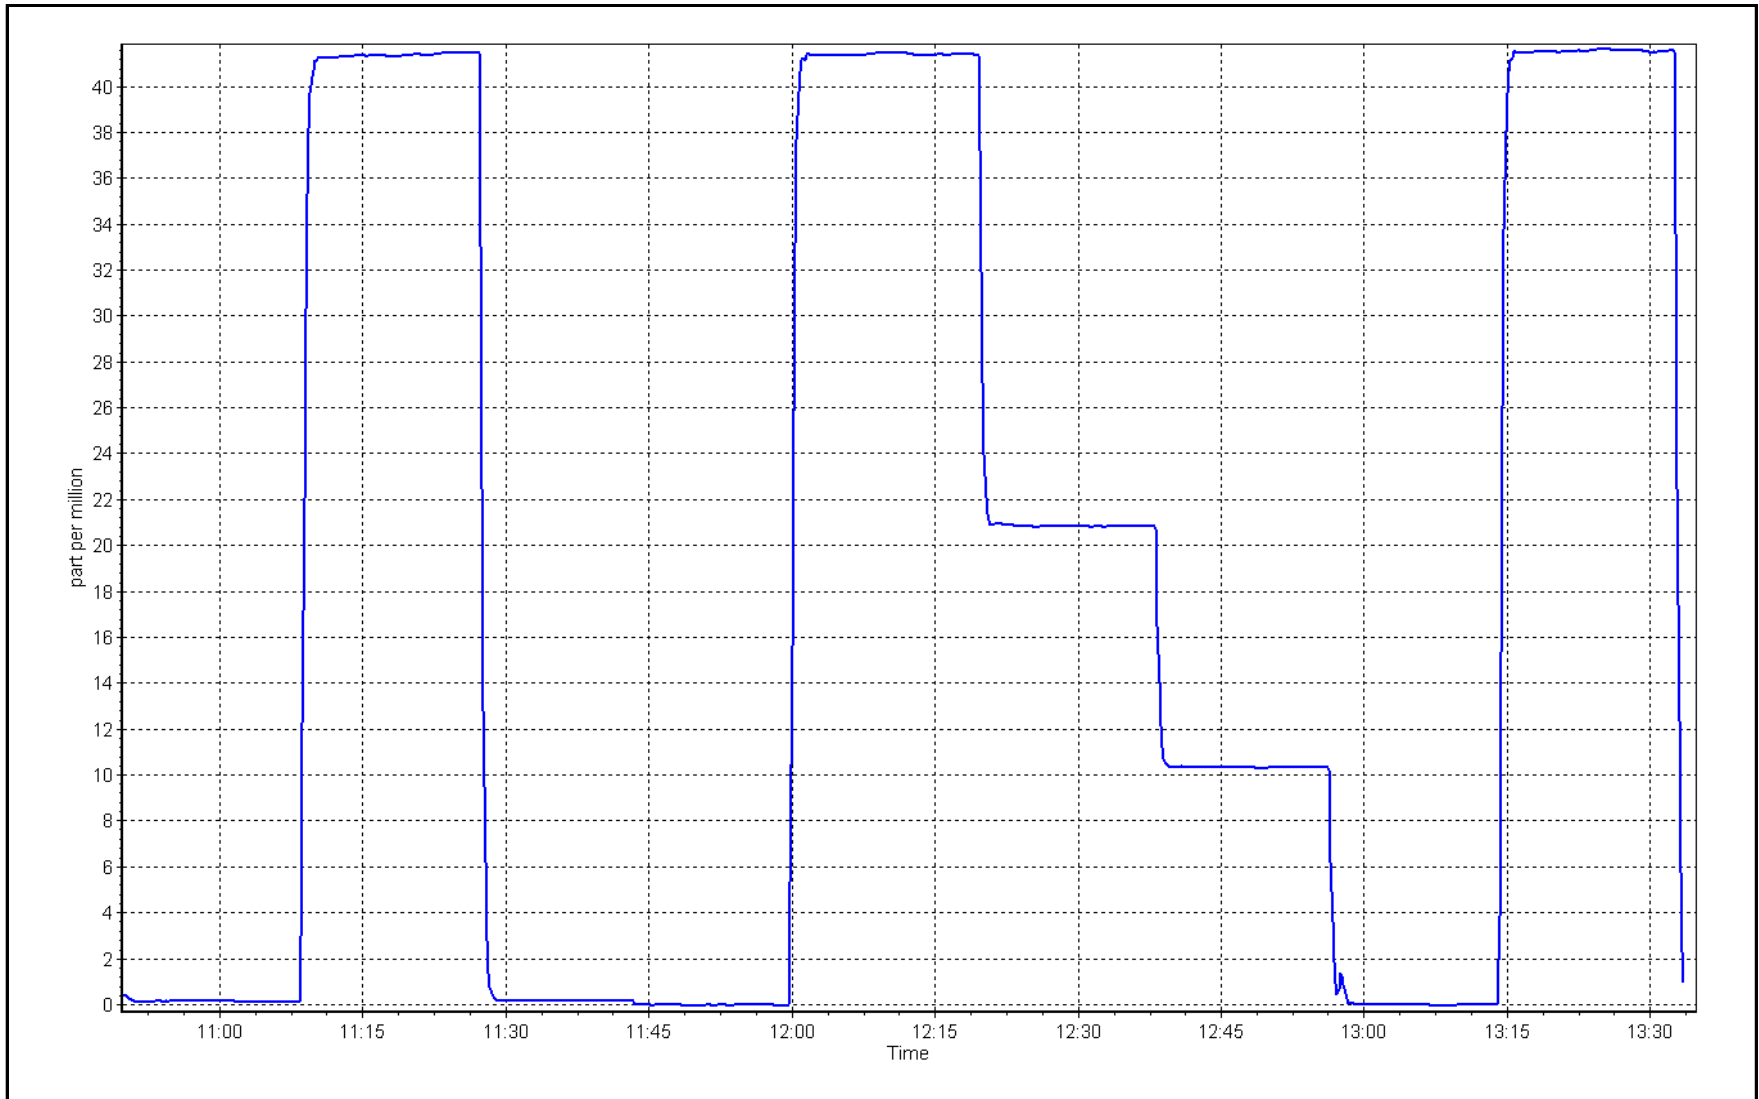



Wood Buffalo Environmental Association

CO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Stony Mountain	Station number:	AMS 18
Calibration Date:	January 12, 2023	Last Cal Date:	December 13, 2022
Start time (MST):	10:50	End time (MST):	13:52
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	60,220	ppm	Cal Gas Exp Date:	December 1, 2026
Cal Gas Cylinder #:	ALM063503			
Removed Cal Gas Conc:	60,220	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	2658
N2 Gen Make/Model:	Peak Scientific		Serial Number:	771048317

Analyzer Information

Analyzer make:	API T360	Analyzer serial #:	283
Analyzer Range	0 - 2,000 ppm		

	Start	Finish		Start	Finish
Calibration slope:	1.000503	1.000425	Backgd or Offset:	-0.045	-0.045
Calibration intercept:	2.940000	5.520000	Coeff or Slope:	1.051	1.051

CO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	3000	0.0	0.0	0.6	----
as found span	2930	80.0	1600.5	1602.5	0.999
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	3000	0.0	0.0	0.8	----
high point	2930	80.0	1600.5	1601.9	0.999
second point	2970	40.0	800.3	815.9	0.981
third point	2990	20.0	400.1	405.6	0.987
as left zero	3000	0.0	0.0	0.7	----
as left span	2930	80.0	1600.5	1606.2	0.996
Average Correction Factor					0.989

Baseline Corr As found:	1601.90	Prev response:	1604.28	*% change:	-0.1%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Sample inlet filter changed after as founds. No adjustments were made.

Calibration Performed By: Karan Pandit and Karina Fenwick



Wood Buffalo Environmental Association

CO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date	January 12, 2023	Previous Calibration	December 13, 2022
Station Name	Stony Mountain	Station Number	AMS 18
Start Time (MST)	10:50	End Time (MST)	13:52
Analyzer make	API T360	Analyzer serial #	283

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.8	----	Correlation Coefficient	0.999899	≥0.995
1600.5	1601.9	0.9991			
800.3	815.9	0.9808	Slope	1.000425	0.90 - 1.10
400.1	405.6	0.9865			
			Intercept	5.520000	+/-10

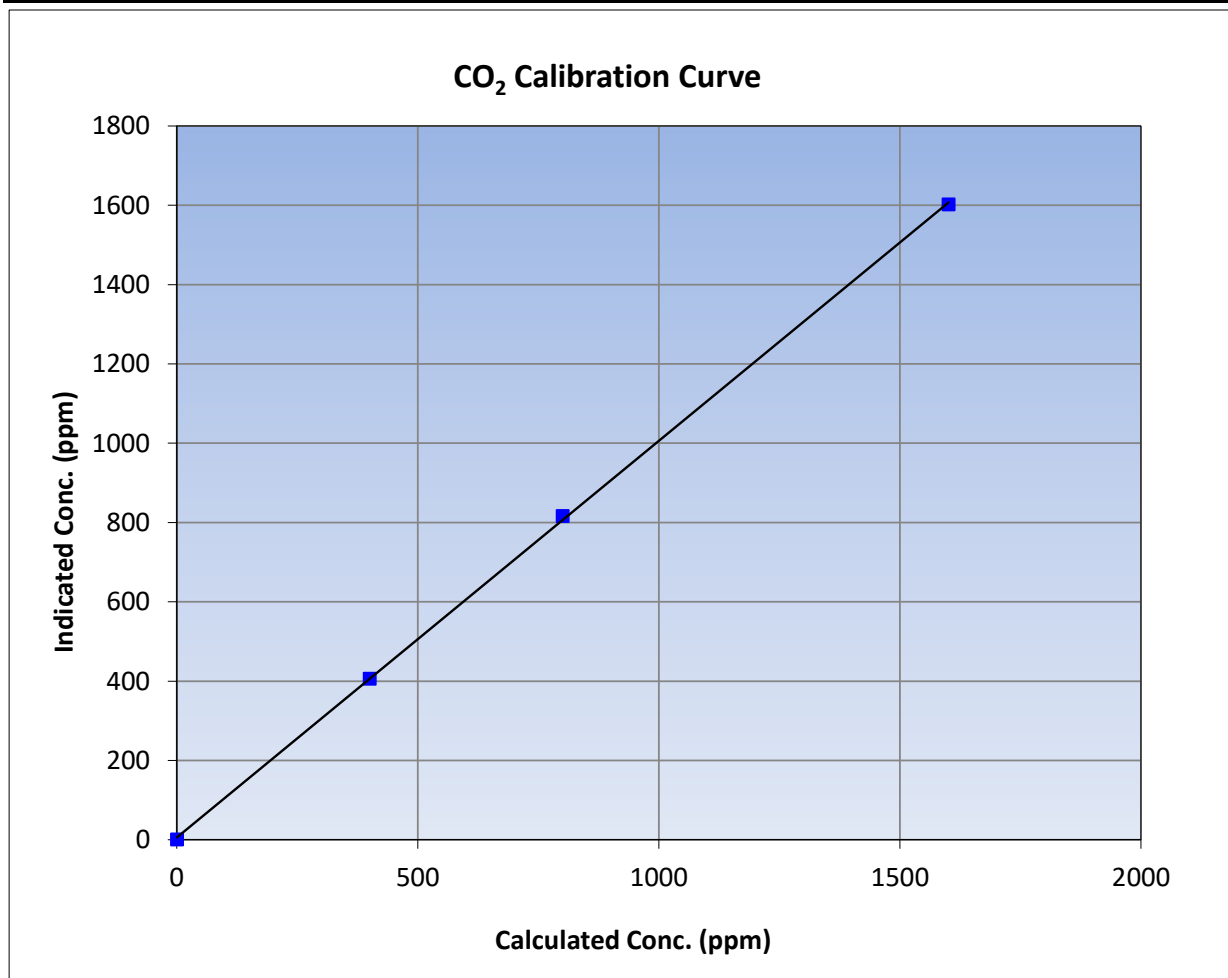

CO₂ Calibration Plot

Date: January 12, 2023

Location: Stony Mountain

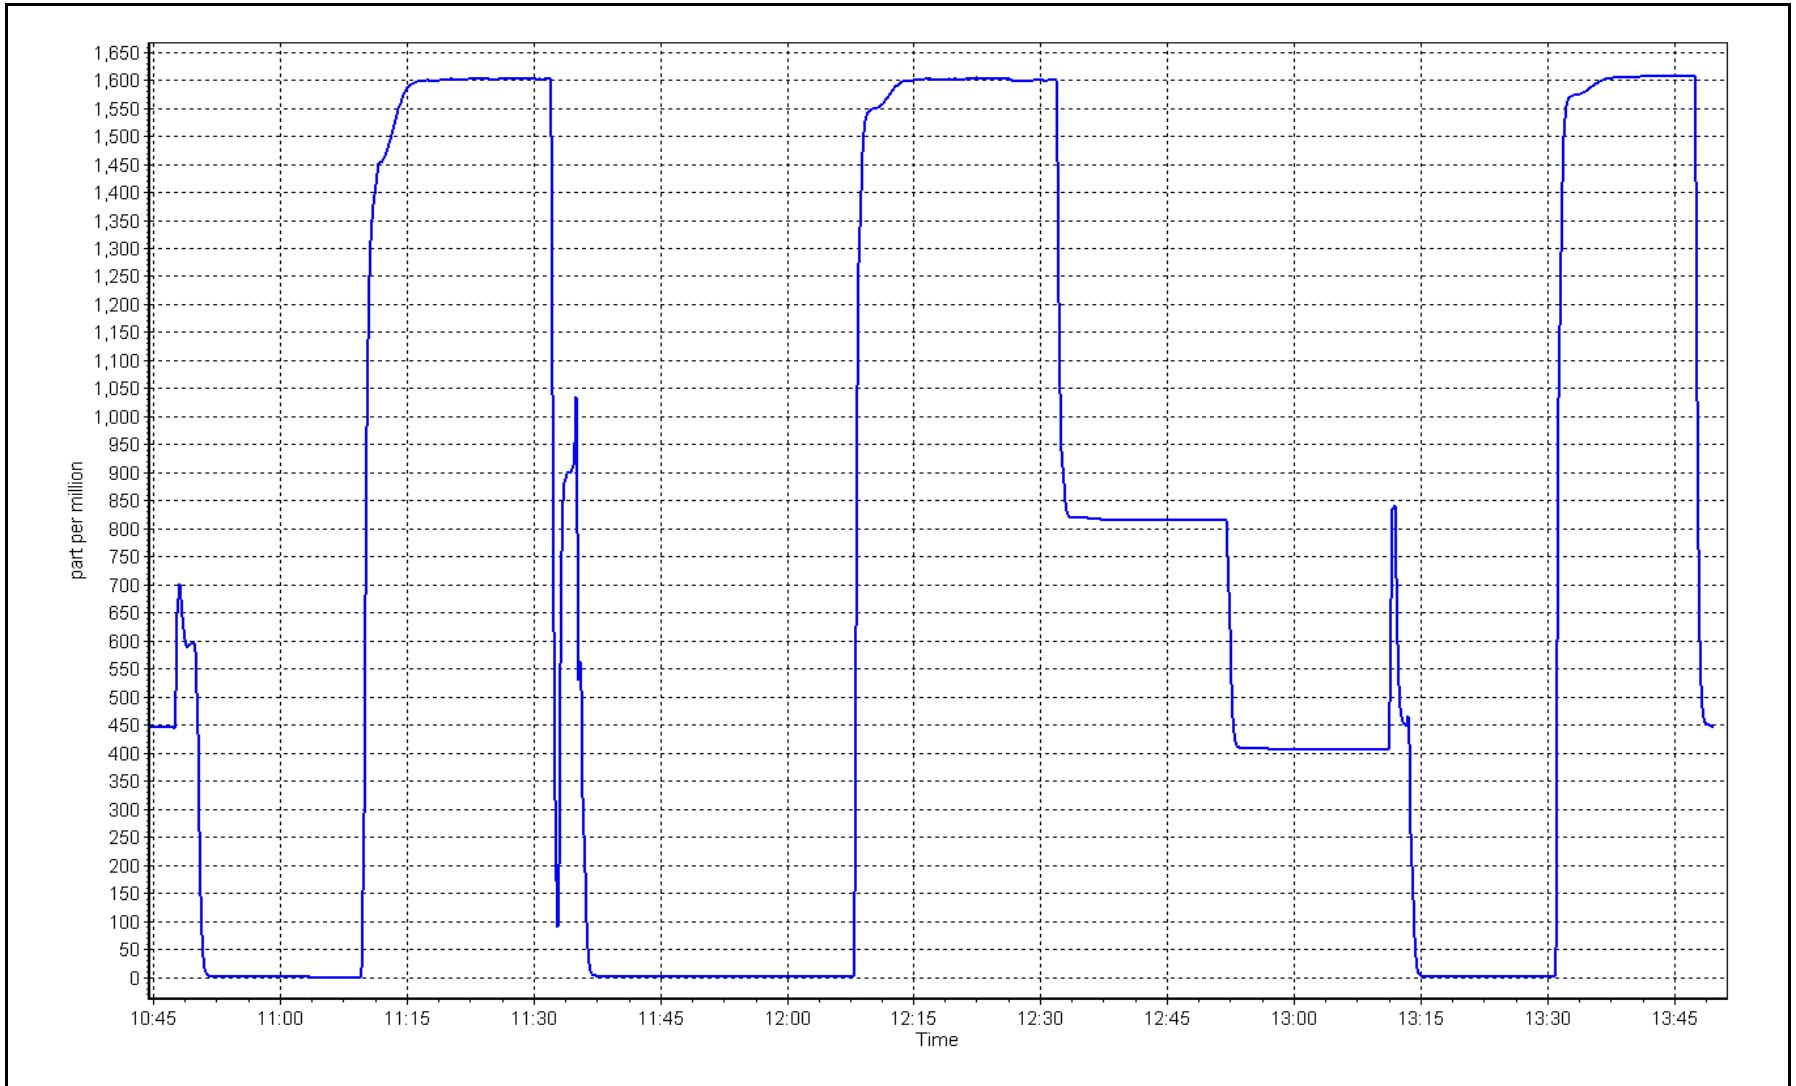



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS19 FIREBAG JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023





Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Firebag	Station number:	AMS 19
Calibration Date:	January 26, 2023	Last Cal Date:	December 5, 2022
Start time (MST):	11:22	End time (MST):	15:36
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.29	ppm	Cal Gas Exp Date:	February 23, 2025
Cal Gas Cylinder #:	CC716618			
Removed Cal Gas Conc:	49.29	ppm	Rem Gas Exp Date:	
Removed Gas Cyl #:			Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	1607
ZAG Make/Model:	API T701		Serial Number:	1118

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	1410661308
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.002165	0.997774	Backgd or Offset:	10.1	10.2
Calibration intercept:	-0.042557	-0.381080	Coeff or Slope:	0.987	0.987

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	4999	0.0	0.0	-0.5	----
as found span	4919	81.1	799.5	797.1	1.003
as found 2nd point	4959	40.6	400.3	399.3	1.002
as found 3rd point	4980	20.3	200.1	200.5	0.998
new cylinder response					
calibrator zero	4999	0.0	0.0	-0.2	----
high point	4919	81.1	799.5	797.7	1.002
second point	4959	40.6	400.3	398.0	1.006
third point	4980	20.3	200.1	199.7	1.002
as left zero	4999	0.0	0.0	-0.3	----
as left span	4919	81.1	799.5	802.0	0.997
Average Correction Factor					1.003

Baseline Corr As found:	797.60	Previous response	801.16	*% change	-0.4%
Baseline Corr 2nd AF pt:	399.80	AF Slope:	0.997147	AF Intercept:	0.138400
Baseline Corr 3rd AF pt:	201.00	AF Correlation:	0.999997		

* = > +/-5% change initiates investigation

Notes: No adjustments made. Swapped THC valve after MPAF's. Changed sample inlet filter after as founds.

Calibration Performed By: Braiden Boutilier



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	December 5, 2022
Station Name:	Firebag	Station Number:	AMS 19
Start Time (MST):	11:22	End Time (MST):	15:36
Analyzer make:	Thermo 43i	Analyzer serial #:	1410661308

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	-0.2	----	Correlation Coefficient	0.999996
799.5	797.7	1.0022		
400.3	398.0	1.0057	Slope	0.997774
200.1	199.7	1.0020		
			Intercept	-0.381080
				+/-30

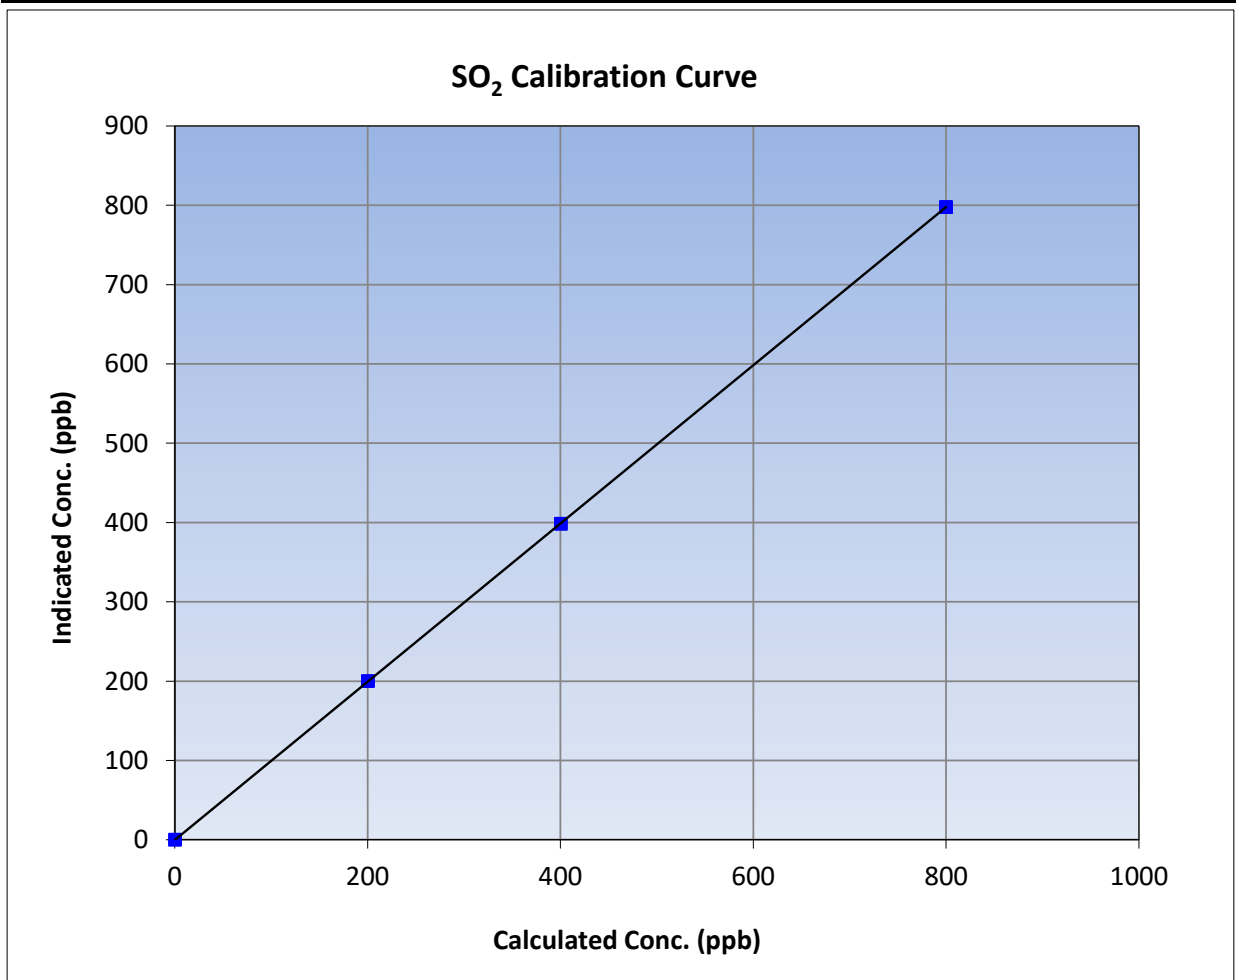

SO2 Calibration Plot

Date: January 26, 2023

Location: Firebag

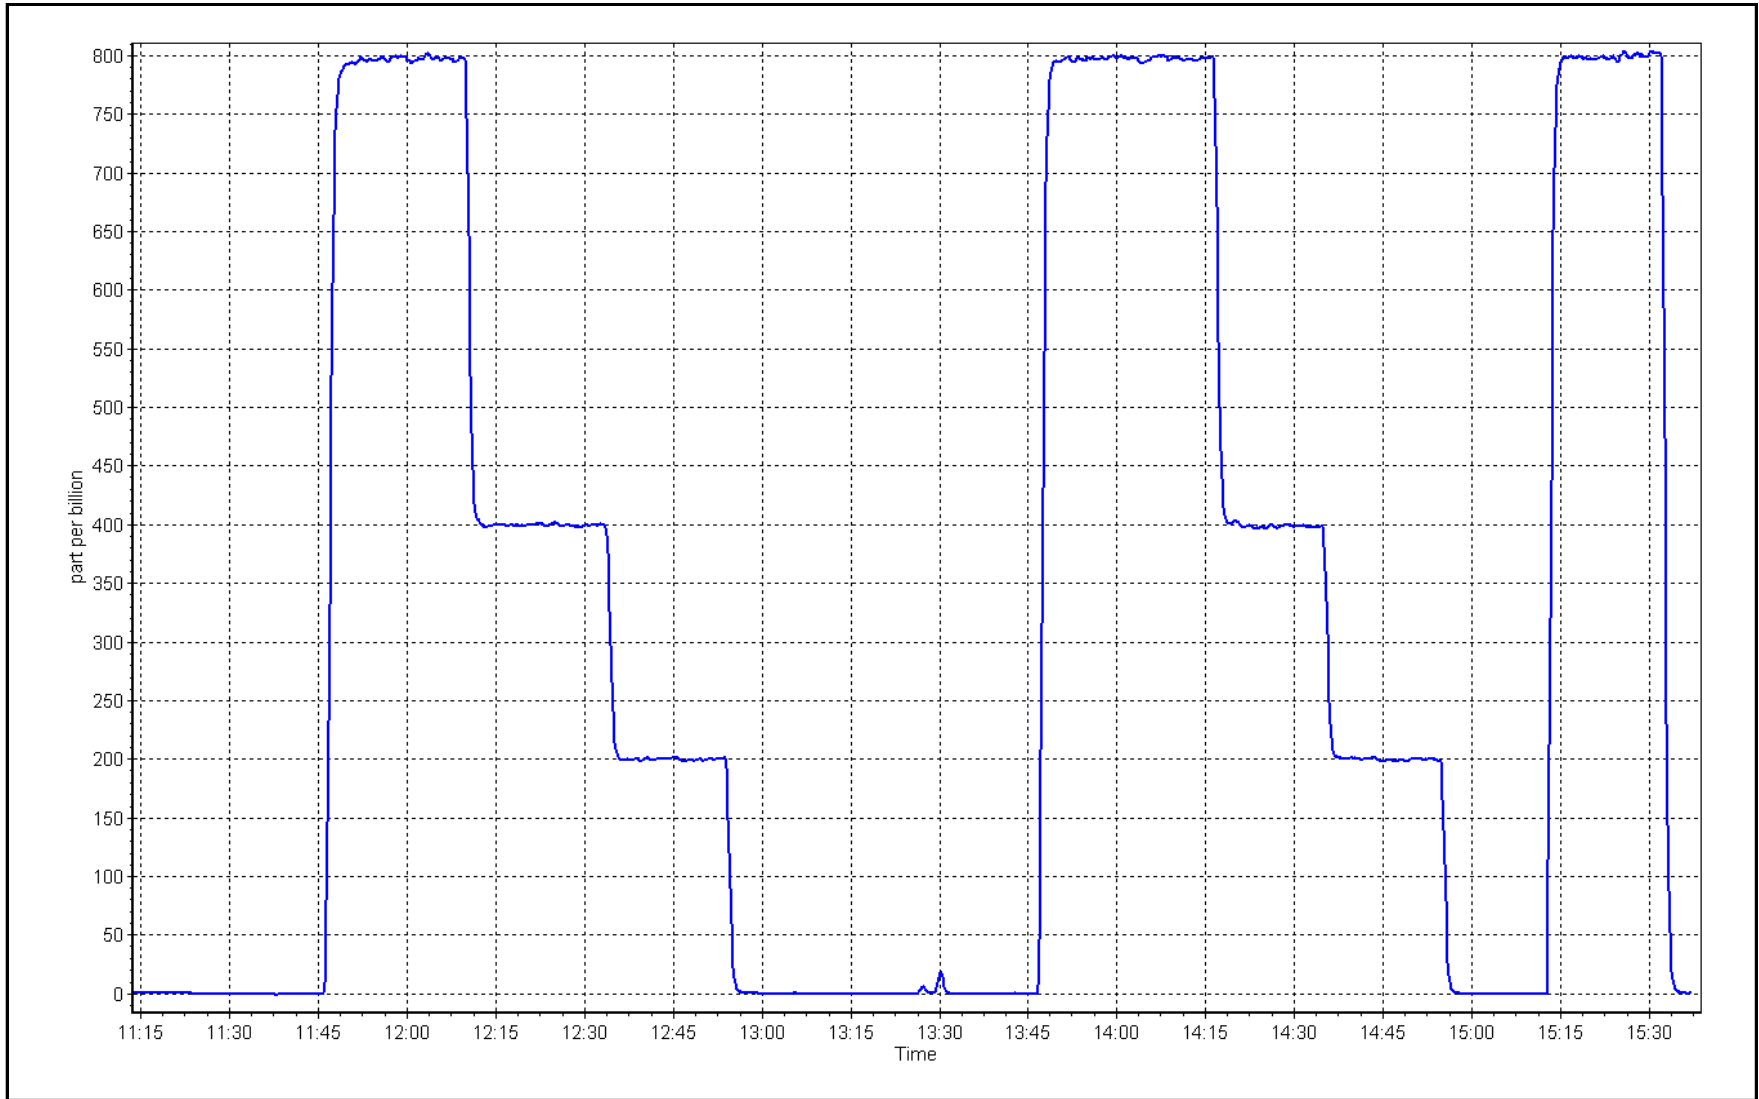



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Firebag Station number: AMS19
 Calibration Date: January 17, 2023 Last Cal Date: December 1, 2022
 Start time (MST): 10:31 End time (MST): 12:42
 Reason: Removal

Calibration Standards

Cal Gas Concentration: 5.114 ppm Cal Gas Exp Date: February 5, 2024
 Cal Gas Cylinder #: CC517427
 Removed Cal Gas Conc: 5.114 ppm Rem Gas Exp Date: n/a
 Removed Gas Cyl #: n/a Diff between cyl:
 Calibrator Make/Model: Teledyne API T700 Serial Number: 1607
 ZAG Make/Model: Teledyne API T701 Serial Number: 1118

Analyzer Information

Analyzer make: Thermo 450i Analyzer serial #: CM18360223
 Converter make: n/a Converter serial #: n/a
 Analyzer Range 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.991477		Backgd or Offset: 22.3	22.3
Calibration intercept:	-0.081394		Coeff or Slope: 0.980	0.980

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	1.4	----
as found span	4922	78.2	80.0	82.2	0.990
as found 2nd point	4961	39.1	40.0	41.4	1.000
as found 3rd point	4980	19.6	20.0	21.3	1.007
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero					
high point					
second point					
third point					
as left zero					
as left span					

SO₂ Scrubber Check

Date of last scrubber change:	December 9, 2021	Ave Corr Factor	
Date of last converter efficiency test:	n/a	efficiency	

Baseline Corr As found: 80.8 Prev response: 79.22 *% change: 2.0%
 Baseline Corr 2nd AF pt: 40.0 AF Slope: 1.011199 AF Intercept: 1.178264
 Baseline Corr 3rd AF pt: 19.9 AF Correlation: 0.999961

* = > +/-5% change initiates investigation


Notes: Removed 450i, replacing with a 43iTLE and external converter.

Calibration Performed By: Braiden Boutillier

H₂S Calibration Plot

Date: January 17, 2023

Location: Firebag

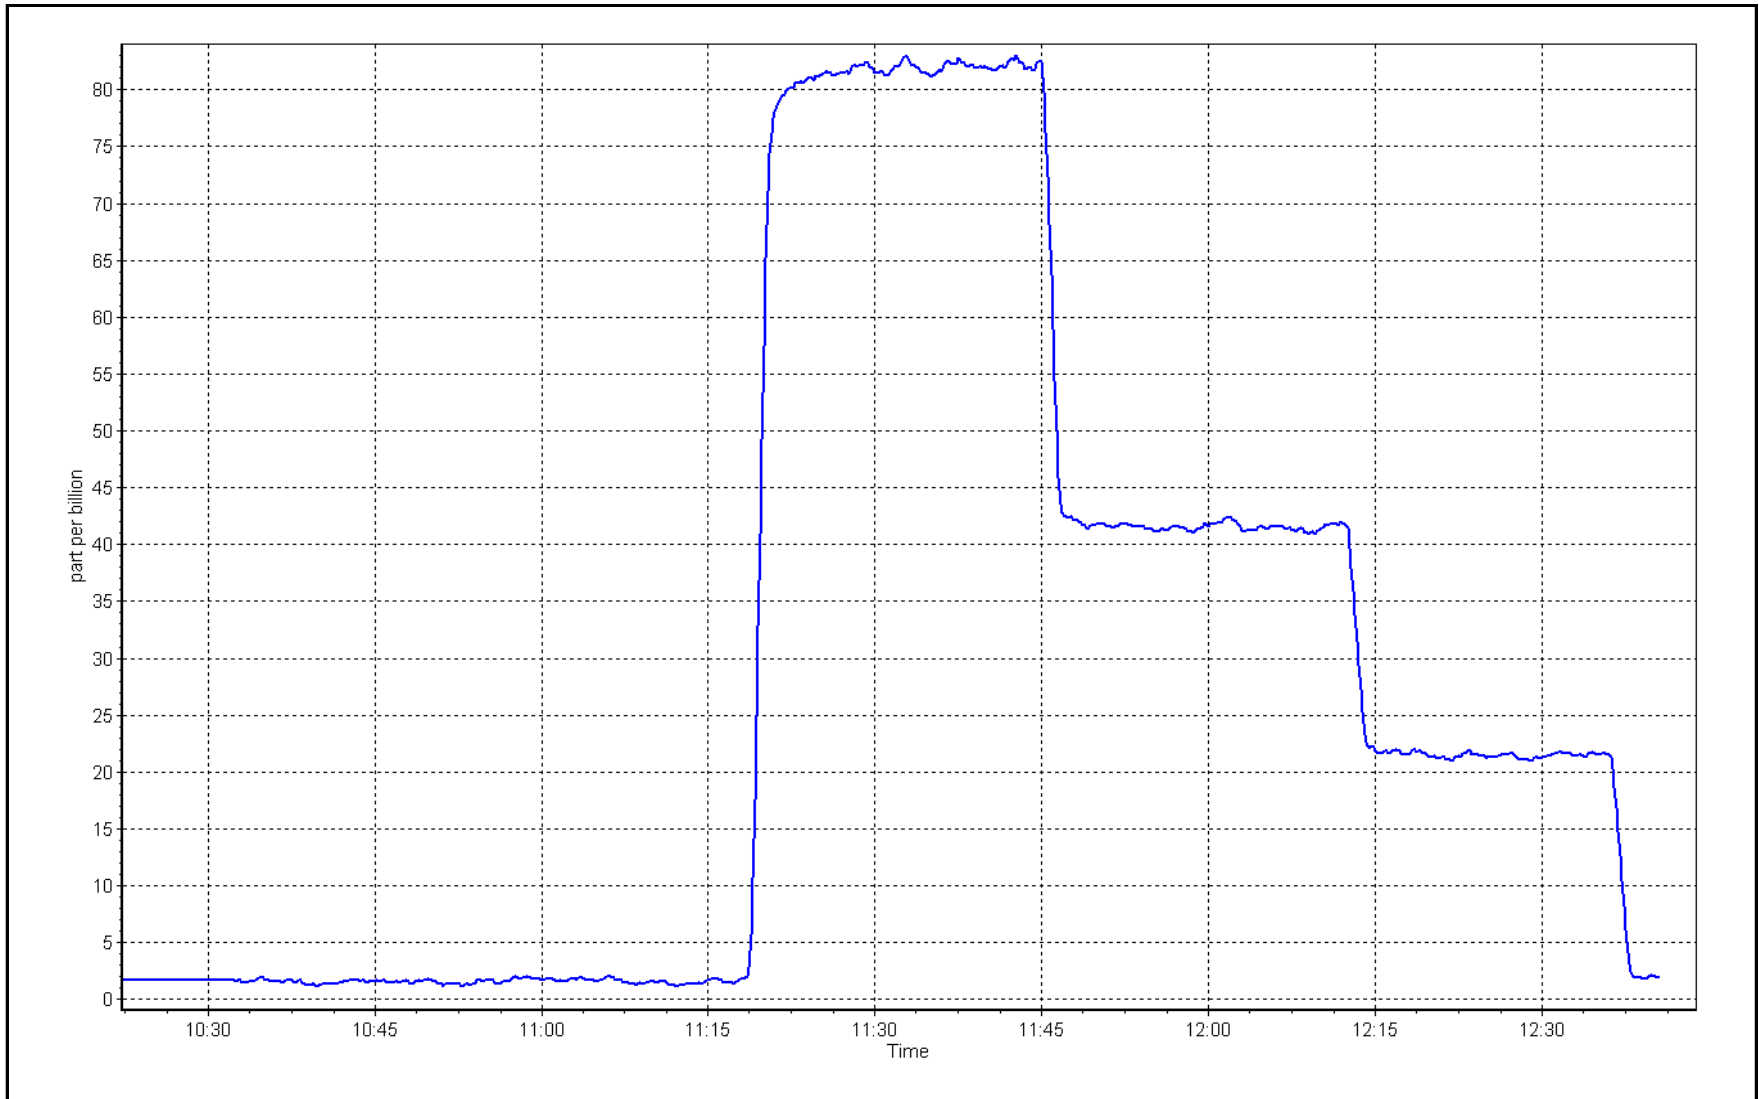



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name:	Firebag	Station number:	AMS19
Calibration Date:	January 18, 2023	Last Cal Date:	December 1, 2022
Start time (MST):	11:07	End time (MST):	14:56
Reason:	Install		

Calibration Standards

Cal Gas Concentration:	5.114	ppm	Cal Gas Exp Date:	February 5, 2024
Cal Gas Cylinder #:	CC517427			
Removed Cal Gas Conc:	5.114	ppm	Rem Gas Exp Date:	n/a
Removed Gas Cyl #:	n/a		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	1607
ZAG Make/Model:	Teledyne API T701		Serial Number:	1118

Analyzer Information

Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1336160090
Converter make:	Global	Converter serial #:	2022-222
Analyzer Range	0 - 100 ppb		

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:		0.998910	Backgd or Offset:	2.88
Calibration intercept:		0.058437	Coeff or Slope:	0.955

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero					
as found span					
as found 2nd point					
as found 3rd point					
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.0	----
high point	4922	78.2	80.0	79.9	1.001
second point	4961	39.1	40.0	40.1	0.997
third point	4980	19.6	20.0	20.1	0.997
as left zero	5000	0.0	0.0	0.1	----
as left span	4922	78.2	80.0	80.3	0.996
SO2 Scrubber Check	4922	78.3	800.2		----
Date of last scrubber change:	December 9, 2021			Ave Corr Factor	0.999
Date of last converter efficiency test:	n/a			efficiency	

Baseline Corr As found:	NA	Prev response:	NA	*% change:	NA
Baseline Corr 2nd AF pt:	NA	AF Slope:	NA	AF Intercept:	NA
Baseline Corr 3rd AF pt:	NA	AF Correlation:	NA		

* = > +/-5% change initiates investigation

Notes: Installed 43i-TLE. Adjusted the zero and span.

Calibration Performed By: Braiden Boutillier



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 18, 2023	Previous Calibration:	December 1, 2022
Station Name:	Firebag	Station Number:	AMS19
Start Time (MST):	11:07	End Time (MST):	14:56
Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1336160090

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	0.999996	≥0.995
80.0	79.9	1.0010			
40.0	40.1	0.9973	Slope	0.998910	0.90 - 1.10
20.0	20.1	0.9974			
			Intercept	0.058437	+/-3

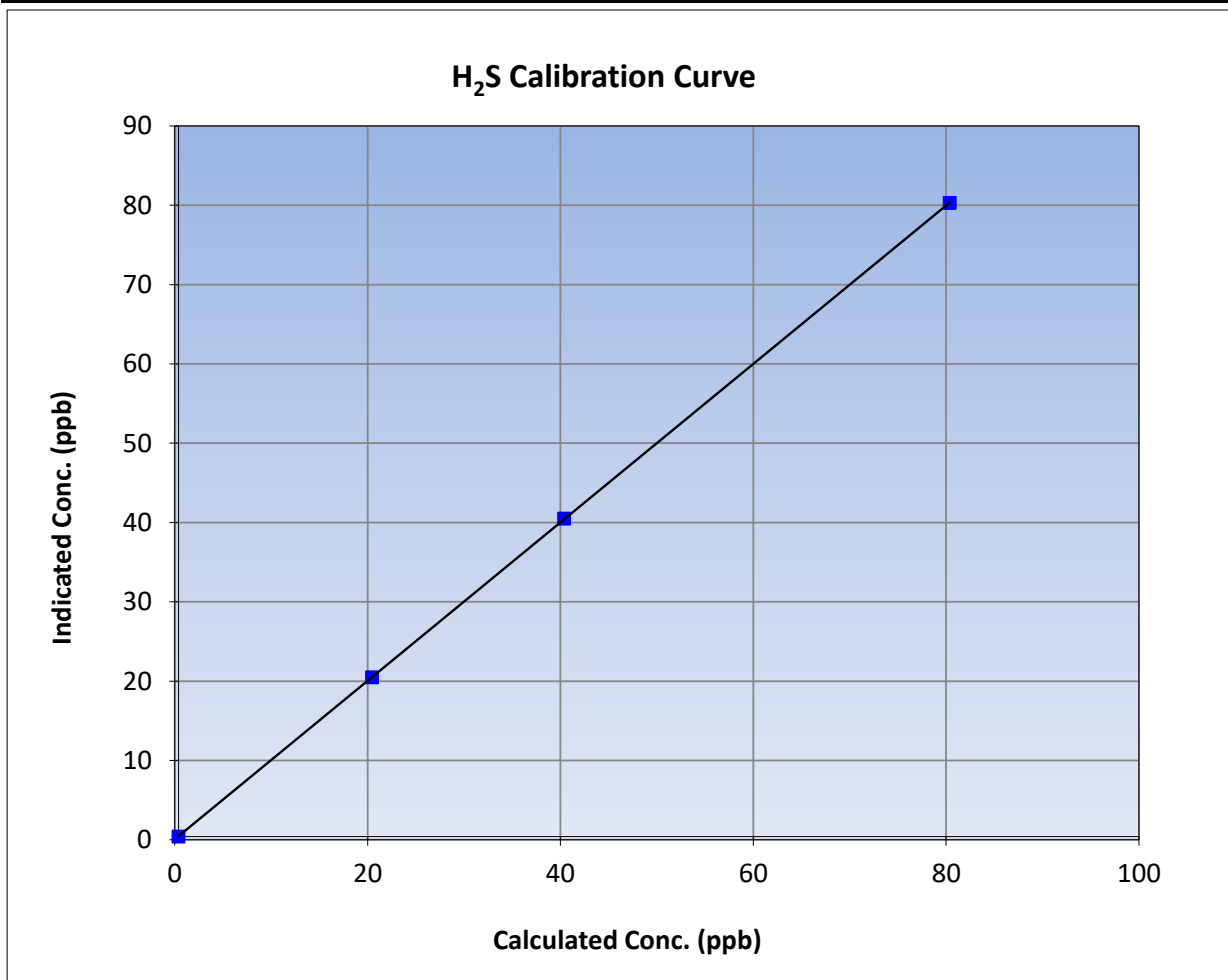

H₂S Calibration Plot

Date: January 18, 2023

Location: Firebag

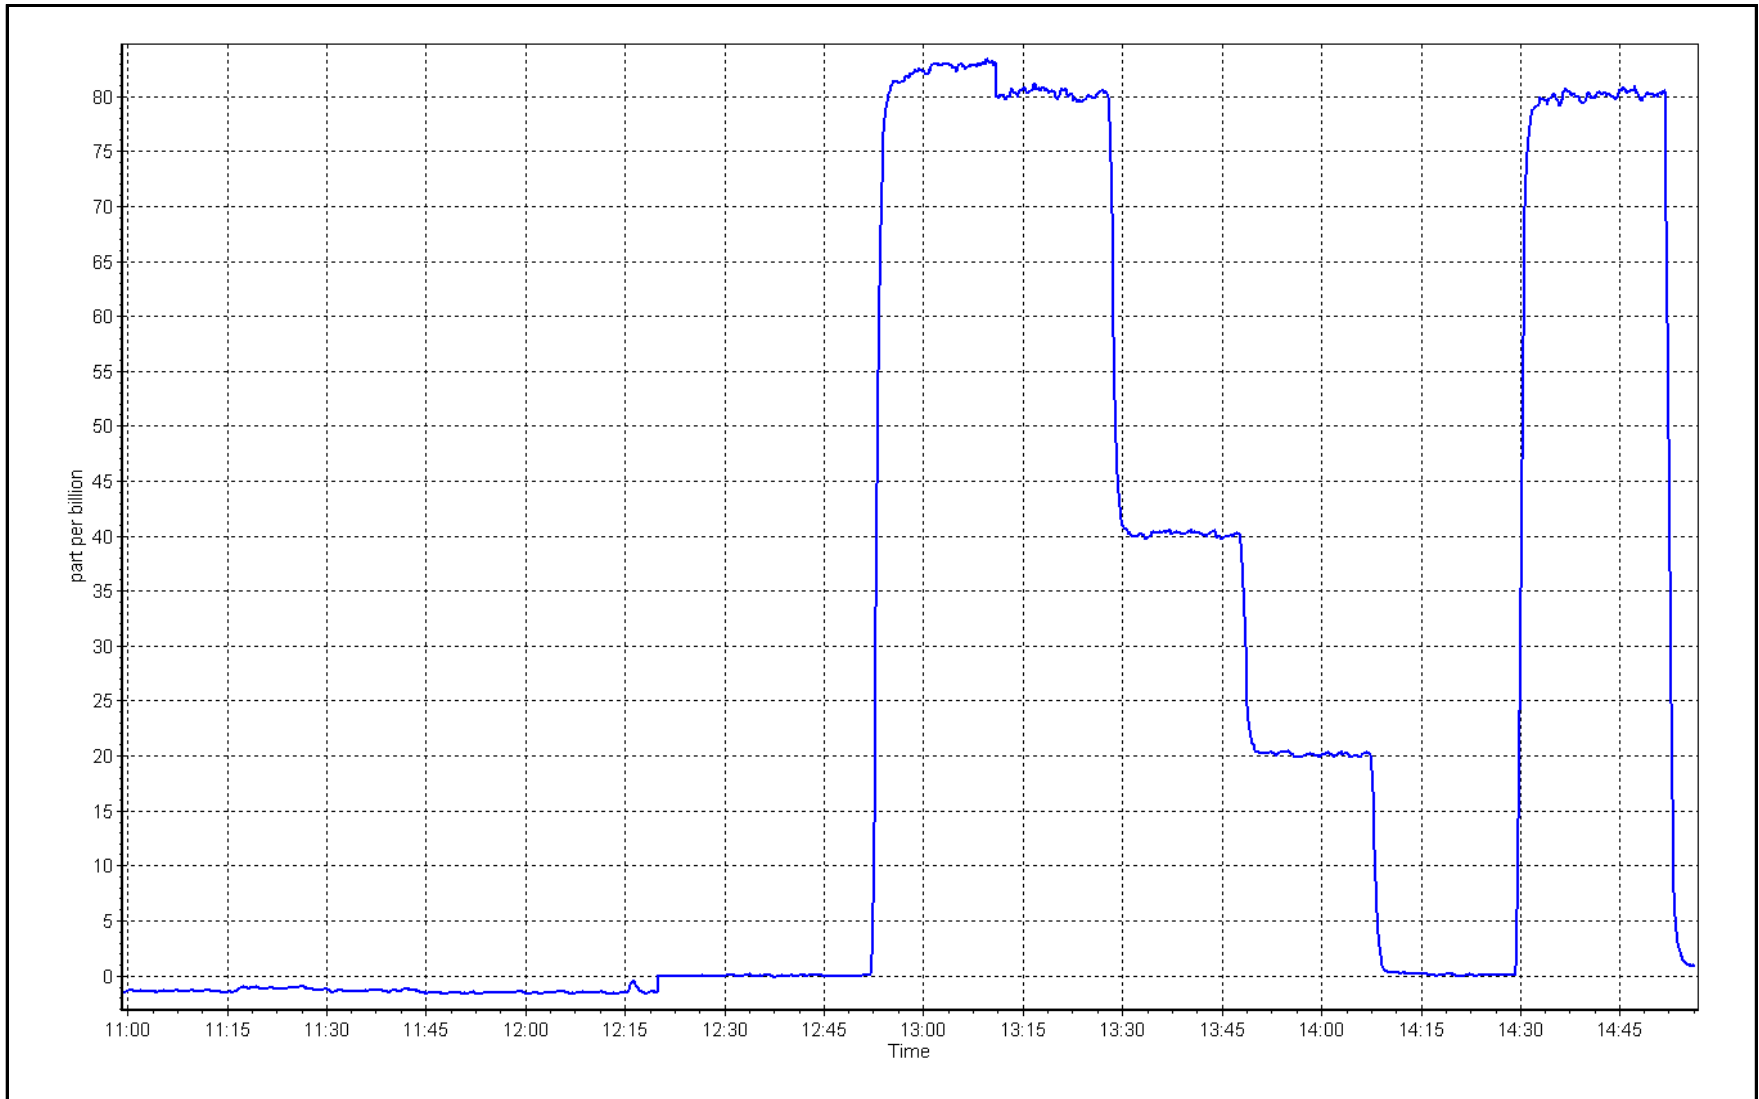



Wood Buffalo Environmental Association

THC Calibration Report

Version-01-2020

Station Information

Station Name: Firebag Station number: AMS 19
 Calibration Date: January 26, 2023 Last Cal Date: December 21, 2022
 Start time (MST): 11:22 End time (MST): 15:36
 Reason: Routine

Calibration Standards

Gas Cert Reference: CC716618 Cal Gas Expiry Date: February 23, 2025
 CH4 Cal Gas Conc. 500.7 ppm CH4 Equiv Conc. 1066.9 ppm
 C3H8 Cal Gas Conc. 205.9 ppm
 Removed Gas Cert: Removed Gas Expiry:
 Removed CH4 Conc. 500.7 ppm CH4 Equiv Conc. 1066.9 ppm
 Removed C3H8 Conc. 205.9 ppm Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 1607
 ZAG Make/Model: API T701 Serial Number: 1118

Analyzer Information

Analyzer make: Thermo 51i-LT Analyzer serial #: 1336160089
 Analyzer Range: 0 - 20 ppm

Calibration slope:	<u>Start</u>	<u>Finish</u>	Background:	<u>Start</u>	<u>Finish</u>
Calibration intercept:	0.998886	1.001270	Coefficient:	2.24	2.25
	-0.003747	-0.051562		3.754	3.774

THC Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated Concentration (ppm) (Cc)	Indicated Concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.00	-0.06	----
as found span	4919	81.1	17.31	17.18	1.007
as found 2nd point	4959	40.6	8.66	8.49	1.021
as found 3rd point	4980	20.3	4.33	4.14	1.048
new cylinder response					
calibrator zero	4999	0.0	0.00	-0.03	----
high point	4919	81.1	17.31	17.29	1.001
second point	4959	40.6	8.66	8.60	1.007
third point	4980	20.3	4.33	4.28	1.013
as left zero	5000	0.0	0.00	-0.06	----
as left span	4919	81.1	17.31	17.31	1.000
Average Correction Factor					1.007
Baseline Corr As found:	17.24	Previous response	17.28	*% change	-0.2%
Baseline Corr 2nd AF pt:	8.55	AF Slope:	0.998210	AF Intercept:	-0.126132
Baseline Corr 3rd AF pt:	4.20	AF Correlation:	0.999939		

* = > +/-5% change initiates investigation

Notes: Adjusted span. Changed zero/span valve after MPAF's. Changed sample inlet filter after as founds.

Calibration Performed By: Braiden Boutillier



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	December 21, 2022
Station Name:	Firebag	Station Number:	AMS 19
Start Time (MST):	11:22	End Time (MST):	15:36
Analyzer make:	Thermo 51i-LT	Analyzer serial #:	1336160089

Calibration Data


Calculated Concentration (ppm) (Cc)	Indicated Concentration (ppm) (lc)	Correction factor (Cc/lc)	Statistical Evaluation	<u>Limits</u>	
0.00	-0.03	----	Correlation Coefficient	0.999992	≥0.995
17.31	17.29	1.0009			
8.66	8.60	1.0075	Slope	1.001270	0.90 - 1.10
4.33	4.28	1.0132			
			Intercept	-0.051562	+/-1.5

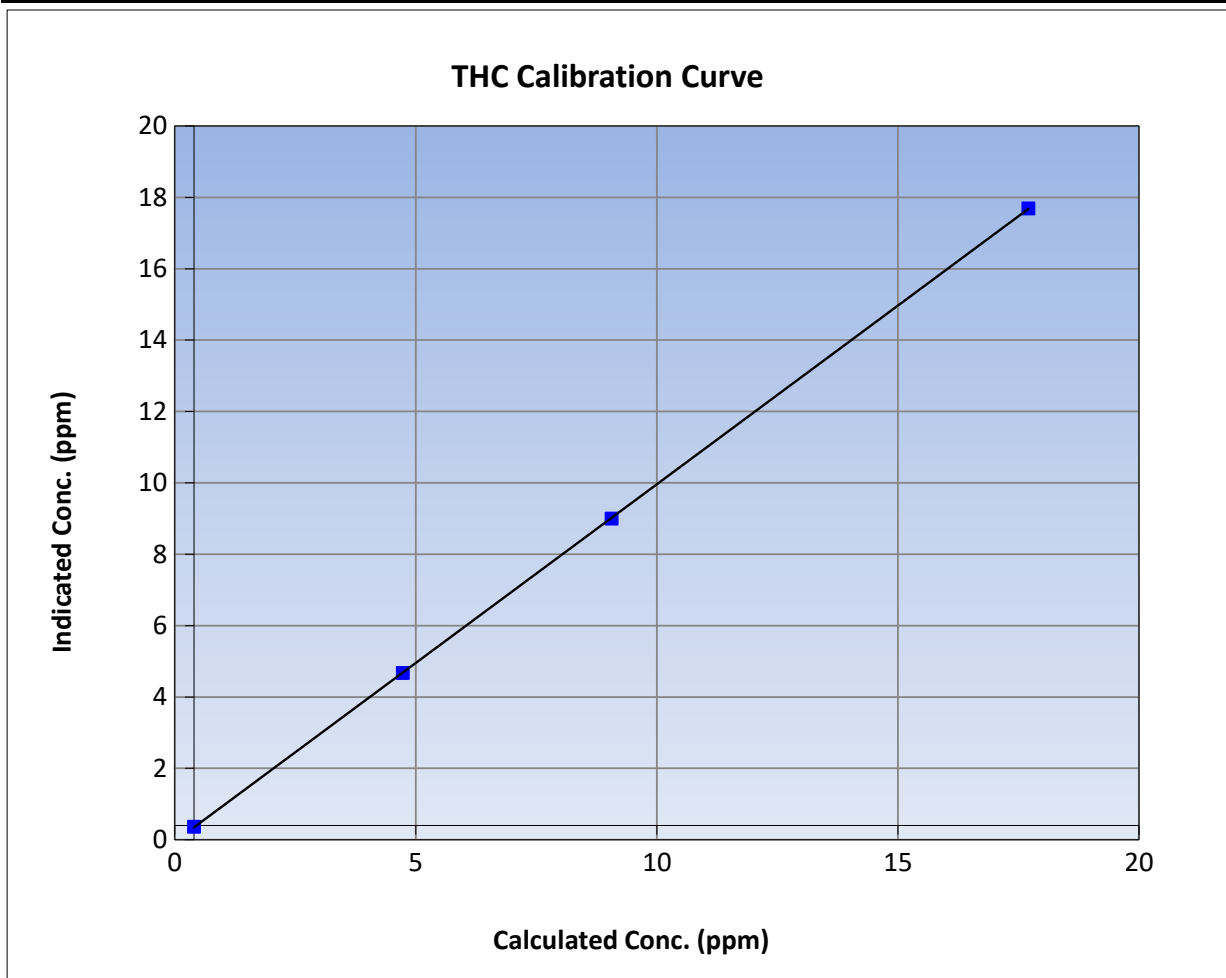

THC Calibration Plot

Date: January 26, 2023

Location: Firebag

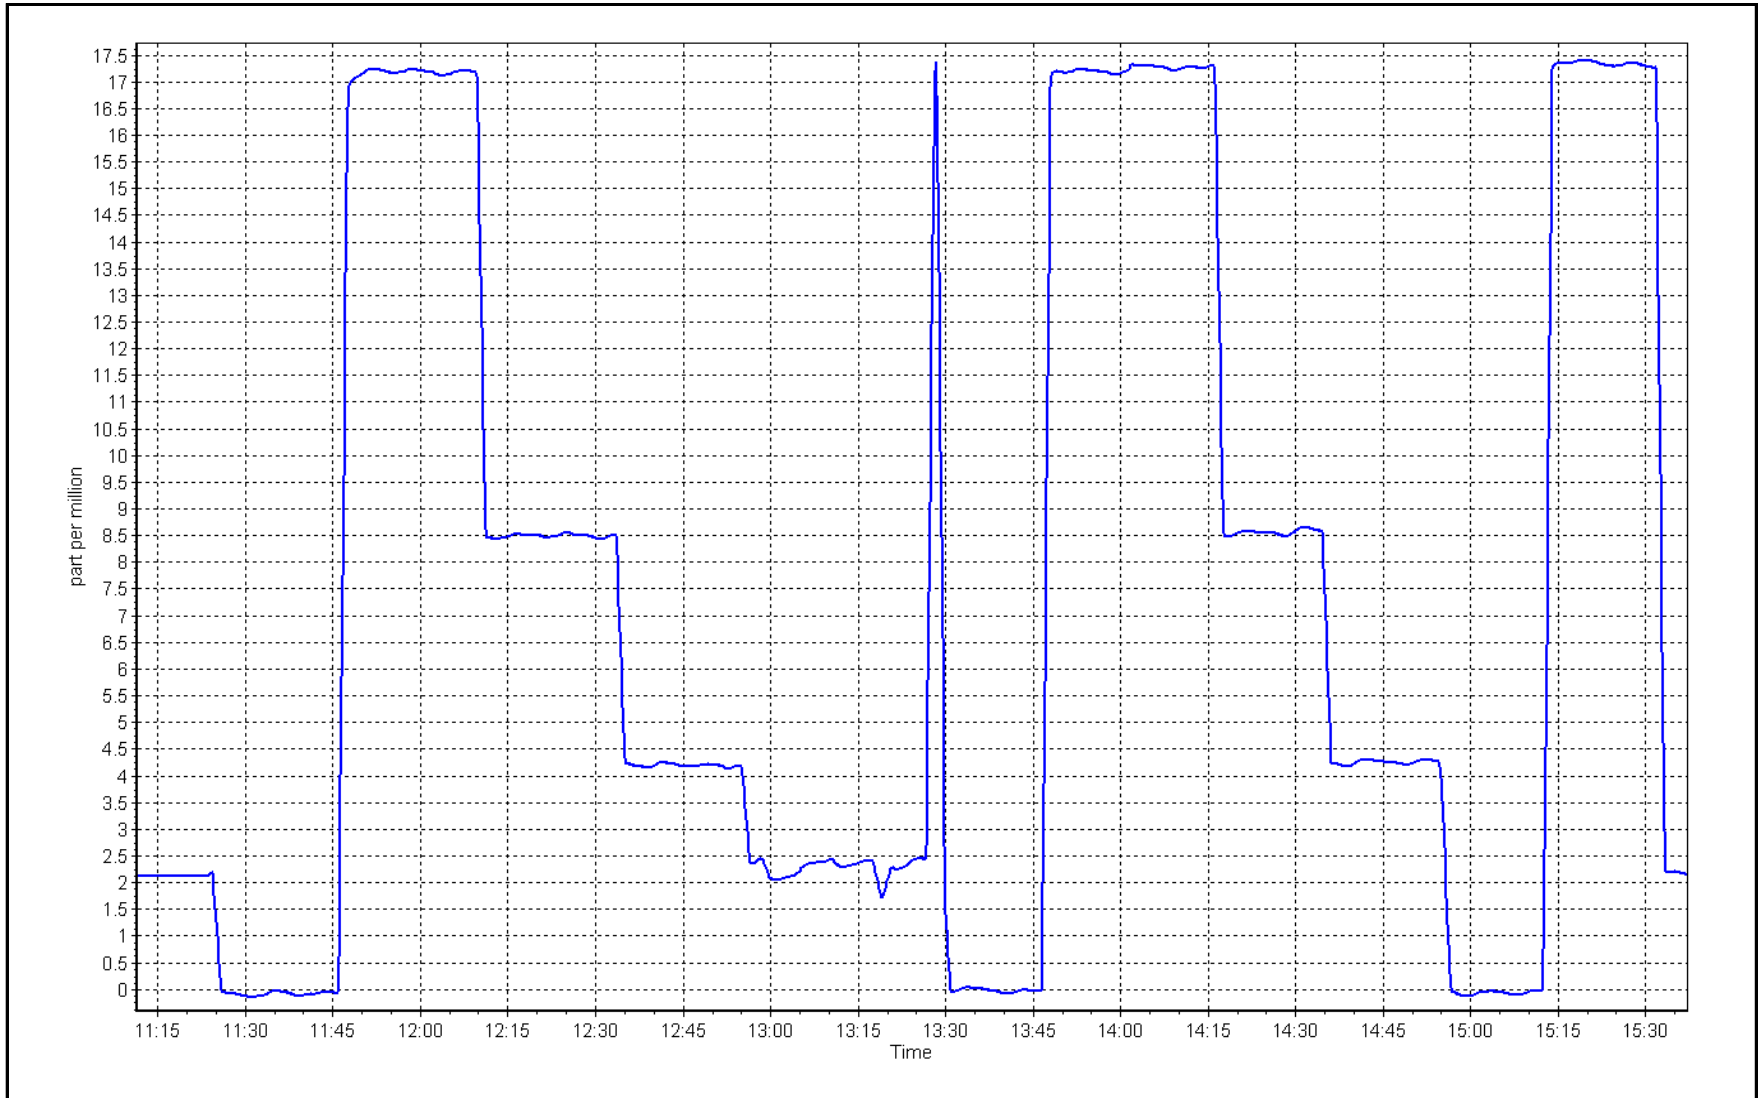



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Firebag
Calibration Date: January 19, 2023
Start time (MST): 10:45
Reason: Routine
Station number: AMS 19
Last Cal Date: December 1, 2022
End time (MST): 15:05

Calibration Standards

NO Gas Cylinder #: T2Y1K63
NOX Cal Gas Conc: 51.12 ppm
Removed Cylinder #: n/a
Removed Gas NOX Conc: 51.12 ppm
NOX gas Diff:
Calibrator Model: Teledyne API T700
ZAG make/model: Teledyne API T701
Cal Gas Expiry Date: November 30, 2023
NO Cal Gas Conc: 49.40 ppm
Removed Gas Exp Date: n/a
Removed Gas NO Conc: 49.40 ppm
NO gas Diff:
Serial Number: 1607
Serial Number: 1118

Analyzer Information

Analyzer make: Thermo 42i
NOX Range (ppb): 0 - 1000 ppb
Analyzer serial #: 1410661309

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.041	1.041	NO bkgnd or offset:	7.2	7.2
NOX coeff or slope:	0.996	0.996	NOX bkgnd or offset:	7.3	7.3
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	209.4	207.8

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	0.997409	0.990896
NO _x Cal Offset:	0.215620	0.574492
NO Cal Slope:	0.999812	0.991188
NO Cal Offset:	-0.371292	0.047030
NO ₂ Cal Slope:	0.999908	1.003489
NO ₂ Cal Offset:	-0.728179	-1.311603



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	4999	0.0	0.0	0.0	0.0	0.0	-0.2	0.2	----	----
as found span	4919	81.0	828.1	800.3	27.9	824.0	791.2	32.5	1.0050	1.0115
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	4999	0.0	0.0	0.0	0.0	0.0	-0.1	0.1	----	----
high point	4919	81.0	828.1	800.3	27.9	821.0	793.2	27.8	1.0087	1.0089
second point	4960	40.5	414.0	400.1	13.9	410.8	396.7	14.1	1.0079	1.0086
third point	4980	20.2	206.5	199.6	6.9	206.0	198.0	8.0	1.0025	1.0079
as left zero	4999	0.0	0.0	0.0	0.0	0.0	-0.1	0.1	----	----
as left span	4919	81.0	828.1	363.9	464.3	815.0	350.6	464.5	1.0161	1.0379
Average Correction Factor									1.0064	1.0085

Corrected As found	NO _x = 824.0 ppb	NO = 791.4 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -0.3%	
Previous Response	NO _x = 826.2 ppb	NO = 799.8 ppb		*Percent Change	NO = -1.1%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	788.8	352.4	464.3	465.1	0.9982	100.2%
2nd GPT point (200 ppb O3)	788.8	571.1	245.6	245.3	1.0011	99.9%
3rd GPT point (100 ppb O3)	788.8	679.6	137.1	134.1	1.0221	97.8%
Average Correction Factor					1.0071	99.3%

Notes:

No adjustments made. Changed sample inlet filter after as founds.

Calibration Performed By:

Braiden Boutilier



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 1, 2022
Station Name:	Firebag	Station Number:	AMS 19
Start Time (MST):	10:45	End Time (MST):	15:05
Analyzer make:	Thermo 42i	Analyzer serial #:	1410661309

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.0	----	Correlation Coefficient	≥0.995	
828.1	821.0	1.0087			
414.0	410.8	1.0079			
206.5	206.0	1.0025			
			Slope	0.990896	0.90 - 1.10
			Intercept	0.574492	+/-20

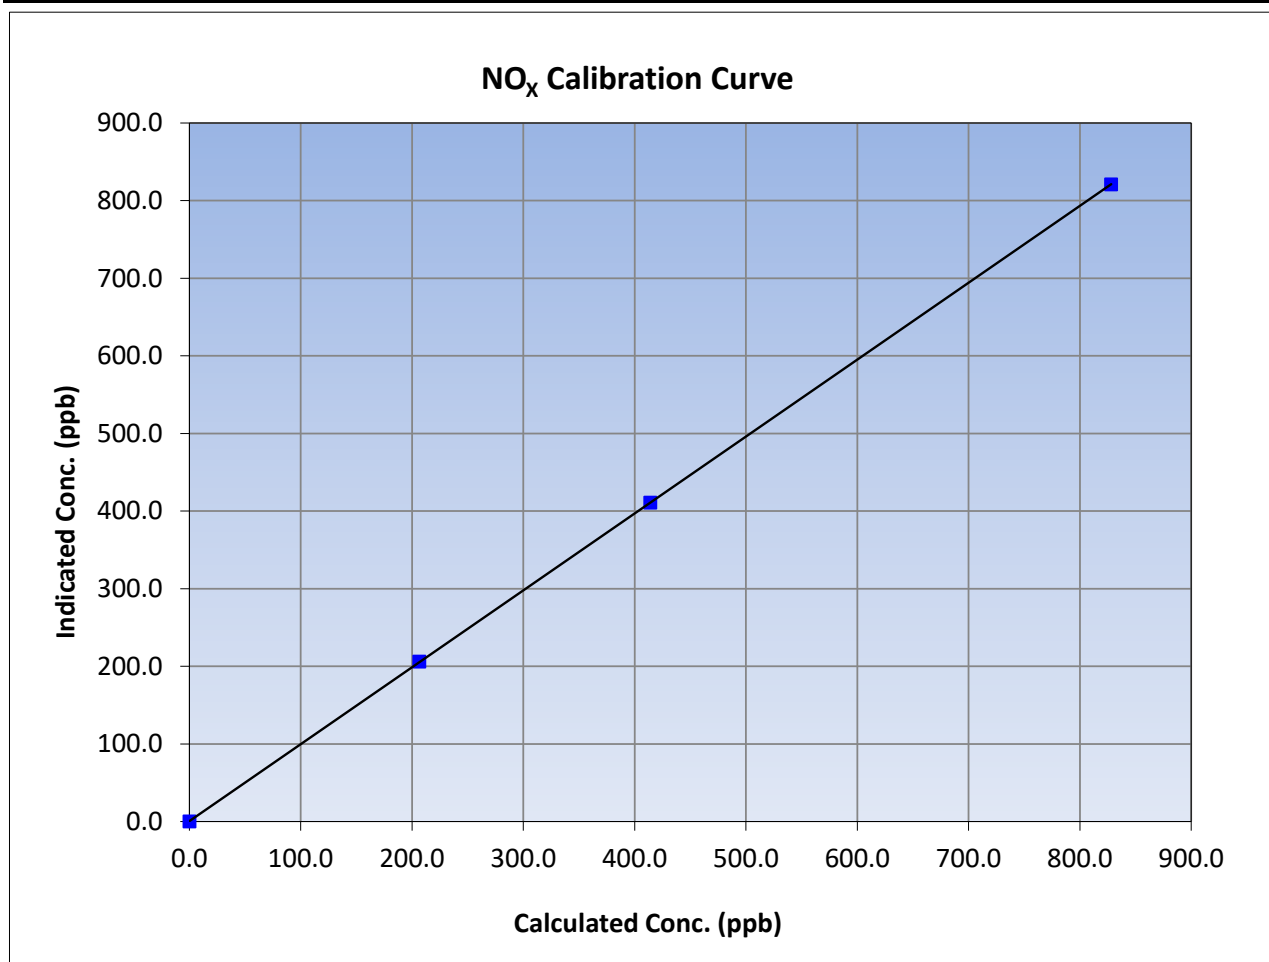



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 1, 2022
Station Name:	Firebag	Station Number:	AMS 19
Start Time (MST):	10:45	End Time (MST):	15:05
Analyzer make:	Thermo 42i	Analyzer serial #:	1410661309

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	-0.1	----	Correlation Coefficient	≥0.995	
800.3	793.2	1.0089			
400.1	396.7	1.0086			
199.6	198.0	1.0079			
			Slope	0.991188	0.90 - 1.10
			Intercept	0.047030	+/-20

NO Calibration Curve

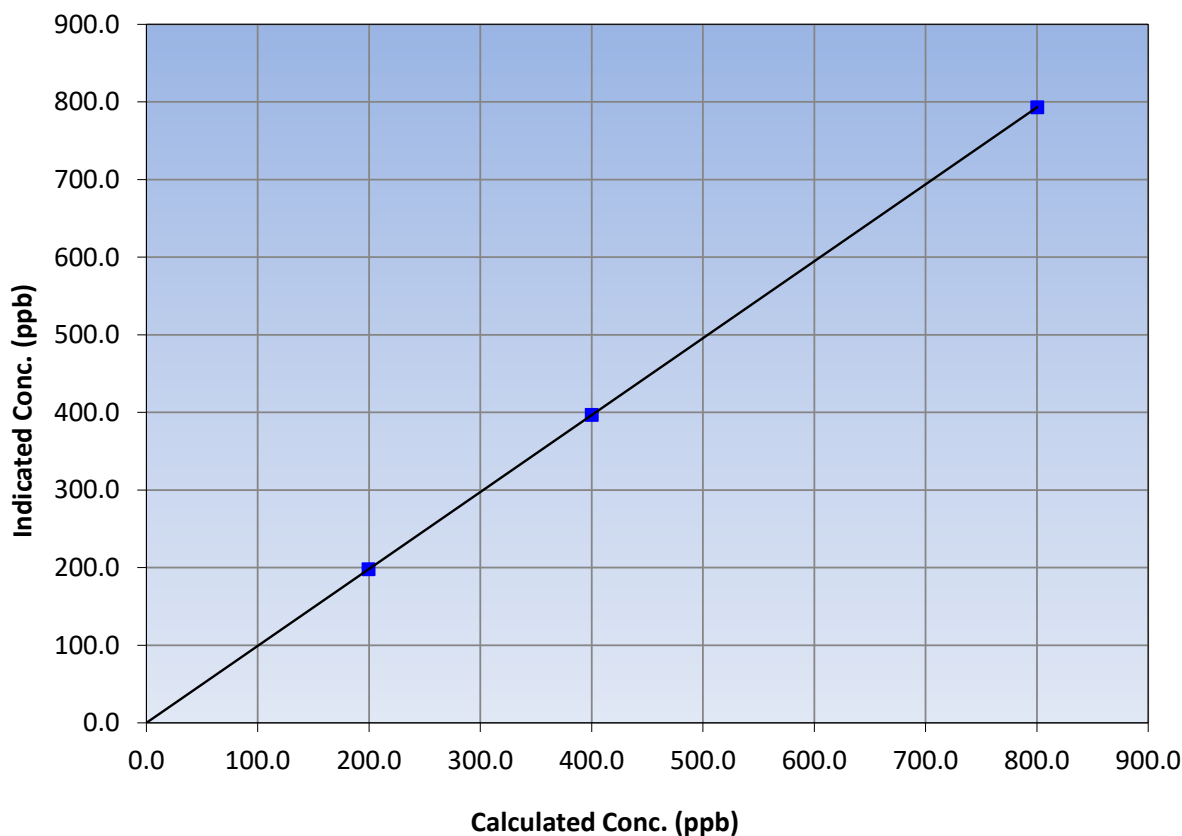



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 1, 2022
Station Name:	Firebag	Station Number:	AMS 19
Start Time (MST):	10:45	End Time (MST):	15:05
Analyzer make:	Thermo 42i	Analyzer serial #:	1410661309

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>
0.0	0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
464.3	465.1	0.9982		
245.6	245.3	1.0011		
137.1	134.1	1.0221		
			0.999941	
			1.003489	
			-1.311603	


NO₂ Calibration Curve

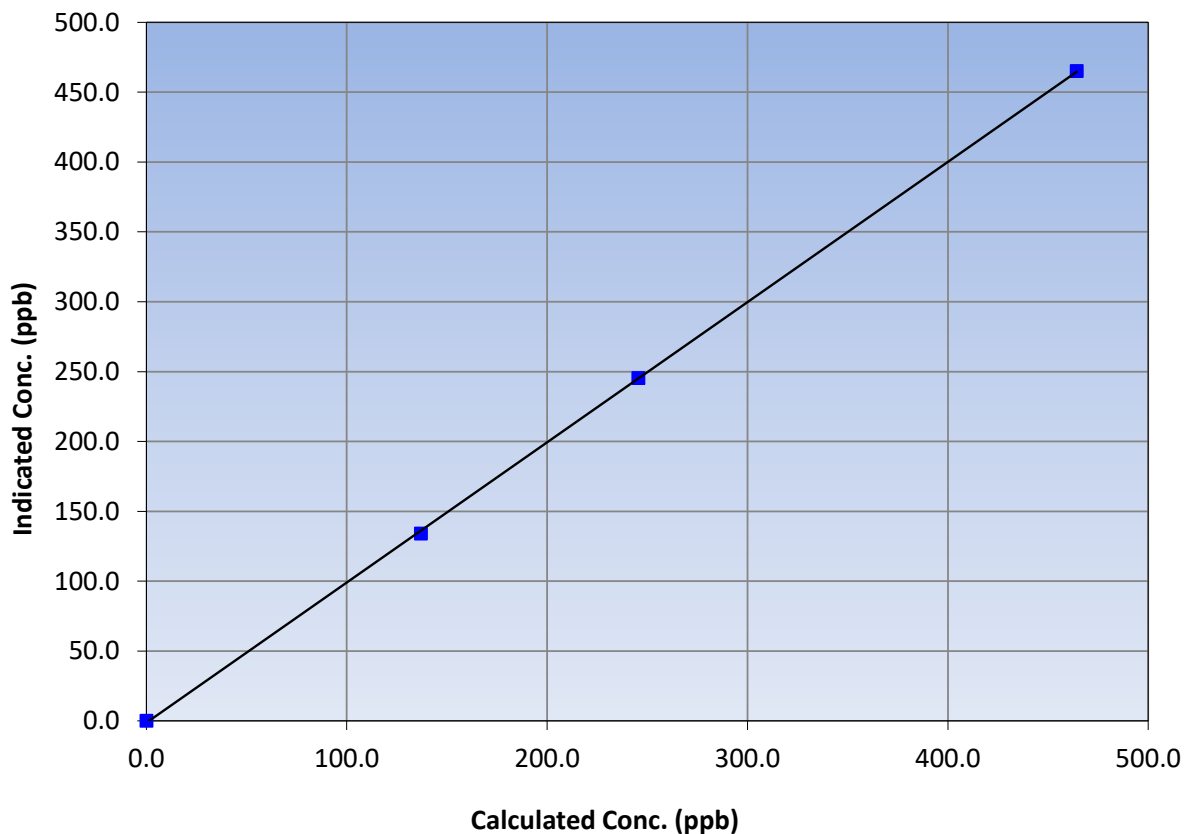

NO_x Calibration Plot

Date: January 19, 2023

Location: Firebag

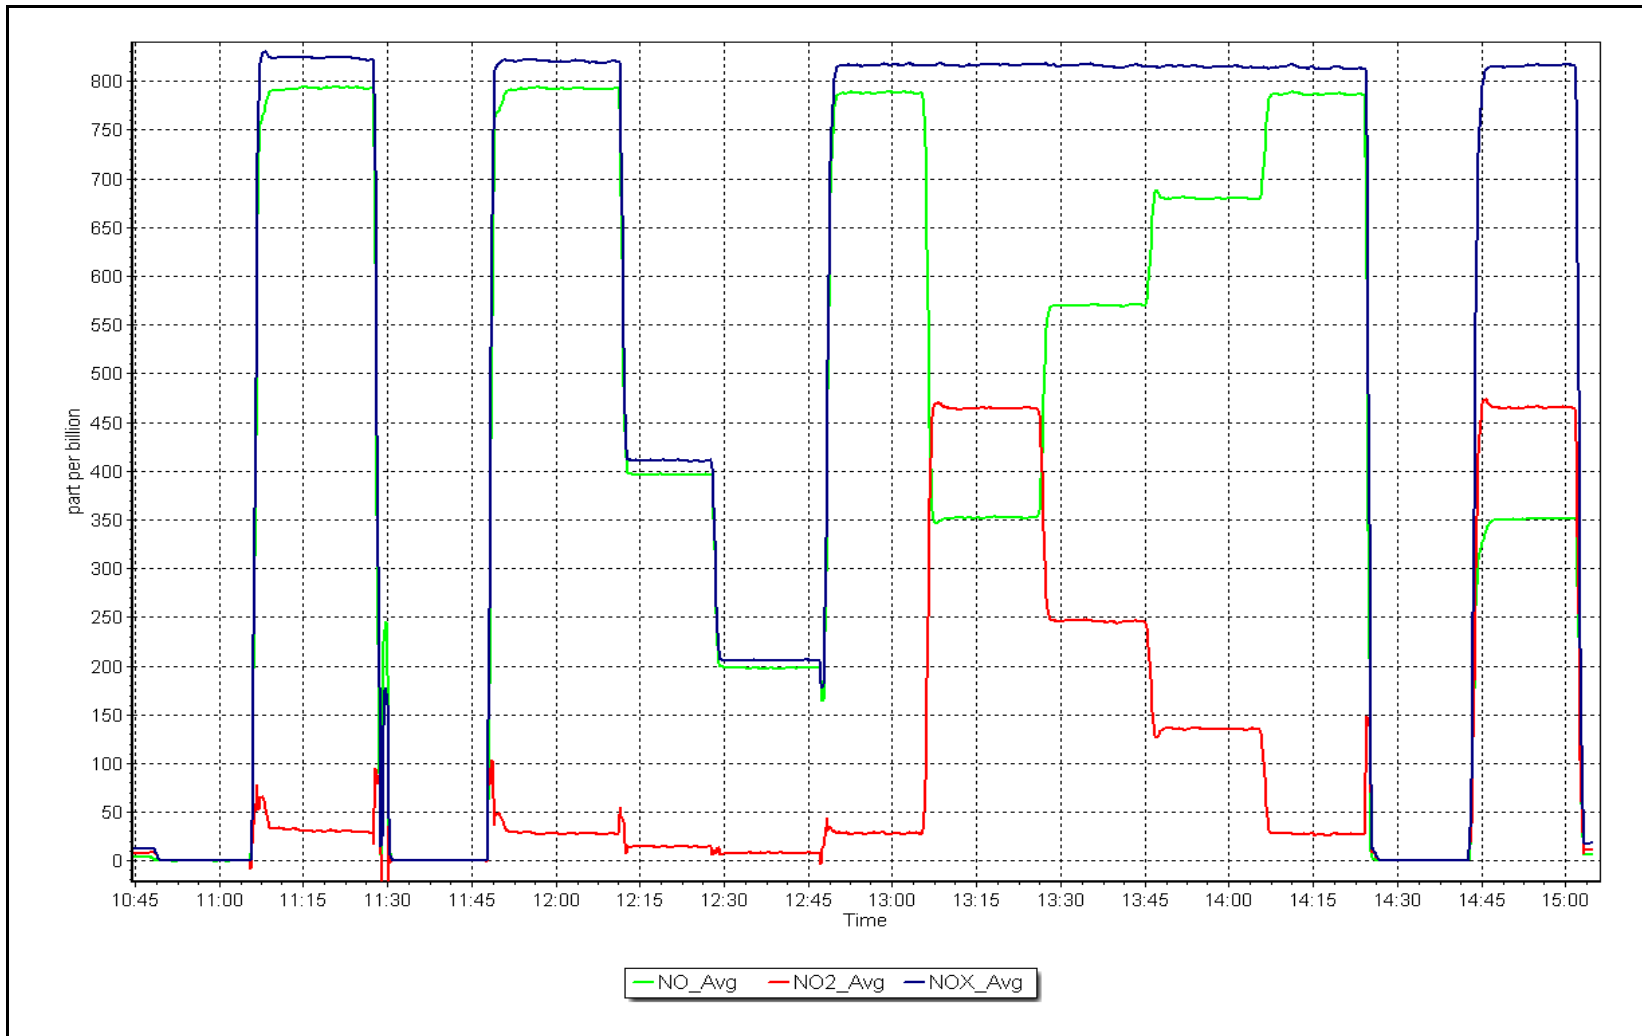



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS20 MACKAY RIVER JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 2, 2022
Station Name:	MacKay River	Station Number:	AMS20
Start Time (MST):	10:55	End Time (MST):	14:15
Analyzer make:	Thermo 43i	Analyzer serial #:	1501301450

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.1	----	Correlation Coefficient	0.999892	
800.3	797.4	1.0036			≥0.995
400.7	403.1	0.9940	Slope	0.993569	
199.8	206.8	0.9663			0.90 - 1.10
			Intercept	3.910928	+/-30

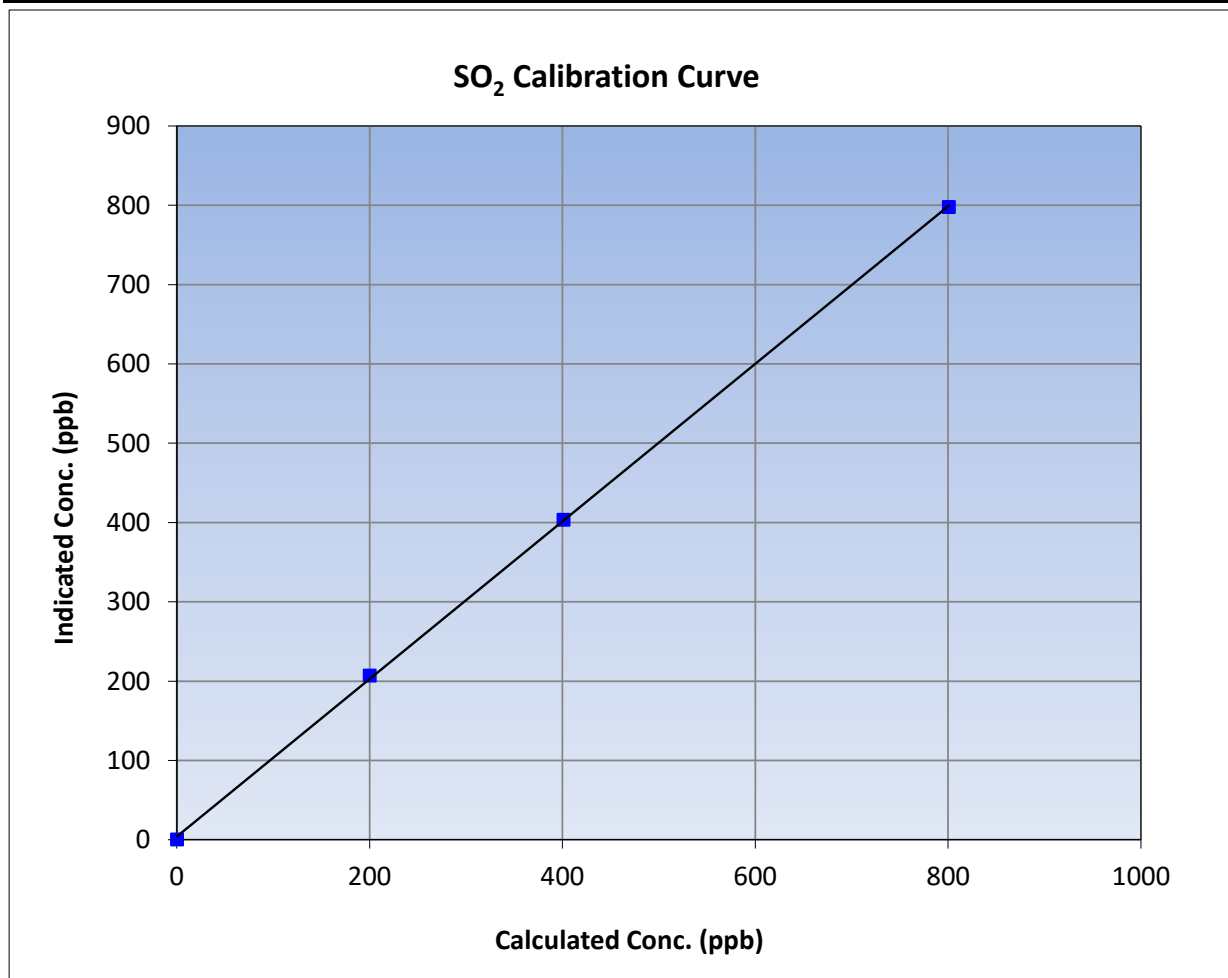

SO2 Calibration Plot

Date: January 17, 2023

Location: MacKay River

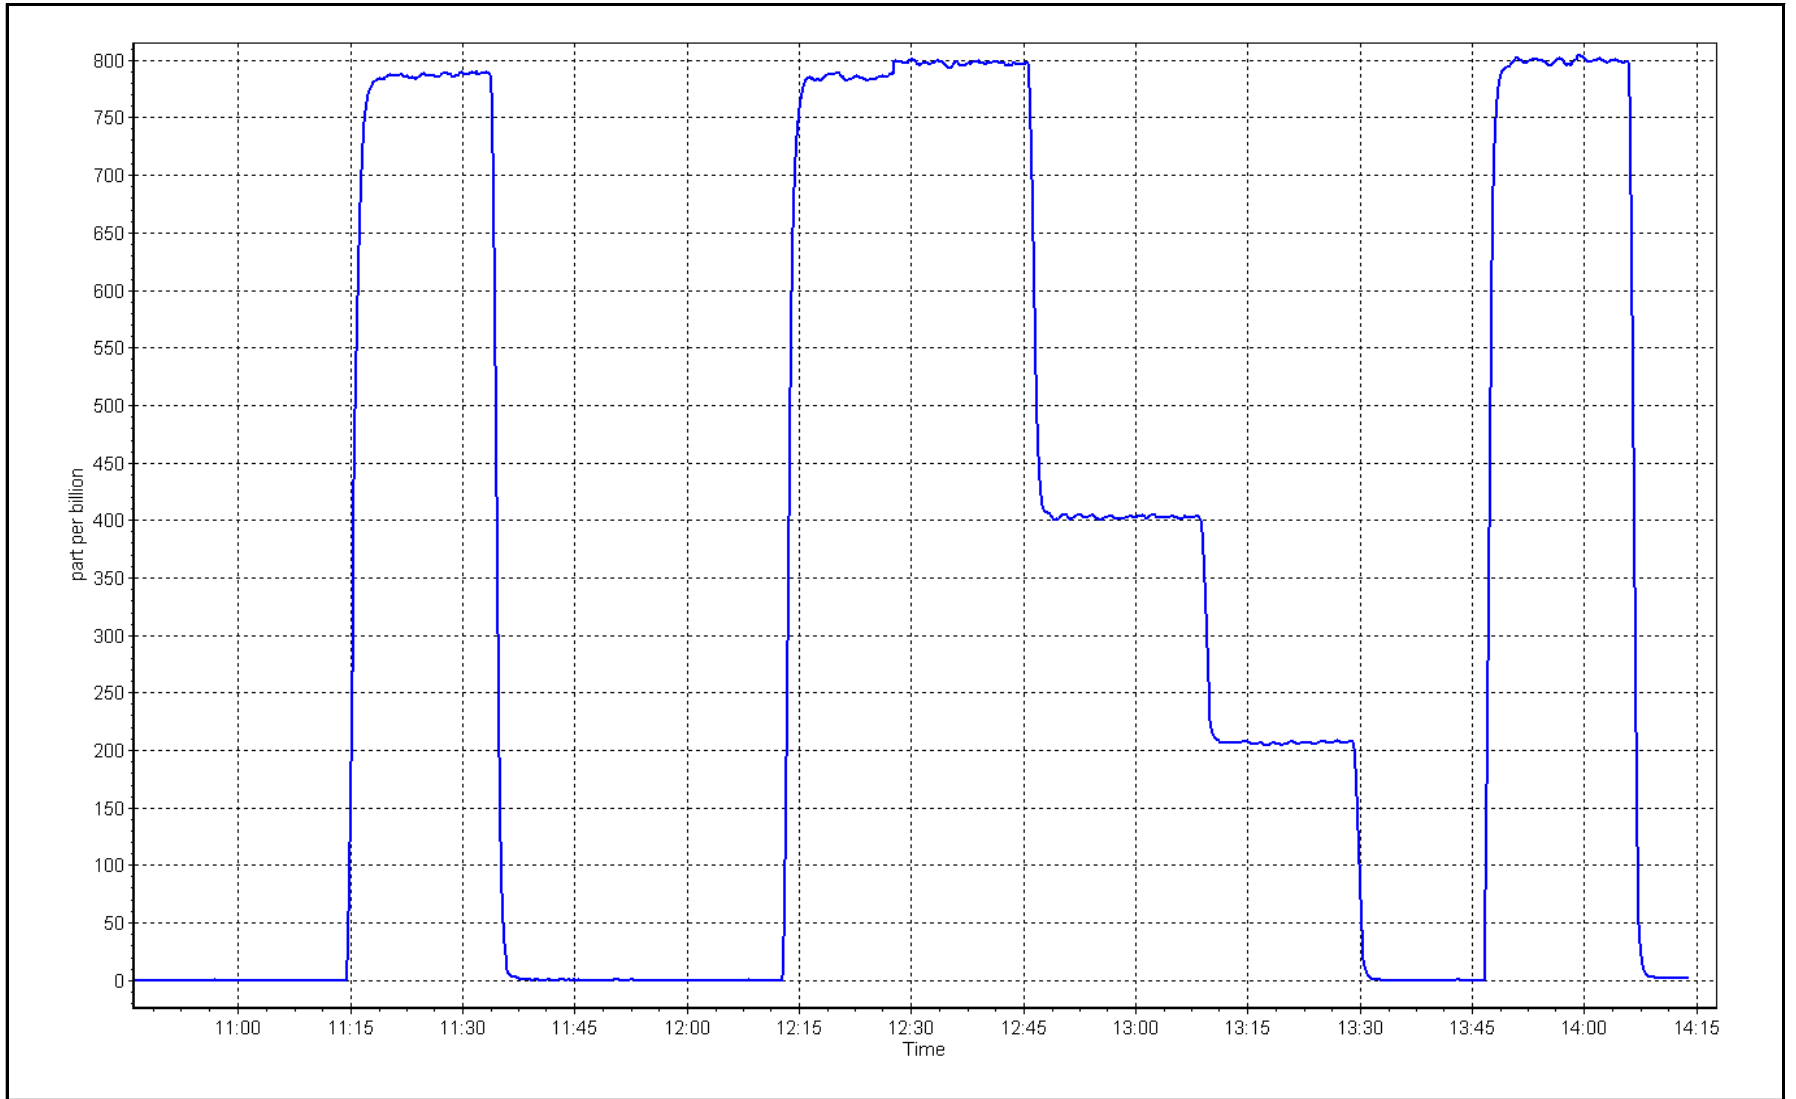



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: MacKay River Station number: AMS20
 Calibration Date: January 23, 2023 Last Cal Date: December 6, 2022
 Start time (MST): 11:31 End time (MST): 15:44
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 4.87 ppm Cal Gas Exp Date: May 5, 2023
 Cal Gas Cylinder #: EY0001922
 Removed Cal Gas Conc: 4.87 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: Teledyne API T700 Serial Number: 1220
 ZAG Make/Model: Teledyne API 701 Serial Number: 4522

Analyzer Information

Analyzer make: Teledyne API T101 Analyzer serial #: 196
 Converter make: Internal Converter serial #: NA
 Analyzer Range 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	1.004863	0.999429	Backgd or Offset: 46.3	46.3
Calibration intercept:	-0.061013	0.379115	Coeff or Slope: 1.035	0.981

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.0	----
as found span	4918	82.1	80.0	84.9	0.942
as found 2nd point	4959	41.1	40.0	43.0	0.931
as found 3rd point	4979	20.5	20.0	22.0	0.908
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.1	----
high point	4918	82.1	80.0	80.2	0.997
second point	4959	41.1	40.0	40.4	0.991
third point	4979	20.5	20.0	20.7	0.965
as left zero	5000	0.0	0.0	0.2	----
as left span	4918	82.1	80.0	79.9	1.001
SO2 Scrubber Check	4919	80.0	800.2	0.0	----
Date of last scrubber change:	December 15, 2020			Ave Corr Factor	0.984
Date of last converter efficiency test:					efficiency

Baseline Corr As found: 84.9 Prev response: 80.29 *% change: 5.4%
 Baseline Corr 2nd AF pt: 43.0 AF Slope: 1.059020 AF Intercept: 0.418989
 Baseline Corr 3rd AF pt: 22.0 AF Correlation: 0.999888

* = > +/-5% change initiates investigation

Notes: Changed inlet filter after multi point as founds. Scrubber test after calibrator zero. Adjusted span only.

Calibration Performed By: Sean Bala



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 23, 2023	Previous Calibration:	December 6, 2022
Station Name:	MacKay River	Station Number:	AMS20
Start Time (MST):	11:31	End Time (MST):	15:44
Analyzer make:	Teledyne API T101	Analyzer serial #:	196

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.1	----	Correlation Coefficient	0.999937	≥0.995
80.0	80.2	0.9971			
40.0	40.4	0.9909	Slope	0.999429	0.90 - 1.10
20.0	20.7	0.9647			
			Intercept	0.379115	+/-3

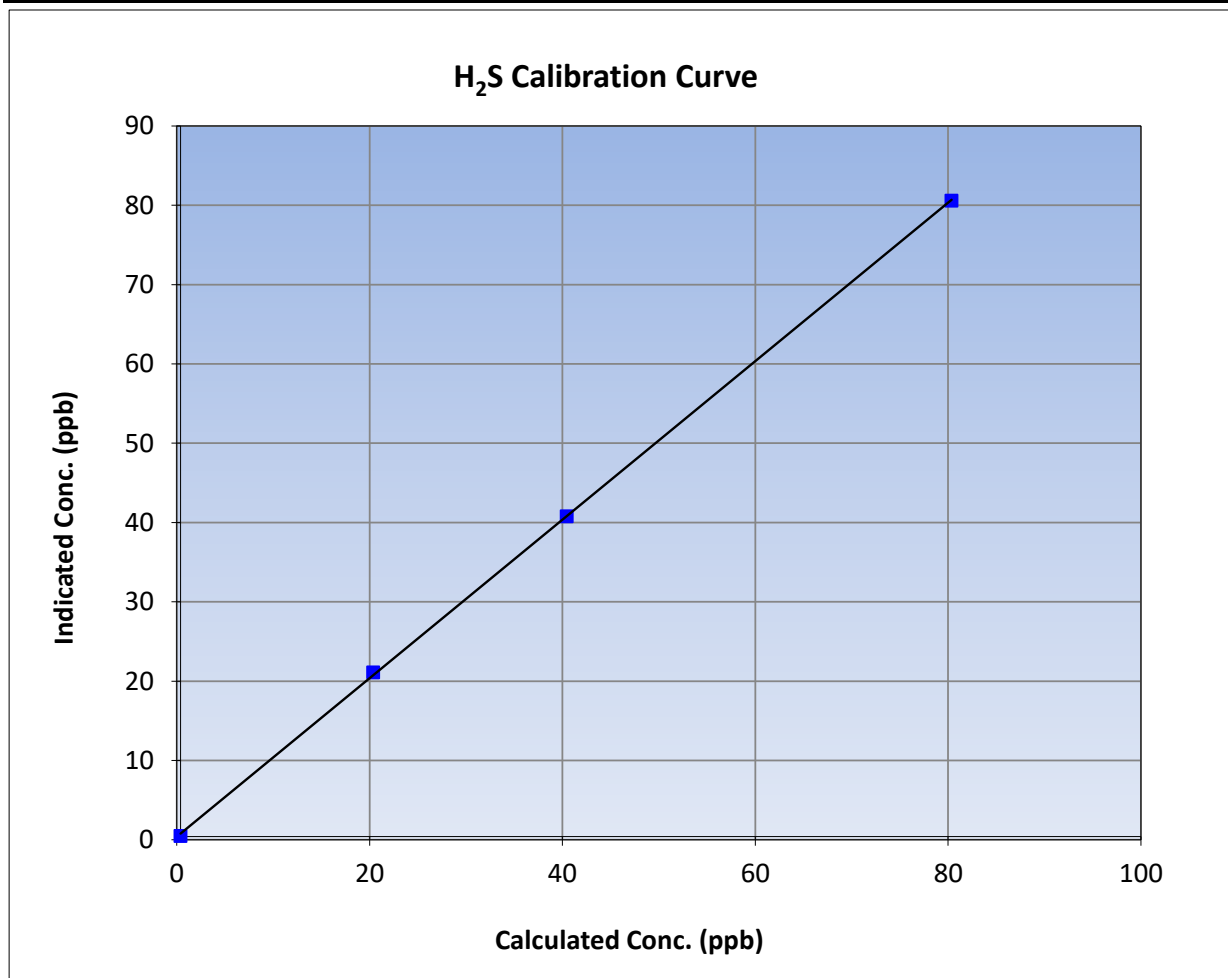

H₂S Calibration Plot

Date: January 23, 2023

Location: MacKay River

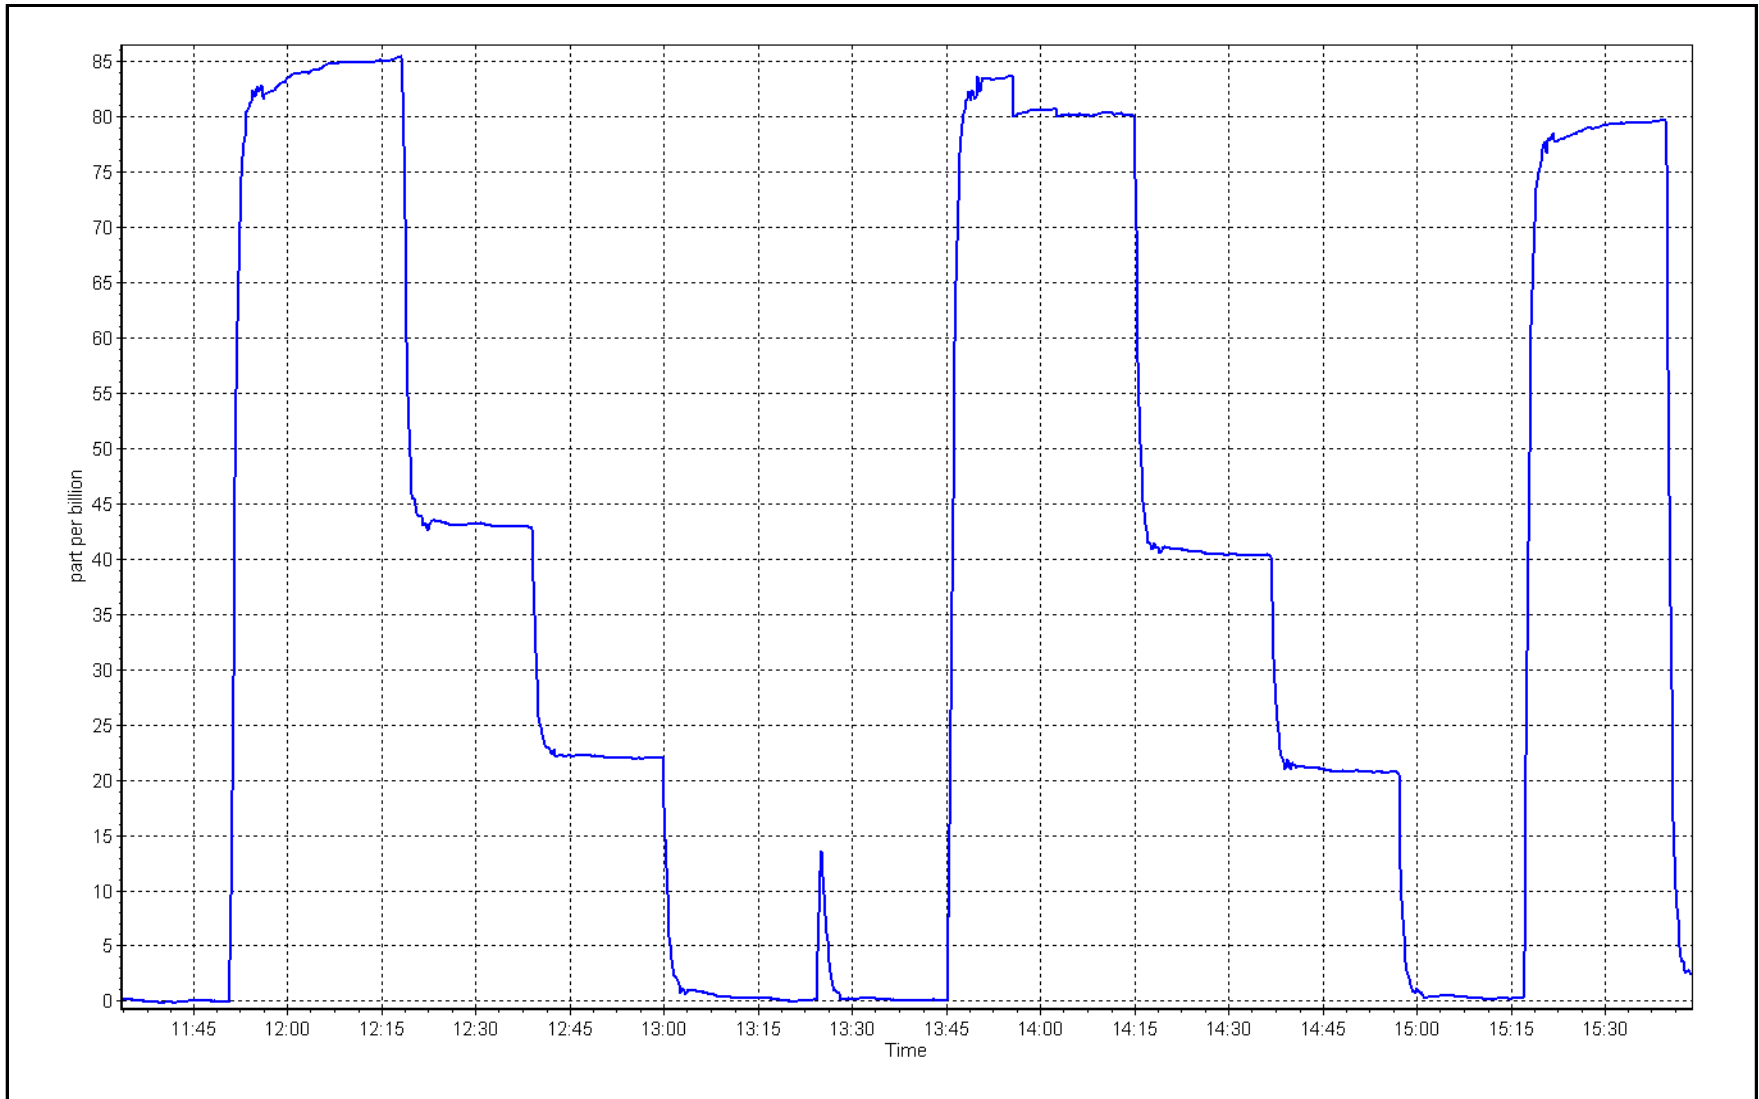



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 2, 2022
Station Name:	MacKay River	Station Number:	AMS20
Start Time (MST):	10:55	End Time (MST):	14:15
Analyzer make:	Thermo 51i-LT	Analyzer serial #:	1501663727

Calibration Data

Calculated Concentration (ppm) (Cc)	Indicated Concentration (ppm) (lc)	Correction factor (Cc/lc)	Statistical Evaluation	<u>Limits</u>	
0.00	0.06	----	Correlation Coefficient	0.999884	
17.34	17.20	1.0080			≥0.995
8.68	8.74	0.9933	Slope	0.986110	
4.33	4.50	0.9613			0.90 - 1.10
			Intercept	0.143798	+/-1.5

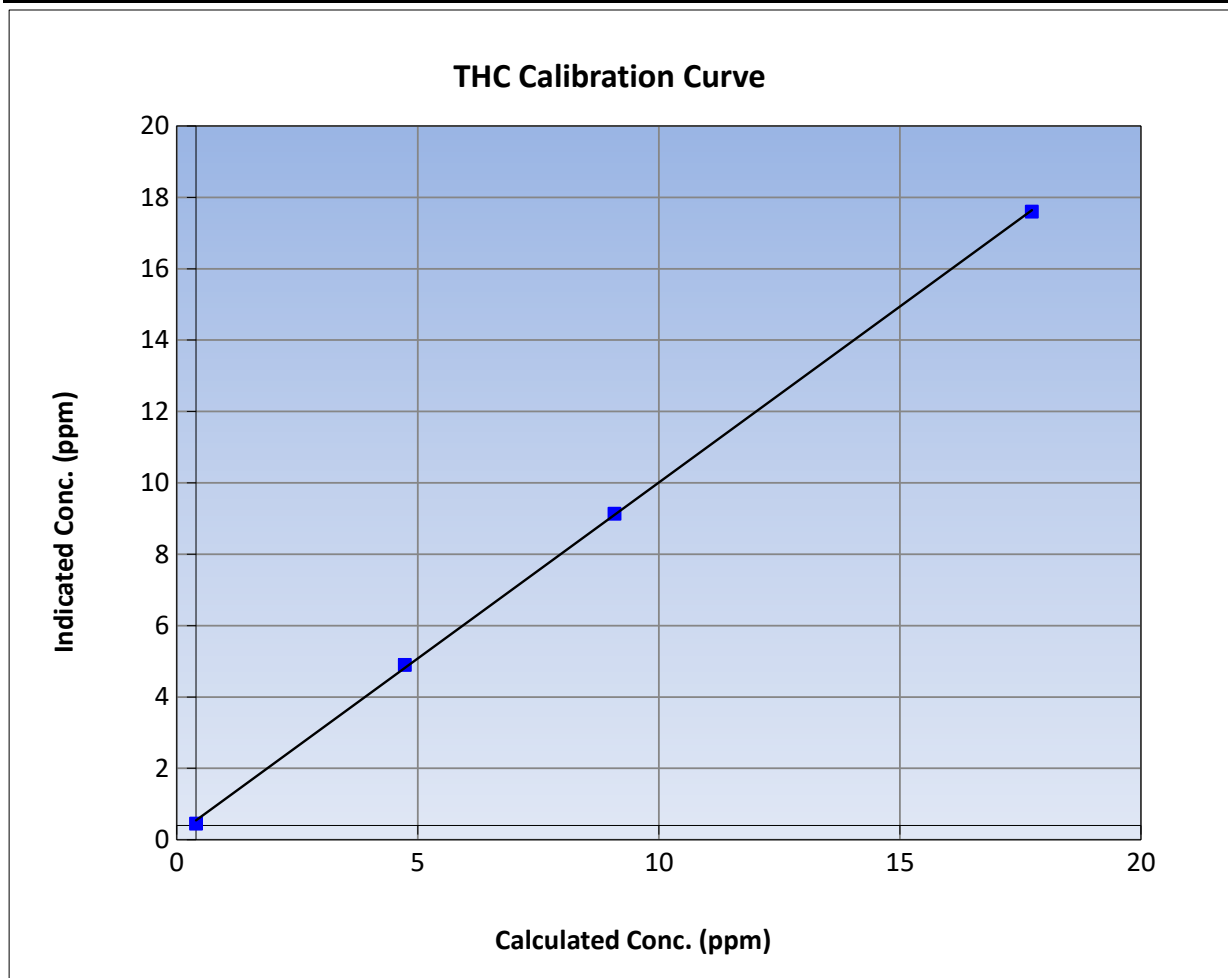

THC Calibration Plot

Date: January 17, 2023

Location: MacKay River





Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: MacKay River Station number: AMS20
Calibration Date: January 24, 2023 Last Cal Date: December 8, 2022
Start time (MST): 9:43 End time (MST): 13:48
Reason: Routine

Calibration Standards

NO Gas Cylinder #: T376265 Cal Gas Expiry Date: April 13, 2025
NOX Cal Gas Conc: 49.19 ppm NO Cal Gas Conc: 48.04 ppm
Removed Cylinder #: NA Removed Gas Exp Date: NA
Removed Gas NOX Conc: 49.19 ppm Removed Gas NO Conc: 48.04 ppm
NOX gas Diff: NO gas Diff:
Calibrator Model: Teledyne API T700 Serial Number: 1220
ZAG make/model: Teledyne API 701 Serial Number: 4766

Analyzer Information

Analyzer make: Thermo 42i Analyzer serial #: 1505164379
NOX Range (ppb): 0 - 1000 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.379	1.409	NO bkgnd or offset:	3.8	3.9
NOX coeff or slope:	0.995	0.995	NOX bkgnd or offset:	3.8	3.9
NO2 coeff or slope:	0.995	0.995	Reaction cell Press:	172.3	175.0

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	0.995546	0.996925
NO _x Cal Offset:	1.090368	2.570800
NO Cal Slope:	0.995349	0.998231
NO Cal Offset:	-0.168545	1.372065
NO ₂ Cal Slope:	1.008585	1.007507
NO ₂ Cal Offset:	-0.287241	-1.673176



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-0.1	-0.1	0.1	----	----
as found span	4917	83.3	819.5	800.3	19.2	815.9	789.1	26.8	1.0044	1.0142
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.1	0.0	0.1	----	----
high point	4917	83.3	819.5	800.3	19.2	819.0	800.3	18.6	1.0006	1.0000
second point	4956	41.7	410.4	400.8	9.6	410.8	400.0	10.8	0.9991	1.0021
third point	4979	20.8	204.6	199.9	4.8	210.5	203.7	6.8	0.9722	0.9811
as left zero	5000	0.0	0.0	0.0	0.0	0.1	0.0	0.1	----	----
as left span	4917	83.3	819.5	466.6	352.9	814.1	453.9	360.1	1.0066	1.0280
Average Correction Factor									0.9906	0.9944

Corrected As found	NO _x = 816.0 ppb	NO = 789.2 ppb	* => +/-5% change initiates investigation	*Percent Change	NO _x = -0.1%	
Previous Response	NO _x = 816.9 ppb	NO = 796.4 ppb		*Percent Change	NO = -0.9%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO ₂)						
as found GPT point (200 ppb NO ₂)						
as found GPT point (100 ppb NO ₂)						
1st GPT point (400 ppb O ₃)	785.7	452.0	352.9	355.4	0.9928	100.7%
2nd GPT point (200 ppb O ₃)	785.7	611.5	193.4	190.9	1.0129	98.7%
3rd GPT point (100 ppb O ₃)	785.7	695.8	109.1	107.1	1.0183	98.2%
Average Correction Factor					1.0080	99.2%

Notes:

Adjusted the span only.

Calibration Performed By:

Denny Ray Estador



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 8, 2022
Station Name:	Mackay River	Station Number:	AMS20
Start Time (MST):	9:43	End Time (MST):	13:48
Analyzer make:	Thermo 42i	Analyzer serial #:	1505164379

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.1	----	Correlation Coefficient	≥0.995	
819.5	819.0	1.0006			
410.4	410.8	0.9991			
204.6	210.5	0.9722			
			Slope	0.996925	0.90 - 1.10
			Intercept	2.570800	+/-20

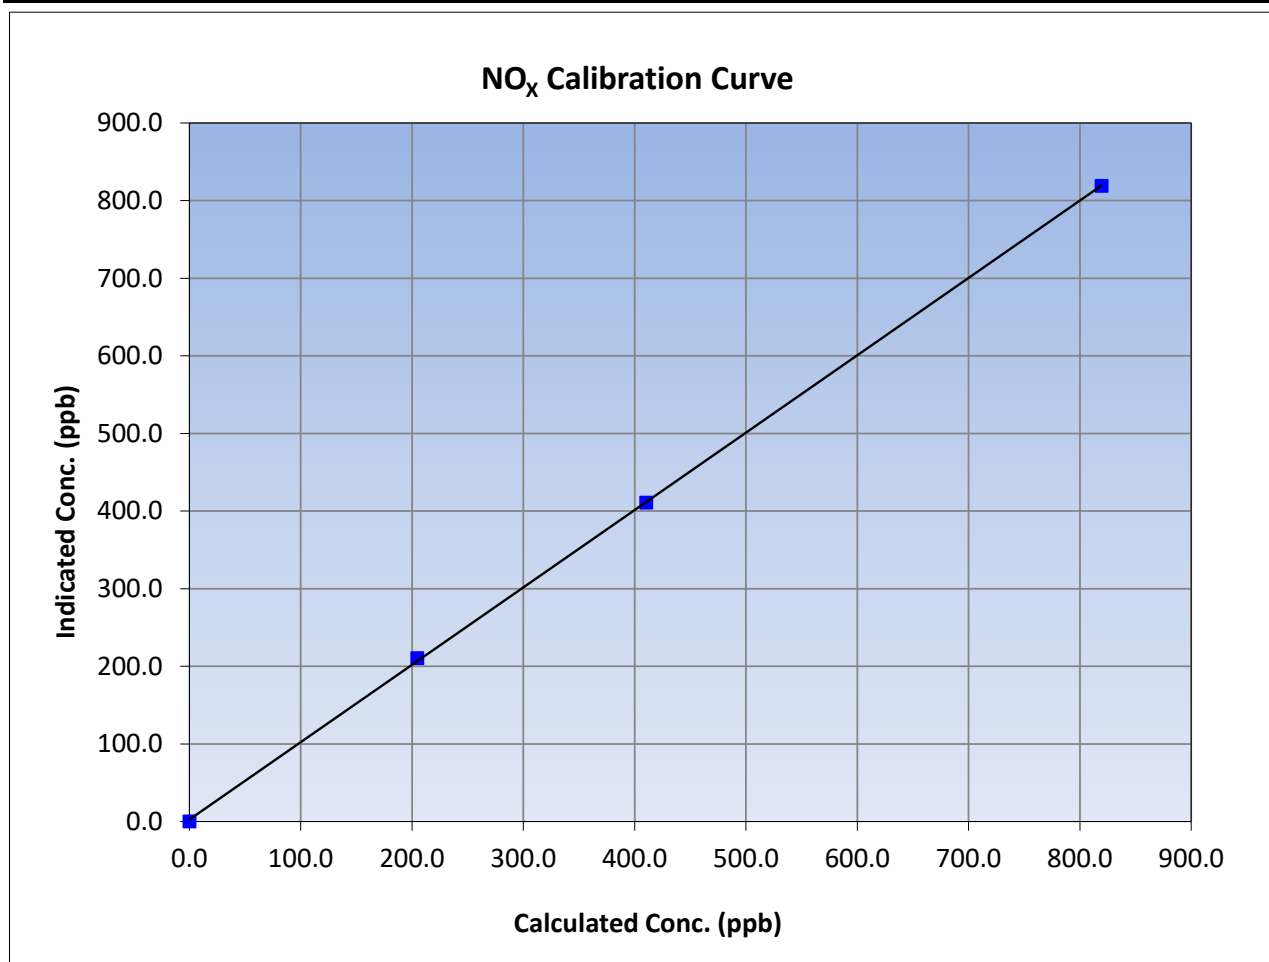



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 8, 2022
Station Name:	Mackay River	Station Number:	AMS20
Start Time (MST):	9:43	End Time (MST):	13:48
Analyzer make:	Thermo 42i	Analyzer serial #:	1505164379

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥ 0.995 $0.90 - 1.10$ $+/-20$
800.3	800.3	1.0000		
400.8	400.0	1.0021		
199.9	203.7	0.9811		
			0.999965	
			0.998231	
			1.372065	

NO Calibration Curve

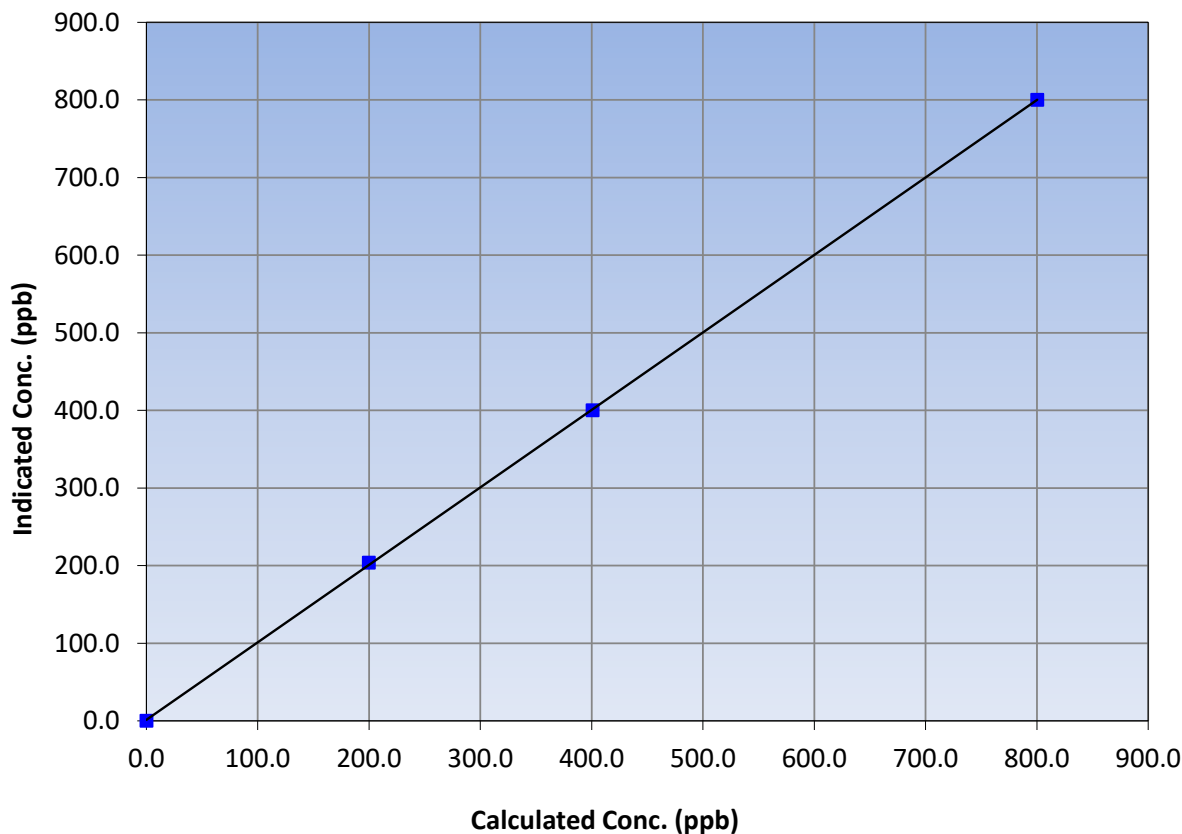



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 8, 2022
Station Name:	MacKay River	Station Number:	AMS20
Start Time (MST):	9:43	End Time (MST):	13:48
Analyzer make:	Thermo 42i	Analyzer serial #:	1505164379

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		Limits			
0.0	0.1	----	Correlation Coefficient	0.999825	≥0.995			
352.9	355.4	0.9928						
193.4	190.9	1.0129				Slope	1.007507	0.90 - 1.10
109.1	107.1	1.0183						
			Intercept	-1.673176	+/-20			

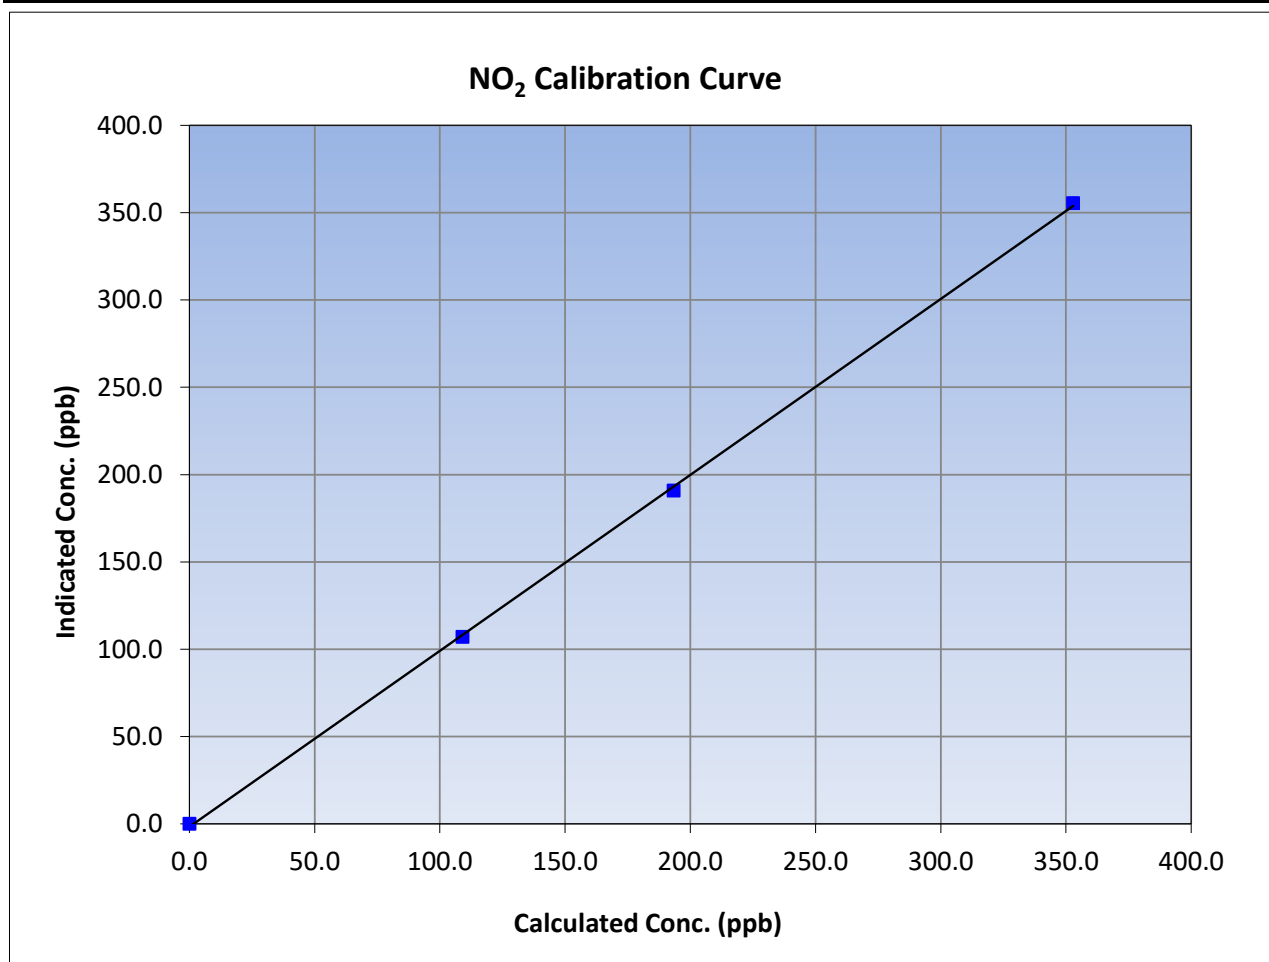

NO_x Calibration Plot

Date: January 24, 2023

Location: MacKay River

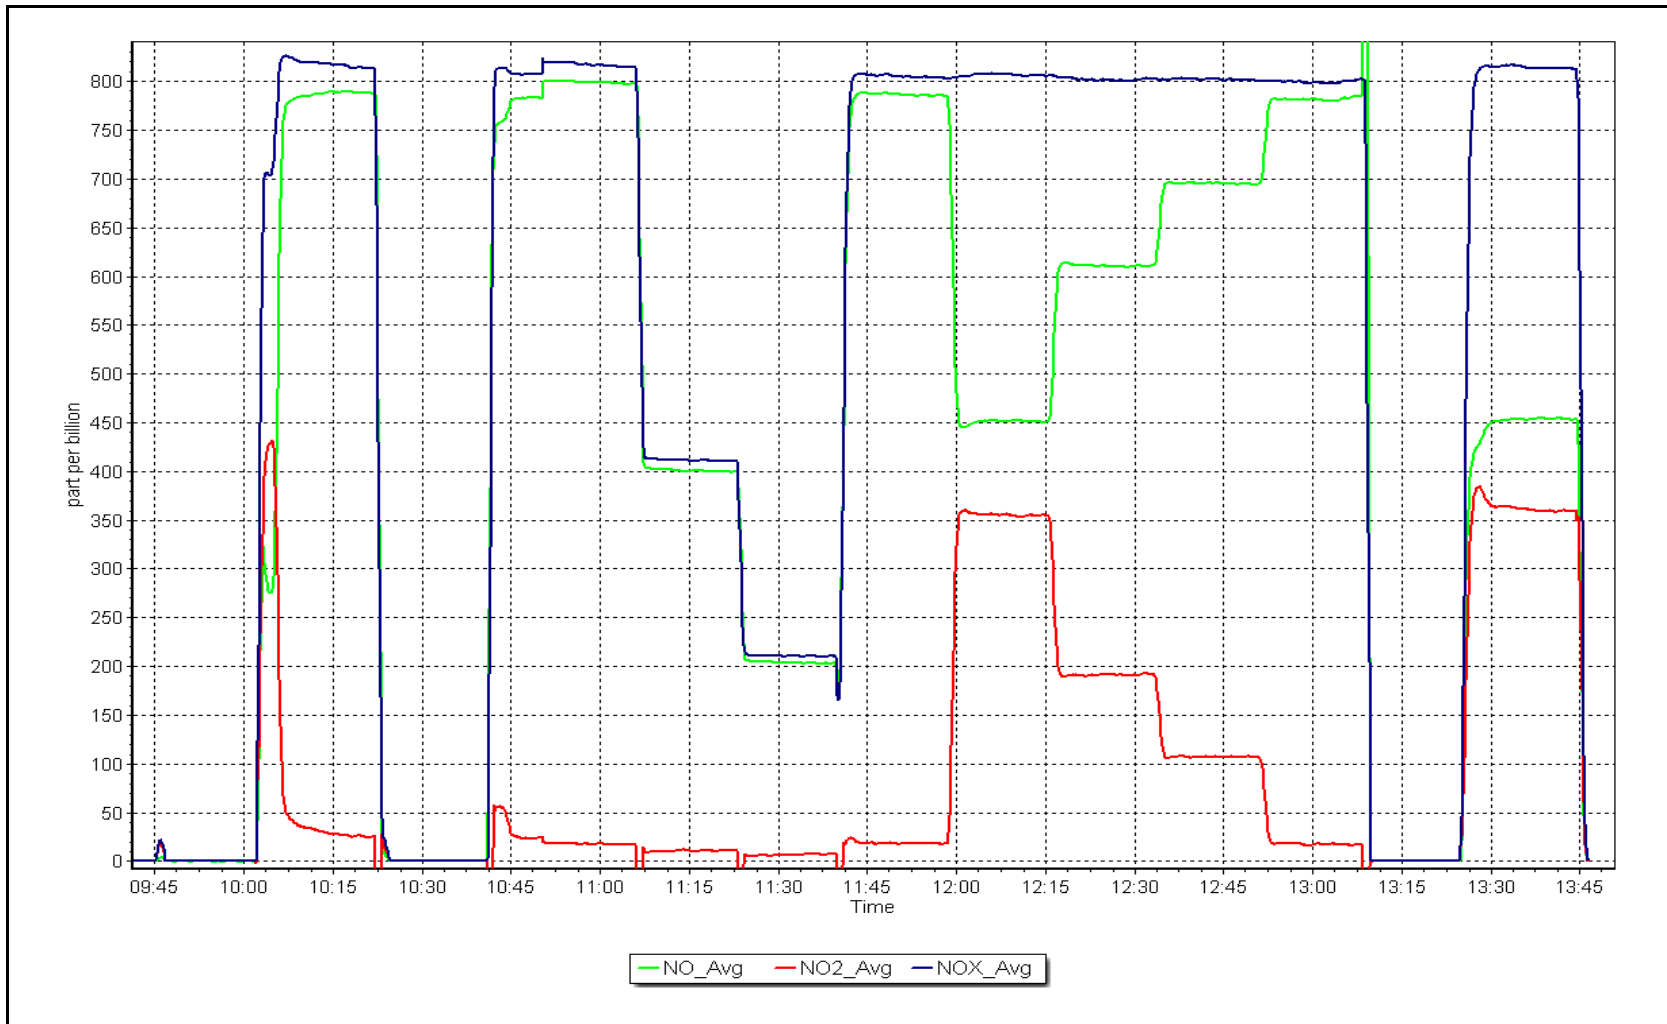



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

**AMS21
CONKLIN
JANUARY 2023**

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name: Conklin Station number: AMS21
 Calibration Date: January 3, 2023 Last Cal Date: December 13, 2022
 Start time (MST): 11:33 End time (MST): 14:50
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 49.93 ppm Cal Gas Exp Date: January 5, 2025
 Cal Gas Cylinder #: CC259455
 Removed Cal Gas Conc: 49.93 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: Diff between cyl:
 Calibrator Make/Model: Teledyne API T700 Serial Number: 3810
 ZAG Make/Model: Teledyne API 701 Serial Number: 262

Analyzer Information

Analyzer make: Thermo 43i Analyzer serial #: 1428701363
 Analyzer Range 0 - 1000 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.997976	1.003298	Backgd or Offset: 27.0	27.9
Calibration intercept:	1.435794	0.595998	Coeff or Slope: 0.914	0.914

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5005	0.0	0.0	0.5	----
as found span	4920	80.2	800.8	801.0	1.000
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5005	0.0	0.0	0.1	----
high point	4920	80.2	800.8	804.1	0.996
second point	4960	40.1	400.4	401.8	0.997
third point	4980	20.0	200.1	202.4	0.989
as left zero	5005	0.0	0.0	0.2	----
as left span	4920	80.2	800.8	802.0	0.999
Average Correction Factor					0.994

Baseline Corr As found: 800.50 Previous response 800.66 *% change 0.0%
 Baseline Corr 2nd AF pt: NA AF Slope: AF Intercept:
 Baseline Corr 3rd AF pt: NA AF Correlation:

* = > +/-5% change initiates investigation

Notes: Adjusted the zero only.

Calibration Performed By: Denny Ray Estador



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 13, 2022
Station Name:	Conklin	Station Number:	AMS21
Start Time (MST):	11:33	End Time (MST):	14:50
Analyzer make:	Thermo 43i	Analyzer serial #:	1428701363

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.1	----	Correlation Coefficient	0.999995	≥0.995
800.8	804.1	0.9960			
400.4	401.8	0.9966	Slope	1.003298	0.90 - 1.10
200.1	202.4	0.9887			
			Intercept	0.595998	+/-30

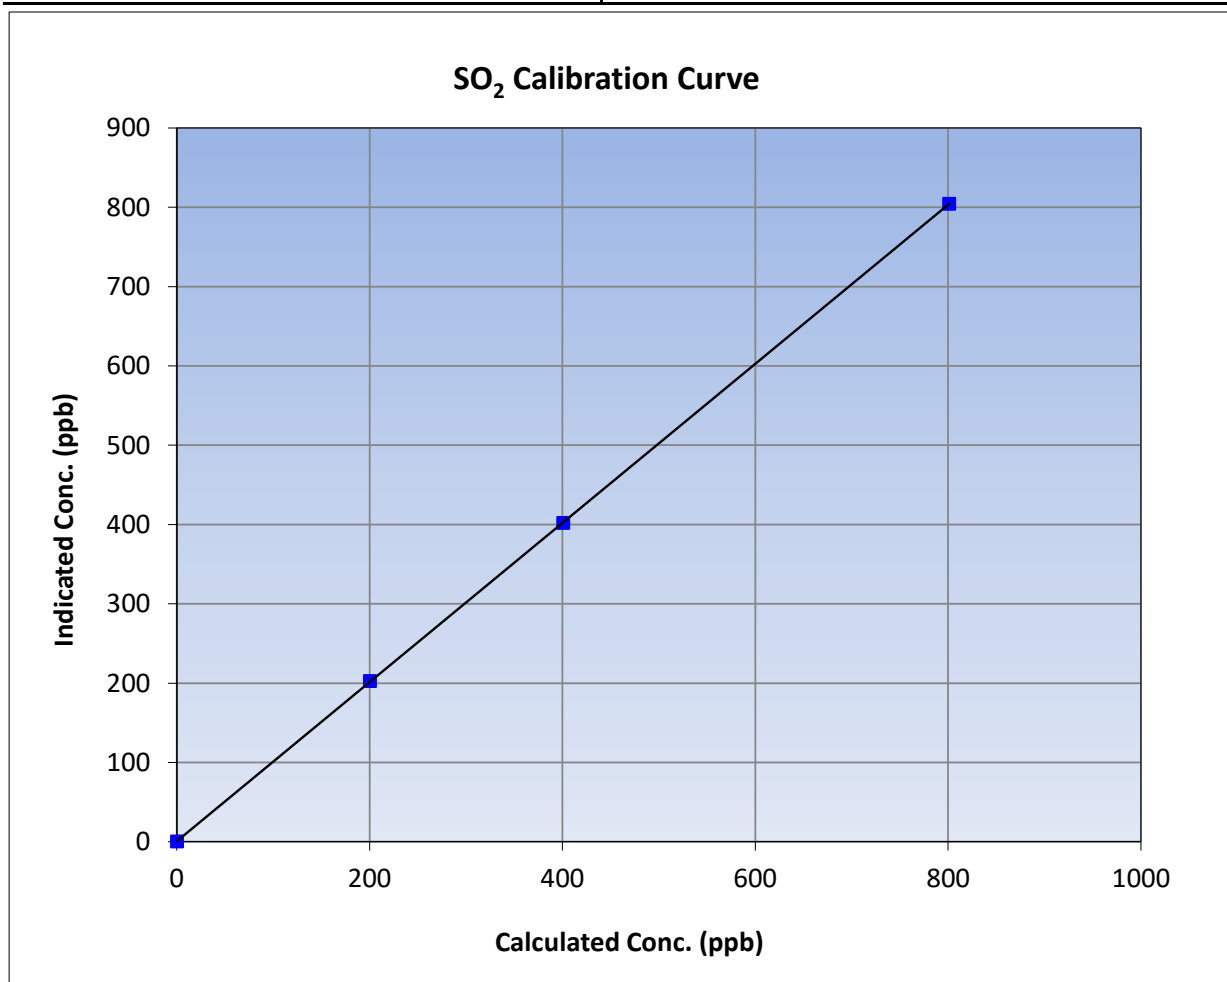

SO2 Calibration Plot

Date: January 3, 2023

Location: Conklin

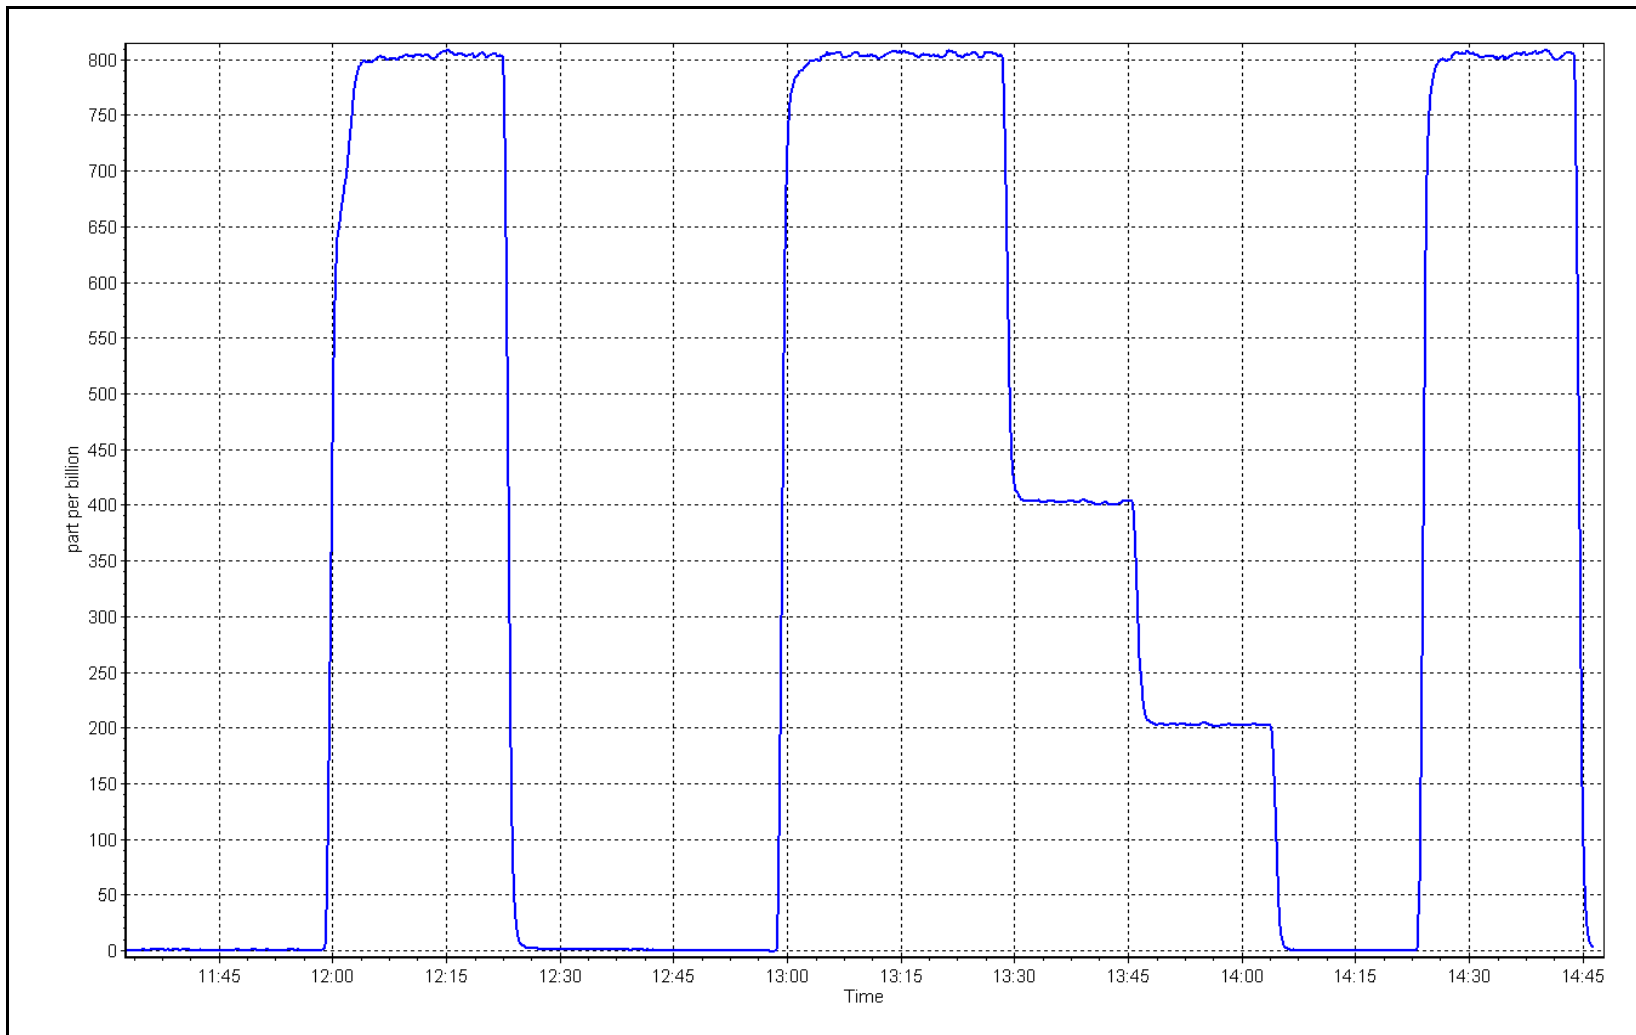



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name: Conklin Station number: AMS21
 Calibration Date: January 9, 2023 Last Cal Date: December 22, 2022
 Start time (MST): 9:05 End time (MST): 12:51
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.03 ppm Cal Gas Exp Date: April 16, 2022
 Cal Gas Cylinder #: CC505493
 Removed Cal Gas Conc: 5.03 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 3810
 ZAG Make/Model: API 701 Serial Number: 263

Analyzer Information

Analyzer make: Thermo 43i-TLE Analyzer serial #: 1236656116
 Converter make: CD-Nova 101 Converter serial #: NA
 Analyzer Range 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.999155	1.005143	Backgd or Offset:	3.0
Calibration intercept:	0.597263	-0.162334	Coeff or Slope:	1.055
				2.8
				0.951

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	-0.4	----
as found span	4921	79.5	80.0	89.1	0.894
as found 2nd point	4960	39.8	40.0	44.6	0.890
as found 3rd point	4980	19.9	20.0	22.3	0.882
new cylinder response					

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	-0.2	----
high point	4921	79.5	80.0	80.2	0.997
second point	4960	39.8	40.0	40.1	0.999
third point	4980	19.9	20.0	20.0	1.001
as left zero	5000	0.0	0.0	0.0	----
as left span	4921	79.5	80.0	79.4	1.007
SO2 Scrubber Check	4920	80.2	802.0	0.0	----
Date of last scrubber change:				Ave Corr Factor	0.999
Date of last converter efficiency test:				efficiency	

Baseline Corr As found: 89.5 Prev response: 80.50 *% change: **10.1%**
 Baseline Corr 2nd AF pt: 45.0 AF Slope: 1.118193 AF Intercept: -0.244908
 Baseline Corr 3rd AF pt: 22.7 AF Correlation: 0.999986

* = > +/-5% change initiates investigation

Notes: Adjusted both zero and span.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 9, 2023	Previous Calibration:	December 22, 2022
Station Name:	Conklin	Station Number:	AMS21
Start Time (MST):	9:05	End Time (MST):	12:51
Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1236656116

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	-0.2	----	Correlation Coefficient	0.999999	
80.0	80.2	0.9971			≥0.995
40.0	40.1	0.9985	Slope	1.005143	
20.0	20.0	1.0010			0.90 - 1.10
			Intercept	-0.162334	+/-3

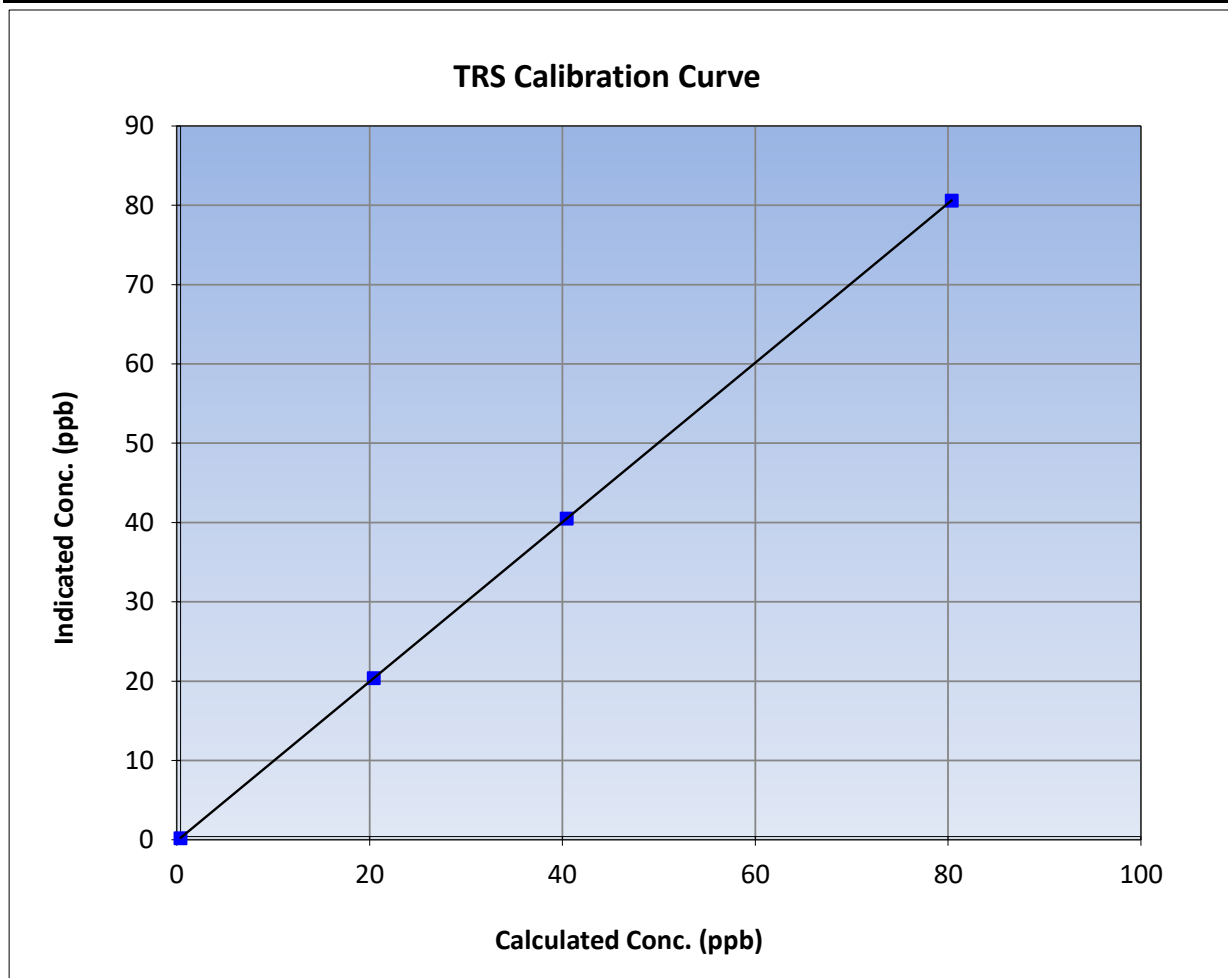

TRS Calibration Plot

Date: January 9, 2023

Location: Conklin

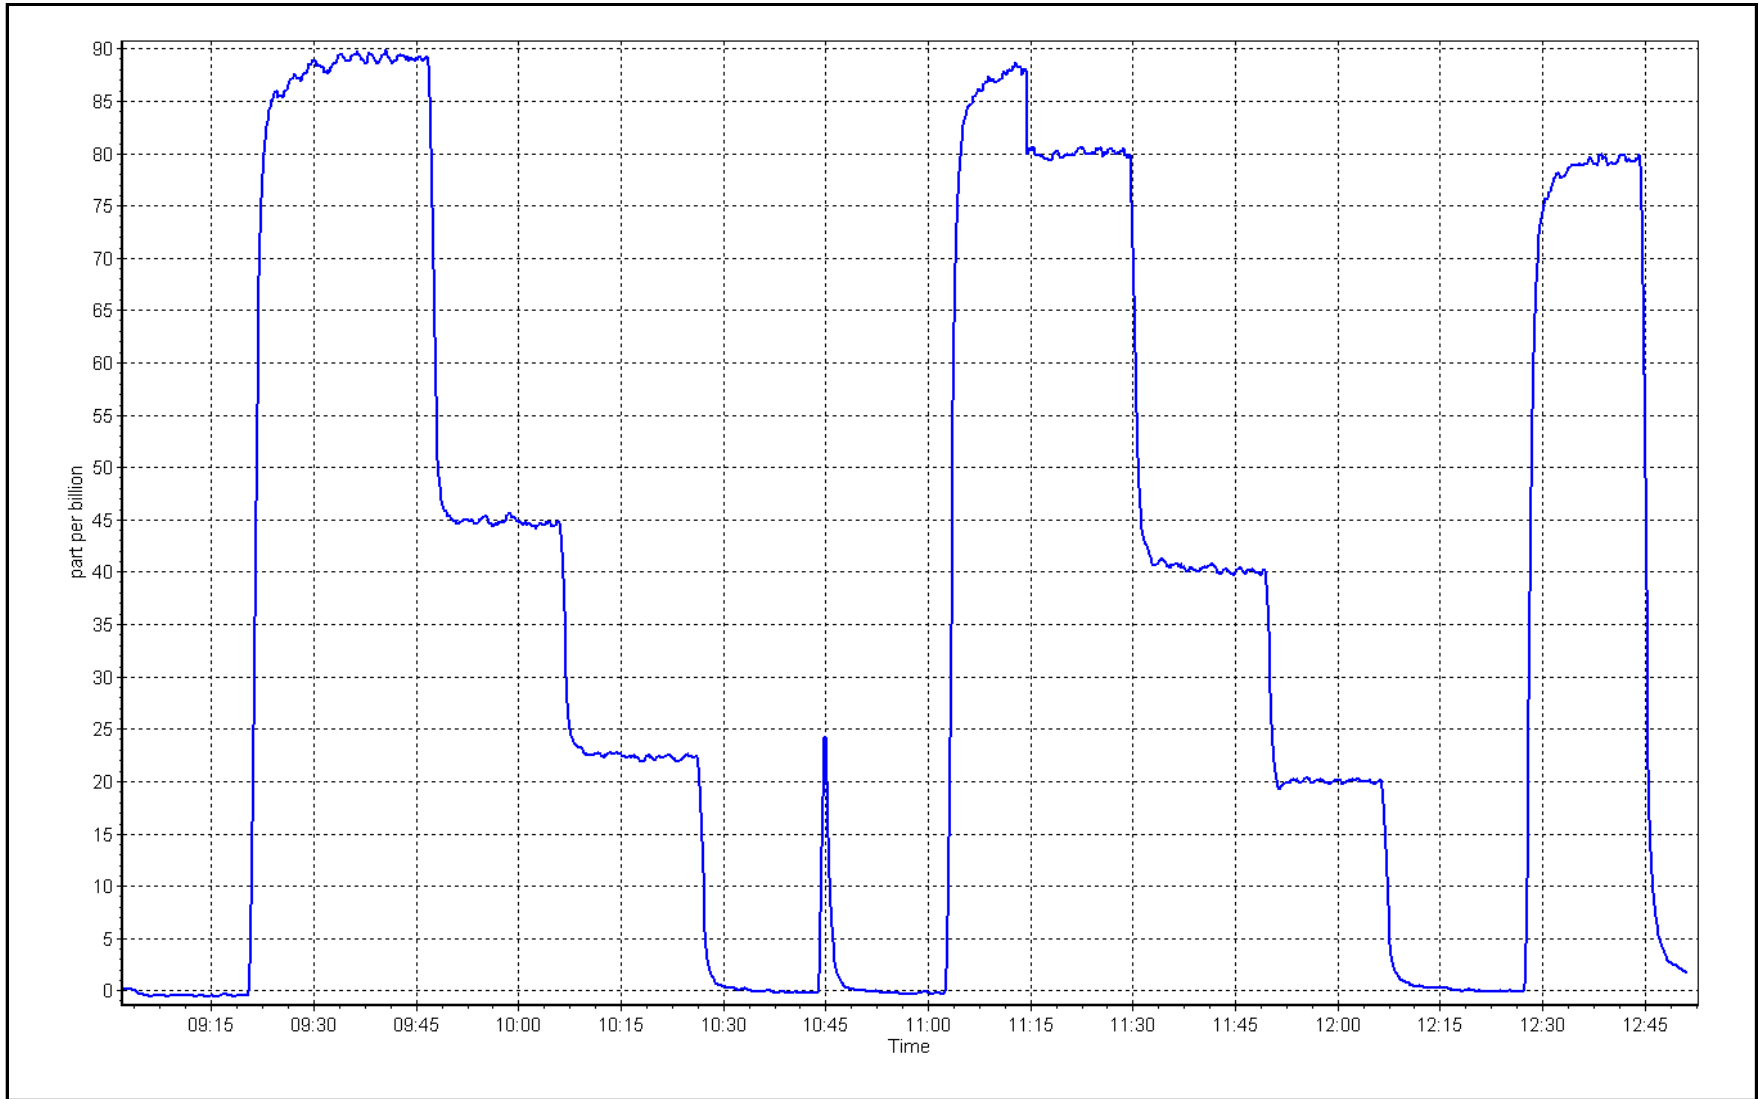



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Conklin	Station number:	AMS21
Calibration Date:	January 3, 2023	Last Cal Date:	December 13, 2022
Start time (MST):	11:33	End time (MST):	14:50
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC259455	Cal Gas Expiry Date:	January 5, 2025
CH ₄ Cal Gas Conc.	497.9 ppm	CH ₄ Equiv Conc.	1067.7 ppm
C ₃ H ₈ Cal Gas Conc.	207.2 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	497.9 ppm	CH ₄ Equiv Conc.	1067.7 ppm
Removed C ₃ H ₈ Conc.	207.2 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	Teledyne API T700	Serial Number:	3810
ZAG make/model:	Teledyne API 701	Serial Number:	262

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	118148495
THC Range (ppm):	0 - 20 ppm	CH ₄ Range (ppm):	0 - 10 ppm
NMHC Range (ppm):	0 - 10 ppm		

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	1.81E-04	1.85E-04	NMHC SP Ratio:	4.48E-05
CH ₄ Retention time:	12.4	12.2	NMHC Peak Area:	203812
				196117

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.2	17.13	13.17	1.301
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.2	17.13	17.13	1.000
second point	4960	40.1	8.56	8.55	1.001
third point	4980	20.0	4.27	4.31	0.991
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.2	17.13	17.03	1.006

Average Correction Factor				0.997
Baseline Corr AF:	13.17	Prev response	16.89	*% change -28.3%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4920	80.2	9.14	6.78	1.347
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4920	80.2	9.14	9.13	1.001
second point	4960	40.1	4.57	4.58	0.999
third point	4980	20	2.28	2.31	0.989
as left zero	5000	0	0.00	0.00	----
as left span	4920	80.2	9.14	9.05	1.010
Average Correction Factor					0.996
Baseline Corr AF:	6.78	Prev response	8.99	*% change	-32.6%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.2	7.99	6.38	1.252
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.2	7.99	8.00	0.999
second point	4960	40.1	3.99	3.98	1.004
third point	4980	20.0	1.99	2.01	0.993
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.2	7.99	7.97	1.002
Average Correction Factor					0.998
Baseline Corr AF:	6.38	Prev response	7.89	*% change	-23.7%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	0.986853	0.999155
THC Cal Offset:	-0.014487	0.013380
CH ₄ Cal Slope:	0.989953	1.000338
CH ₄ Cal Offset:	-0.012077	0.001151
NMHC Cal Slope:	0.984570	0.998171
NMHC Cal Offset:	-0.003608	0.013029

Notes: Adjusted the span only. N2 and H2 cylinders changed.

Calibration Performed By: Denny Ray Estador



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 13, 2022
Station Name:	Conklin	Station Number:	AMS21
Start Time (MST):	11:33	End Time (MST):	14:50
Analyzer make:	Thermo 55i	Analyzer serial #:	118148495

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999991	≥ 0.995
17.13	17.13	1.0000			
8.56	8.55	1.0015			
4.27	4.31	0.9907			
			Slope	0.999155	0.90 - 1.10
			Intercept	0.013380	+/-0.5

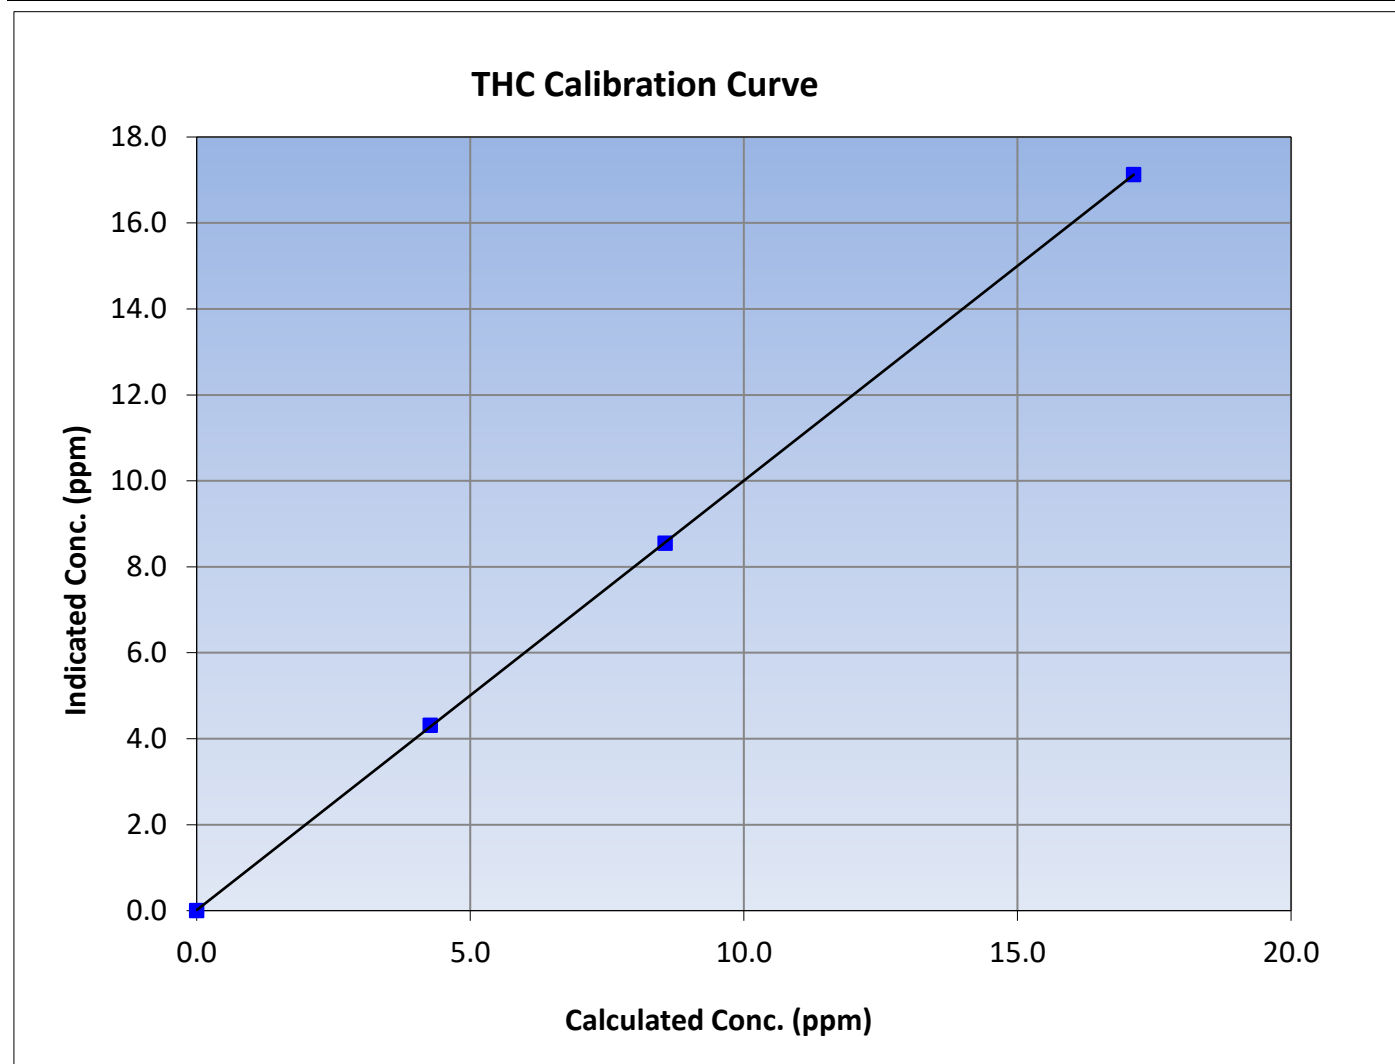



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 13, 2022
Station Name:	Conklin	Station Number:	AMS21
Start Time (MST):	11:33	End Time (MST):	14:50
Analyzer make:	Thermo 55i	Analyzer serial #:	118148495

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999987	≥ 0.995
7.99	8.00	0.9989			
3.99	3.98	1.0035			
1.99	2.01	0.9928			
			Slope	1.000338	0.90 - 1.10
			Intercept	0.001151	+/-0.5

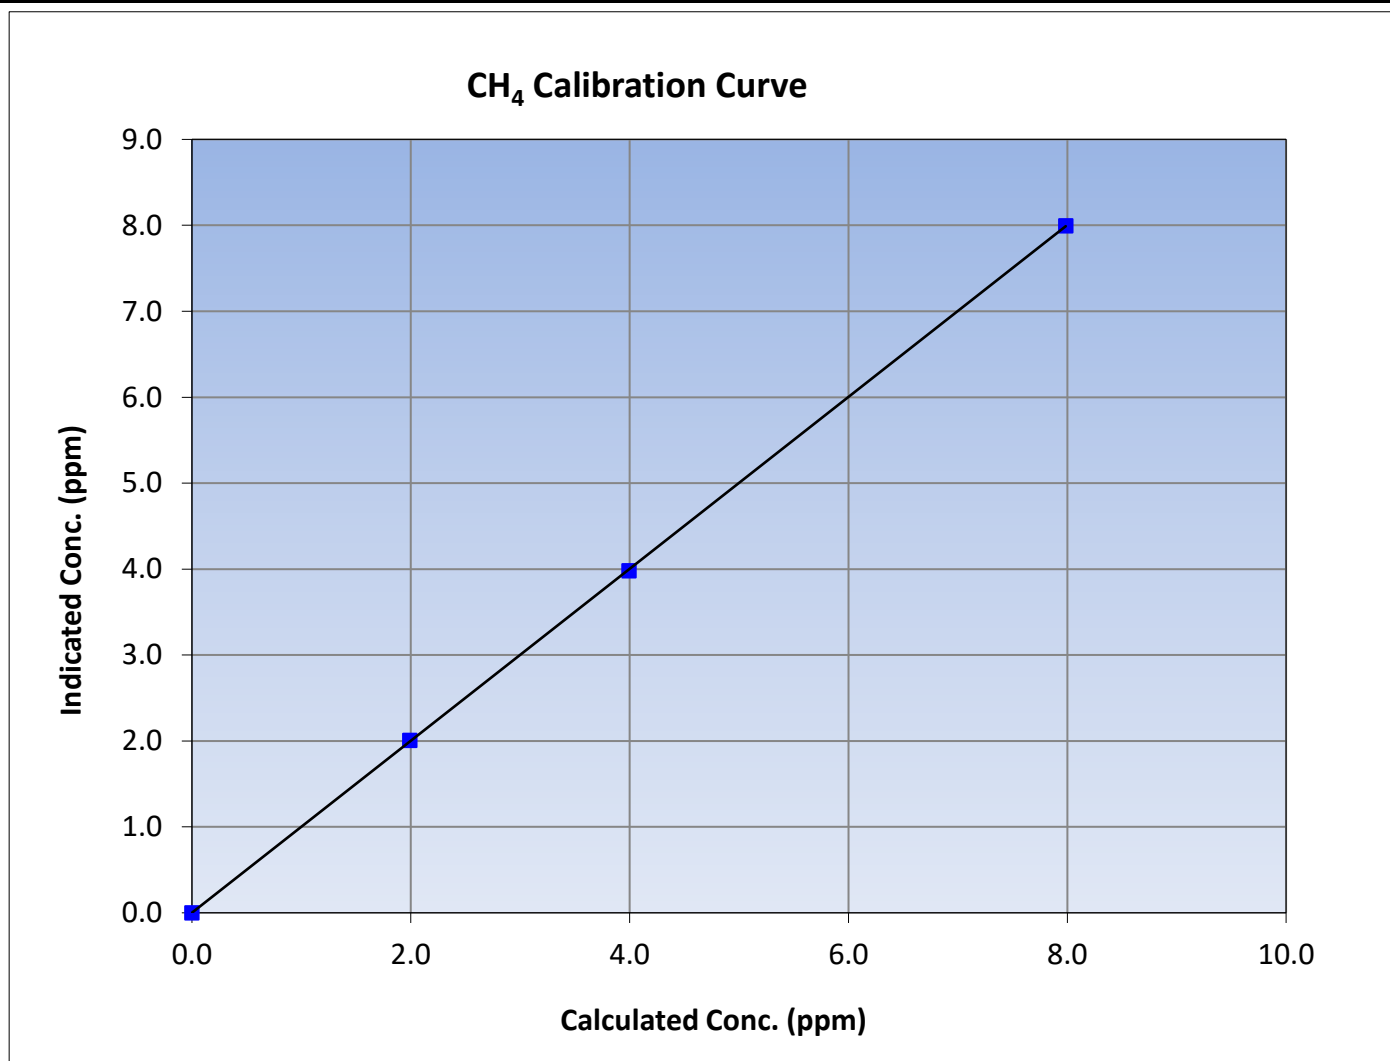



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 13, 2022
Station Name:	Conklin	Station Number:	AMS21
Start Time (MST):	11:33	End Time (MST):	14:50
Analyzer make:	Thermo 55i	Analyzer serial #:	118148495

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999990	≥ 0.995			
9.14	9.13	1.0009						
4.57	4.58	0.9988				Slope	0.998171	0.90 - 1.10
2.28	2.31	0.9888						
			Intercept	0.013029	± 0.5			

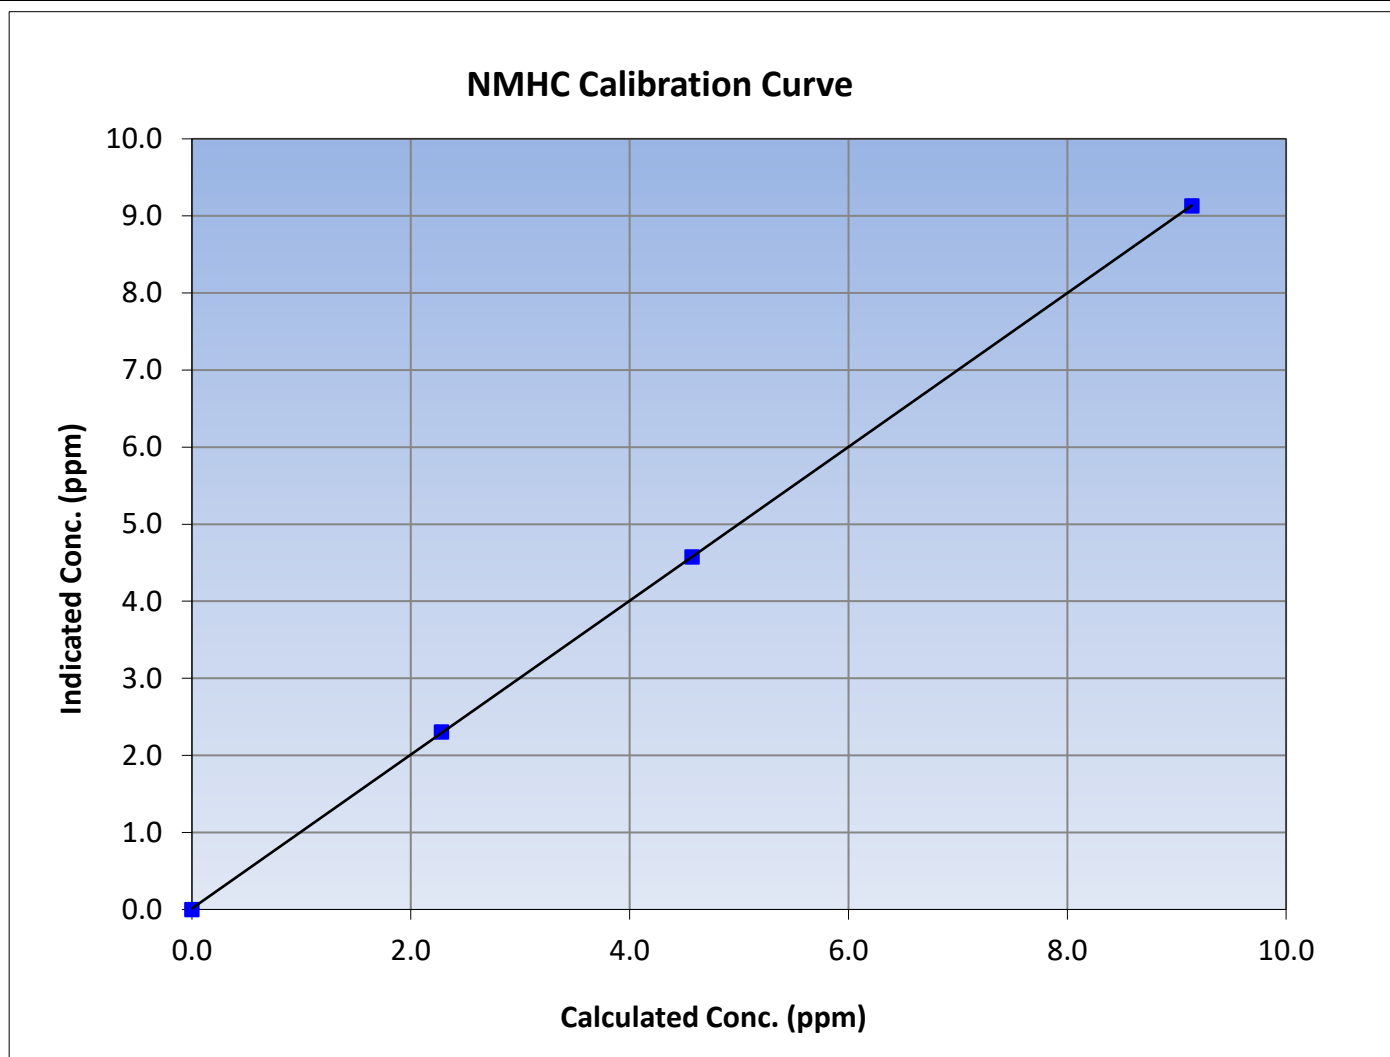

NMHC Calibration Plot

Date: January 3, 2023

Location: Conklin

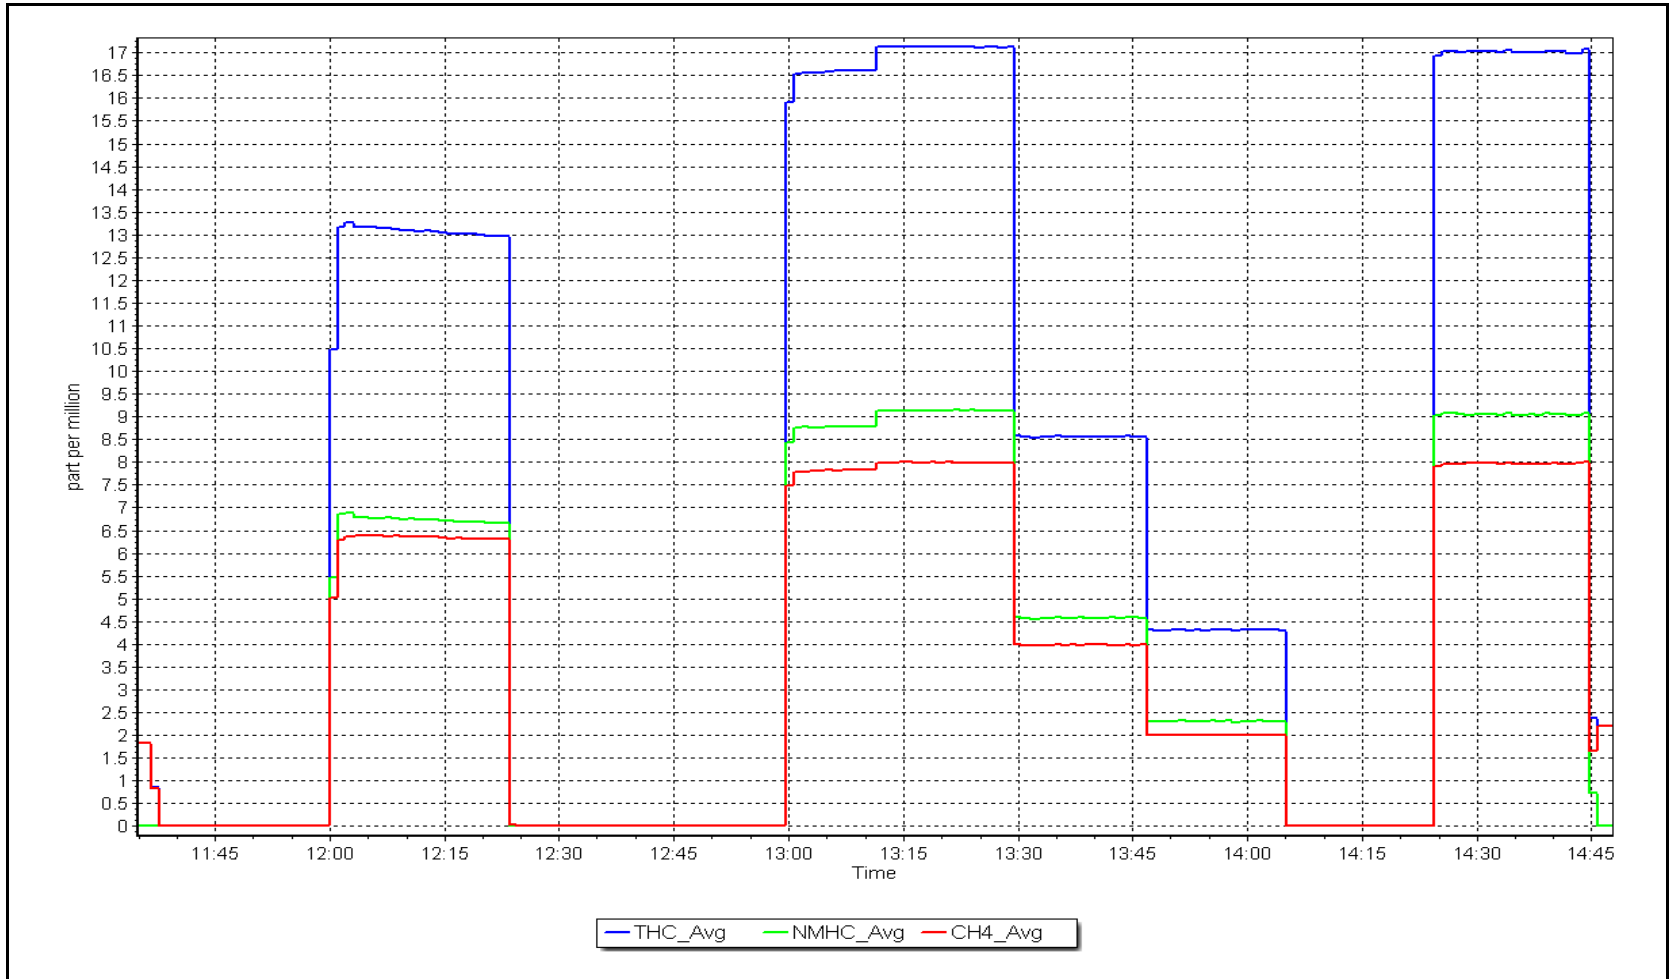



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Conklin	Station number:	AMS21
Calibration Date:	January 4, 2023	Last Cal Date:	January 3, 2023
Start time (MST):	9:40	End time (MST):	13:40
Reason:	Other: As Lefts		

Calibration Standards

Gas Cert Reference:	CC259455	Cal Gas Expiry Date:	January 5, 2025
CH ₄ Cal Gas Conc.	497.9 ppm	CH ₄ Equiv Conc.	1067.7 ppm
C ₃ H ₈ Cal Gas Conc.	207.2 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH ₄ Conc.	497.9 ppm	CH ₄ Equiv Conc.	1067.7 ppm
Removed C ₃ H ₈ Conc.	207.2 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	Teledyne API T700	Serial Number:	3810
ZAG make/model:	Teledyne API 701	Serial Number:	262

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	118148495
THC Range (ppm):	0 - 20 ppm	CH ₄ Range (ppm):	0 - 10 ppm
NMHC Range (ppm):	0 - 10 ppm		

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	1.81E-04	1.85E-04	NMHC SP Ratio:	4.48E-05
CH ₄ Retention time:	12.4	12.2	NMHC Peak Area:	203812
				196117

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero					
as found span					
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero					
high point					
second point					
third point					
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.2	17.13	17.03	1.006

Average Correction Factor					
Baseline Corr AF:	NA	Prev response	NA	*% change	NA
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* => +/-5% change initiates investigation	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero					
as found span					
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero					
high point					
second point					
third point					
as left zero	5000	0	0.00	0.00	----
as left span	4920	80.2	9.14	9.10	1.004
Average Correction Factor					
Baseline Corr AF:	NA	Prev response	NA	*% change	NA
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero					
as found span					
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero					
high point					
second point					
third point					
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.2	7.99	7.93	1.007
Average Correction Factor					
Baseline Corr AF:	NA	Prev response	NA	*% change	NA
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
THC Cal Slope:	0.986853	
THC Cal Offset:	-0.014487	
CH ₄ Cal Slope:	0.989953	
CH ₄ Cal Offset:	-0.012077	
NMHC Cal Slope:	0.984570	
NMHC Cal Offset:	-0.003608	


Notes: H2 leak at cylinder disrupted analyzer operation; leak fixed; as lefts points completed to verify analyzer operation.

Calibration Performed By: Denny Ray Estador

NMHC Calibration Plot

Date: January 4, 2023

Location: Conklin

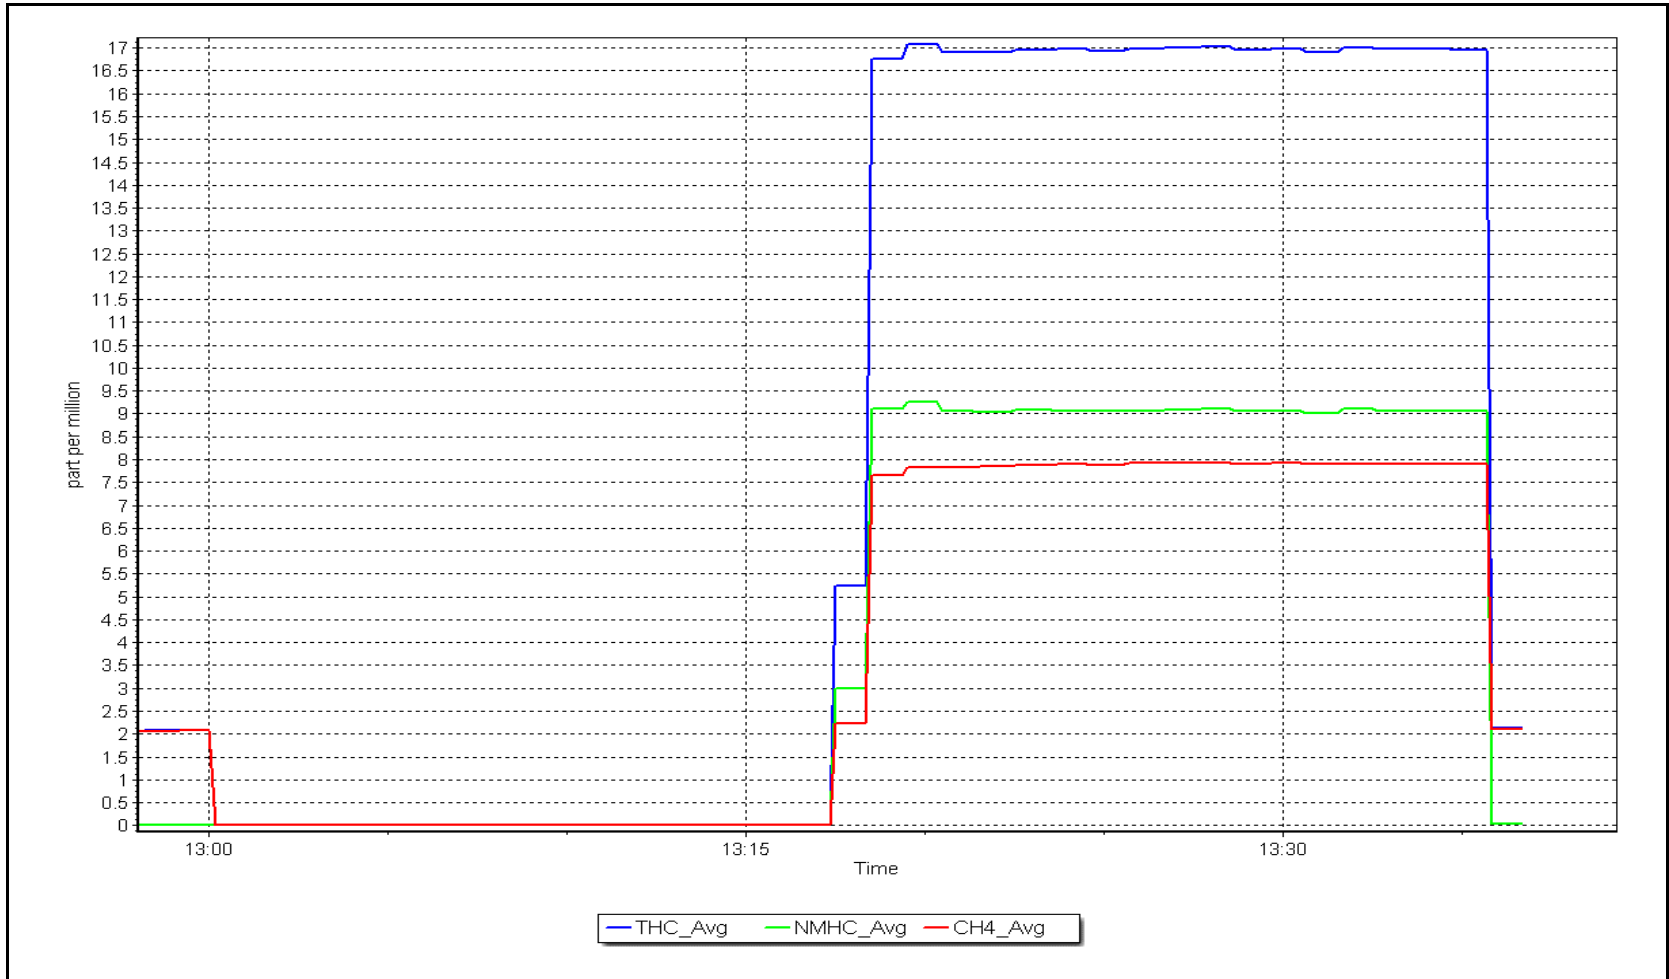



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Conklin
Calibration Date: January 17, 2023
Start time (MST): 9:28
Reason: Routine
Station number: AMS21
Last Cal Date: December 7, 2022
End time (MST): 13:30

Calibration Standards

NO Gas Cylinder #: T2Y1P1H
NOX Cal Gas Conc: 51.09 ppm
Removed Cylinder #: n/a
Removed Gas NOX Conc: 51.09 ppm
NOX gas Diff:
Calibrator Model: Teledyne API T750
ZAG make/model: Teledyne API T701
Cal Gas Expiry Date: December 11, 2023
NO Cal Gas Conc: 50.39 ppm
Removed Gas Exp Date: n/a
Removed Gas NO Conc: 50.39 ppm
NO gas Diff:
Serial Number: 282
Serial Number: 361

Analyzer Information

Analyzer make: Thermo 42i
NOX Range (ppb): 0 - 1000 ppb
Analyzer serial #: 1501663731

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.144	1.144	NO bkgnd or offset:	11.7	11.7
NOX coeff or slope:	1.001	1.001	NOX bkgnd or offset:	11.9	11.9
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	231.2	226.7

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	0.998786	1.001997
NO _x Cal Offset:	1.643904	1.704503
NO Cal Slope:	0.998353	0.998723
NO Cal Offset:	1.000893	1.321276
NO ₂ Cal Slope:	0.997669	0.999769
NO ₂ Cal Offset:	-1.114017	-0.317822



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-0.2	-0.2	0.0	----	----
as found span	4921	79.4	811.2	800.1	11.1	812.0	799.0	13.5	0.9991	1.0014
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.0	0.0	0.0	----	----
high point	4921	79.4	811.2	800.1	11.1	813.8	799.9	13.9	0.9969	1.0003
second point	4960	39.7	405.7	400.1	5.6	408.8	401.2	7.6	0.9924	0.9973
third point	4980	19.8	202.3	199.6	2.8	206.3	202.2	4.1	0.9807	0.9869
as left zero	5000	0.0	0.0	0.0	0.0	0.0	0.0	0.0	----	----
as left span	4921	79.4	811.2	390.7	420.5	812.0	392.2	419.8	0.9991	0.9962
Average Correction Factor									0.9900	0.9948

Corrected As found	NO _x = 812.2 ppb	NO = 799.2 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = 0.0%
Previous Response	NO _x = 811.9 ppb	NO = 799.8 ppb		*Percent Change	NO = -0.1%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI: ;

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	798.8	389.4	420.5	420.2	1.0007	99.9%
2nd GPT point (200 ppb O3)	798.8	589.6	220.3	220.0	1.0014	99.9%
3rd GPT point (100 ppb O3)	798.8	695.9	114.0	113.2	1.0072	99.3%
Average Correction Factor					1.0031	99.7%

Notes:

No adjustments required.

Calibration Performed By:

Denny Ray Estador



Wood Buffalo Environmental Association

NO_x Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 7, 2022
Station Name:	Conklin	Station Number:	AMS21
Start Time (MST):	9:28	End Time (MST):	13:30
Analyzer make:	Thermo 42i	Analyzer serial #:	1501663731

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20	
811.2	813.8	0.9969			
405.7	408.8	0.9924			
202.3	206.3	0.9807			
			Correlation Coefficient	0.999980	≥0.995
			Slope	1.001997	0.90 - 1.10
			Intercept	1.704503	+/-20

NO_x Calibration Curve

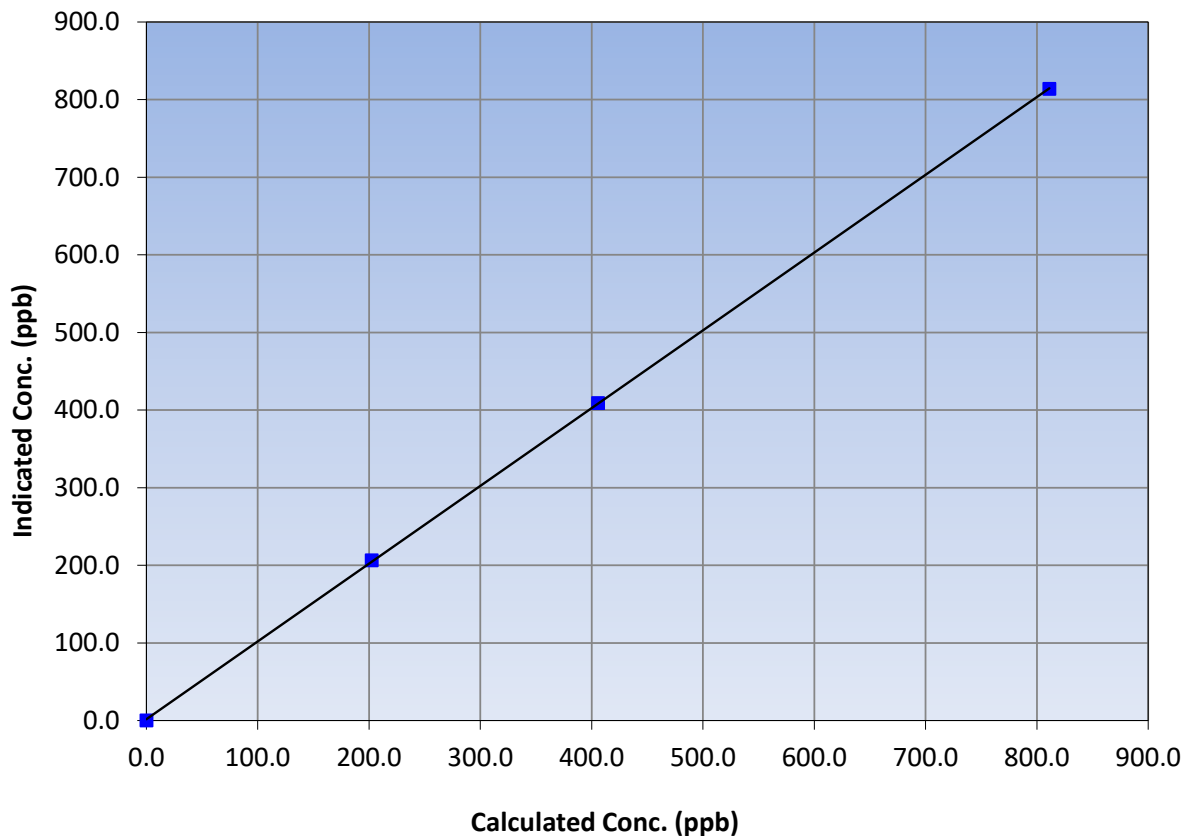



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 7, 2022
Station Name:	Conklin	Station Number:	AMS21
Start Time (MST):	9:28	End Time (MST):	13:30
Analyzer make:	Thermo 42i	Analyzer serial #:	1501663731

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.0	----	Correlation Coefficient	≥0.995	
800.1	799.9	1.0003			
400.1	401.2	0.9973			
199.6	202.2	0.9869			
			Slope	0.998723	0.90 - 1.10
			Intercept	1.321276	+/-20

NO Calibration Curve

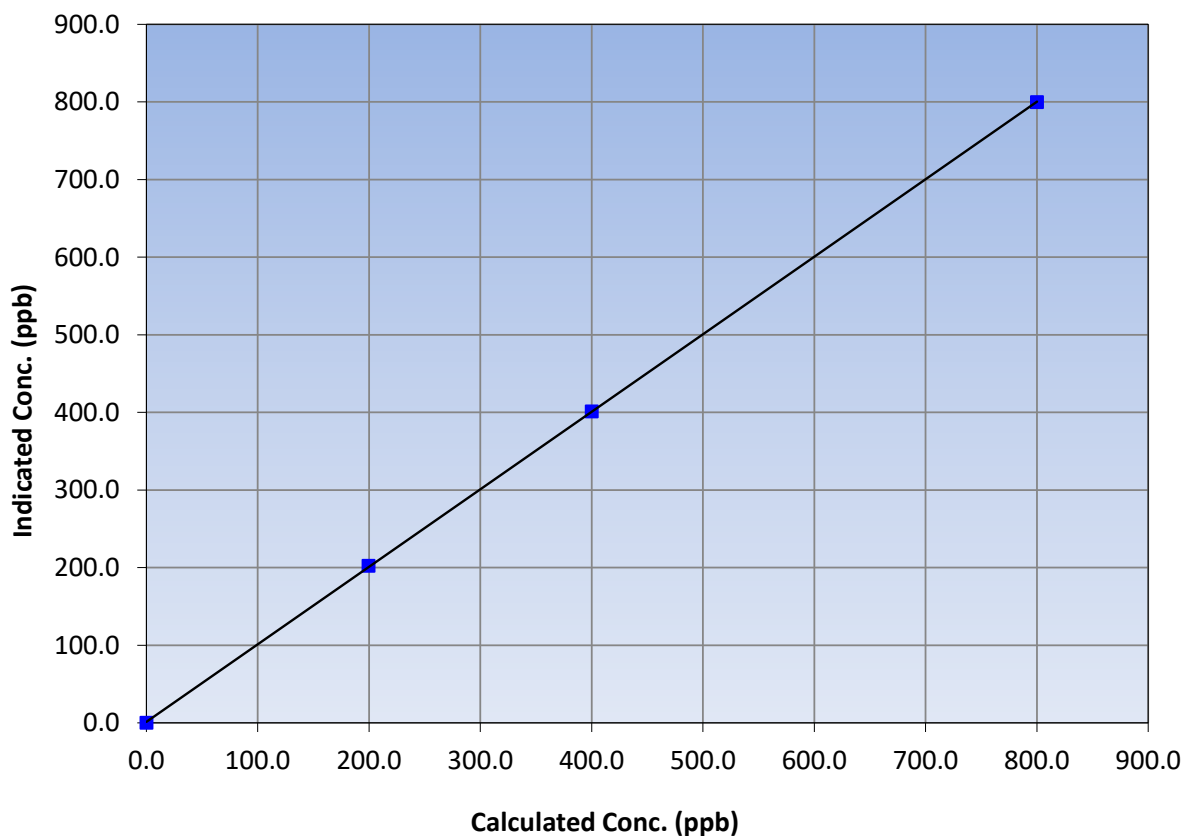



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 7, 2022
Station Name:	Conklin	Station Number:	AMS21
Start Time (MST):	9:28	End Time (MST):	13:30
Analyzer make:	Thermo 42i	Analyzer serial #:	1501663731

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
420.5	420.2	1.0007		
220.3	220.0	1.0014		
114.0	113.2	1.0072		


NO₂ Calibration Curve

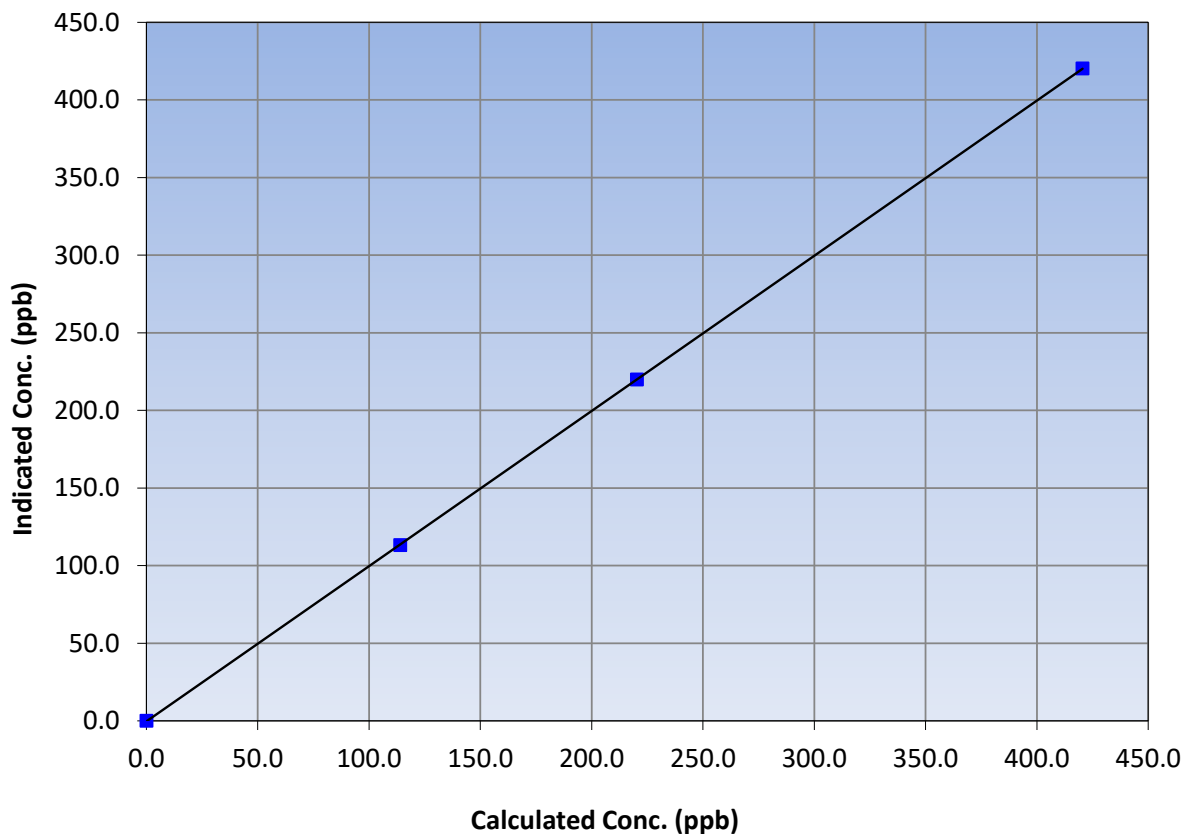

NO_x Calibration Plot

Date: January 17, 2023

Location: Conklin

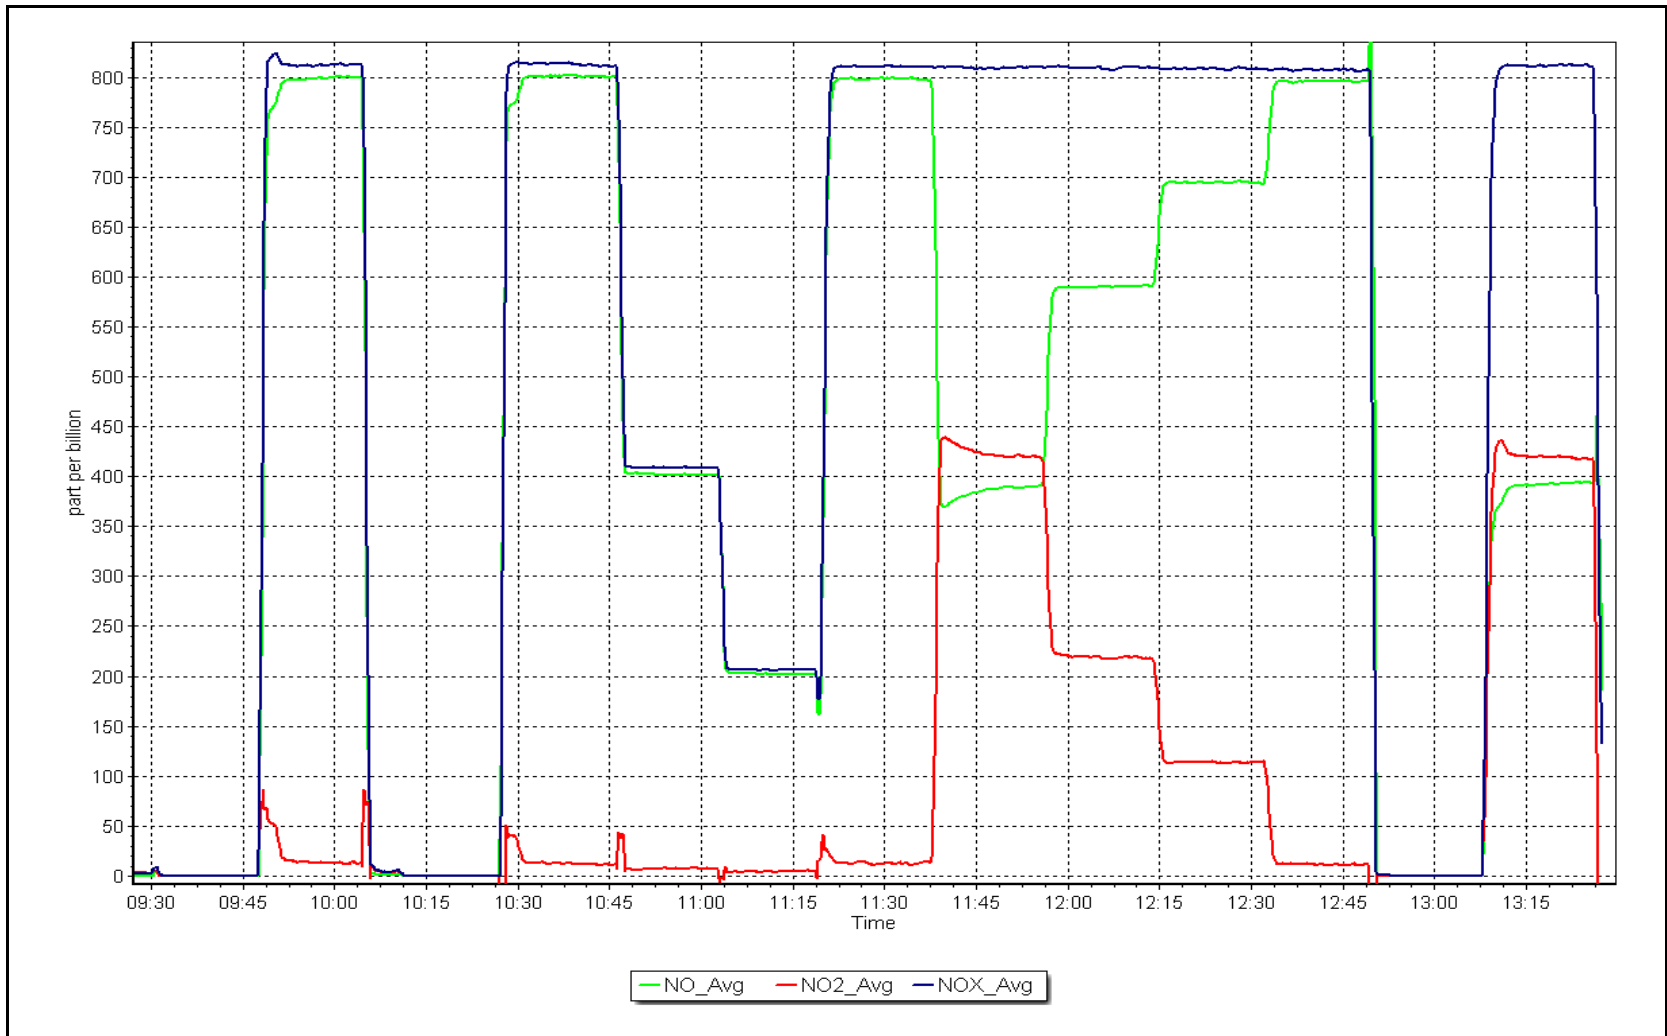



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 6, 2022
Station Name:	Conklin	Station Number:	AMS21
Start Time (MST):	9:32	End Time (MST):	12:50
Analyzer make:	Thermo 49i	Analyzer serial #:	1501663734

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	-0.3	----	Correlation Coefficient	0.999991	≥0.995
400.0	399.0	1.0025			
200.0	200.3	0.9985	Slope	0.997857	0.90 - 1.10
100.0	100.3	0.9970			
			Intercept	0.200000	+/- 5

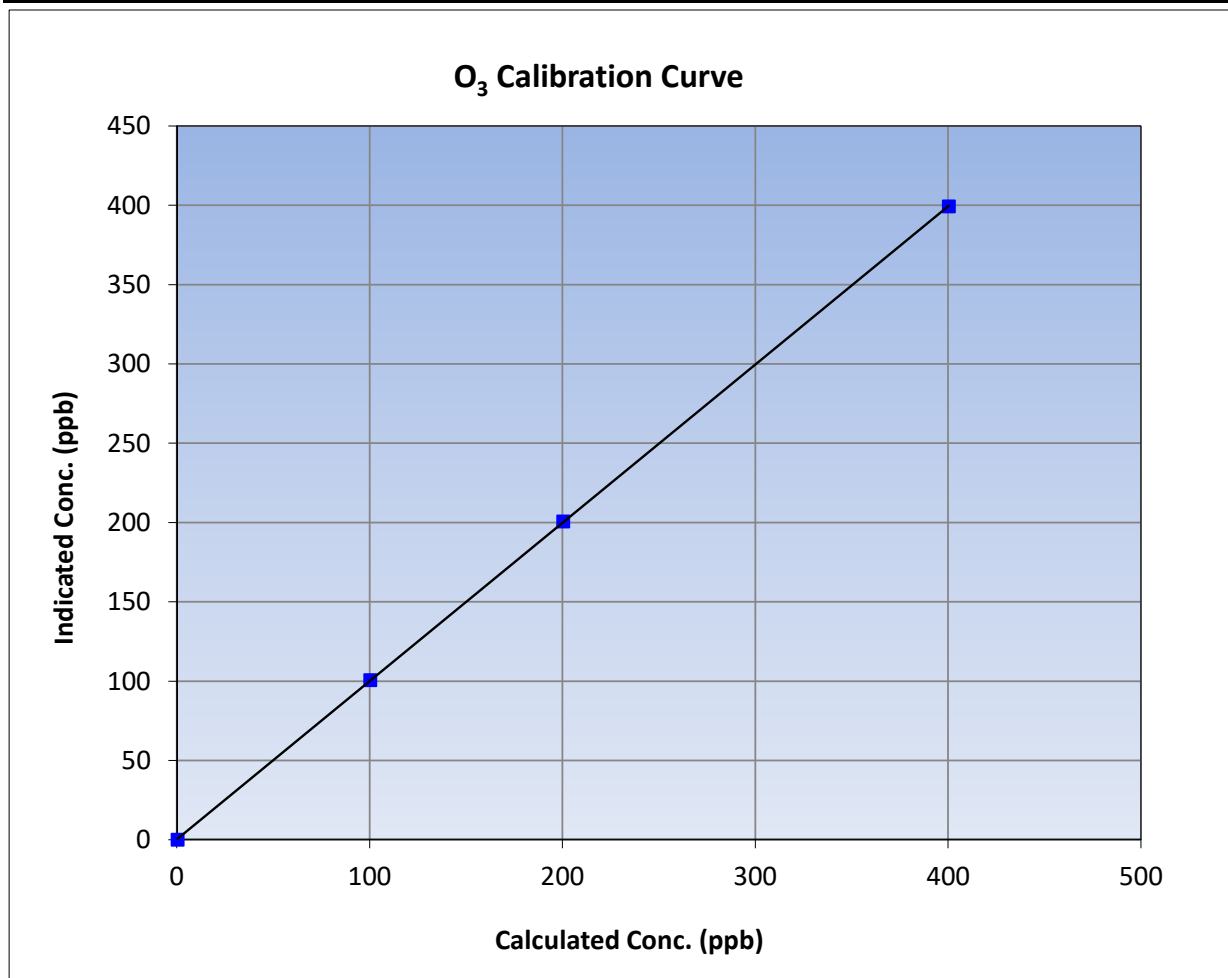

O₃ Calibration Plot

Date: January 20, 2023

Location: Conklin

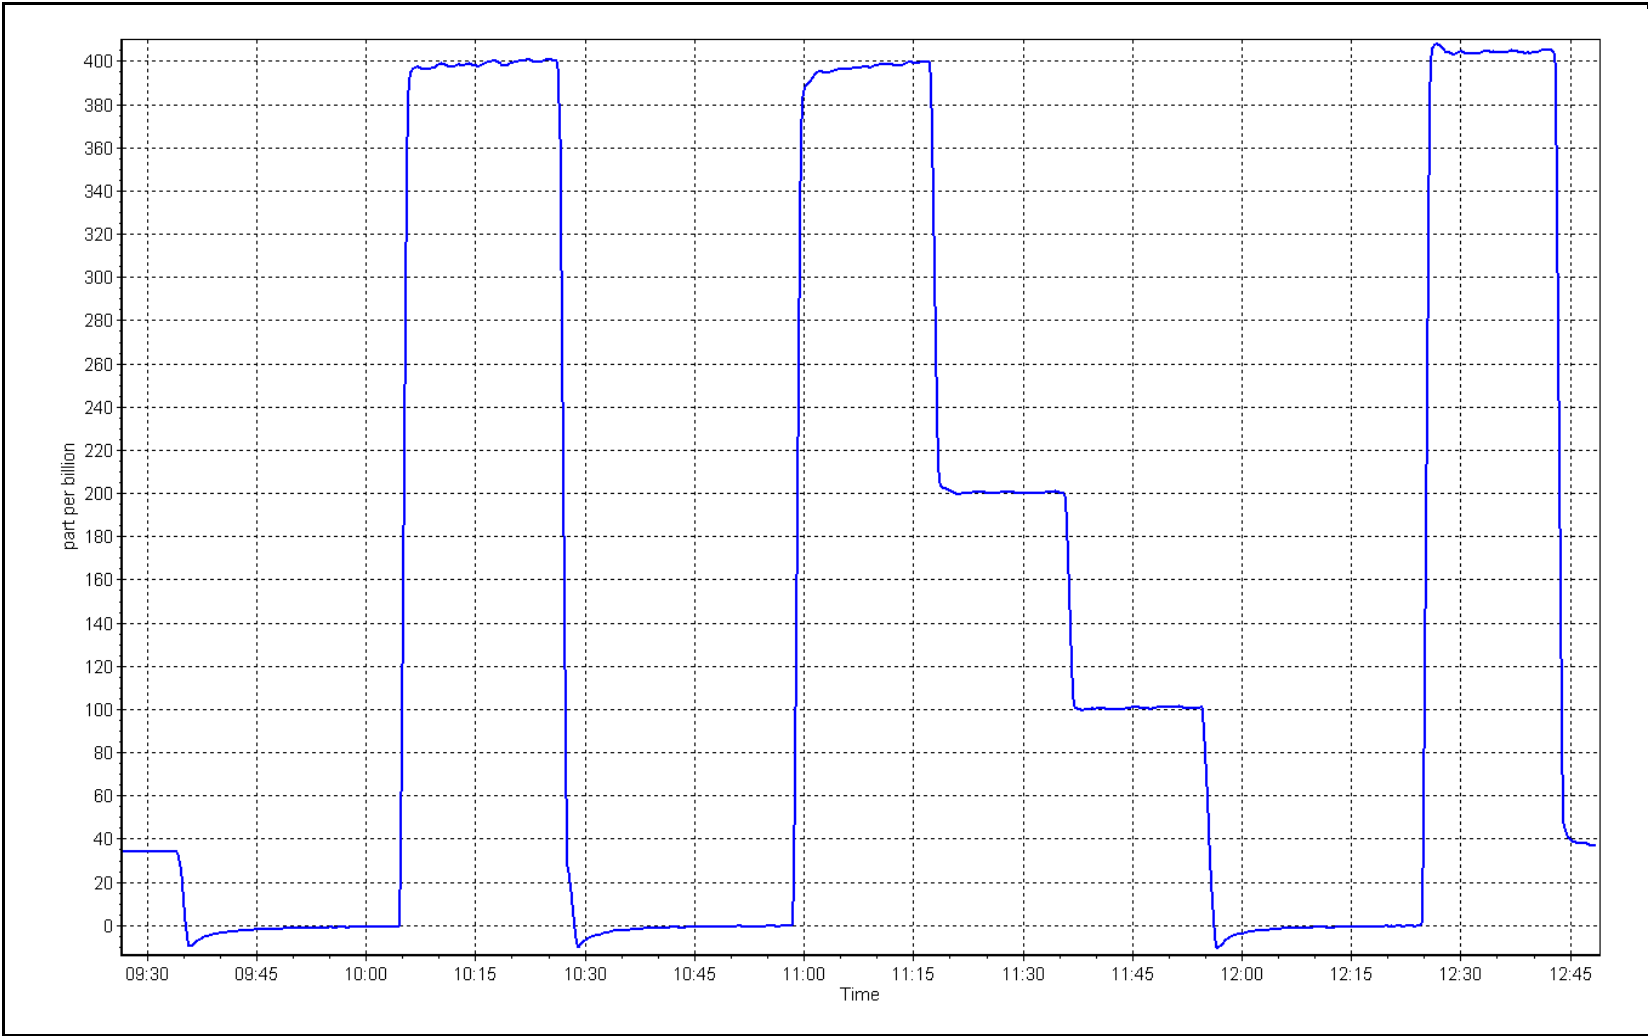



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Conklin Station number: AMS 21
Calibration Date: January 4, 2023 Last Cal Date: December 22, 2022
Start time (MST): 11:15 End time (MST): 11:50

Analyzer Make: API T640 S/N: 1547
Particulate Fraction: PM2.5

Flow Meter Make/Model: DeltaCal S/N: 954
Temp/RH standard: DeltaCal S/N: 954

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-8	-7.6	-8	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	709.4	703.9	709.4	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5.02	5.13	5.02	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of Check: January 4, 2023 Last Cal Date: December 22, 2022
PM w/o HEPA: 7.3 PM w/ HEPA: 0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test		-----		<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: N/A
Disposable Filter Changed: N/A

Annual Maintenance

Date Sample Tube Cleaned: N/A
Date RH/T Sensor Cleaned: N/A

Notes:

Recently installed last December 2022, first monthly calibration test.

Calibration by: Denny Ray Estador



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

**AMS22
JANVIER
JANUARY 2023**

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Janvier	Station number:	AMS 22
Calibration Date:	January 17, 2023	Last Cal Date:	December 6, 2022
Start time (MST):	12:10	End time (MST):	16:51
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	50.11	ppm	Cal Gas Exp Date:	January 18, 2029
Cal Gas Cylinder #:	CC281519			
Removed Cal Gas Conc:	50.11	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	3806
ZAG Make/Model:	Teledyne API T701		Serial Number:	4890

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	1152430006
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.000878	1.000335	Backgd or Offset:	19.3	19.2
Calibration intercept:	0.164277	0.604356	Coeff or Slope:	1.016	1.007

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4920	79.8	799.8	806.7	0.991
as found 2nd point	4960	39.9	399.9	404.5	0.989
as found 3rd point	4980	20.0	200.4	202.8	0.988
new cylinder response					
calibrator zero	5000	0.0	0.0	0.2	----
high point	4920	79.8	799.8	800.2	0.999
second point	4960	39.9	399.9	401.6	0.996
third point	4980	20.0	200.4	201.0	0.997
as left zero	5000	0.0	0.0	0.4	----
as left span	4920	79.8	799.8	802.4	0.997
Average Correction Factor					0.997

Baseline Corr As found:	806.60	Previous response	800.65	*% change	0.7%
Baseline Corr 2nd AF pt:	404.40	AF Slope:	1.008439	AF Intercept:	0.542651
Baseline Corr 3rd AF pt:	202.70	AF Correlation:	0.999998		

* = > +/-5% change initiates investigation

Notes: Inlet filter changed after as founds. Adjusted span only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 6, 2022
Station Name:	Janvier	Station Number:	AMS 22
Start Time (MST):	12:10	End Time (MST):	16:51
Analyzer make:	Thermo 43i	Analyzer serial #:	1152430006

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.2	----	Correlation Coefficient	0.999996	
799.8	800.2	0.9995			≥0.995
399.9	401.6	0.9957	Slope	1.000335	
200.4	201.0	0.9972			0.90 - 1.10
			Intercept	0.604356	+/-30

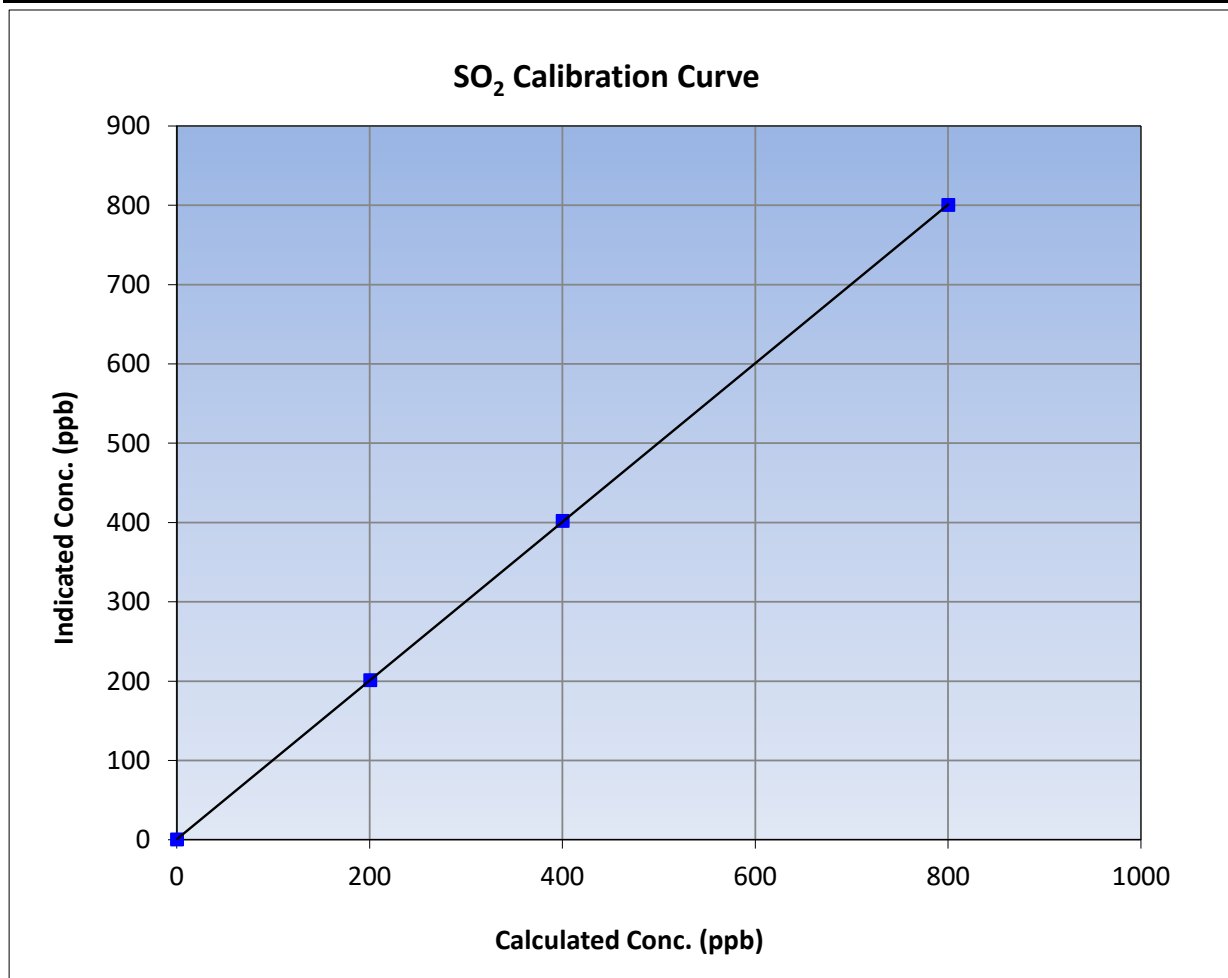

SO2 Calibration Plot

Date: January 17, 2023

Location: Janvier

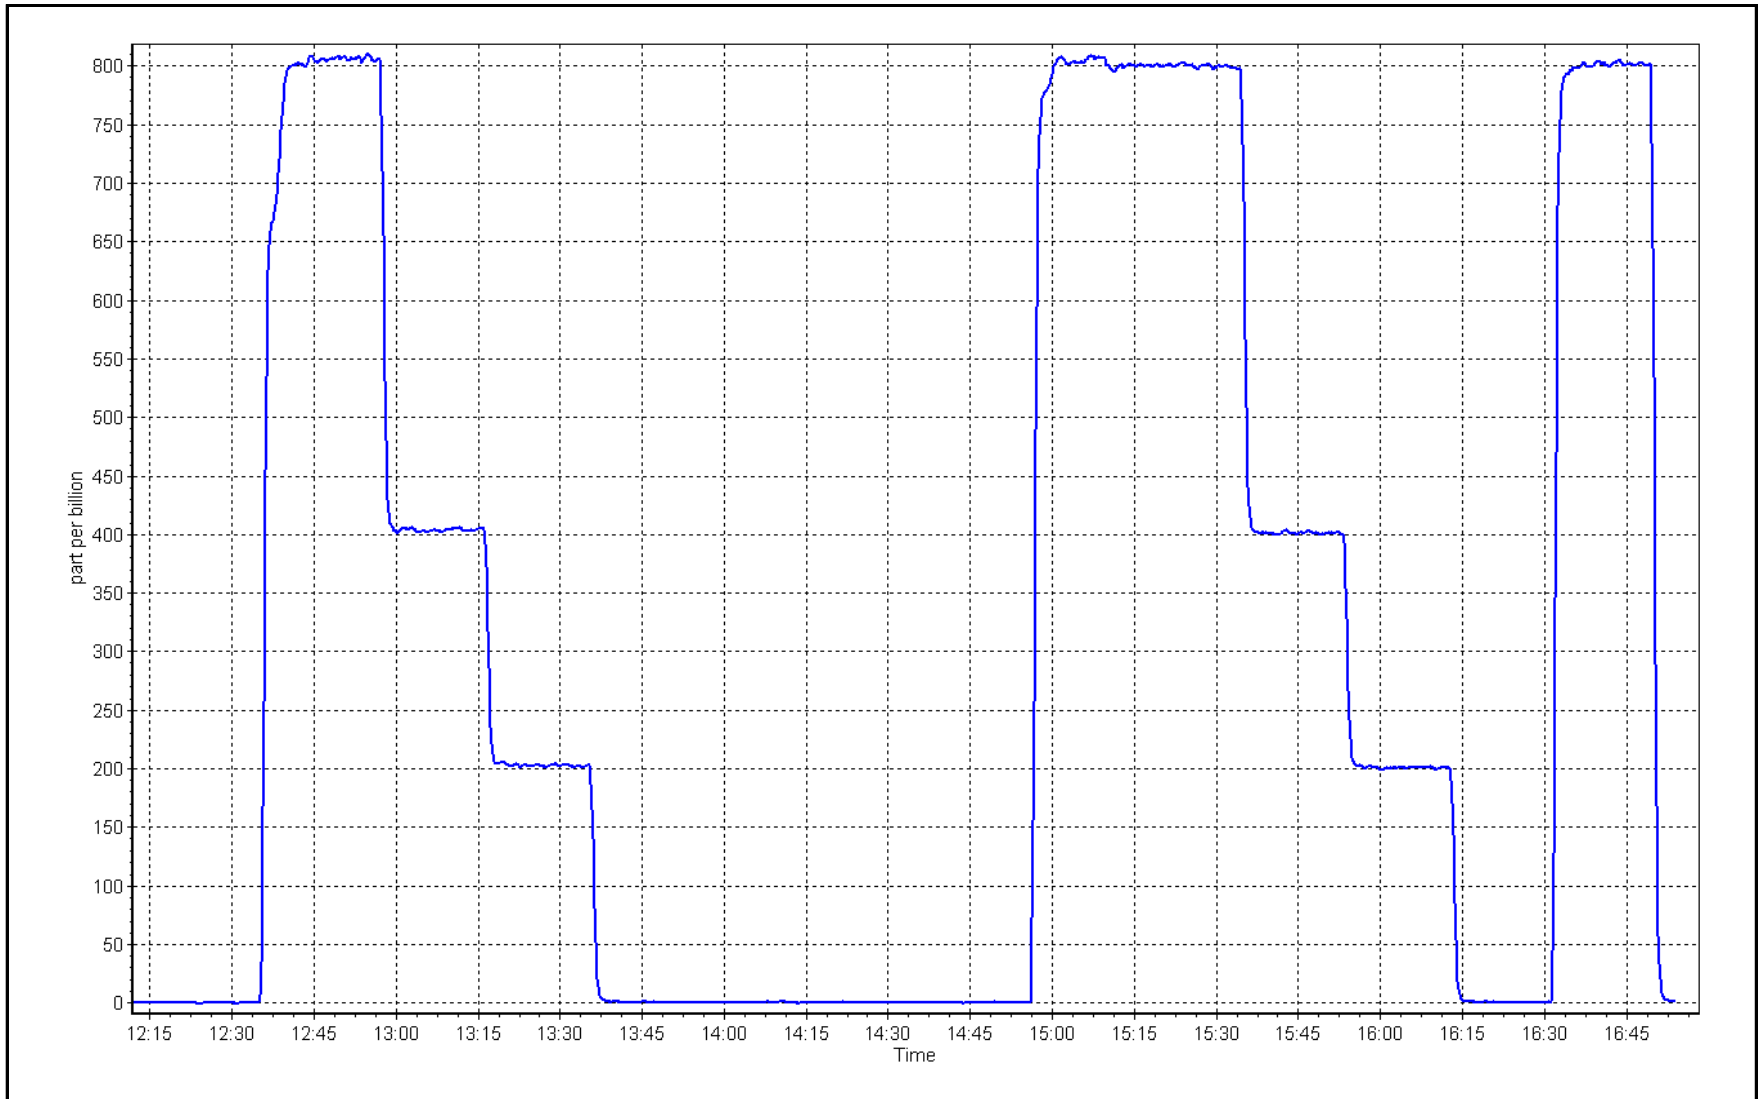



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name:	Janvier	Station number:	AMS22
Calibration Date:	January 20, 2023	Last Cal Date:	December 15, 2022
Start time (MST):	10:30	End time (MST):	15:45
Reason:	Maintenance		

Calibration Standards

Cal Gas Concentration:	5.03	ppm	Cal Gas Exp Date:	April 16, 2022
Cal Gas Cylinder #:	DT0018680			
Removed Cal Gas Conc:	5.03	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700		Serial Number:	3806
ZAG Make/Model:	Teledyne API T701		Serial Number:	4890

Analyzer Information

Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1151680031
Converter make:	CDN-101	Converter serial #:	587
Analyzer Range	0 - 100 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.999078	1.005365	Backgd or Offset:	3.39	3.42
Calibration intercept:	0.320986	0.000881	Coeff or Slope:	1.223	1.239

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero					
as found span					
as found 2nd point					
as found 3rd point					
new cylinder response					

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.2	----
high point	4920	79.5	80.0	80.4	0.995
second point	4960	39.8	40.0	40.5	0.989
third point	4980	19.9	20.0	19.7	1.016
as left zero	5000	0.0	0.0	0.2	----
as left span	4920	79.5	80.0	79.9	1.001
SO2 Scrubber Check	4920	79.8	798.0	0.1	----
Date of last scrubber change:				Ave Corr Factor	1.000
Date of last converter efficiency test:				efficiency	

Baseline Corr As found:	NA	Prev response:	NA	*% change:	NA
Baseline Corr 2nd AF pt:	NA	AF Slope:	NA	AF Intercept:	NA
Baseline Corr 3rd AF pt:	NA	AF Correlation:	NA		

* = > +/-5% change initiates investigation

Notes: No as founds completed because of a converter failure. Replaced the TRS converter. Changed out the inlet filter. Scrubber check passed. Increased the converter temperature to 840C. Adjusted span only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	December 15, 2022
Station Name:	Janvier	Station Number:	AMS22
Start Time (MST):	10:30	End Time (MST):	15:45
Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1151680031

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999920	≥0.995
80.0	80.4	0.9948			
40.0	40.5	0.9887	Slope	1.005365	0.90 - 1.10
20.0	19.7	1.0162			
			Intercept	0.000881	+/-3

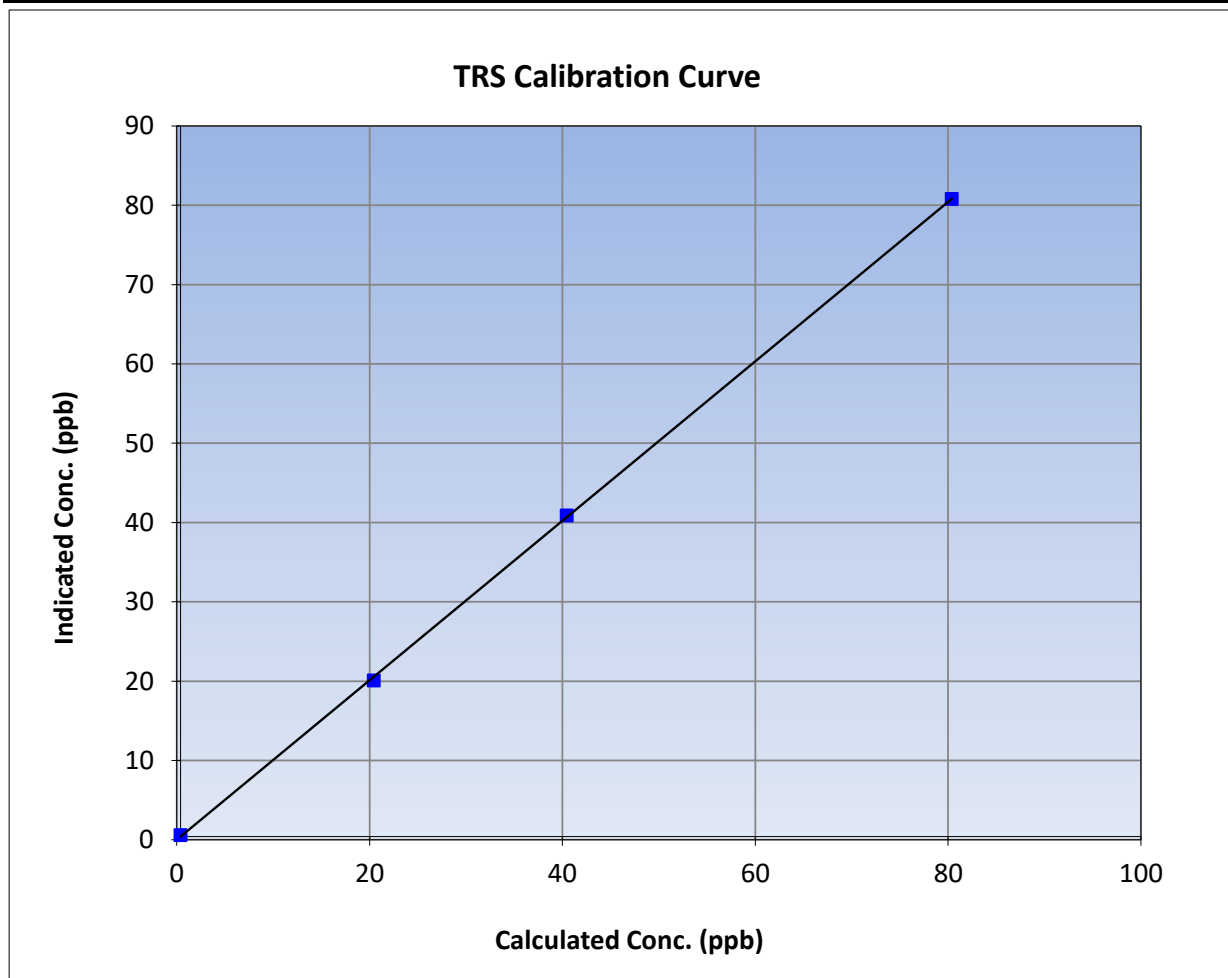

TRS Calibration Plot

Date: January 20, 2023

Location: Janvier

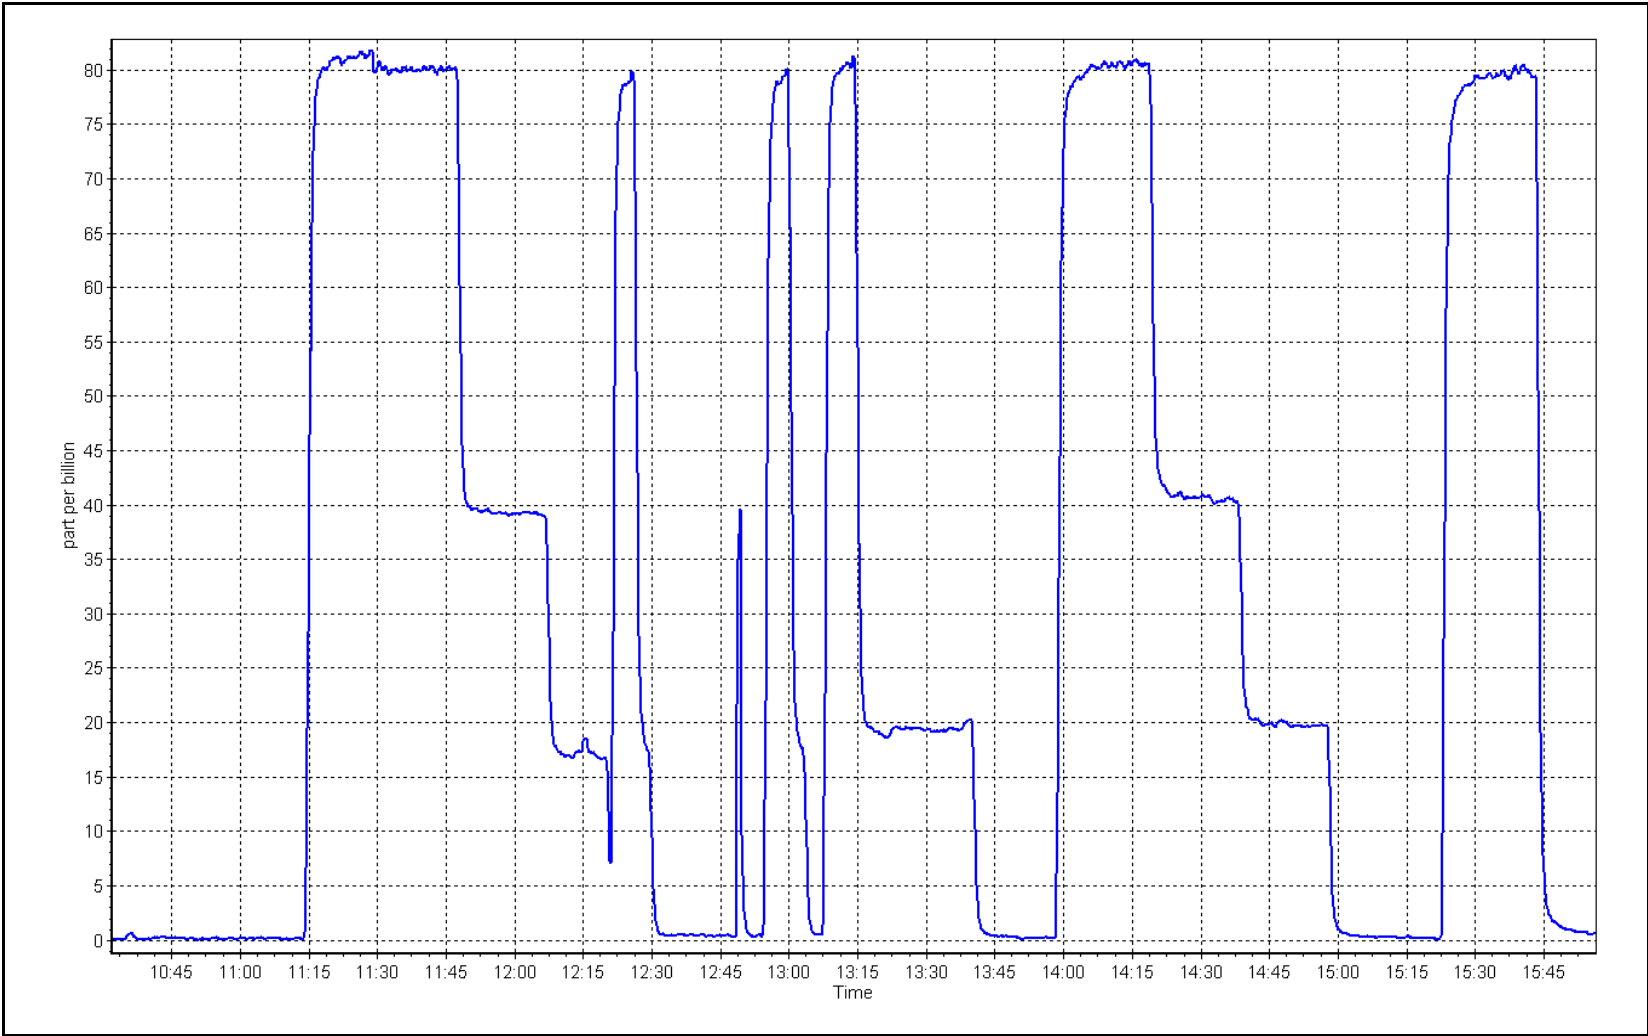



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Janvier	Station number:	AMS 22
Calibration Date:	January 17, 2023	Last Cal Date:	December 6, 2022
Start time (MST):	12:10	End time (MST):	16:51
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC281519	Cal Gas Expiry Date:	January 18, 2029
CH ₄ Cal Gas Conc.	502.8 ppm	CH ₄ Equiv Conc.	1075.9 ppm
C ₃ H ₈ Cal Gas Conc.	208.4 ppm		
Removed Gas Cert:	N/A	Removed Gas Expiry:	N/A
Removed CH ₄ Conc.	502.8 ppm	CH ₄ Equiv Conc.	1075.9 ppm
Removed C ₃ H ₈ Conc.	208.4 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	Teledyne API 700	Serial Number:	3806
ZAG make/model:	Teledyne API 701	Serial Number:	4890

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1172750023
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	2.180E-04	2.180E-04	NMHC SP Ratio:	4.62E-05
CH ₄ Retention time:	12.80	13.00	NMHC Peak Area:	198163
				195272

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	79.8	17.17	17.34	0.990
as found 2nd point	4960	39.9	8.59	8.63	0.995
as found 3rd point	4980	20.0	4.30	4.32	0.996
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	79.8	17.17	17.14	1.002
second point	4960	39.9	8.59	8.52	1.008
third point	4980	20.0	4.30	4.22	1.020
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	79.8	17.17	17.11	1.004
Average Correction Factor					1.010
Baseline Corr AF:	17.34	Prev response	17.16	*% change	1.0%
Baseline Corr 2nd AF:	8.6	AF Slope:	1.009988	AF Intercept:	-0.017439
Baseline Corr 3rd AF:	4.3	AF Correlation:	0.999993	* => +/-5% change initiates investigation	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4920	79.8	9.15	9.17	0.997
as found 2nd point	4960	39.9	4.57	4.59	0.997
as found 3rd point	4980	20	2.29	2.28	1.005
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4920	79.8	9.15	9.11	1.004
second point	4960	39.9	4.57	4.53	1.010
third point	4980	20.0	2.29	2.25	1.021
as left zero	5000	0	0.00	0.00	----
as left span	4920	79.8	9.15	9.10	1.006
Average Correction Factor					1.011
Baseline Corr AF:	9.17	Prev response	9.16	*% change	0.1%
Baseline Corr 2nd AF:	4.6	AF Slope:	1.003390	AF Intercept:	-0.006039
Baseline Corr 3rd AF:	2.3	AF Correlation:	0.999995	* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	79.8	8.03	8.16	0.984
as found 2nd point	4960	39.9	4.01	4.04	0.994
as found 3rd point	4980	20.0	2.01	2.04	0.986
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	79.8	8.03	8.03	1.000
second point	4960	39.9	4.01	3.99	1.005
third point	4980	20.0	2.01	1.97	1.020
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	79.8	8.03	8.01	1.001
Average Correction Factor					1.008
Baseline Corr AF:	8.16	Prev response	8.00	*% change	2.0%
Baseline Corr 2nd AF:	4.04	AF Slope:	1.016305	AF Intercept:	-0.010190
Baseline Corr 3rd AF:	2.04	AF Correlation:	0.999967	* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	0.999736	0.999594
THC Cal Offset:	-0.008390	-0.041578
CH ₄ Cal Slope:	0.997864	1.001935
CH ₄ Cal Offset:	-0.011155	-0.020955
NMHC Cal Slope:	1.001366	0.997466
NMHC Cal Offset:	0.002565	-0.020822

Notes: Changed the inlet filter after as founds. Changed out the N2 and H2 cylinders. Adjusted span only.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 6, 2022
Station Name:	Janvier	Station Number:	AMS 22
Start Time (MST):	12:10	End Time (MST):	16:51
Analyzer make:	Thermo 55i	Analyzer serial #:	1172750023

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999973	≥ 0.995			
17.17	17.14	1.0016						
8.59	8.52	1.0076				Slope	0.999594	0.90 - 1.10
4.30	4.22	1.0203						
			Intercept	-0.041578	± 0.5			

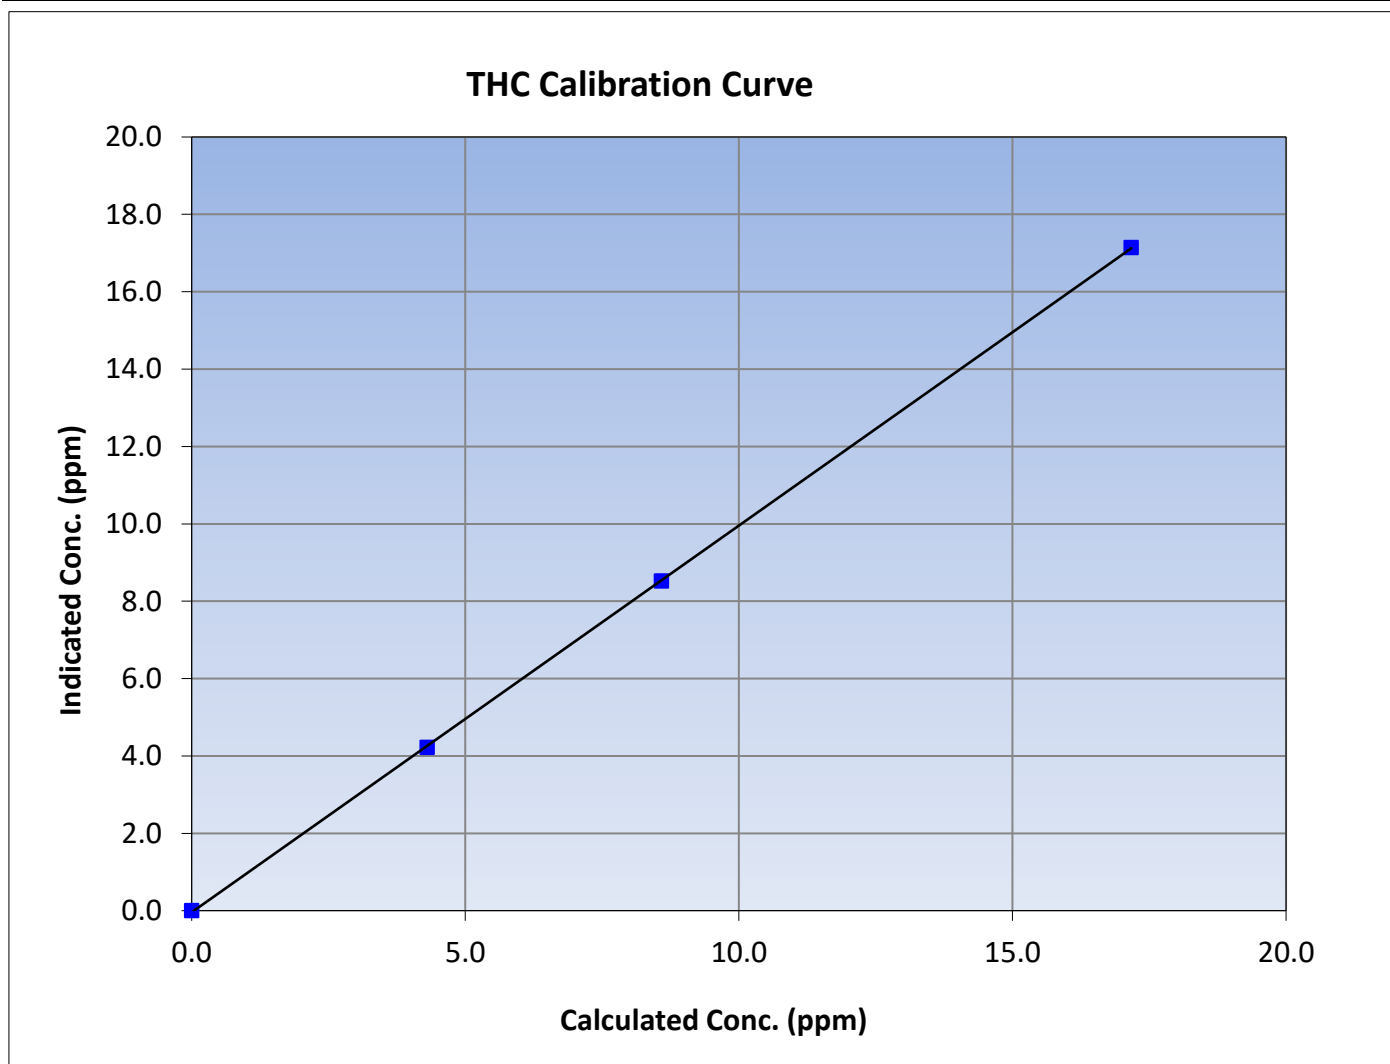



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 6, 2022
Station Name:	Janvier	Station Number:	AMS 22
Start Time (MST):	12:10	End Time (MST):	16:51
Analyzer make:	Thermo 55i	Analyzer serial #:	1172750023

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999968	≥ 0.995			
8.03	8.03	0.9995						
4.01	3.99	1.0051				Slope	1.001935	0.90 - 1.10
2.01	1.97	1.0204						
			Intercept	-0.020955	± 0.5			

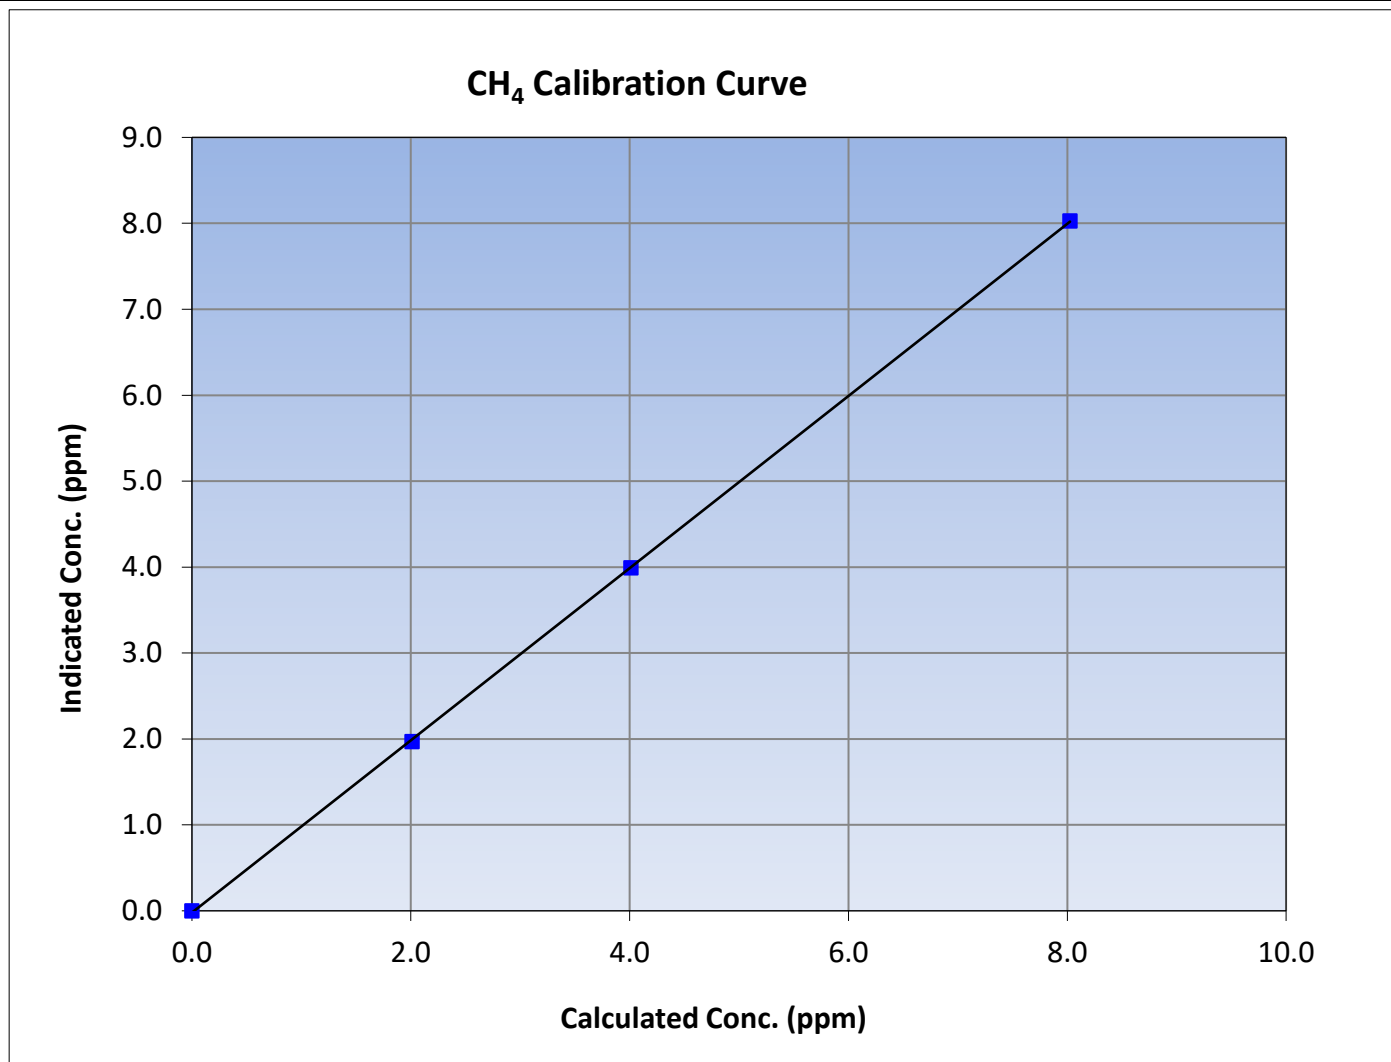



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 17, 2023	Previous Calibration:	December 6, 2022
Station Name:	Janvier	Station Number:	AMS 22
Start Time (MST):	12:10	End Time (MST):	16:51
Analyzer make:	Thermo 55i	Analyzer serial #:	1172750023

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999976	≥ 0.995			
9.15	9.11	1.0036						
4.57	4.53	1.0098				Slope	0.997466	0.90 - 1.10
2.29	2.25	1.0207						
			Intercept	-0.020822	± 0.5			

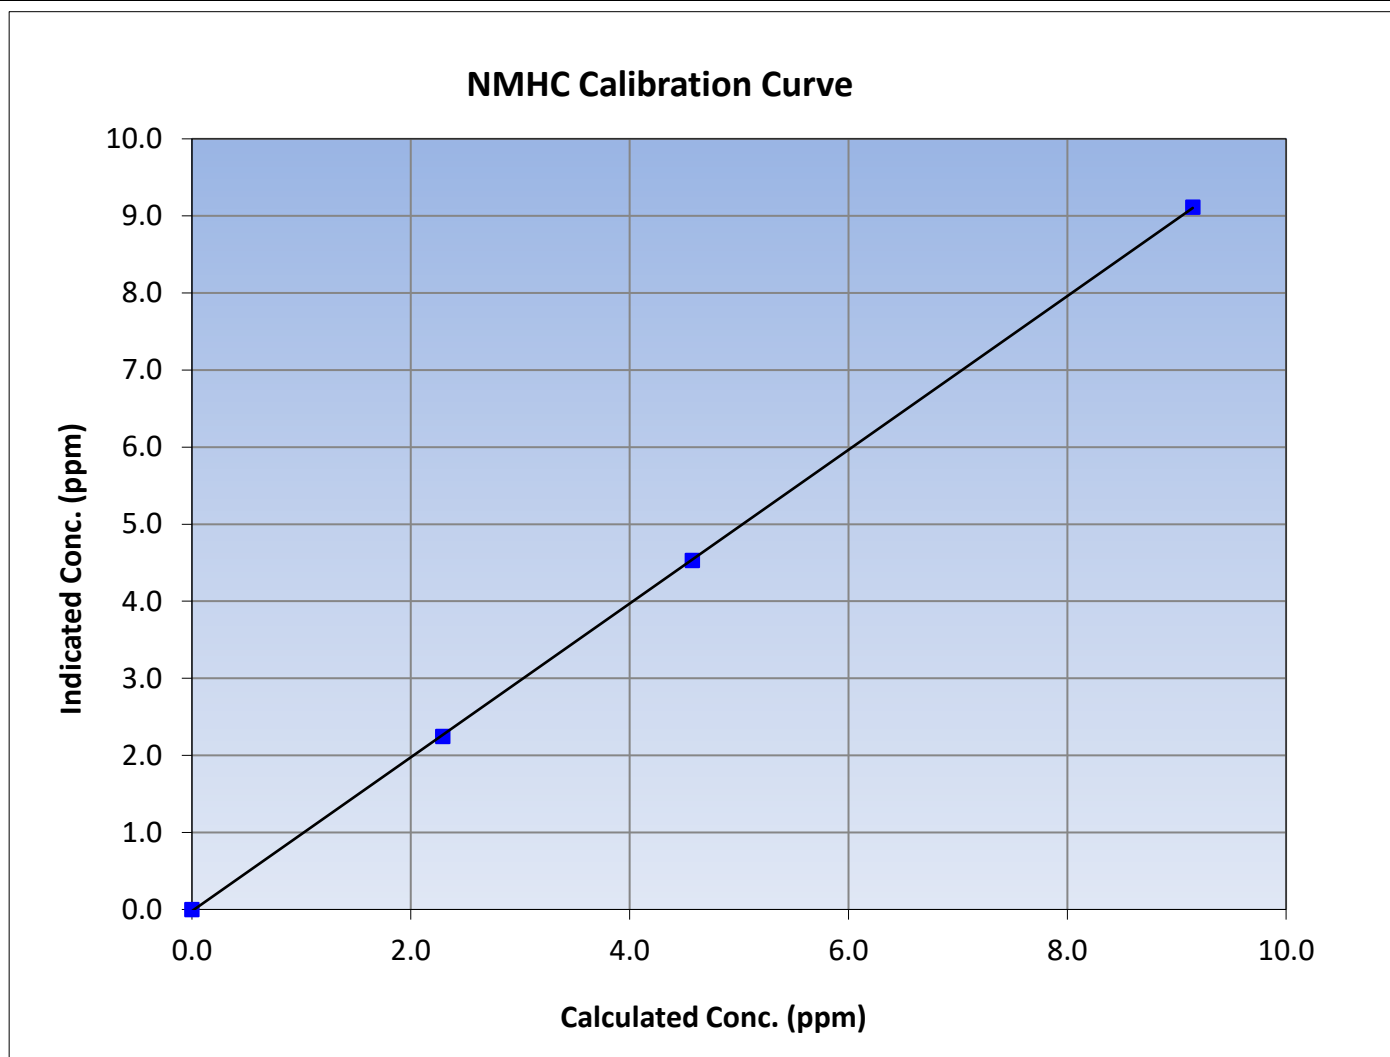

NMHC Calibration Plot

Date: January 17, 2023

Location: Janvier





Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Janvier Station number: AMS 22
Calibration Date: January 26, 2023 Last Cal Date: December 1, 2022
Start time (MST): 12:16 End time (MST): 17:52
Reason: Routine

Calibration Standards

NO Gas Cylinder #: CC424183 Cal Gas Expiry Date: April 16, 2023
NOX Cal Gas Conc: 48.60 ppm NO Cal Gas Conc: 48.60 ppm
Removed Cylinder #: NA Removed Gas Exp Date: NA
Removed Gas NOX Conc: 48.60 ppm Removed Gas NO Conc: 48.60 ppm
NOX gas Diff: NO gas Diff:
Calibrator Model: Teledyne API T700 Serial Number: 3806
ZAG make/model: Teledyne API T701 Serial Number: 4890

Analyzer Information

Analyzer make: Teledyne API T200 Analyzer serial #: 7117
NOX Range (ppb): 0 - 1000 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.018	1.015	NO bkgnd or offset:	0.0	-0.3
NOX coeff or slope:	1.007	1.004	NOX bkgnd or offset:	0.3	0.4
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	5.0	5.0

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.003274	1.004514
NO _x Cal Offset:	0.187776	-0.271695
NO Cal Slope:	1.003586	1.003357
NO Cal Offset:	-0.871493	-0.891348
NO ₂ Cal Slope:	1.001086	0.999938
NO ₂ Cal Offset:	0.486335	0.560426



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.9	-0.2	1.0	----	----
as found span	4918	82.3	799.9	799.9	0.0	795.6	791.7	4.0	1.0054	1.0104
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	-0.1	0.0	-0.1	----	----
high point	4918	82.3	799.9	799.9	0.0	803.6	802.2	1.5	0.9954	0.9971
second point	4959	41.2	400.4	400.4	0.0	401.1	400.3	0.9	0.9984	1.0004
third point	4980	20.6	200.2	200.2	0.0	201.2	199.2	2.0	0.9951	1.0051
as left zero	5000	0.0	0.0	0.0	0.0	0.0	0.2	-0.2	----	----
as left span	4918	82.3	799.9	411.7	388.2	796.0	409.1	386.9	1.0049	1.0064
Average Correction Factor									0.9963	1.0009

Corrected As found	NO _x = 794.7 ppb	NO = 791.9 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -1.0%	
Previous Response	NO _x = 802.7 ppb	NO = 801.9 ppb		*Percent Change	NO = -1.3%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO ₂)						
as found GPT point (200 ppb NO ₂)						
as found GPT point (100 ppb NO ₂)						
1st GPT point (400 ppb O ₃)	797.7	409.5	388.2	388.5	0.9992	100.1%
2nd GPT point (200 ppb O ₃)	797.7	605.4	192.3	192.9	0.9969	100.3%
3rd GPT point (100 ppb O ₃)	797.7	700.8	96.9	98.3	0.9858	101.4%
Average Correction Factor					0.9940	100.6%

Notes: Changed the inlet filter after as founds. Changed out the Purafil and charcoal scrubber canisters on the ZAG. Adjusted both zero and span.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

NO_x Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	December 1, 2022
Station Name:	Janvier	Station Number:	AMS 22
Start Time (MST):	12:16	End Time (MST):	17:52
Analyzer make:	Teledyne API T200	Analyzer serial #:	7117

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	-0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
799.9	803.6	0.9954		
400.4	401.1	0.9984		
200.2	201.2	0.9951		
			0.999997	
			1.004514	
			-0.271695	

NO_x Calibration Curve

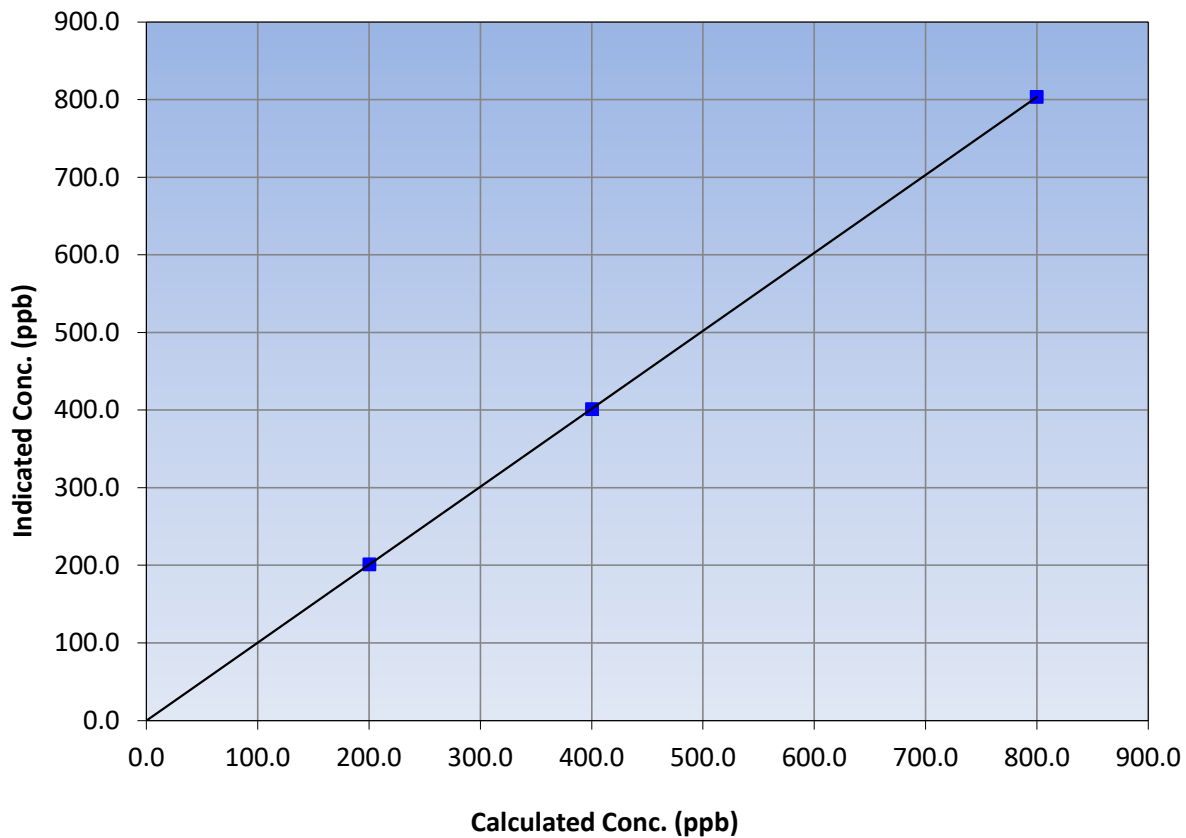



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	December 1, 2022
Station Name:	Janvier	Station Number:	AMS 22
Start Time (MST):	12:16	End Time (MST):	17:52
Analyzer make:	Teledyne API T200	Analyzer serial #:	7117

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
799.9	802.2	0.9971		
400.4	400.3	1.0004		
200.2	199.2	1.0051		

NO Calibration Curve

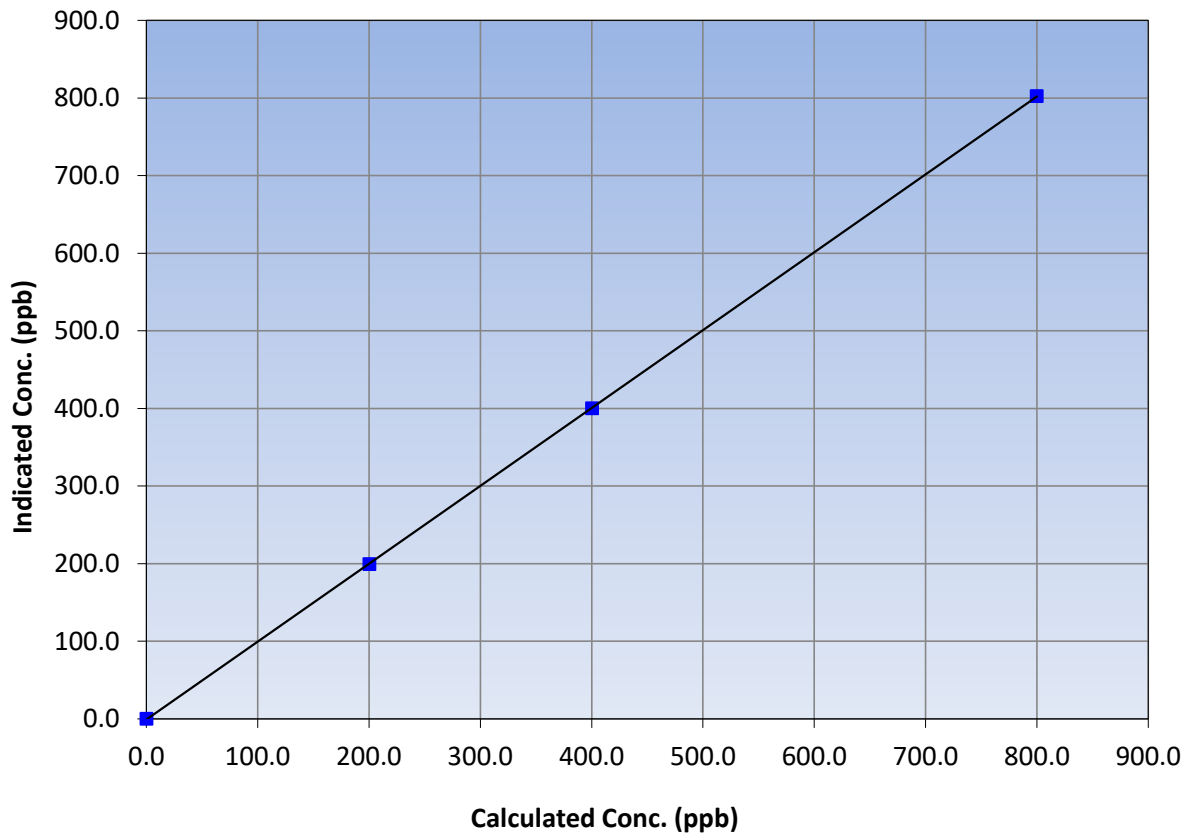



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 26, 2023	Previous Calibration:	December 1, 2022
Station Name:	Janvier	Station Number:	AMS 22
Start Time (MST):	12:16	End Time (MST):	17:52
Analyzer make:	Teledyne API T200	Analyzer serial #:	7117

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	-0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
388.2	388.5	0.9992		
192.3	192.9	0.9969		
96.9	98.3	0.9858		
			0.999985	
			0.999938	
			0.560426	


NO₂ Calibration Curve

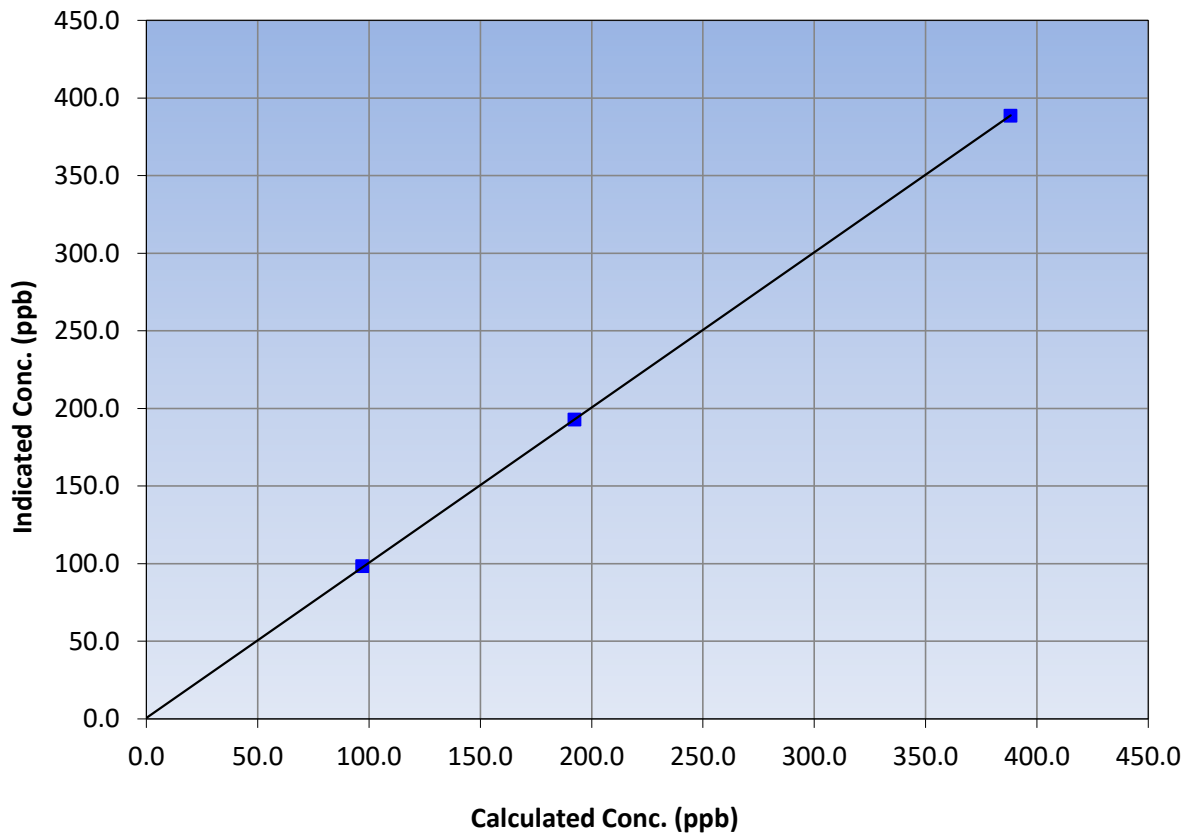

NO_x Calibration Plot

Date: January 26, 2023

Location: Janvier

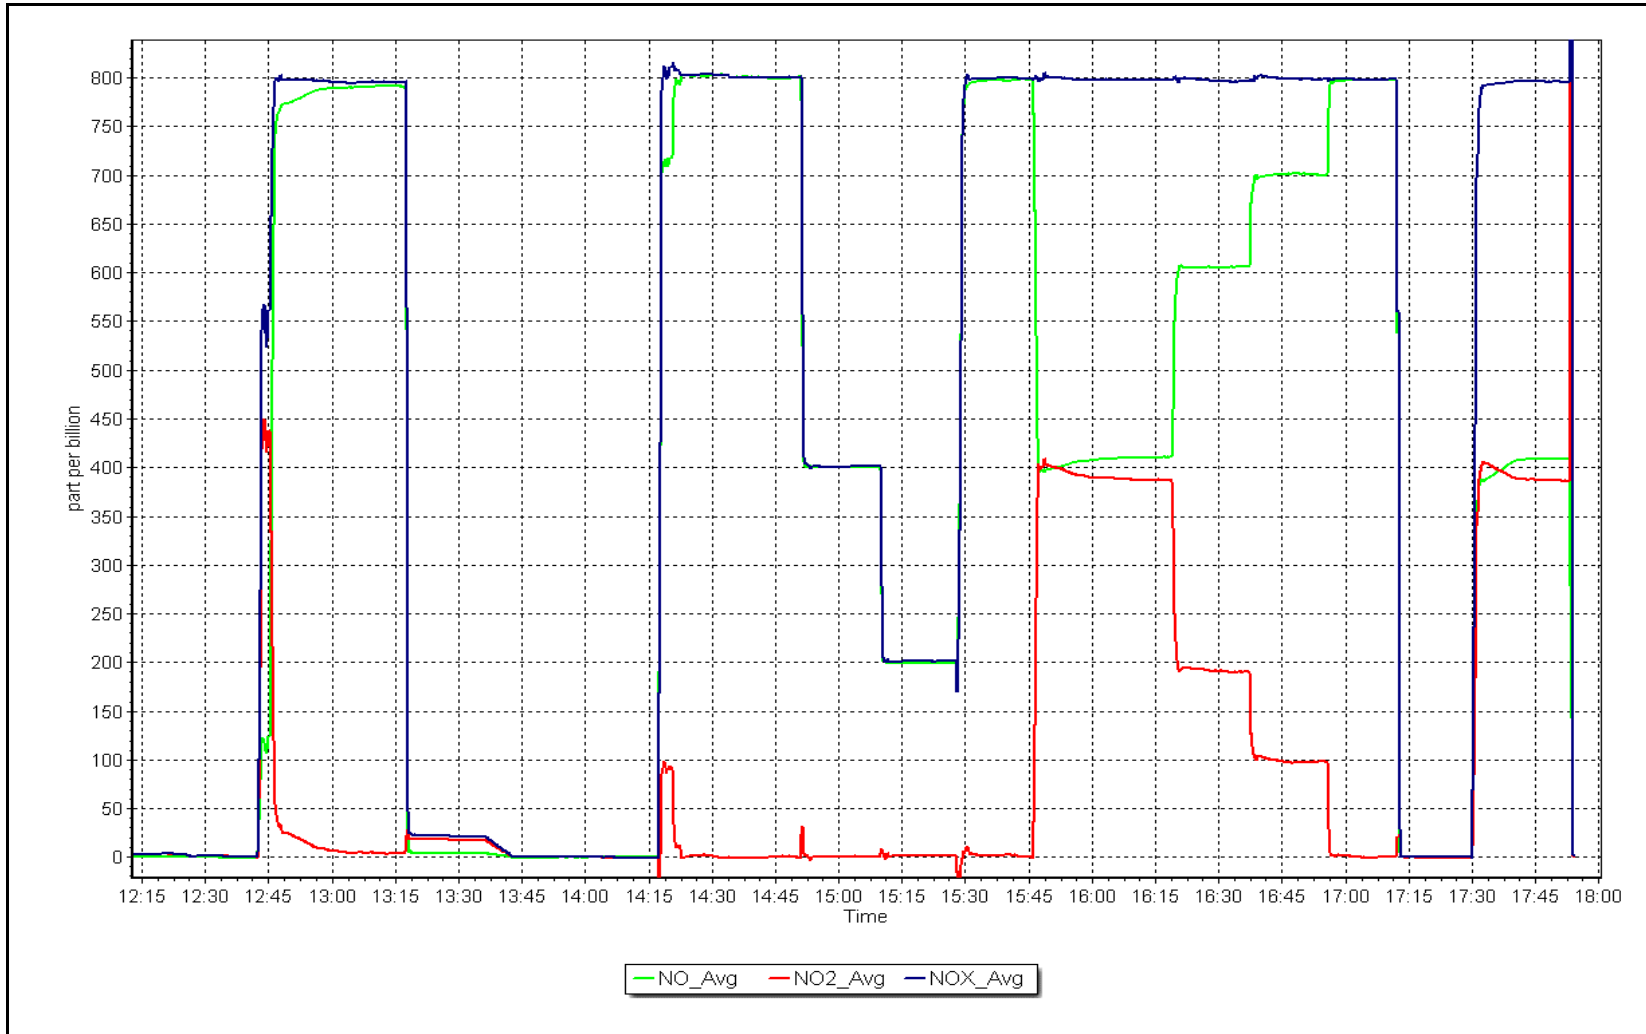



Wood Buffalo Environmental Association

O₃ Calibration Report

Version-01-2020

Station Information

Station Name: Janvier Station number: AMS 22
 Calibration Date: January 25, 2023 Last Cal Date: December 16, 2022
 Start time (MST): 11:15 End time (MST): 14:12
 Reason: Routine

Calibration Standards

O3 generation mode: Photometer
 Calibrator Make/Model: Teledyne API T700 Serial Number: 3806
 ZAG Make/Model: Teledyne API T701 Serial Number: 201

Analyzer Information

Analyzer make: Teledyne API T400 Analyzer serial #: 3869
 Analyzer Range 0 - 500 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.998686	0.998486	Backgd or Offset:	-2.0	-2.0
Calibration intercept:	0.480000	0.240000	Coeff or Slope:	1.011	1.011

O₃ Calibration Data

Set Point	Total air flow rate (sccm)	Calibrator Lamp Voltage Drive	Calculated concentration (ppb) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	800.0	0.0	0.0	----
as found span	4893	892.5	400.0	398.4	1.004
as found 2nd point					
as found 3rd point					
calibrator zero	5000	800.0	0.0	0.1	----
high point	4893	892.5	400.0	399.6	1.001
second point	4893	747.3	200.0	199.9	1.001
third point	4893	648.9	100.0	100.3	0.997
as left zero	5000	800.0	0.0	0.4	----
as left span	4816	892.5	400.0	401.0	0.998
Average Correction Factor					1.000

Baseline Corr As found:	398.4	Previous response	400.0	*% change	-0.4%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed inlet filter after as founds. No adjustments made.

Calibration Performed By: Rene Chamberland



Wood Buffalo Environmental Association

O₃ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 25, 2023	Previous Calibration:	December 16, 2022
Station Name:	Janvier	Station Number:	AMS 22
Start Time (MST):	11:15	End Time (MST):	14:12
Analyzer make:	Teledyne API T400	Analyzer serial #:	3869

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.1	----	Correlation Coefficient	0.999999	≥0.995
400.0	399.6	1.0010			
200.0	199.9	1.0005	Slope	0.998486	0.90 - 1.10
100.0	100.3	0.9970			
			Intercept	0.240000	+/- 5

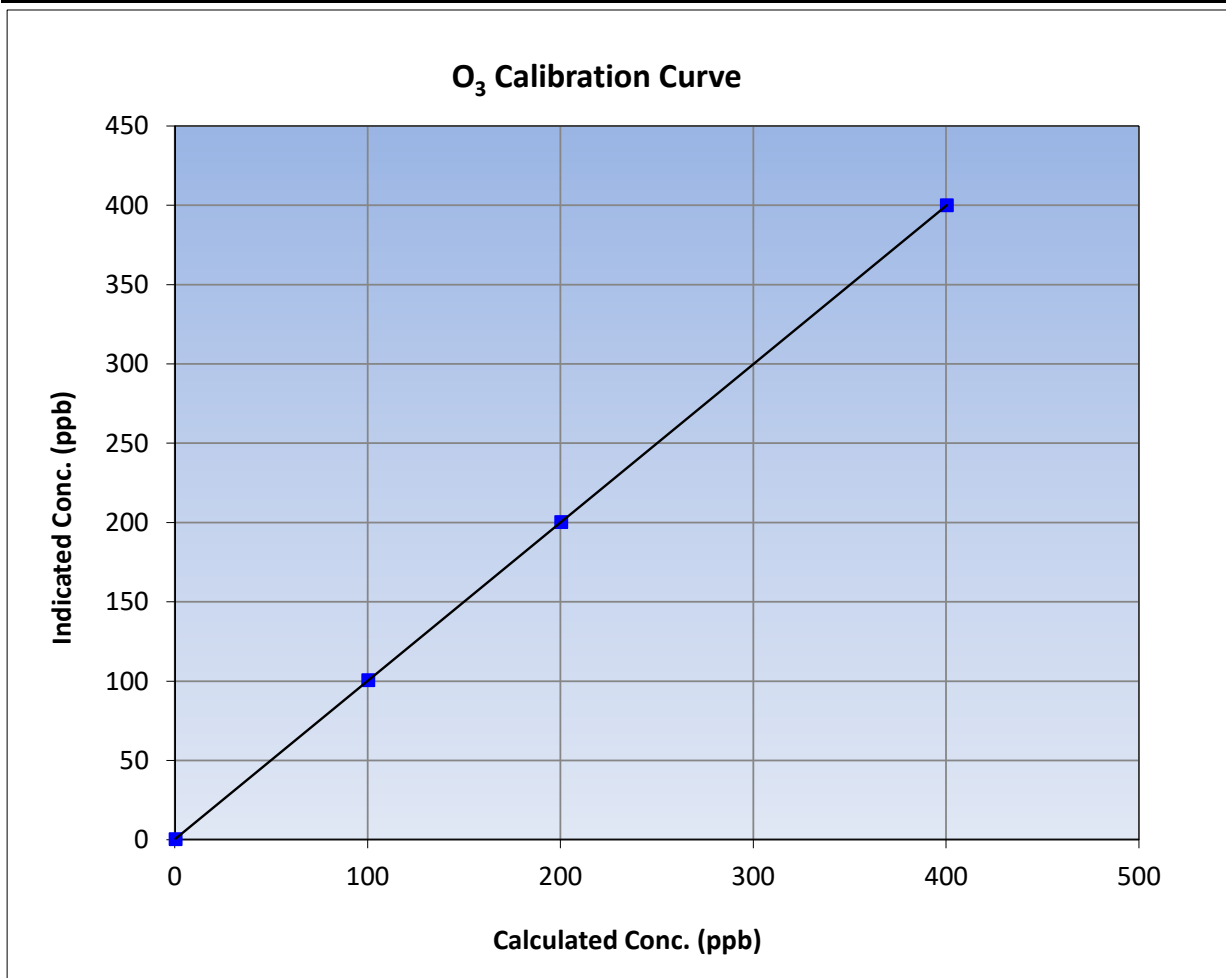

O₃ Calibration Plot

Date: January 25, 2023

Location: Janvier

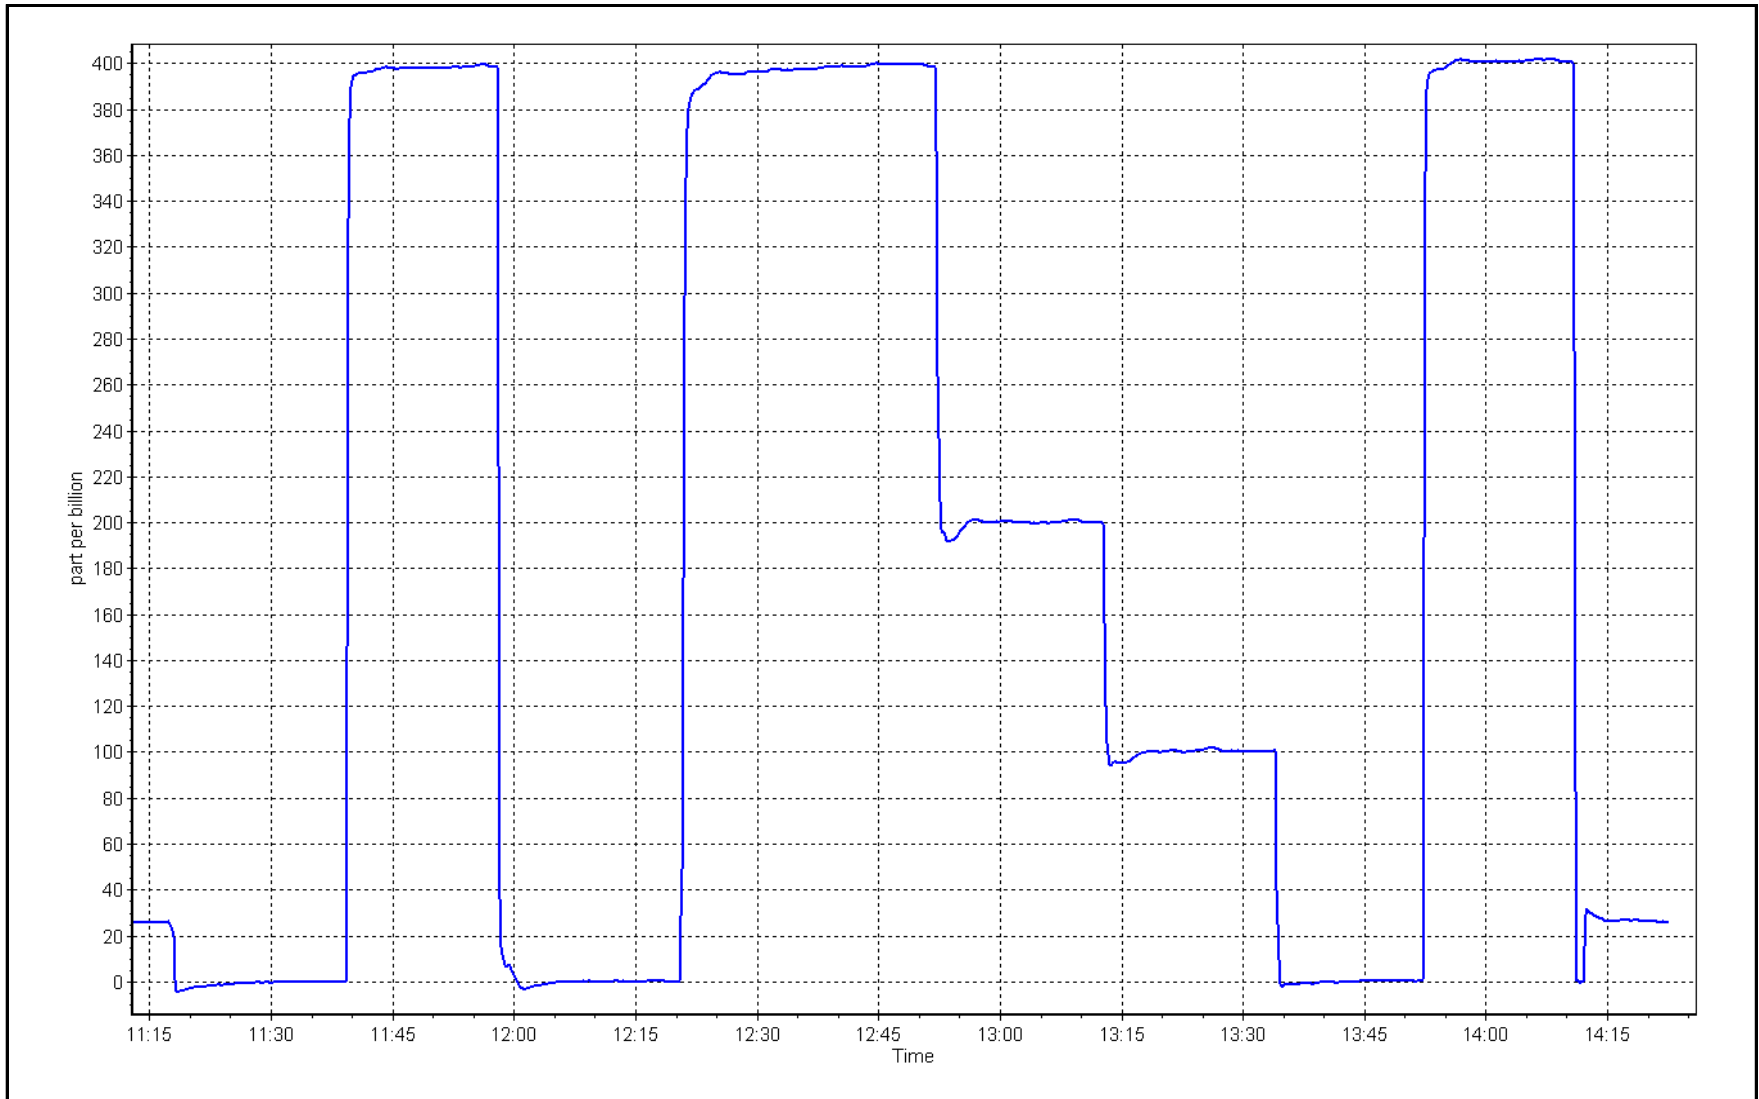



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Janvier Station number: AMS 22
Calibration Date: January 26, 2023 Last Cal Date: December 16, 2022
Start time (MST): 14:47 End time (MST): 16:29

Analyzer Make: API T640 S/N: 325
Particulate Fraction: PM2.5

Flow Meter Make/Model: Delta Cal S/N: 1450
Temp/RH standard: Delta Cal S/N: 1450

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-3.4	-2.7	-3.4	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	715.1	713.2	715.1	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5.01	5.06	5.01	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 26, 2023 December 16, 2022
PM w/o HEPA: 2.8 PM w/ HEPA: 0.0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test	10.1	-----	11.0	<input checked="" type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: January 26, 2023
Disposable Filter Changed: January 26, 2023

Annual Maintenance

Date Sample Tube Cleaned: October 6, 2022
Date RH/T Sensor Cleaned: October 6, 2022

Notes: Verified flow, temperature, and pressure. Leak test passed. PMT peak voltage adjusted from 1382V to 1385V. Optical chamber cleaned and disposable filter changed.

Calibration by: Rene Chamberland



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS23 FORT HILLS JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Fort Hills	Station number:	AMS23
Calibration Date:	January 4, 2023	Last Cal Date:	December 5, 2022
Start time (MST):	10:43	End time (MST):	13:50
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	49.76	ppm	Cal Gas Exp Date:	January 5, 2025
Cal Gas Cylinder #:	CC281425			
Removed Cal Gas Conc:	49.76	ppm	Rem Gas Exp Date:	N/A
Removed Gas Cyl #:	N/A		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	451
ZAG Make/Model:	API T701		Serial Number:	5611

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	1160290012
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.992999	0.999236	Backgd or Offset:	17.1	18.1
Calibration intercept:	-0.521973	-0.603450	Coeff or Slope:	1.036	1.048

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.4	----
as found span	4920	80.3	799.1	788.2	1.014
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.1	----
high point	4920	80.3	799.1	798.1	1.001
second point	4960	40.2	400.1	399.2	1.002
third point	4980	20.1	200.0	198.3	1.009
as left zero	5000	0.0	0.0	0.0	----
as left span	4920	80.3	799.1	801.3	0.997
Average Correction Factor					1.004

Baseline Corr As found:	787.80	Previous response	792.98	*% change	-0.7%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds. Adjusted zero and span.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 5, 2022
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:43	End Time (MST):	13:50
Analyzer make:	Thermo 43i	Analyzer serial #:	1160290012

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.1	----	Correlation Coefficient	0.999996	≥0.995
799.1	798.1	1.0013			
400.1	399.2	1.0021	Slope	0.999236	0.90 - 1.10
200.0	198.3	1.0087			
			Intercept	-0.603450	+/-30

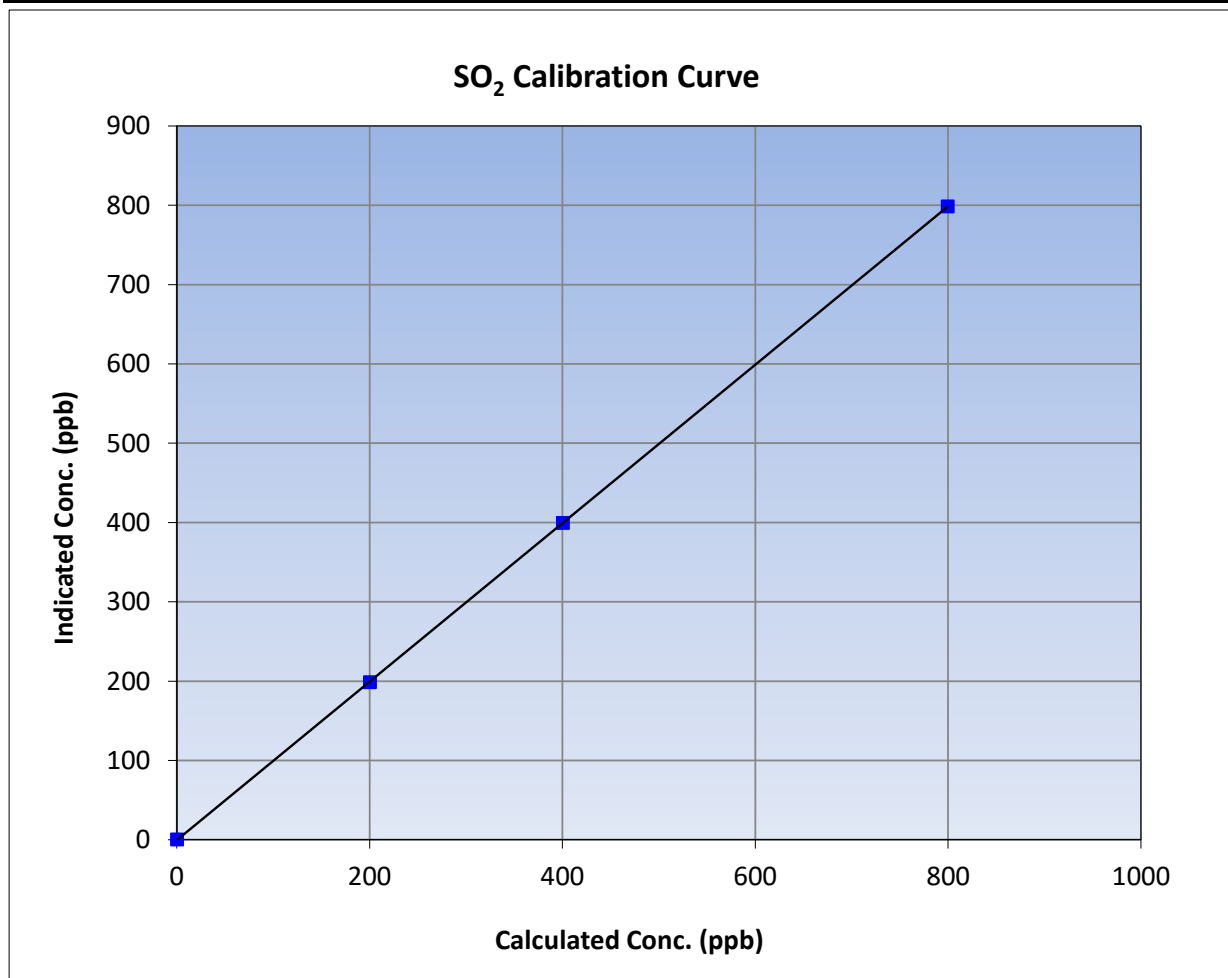

SO2 Calibration Plot

Date: January 4, 2023

Location: Fort Hills

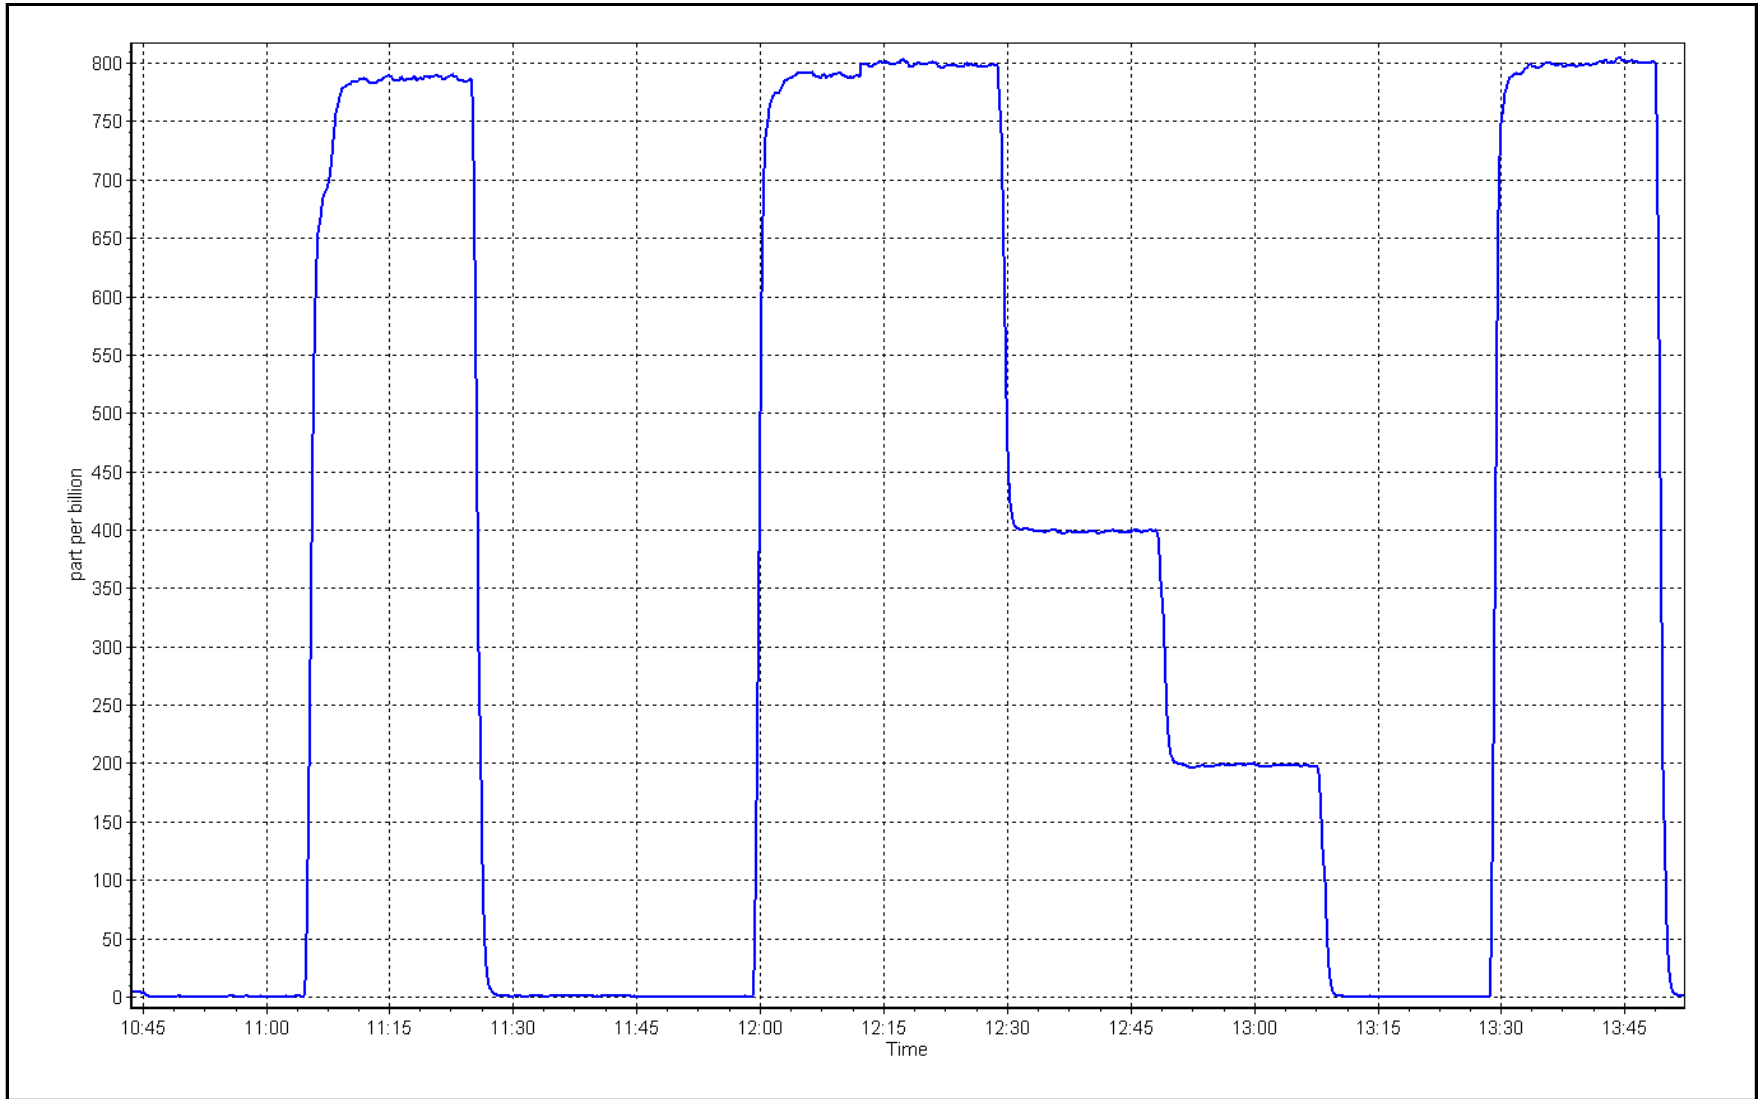



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name: Fort Hills Station number: AMS23
 Calibration Date: January 10, 2023 Last Cal Date: December 8, 2022
 Start time (MST): 11:01 End time (MST): 14:52
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.20 ppm Cal Gas Exp Date: February 5, 2024
 Cal Gas Cylinder #: CC517372
 Removed Cal Gas Conc: 5.20 ppm Rem Gas Exp Date: N/A
 Removed Gas Cyl #: N/A Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 451
 ZAG Make/Model: API T701 Serial Number: 5611

Analyzer Information

Analyzer make: Thermo 43iQ TLE Analyzer serial #: 12113311965
 Converter make: CDN-101 Converter serial #: 594
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.000594	0.988739	Backgd or Offset:	0.96	0.96
Calibration intercept:	0.442079	0.581876	Coeff or Slope:	0.714	0.714

H₂S/TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4923	77.0	80.0	79.1	1.013
as found 2nd point	4962	38.5	40.0	39.4	1.018
as found 3rd point	4981	19.2	19.9	19.6	1.023
new cylinder response					

H₂S/TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.1	----
high point	4923	77.0	80.0	79.4	1.008
second point	4962	38.5	40.0	40.5	0.988
third point	4981	19.2	19.9	20.7	0.964
as left zero	5000	0.0	0.0	1.4	----
as left span	4923	77.0	80.0	80.9	0.989
SO2 Scrubber Check	4922	78.3	783.0	0.1	----
Date of last scrubber change:				Ave Corr Factor	0.986
Date of last converter efficiency test:				efficiency	

Baseline Corr As found: 79.0 Prev response: 80.49 *% change: -1.9%
 Baseline Corr 2nd AF pt: 39.3 AF Slope: 0.988032 AF Intercept: -0.018415
 Baseline Corr 3rd AF pt: 19.5 AF Correlation: 0.999989

* = > +/-5% change initiates investigation

Notes: Changed the inlet filter after as founds, ran a SO2 scrubber check after calibrator zero. No adjustments made.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

H₂S/TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 8, 2022
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	11:01	End Time (MST):	14:52
Analyzer make:	Thermo 43iQ TLE	Analyzer serial #:	12113311965

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.1	----	Correlation Coefficient	0.999823	
80.0	79.4	1.0076			≥0.995
40.0	40.5	0.9876	Slope	0.988739	
19.9	20.7	0.9637			0.90 - 1.10
			Intercept	0.581876	+/-3

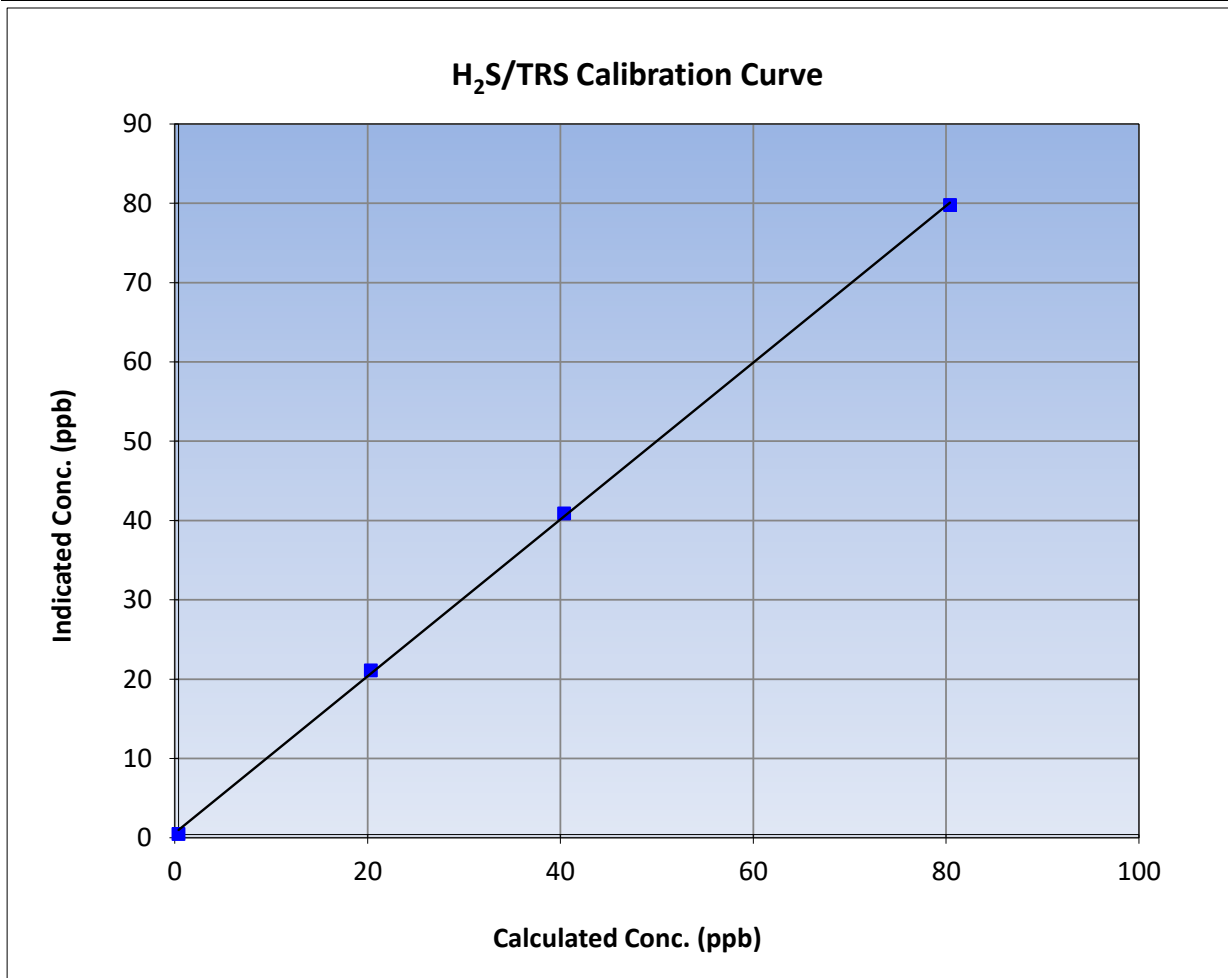

H₂S/TRS Calibration Plot

Date: January 10, 2023

Location: Fort Hills

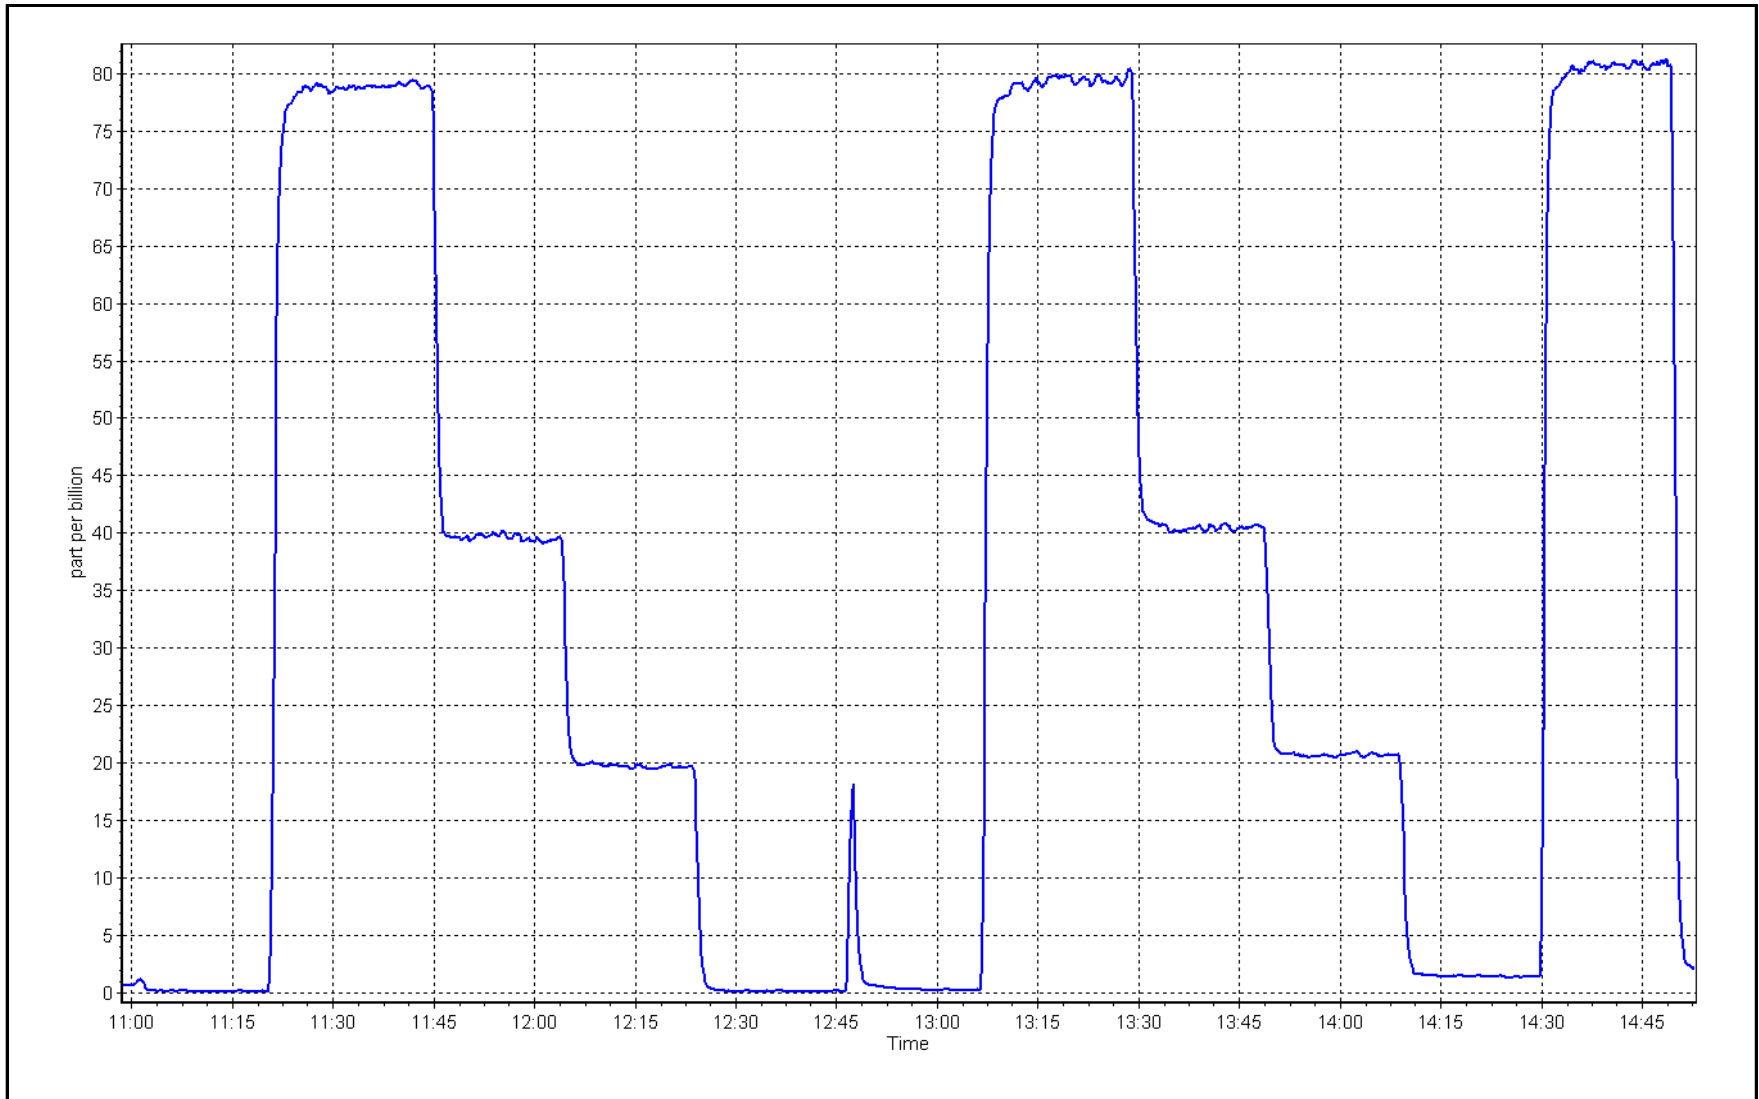



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Fort Hills	Station number:	AMS23
Calibration Date:	January 4, 2023	Last Cal Date:	December 5, 2022
Start time (MST):	10:43	End time (MST):	13:50
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC281425	Cal Gas Expiry Date:	January 5, 2025
CH ₄ Cal Gas Conc.	500.2 ppm	CH ₄ Equiv Conc.	1070.6 ppm
C ₃ H ₈ Cal Gas Conc.	207.4 ppm		
Removed Gas Cert:	N/A	Removed Gas Expiry:	N/A
Removed CH ₄ Conc.	500.2 ppm	CH ₄ Equiv Conc.	1070.6 ppm
Removed C ₃ H ₈ Conc.	207.4 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	451
ZAG make/model:	API T701	Serial Number:	5611

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1193585648
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	2.28E-04	2.33E-04	NMHC SP Ratio:	5.04E-05
CH ₄ Retention time:	13.0	13.0	NMHC Peak Area:	182523
				180258

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.3	17.19	17.03	1.010
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.3	17.19	17.38	0.989
second point	4960	40.2	8.61	8.65	0.995
third point	4980	20.1	4.30	4.33	0.994
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.3	17.19	17.35	0.991

Average Correction Factor				0.993
Baseline Corr AF:	17.03	Prev response	17.22	*% change -1.1%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.3	9.16	9.09	1.008
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.3	9.16	9.21	0.995
second point	4960	40.2	4.59	4.64	0.988
third point	4980	20.1	2.29	2.34	0.981
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.3	9.16	9.19	0.996
Average Correction Factor					0.988
Baseline Corr AF:	9.09	Prev response	9.18	*% change	-1.0%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.3	8.03	7.94	1.011
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.3	8.03	8.17	0.984
second point	4960	40.2	4.02	4.01	1.003
third point	4980	20.1	2.01	2.00	1.008
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.3	8.03	8.16	0.985
Average Correction Factor					0.998
Baseline Corr AF:	7.94	Prev response	8.04	*% change	-1.3%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	1.002403	1.010672
THC Cal Offset:	-0.010188	-0.017415
CH ₄ Cal Slope:	1.004851	1.017425
CH ₄ Cal Offset:	-0.027043	-0.035257
NMHC Cal Slope:	1.000606	1.004438
NMHC Cal Offset:	0.016455	0.018841

Notes: Changed the inlet filter after as founds. Adjusted the span only.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 5, 2022
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:43	End Time (MST):	13:50
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585648

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999990	≥ 0.995
17.19	17.38	0.9895			
8.61	8.65	0.9952			
4.30	4.33	0.9937			
			Slope	1.010672	0.90 - 1.10
			Intercept	-0.017415	+/-0.5

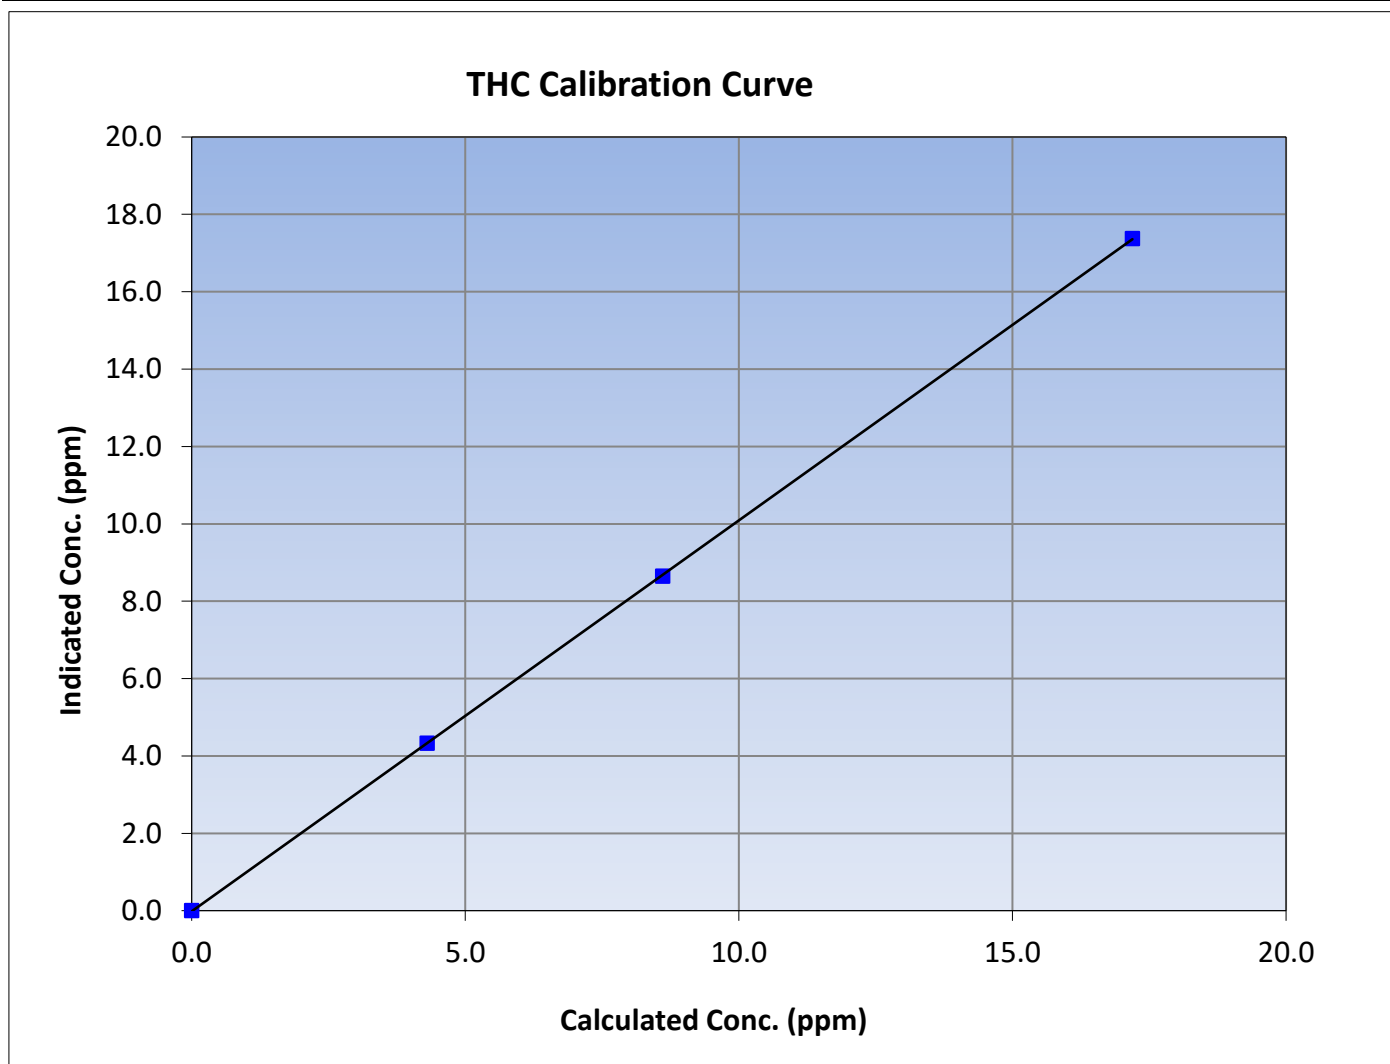



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 5, 2022
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:43	End Time (MST):	13:50
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585648

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999877	≥0.995
8.03	8.17	0.9838			
4.02	4.01	1.0031			
2.01	2.00	1.0079			
			Slope	1.017425	0.90 - 1.10
			Intercept	-0.035257	+/-0.5

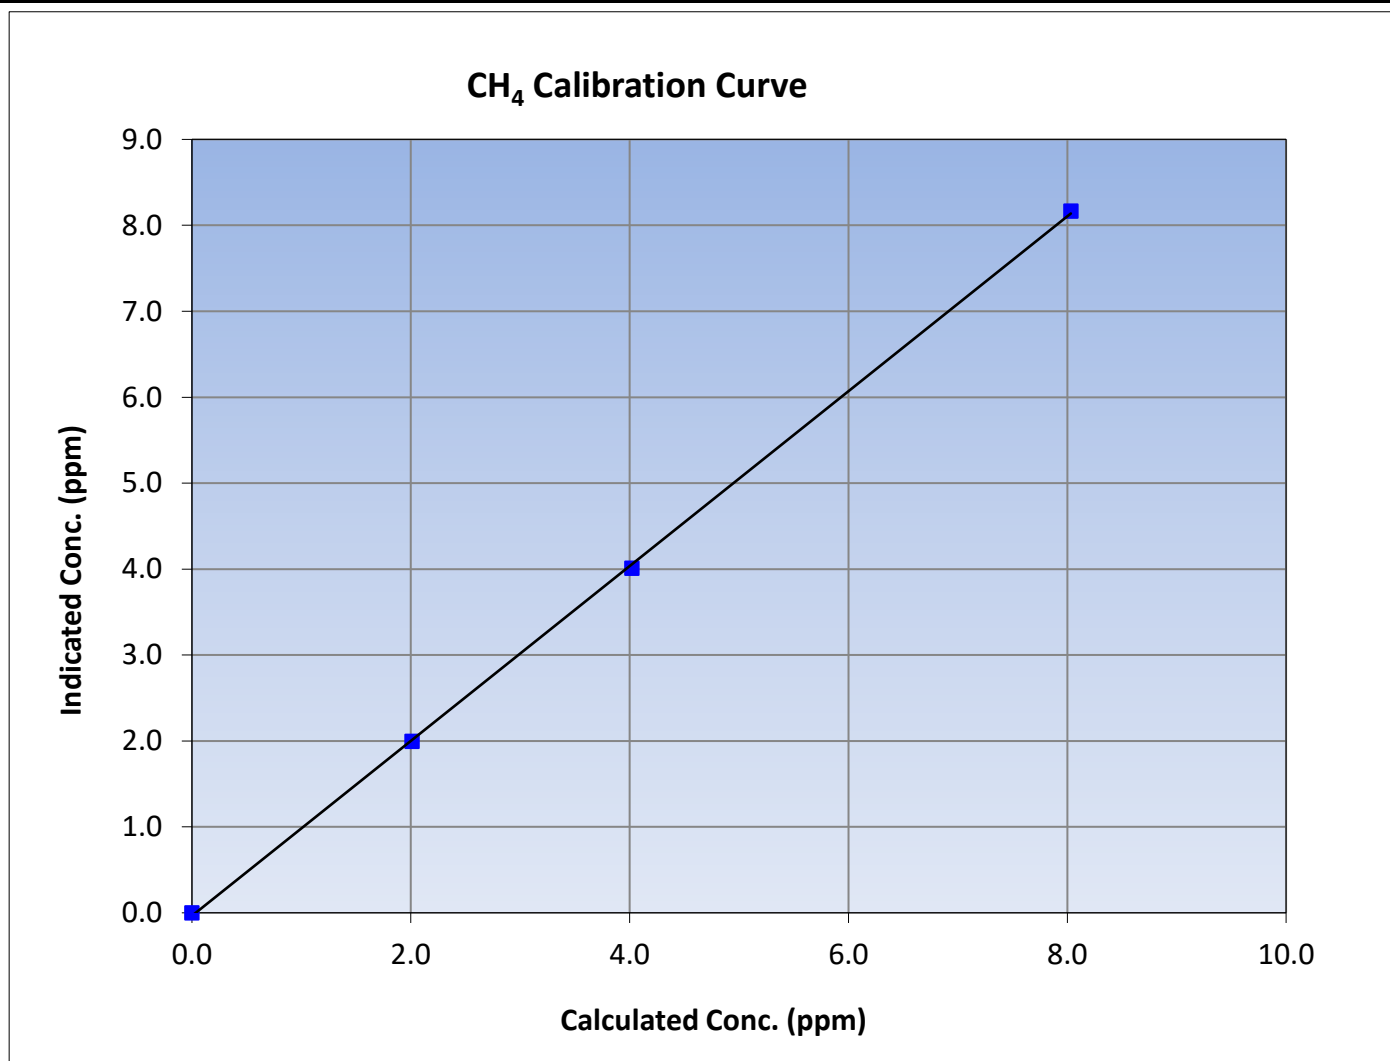



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 5, 2022
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:43	End Time (MST):	13:50
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585648

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999979	≥ 0.995			
9.16	9.21	0.9948						
4.59	4.64	0.9880				Slope	1.004438	0.90 - 1.10
2.29	2.34	0.9815						
			Intercept	0.018841	± 0.5			

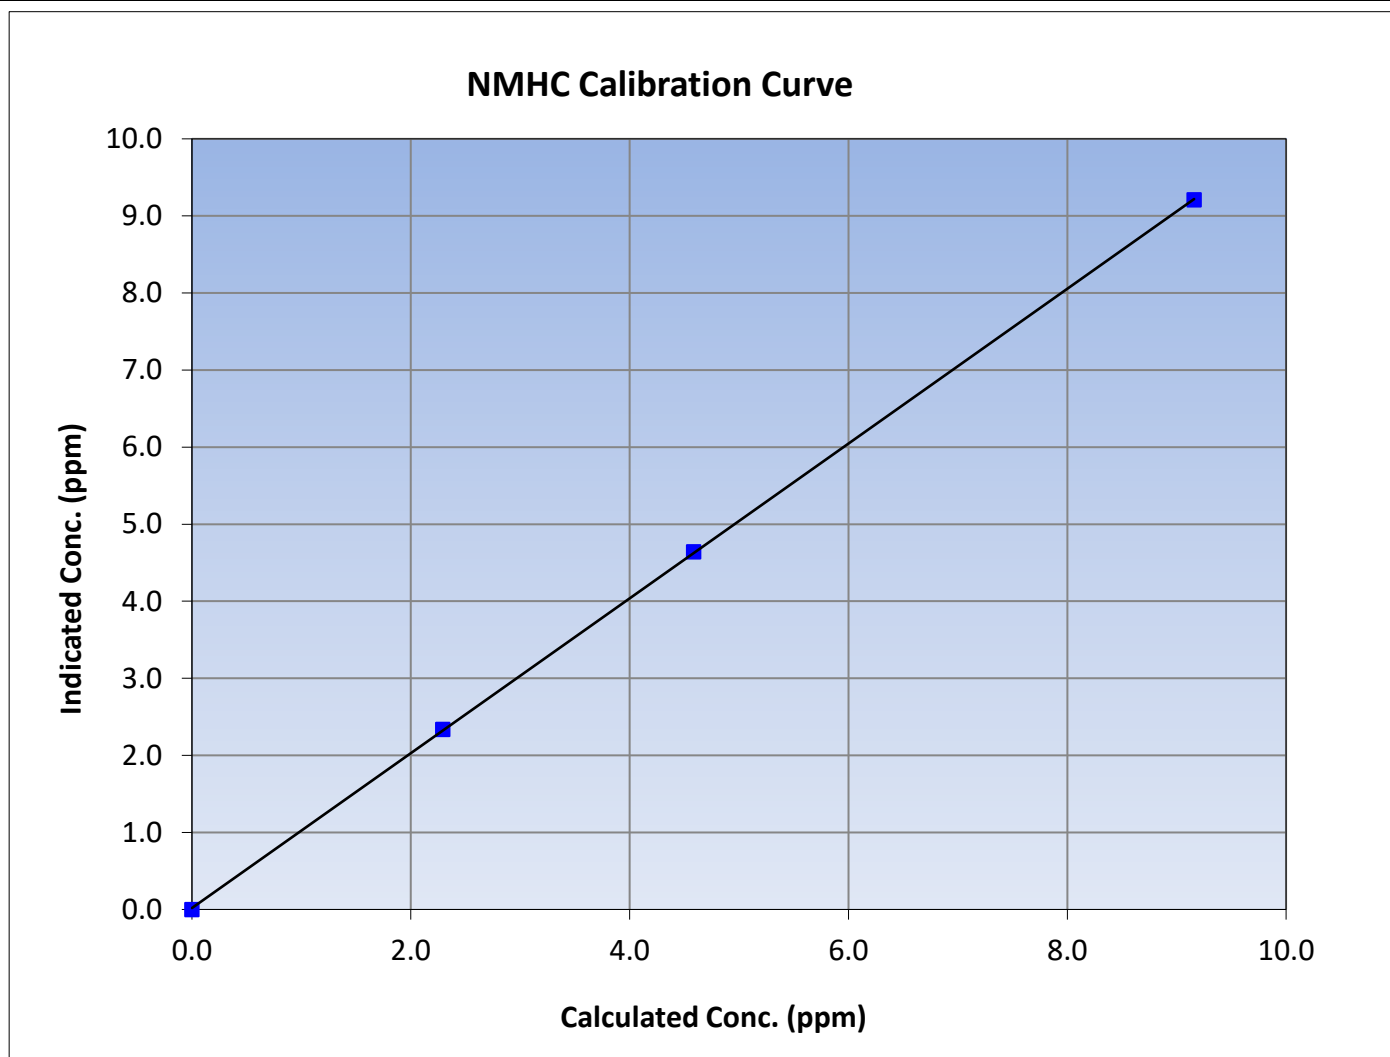

NMHC Calibration Plot

Date: January 4, 2023

Location: Fort Hills

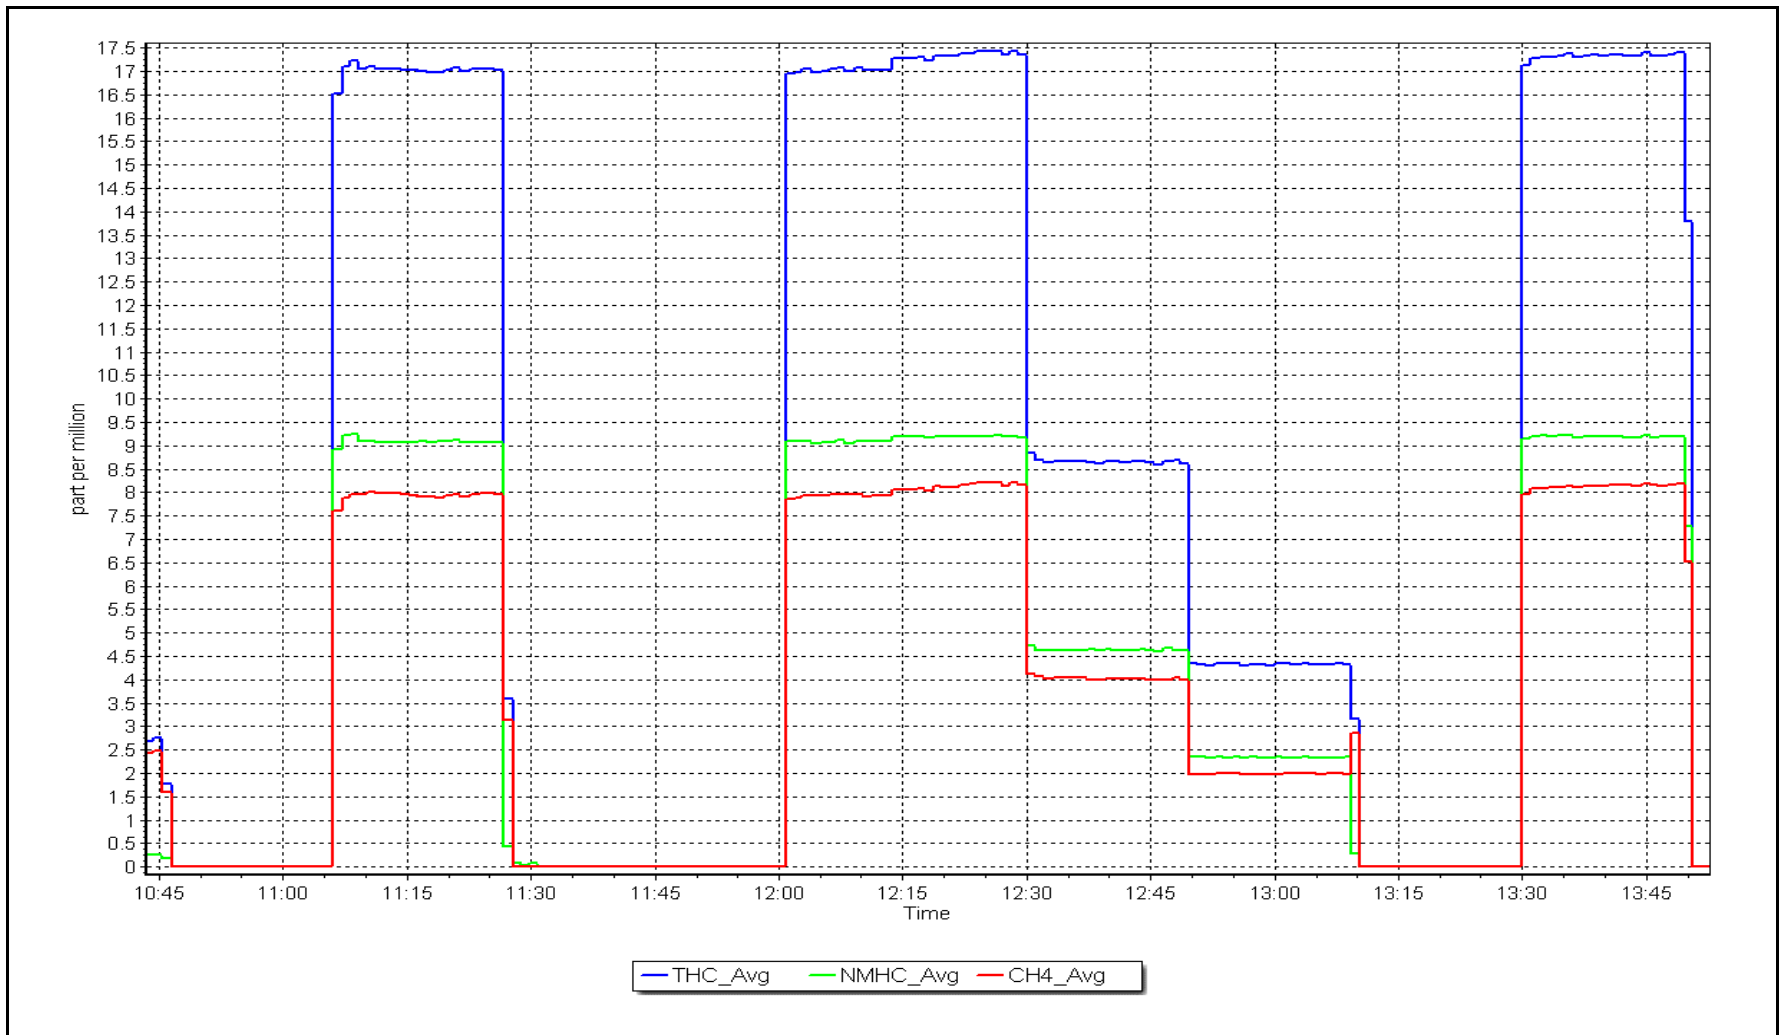



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Fort Hills	Station number:	AMS23
Calibration Date:	January 18, 2023	Last Cal Date:	January 4, 2023
Start time (MST):	10:24	End time (MST):	14:24
Reason:	Maintenance		

Calibration Standards

Gas Cert Reference:	CC281425	Cal Gas Expiry Date:	January 5, 2025
CH ₄ Cal Gas Conc.	500.2 ppm	CH ₄ Equiv Conc.	1070.6 ppm
C ₃ H ₈ Cal Gas Conc.	207.4 ppm		
Removed Gas Cert:	N/A	Removed Gas Expiry:	N/A
Removed CH ₄ Conc.	500.2 ppm	CH ₄ Equiv Conc.	1070.6 ppm
Removed C ₃ H ₈ Conc.	207.4 ppm	Diff between cyl (THC):	
Diff between cyl (CH ₄):		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	451
ZAG make/model:	API T701	Serial Number:	5611

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1193585648
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	2.33E-04	2.33E-04	NMHC SP Ratio:	5.01E-05
CH ₄ Retention time:	13.0	13.0	NMHC Peak Area:	180258
				180258

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.3	17.19	14.50	1.185
as found 2nd point	4960	40.2	8.61	7.15	1.203
as found 3rd point	4980	20.1	4.30	3.65	1.180
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.3	17.19	17.17	1.001
second point	4960	40.2	8.61	8.61	1.000
third point	4980	20.1	4.30	4.31	0.999
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.3	17.19	17.28	0.995
Average Correction Factor					1.000
Baseline Corr AF:	14.50	Prev response	17.36	*% change	-19.7%
Baseline Corr 2nd AF:	7.2	AF Slope:	0.842506	AF Intercept:	-0.014862
Baseline Corr 3rd AF:	3.6	AF Correlation:	0.999919	* = > +/-5% change initiates investigation	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.3	9.16	7.54	1.214
as found 2nd point	4960	40.2	4.59	3.74	1.225
as found 3rd point	4980	20.1	2.29	1.93	1.186
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.3	9.16	9.13	1.003
second point	4960	40.2	4.59	4.60	0.996
third point	4980	20.1	2.29	2.33	0.985
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.3	9.16	9.17	0.999
Average Correction Factor					0.995
Baseline Corr AF:	7.54	Prev response	9.22	*% change	-22.2%
Baseline Corr 2nd AF:	3.7	AF Slope:	0.821429	AF Intercept:	0.011089
Baseline Corr 3rd AF:	1.9	AF Correlation:	0.999905	* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4920	80.3	8.03	6.96	1.154
as found 2nd point	4960	40.2	4.02	3.41	1.179
as found 3rd point	4980	20.1	2.01	1.71	1.174
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4920	80.3	8.03	8.04	0.999
second point	4960	40.2	4.02	4.01	1.004
third point	4980	20.1	2.01	1.98	1.015
as left zero	5000	0.0	0.00	0.00	----
as left span	4920	80.3	8.03	8.12	0.990
Average Correction Factor					1.006
Baseline Corr AF:	6.96	Prev response	8.14	*% change	-16.9%
Baseline Corr 2nd AF:	3.41	AF Slope:	0.866538	AF Intercept:	-0.025951
Baseline Corr 3rd AF:	1.71	AF Correlation:	0.999869	* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	1.010672	0.998822
THC Cal Offset:	-0.017415	0.006016
CH ₄ Cal Slope:	1.017425	1.001922
CH ₄ Cal Offset:	-0.035257	-0.016245
NMHC Cal Slope:	1.004438	0.996115
NMHC Cal Offset:	0.018841	0.022460

Notes: Due to pump failure low as founds. Swapped out the pump and the inlet filter after multipoint as founds. No adjustments needed.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 18, 2023	Previous Calibration:	January 4, 2023
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:24	End Time (MST):	14:24
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585648

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999999	≥ 0.995			
17.19	17.17	1.0010						
8.61	8.61	0.9999				Slope	0.998822	0.90 - 1.10
4.30	4.31	0.9987						
			Intercept	0.006016	± 0.5			

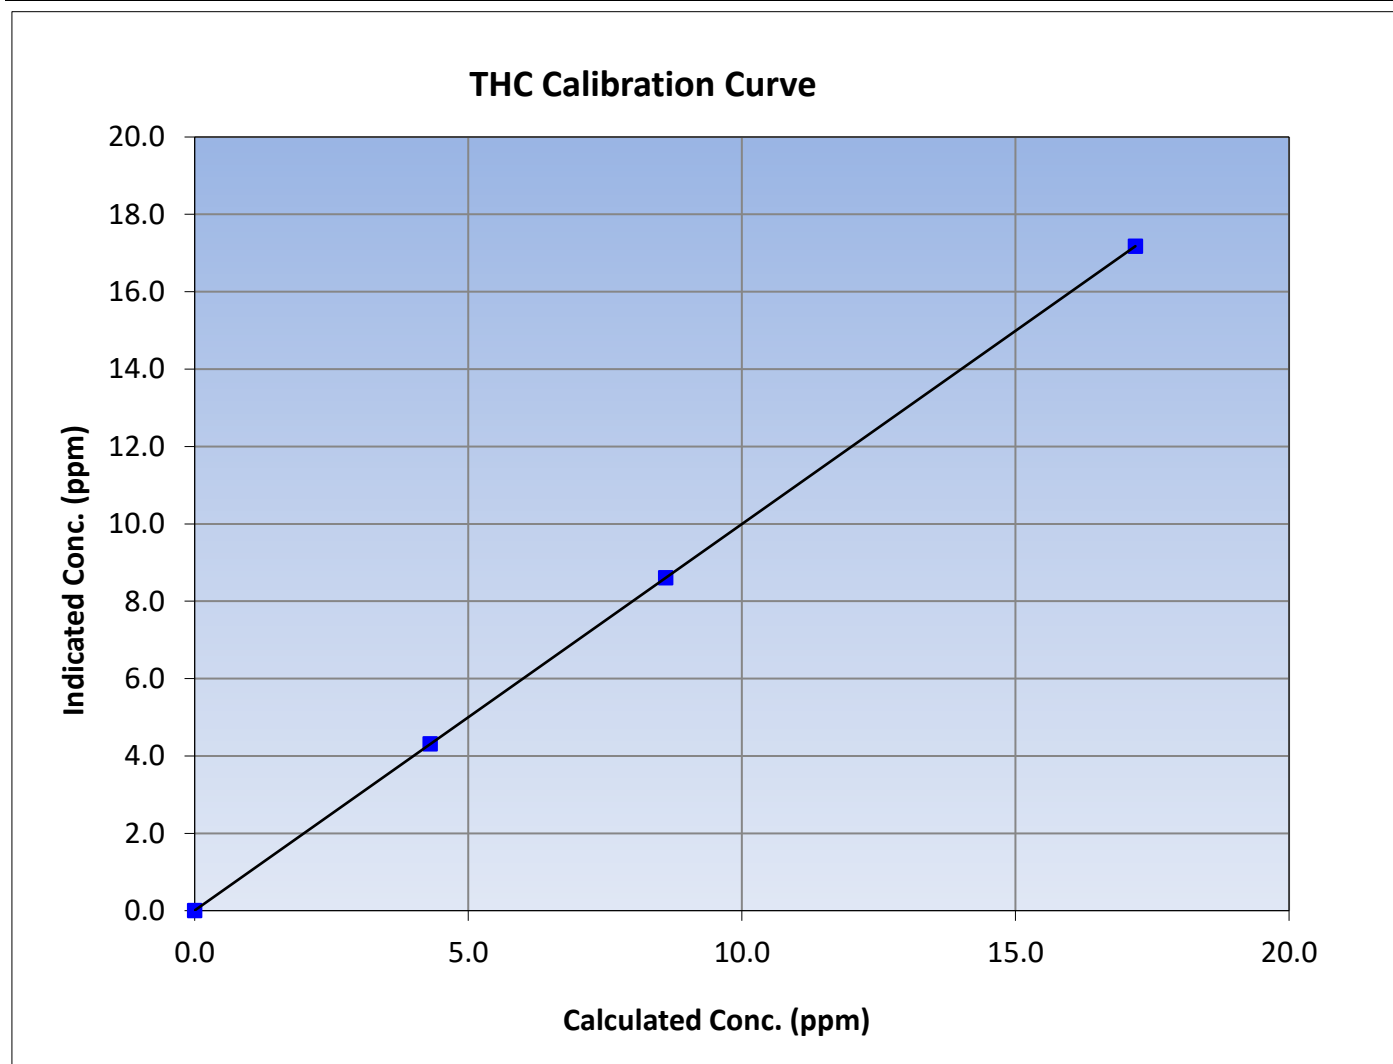



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 18, 2023	Previous Calibration:	January 4, 2023
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:24	End Time (MST):	14:24
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585648

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999981	≥ 0.995			
8.03	8.04	0.9991						
4.02	4.01	1.0041				Slope	1.001922	0.90 - 1.10
2.01	1.98	1.0145						
			Intercept	-0.016245	± 0.5			

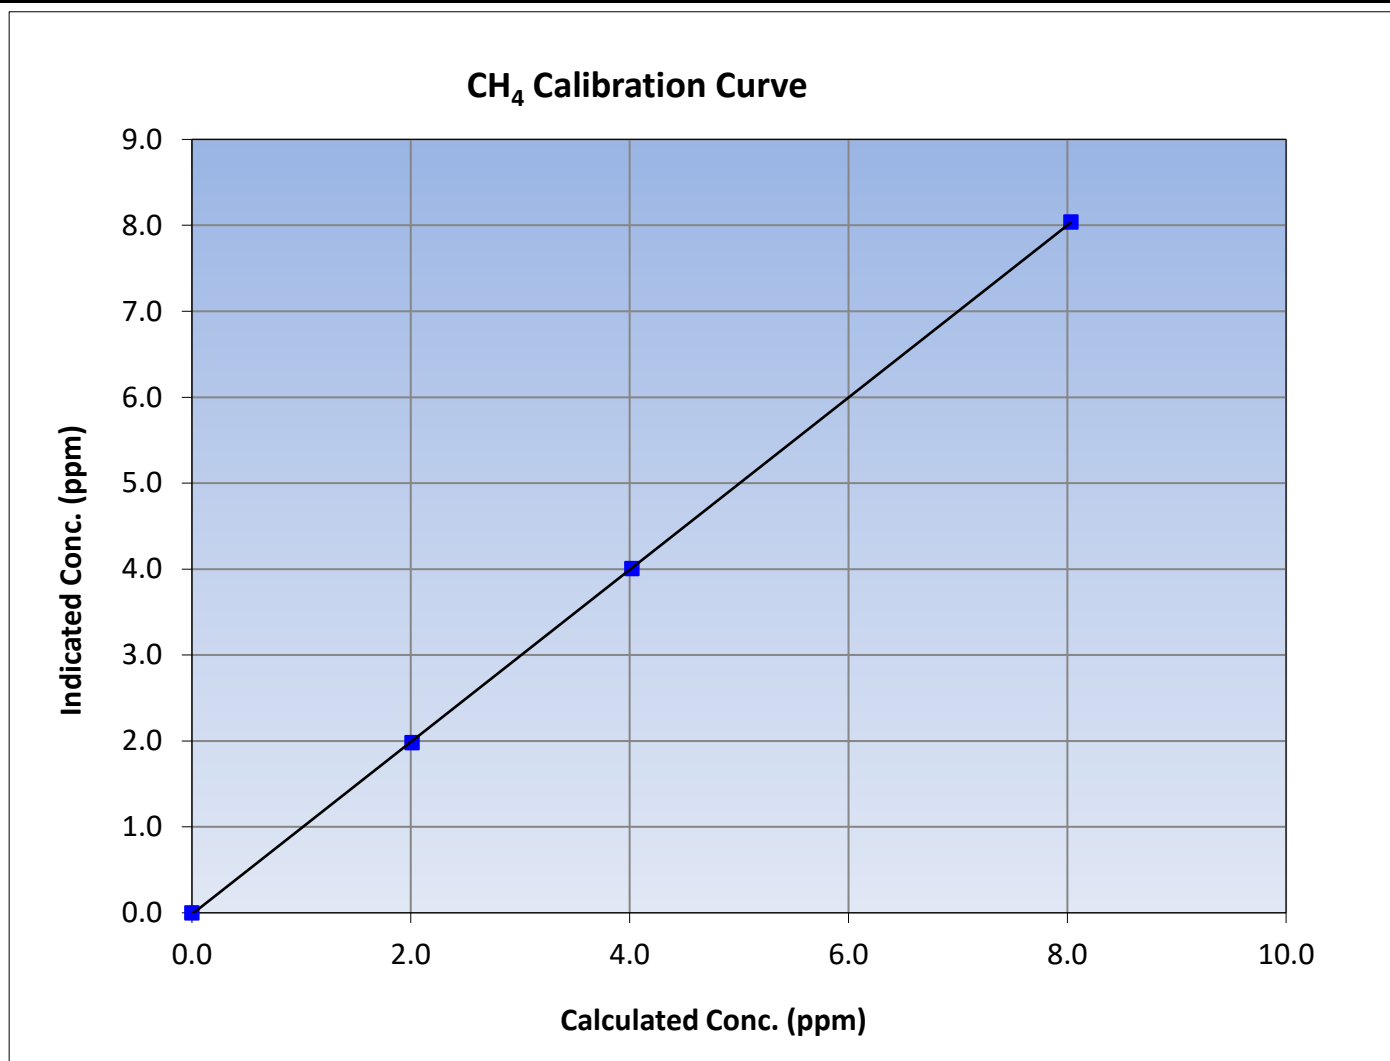



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 18, 2023	Previous Calibration:	January 4, 2023
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:24	End Time (MST):	14:24
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585648

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999972	≥ 0.995			
9.16	9.13	1.0028						
4.59	4.60	0.9960				Slope	0.996115	0.90 - 1.10
2.29	2.33	0.9853						
			Intercept	0.022460	± 0.5			

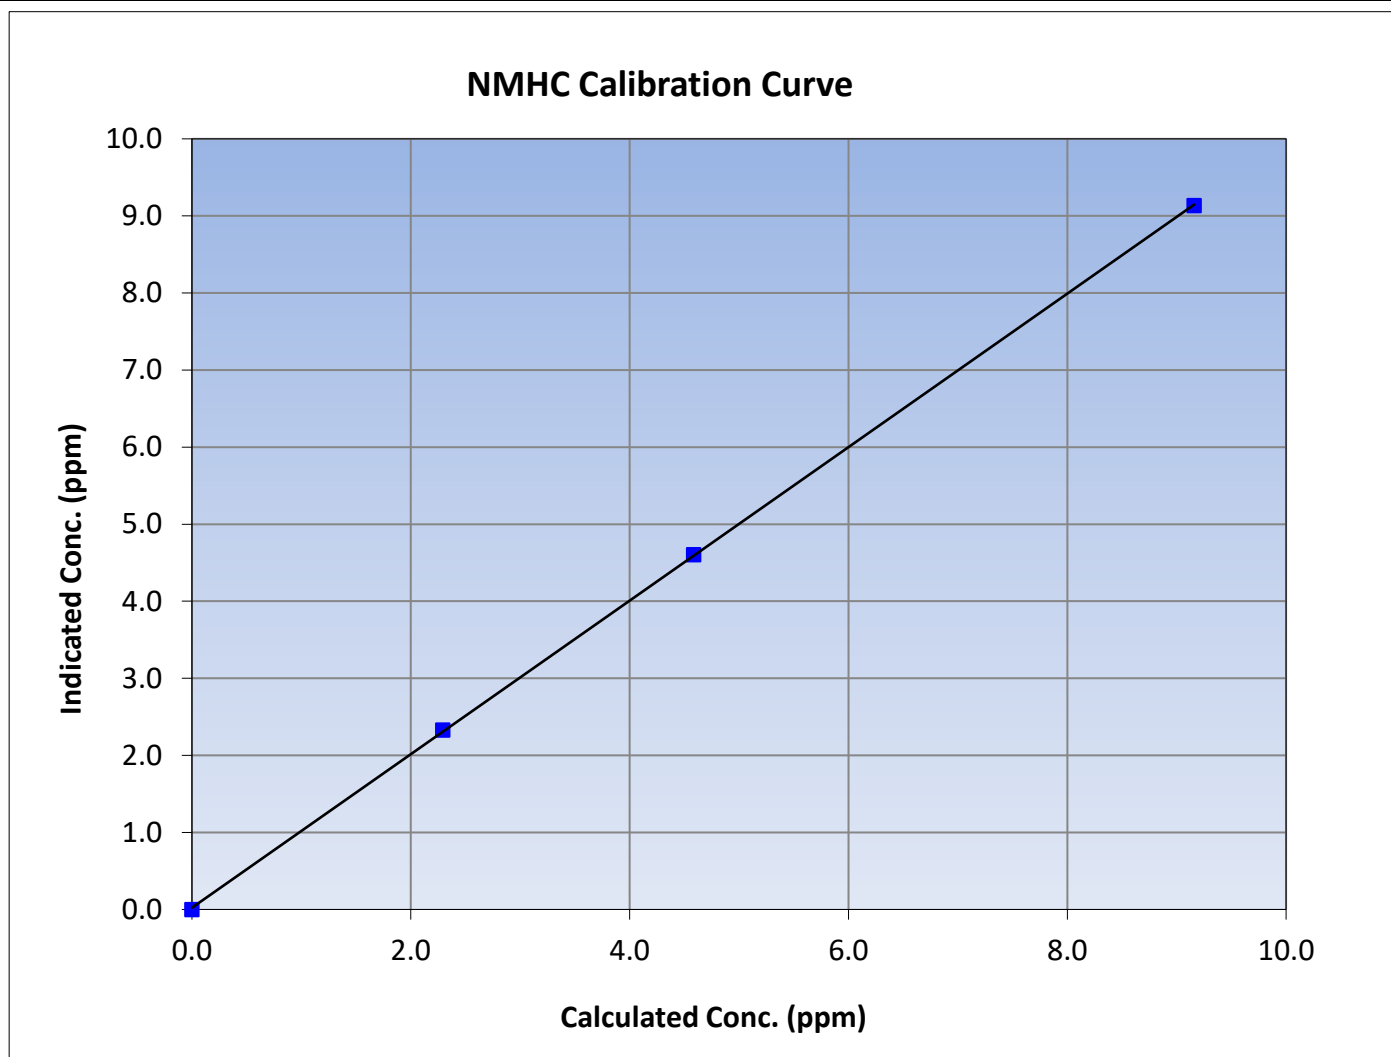

NMHC Calibration Plot

Date: January 18, 2023

Location: Fort Hills

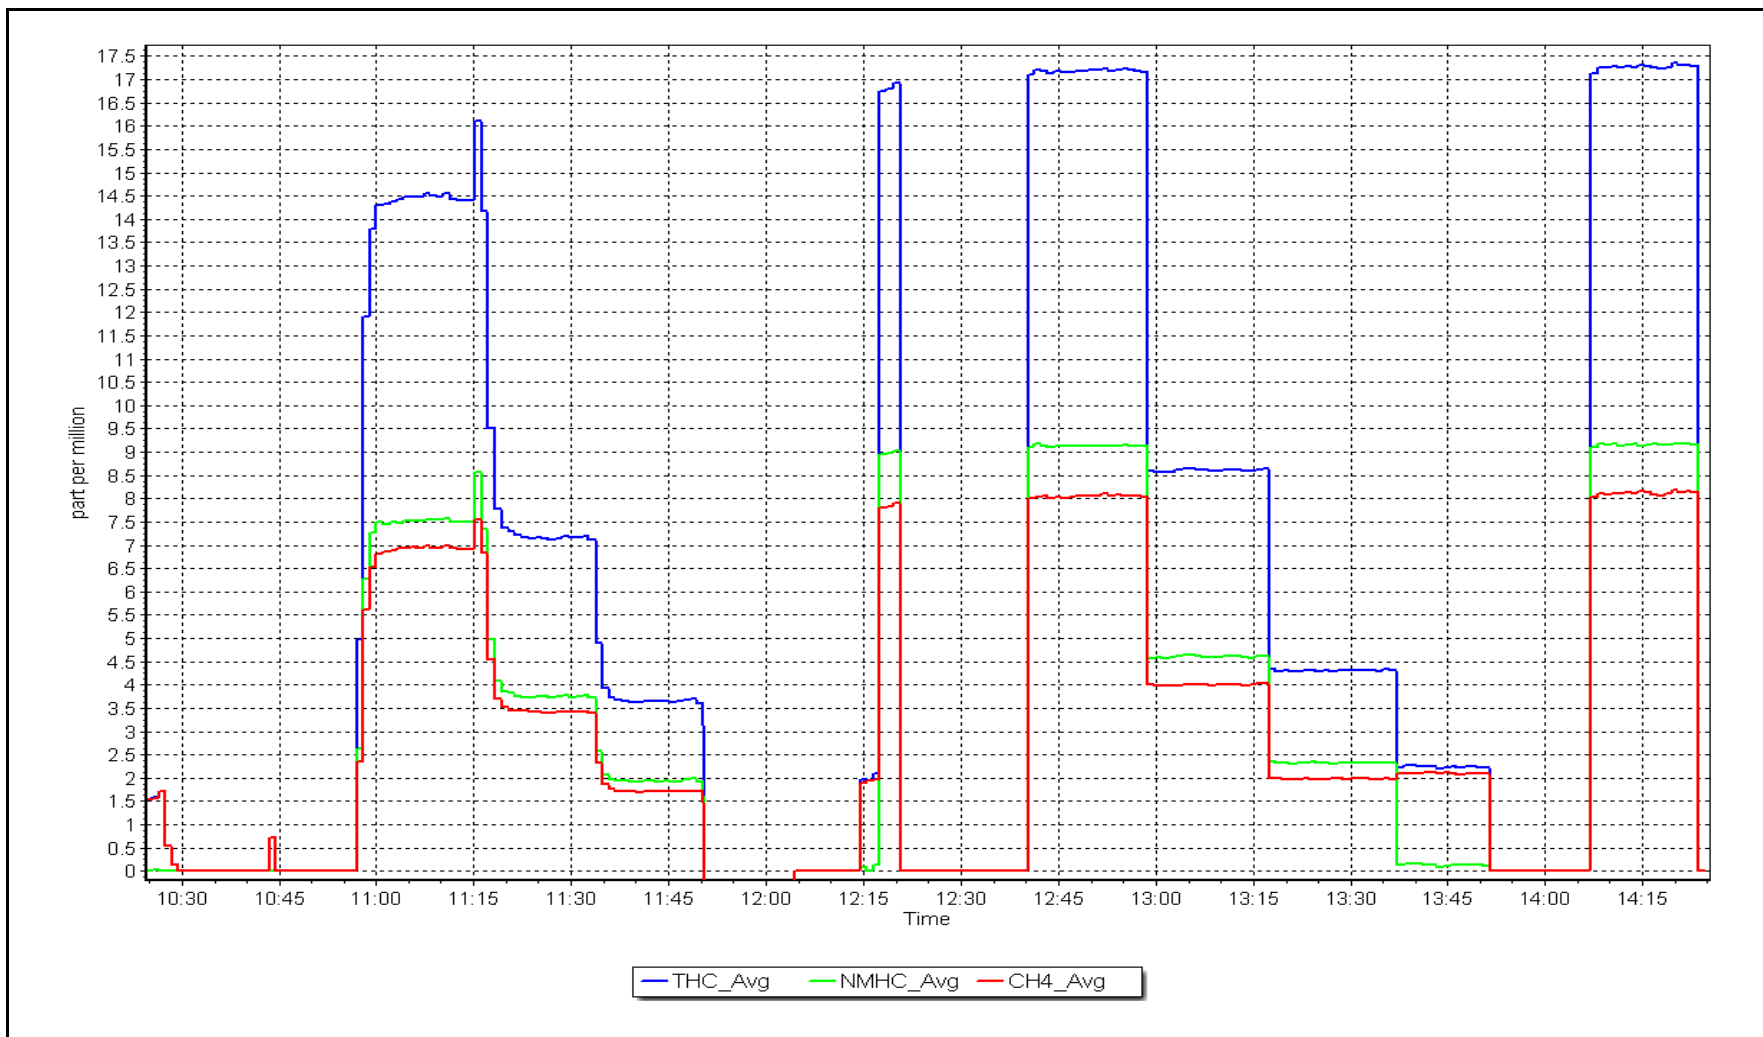



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Fort Hills
Calibration Date: January 24, 2023
Start time (MST): 10:04
Reason: Routine
Station number: AMS23
Last Cal Date: December 7, 2022
End time (MST): 15:17

Calibration Standards

NO Gas Cylinder #: CC332703
NOX Cal Gas Conc: 49.7 ppm
Removed Cylinder #: N/A
Removed Gas NOX Conc: 49.7 ppm
NOX gas Diff:
Calibrator Model: Teledyne API T750
ZAG make/model: Teledyne API T751H
Cal Gas Expiry Date: January 28, 2024
NO Cal Gas Conc: 49.7 ppm
Removed Gas Exp Date: N/A
Removed Gas NO Conc: 49.7 ppm
NO gas Diff:
Serial Number: 275
Serial Number: 307

Analyzer Information

Analyzer make: Thermo 42i
NOX Range (ppb): 0 - 1000 ppb
Analyzer serial #: 1152430007

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.501	1.527	NO bkgnd or offset:	4.2	4.3
NOX coeff or slope:	0.995	0.997	NOX bkgnd or offset:	4.6	4.7
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	221.4	225.4

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	0.994625	0.999637
NO _x Cal Offset:	-0.277404	0.644160
NO Cal Slope:	0.996641	0.999282
NO Cal Offset:	-1.157676	-0.256715
NO ₂ Cal Slope:	0.992164	1.001046
NO ₂ Cal Offset:	-0.103647	0.284247



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-0.2	0.1	-0.2	----	----
as found span	4920	80.5	800.2	800.2	0.0	787.7	786.0	1.7	1.016	1.018
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	-0.1	0.2	-0.2	----	----
high point	4920	80.5	800.2	800.2	0.0	799.9	799.5	0.4	1.000	1.001
second point	4960	40.2	399.6	399.6	0.0	401.2	399.0	2.2	0.996	1.001
third point	4980	20.1	199.8	199.8	0.0	200.6	198.8	1.8	0.996	1.005
as left zero	5000	0.0	0.0	0.0	0.0	-0.4	-0.2	-0.3	----	----
as left span	4920	80.5	800.2	436.5	363.7	802.5	435.9	366.6	0.997	1.001
Average Correction Factor									0.997	1.002

Corrected As found	NO _x = 787.9 ppb	NO = 785.9 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -1.0%	
Previous Response	NO _x = 795.6 ppb	NO = 796.3 ppb		*Percent Change	NO = -1.3%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO ₂)						
as found GPT point (200 ppb NO ₂)						
as found GPT point (100 ppb NO ₂)						
1st GPT point (400 ppb O ₃)	796.0	432.3	363.7	364.0	0.999	100.1%
2nd GPT point (200 ppb O ₃)	796.0	617.2	178.8	179.9	0.994	100.6%
3rd GPT point (100 ppb O ₃)	796.0	704.4	91.6	92.2	0.993	100.7%
Average Correction Factor					0.996	100.5%

Notes: Changed the inlet filter after as founds. Adjusted the span only.

Calibration Performed By: Max Farrell



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 7, 2022
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:04	End Time (MST):	15:17
Analyzer make:	Thermo 42i	Analyzer serial #:	1152430007

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	-0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
800.2	799.9	1.0003		
399.6	401.2	0.9959		
199.8	200.6	0.9960		
			0.999994	
			0.999637	
			0.644160	

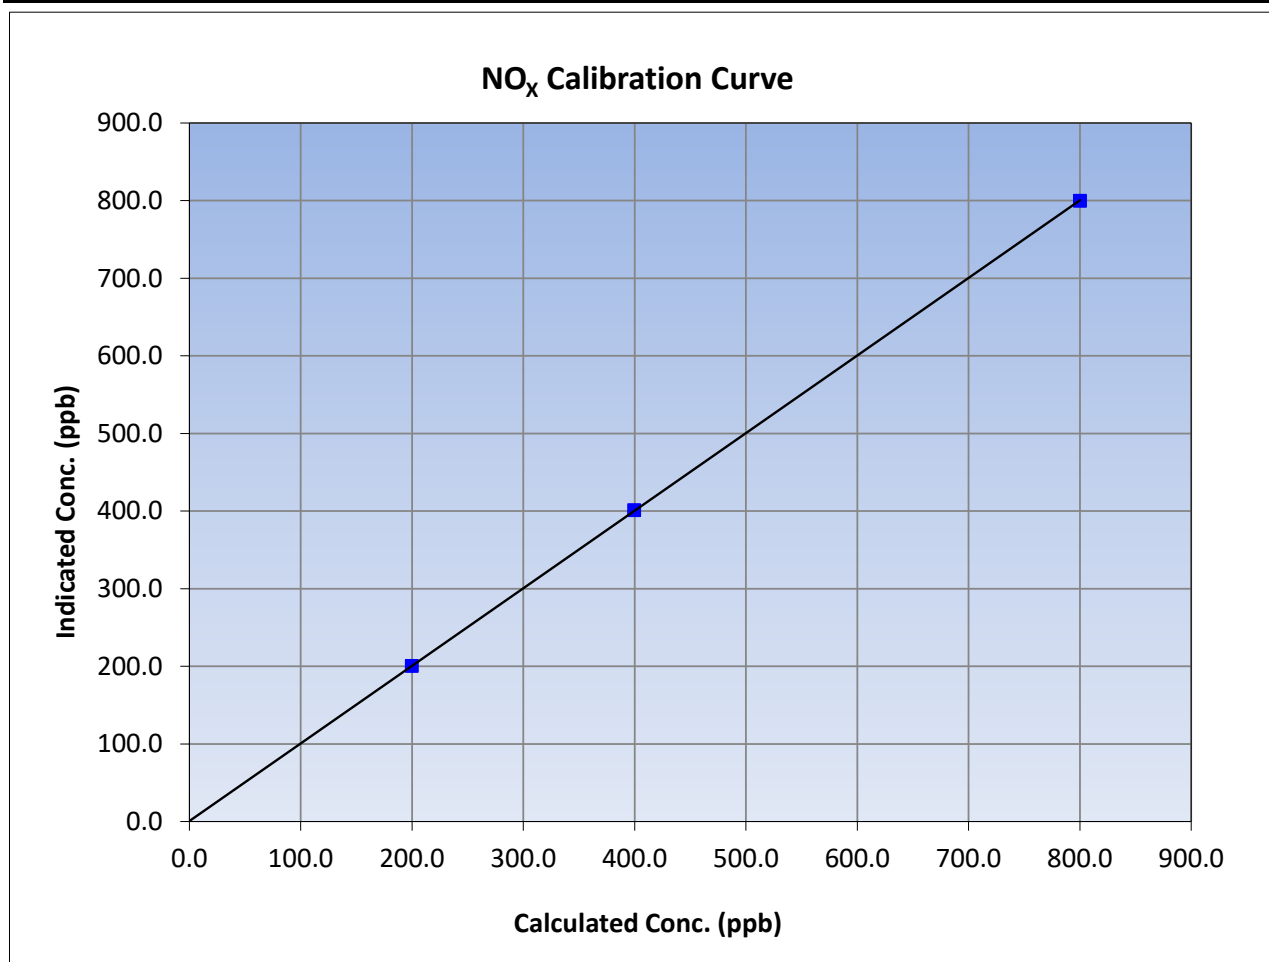



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 7, 2022
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:04	End Time (MST):	15:17
Analyzer make:	Thermo 42i	Analyzer serial #:	1152430007

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	0.2	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
800.2	799.5	1.0008		
399.6	399.0	1.0014		
199.8	198.8	1.0050		
			0.999998	
			0.999282	
			-0.256715	

NO Calibration Curve

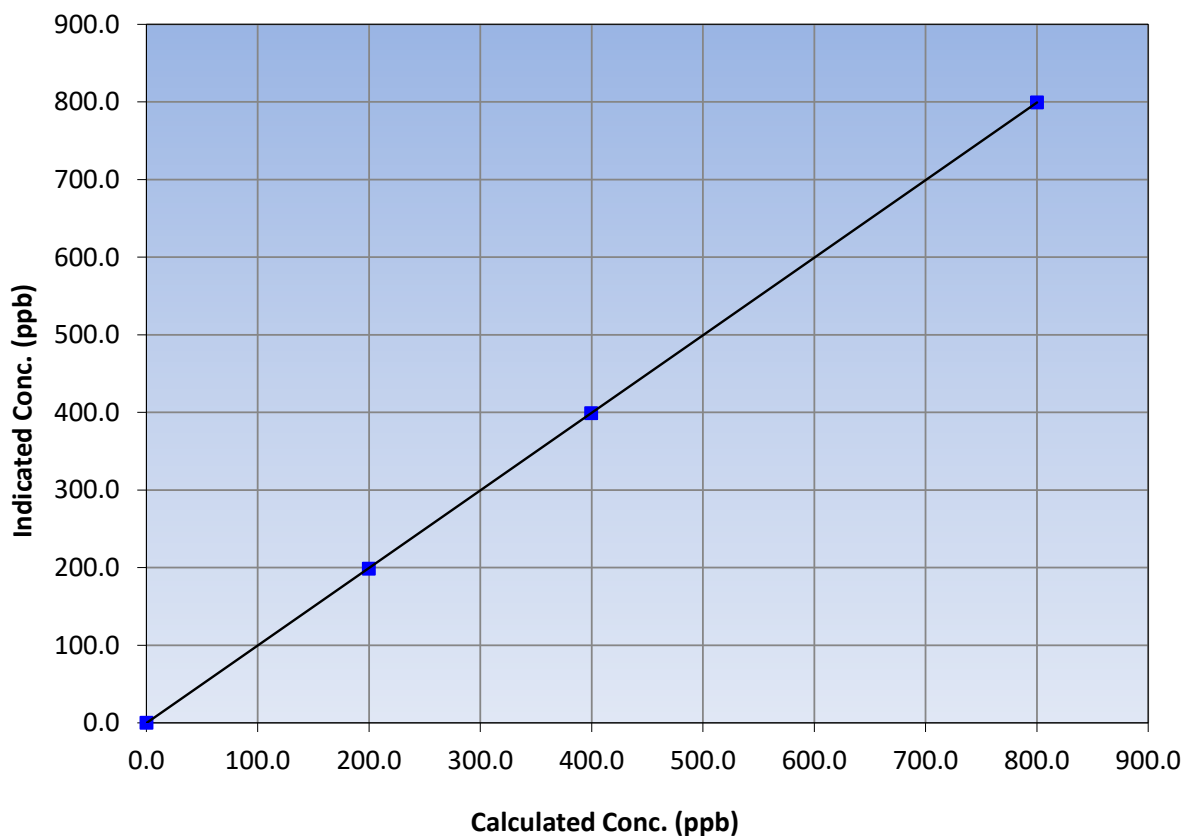



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 7, 2022
Station Name:	Fort Hills	Station Number:	AMS23
Start Time (MST):	10:04	End Time (MST):	15:17
Analyzer make:	Thermo 42i	Analyzer serial #:	1152430007

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	-0.2	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
363.7	364.0	0.9992		
178.8	179.9	0.9939		
91.6	92.2	0.9935		
			0.999989	
			1.001046	
			0.284247	

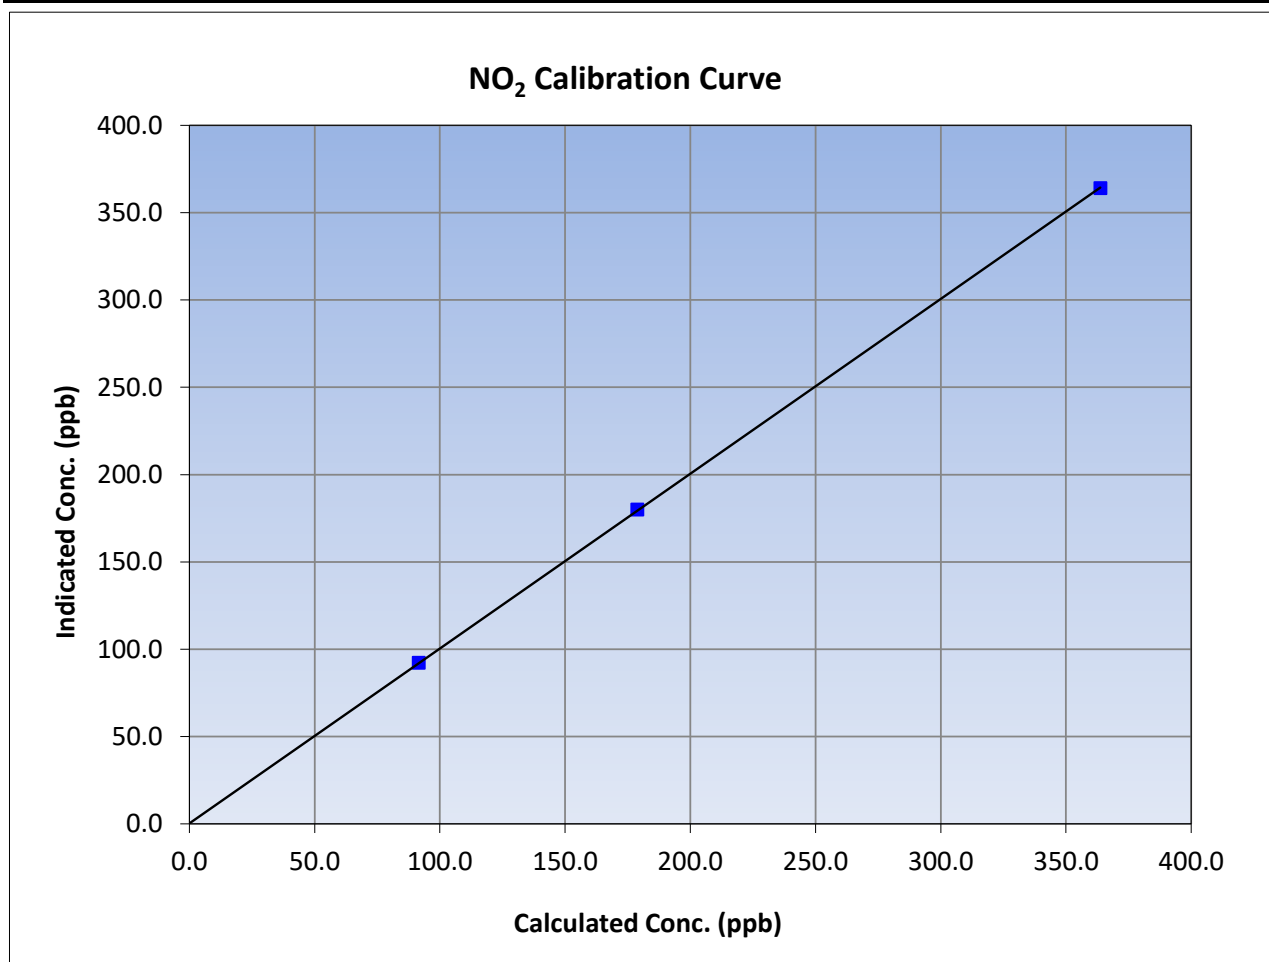

NO_x Calibration Plot

Date: January 24, 2023

Location: Fort Hills

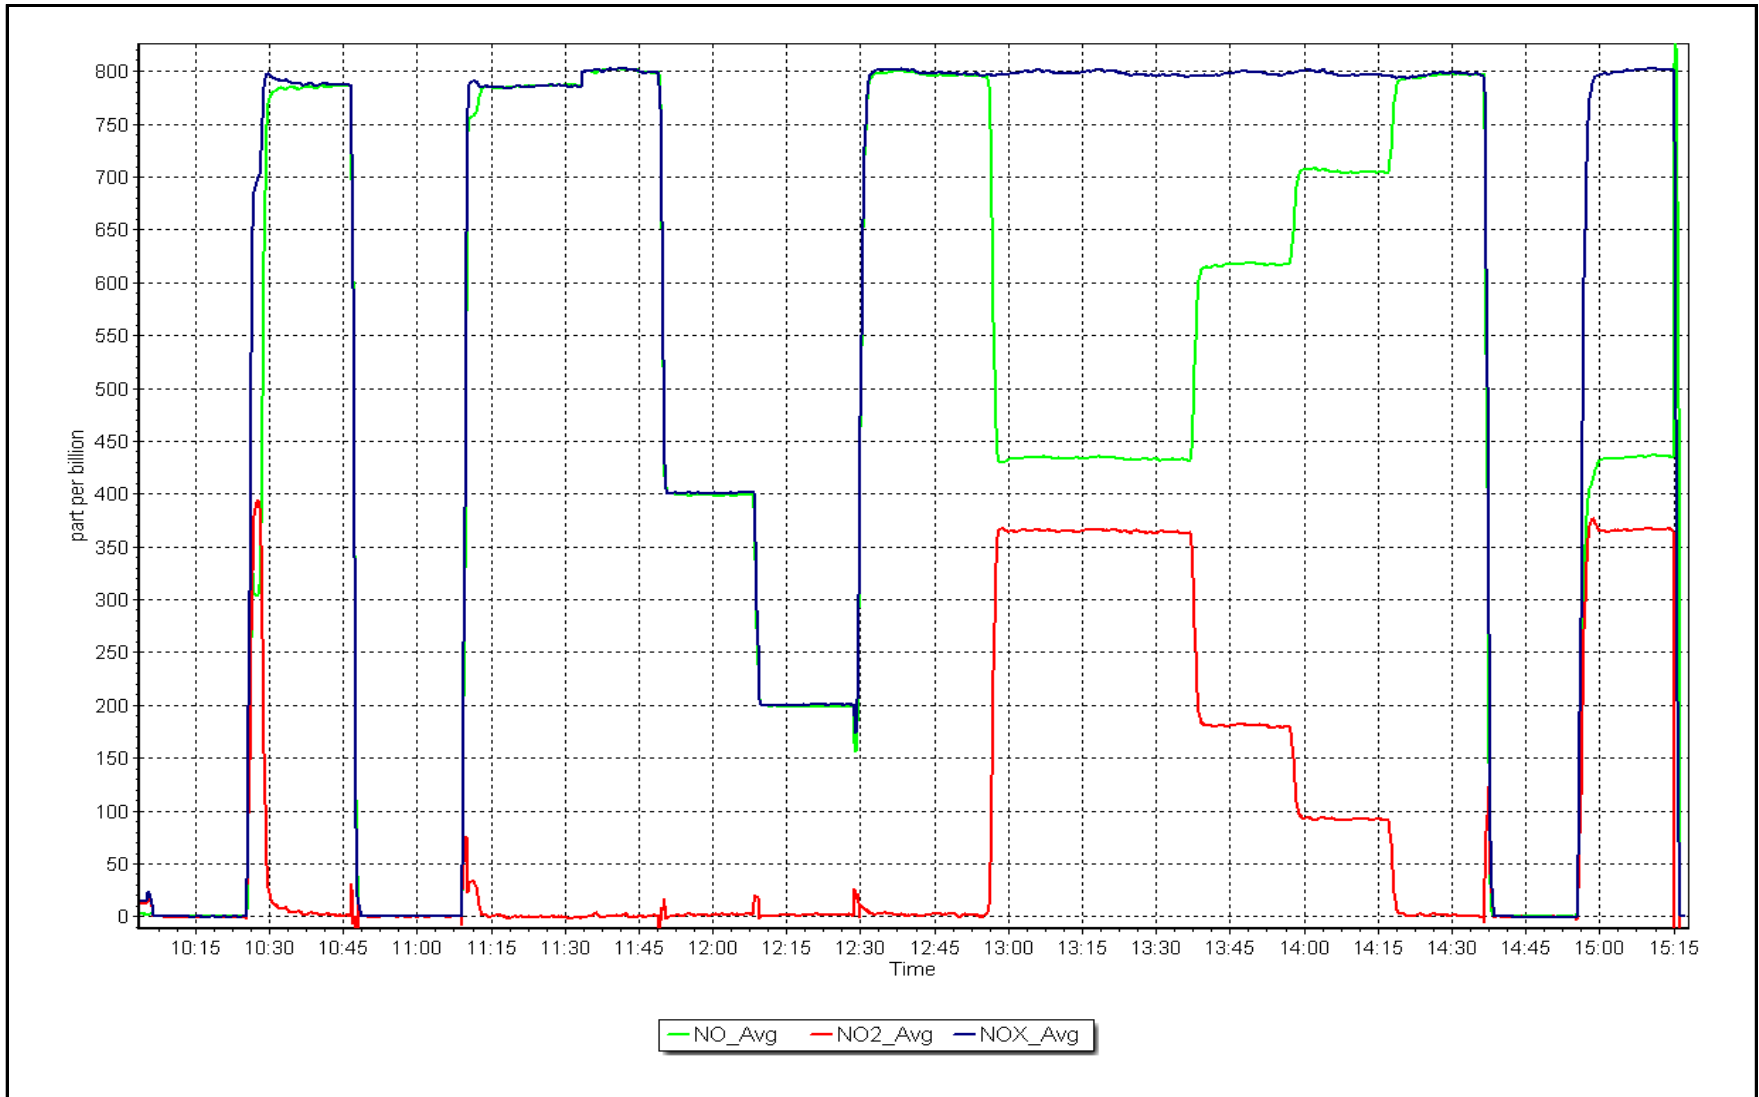



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS25 WASKŌW OHCI PIMÂTISIWIN JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Waskow ohci Pimatisiwin	Station number:	AMS25
Calibration Date:	January 3, 2023	Last Cal Date:	December 16, 2022
Start time (MST):	10:15	End time (MST):	13:10
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	52.4	ppm	Cal Gas Exp Date:	October 19, 2022
Cal Gas Cylinder #:	ET0016672			
Removed Cal Gas Conc:	52.4	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	NA		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	747
ZAG Make/Model:	API T701		Serial Number:	261

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	1118148497
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.003529	0.999783	Backgd or Offset:	9.9	11.0
Calibration intercept:	0.624937	-0.314119	Coeff or Slope:	1.212	1.212

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.9	----
as found span	4924	76.3	799.6	798.9	1.001
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.0	----
high point	4924	76.3	799.6	799.3	1.000
second point	4962	38.2	400.3	399.6	1.002
third point	4981	19.1	200.2	199.6	1.003
as left zero	5000	0.0	0.0	-0.2	----
as left span	4924	76.3	799.6	797.6	1.002
Average Correction Factor					1.002

Baseline Corr As found:	798.00	Previous response	803.02	*% change	-0.6%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Zero adjusted. No maintenance done.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 16, 2022
Station Name:	Waskow ohci Pimatisiwin	Station Number:	AMS25
Start Time (MST):	10:15	End Time (MST):	13:10
Analyzer make:	Thermo 43i	Analyzer serial #:	1118148497

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	0.999999	
799.6	799.3	1.0003			≥0.995
400.3	399.6	1.0018	Slope	0.999783	
200.2	199.6	1.0028			0.90 - 1.10
			Intercept	-0.314119	+/-30

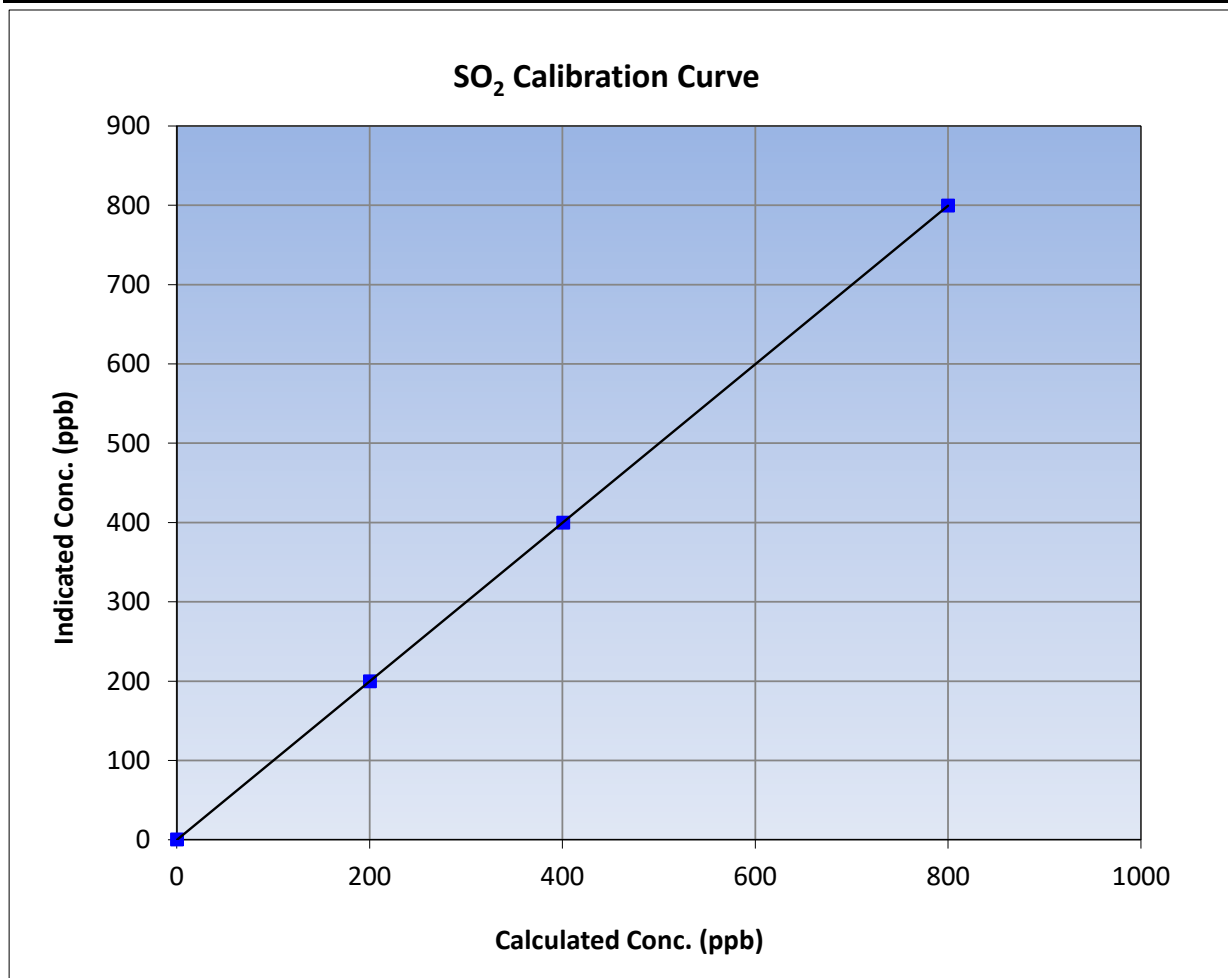

SO2 Calibration Plot

Date: January 3, 2023

Location: Waskow ohci Pimatisiwin

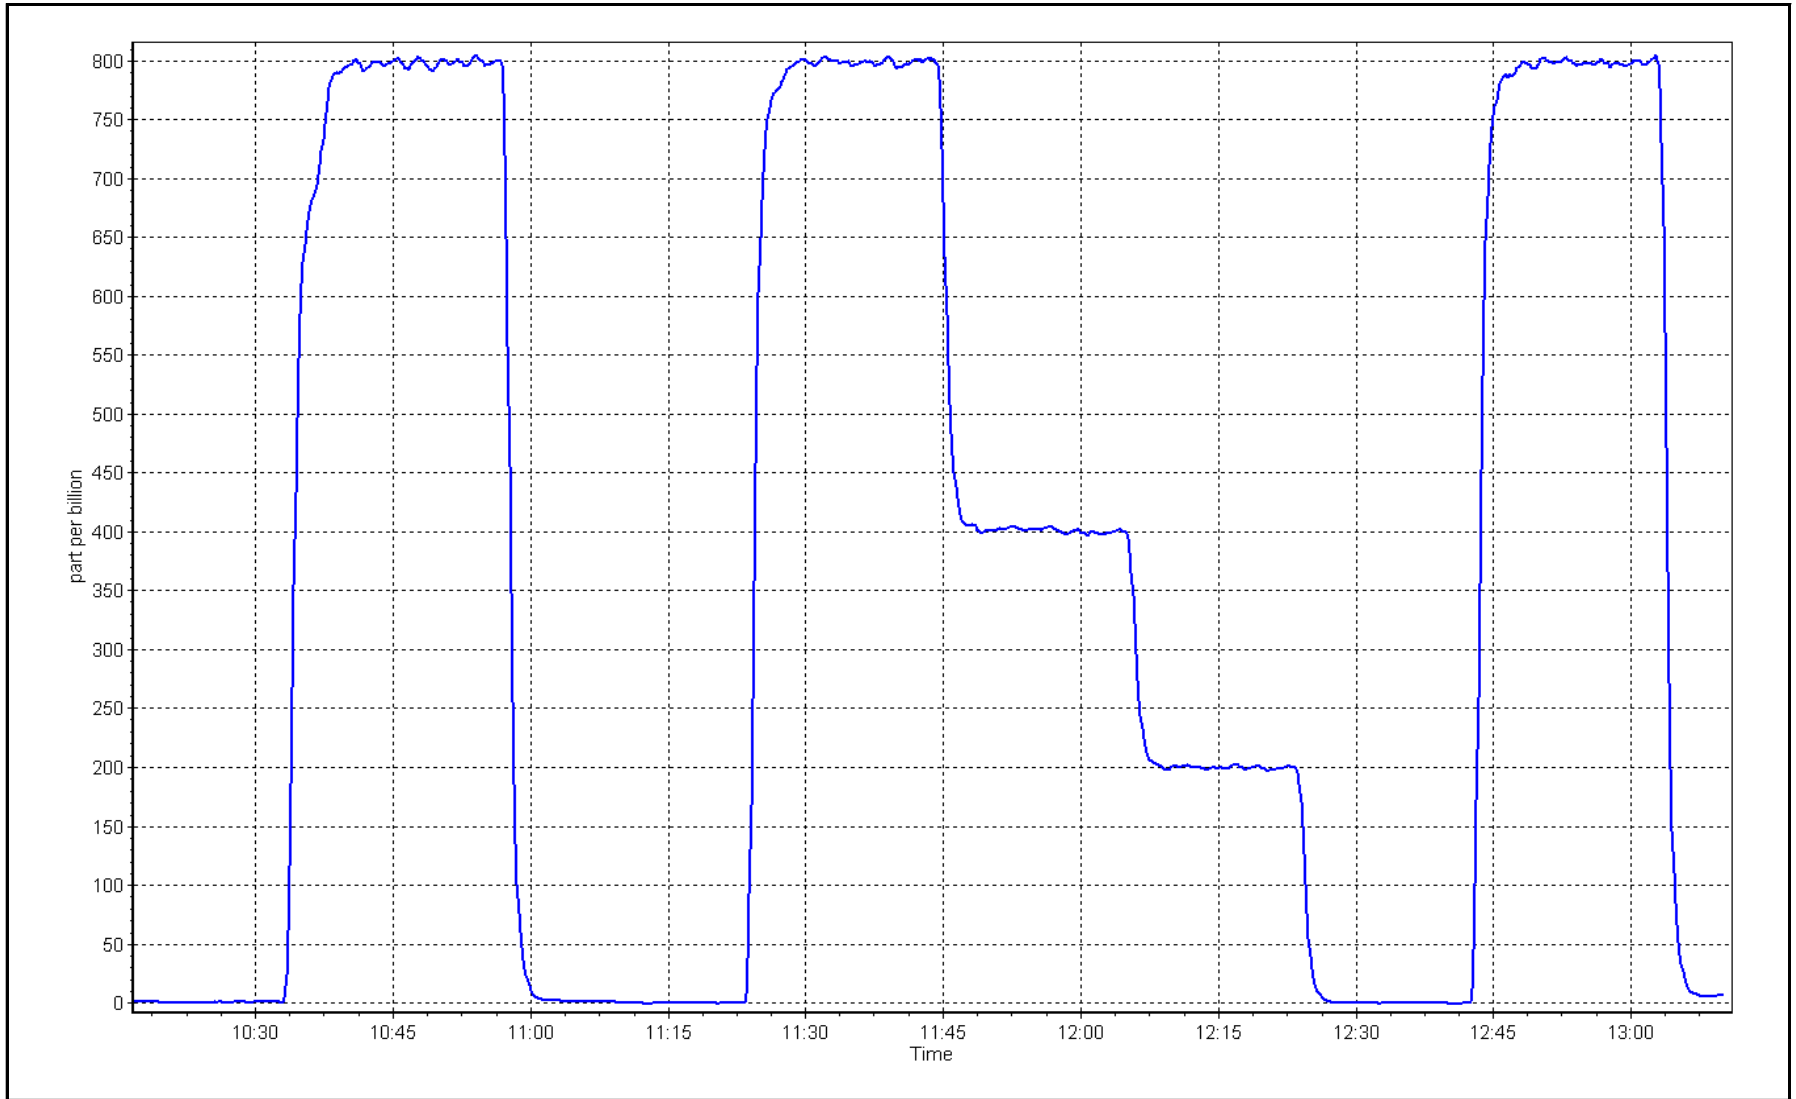



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Waskow ohci Pimatisiwin Station number: AMS25
 Calibration Date: January 11, 2023 Last Cal Date: December 7, 2022
 Start time (MST): 8:20 End time (MST): 12:44
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 4.90 ppm Cal Gas Exp Date: May 5, 2023
 Cal Gas Cylinder #: LL119538
 Removed Cal Gas Conc: 4.90 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 747
 ZAG Make/Model: API T701 Serial Number: 261

Analyzer Information

Analyzer make: Thermo 43i-LTE Analyzer serial #: 1170050146
 Converter make: Thermo 43C Converter serial #: 328702539
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	1.002595	1.002738	Backgd or Offset: 3.3	3.3
Calibration intercept:	0.421608	0.341605	Coeff or Slope: 1.085	1.085

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.2	----
as found span	4918	81.6	80.0	80.7	0.993
as found 2nd point	4959	40.8	40.0	40.5	0.992
as found 3rd point	4980	20.4	20.0	20.3	0.995
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.3	----
high point	4918	81.6	80.0	80.5	0.993
second point	4959	40.8	40.0	40.5	0.987
third point	4980	20.4	20.0	20.4	0.980
as left zero	5000	0.0	0.0	0.2	----
as left span	4912	88.3	800.0	801.2	0.999
SO2 Scrubber Check	4924	76.3	800.0	0.1	----
Date of last scrubber change:	19-Jul-10			Ave Corr Factor	0.987
Date of last converter efficiency test:	efficiency				

Baseline Corr As found: 80.5 Prev response: 80.60 *% change: -0.1%
 Baseline Corr 2nd AF pt: 40.3 AF Slope: 1.006739 AF Intercept: 0.201610
 Baseline Corr 3rd AF pt: 20.1 AF Correlation: 0.999999

* = > +/-5% change initiates investigation

Notes: Sox scrubber checked after the calibrator zero. No maintenance or adjustments done.

Calibration Performed By: Melissa Lemay



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 7, 2022
Station Name:	Waskow ohci Pimatisiwin	Station Number:	AMS25
Start Time (MST):	8:20	End Time (MST):	12:44
Analyzer make:	Thermo 43i-LTE	Analyzer serial #:	1170050146

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	0.999998	
80.0	80.5	0.9935			≥0.995
40.0	40.5	0.9873	Slope	1.002738	
20.0	20.4	0.9799			0.90 - 1.10
			Intercept	0.341605	+/-3

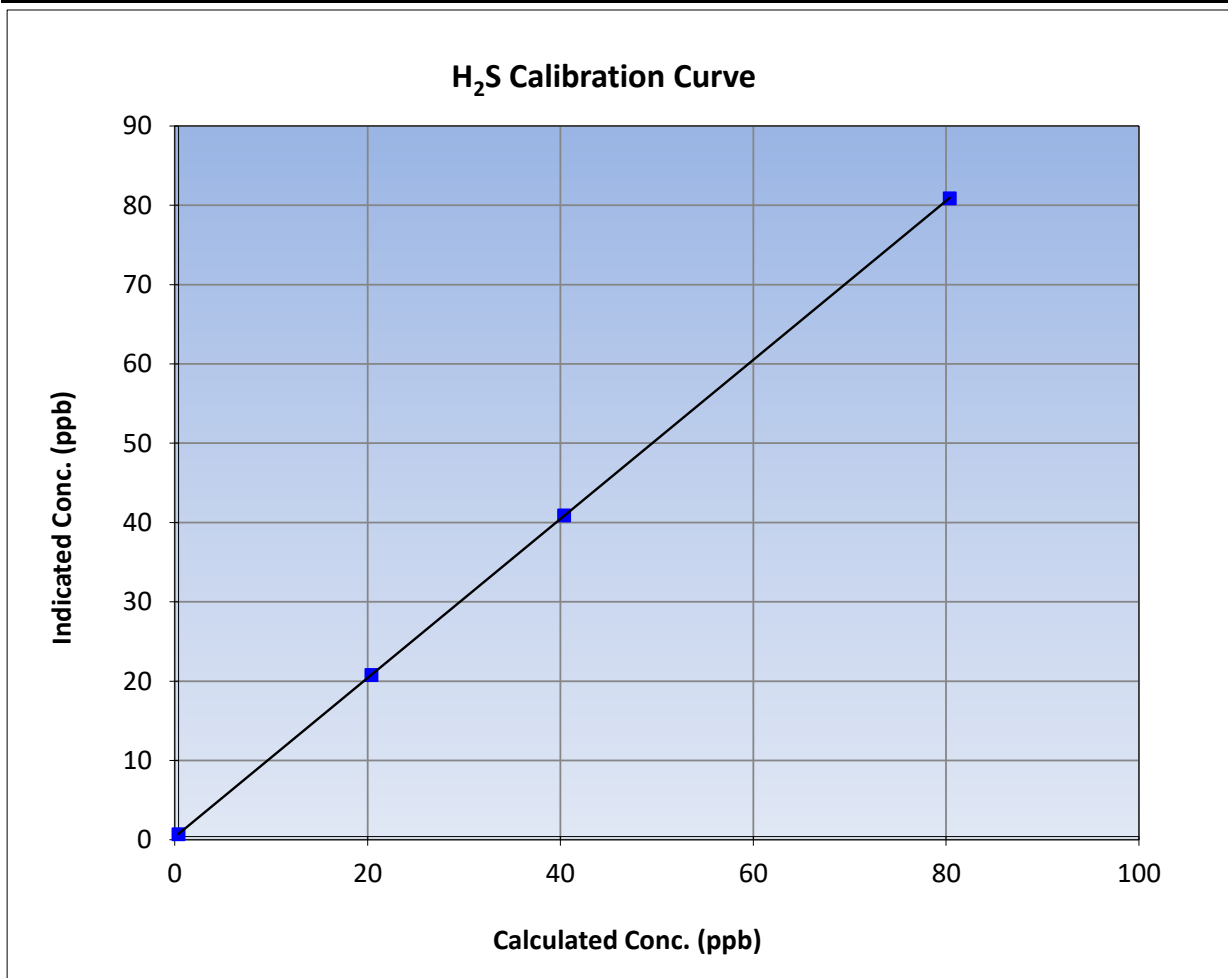

H₂S Calibration Plot

Date: January 11, 2023

Location: Waskow ohci Pimatisiwin

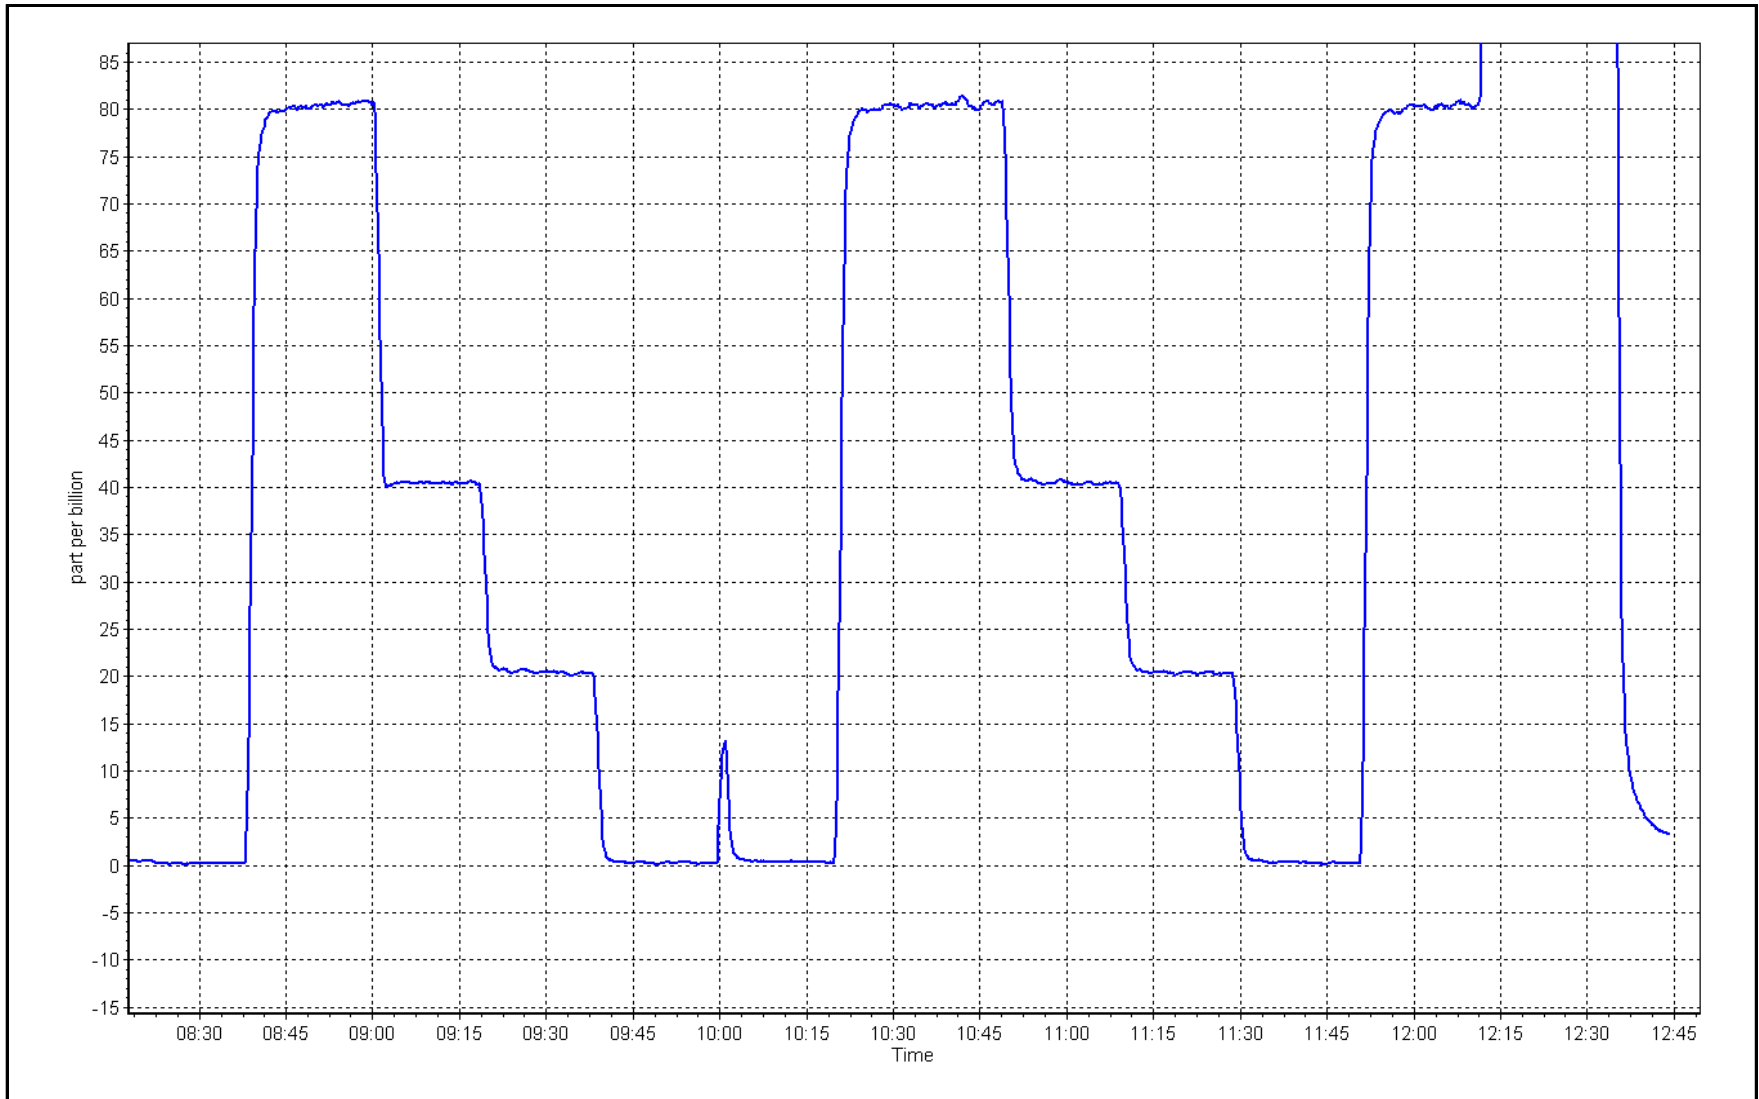



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS26 CHRISTINA LAKE JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 25, 2023	Previous Calibration:	December 15, 2022
Station Name:	Christina Lake	Station Number:	AMS 26
Start Time (MST):	8:40	End Time (MST):	12:54
Analyzer make:	Thermo 43i	Analyzer serial #:	1173410001

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	-0.1	----	Correlation Coefficient	0.999943	
799.0	797.9	1.0013			≥0.995
399.4	396.1	1.0084	Slope	1.000779	
200.2	194.3	1.0304			0.90 - 1.10
			Intercept	-2.876133	+/-30

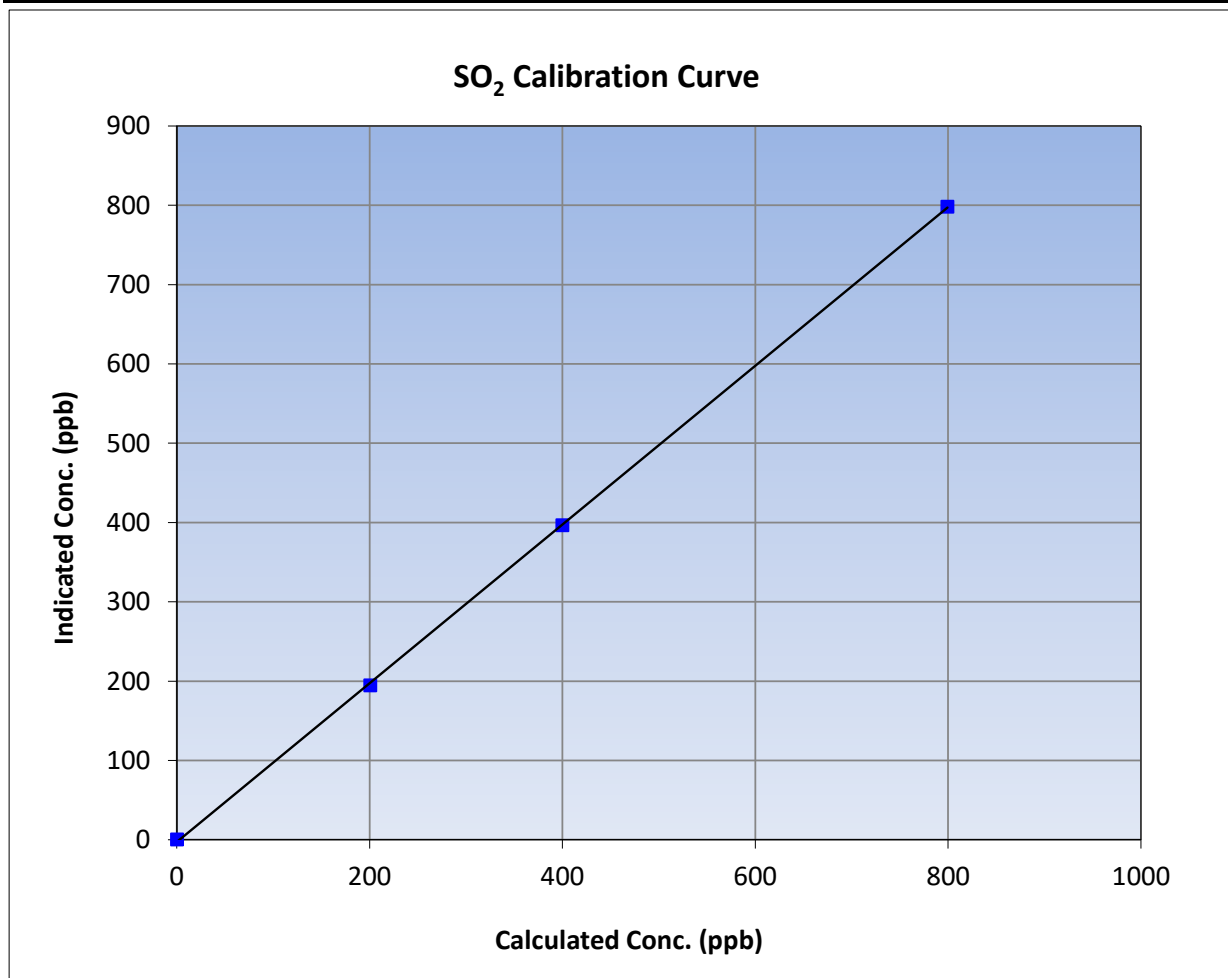

SO2 Calibration Plot

Date: January 25, 2023

Location: Christina Lake

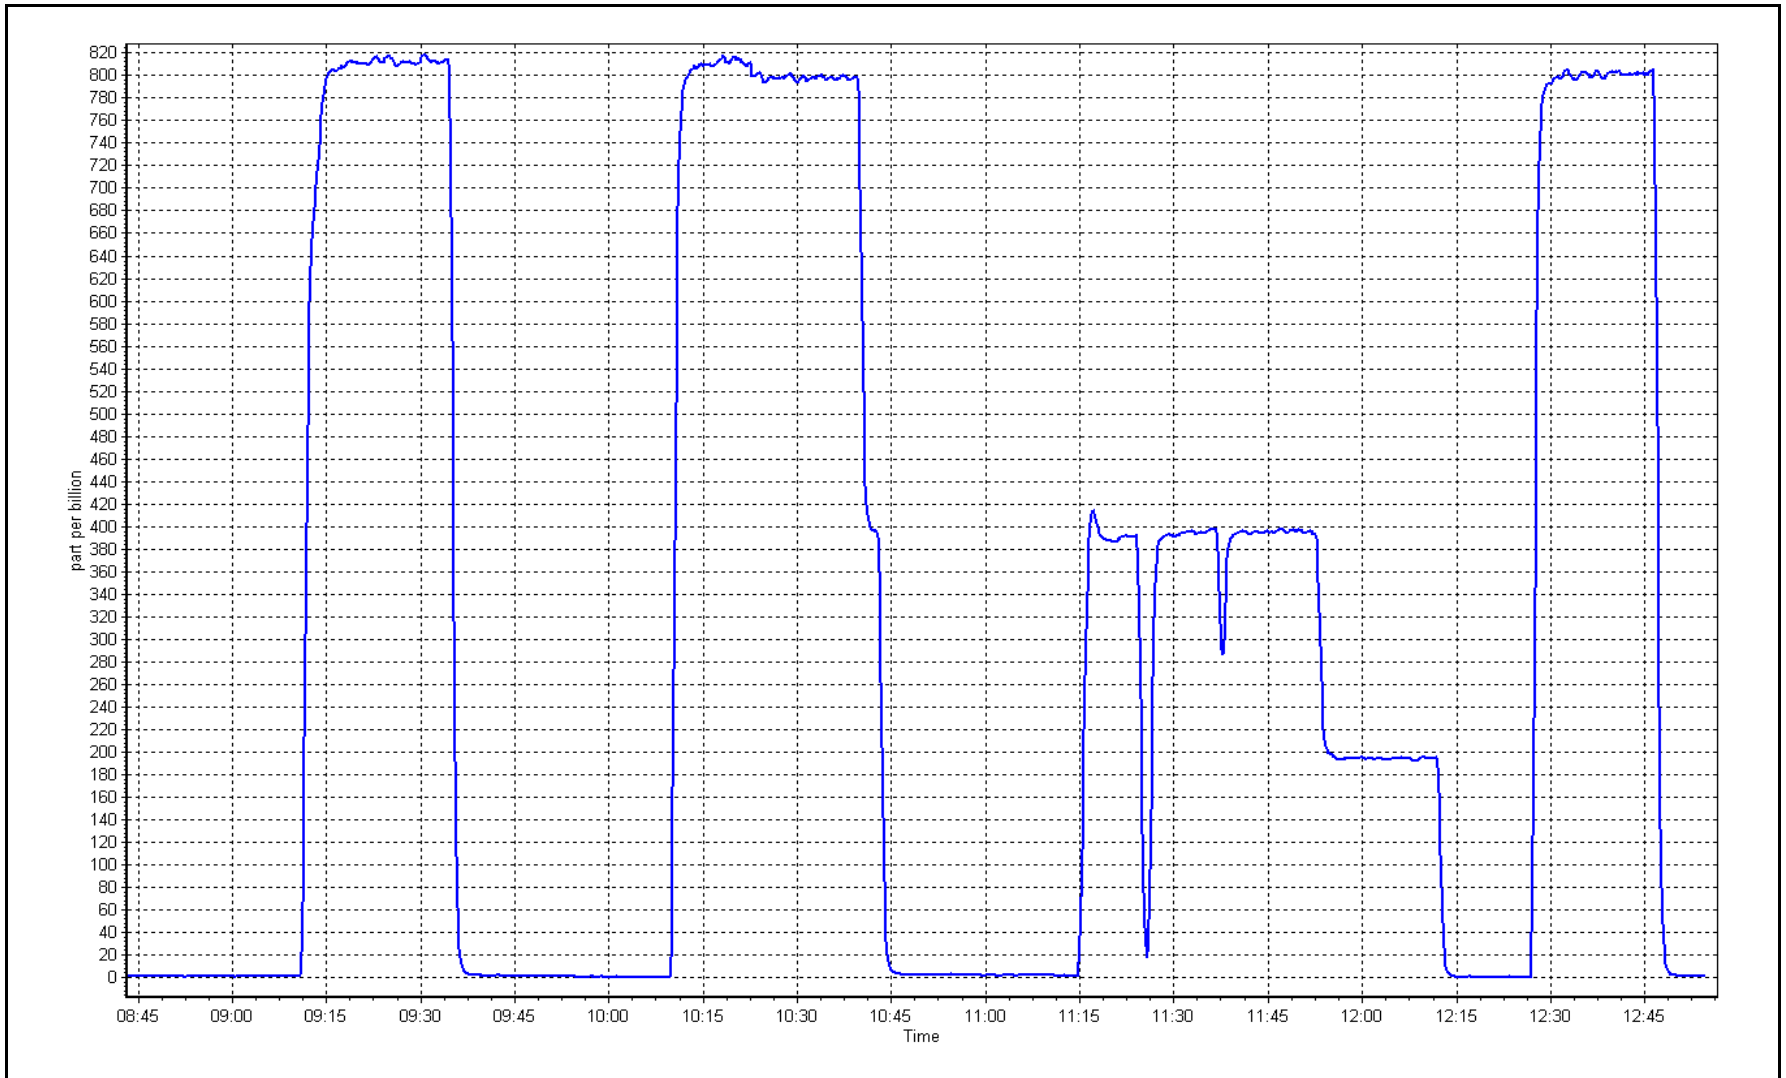



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Christina Lake Station number: AMS26
 Calibration Date: January 25, 2023 Last Cal Date: December 13, 2022
 Start time (MST): 8:40 End time (MST): 13:36
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 4.89 ppm Cal Gas Exp Date: February 9, 2024
 Cal Gas Cylinder #: EY0002466
 Removed Cal Gas Conc: 4.89 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T750 Serial Number: 282
 ZAG Make/Model: API T751H Serial Number: 322

Analyzer Information

Analyzer make: Thermo 450i Analyzer serial #: 1180030032
 Converter make: NA Converter serial #: NA
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.993615	1.010037	Backgd or Offset: 33.3	33.3
Calibration intercept:	-0.141127	0.159267	Coeff or Slope: 1.113	1.113

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	-0.2	----
as found span	4918	81.8	80.0	80.8	0.988
as found 2nd point	4959	40.9	40.0	40.3	0.988
as found 3rd point	4979	20.4	20.0	20.0	0.988
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.2	----
high point	4918	81.8	80.0	81.0	0.988
second point	4959	40.9	40.0	40.5	0.988
third point	4979	20.4	20.0	20.3	0.983
as left zero	5000	0.0	0.0	0.2	----
as left span	4918	81.8	80.0	80.2	0.998
SO2 Scrubber Check	4919	80.6	806.1	0.0	----
Date of last scrubber change:	27-Feb-19			Ave Corr Factor	0.986
Date of last converter efficiency test:					efficiency

Baseline Corr As found: 81.0 Prev response: 79.35 *% change: 2.0%
 Baseline Corr 2nd AF pt: 40.5 AF Slope: 1.012465 AF Intercept: -0.200681
 Baseline Corr 3rd AF pt: 20.2 AF Correlation: 1.000000

* = > +/-5% change initiates investigation

Notes: Ran scrubber check after calibrator zero. No adjustments made.

Calibration Performed By: Braiden Boutillier



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 25, 2023	Previous Calibration:	December 13, 2022
Station Name:	Christina Lake	Station Number:	AMS26
Start Time (MST):	8:40	End Time (MST):	13:36
Analyzer make:	Thermo 450i	Analyzer serial #:	1180030032

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999998	
80.0	81.0	0.9877			≥0.995
40.0	40.5	0.9877	Slope	1.010037	
20.0	20.3	0.9829			0.90 - 1.10
			Intercept	0.159267	+/-3

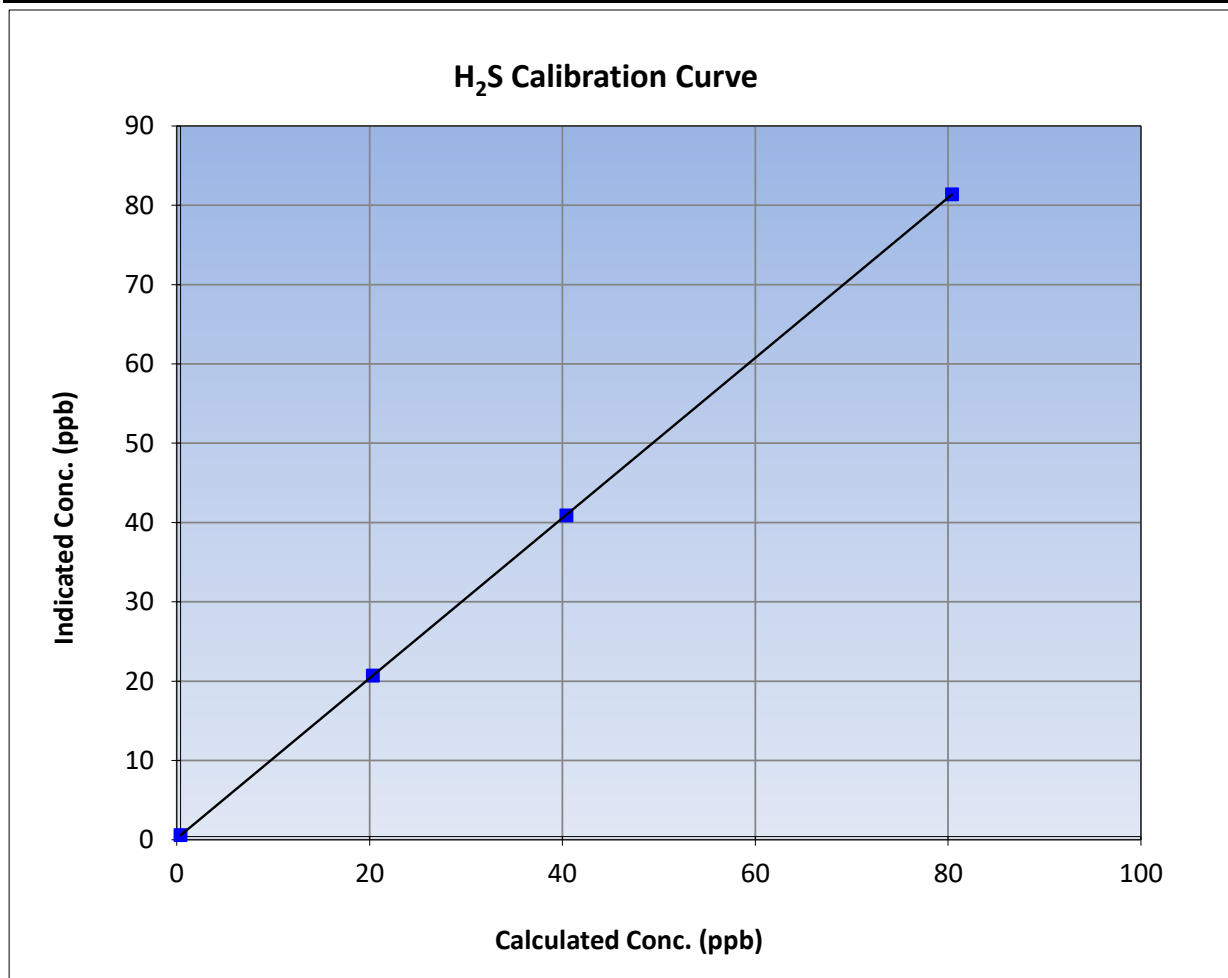

H₂S Calibration Plot

Date: January 25, 2023

Location: Christina Lake

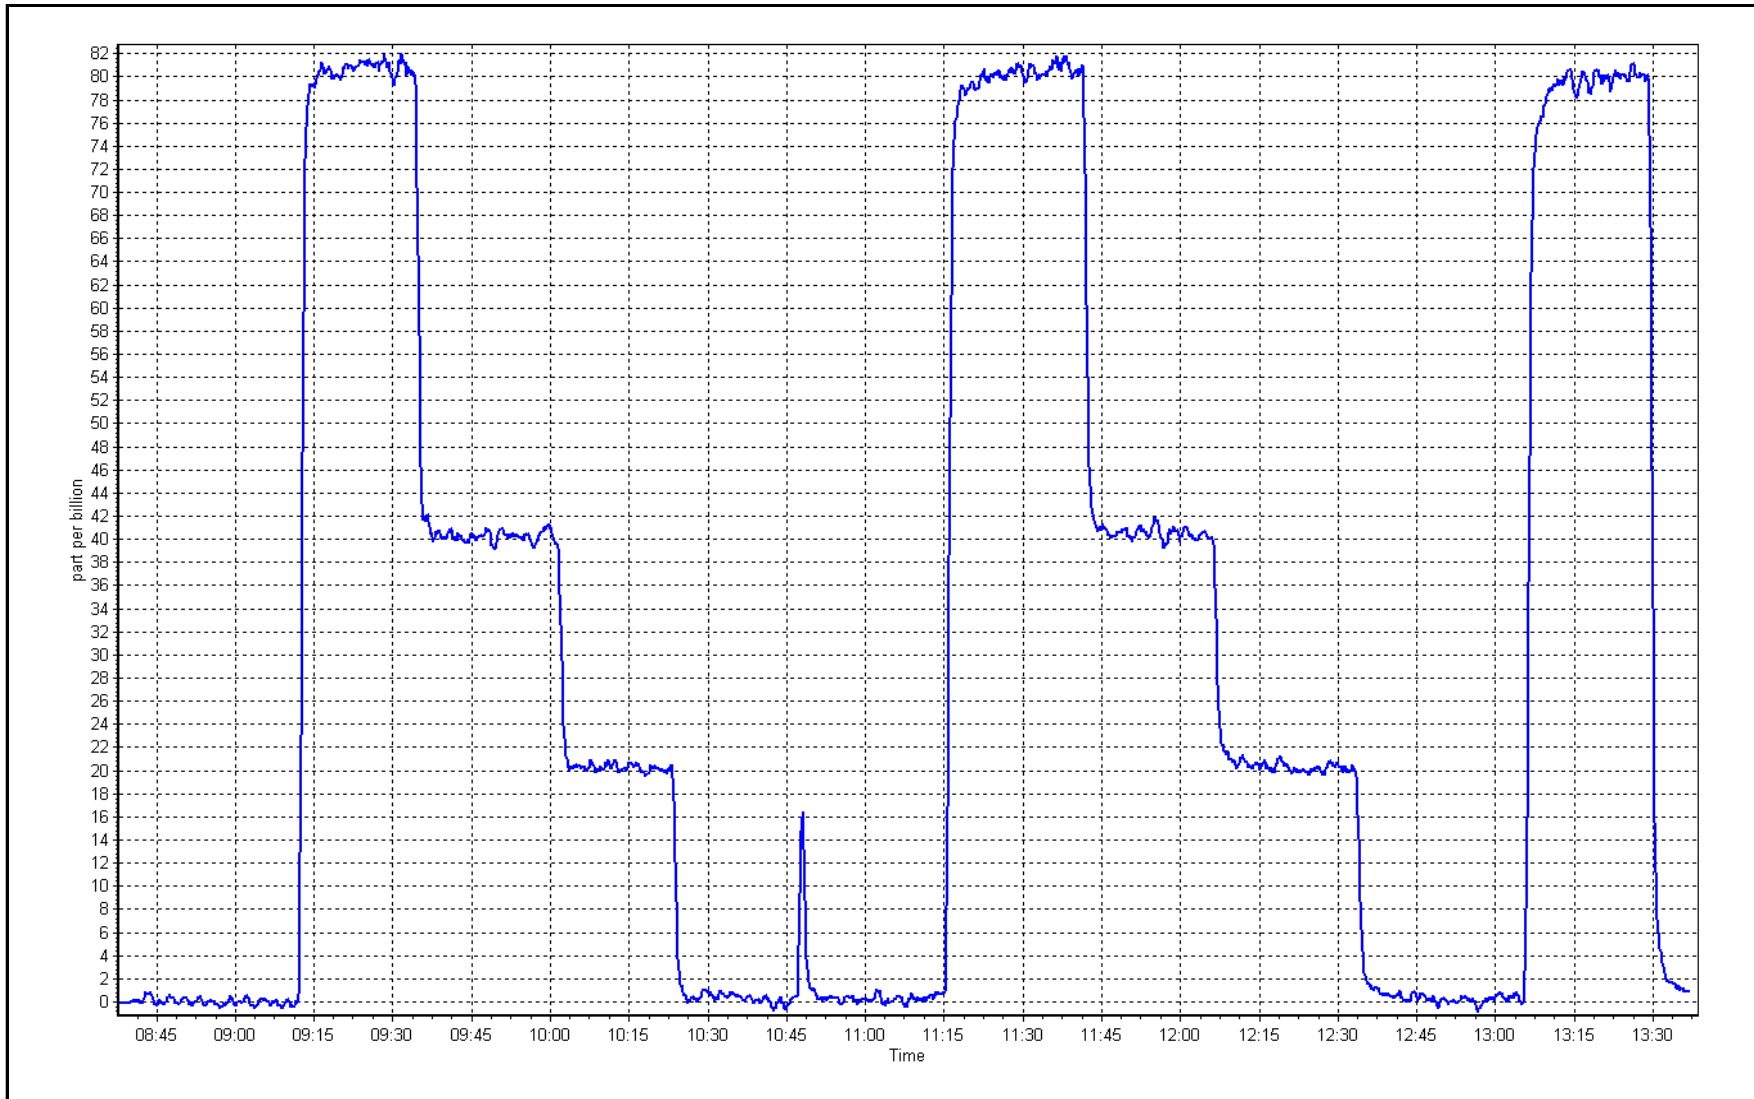



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.0	0.0	0.0	----	----
as found span	4920	80.0	813.1	800.3	12.8	805.0	791.5	13.2	1.0101	1.0111
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.1	0.0	0.0	----	----
high point	4920	80.0	813.1	800.3	12.8	812.0	799.6	12.1	1.0014	1.0009
second point	4960	40.0	406.6	400.2	6.4	402.9	395.1	7.8	1.0091	1.0128
third point	4980	20.0	203.3	200.1	3.2	198.4	194.3	4.1	1.0246	1.0297
as left zero	5000	0.0	0.0	0.0	0.0	0.1	0.1	0.0	----	----
as left span	4920	80.0	813.1	392.5	420.6	812.0	387.4	424.2	1.0014	1.0132
Average Correction Factor									1.0117	1.0145

Corrected As found	NO _x = 805.0 ppb	NO = 791.5 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -0.7%
Previous Response	NO _x = 810.9 ppb	NO = 798.2 ppb		*Percent Change	NO = -0.8%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	795.9	388.1	420.6	419.5	1.0026	99.7%
2nd GPT point (200 ppb O3)	795.9	596.1	212.6	211.3	1.0062	99.4%
3rd GPT point (100 ppb O3)	795.9	698.9	109.8	109.3	1.0046	99.5%
Average Correction Factor					1.0044	99.6%

Notes: Changed sample inlet filter after as founds. Adjusted span only.

Calibration Performed By: Braiden Boutilier



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 14, 2022
Station Name:	Christina Lake	Station Number:	AMS 26
Start Time (MST):	11:33	End Time (MST):	16:36
Analyzer make:	Thermo 42i	Analyzer serial #:	14:00

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>
0.0	0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
813.1	812.0	1.0014		
406.6	402.9	1.0091		
203.3	198.4	1.0246		

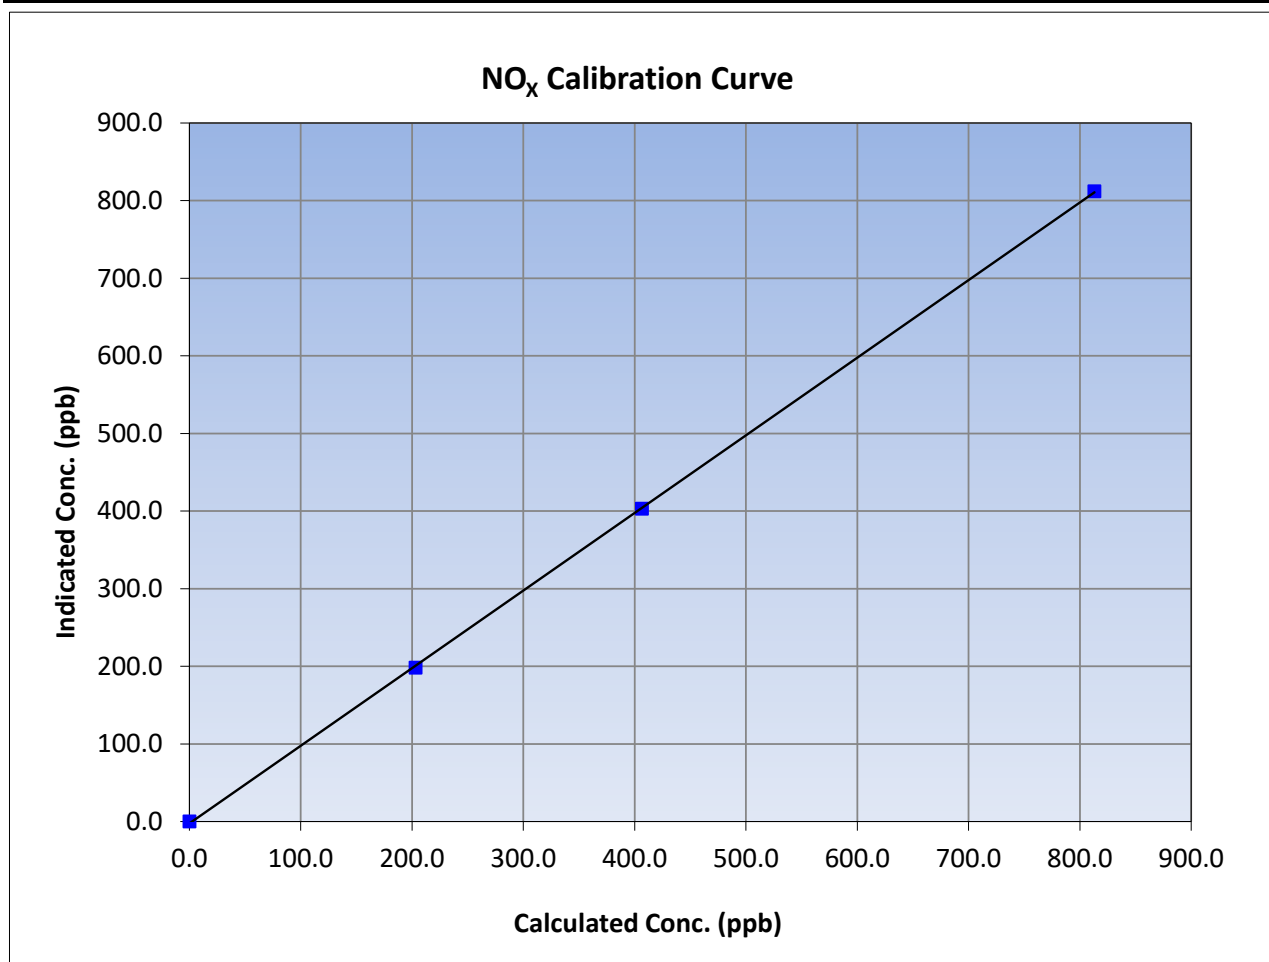



Wood Buffalo Environmental Association

NO Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 14, 2022
Station Name:	Christina Lake	Station Number:	AMS 26
Start Time (MST):	11:33	End Time (MST):	16:36
Analyzer make:	Thermo 42i	Analyzer serial #:	14:00

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥ 0.995 $0.90 - 1.10$ $+/-20$
800.3	799.6	1.0009		
400.2	395.1	1.0128		
200.1	194.3	1.0297		

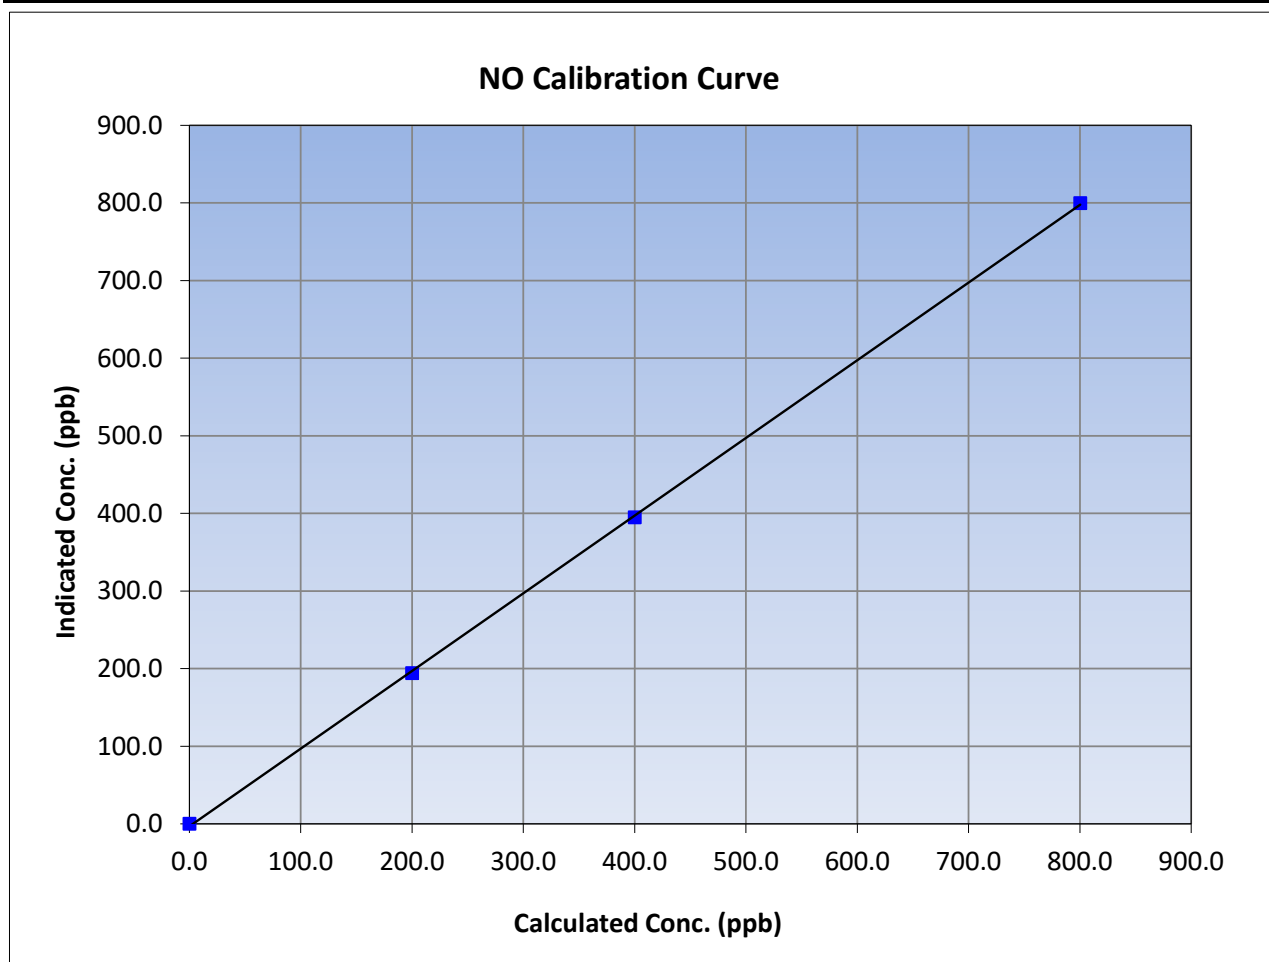



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 14, 2022
Station Name:	Christina Lake	Station Number:	AMS 26
Start Time (MST):	11:33	End Time (MST):	16:36
Analyzer make:	Thermo 42i	Analyzer serial #:	14:00

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
420.6	419.5	1.0026		
212.6	211.3	1.0062		
109.8	109.3	1.0046		

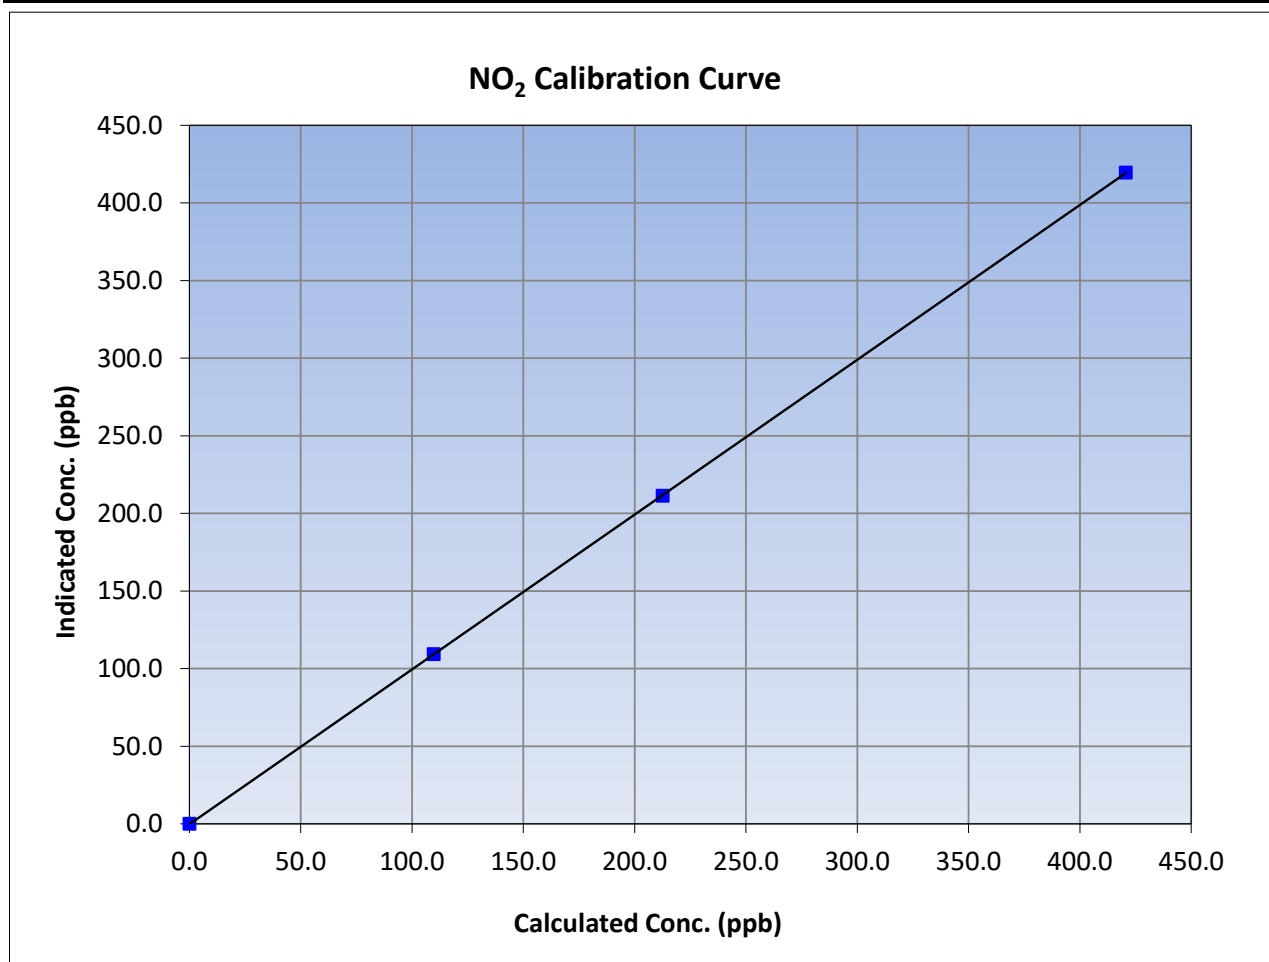

NO_x Calibration Plot

Date: January 24, 2023

Location: Christina Lake

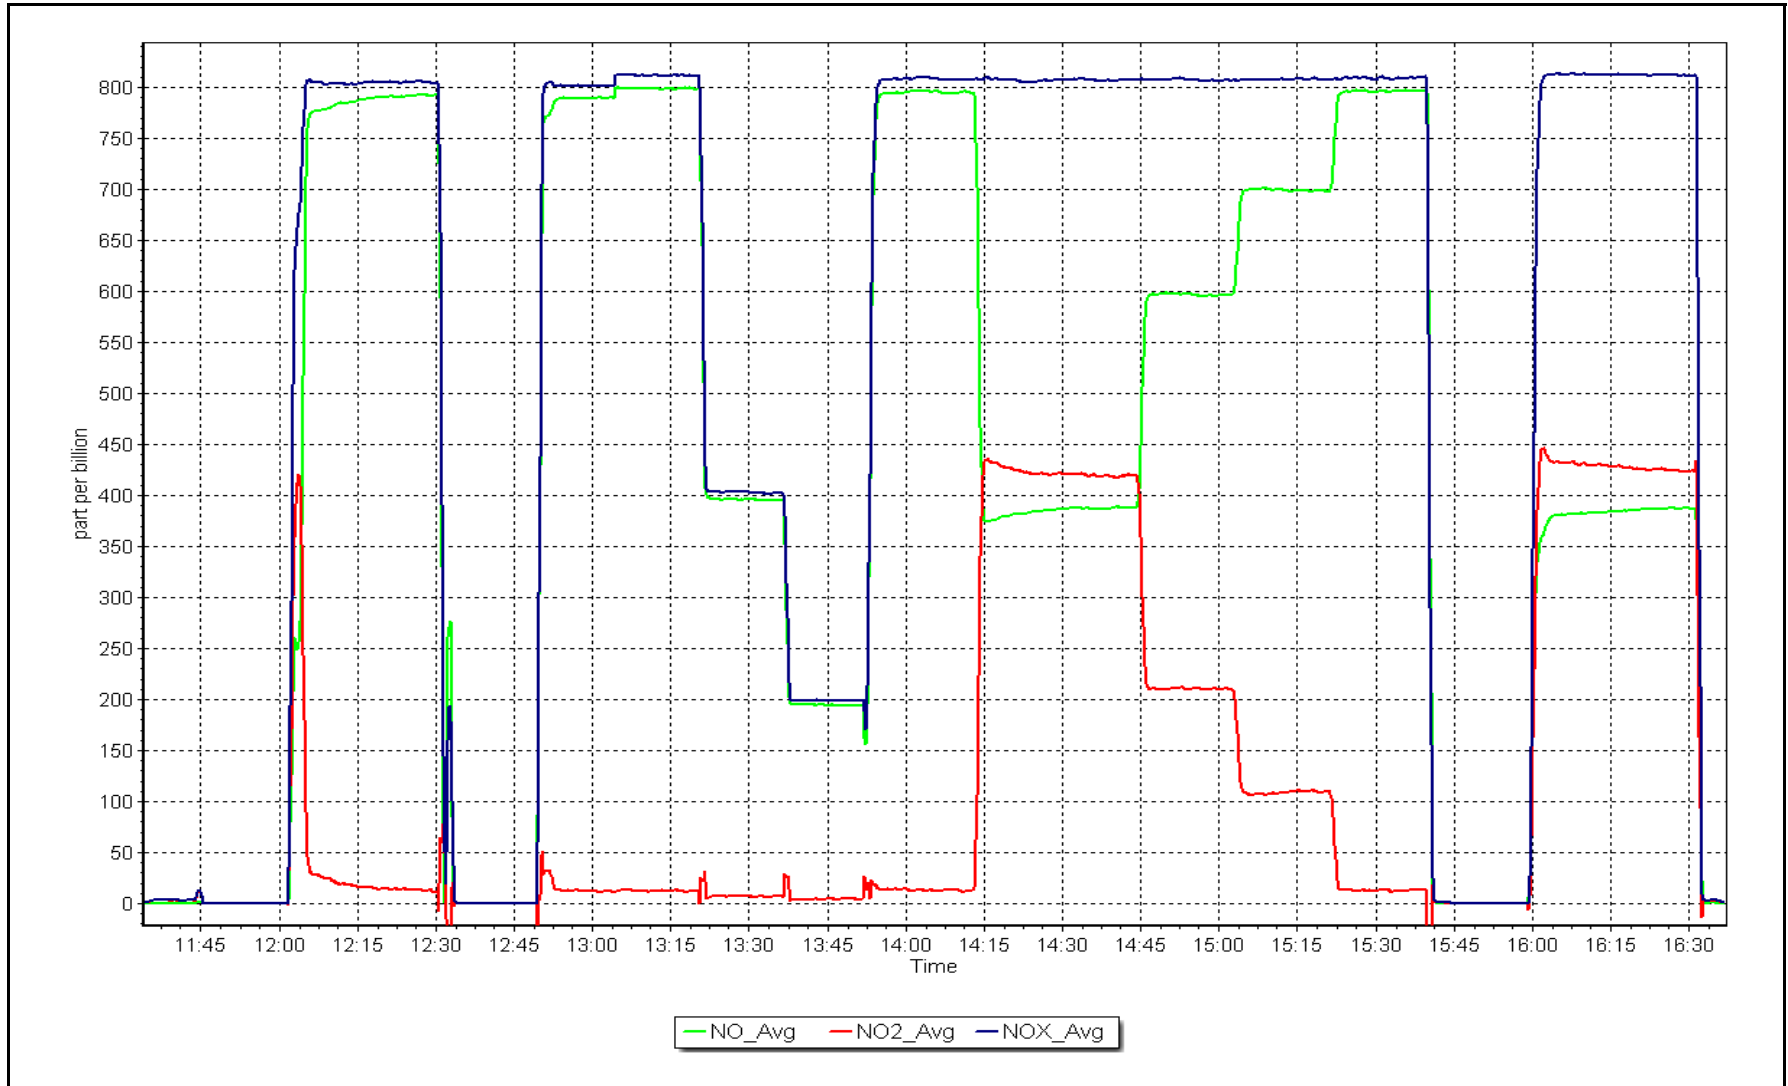



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS27
JACKFISH 2/3
JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Jackfish 2/3	Station number:	AMS 27
Calibration Date:	January 19, 2023	Last Cal Date:	December 8, 2022
Start time (MST):	10:10	End time (MST):	12:45
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	50.58	ppm	Cal Gas Exp Date:	December 29, 2028
Cal Gas Cylinder #:	<u>SG9133974BAL</u>			
Removed Cal Gas Conc:	50.58	ppm	Rem Gas Exp Date:	NA
Removed Gas Cyl #:	<u>NA</u>		Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	3811
ZAG Make/Model:	API 701		Serial Number:	364

Analyzer Information

Analyzer make:	Thero 43iQ	Analyzer serial #:	12124313138
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.001034	1.001858	Backgd or Offset:	7.6	7.4
Calibration intercept:	-1.838597	-1.876897	Coeff or Slope:	1.002	0.979

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	----
as found span	4921	79.1	800.2	815.0	0.982
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	0.2	----
high point	4921	79.1	800.2	800.1	1.000
second point	4961	39.5	399.5	399.5	1.000
third point	4980	19.8	200.3	195.3	1.026
as left zero	5000	0.0	0.0	0.2	----
as left span	4921	79.1	800.2	800.2	1.000
Average Correction Factor					1.009

Baseline Corr As found:	815.00	Previous response	799.15	*% change	1.9%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Adjusted the span only.

Calibration Performed By: Denny Ray Estador



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 19, 2023	Previous Calibration:	December 8, 2022
Station Name:	Jackfish 2/3	Station Number:	AMS 27
Start Time (MST):	10:10	End Time (MST):	12:45
Analyzer make:	Thero 43iQ	Analyzer serial #:	12124313138

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.2	----	Correlation Coefficient	0.999949	
800.2	800.1	1.0001			≥0.995
399.5	399.5	1.0001	Slope	1.001858	
200.3	195.3	1.0256			0.90 - 1.10
			Intercept	-1.876897	+/-30

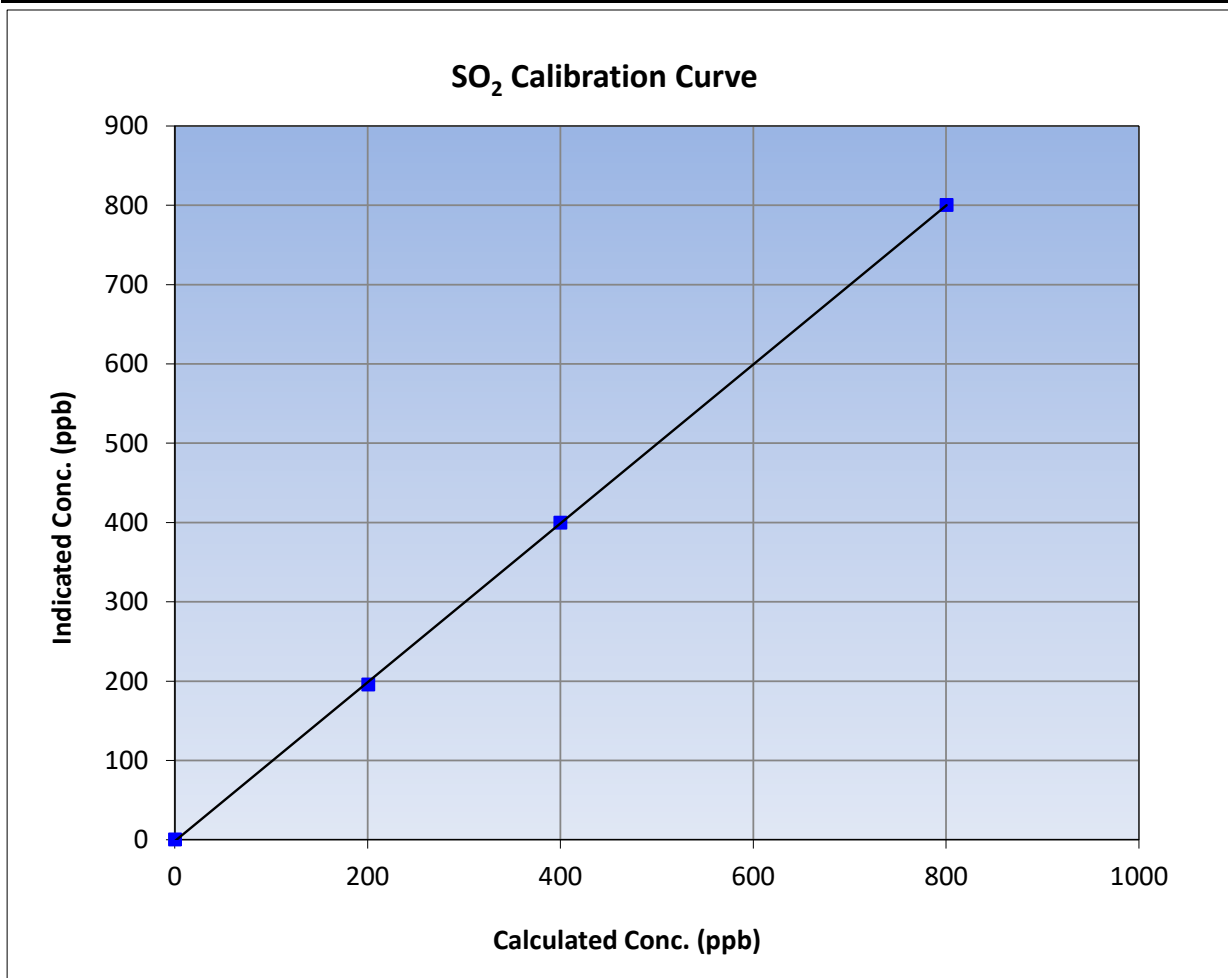

SO2 Calibration Plot

Date: January 19, 2023

Location: Jackfish 2/3

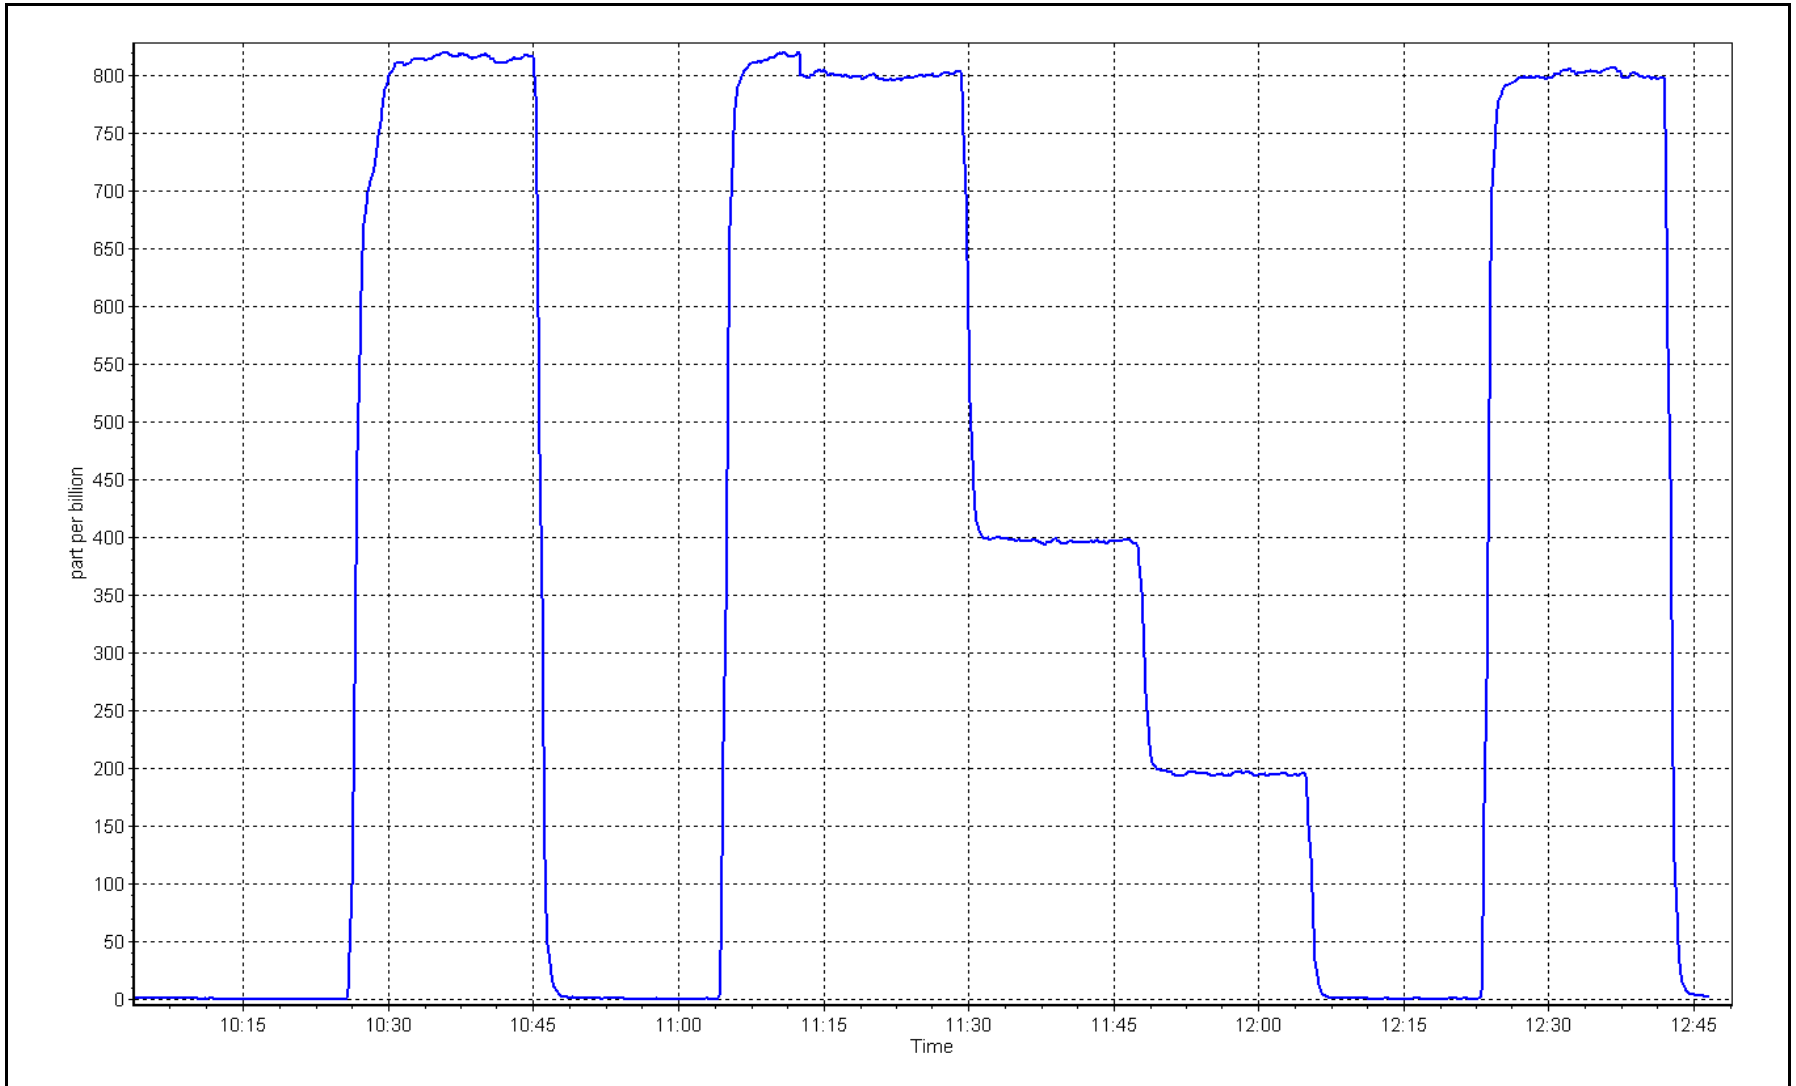



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Jackfish 2/3 Station number: AMS27
 Calibration Date: January 11, 2023 Last Cal Date: December 14, 2022
 Start time (MST): 10:13 End time (MST): 13:40
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.41 ppm Cal Gas Exp Date: January 4, 2025
 Cal Gas Cylinder #: CC345023
 Removed Cal Gas Conc: 5.41 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 3811
 ZAG Make/Model: API 701 Serial Number: 364

Analyzer Information

Analyzer make: API T101 Analyzer serial #: 621
 Converter make: Converter serial #:
 Analyzer Range 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	1.003337	0.997920	Backgd or Offset: 24.3	24.3
Calibration intercept:	-0.197871	0.042016	Coeff or Slope: 0.965	0.965

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.2	----
as found span	4926	74.1	80.2	81.0	0.992
as found 2nd point	4963	37.0	40.0	40.2	1.001
as found 3rd point	4982	18.5	20.0	19.9	1.016
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.2	----
high point	4926	74.1	80.2	80.1	1.001
second point	4963	37.0	40.0	40.0	1.001
third point	4982	18.5	20.0	19.8	1.011
as left zero	5000	0.0	0.0	0.3	----
as left span	4926	74.1	80.2	80.0	1.002
SO2 Scrubber Check	4921	79.1	791.0	0.1	----
Date of last scrubber change:				Ave Corr Factor	1.004
Date of last converter efficiency test:				efficiency	

Baseline Corr As found: 80.8 Prev response: 80.24 *% change: 0.7%
 Baseline Corr 2nd AF pt: 40.0 AF Slope: 1.009326 AF Intercept: -0.057823
 Baseline Corr 3rd AF pt: 19.7 AF Correlation: 0.999953

* = > +/-5% change initiates investigation

Notes: No adjustments have been made.

Calibration Performed By: Denny Ray Estador



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 14, 2022
Station Name:	Jackfish 2/3	Station Number:	AMS27
Start Time (MST):	10:13	End Time (MST):	13:40
Analyzer make:	API T101	Analyzer serial #:	621

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999979	≥0.995
80.2	80.1	1.0009			
40.0	40.0	1.0009	Slope	0.997920	0.90 - 1.10
20.0	19.8	1.0109			
			Intercept	0.042016	+/-3

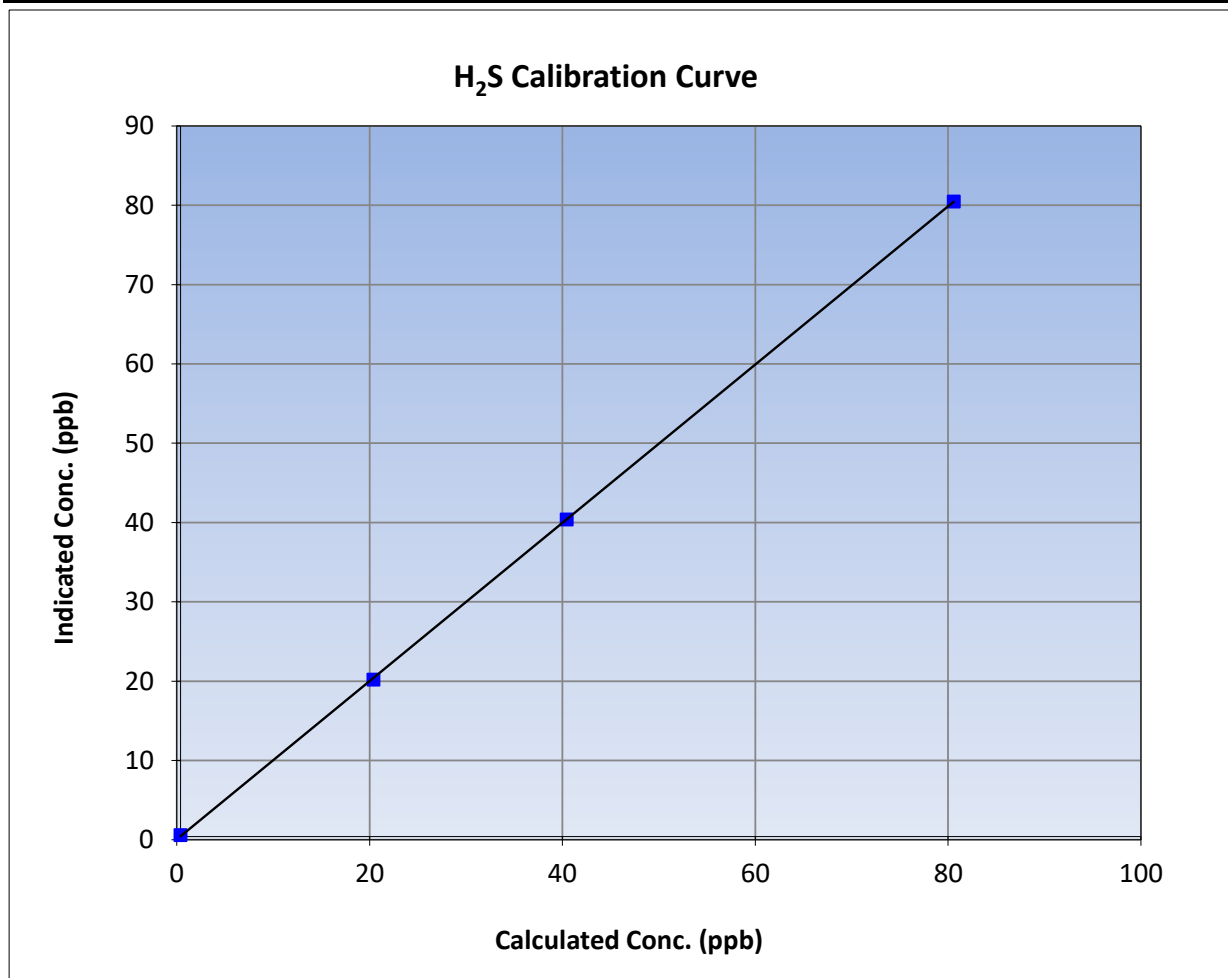

H₂S Calibration Plot

Date: January 11, 2023

Location: Jackfish 2/3

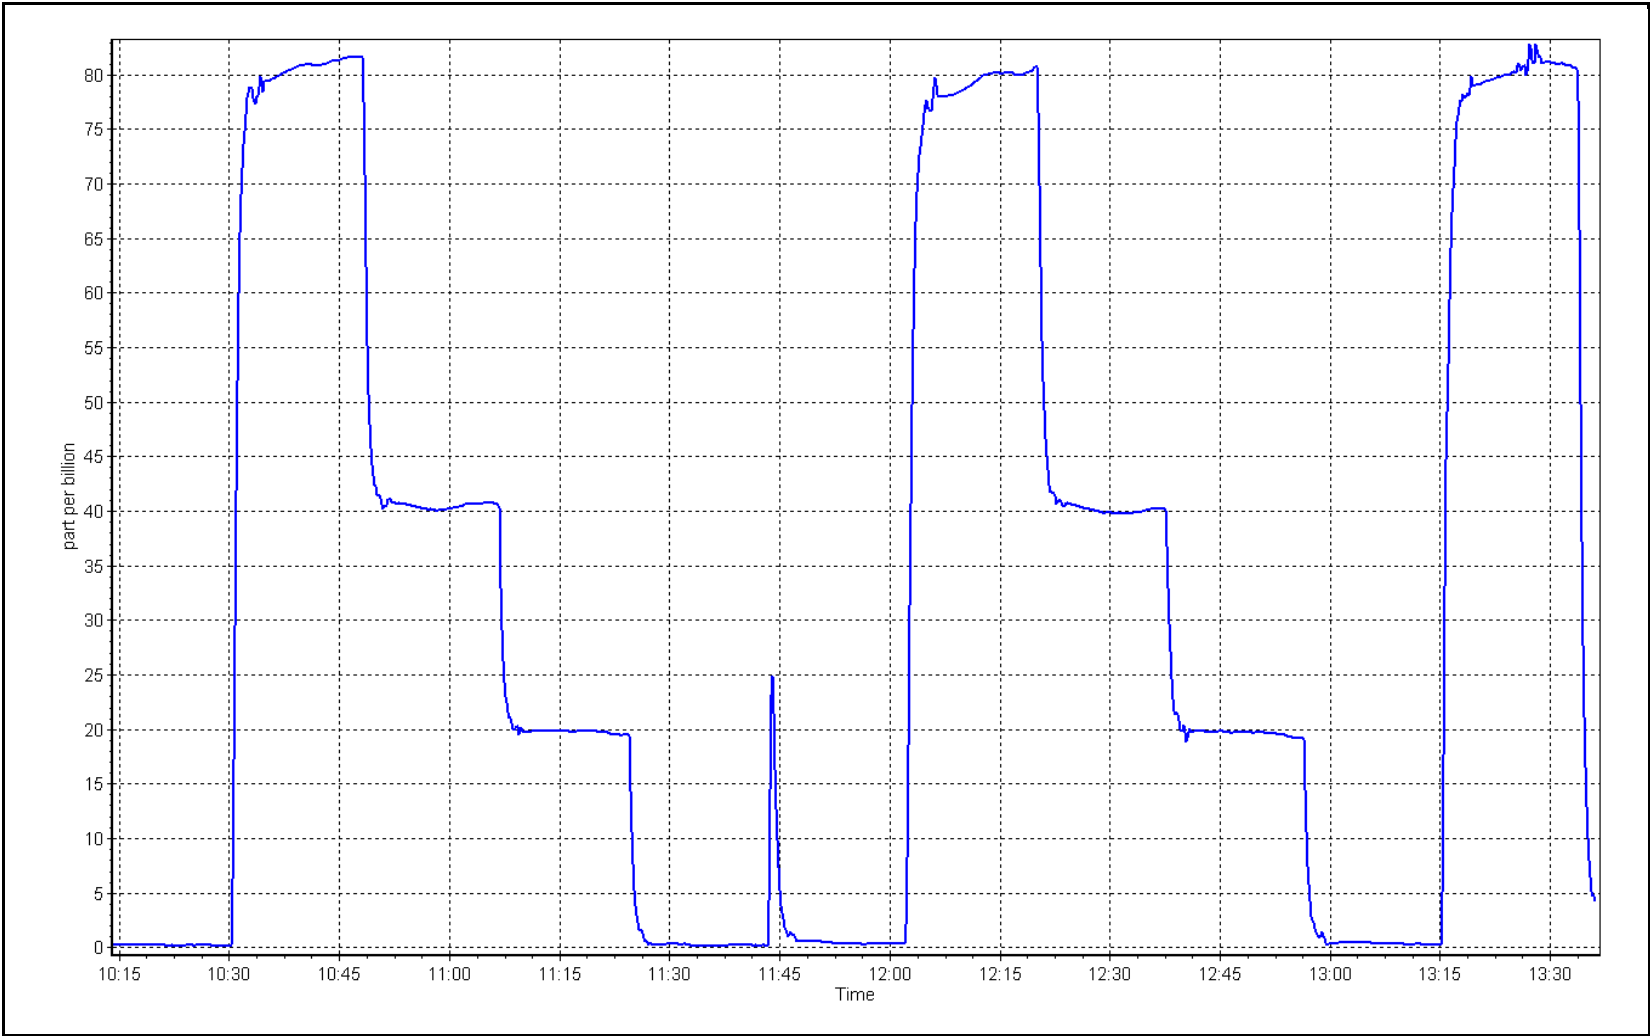



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	-4.6	-1.2	-3.4	----	----
as found span	4921	79.4	816.8	800.3	16.5	829.2	804.5	24.5	0.9850	0.9948
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	-0.2	-0.2	0.1	----	----
high point	4921	79.4	816.8	800.3	16.5	816.0	802.0	13.7	1.0010	0.9979
second point	4960	39.7	408.5	400.2	8.3	405.0	397.2	7.7	1.0085	1.0076
third point	4980	19.8	203.7	199.6	4.1	196.8	191.5	5.4	1.0351	1.0423
as left zero	5000	0.0	0.0	0.0	0.0	-0.4	-0.4	0.0	----	----
as left span	4921	79.4	816.8	395.6	423.2	813.2	391.9	421.2	1.0044	1.0094
Average Correction Factor									1.0149	1.0159

Corrected As found	NO _x = 833.8 ppb	NO = 805.7 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = 2.3%
Previous Response	NO _x = 814.3 ppb	NO = 804.4 ppb		*Percent Change	NO = 0.2%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	800.4	393.7	423.2	422.8	1.0010	99.9%
2nd GPT point (200 ppb O3)	800.4	615.1	201.8	201.7	1.0006	99.9%
3rd GPT point (100 ppb O3)	800.4	711.2	105.7	106.0	0.9973	100.3%
Average Correction Factor					0.9996	100.0%

Notes:

Adjusted both zero and span.

Calibration Performed By:

Denny Ray Estador



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 18, 2023	Previous Calibration:	December 20, 2022
Station Name:	Jackfish 2/3	Station Number:	AMS27
Start Time (MST):	9:08	End Time (MST):	13:30
Analyzer make:	API T200	Analyzer serial #:	4460

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>
0.0	-0.2	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
816.8	816.0	1.0010		
408.5	405.0	1.0085		
203.7	196.8	1.0351		
			0.999926	
			1.001608	
			-3.416967	

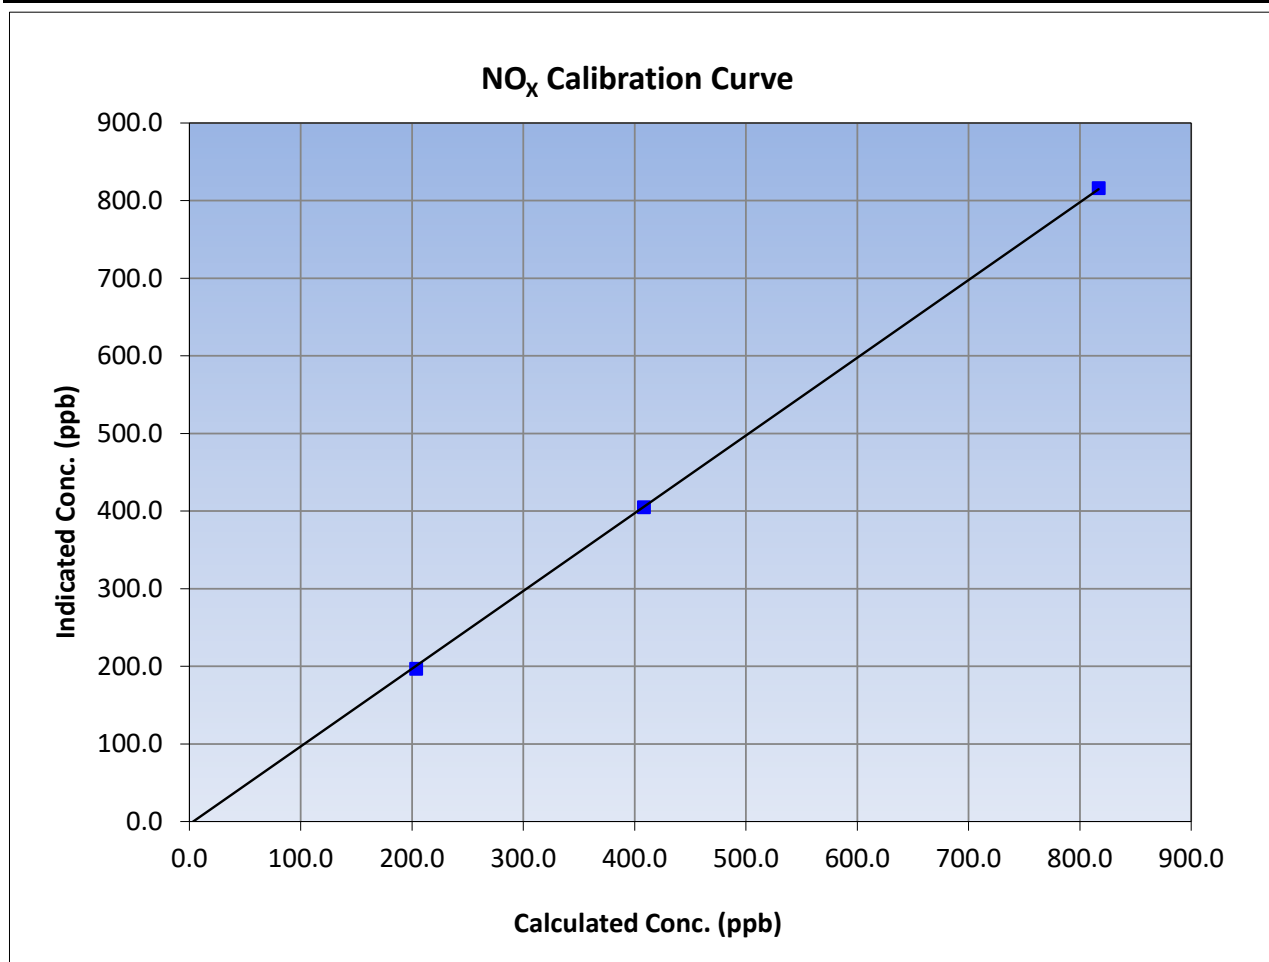



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 18, 2023	Previous Calibration:	December 20, 2022
Station Name:	Jackfish 2/3	Station Number:	AMS27
Start Time (MST):	9:08	End Time (MST):	13:30
Analyzer make:	API T200	Analyzer serial #:	4460

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	-0.2	----	Correlation Coefficient Slope Intercept	≥ 0.995 0.90 - 1.10 +/-20
800.3	802.0	0.9979		
400.2	397.2	1.0076		
199.6	191.5	1.0423		

NO Calibration Curve

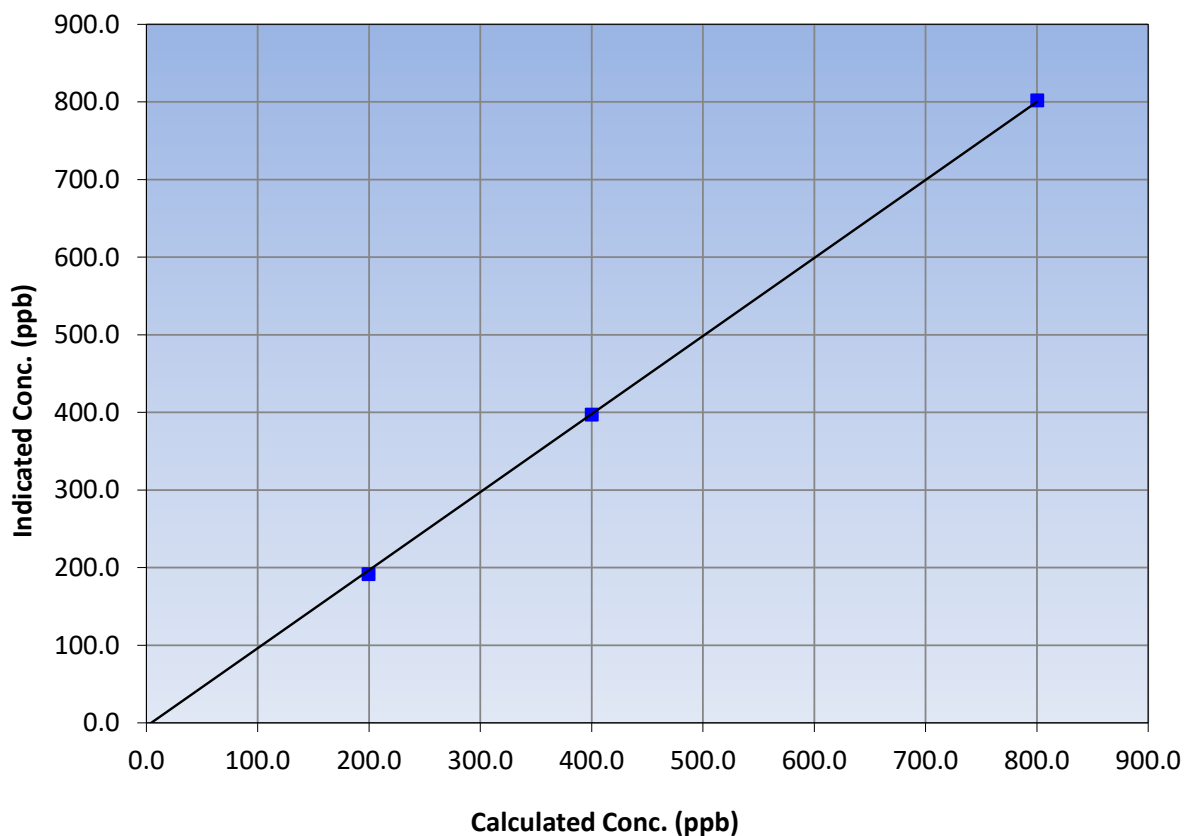



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 18, 2023	Previous Calibration:	December 20, 2022
Station Name:	Jackfish 2/3	Station Number:	AMS27
Start Time (MST):	9:08	End Time (MST):	13:30
Analyzer make:	API T200	Analyzer serial #:	4460

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
423.2	422.8	1.0010		
201.8	201.7	1.0006		
105.7	106.0	0.9973		

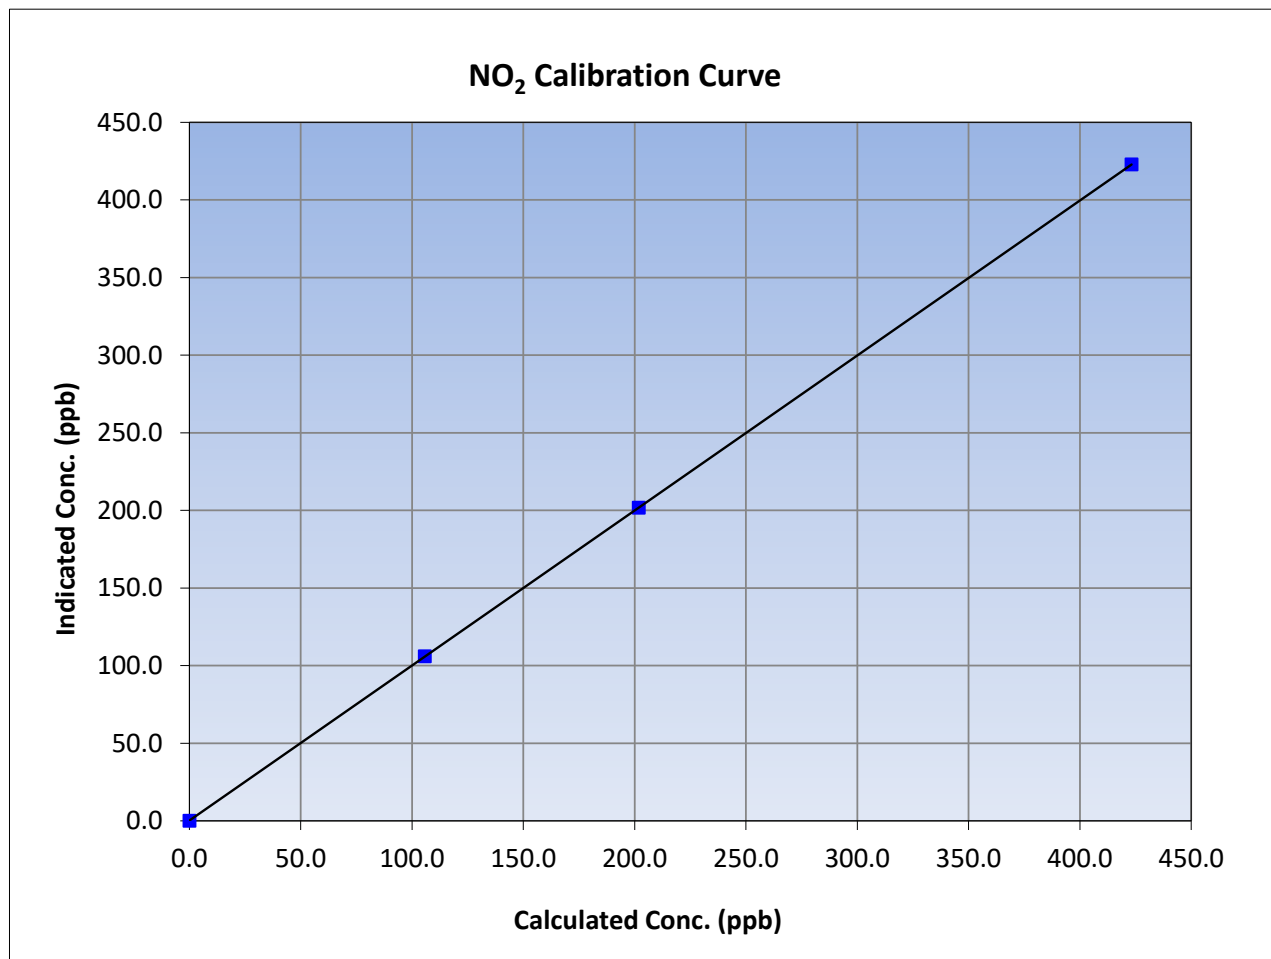

NO_x Calibration Plot

Date: January 18, 2023

Location: Jackfish 2/3

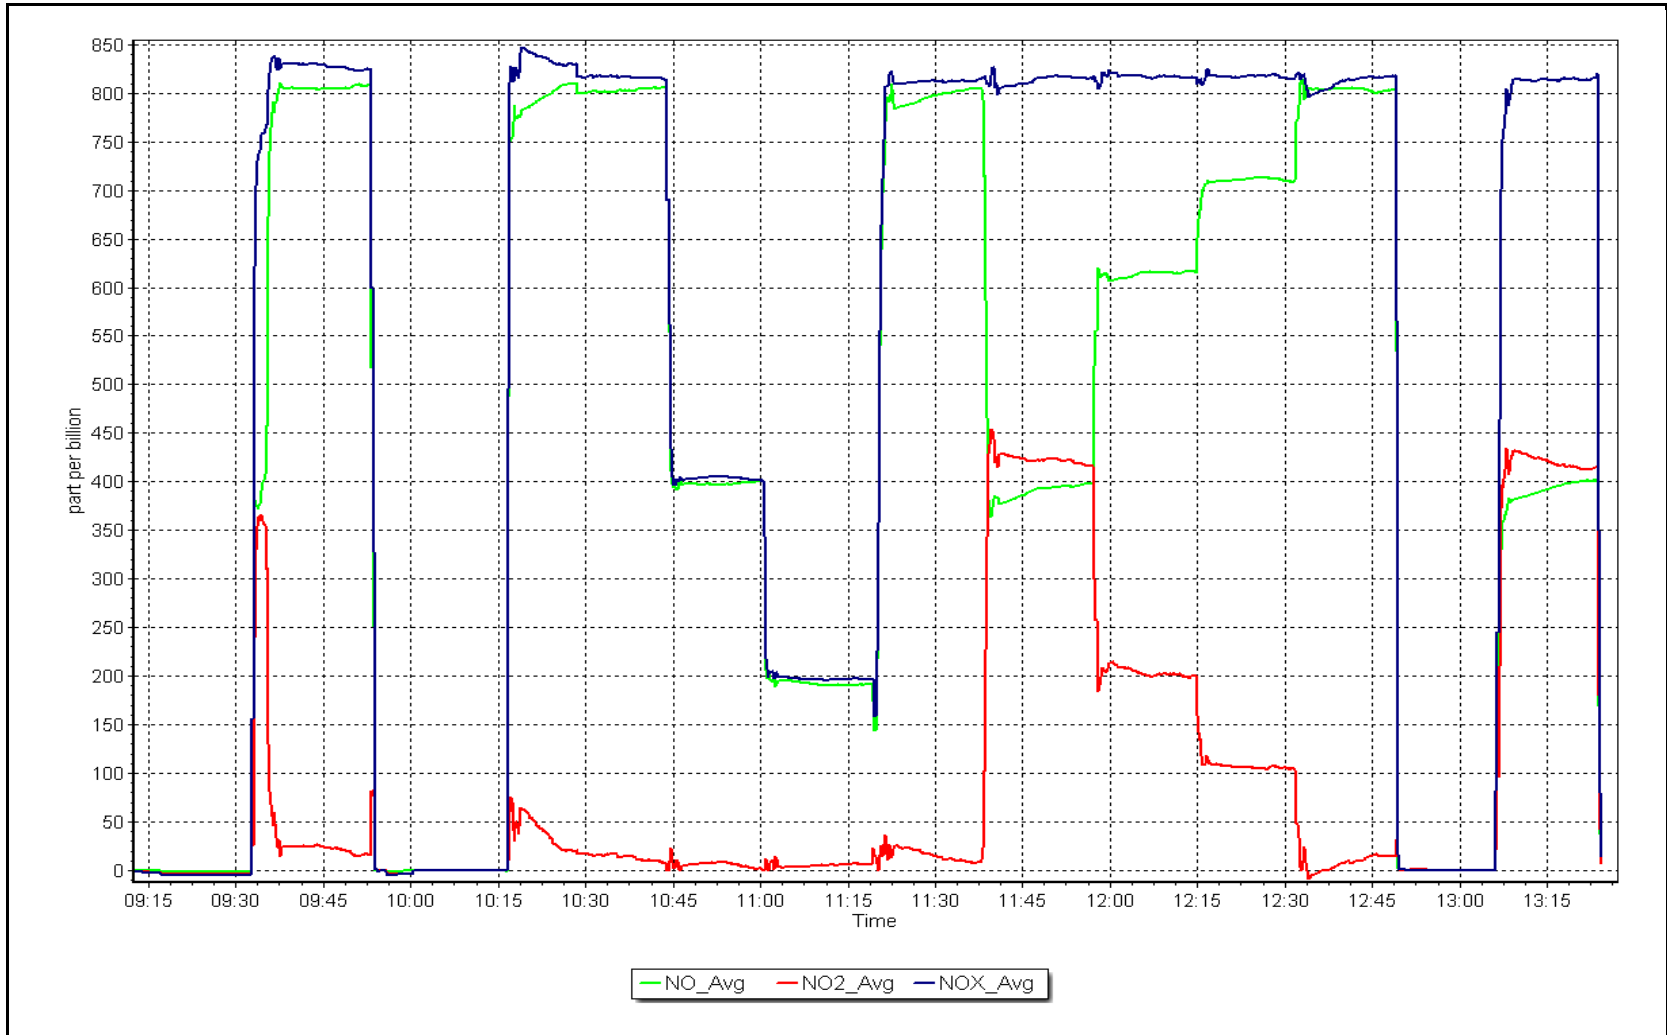



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS29 SURMONT 2 JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 15, 2022
Station Name:	Surmont 2	Station Number:	AMS29
Start Time (MST):	11:24	End Time (MST):	15:04
Analyzer make:	Thermo 43i	Analyzer serial #:	1170050150

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.3	----	Correlation Coefficient	0.999994	
800.1	797.9	1.0028			≥0.995
400.6	398.1	1.0063	Slope	0.997244	
199.8	198.1	1.0087			0.90 - 1.10
			Intercept	-0.565207	+/-30

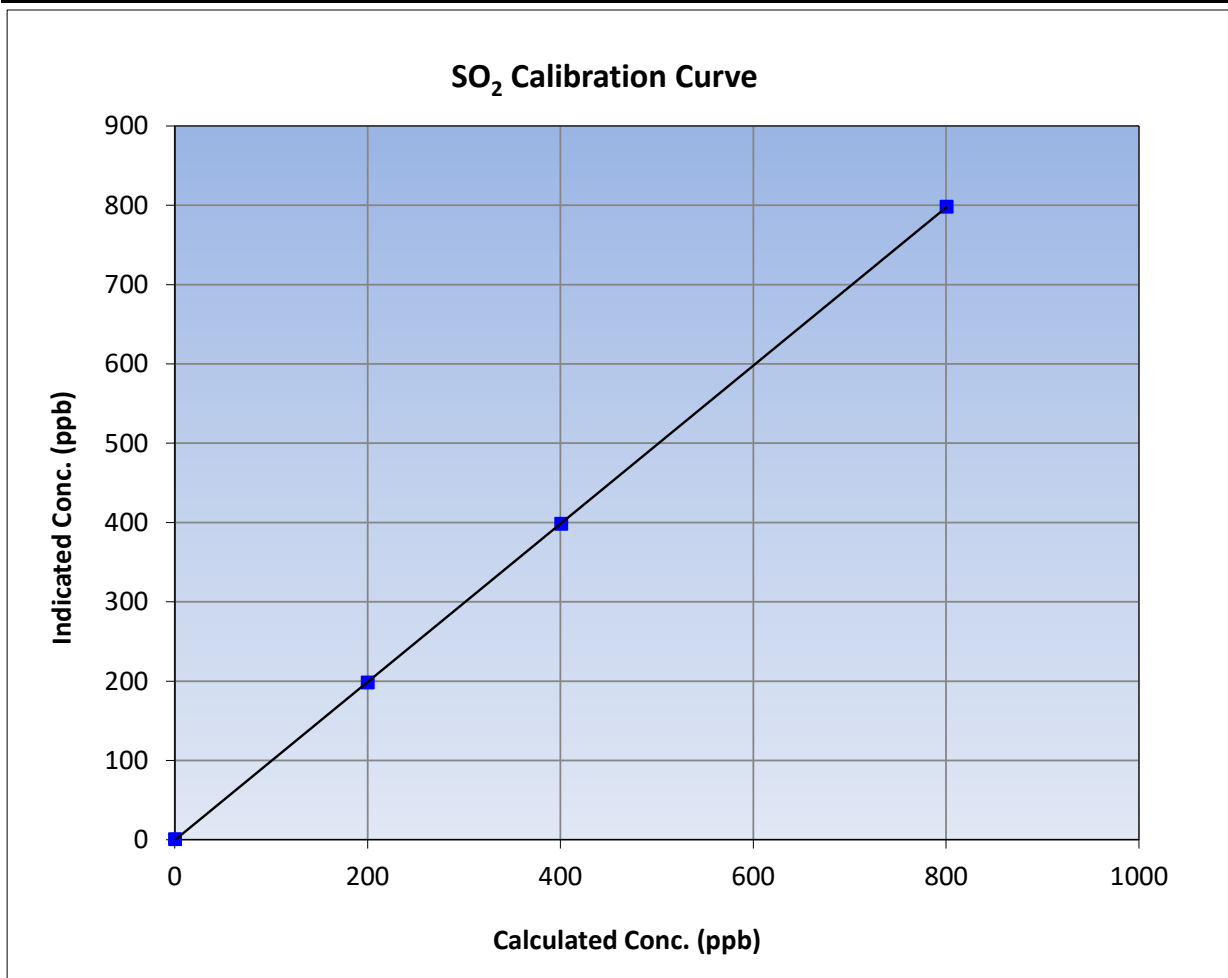

SO2 Calibration Plot

Date: January 3, 2023

Location: Surmont 2

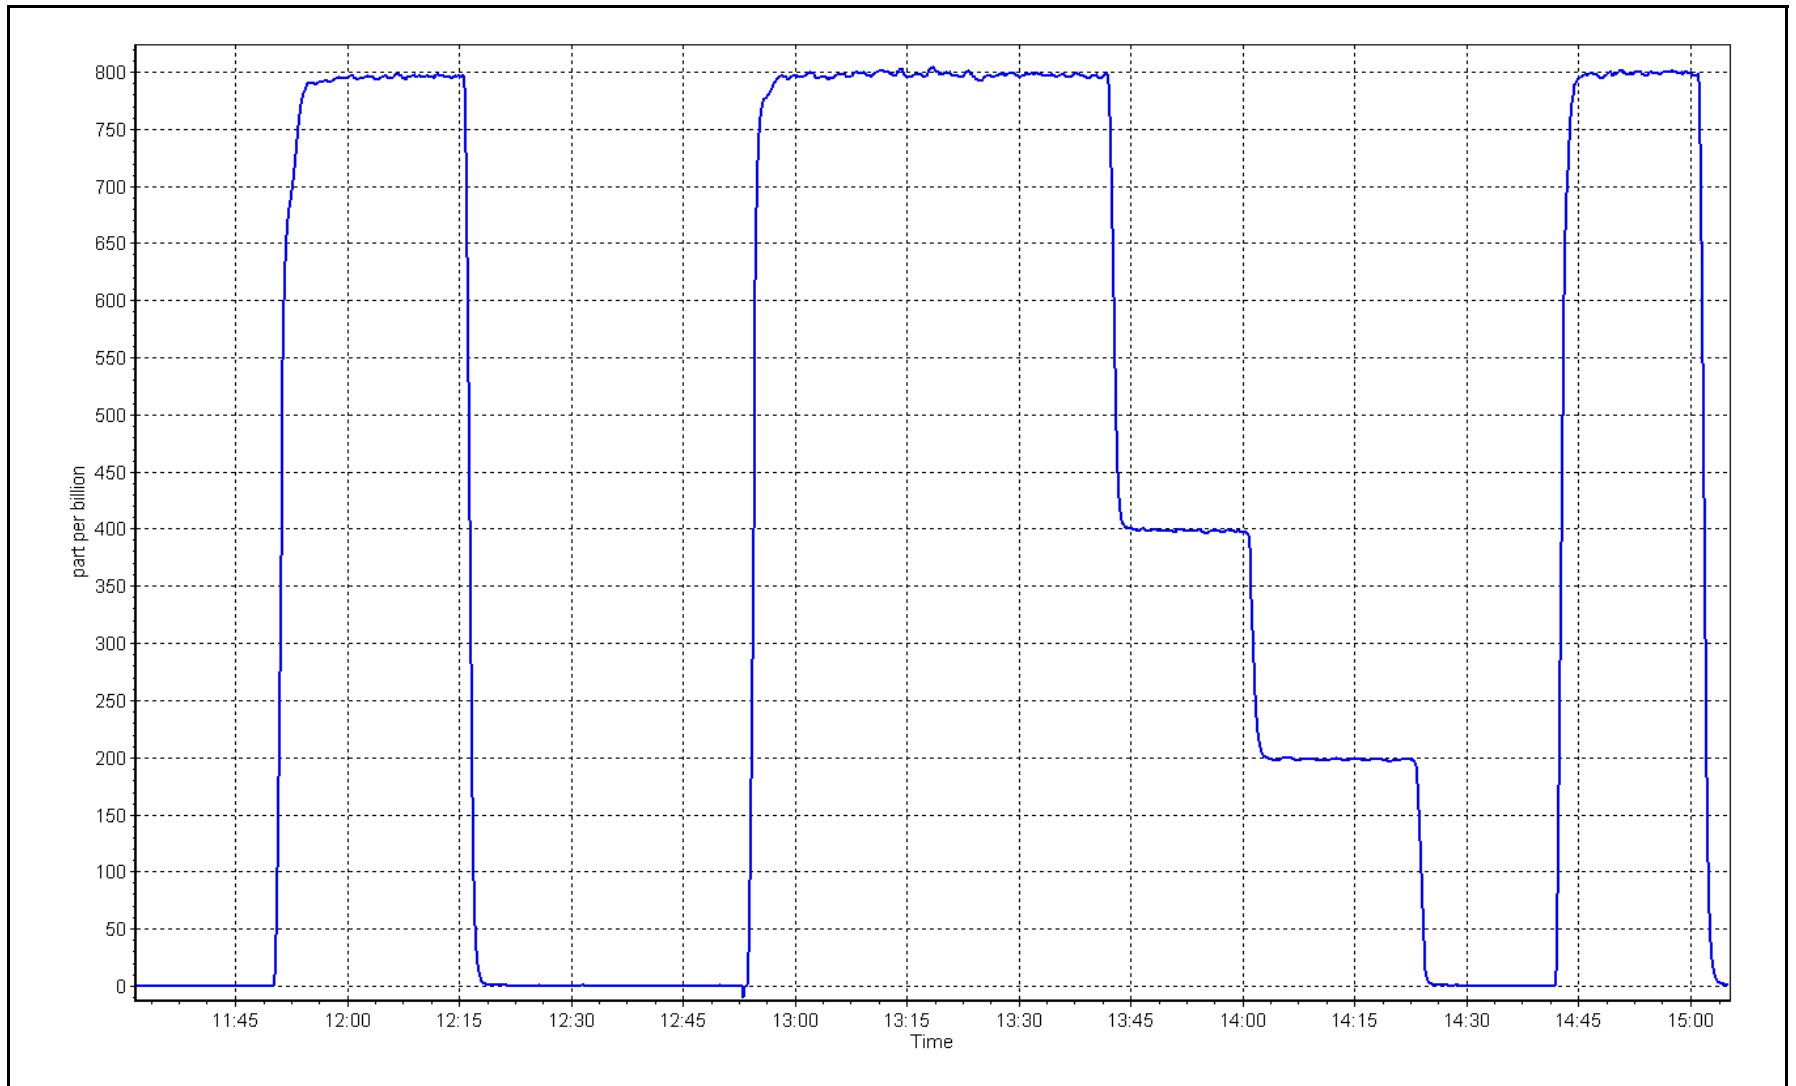



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 9, 2023	Previous Calibration:	December 14, 2022
Station Name:	Surmont 2	Station Number:	AMS29
Start Time (MST):	11:00	End Time (MST):	15:19
Analyzer make:	Thermo 450i	Analyzer serial #:	1170050142

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.4	----	Correlation Coefficient	0.999963	≥0.995
80.0	80.0	1.0000			
40.1	40.1	1.0002	Slope	0.996612	0.90 - 1.10
20.1	19.9	1.0077			
			Intercept	0.177532	+/-3

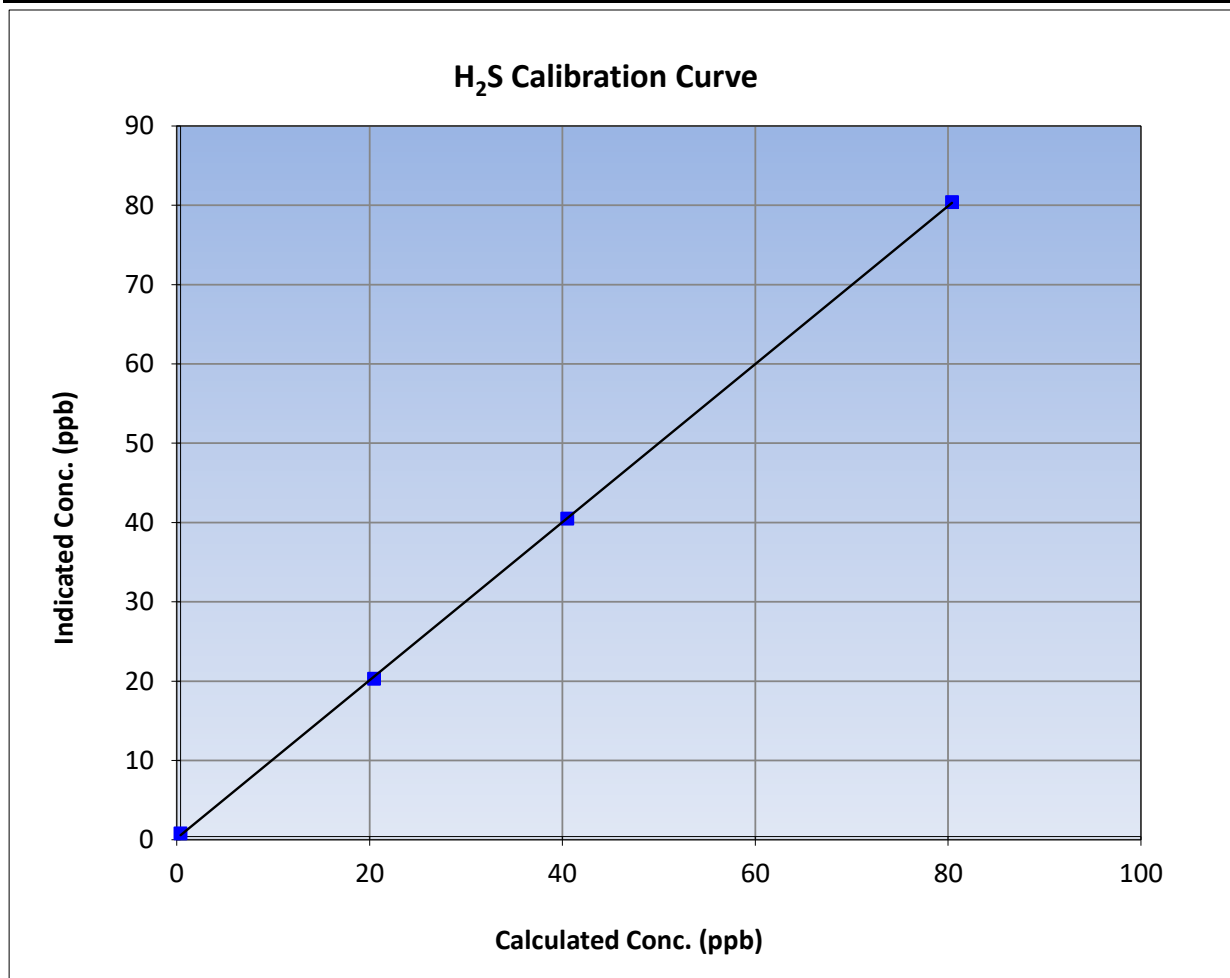

H₂S Calibration Plot

Date: January 9, 2023

Location: Surmont 2

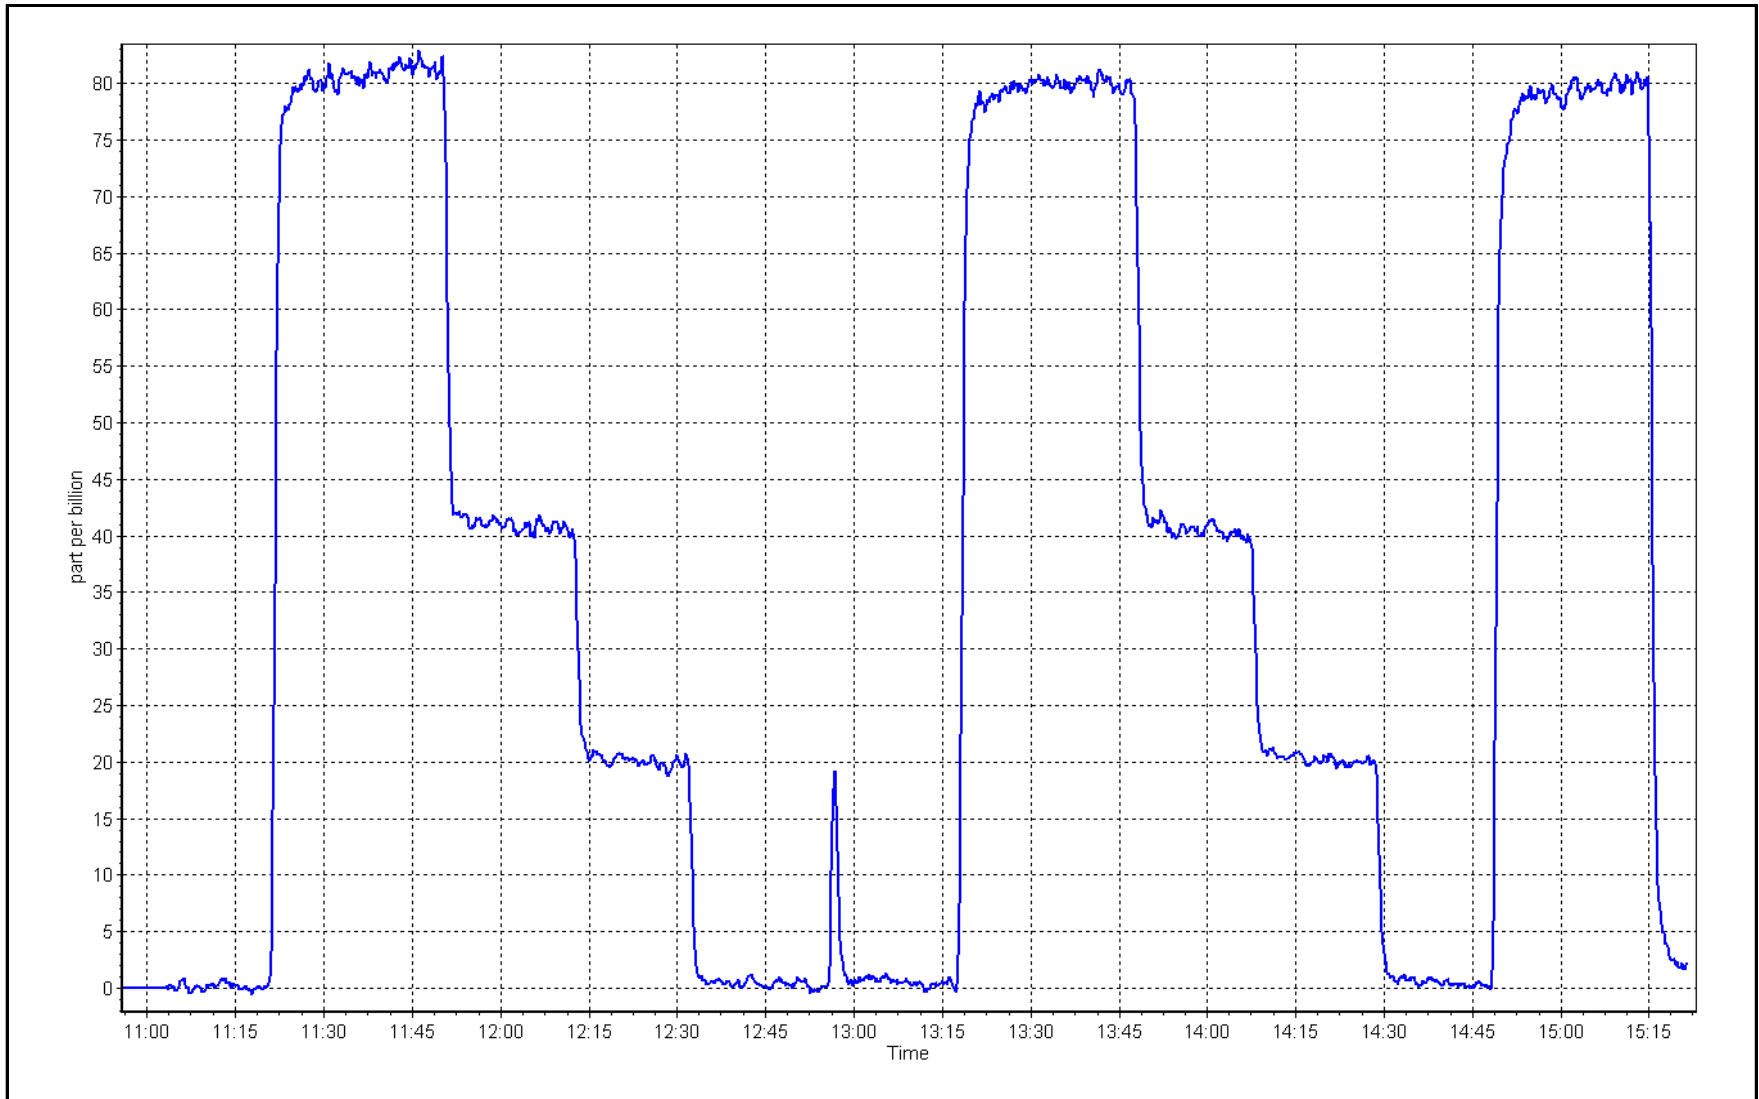



Wood Buffalo Environmental Association

THC Calibration Report

Version-01-2020

Station Information

Station Name:	Surmont 2	Station number:	AMS29
Calibration Date:	January 3, 2023	Last Cal Date:	December 15, 2022
Start time (MST):	11:24	End time (MST):	15:04
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC356008	Cal Gas Expiry Date:	February 23, 2025
CH4 Cal Gas Conc.	<u>499.0</u> ppm	CH4 Equiv Conc.	1064.7 ppm
C3H8 Cal Gas Conc.	<u>205.7</u> ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH4 Conc.	<u>499.0</u> ppm	CH4 Equiv Conc.	1064.7 ppm
Removed C3H8 Conc.	<u>205.7</u> ppm	Diff between cyl:	
Calibrator Make/Model:	Teledyne API T700	Serial Number:	3808
ZAG Make/Model:	Teledyne API T701	Serial Number:	4297

Analyzer Information

Analyzer make: Thermo 51i-LT Analyzer serial #: 1170050149
 Analyzer Range: 0 - 20 ppm

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.000353	0.999326	Background:	4.240	4.510
Calibration intercept:	0.055778	-0.002444	Coefficient:	5.163	5.288

THC Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated Concentration (ppm) (Cc)	Indicated Concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.10	----
as found span	4918	81.3	17.31	17.07	1.014
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.02	----
high point	4918	81.3	17.31	17.32	1.000
second point	4959	40.7	8.67	8.62	1.005
third point	4979	20.3	4.32	4.32	1.002
as left zero	5000	0.0	0.00	-0.09	----
as left span	4918	81.3	17.31	17.47	0.991
Average Correction Factor					1.002
Baseline Corr As found:	16.97	Previous response	17.38	*% change	-2.4%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Changed sample inlet filter after as founds. Adjusted zero and span.

Calibration Performed By: Braiden Boutillier



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 3, 2023	Previous Calibration:	December 15, 2022
Station Name:	Surmont 2	Station Number:	AMS29
Start Time (MST):	11:24	End Time (MST):	15:04
Analyzer make:	Thermo 51i-LT	Analyzer serial #:	1170050149

Calibration Data


Calculated Concentration (ppm) (Cc)	Indicated Concentration (ppm) (lc)	Correction factor (Cc/lc)	Statistical Evaluation	<i>Limits</i>	
0.00	0.02	----	Correlation Coefficient	0.999986	
17.31	17.32	0.9997			≥0.995
8.67	8.62	1.0054	Slope	0.999326	
4.32	4.32	1.0019			0.90 - 1.10
			Intercept	-0.002444	+/-1.5

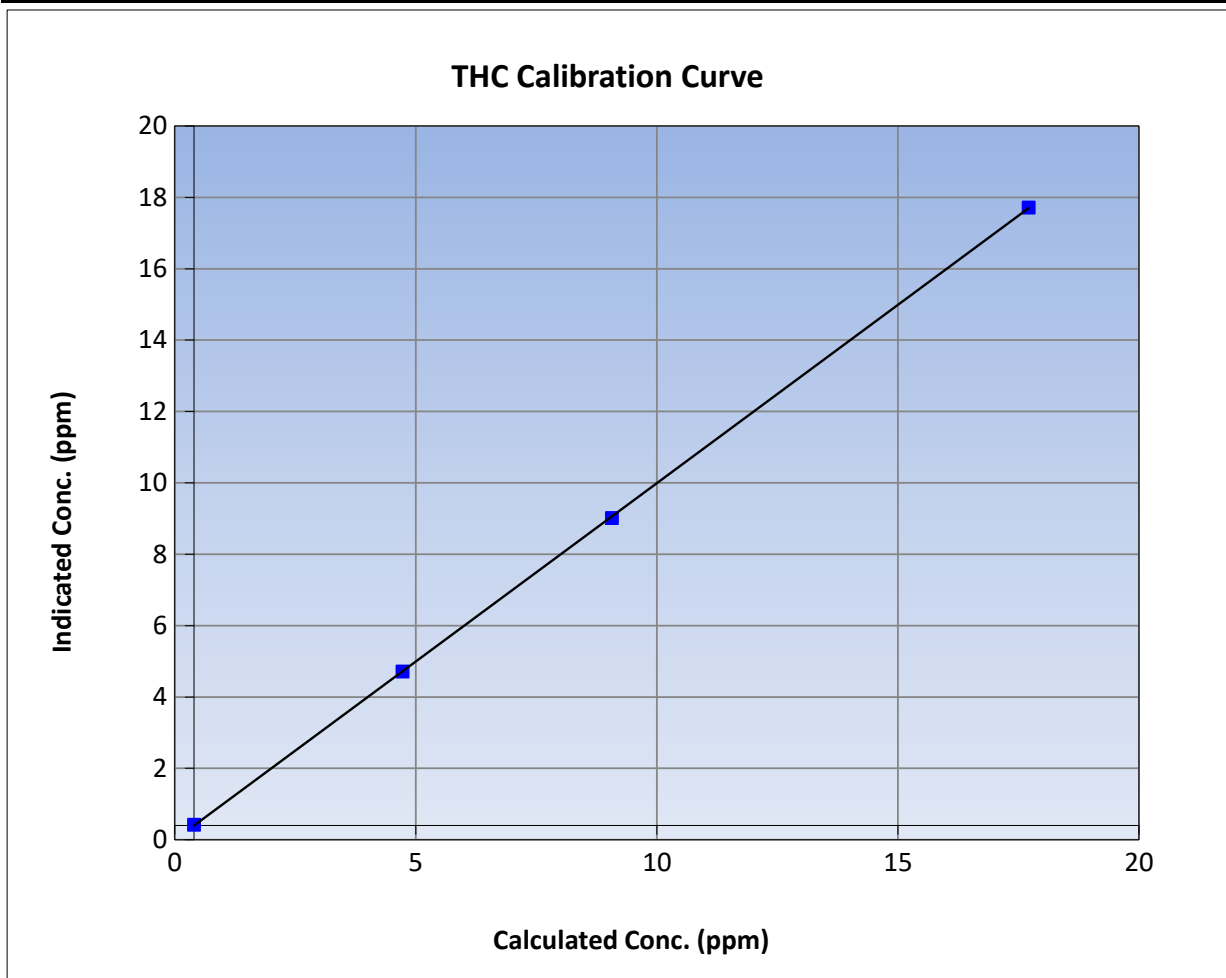

THC Calibration Plot

Date: January 3, 2023

Location: Surmont 2

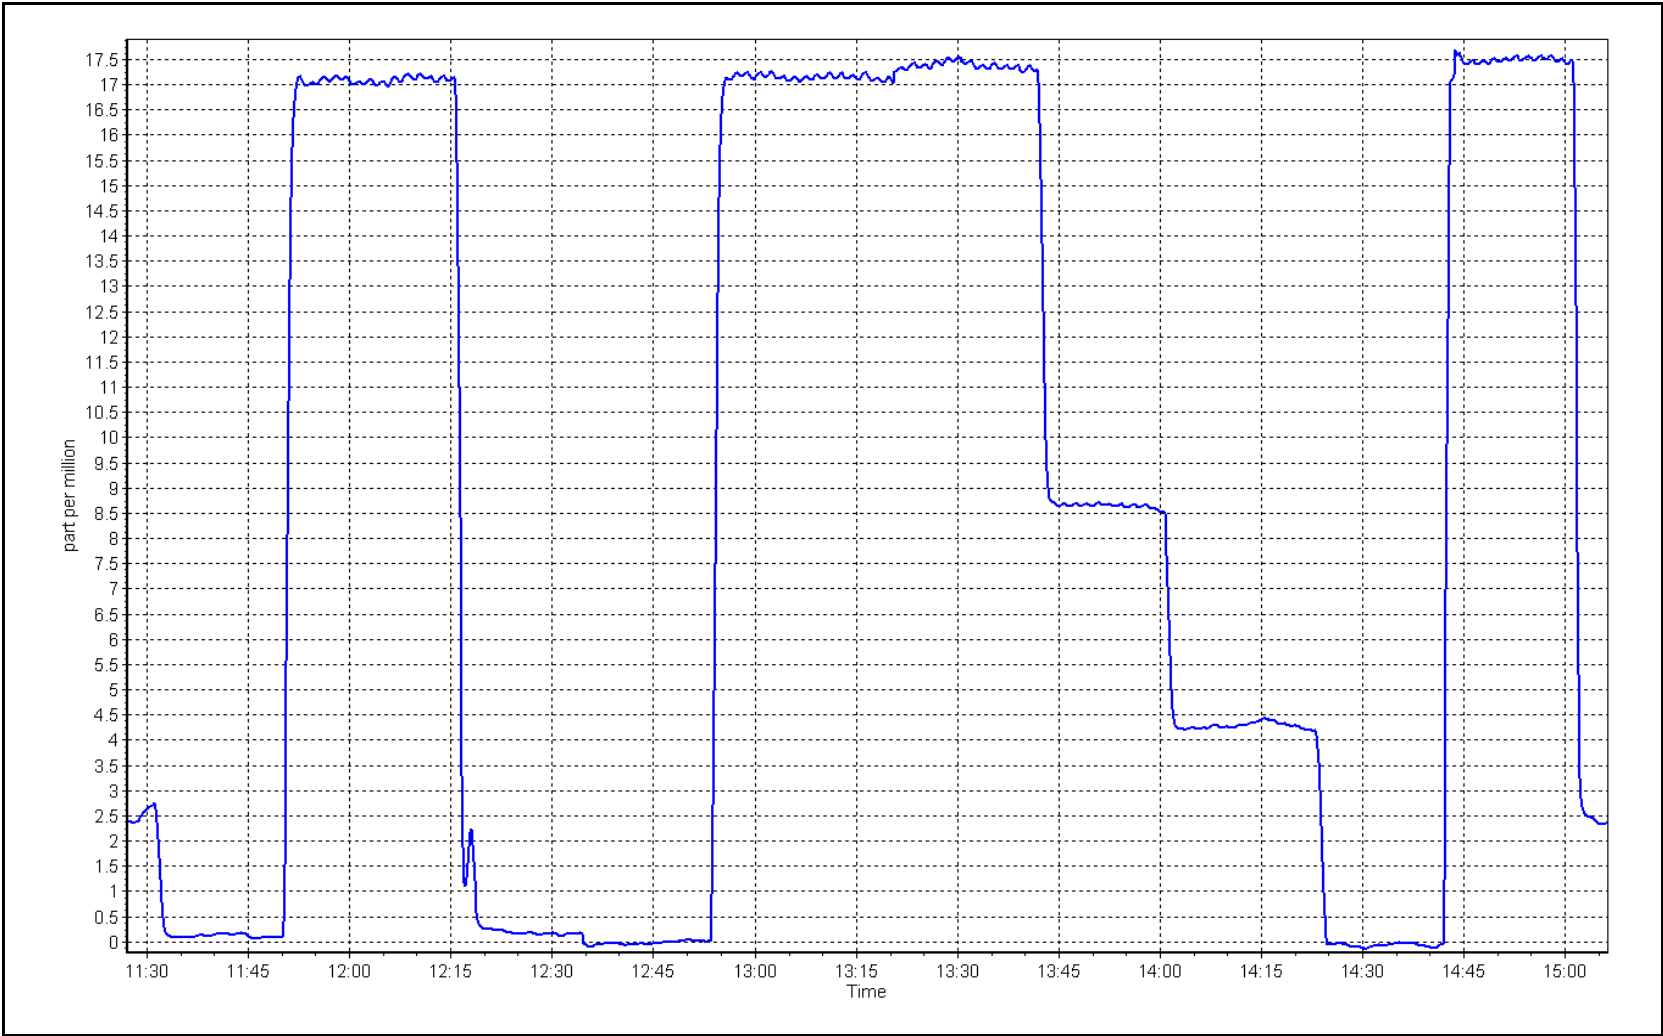



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.2	0.0	0.2	----	----
as found span	4916	84.2	799.2	799.2	0.0	813.1	812.8	0.2	0.9829	0.9833
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.6	0.0	0.6	----	----
high point	4916	84.2	799.2	799.2	0.0	798.4	799.1	-0.6	1.0010	1.0001
second point	4958	42.1	399.6	399.6	0.0	400.3	400.1	0.2	0.9983	0.9988
third point	4979	21.1	200.3	200.3	0.0	200.6	199.4	1.1	0.9984	1.0044
as left zero	5000	0.0	0.0	0.0	0.0					
as left span	4916	84.2	799.2	256.7	542.5					

Average Correction Factor	0.9992	1.0011
---------------------------	--------	--------

Corrected As found	NO _x = 812.9 ppb	NO = 812.8 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = 1.2%
Previous Response	NO _x = 803.5 ppb	NO = 804.0 ppb		*Percent Change	NO = 1.1%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	798.3	255.8	542.5	541.0	1.0028	99.7%
2nd GPT point (200 ppb O3)	798.3	588.8	209.5	207.7	1.0087	99.1%
3rd GPT point (100 ppb O3)	798.3	690.9	107.4	105.5	1.0180	98.2%
Average Correction Factor					1.0098	99.0%

Notes: Changed sample inlet filter after as founds. No adjustments made.

Calibration Performed By: Braiden Boutilier



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 1, 2023	Previous Calibration:	December 6, 2022
Station Name:	Surmont 2	Station Number:	AMS29
Start Time (MST):	12:58	End Time (MST):	17:05
Analyzer make:	Thermo 42i	Analyzer serial #:	1170050148

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.6	----	Correlation Coefficient	≥0.995	
799.2	798.4	1.0010			
399.6	400.3	0.9983			
200.3	200.6	0.9984			
			Slope	0.998337	0.90 - 1.10
			Intercept	0.787346	+/-20

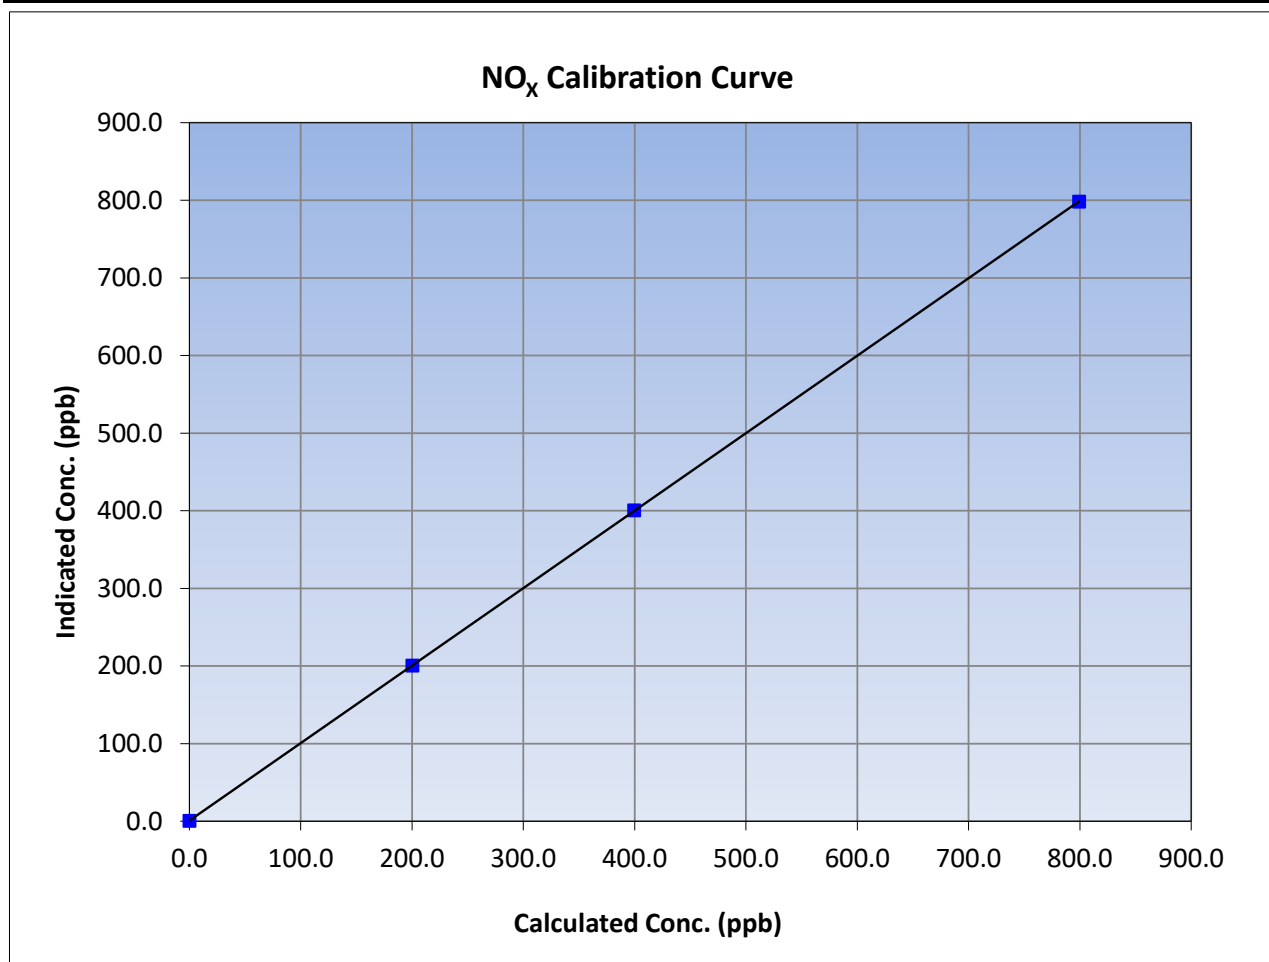



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 1, 2023	Previous Calibration:	December 6, 2022
Station Name:	Surmont 2	Station Number:	AMS29
Start Time (MST):	12:58	End Time (MST):	17:05
Analyzer make:	Thermo 42i	Analyzer serial #:	1170050148

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.0	----	Correlation Coefficient	≥0.995	
799.2	799.1	1.0001			
399.6	400.1	0.9988			
200.3	199.4	1.0044			
			Slope	1.000325	0.90 - 1.10
			Intercept	-0.232760	+/-20

NO Calibration Curve

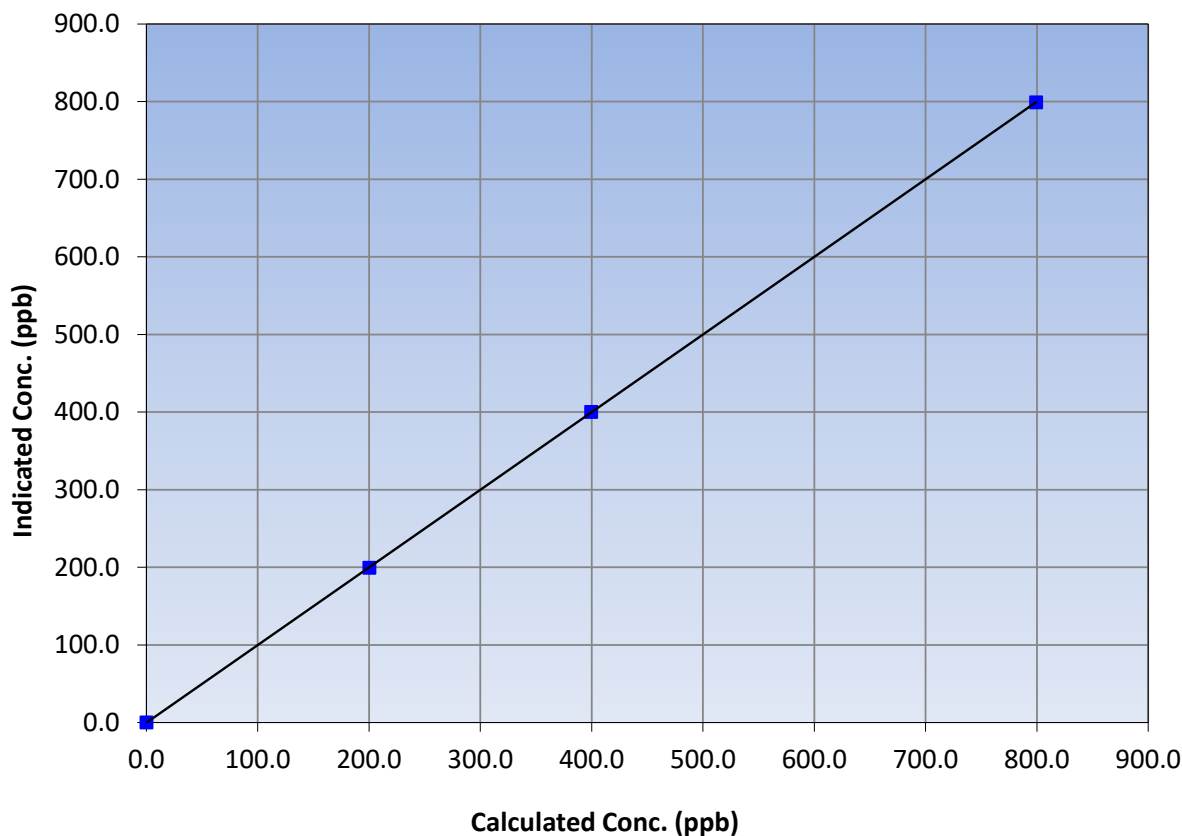



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 1, 2023	Previous Calibration:	December 6, 2022
Station Name:	Surmont 2	Station Number:	AMS29
Start Time (MST):	12:58	End Time (MST):	17:05
Analyzer make:	Thermo 42i	Analyzer serial #:	1170050148

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.6	----	Correlation Coefficient	≥0.995	
542.5	541.0	1.0028			
209.5	207.7	1.0087			
107.4	105.5	1.0180			
			Slope	0.997537	0.90 - 1.10
			Intercept	-0.620843	+/-20

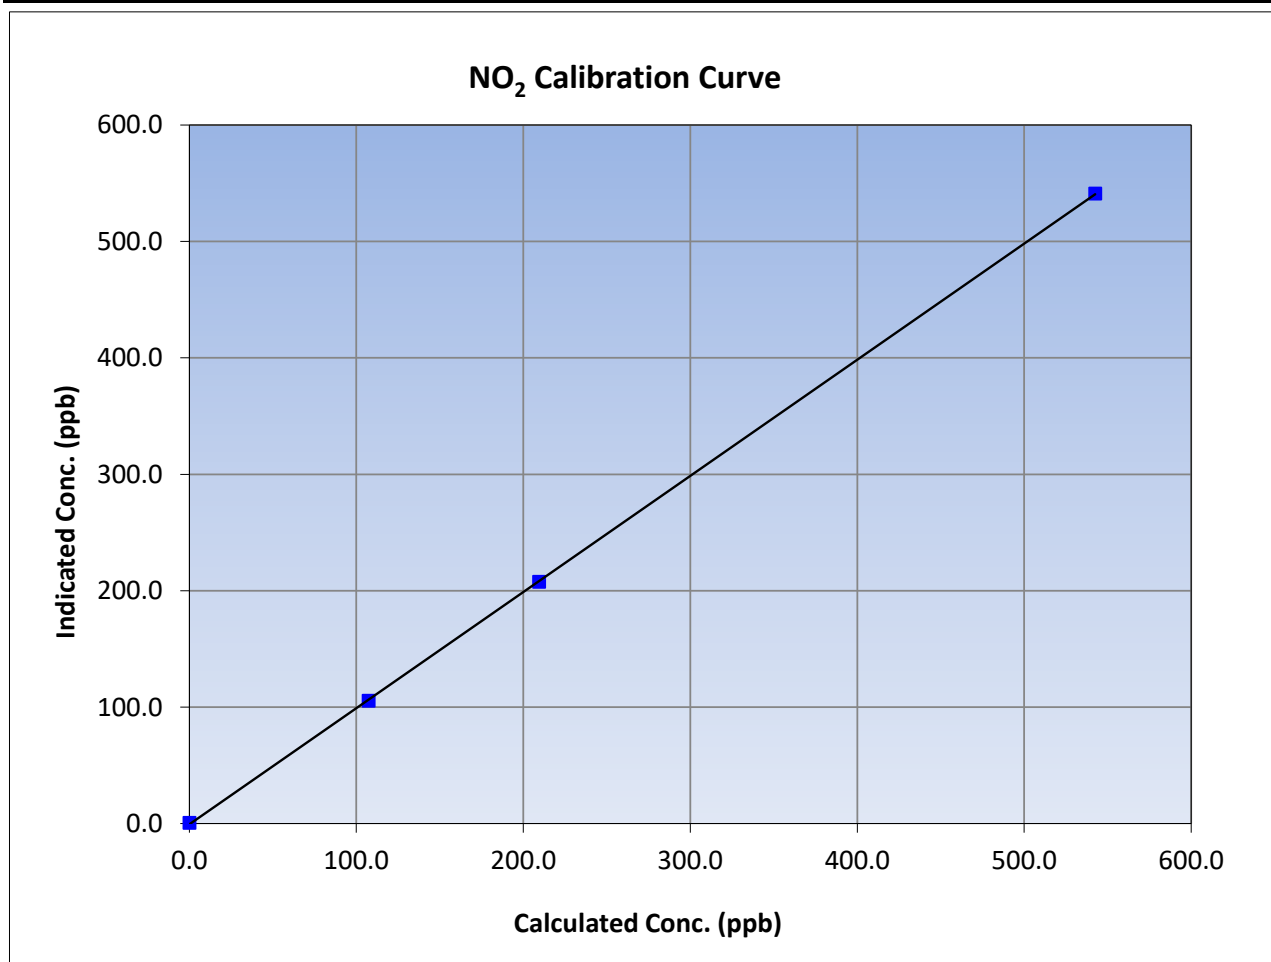

NO_x Calibration Plot

Date: January 1, 2023

Location: Surmont 2

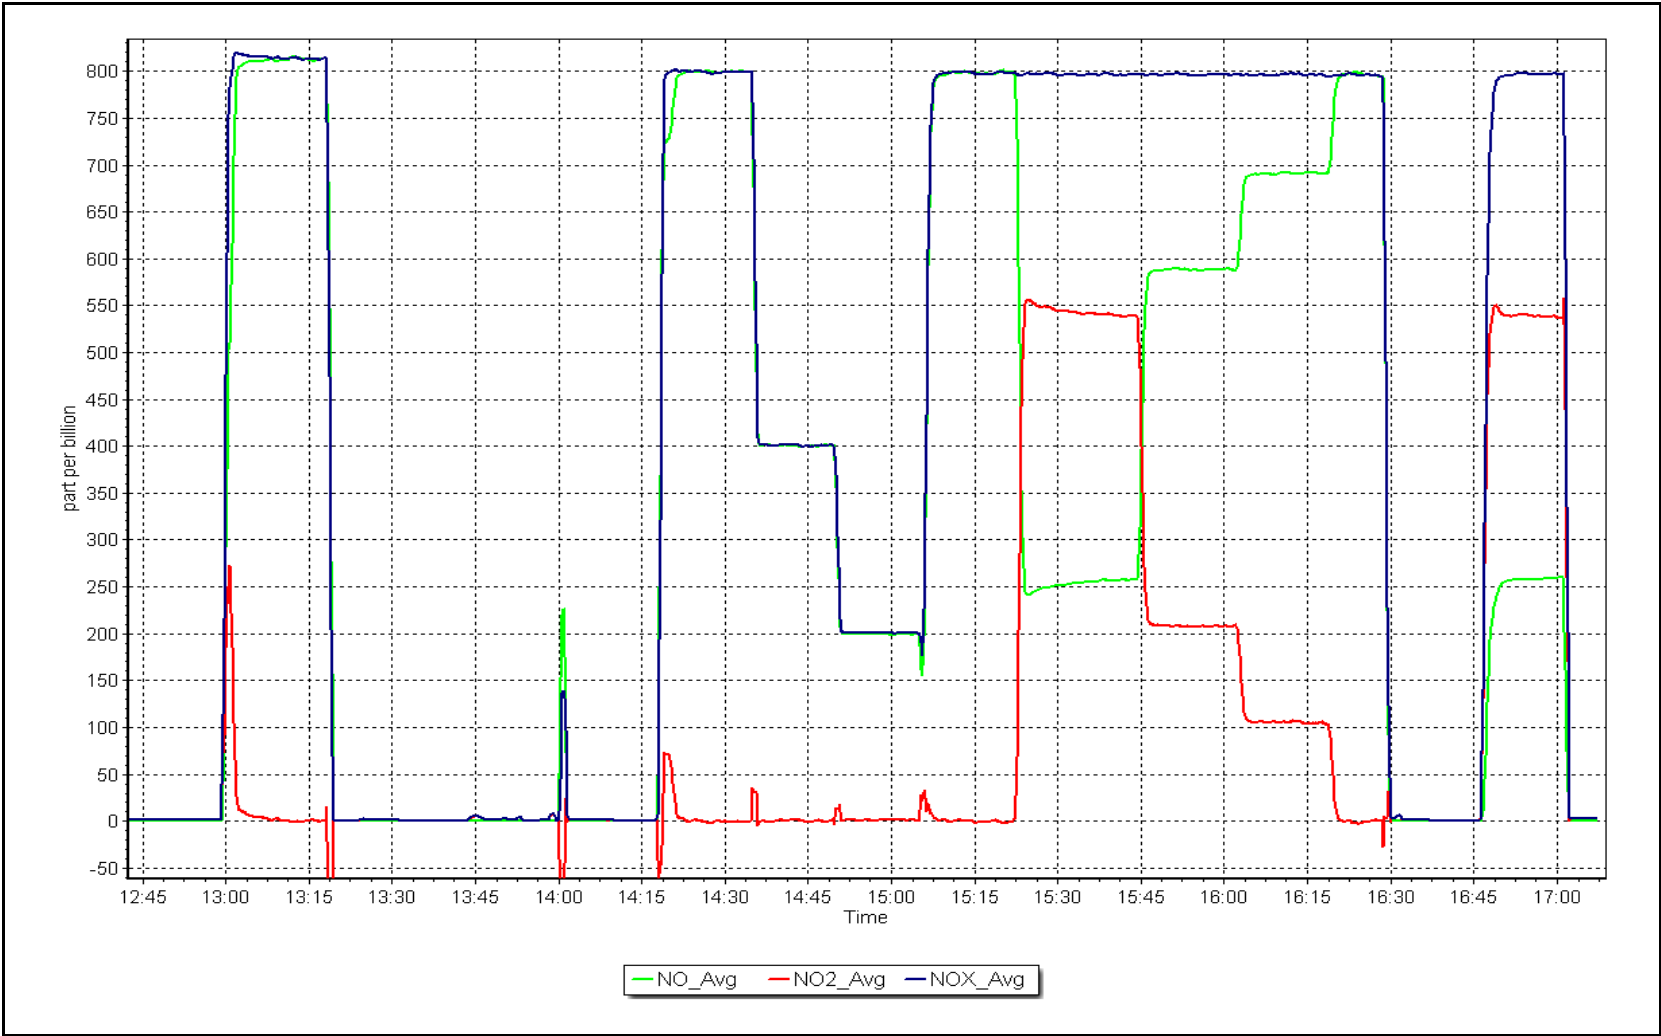



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Surmont 2 Station number: AMS 29
Calibration Date: January 12, 2023 Last Cal Date: December 15, 2022
Start time (MST): 14:24 End time (MST): 14:46

Analyzer Make: API T640 S/N: 253
Particulate Fraction: PM2.5

Flow Meter Make/Model: Delta Cal S/N: 1018
Temp/RH standard: Delta Cal S/N: 1018

Monthly Calibration Test

Parameter	As found	Measured	As left	Adjusted	(Limits)
T (°C)	-8.4	-7.8	-8.4	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	710.4	707.4	710.4	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	4.99	4.98	4.99	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 12, 2023 Last Cal Date: December 15, 2022
PM w/o HEPA: 9.5 PM w/ HEPA: 0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

Parameter	As found	Measured	As left	Adjusted	(Limits)
PMT Peak Test				<input type="checkbox"/>	11.3 +/- 0.5

Date Optical Chamber Cleaned: _____
Disposable Filter Changed: September 30, 2022

Annual Maintenance

Date Sample Tube Cleaned: September 30, 2022
Date RH/T Sensor Cleaned: October 6, 2022

Notes: No adjustments made.

Calibration by: Braiden Boutilier



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS30 ELLS RIVER JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Report

Version-01-2020

Station Information

Station Name:	Ells River	Station number:	AMS 30
Calibration Date:	January 10, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	10:08	End time (MST):	13:15
Reason:	Routine		

Calibration Standards

Cal Gas Concentration:	50.53	ppm	Cal Gas Exp Date:	December 29, 2028
Cal Gas Cylinder #:	CC494126			
Removed Cal Gas Conc:	50.53	ppm	Rem Gas Exp Date:	
Removed Gas Cyl #:			Diff between cyl:	
Calibrator Make/Model:	API T700		Serial Number:	3061
ZAG Make/Model:	API T701H		Serial Number:	358

Analyzer Information

Analyzer make:	Thermo 43i	Analyzer serial #:	1008841397
Analyzer Range	0 - 1000 ppb		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.005272	1.003501	Backgd or Offset:	9.1	9.3
Calibration intercept:	-2.195981	-2.675936	Coeff or Slope:	0.978	0.988

SO₂ Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	-0.5	----
as found span	4921	79.2	800.4	790.7	1.012
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.0	-0.1	----
high point	4921	79.2	800.4	802.0	0.998
second point	4960	39.6	400.2	397.0	1.008
third point	4980	19.8	200.1	196.0	1.021
as left zero	5000	0.0	0.0	-0.3	----
as left span	4921	79.2	800.4	803.1	0.997
Average Correction Factor					1.009

Baseline Corr As found:	791.20	Previous response	802.39	*% change	-1.4%
Baseline Corr 2nd AF pt:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF pt:	NA	AF Correlation:			

* = > +/-5% change initiates investigation

Notes: Adjusted the span only.

Calibration Performed By: Denny Ray Estador



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 2, 2022
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	10:08	End Time (MST):	13:15
Analyzer make:	Thermo 43i	Analyzer serial #:	1008841397

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	-0.1	----	Correlation Coefficient	0.999951	≥0.995
800.4	802.0	0.9980			
400.2	397.0	1.0081	Slope	1.003501	0.90 - 1.10
200.1	196.0	1.0210			
			Intercept	-2.675936	+/-30

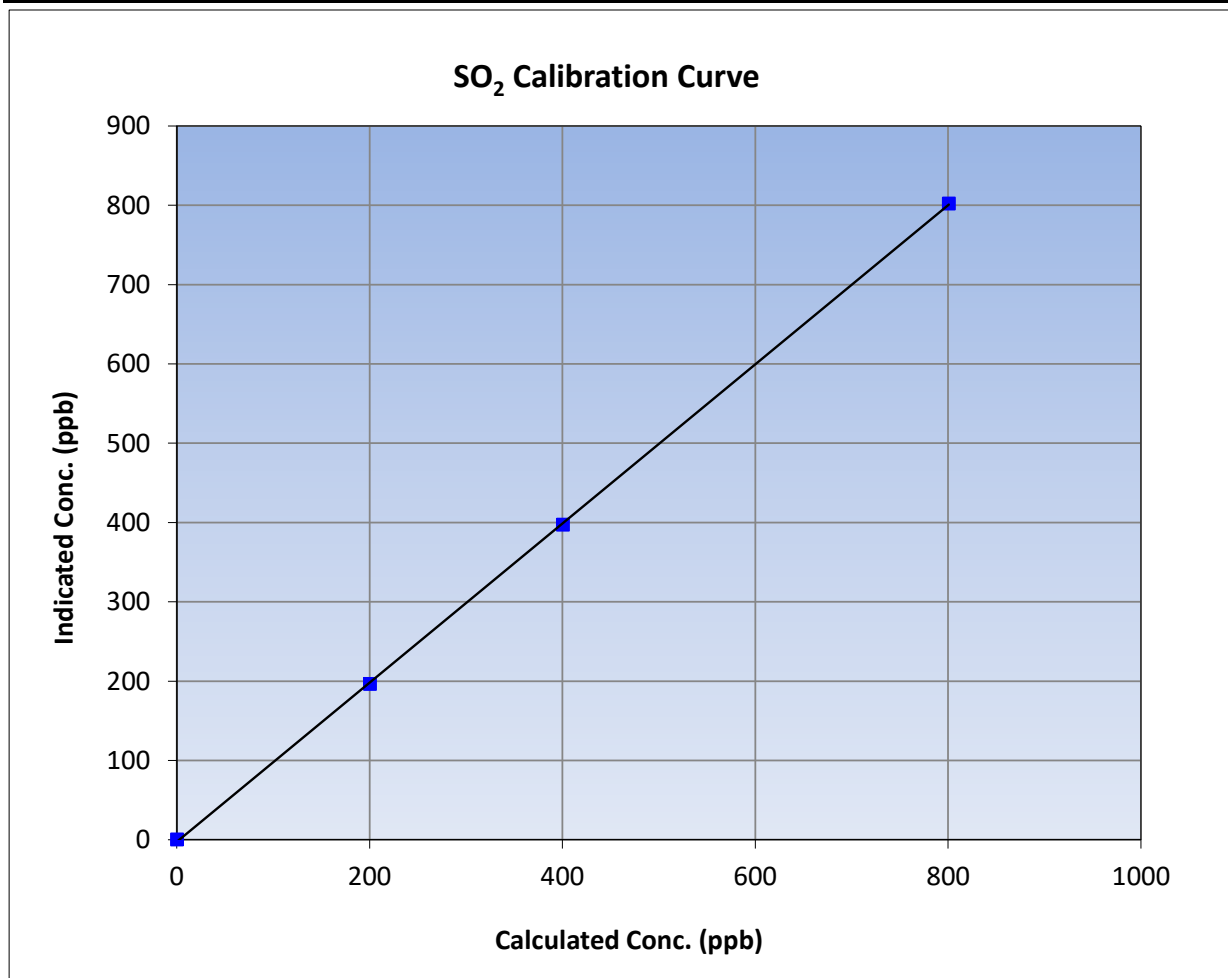

SO2 Calibration Plot

Date: January 10, 2023

Location: Ells River

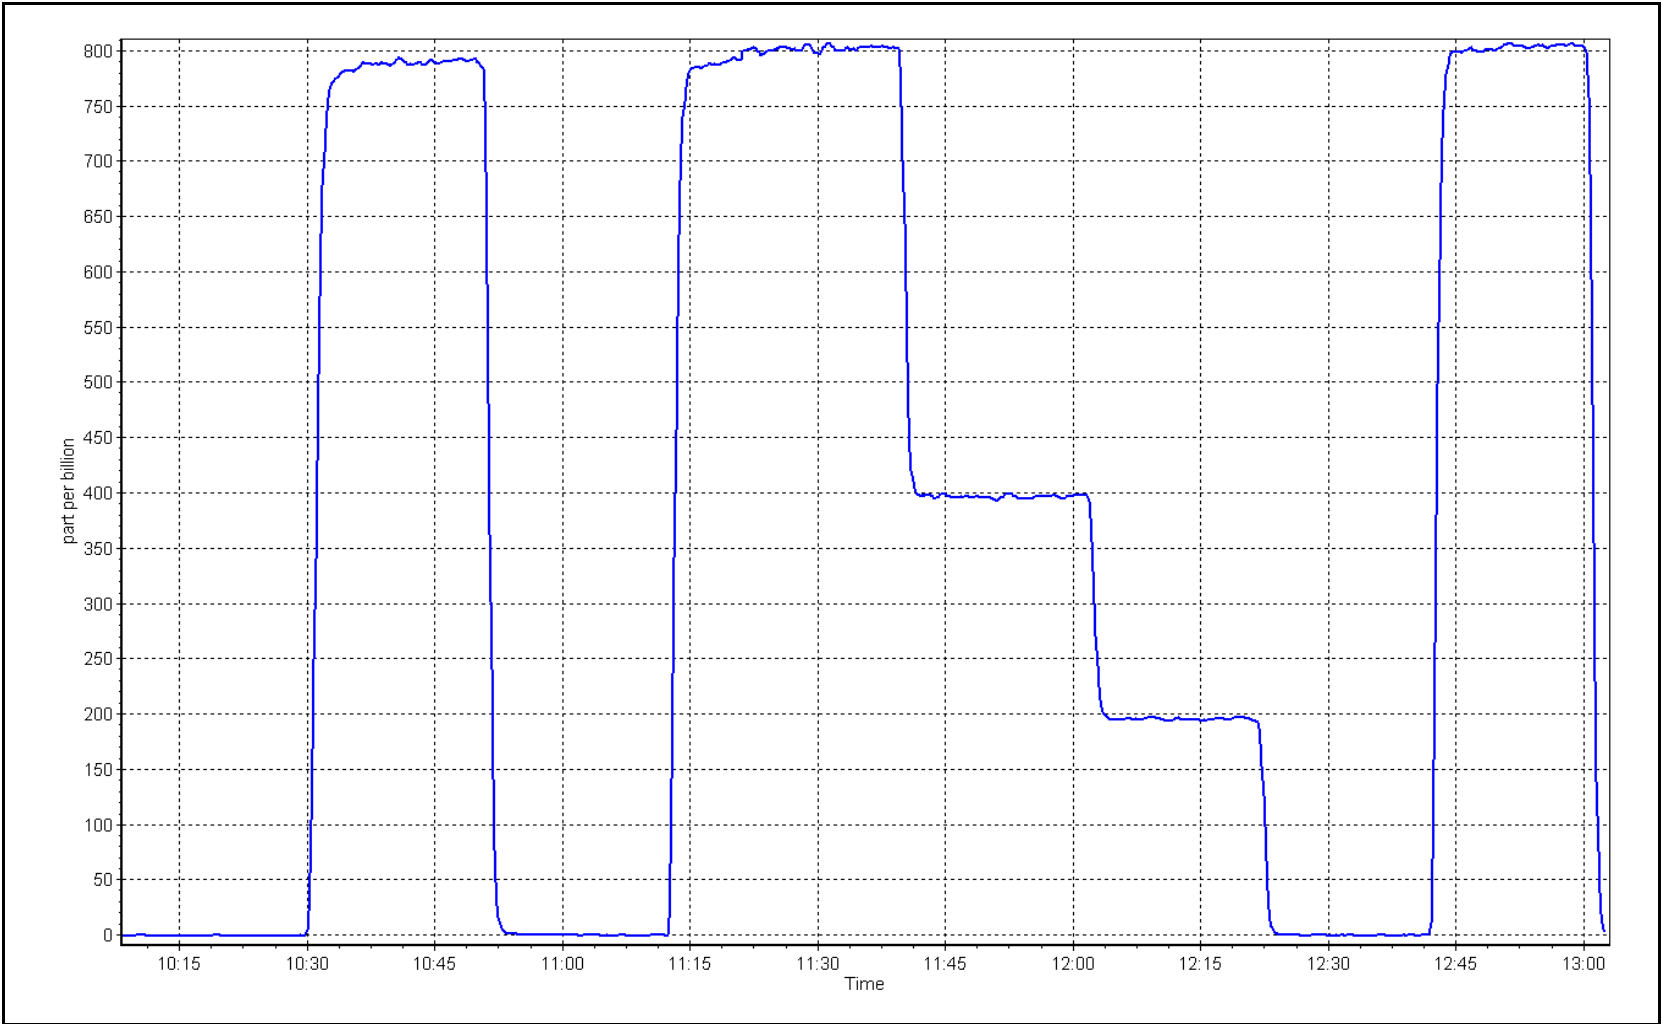



Wood Buffalo Environmental Association

TRS Calibration Report

Version-11-2021

Station Information

Station Name: Ells River Station number: AMS30
 Calibration Date: January 5, 2023 Last Cal Date: December 5, 2022
 Start time (MST): 8:33 End time (MST): 12:20
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.08 ppm Cal Gas Exp Date: February 9, 2024
 Cal Gas Cylinder #: EY0002443
 Removed Cal Gas Conc: 5.08 ppm Rem Gas Exp Date:
 Removed Gas Cyl #: Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 3061
 ZAG Make/Model: API T701H Serial Number: 358

Analyzer Information

Analyzer make: Thermo 43i TLE Analyzer serial #: 1410661331
 Converter make: CDN - 101 Converter serial #: 555
 Analyzer Range 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.027511	1.029508	Backgd or Offset:	1.58	1.59
Calibration intercept:	0.160157	0.140267	Coeff or Slope:	1.123	1.123

TRS As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.0	----
as found span	4921	78.7	80.0	82.2	0.973
as found 2nd point	4961	39.4	40.0	40.7	0.983
as found 3rd point	4980	19.7	20.0	20.3	0.986
new cylinder response					

TRS Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.2	----
high point	4921	78.7	80.0	82.5	0.969
second point	4961	39.4	40.0	41.3	0.969
third point	4980	19.7	20.0	20.7	0.967
as left zero	5000	0.0	0.0	0.4	----
as left span	4921	78.7	80.0	82.3	0.972
SO2 Scrubber Check	4921	79.2	800.4	-0.1	----
Date of last scrubber change:	N/A		Ave Corr Factor		0.968
Date of last converter efficiency test:	N/A		95.1% efficiency		

Baseline Corr As found: 82.2 Prev response: 82.32 *% change: -0.2%
 Baseline Corr 2nd AF pt: 40.7 AF Slope: 1.028504 AF Intercept: -0.199604
 Baseline Corr 3rd AF pt: 20.3 AF Correlation: 0.999961

* = > +/-5% change initiates investigation

Notes: No adjustments required.

Calibration Performed By: Denny Ray Estador



Wood Buffalo Environmental Association

TRS Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 5, 2023	Previous Calibration:	December 5, 2022
Station Name:	Ells River	Station Number:	AMS30
Start Time (MST):	8:33	End Time (MST):	12:20
Analyzer make:	Thermo 43i TLE	Analyzer serial #:	1410661331

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.2	----	Correlation Coefficient	0.999997	
80.0	82.5	0.9693			≥0.995
40.0	41.3	0.9692	Slope	1.029508	
20.0	20.7	0.9670			0.90 - 1.10
			Intercept	0.140267	+/-3

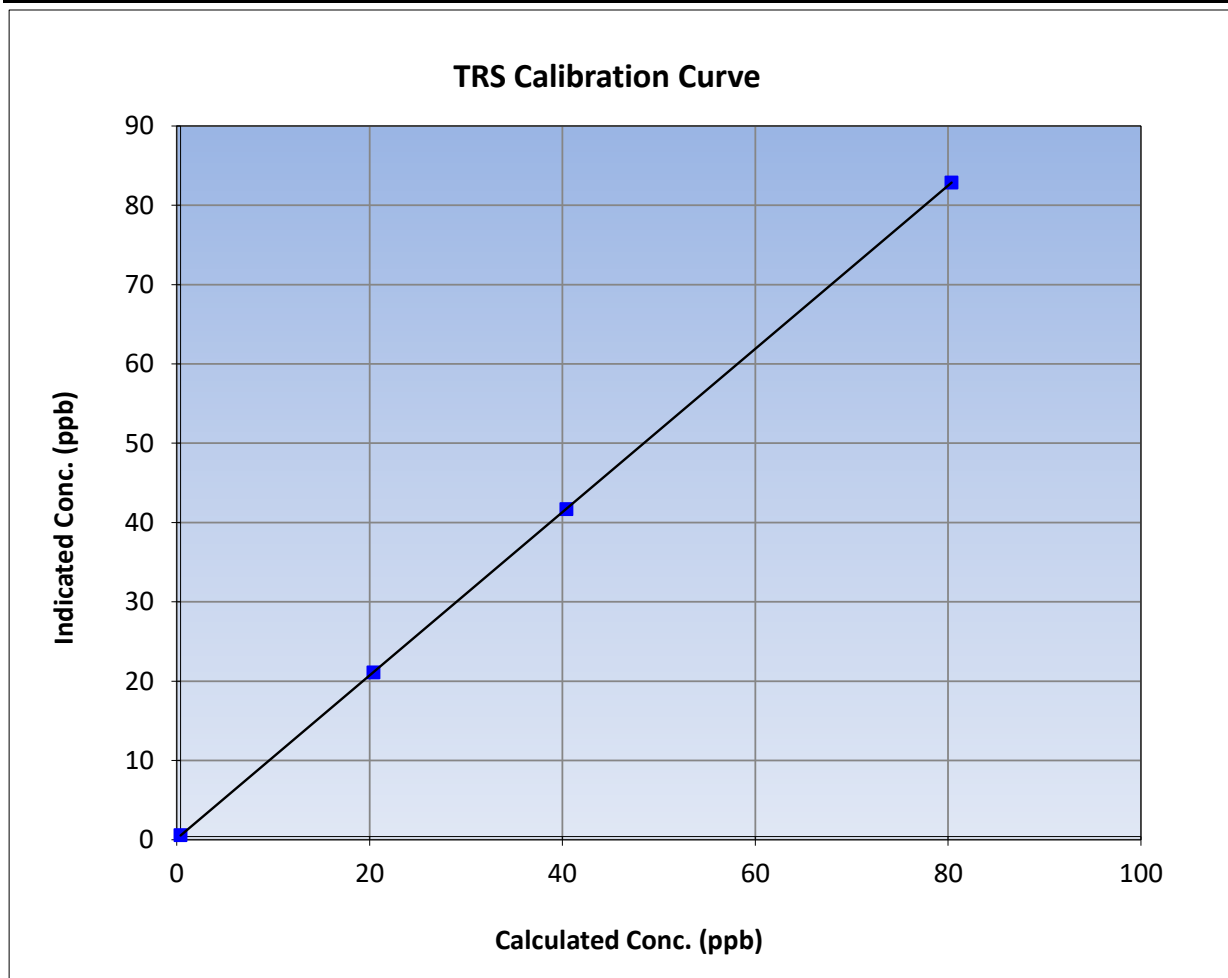

TRS Calibration Plot

Date: January 5, 2023

Location: Ells River

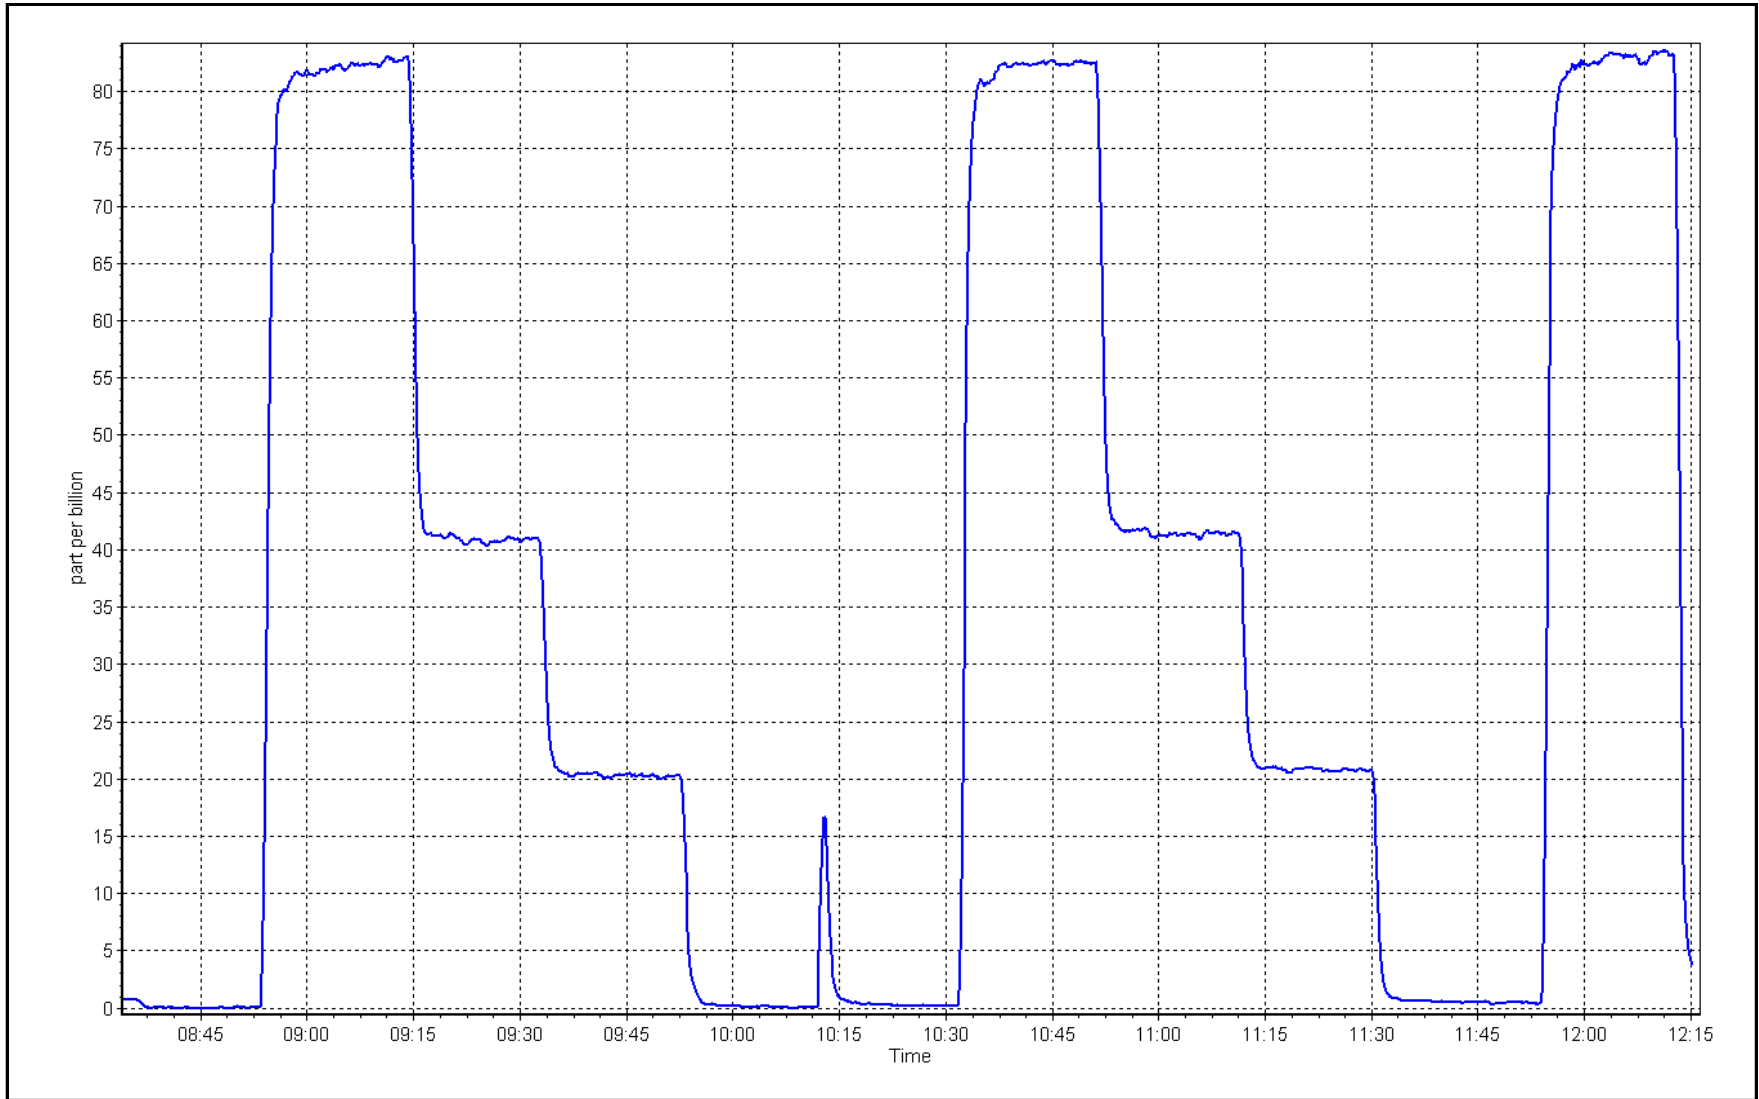



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Ells River	Station number:	AMS 30
Calibration Date:	January 1, 2023	Last Cal Date:	December 2, 2022
Start time (MST):	13:30	End time (MST):	17:40
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC494126	Cal Gas Expiry Date:	December 29, 2028
CH ₄ Cal Gas Conc.	499.7 ppm	CH ₄ Equiv Conc.	1075.0 ppm
C ₃ H ₈ Cal Gas Conc.	209.2 ppm		
Removed Gas Cert:		Removed Gas Expiry:	
Removed CH ₄ Conc.	499.7 ppm	CH ₄ Equiv Conc.	1075.0 ppm
Removed C ₃ H ₈ Conc.	209.2 ppm		
Diff between cyl (CH ₄):		Diff between cyl (THC):	
Calibrator Model:	API T700	Diff between cyl (NM):	
ZAG make/model:	API T701H	Serial Number:	3061
		Serial Number:	358

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1193585650
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	0.000236	0.000256	NMHC SP Ratio:	5.05E-05
CH ₄ Retention time:	13.2	13.2	NMHC Peak Area:	177985

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4921	79.2	17.03	16.94	1.005
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4921	79.2	17.03	16.96	1.004
second point	4960	39.6	8.51	8.37	1.017
third point	4980	19.8	4.26	4.16	1.024
as left zero	5000	0.0	0.00	0.00	----
as left span	4921	79.2	17.03	18.76	0.908

Average Correction Factor				1.015
Baseline Corr AF:	16.94	Prev response	16.94	*% change 0.0%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4921	79.2	9.11	9.05	1.007
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4921	79.2	9.11	9.10	1.001
second point	4960	39.6	4.56	4.52	1.008
third point	4980	19.8	2.28	2.26	1.009
as left zero	5000	0	0.00	0.00	----
as left span	4921	79.2	9.11	10.19	0.894
Average Correction Factor					1.006
Baseline Corr AF:	9.05	Prev response	9.07	*% change	-0.2%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4921	79.2	7.91	7.89	1.003
as found 2nd point					
as found 3rd point					
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4921	79.2	7.91	7.86	1.007
second point	4960	39.6	3.96	3.85	1.027
third point	4980	19.8	1.98	1.90	1.042
as left zero	5000	0.0	0.00	0.00	----
as left span	4921	79.2	7.91	8.57	0.924
Average Correction Factor					1.025
Baseline Corr AF:	7.89	Prev response	7.87	*% change	0.2%
Baseline Corr 2nd AF:	NA	AF Slope:		AF Intercept:	
Baseline Corr 3rd AF:	NA	AF Correlation:		* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	1.000865	0.997012
THC Cal Offset:	-0.098736	-0.054536
CH ₄ Cal Slope:	1.001593	0.994373
CH ₄ Cal Offset:	-0.052956	-0.040955
NMHC Cal Slope:	0.999982	0.998992
NMHC Cal Offset:	-0.044780	-0.012581

Notes: N2 cylinder changed at 14:07 MST. No change in response to span. Noticed ambient readings were below global background, turned on "use zero chromatogram" and calibrated

Calibration Performed By: Ryan Power



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 1, 2023	Previous Calibration:	December 2, 2022
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	13:30	End Time (MST):	17:40
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585650

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999940	≥ 0.995
17.03	16.96	1.0039			
8.51	8.37	1.0170	Slope	0.997012	0.90 - 1.10
4.26	4.16	1.0236			
			Intercept	-0.054536	± 0.5

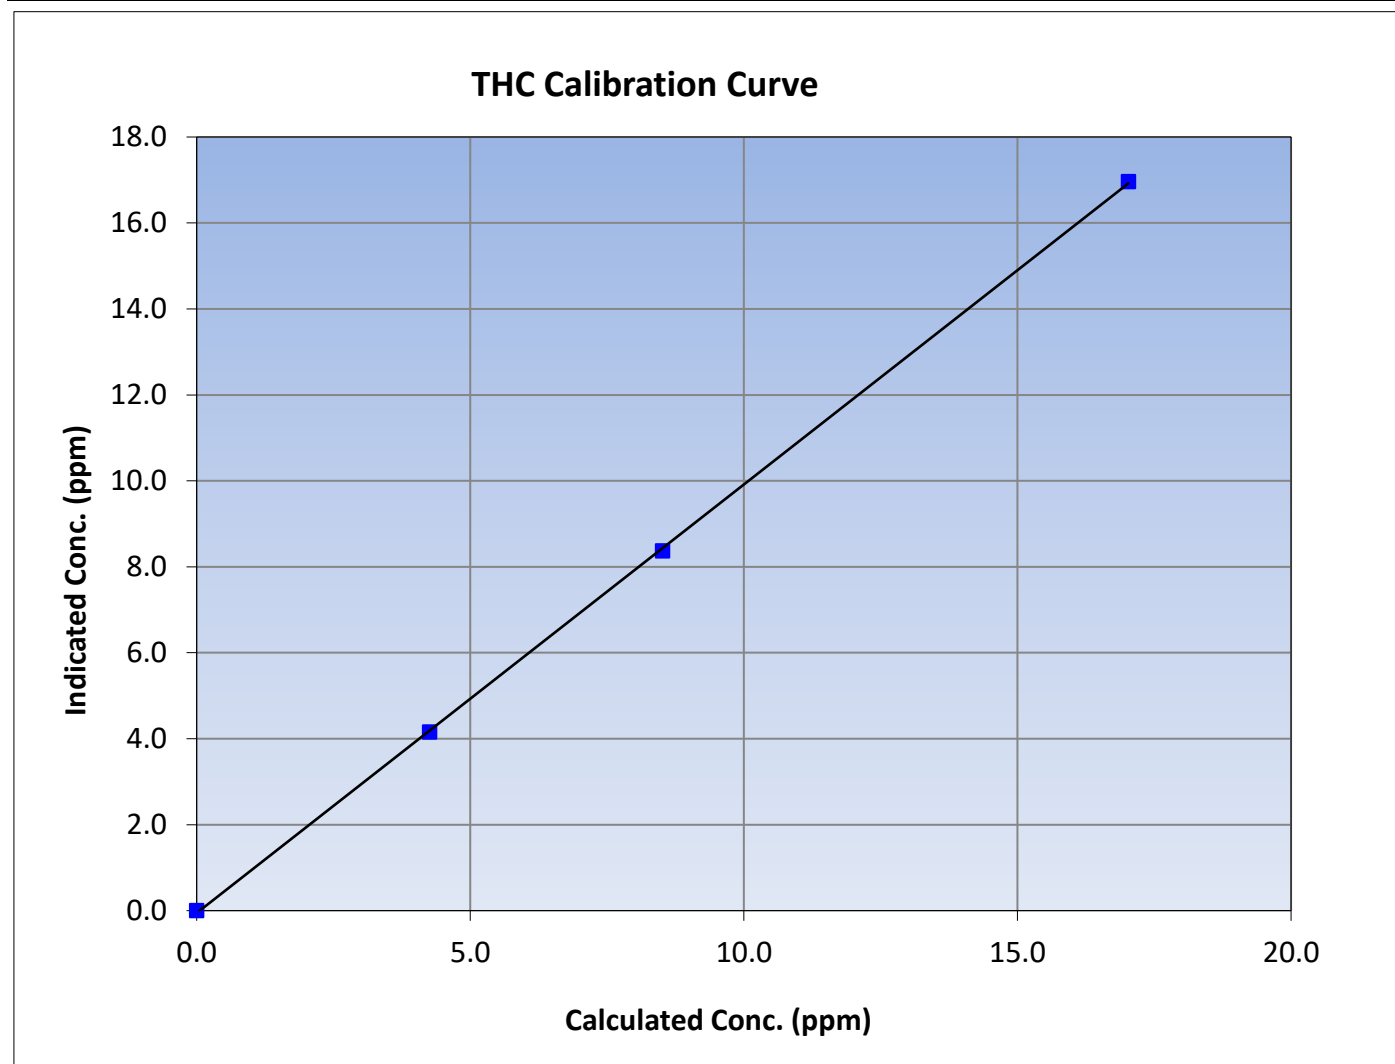



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 1, 2023	Previous Calibration:	December 2, 2022
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	13:30	End Time (MST):	17:40
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585650

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999856	≥0.995
7.91	7.86	1.0074			
3.96	3.85	1.0272			
1.98	1.90	1.0415			
			Slope	0.994373	0.90 - 1.10
			Intercept	-0.040955	+/-0.5

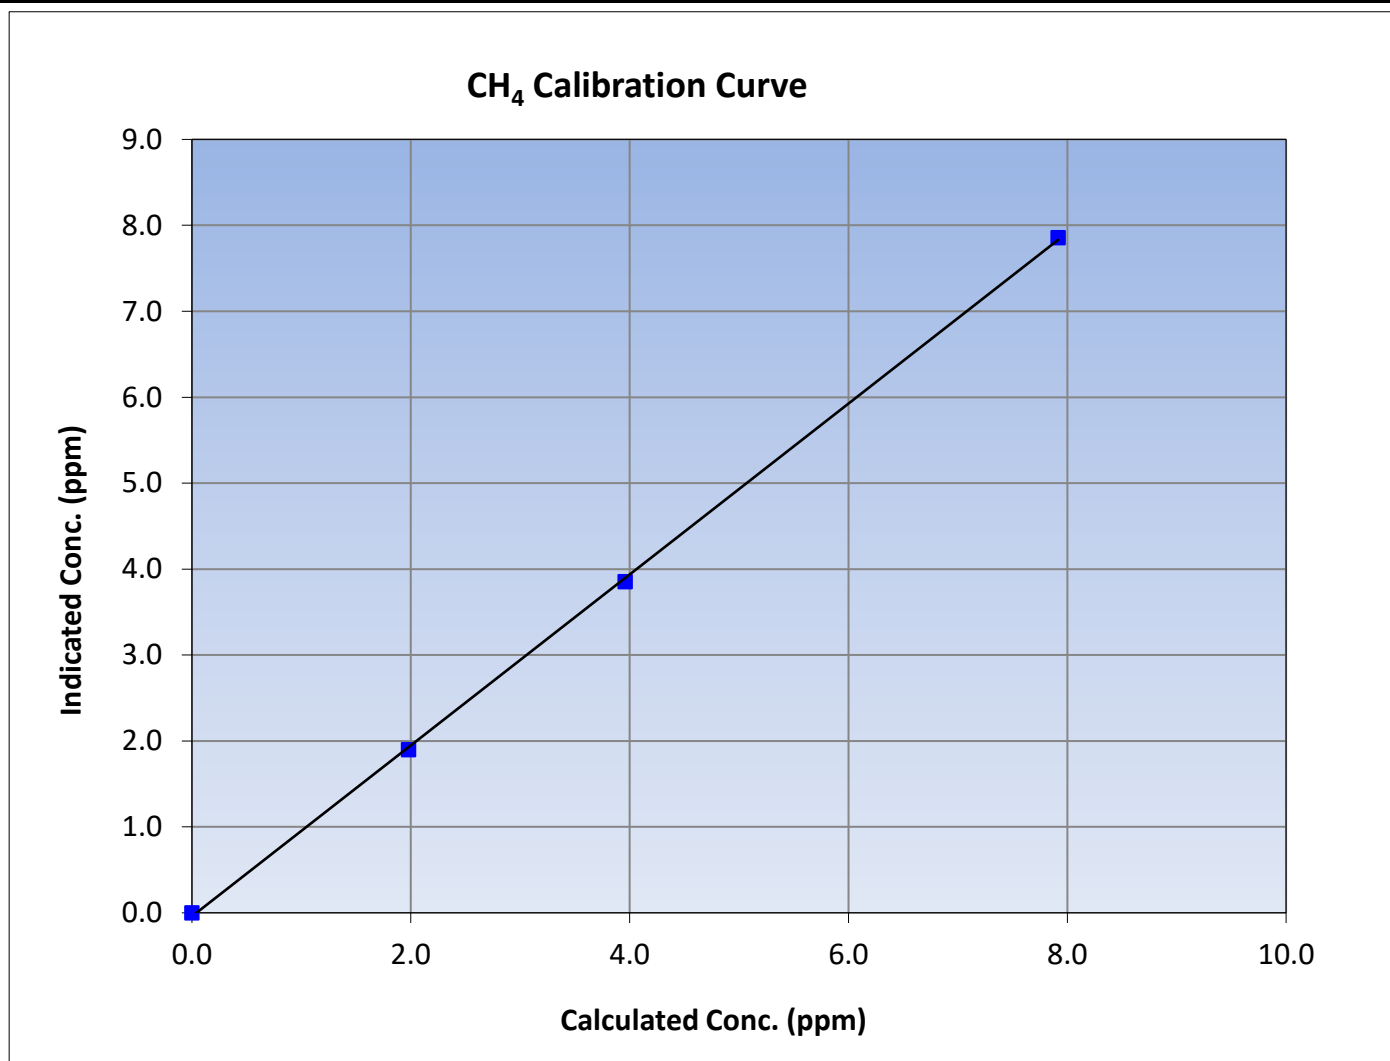



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 1, 2023	Previous Calibration:	December 2, 2022
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	13:30	End Time (MST):	17:40
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585650

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>
0.00	0.00	----	Correlation Coefficient	0.999986	≥ 0.995
9.11	9.10	1.0013			
4.56	4.52	1.0079			
2.28	2.26	1.0085			
			Slope	0.998992	0.90 - 1.10
			Intercept	-0.012581	+/-0.5

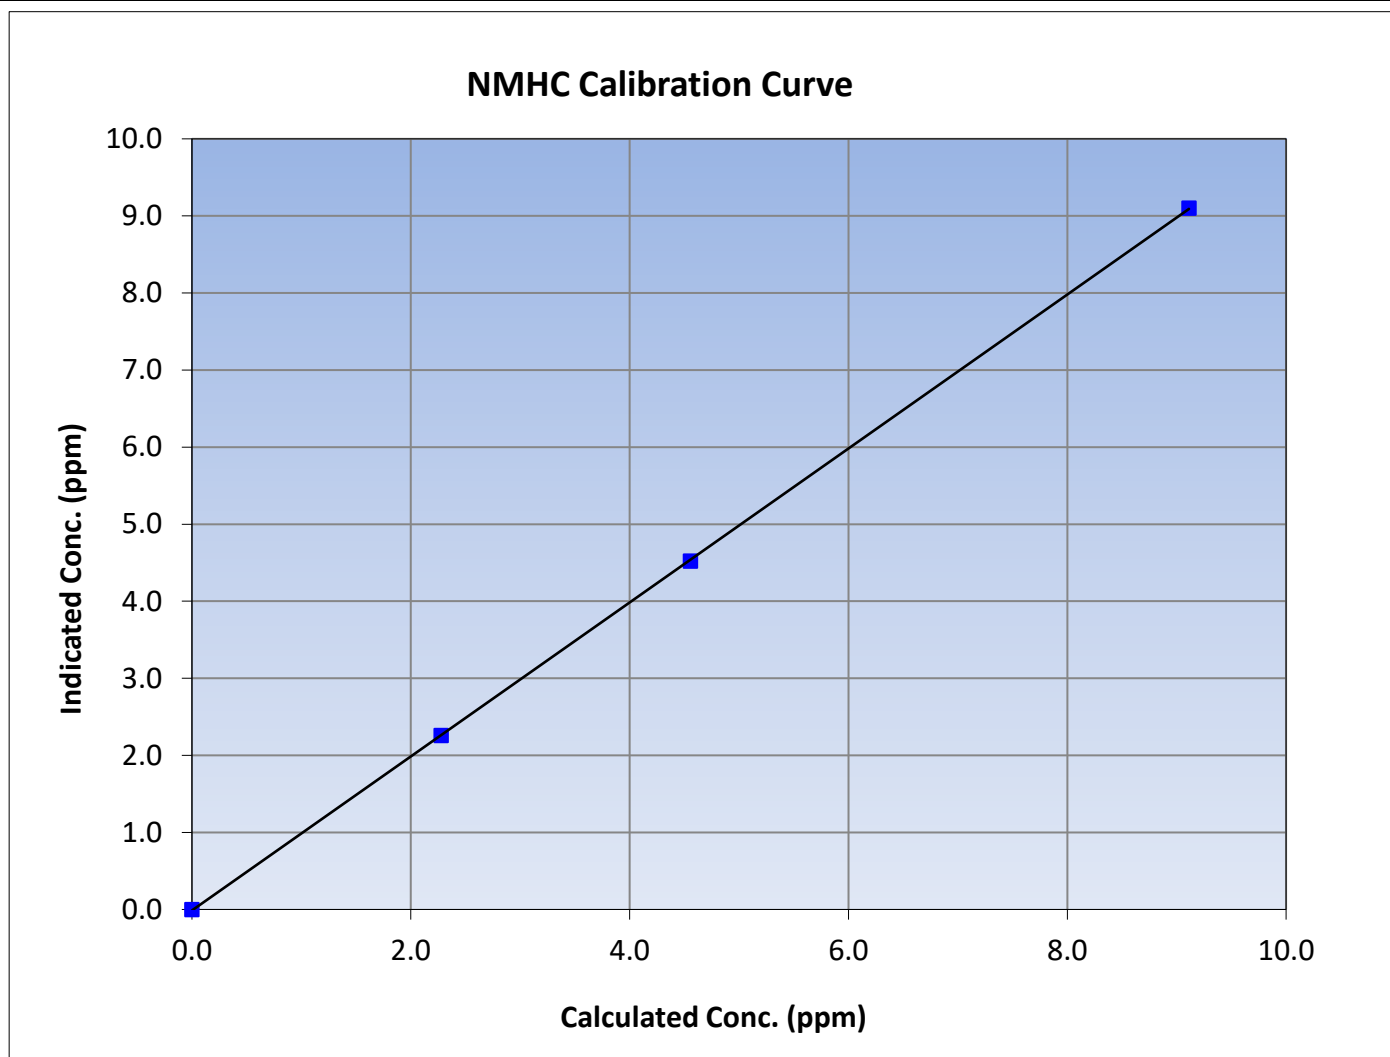

NMHC Calibration Plot

Date: January 1, 2023

Location: Ells River

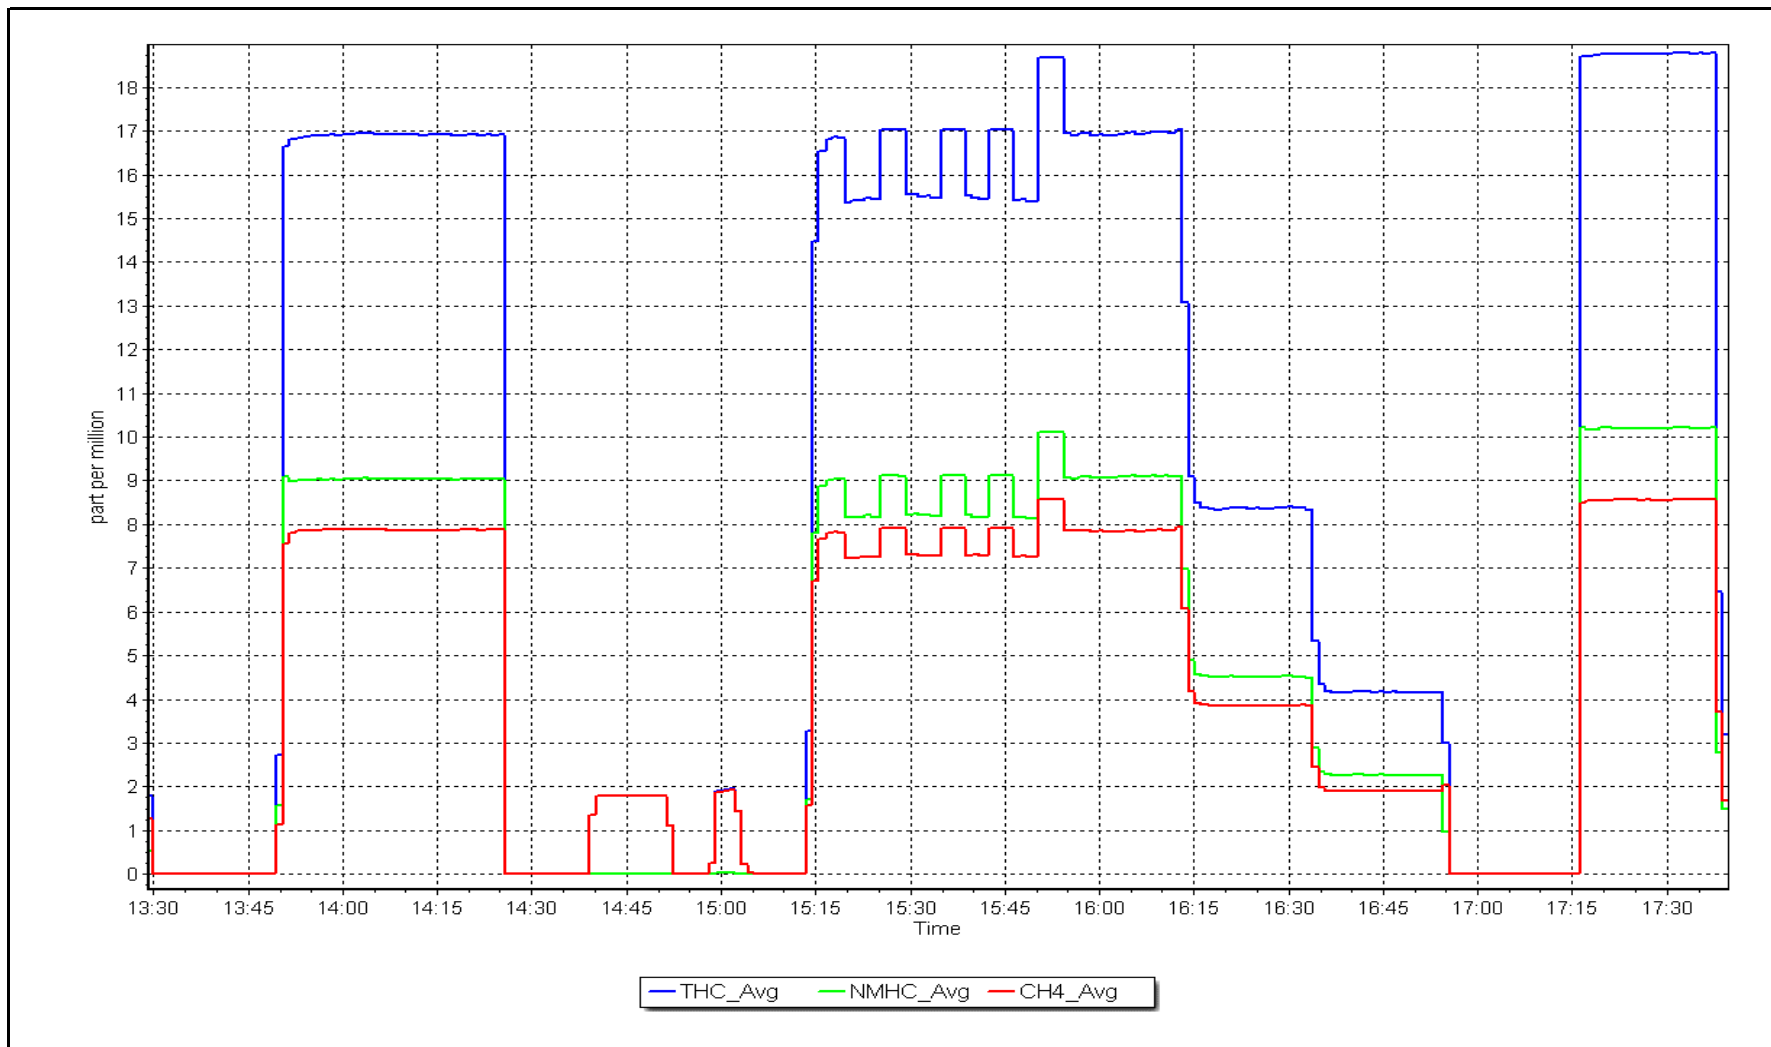



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

Station Information

Station Name:	Ells River	Station number:	AMS 30
Calibration Date:	January 2, 2023	Last Cal Date:	January 1, 2023
Start time (MST):	10:20	End time (MST):	14:51
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC494126	Cal Gas Expiry Date:	December 29, 2028
CH ₄ Cal Gas Conc.	499.7 ppm	CH ₄ Equiv Conc.	1075.0 ppm
C ₃ H ₈ Cal Gas Conc.	209.2 ppm		
Removed Gas Cert:		Removed Gas Expiry:	
Removed CH ₄ Conc.	499.7 ppm	CH ₄ Equiv Conc.	1075.0 ppm
Removed C ₃ H ₈ Conc.	209.2 ppm		
Diff between cyl (CH ₄):		Diff between cyl (THC):	
		Diff between cyl (NM):	
Calibrator Model:	API T700	Serial Number:	3061
ZAG make/model:	API T701H	Serial Number:	358

Analyzer Information

Analyzer make:	Thermo 55i	Analyzer serial #:	1193585650
THC Range (ppm):	0 - 20 ppm		
NMHC Range (ppm):	0 - 10 ppm	CH ₄ Range (ppm):	0 - 10 ppm

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
CH ₄ SP Ratio:	0.000256	0.000234	NMHC SP Ratio:	5.68E-05
CH ₄ Retention time:	13.2	13.2	NMHC Peak Area:	177985
				180847

THC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4921	79.2	17.03	18.22	0.934
as found 2nd point	4960	39.6	8.51	8.89	0.958
as found 3rd point	4980	19.8	4.26	4.38	0.973
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4921	79.2	17.03	17.10	0.996
second point	4960	39.6	8.51	8.41	1.012
third point	4980	19.8	4.26	4.14	1.030
as left zero	5000	0.0	0.00	0.00	----
as left span	4921	79.2	17.03	17.12	0.995
Average Correction Factor					1.013
Baseline Corr AF:	18.22	Prev response	16.92	*% change	7.1%
Baseline Corr 2nd AF:	8.9	AF Slope:	1.072185	AF Intercept:	-0.116558
Baseline Corr 3rd AF:	4.4	AF Correlation:	0.999774	<i>* = > +/-5% change initiates investigation</i>	



Wood Buffalo Environmental Association

THC / CH₄ / NMHC Calibration Report

Version-01-2020

NMHC Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0	0.00	0.00	----
as found span	4921	79.2	9.11	9.88	0.922
as found 2nd point	4960	39.6	4.56	4.84	0.941
as found 3rd point	4980	19.8	2.28	2.40	0.951
new cylinder response					
calibrator zero	5000	0	0.00	0.00	----
high point	4921	79.2	9.11	9.17	0.994
second point	4960	39.6	4.56	4.53	1.006
third point	4980	19.8	2.28	2.24	1.019
as left zero	5000	0	0.00	0.00	----
as left span	4921	79.2	9.11	9.18	0.993
Average Correction Factor					1.006
Baseline Corr AF:	9.88	Prev response	9.09	*% change	8.0%
Baseline Corr 2nd AF:	4.8	AF Slope:	1.085893	AF Intercept:	-0.049795
Baseline Corr 3rd AF:	2.4	AF Correlation:	0.999854	* = > +/-5% change initiates investigation	

CH₄ Calibration Data

Set Point	Dil air flow rate	Source gas flow rate	Calc conc (ppm) (Cc)	Ind conc (ppm) (Ic)	CF <i>Limit= 0.95-1.05</i>
as found zero	5000	0.0	0.00	0.00	----
as found span	4921	79.2	7.91	8.34	0.949
as found 2nd point	4960	39.6	3.96	4.05	0.978
as found 3rd point	4980	19.8	1.98	1.98	0.999
new cylinder response					
calibrator zero	5000	0.0	0.00	0.00	----
high point	4921	79.2	7.91	7.94	0.997
second point	4960	39.6	3.96	3.88	1.020
third point	4980	19.8	1.98	1.90	1.042
as left zero	5000	0.0	0.00	0.00	----
as left span	4921	79.2	7.91	7.94	0.997
Average Correction Factor					1.020
Baseline Corr AF:	8.34	Prev response	7.83	*% change	6.1%
Baseline Corr 2nd AF:	4.05	AF Slope:	1.056173	AF Intercept:	-0.065963
Baseline Corr 3rd AF:	1.98	AF Correlation:	0.999667	* = > +/-5% change initiates investigation	

Calibration Statistics

	<i>Start</i>	<i>Finish</i>
THC Cal Slope:	0.997012	1.006389
THC Cal Offset:	-0.054536	-0.085138
CH ₄ Cal Slope:	0.994373	1.004928
CH ₄ Cal Offset:	-0.040955	-0.050756
NMHC Cal Slope:	0.998992	1.007959
NMHC Cal Offset:	-0.012581	-0.034582

Notes: Troubleshooting after yesterdays failed As Lefts and todays high daily span. Pump changed after As Finds. Tested options for data processing, "use zero chrome" turned on

Calibration Performed By: Ryan Power



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 2, 2023	Previous Calibration:	January 1, 2023
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	10:20	End Time (MST):	14:51
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585650

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999878	≥ 0.995			
17.03	17.10	0.9955						
8.51	8.41	1.0124				Slope	1.006389	0.90 - 1.10
4.26	4.14	1.0295						
			Intercept	-0.085138	± 0.5			

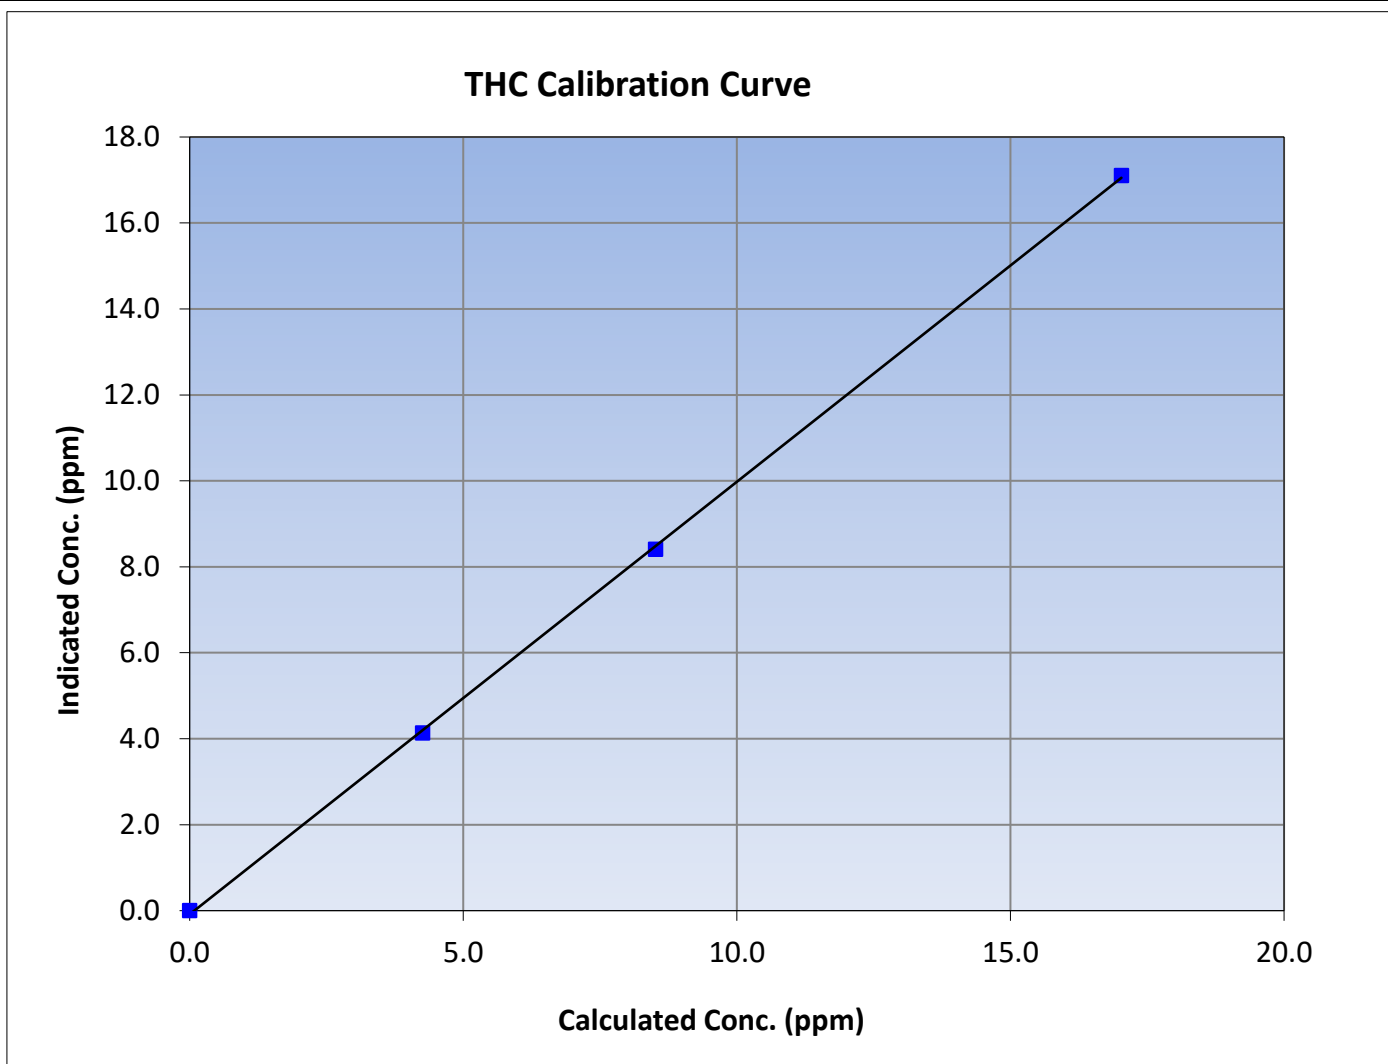



Wood Buffalo Environmental Association

CH₄ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 2, 2023	Previous Calibration:	January 1, 2023
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	10:20	End Time (MST):	14:51
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585650

Calibration Data

Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999797	≥0.995			
7.91	7.94	0.9975						
3.96	3.88	1.0196				Slope	1.004928	0.90 - 1.10
1.98	1.90	1.0415						
			Intercept	-0.050756	+/-0.5			

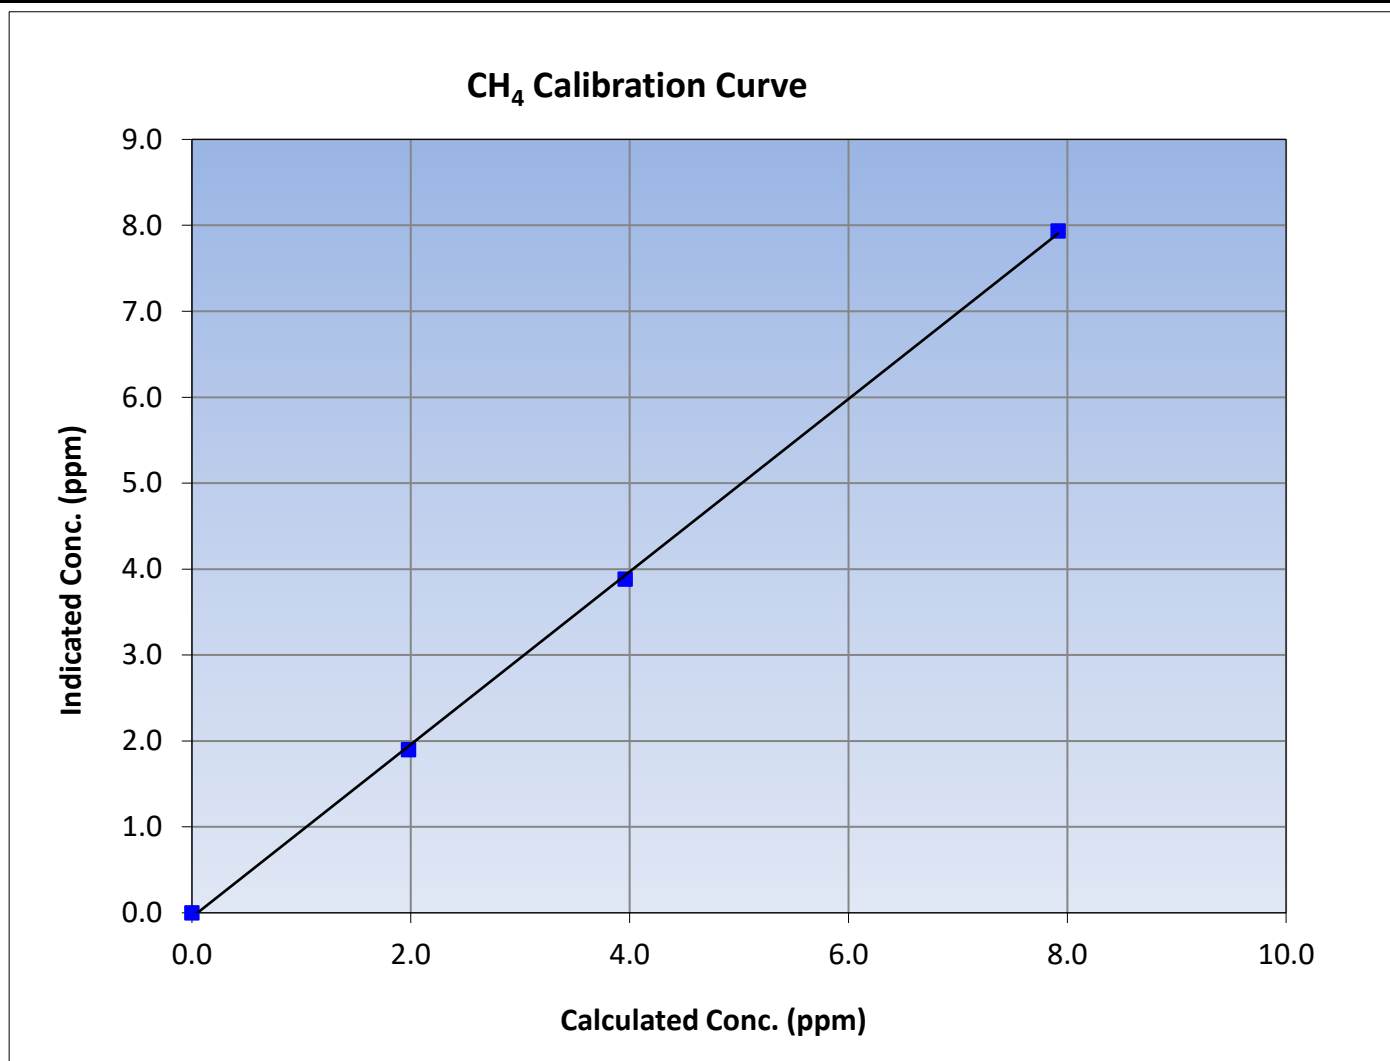



Wood Buffalo Environmental Association

NMHC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 2, 2023	Previous Calibration:	January 1, 2023
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	10:20	End Time (MST):	14:51
Analyzer make:	Thermo 55i	Analyzer serial #:	1193585650

Calibration Data


Calculated concentration (ppm) (Cc)	Indicated concentration (ppm) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		<u>Limits</u>			
0.00	0.00	----	Correlation Coefficient	0.999929	≥ 0.995			
9.11	9.17	0.9935						
4.56	4.53	1.0063				Slope	1.007959	0.90 - 1.10
2.28	2.24	1.0189						
			Intercept	-0.034582	± 0.5			

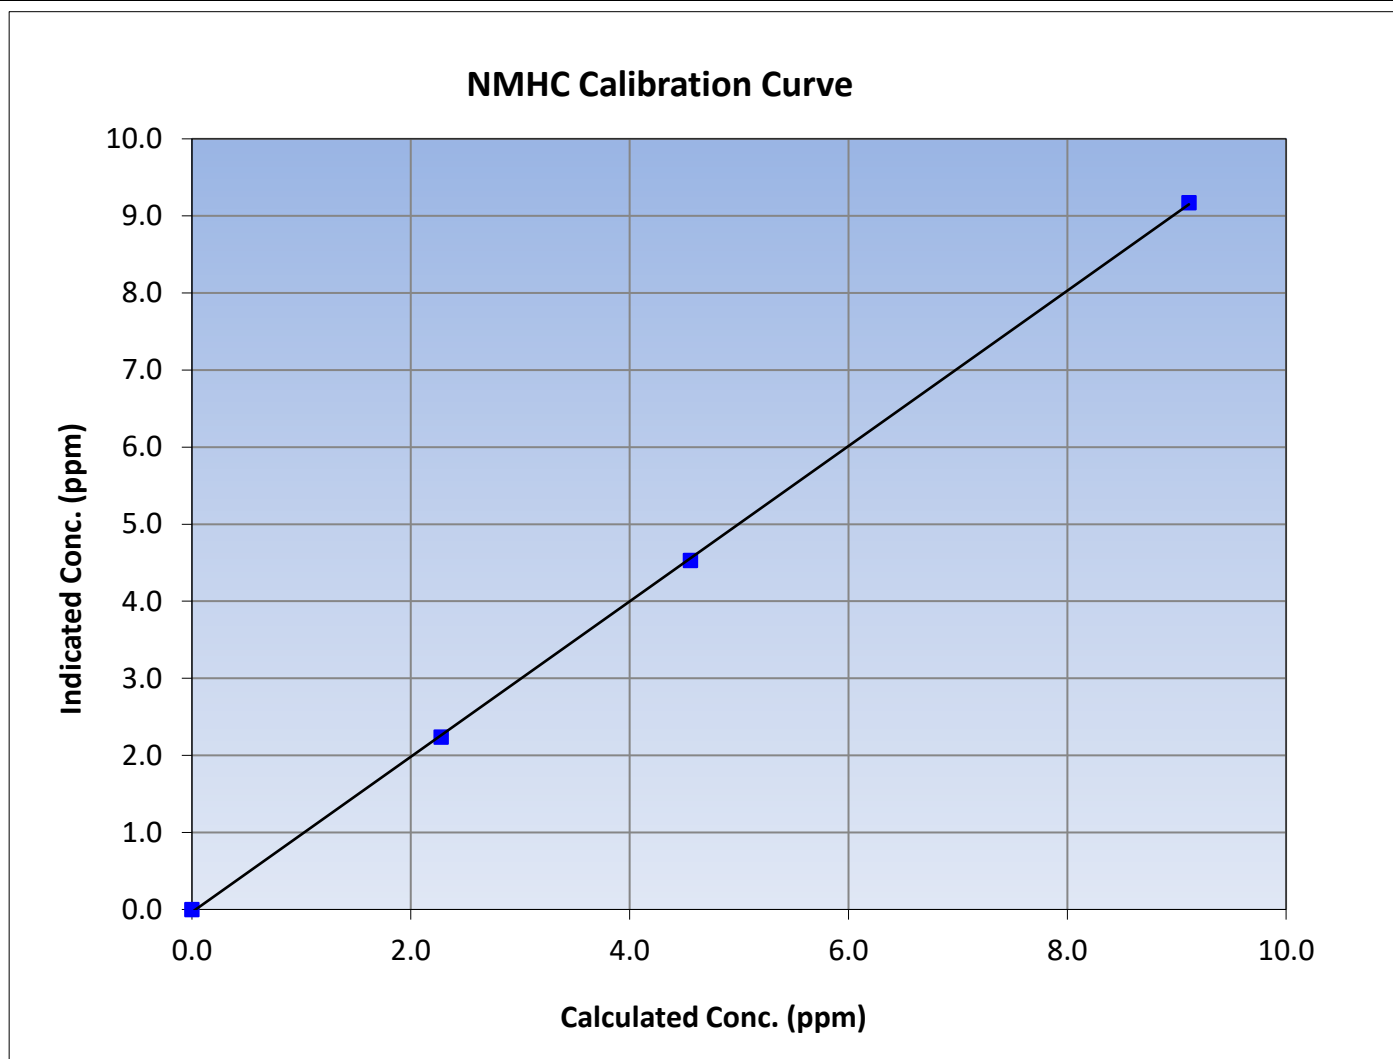

NMHC Calibration Plot

Date: January 2, 2023

Location: Ells River

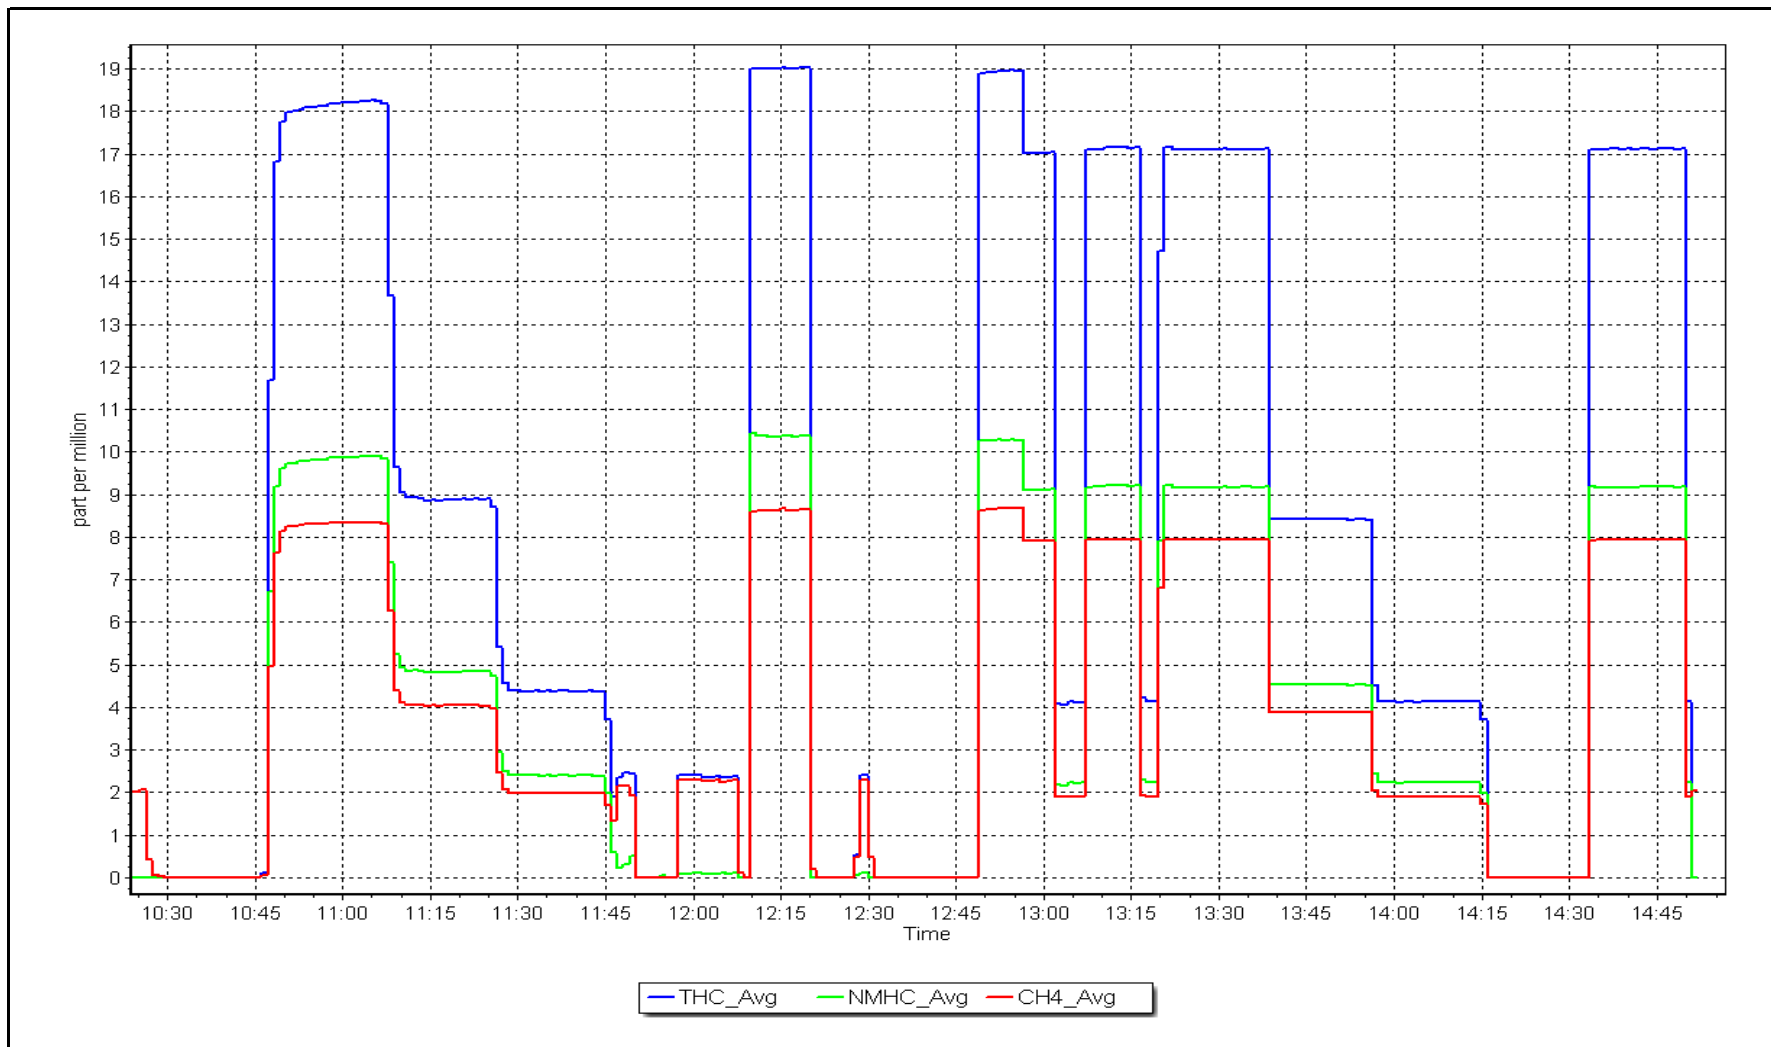



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Station Information

Station Name: Ells River
Calibration Date: January 13, 2023
Start time (MST): 9:13
Reason: Routine
Station number: AMS 30
Last Cal Date: December 12, 2022
End time (MST): 13:30

Calibration Standards

NO Gas Cylinder #: T2Y1P2R
NOX Cal Gas Conc: 50.83 ppm
Removed Cylinder #:
Removed Gas NOX Conc: 50.83 ppm
NOX gas Diff:
Calibrator Model: API T700
ZAG make/model: API T701H
Cal Gas Expiry Date: December 11, 2023
NO Cal Gas Conc: 49.97 ppm
Removed Gas Exp Date:
Removed Gas NO Conc: 49.97 ppm
NO gas Diff:
Serial Number: 3061
Serial Number: 358

Analyzer Information

Analyzer make: Thermo 42i
NOX Range (ppb): 0 - 1000 ppb

Analyzer serial #: 710321429

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
NO coeff or slope:	1.017	1.029	NO bkgnd or offset:	12.4	12.6
NOX coeff or slope:	0.995	0.992	NOX bkgnd or offset:	12.3	12.5
NO2 coeff or slope:	1.000	1.000	Reaction cell Press:	182.1	181.5

Calibration Statistics

	<u>Start</u>	<u>Finish</u>
NO _x Cal Slope:	1.000562	0.998693
NO _x Cal Offset:	-1.060000	-0.720000
NO Cal Slope:	0.996669	0.997541
NO Cal Offset:	-1.600000	-1.280000
NO ₂ Cal Slope:	1.009494	1.000846
NO ₂ Cal Offset:	0.761787	0.511635



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.0	-0.3	0.4	----	----
as found span	4920	80.0	813.3	799.5	13.8	808.1	789.2	18.9	1.0064	1.0131
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.3	0.0	0.3	----	----
high point	4920	80.0	813.3	799.5	13.8	812.0	797.1	14.6	1.0016	1.0030
second point	4960	40.0	406.6	399.8	6.9	404.9	396.3	8.6	1.0043	1.0087
third point	4980	20.0	203.3	199.9	3.4	201.3	197.2	4.1	1.0100	1.0136
as left zero	5000	0.0	0.0	0.0	0.0	0.2	0.0	0.2	----	----
as left span	4920	80.0	813.3	433.3	380.0	813.5	430.9	382.6	0.9997	1.0056
Average Correction Factor									1.0053	1.0085

Corrected As found	NO _x = 808.1 ppb	NO = 789.5 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -0.6%
Previous Response	NO _x = 812.7 ppb	NO = 795.3 ppb		*Percent Change	NO = -0.7%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	793.7	427.5	380.0	380.5	0.9986	100.1%
2nd GPT point (200 ppb O3)	793.7	614.7	192.8	194.1	0.9931	100.7%
3rd GPT point (100 ppb O3)	793.7	702.2	105.3	105.7	0.9958	100.4%
Average Correction Factor					0.9958	100.4%

Notes:

Adjusted the span only.

Calibration Performed By: Denny Ray Estador



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 12, 2022
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	9:13	End Time (MST):	13:30
Analyzer make:	Thermo 42i	Analyzer serial #:	710321429

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.3	----	Correlation Coefficient	≥0.995	
813.3	812.0	1.0016			
406.6	404.9	1.0043			
203.3	201.3	1.0100			
			Slope	0.998693	0.90 - 1.10
			Intercept	-0.720000	+/-20

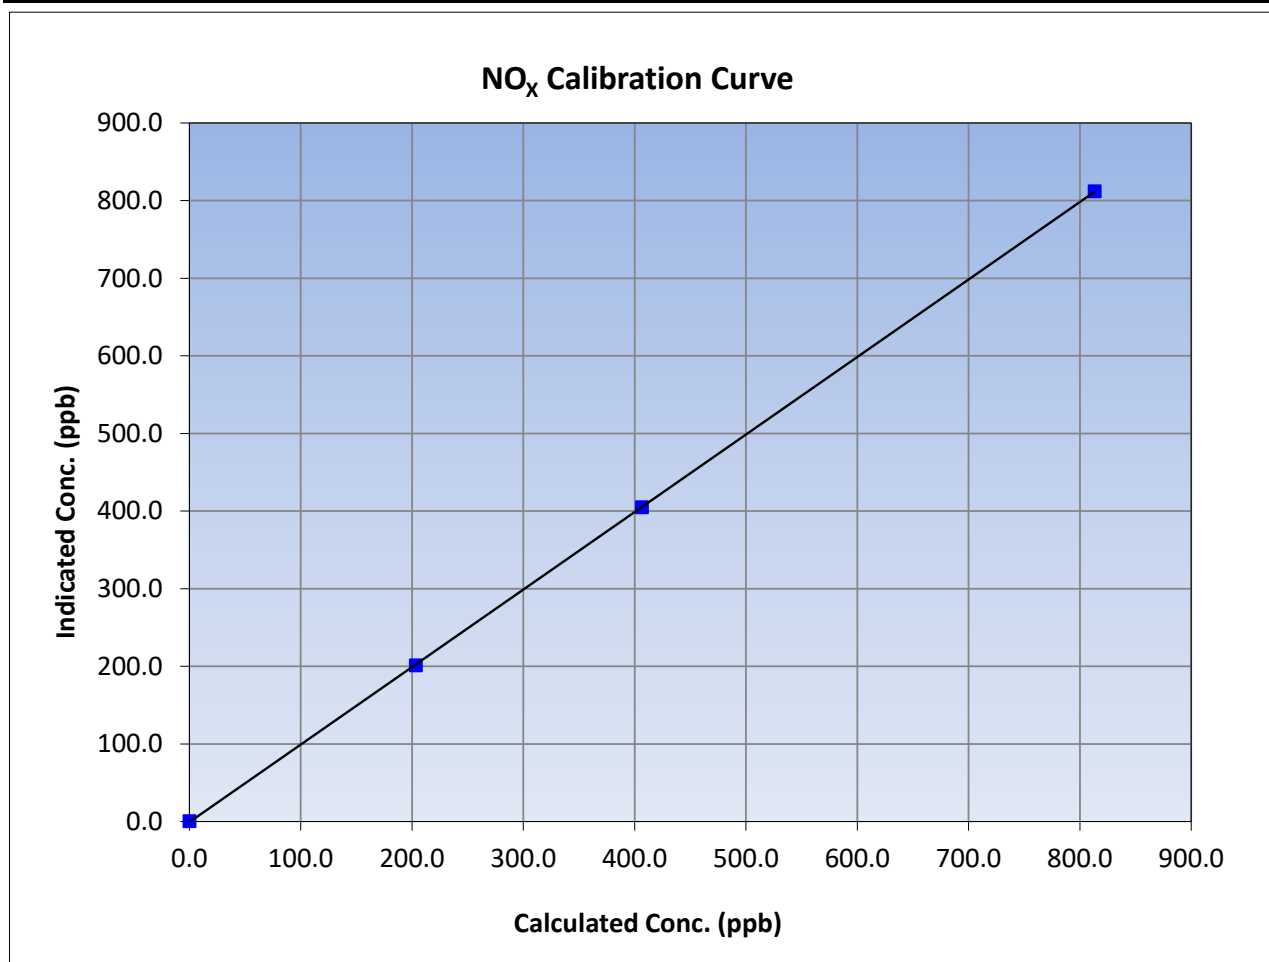



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 12, 2022
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	9:13	End Time (MST):	13:30
Analyzer make:	Thermo 42i	Analyzer serial #:	710321429

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.0	----	Correlation Coefficient	≥0.995	
799.5	797.1	1.0030			
399.8	396.3	1.0087			
199.9	197.2	1.0136			
			Slope	0.997541	0.90 - 1.10
			Intercept	-1.280000	+/-20

NO Calibration Curve

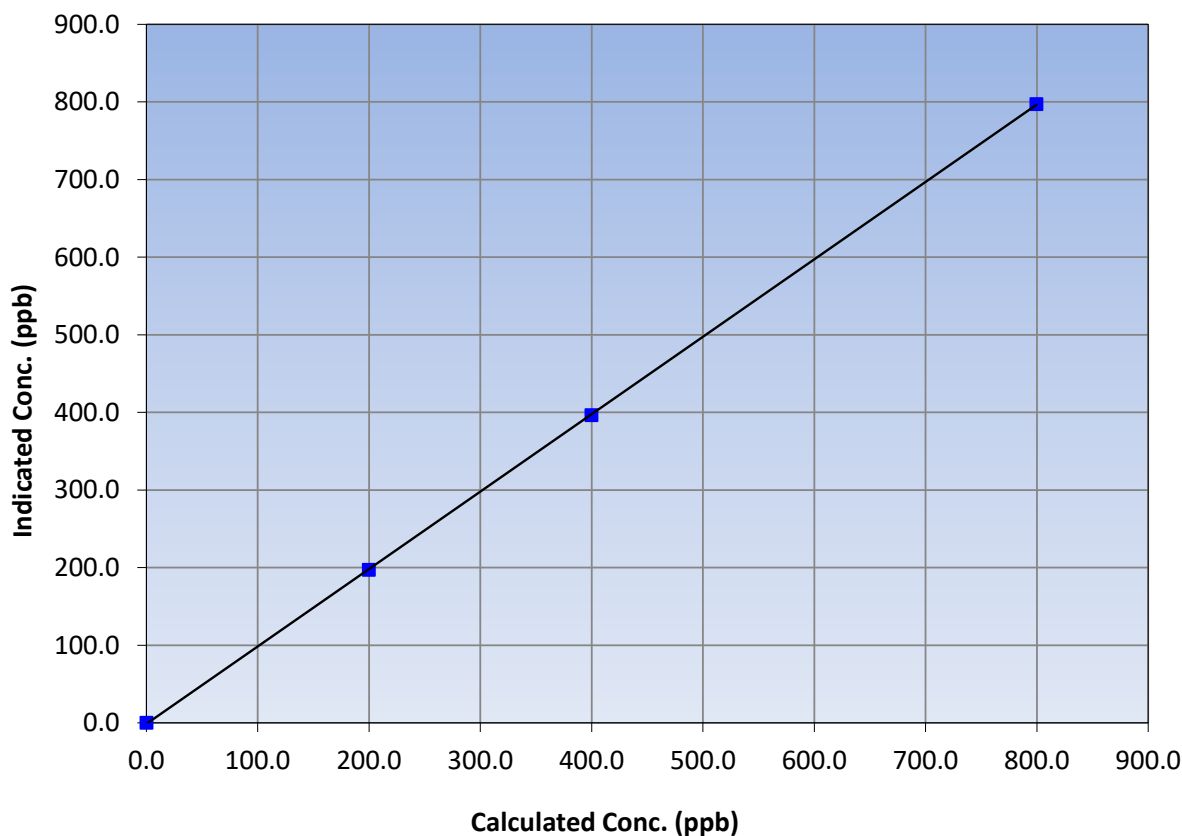



Wood Buffalo Environmental Association

NO₂ Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 13, 2023	Previous Calibration:	December 12, 2022
Station Name:	Ells River	Station Number:	AMS 30
Start Time (MST):	9:13	End Time (MST):	13:30
Analyzer make:	Thermo 42i	Analyzer serial #:	710321429

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation		Limits
0.0	0.3	----	Correlation Coefficient	0.999992	≥0.995
380.0	380.5	0.9986			
192.8	194.1	0.9931			
105.3	105.7	0.9958			
			Slope	1.000846	0.90 - 1.10
			Intercept	0.511635	+/-20

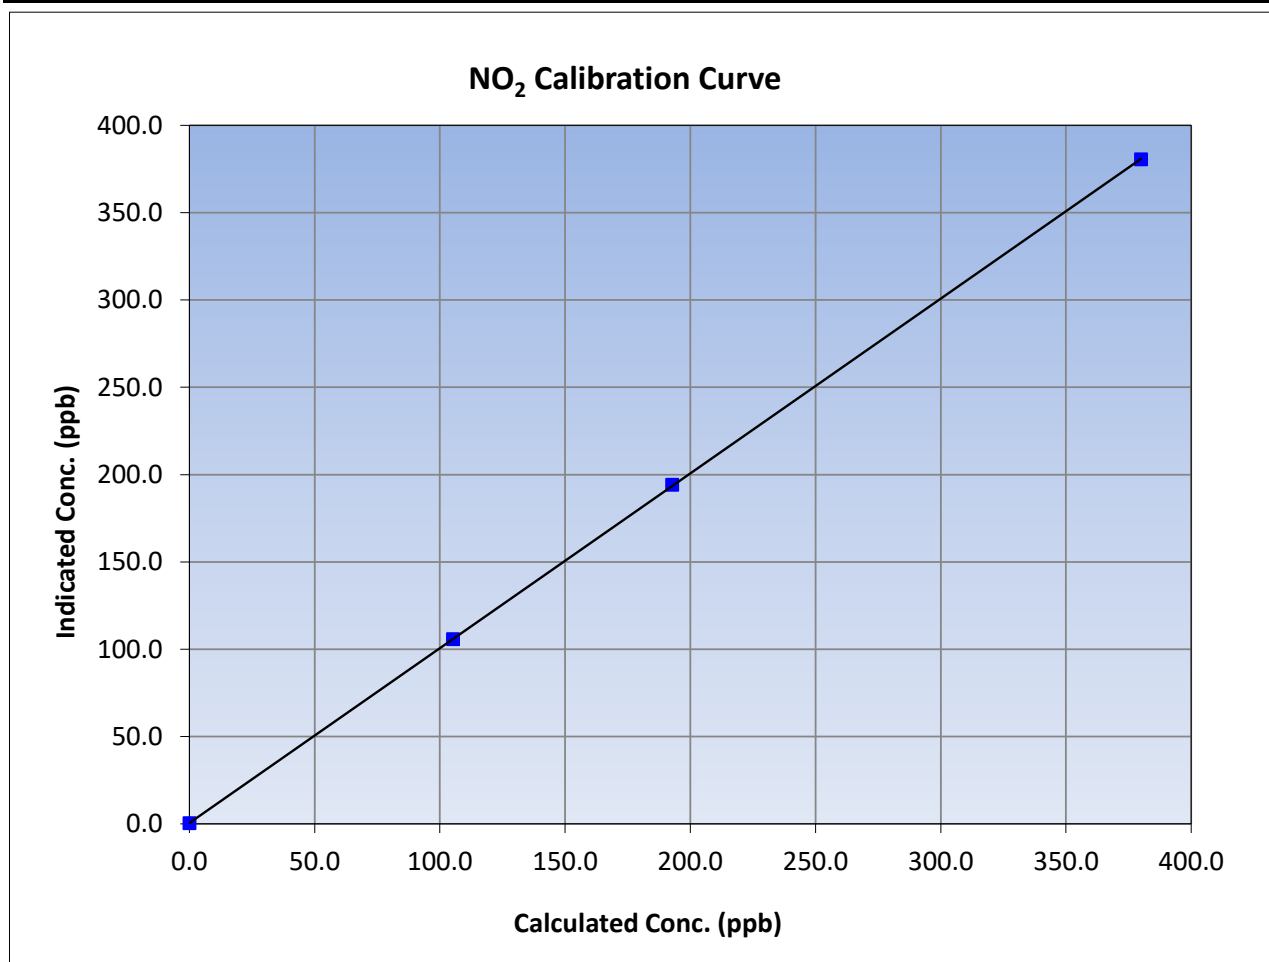

NO_x Calibration Plot

Date: January 13, 2023

Location: Ells River

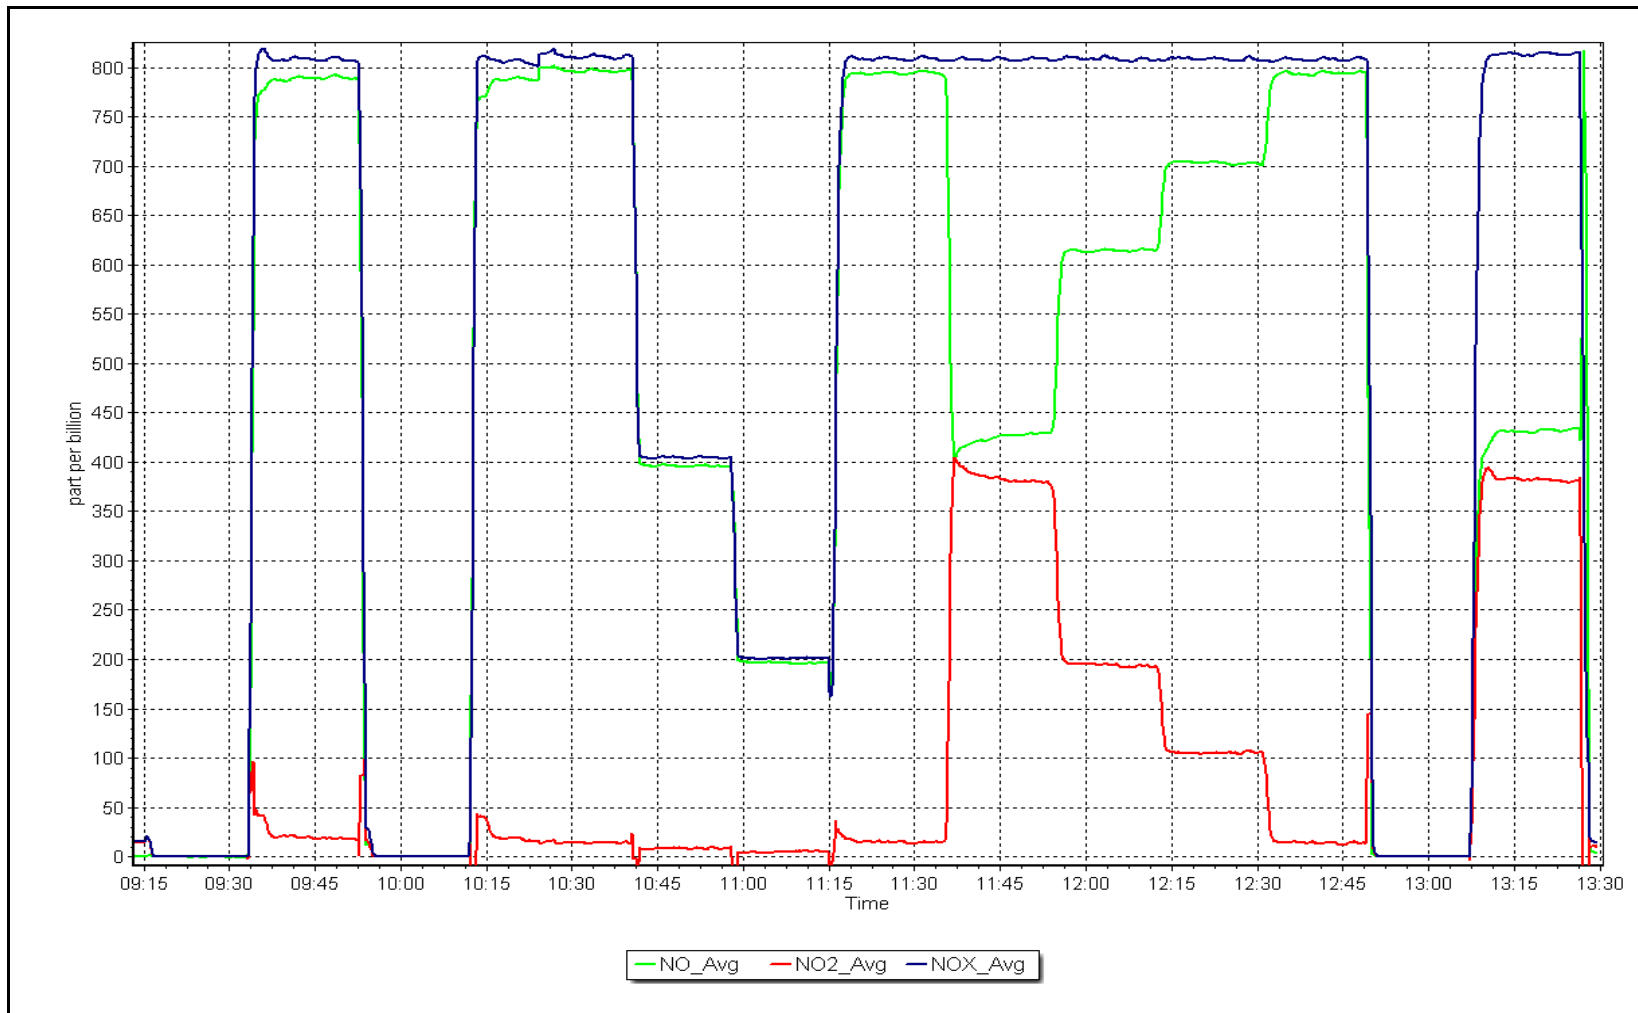



Wood Buffalo Environmental Association

T640 PM_{2.5} CALIBRATION

Version-09-2020

Station Information

Station Name: Ells River Station number: AMS 30
Calibration Date: January 5, 2023 Last Cal Date: December 19, 2022
Start time (MST): 11:42 End time (MST): 12:00

Analyzer Make: API T640 S/N: 875
Particulate Fraction: PM2.5

Flow Meter Make/Model: Delta Cal S/N: 954
Temp/RH standard: Delta Cal S/N: 954

Monthly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
T (°C)	-12.5	-11.9	-12.5	<input type="checkbox"/>	+/- 2 °C
P (mmHg)	731.6	730.5	731.6	<input type="checkbox"/>	+/- 10 mmHg
flow (LPM)	5.02	5.19	5.02	<input type="checkbox"/>	+/- 0.25 LPM

Leak Test: Date of check: January 5, 2023 Last Cal Date: December 19, 2022
PM w/o HEPA: 12.4 PM w/ HEPA: 0.0

Inlet cleaning : Inlet Head

Quarterly Calibration Test

<u>Parameter</u>	<u>As found</u>	<u>Measured</u>	<u>As left</u>	<u>Adjusted</u>	(Limits)
PMT Peak Test				<input type="checkbox"/>	10.9 +/- 0.5

Date Optical Chamber Cleaned: December 19, 2022
Disposable Filter Changed: December 19, 2022

Annual Maintenance

Date Sample Tube Cleaned: October 17, 2022
Date RH/T Sensor Cleaned: October 17, 2022

Notes:

No adjustments required. Inspect inlet head; still clean.

Calibration by: Denny Ray Estador



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS506
JACKFISH 1
JANUARY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 24, 2023	Previous Calibration:	December 16, 2022
Station Name:	Jackfish 1	Station Number:	AMS 506
Start Time (MST):	10:05	End Time (MST):	12:49
Analyzer make:	Thermo 43i	Analyzer serial #:	1160290011

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	-0.3	----	Correlation Coefficient	0.999975	
800.2	804.0	0.9953			≥0.995
400.2	401.5	0.9966	Slope	1.006642	
200.1	197.1	1.0151			0.90 - 1.10
			Intercept	-1.856099	+/-30

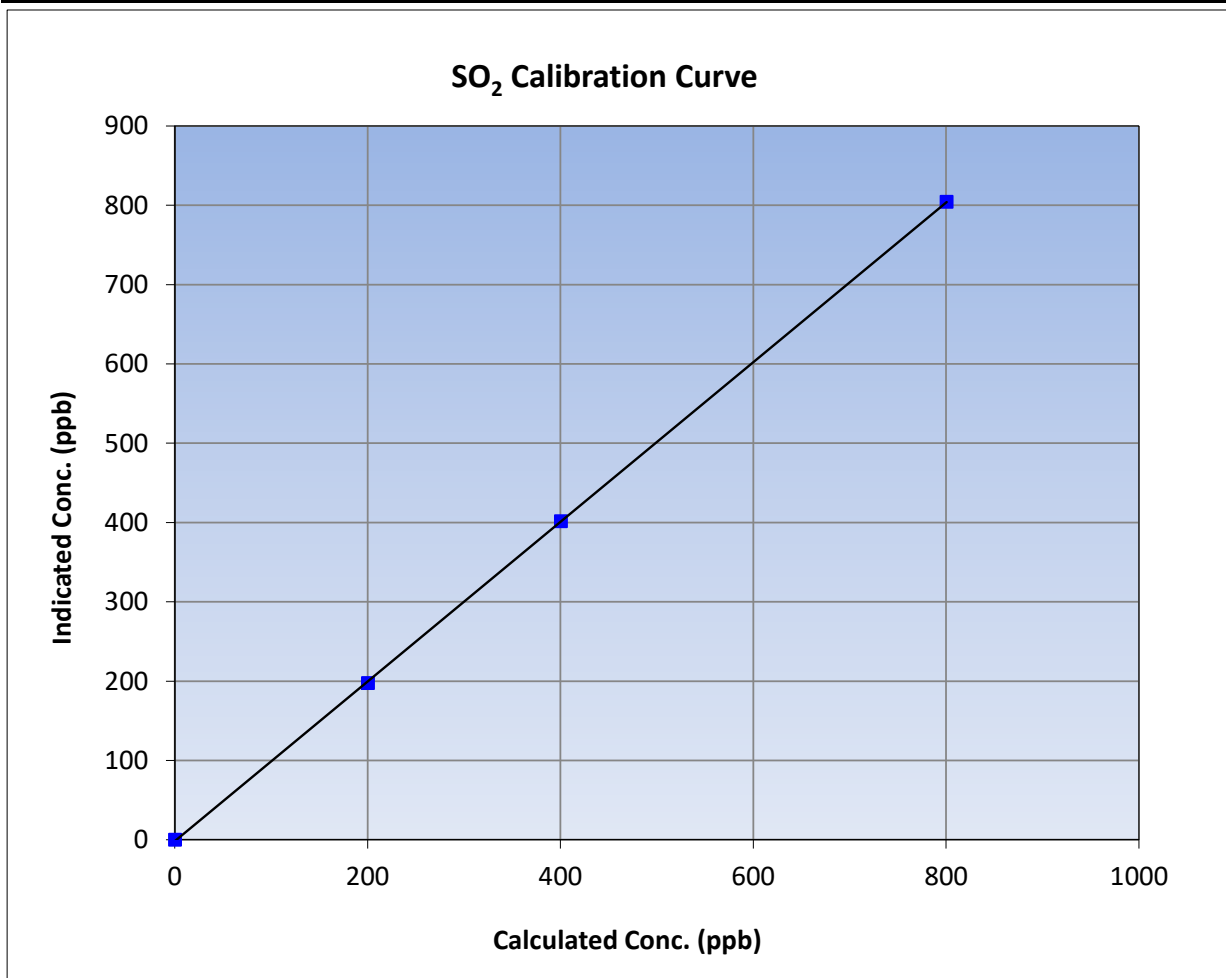

SO2 Calibration Plot

Date: January 24, 2023

Location: Jackfish 1

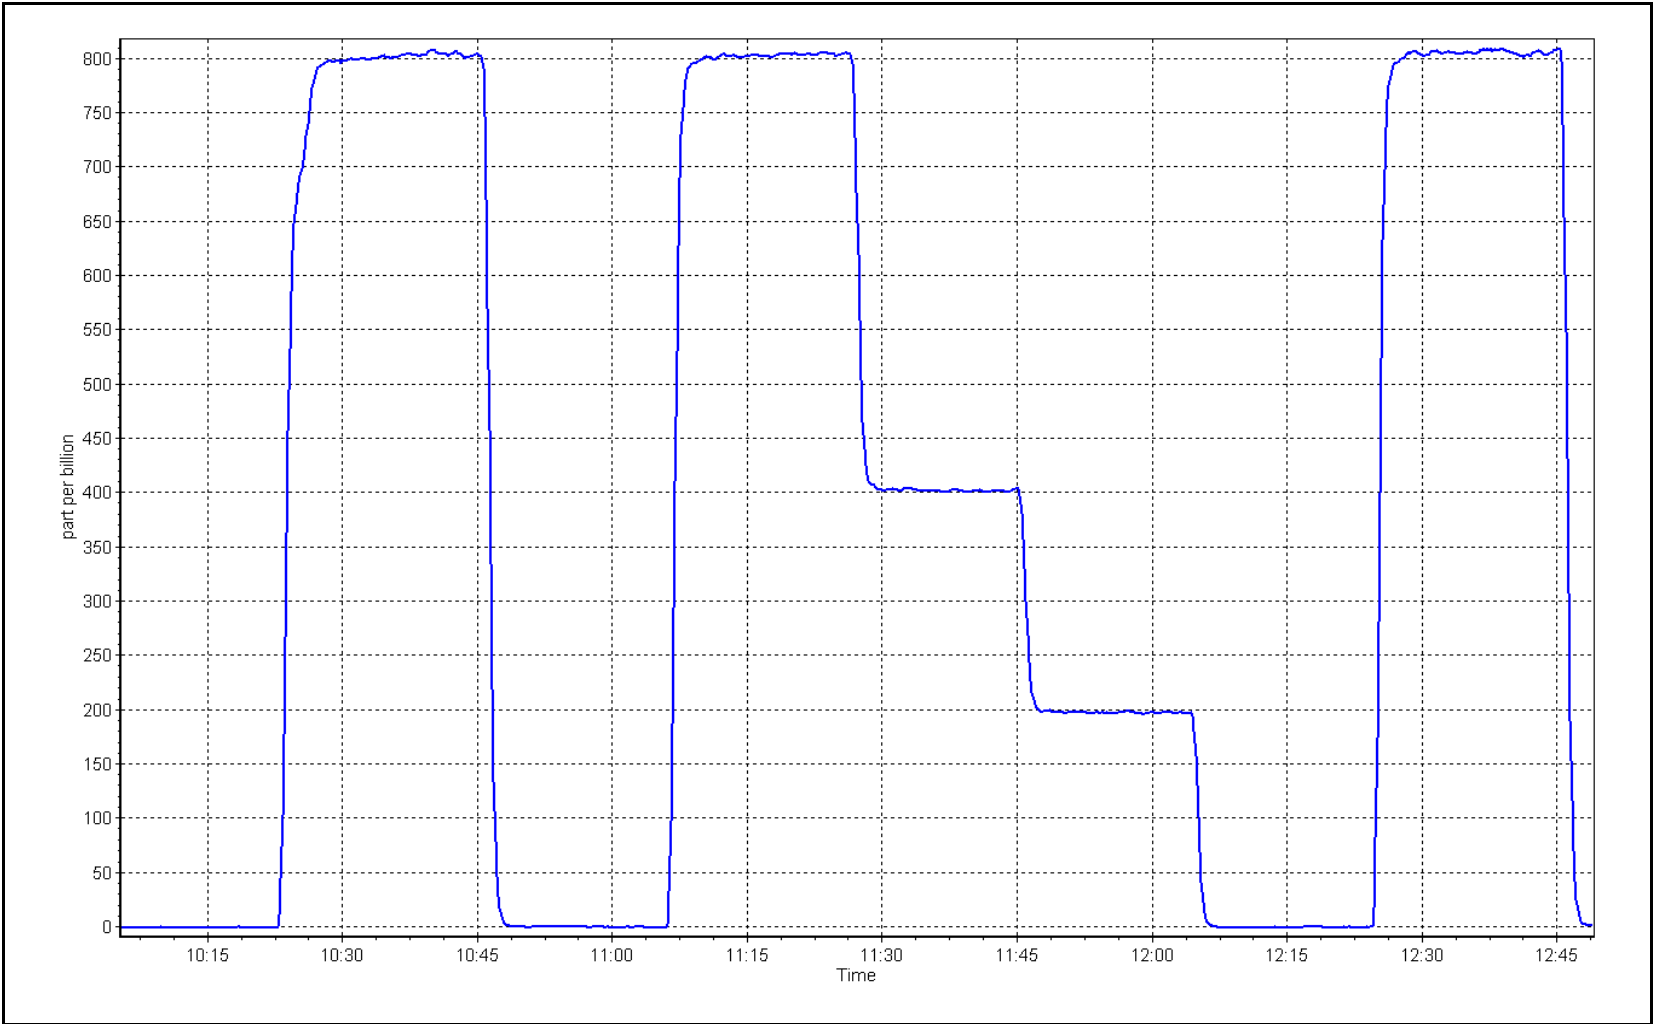



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Jackfish 1 Station number: AMS506
 Calibration Date: January 4, 2023 Last Cal Date: December 20, 2022
 Start time (MST): 11:55 End time (MST): 16:48
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.14 ppm Cal Gas Exp Date: September 16, 2024
 Cal Gas Cylinder #: CC511843
 Removed Cal Gas Conc: 5.14 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 2659
 ZAG Make/Model: API 701 Serial Number: 4427

Analyzer Information

Analyzer make: Thermo 43iQTL Analyzer serial #: 12124313139
 Converter make: Global G150 Converter serial #: 2022-200
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	1.005293	0.999436	Backgd or Offset:	1.08 1.04
Calibration intercept:	-0.338428	-0.058588	Coeff or Slope:	0.774 0.736

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4922	77.8	80.0	77.0	1.040
as found 2nd point	4961	38.9	40.0	37.3	1.075
as found 3rd point	4981	19.4	19.9	17.5	1.146
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.3	----
high point	4922	77.8	80.0	80.0	1.000
second point	4961	38.9	40.0	39.9	1.002
third point	4981	19.4	19.9	19.4	1.028
as left zero	5000	0.0	0.0	0.6	----
as left span	4922	77.8	80.0	79.6	1.005
SO2 Scrubber Check	4921	79.2	792.0	0.1	----

Date of last scrubber change:		Ave Corr Factor	1.010
Date of last converter efficiency test:	December 1, 2022	efficiency	

Baseline Corr As found: 76.9 Prev response: 80.07 *% change: -4.1%
 Baseline Corr 2nd AF pt: 37.2 AF Slope: 0.967301 AF Intercept: -0.859535
 Baseline Corr 3rd AF pt: 17.4 AF Correlation: 0.999297

** = > +/-5% change initiates investigation*

Notes: Arrived to station to investigate low spans, (12.5% low). Hydrator almost empty, inlet filter changed and hydrator filled after third As Found, scrubber check after calibrator zero. Span adjusted

Calibration Performed By: Ryan Power



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 4, 2023	Previous Calibration:	December 20, 2022
Station Name:	Jackfish 1	Station Number:	AMS506
Start Time (MST):	11:55	End Time (MST):	16:48
Analyzer make:	Thermo 43iQTL	Analyzer serial #:	12124313139

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	0.999895	≥0.995
80.0	80.0	0.9998			
40.0	39.9	1.0023	Slope	0.999436	0.90 - 1.10
19.9	19.4	1.0279			
			Intercept	-0.058588	+/-3

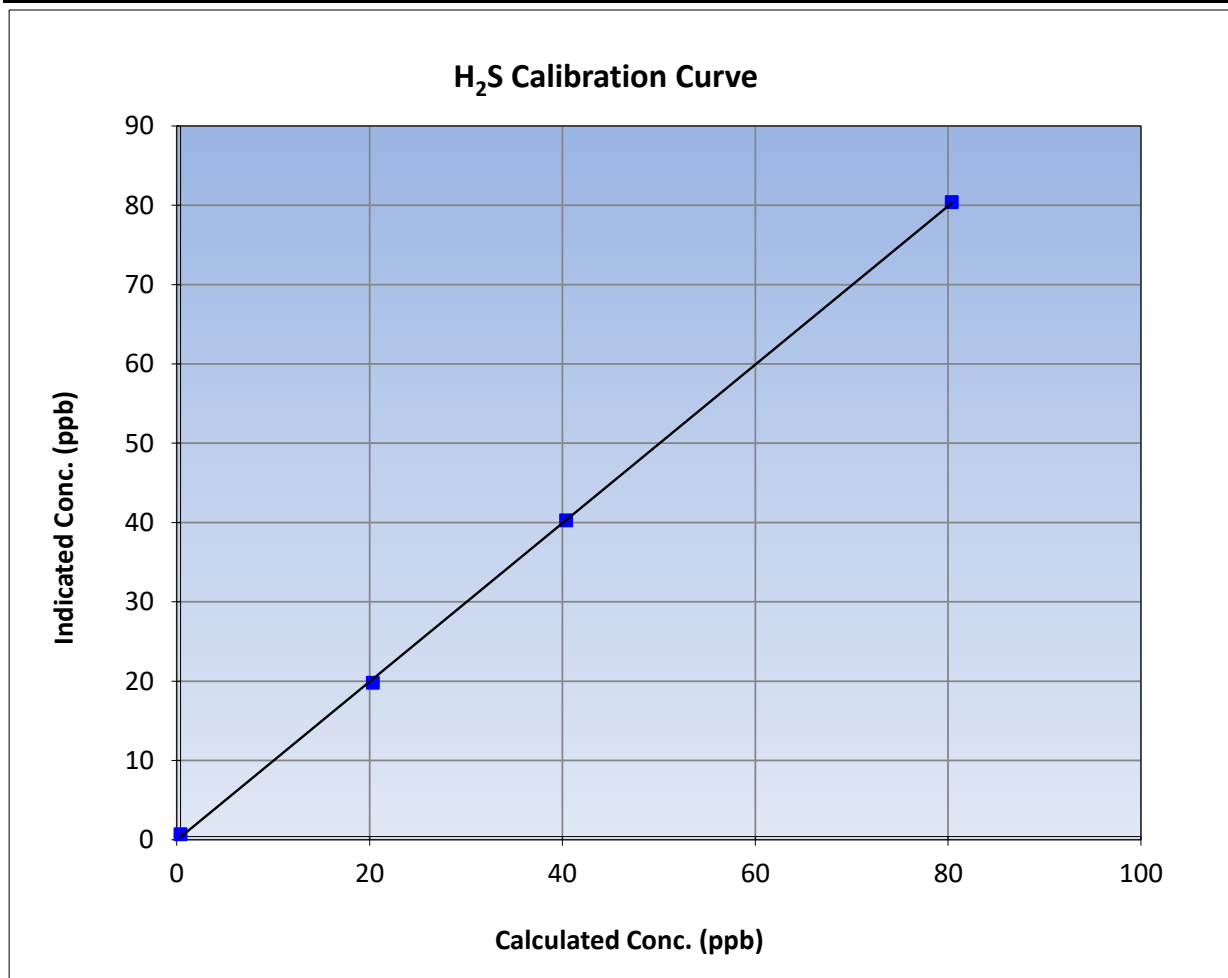

H₂S Calibration Plot

Date: January 4, 2023

Location: Jackfish 1

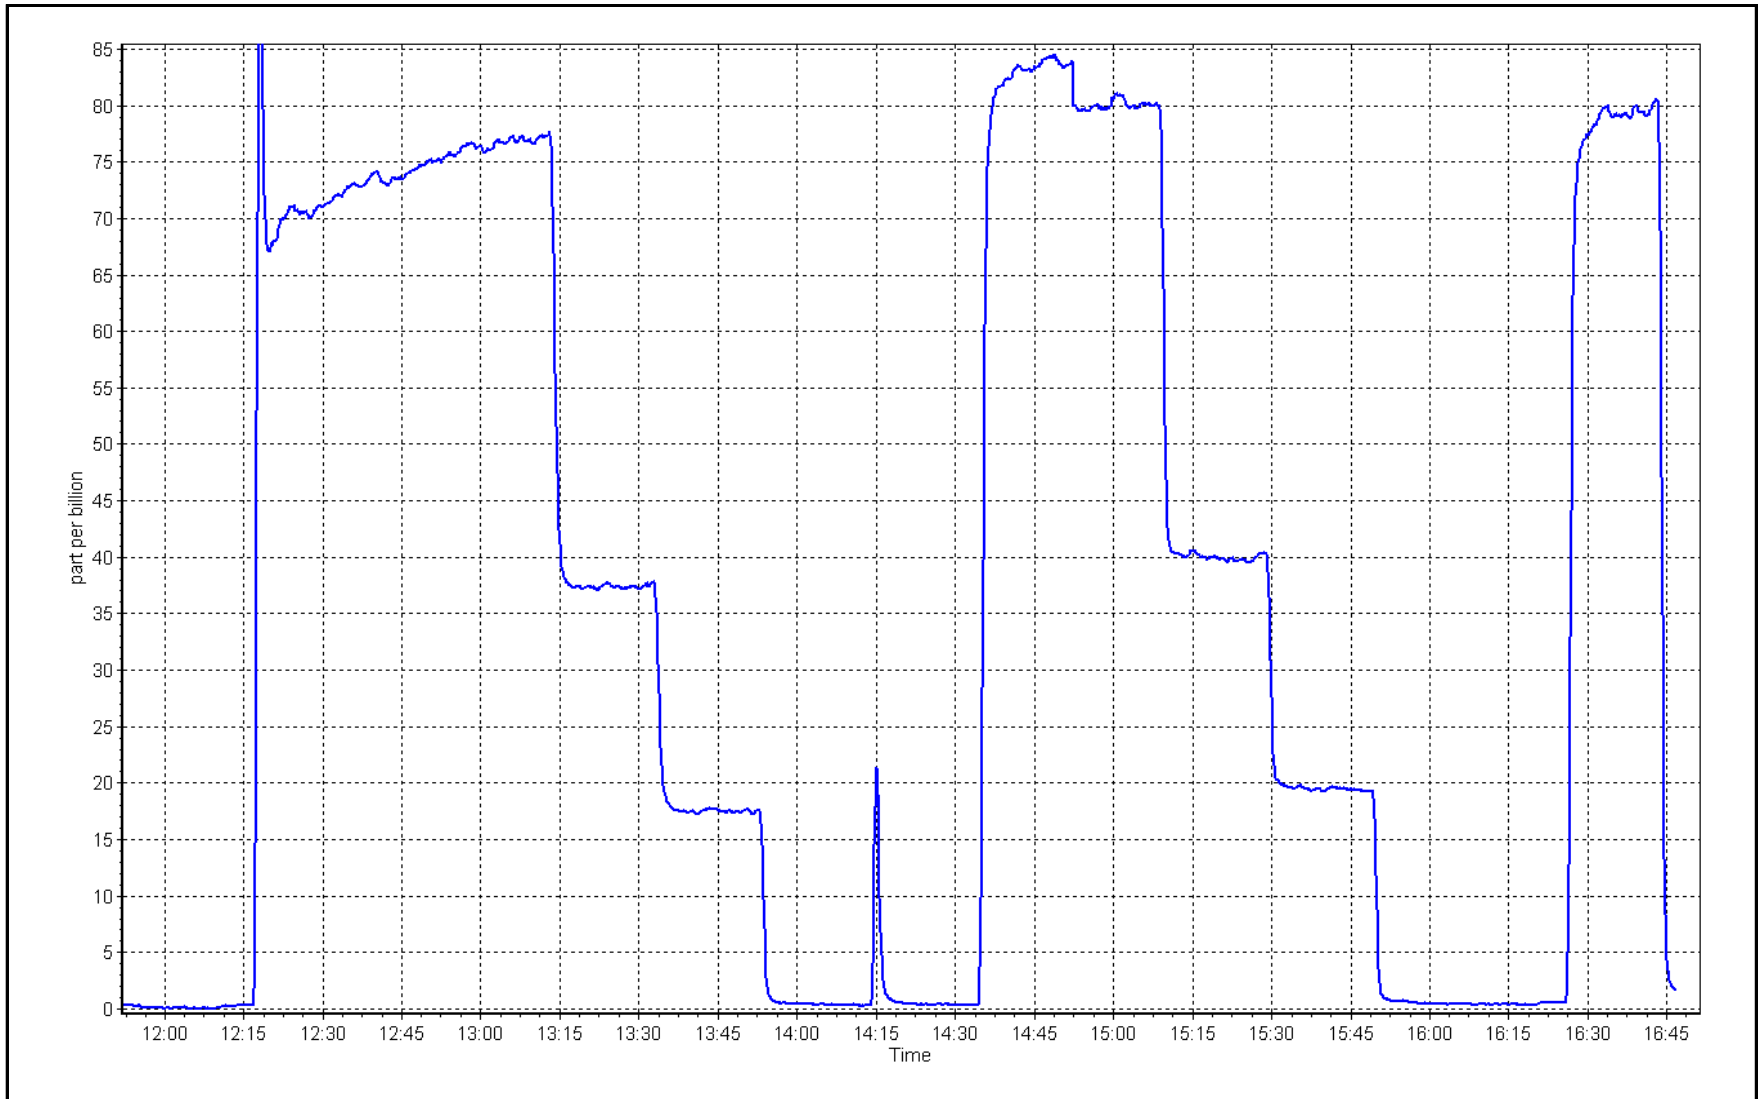



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Jackfish 1 Station number: AMS506
 Calibration Date: January 20, 2023 Last Cal Date: January 4, 2023
 Start time (MST): 9:52 End time (MST): 13:56
 Reason: Maintenance H2S low spans.

Calibration Standards

Cal Gas Concentration: 5.14 ppm Cal Gas Exp Date: September 16, 2024
 Cal Gas Cylinder #: CC511843
 Removed Cal Gas Conc: 5.14 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 2659
 ZAG Make/Model: API 701 Serial Number: 4427

Analyzer Information

Analyzer make: Thermo 43iQTL Analyzer serial #: 12124313139
 Converter make: Global G150 Converter serial #: 2022-200
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>	<u>Start</u>	<u>Finish</u>
Calibration slope:	0.999436	1.008437	Backgd or Offset: 1.04	1.04
Calibration intercept:	-0.058588	-0.098415	Coeff or Slope: 0.736	0.736

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	0.1	----
as found span	4922	77.8	80.0	72.7	1.102
as found 2nd point	4961	38.9	40.0	35.8	1.120
as found 3rd point	4981	19.4	19.9	17.1	1.173
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	0.3	----
high point	4922	77.8	80.0	80.7	0.991
second point	4961	38.9	40.0	40.2	0.995
third point	4981	19.4	19.9	19.5	1.023
as left zero	5000	0.0	0.0	0.5	----
as left span	4922	77.8	80.0	81.1	0.986
SO2 Scrubber Check	4921	79.2	792.0	0.0	----
Date of last scrubber change:				Ave Corr Factor	1.003
Date of last converter efficiency test:		December 1, 2022		efficiency	

Baseline Corr As found: 72.6 Prev response: 79.88 *% change: -10.0%
 Baseline Corr 2nd AF pt: 35.7 AF Slope: 0.911582 AF Intercept: -0.460573
 Baseline Corr 3rd AF pt: 17.0 AF Correlation: 0.999726

* = > +/-5% change initiates investigation

Notes: Hydrator is quarter to empty, inlet filter changed and hydrator filled after third As Found, scrubber check after calibrator zero. No adjustment made.

Calibration Performed By: Sean Bala



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 20, 2023	Previous Calibration:	January 4, 2023
Station Name:	Jackfish 1	Station Number:	AMS506
Start Time (MST):	9:52	End Time (MST):	13:56
Analyzer make:	Thermo 43iQTL	Analyzer serial #:	12124313139

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits	
0.0	0.3	----	Correlation Coefficient	0.999876	≥0.995
80.0	80.7	0.9911			
40.0	40.2	0.9948	Slope	1.008437	0.90 - 1.10
19.9	19.5	1.0226			
			Intercept	-0.098415	+/-3

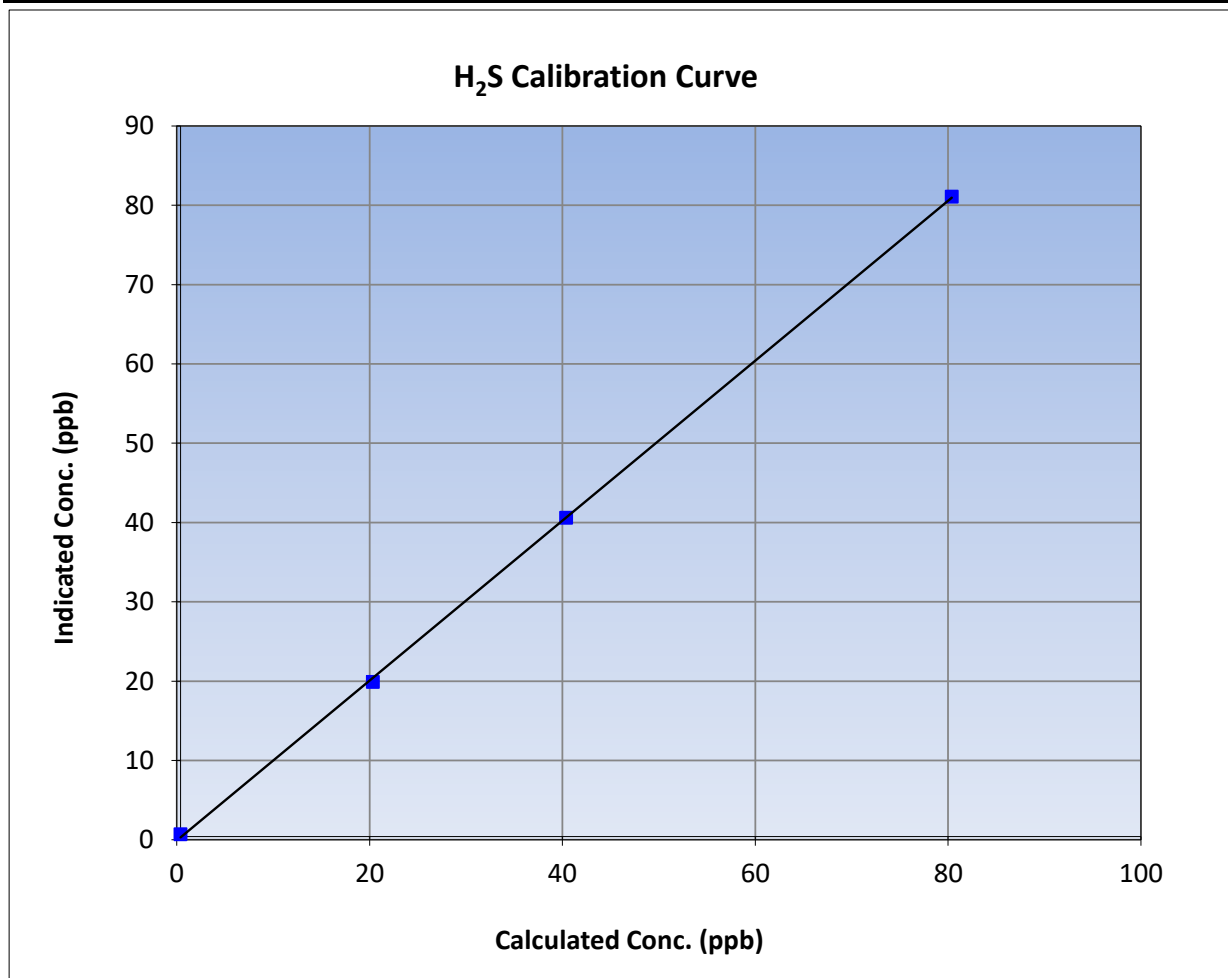

H₂S Calibration Plot

Date: January 20, 2023

Location: Jackfish 1

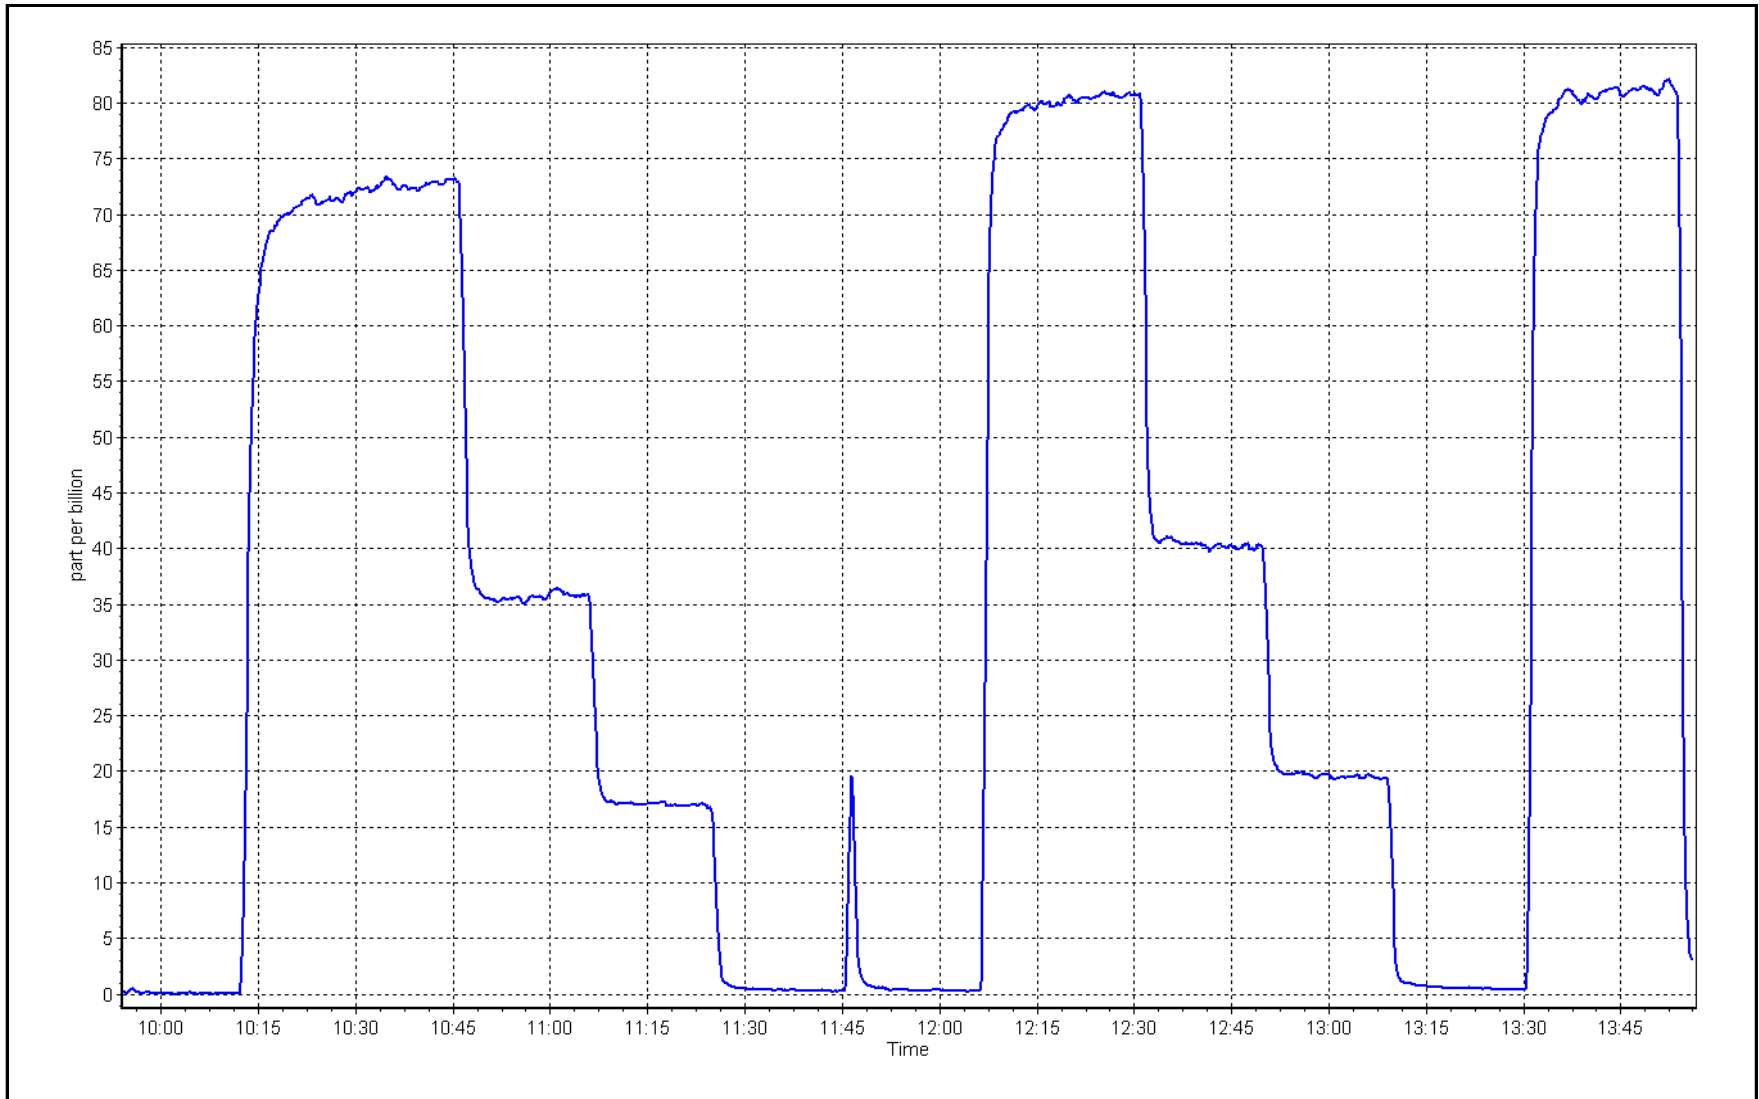



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.1	0.1	0.0	----	----
as found span	4916	84.4	801.1	799.9	1.2	799.4	796.5	3.0	1.0021	1.0042
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.3	0.2	0.1	----	----
high point	4916	84.4	801.1	799.9	1.2	800.0	799.5	0.6	1.0013	1.0005
second point	4958	42.2	400.5	400.0	0.6	400.3	398.6	1.6	1.0006	1.0034
third point	4979	21.1	200.3	200.0	0.3	197.3	195.1	2.3	1.0151	1.0250
as left zero	5000	0.0	0.0	0.0	0.0	0.3	0.3	0.0	----	----
as left span	4916	84.4	801.1	416.2	384.9	795.9	411.4	384.4	1.0065	1.0116
Average Correction Factor									1.0057	1.0096

Corrected As found	NO _x = 799.3 ppb	NO = 796.4 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -0.2%
Previous Response	NO _x = 801.0 ppb	NO = 800.8 ppb		*Percent Change	NO = -0.5%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	794.2	410.5	384.9	385.2	0.9992	100.1%
2nd GPT point (200 ppb O3)	794.2	588.8	206.6	206.6	0.9999	100.0%
3rd GPT point (100 ppb O3)	794.2	686.7	108.7	108.7	0.9998	100.0%
Average Correction Factor					0.9996	100.0%

Notes:

Adjusted the span only.

Calibration Performed By:

Sean Bala



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 25, 2023	Previous Calibration:	December 15, 2022
Station Name:	Jackfish 1	Station Number:	AMS506
Start Time (MST):	9:51	End Time (MST):	14:18
Analyzer make:	Thermo 42i	Analyzer serial #:	1218153356

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.3	----	Correlation Coefficient	≥0.995	
801.1	800.0	1.0013			
400.5	400.3	1.0006			
200.3	197.3	1.0151			
			Slope	0.999577	0.90 - 1.10
			Intercept	-0.847995	+/-20

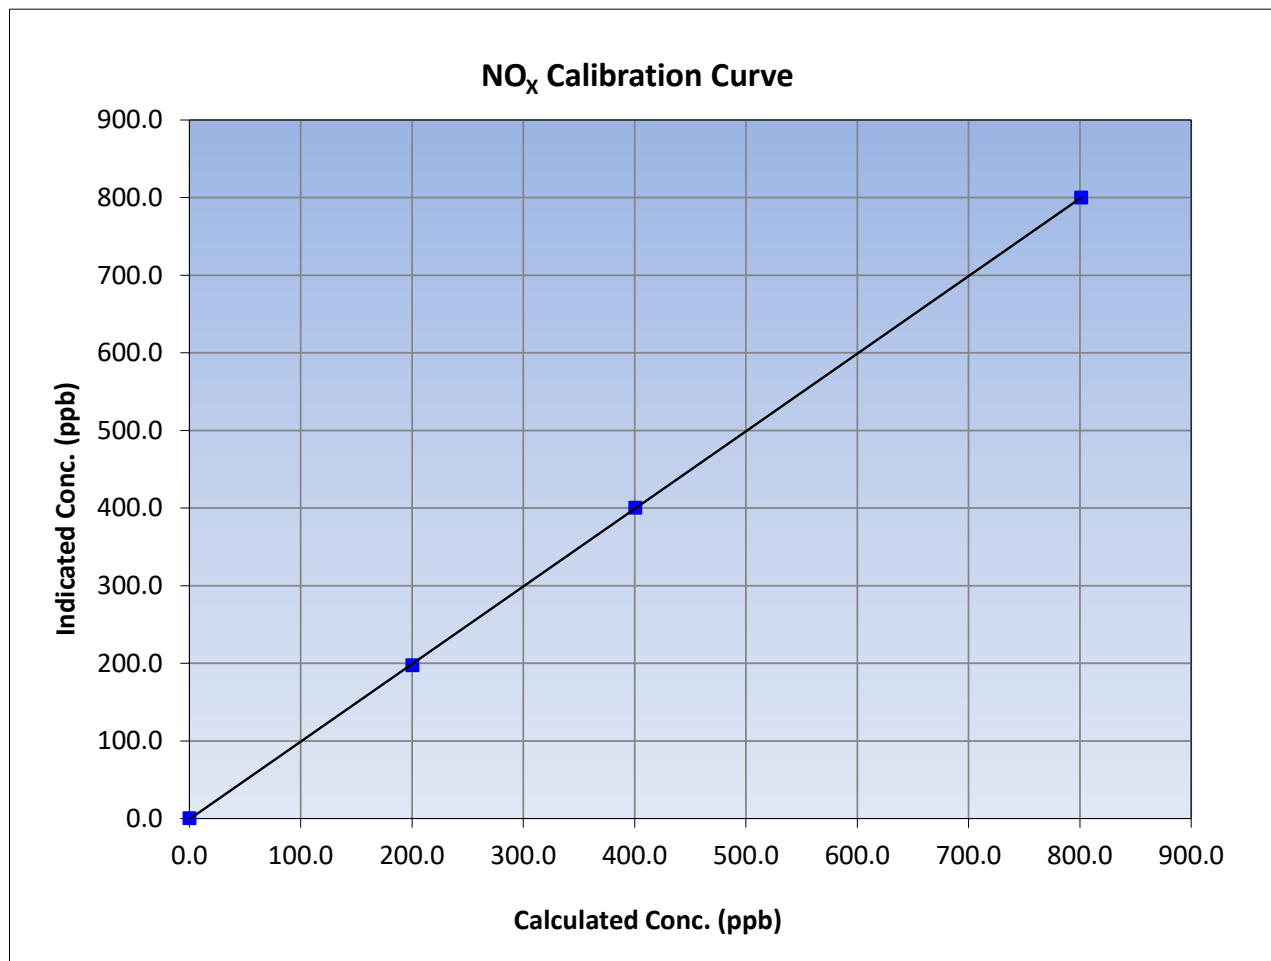



Wood Buffalo Environmental Association

NO Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 25, 2023	Previous Calibration:	December 15, 2022
Station Name:	Jackfish 1	Station Number:	AMS506
Start Time (MST):	9:51	End Time (MST):	14:18
Analyzer make:	Thermo 42i	Analyzer serial #:	1218153356

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	0.2	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
799.9	799.5	1.0005		
400.0	398.6	1.0034		
200.0	195.1	1.0250		

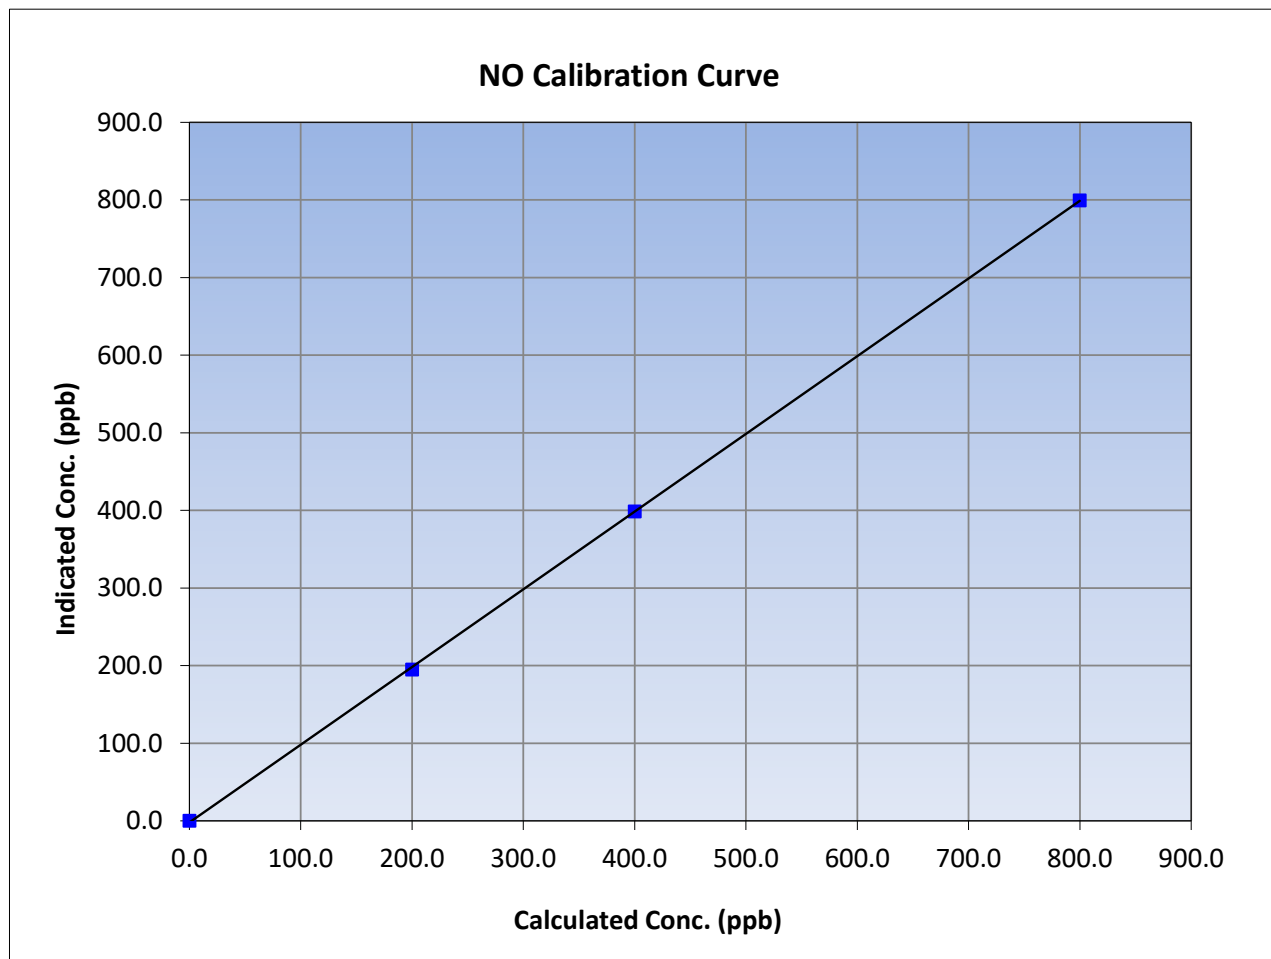



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 25, 2023	Previous Calibration:	December 15, 2022
Station Name:	Jackfish 1	Station Number:	AMS506
Start Time (MST):	9:51	End Time (MST):	14:18
Analyzer make:	Thermo 42i	Analyzer serial #:	1218153356

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.1	----	Correlation Coefficient	≥0.995	
384.9	385.2	0.9992			
206.6	206.6	0.9999			
108.7	108.7	0.9998			
			Slope	1.000608	0.90 - 1.10
			Intercept	0.007440	+/-20


NO₂ Calibration Curve

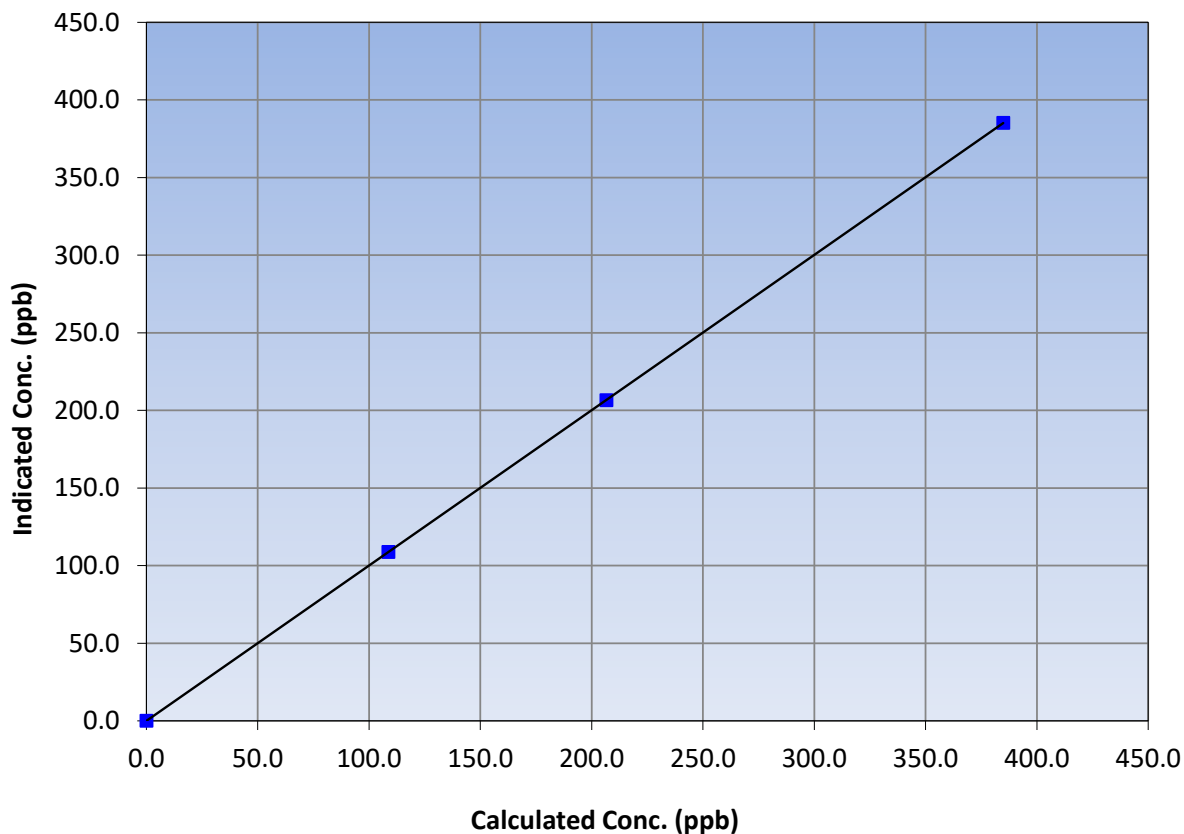

NO_x Calibration Plot

Date: January 25, 2023

Location: Jackfish 1

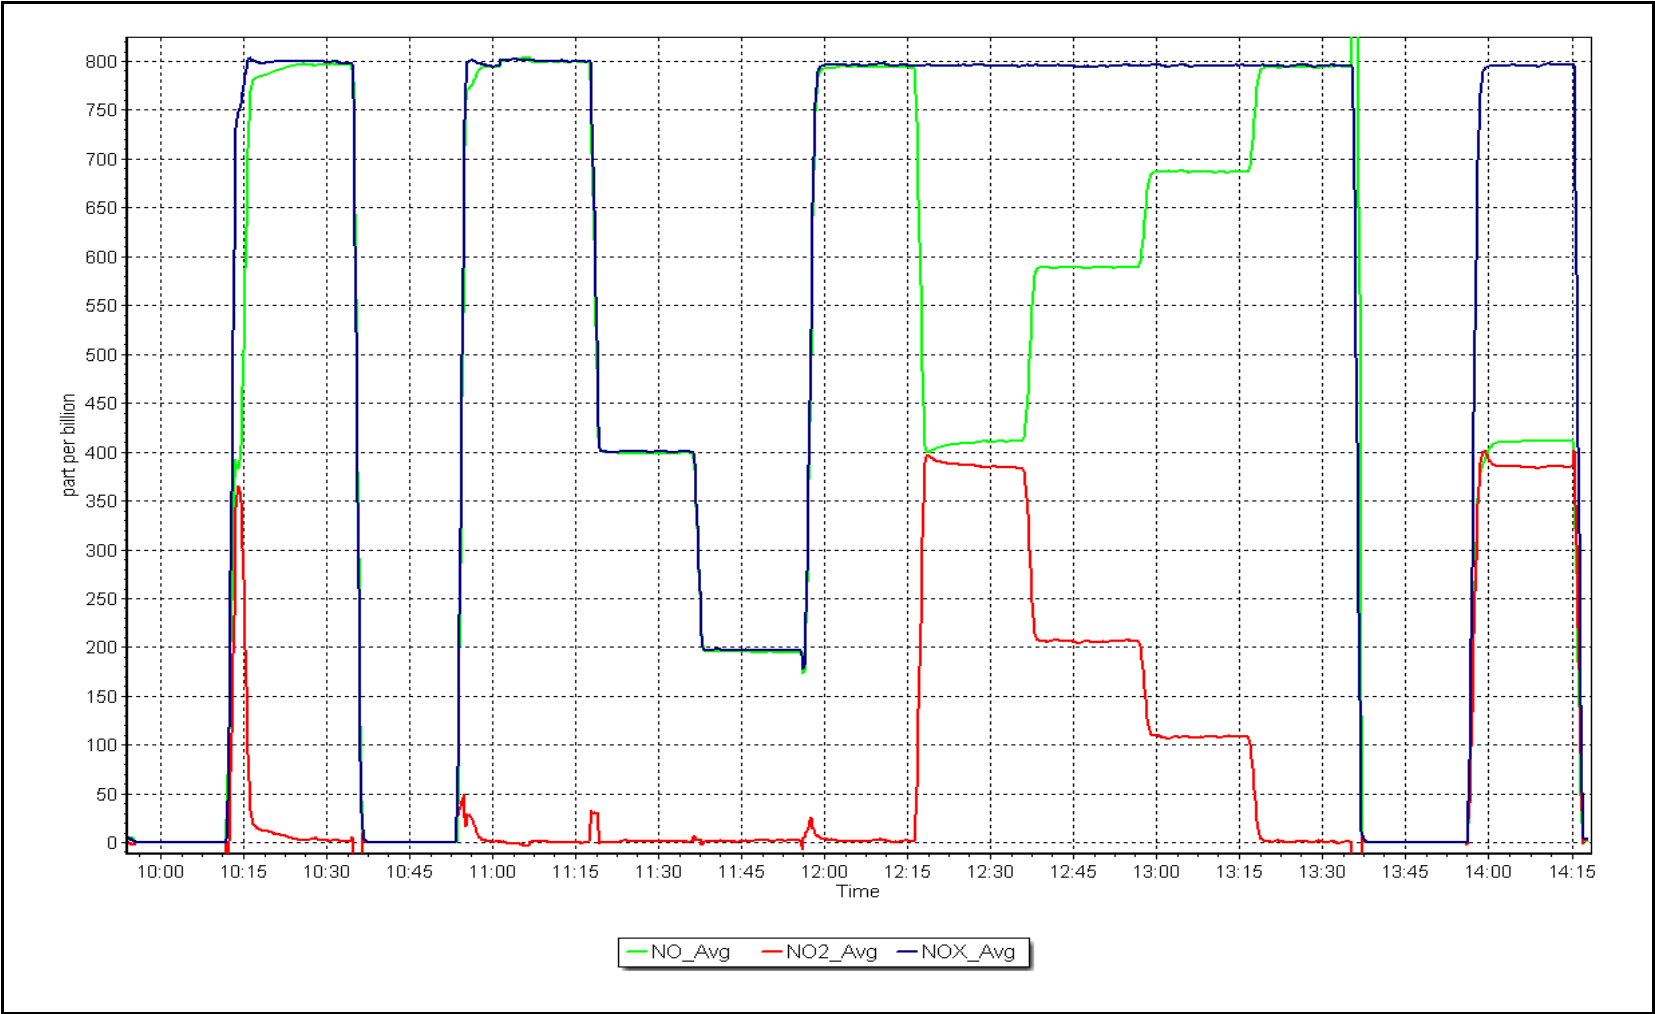



WOOD BUFFALO ENVIRONMENTAL ASSOCIATION

CONTINUOUS AMBIENT AIR QUALITY
MONITORING PROGRAM
CALIBRATION REPORT

AMS508
KIRBY NORTH
JANAURY 2023

Operations, Data Collection,
QA/QC, Data Validation and Reporting by:
Wood Buffalo Environmental Association
Fort McMurray, Alberta

February 28, 2023



Wood Buffalo Environmental Association

SO₂ Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 7, 2022
Station Name:	Kirby North	Station Number:	AMS508
Start Time (MST):	9:07	End Time (MST):	15:03
Analyzer make:	Thermo 43iQ	Analyzer serial #:	1182340007

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<i>Limits</i>	
0.0	0.3	----	Correlation Coefficient	0.999993	
799.6	801.0	0.9983			≥0.995
400.3	399.3	1.0026	Slope	1.001350	
199.7	199.6	1.0003			0.90 - 1.10
			Intercept	-0.328940	+/-30

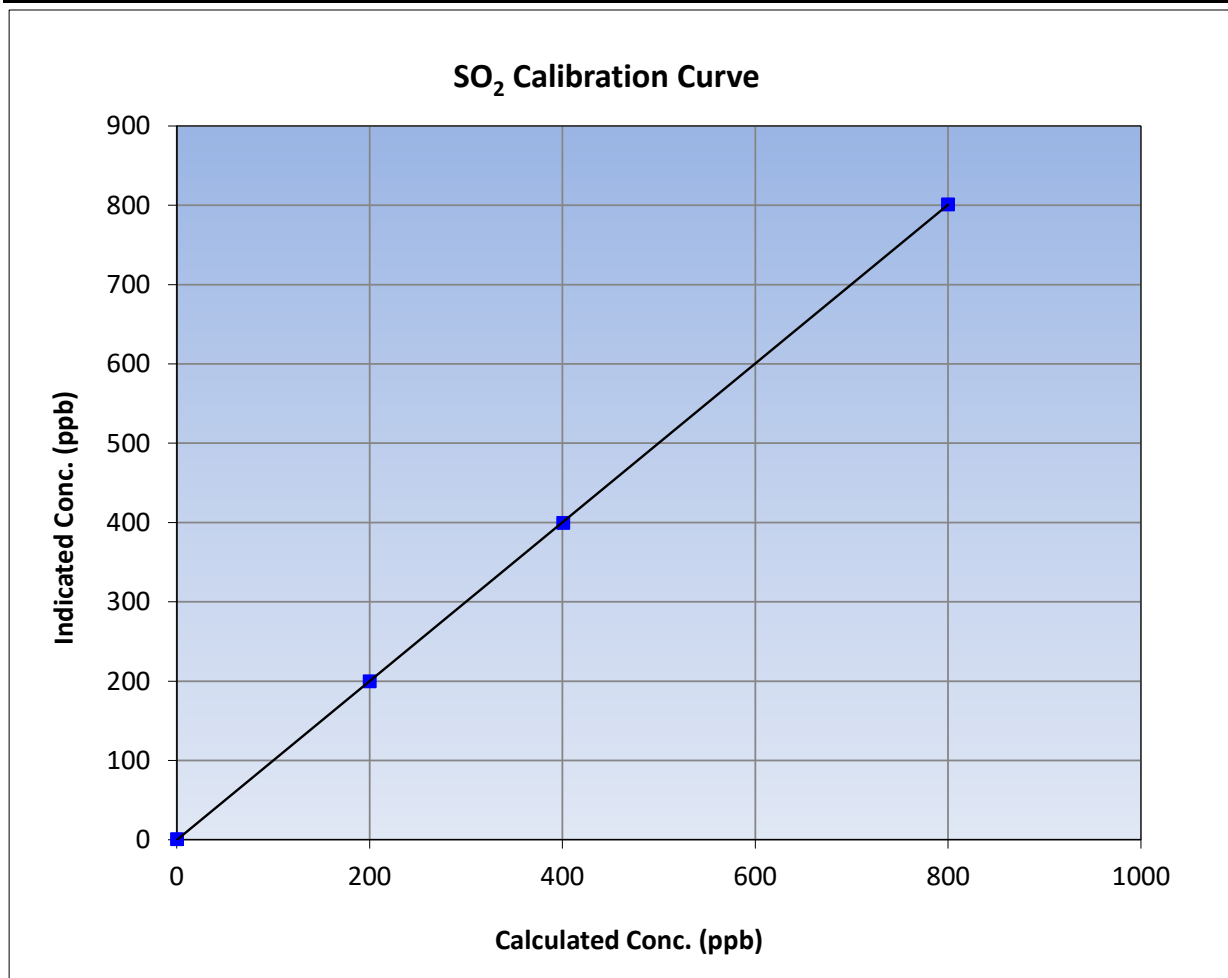

SO2 Calibration Plot

Date: January 11, 2023

Location: Kirby North

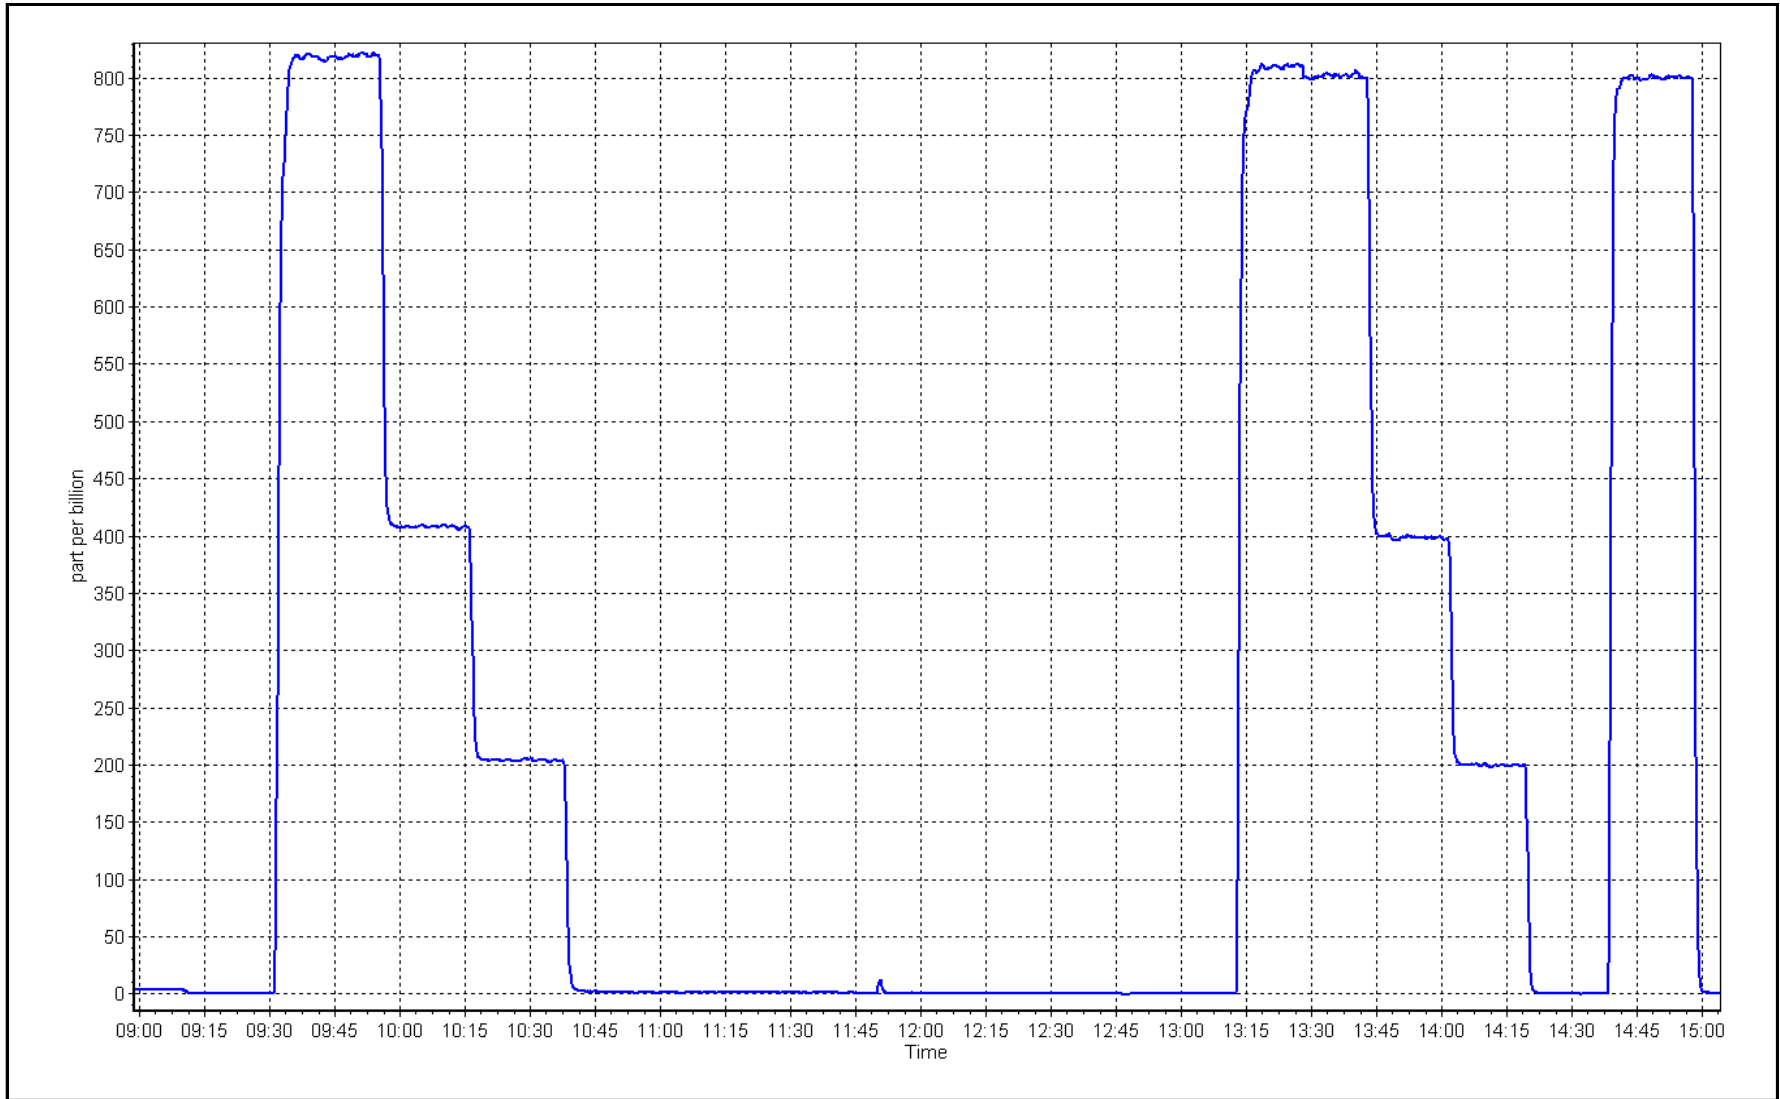



Wood Buffalo Environmental Association

H₂S Calibration Report

Version-11-2021

Station Information

Station Name: Kirby North Station number: AMS508
 Calibration Date: January 12, 2023 Last Cal Date: December 8, 2022
 Start time (MST): 8:05 End time (MST): 12:36
 Reason: Routine

Calibration Standards

Cal Gas Concentration: 5.167 ppm Cal Gas Exp Date: February 5, 2024
 Cal Gas Cylinder #: CC517378
 Removed Cal Gas Conc: 5.167 ppm Rem Gas Exp Date: NA
 Removed Gas Cyl #: NA Diff between cyl:
 Calibrator Make/Model: API T700 Serial Number: 3804
 ZAG Make/Model: API 701H Serial Number: 880

Analyzer Information

Analyzer make: Thermo 43i TLE Analyzer serial #: 1150840012
 Converter make: Global Converter serial #: 2022-197
 Analyzer Range: 0 - 100 ppb

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	1.000172	1.007171	Backgd or Offset:	1.78	1.76
Calibration intercept:	-0.160960	-0.280963	Coeff or Slope:	1.058	1.058

H₂S As Found Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Baseline Adjusted Correction factor (Cc/(Ic-AFzero)) <i>Limit = 0.90-1.10</i>
as found zero	5000	0.0	0.0	-0.2	----
as found span	4923	77.4	80.0	82.3	0.969
as found 2nd point	4961	38.8	40.1	40.8	0.978
as found 3rd point	4981	19.3	19.9	20.1	0.982
new cylinder response					

H₂S Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
calibrator zero	5000	0.0	0.0	-0.1	----
high point	4923	77.4	80.0	80.4	0.995
second point	4961	38.8	40.1	39.9	1.005
third point	4981	19.3	19.9	19.7	1.012
as left zero	5000	0.0	0.0	0.1	----
as left span	4923	77.4	80.0	80.3	0.996
SO2 Scrubber Check	4920	79.8	798.0	0.0	----
Date of last scrubber change:	27-Nov-19			Ave Corr Factor	1.004
Date of last converter efficiency test:					efficiency

Baseline Corr As found: 82.5 Prev response: 79.83 *% change: 3.2%
 Baseline Corr 2nd AF pt: 41.0 AF Slope: 1.032169 AF Intercept: -0.380988
 Baseline Corr 3rd AF pt: 20.3 AF Correlation: 0.999972

* = > +/-5% change initiates investigation

Notes: Changed sample inlet filter after as founds. First scrubber check failed. After rehydrating using DI water in a hydrator second test passed. No adjustments made.

Calibration Performed By: Braiden Boutillier



Wood Buffalo Environmental Association

H₂S Calibration Summary


Version-11-2021

Station Information

Calibration Date:	January 12, 2023	Previous Calibration:	December 8, 2022
Station Name:	Kirby North	Station Number:	AMS508
Start Time (MST):	8:05	End Time (MST):	12:36
Analyzer make:	Thermo 43i-TLE	Analyzer serial #:	1150840012

Calibration Data


Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	Limits
0.0	-0.1	----	Correlation Coefficient	≥0.995
80.0	80.4	0.9948		
40.1	39.9	1.0050	Slope	0.90 - 1.10
19.9	19.7	1.0124		
			Intercept	+/-3

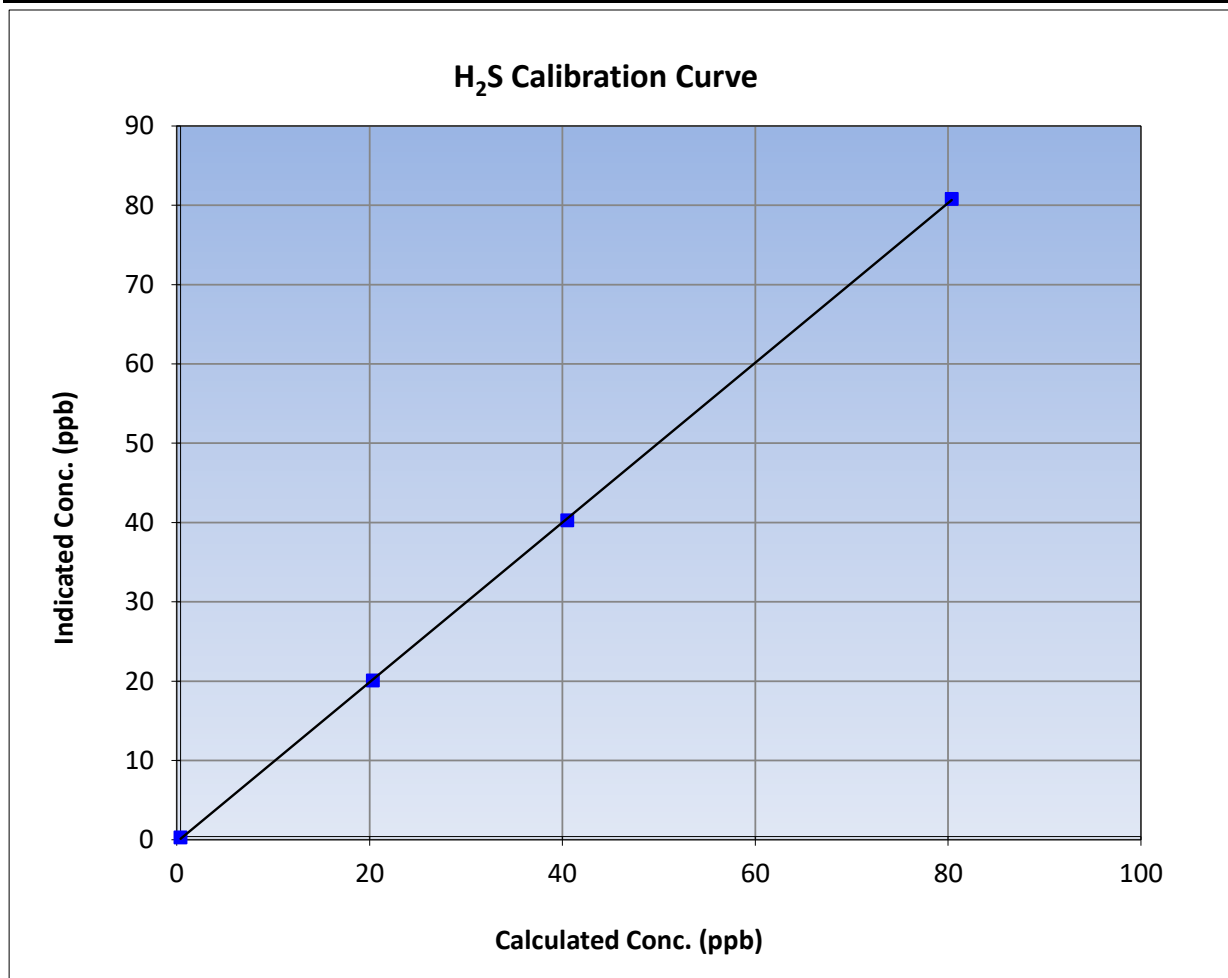

H₂S Calibration Plot

Date: January 12, 2023

Location: Kirby North

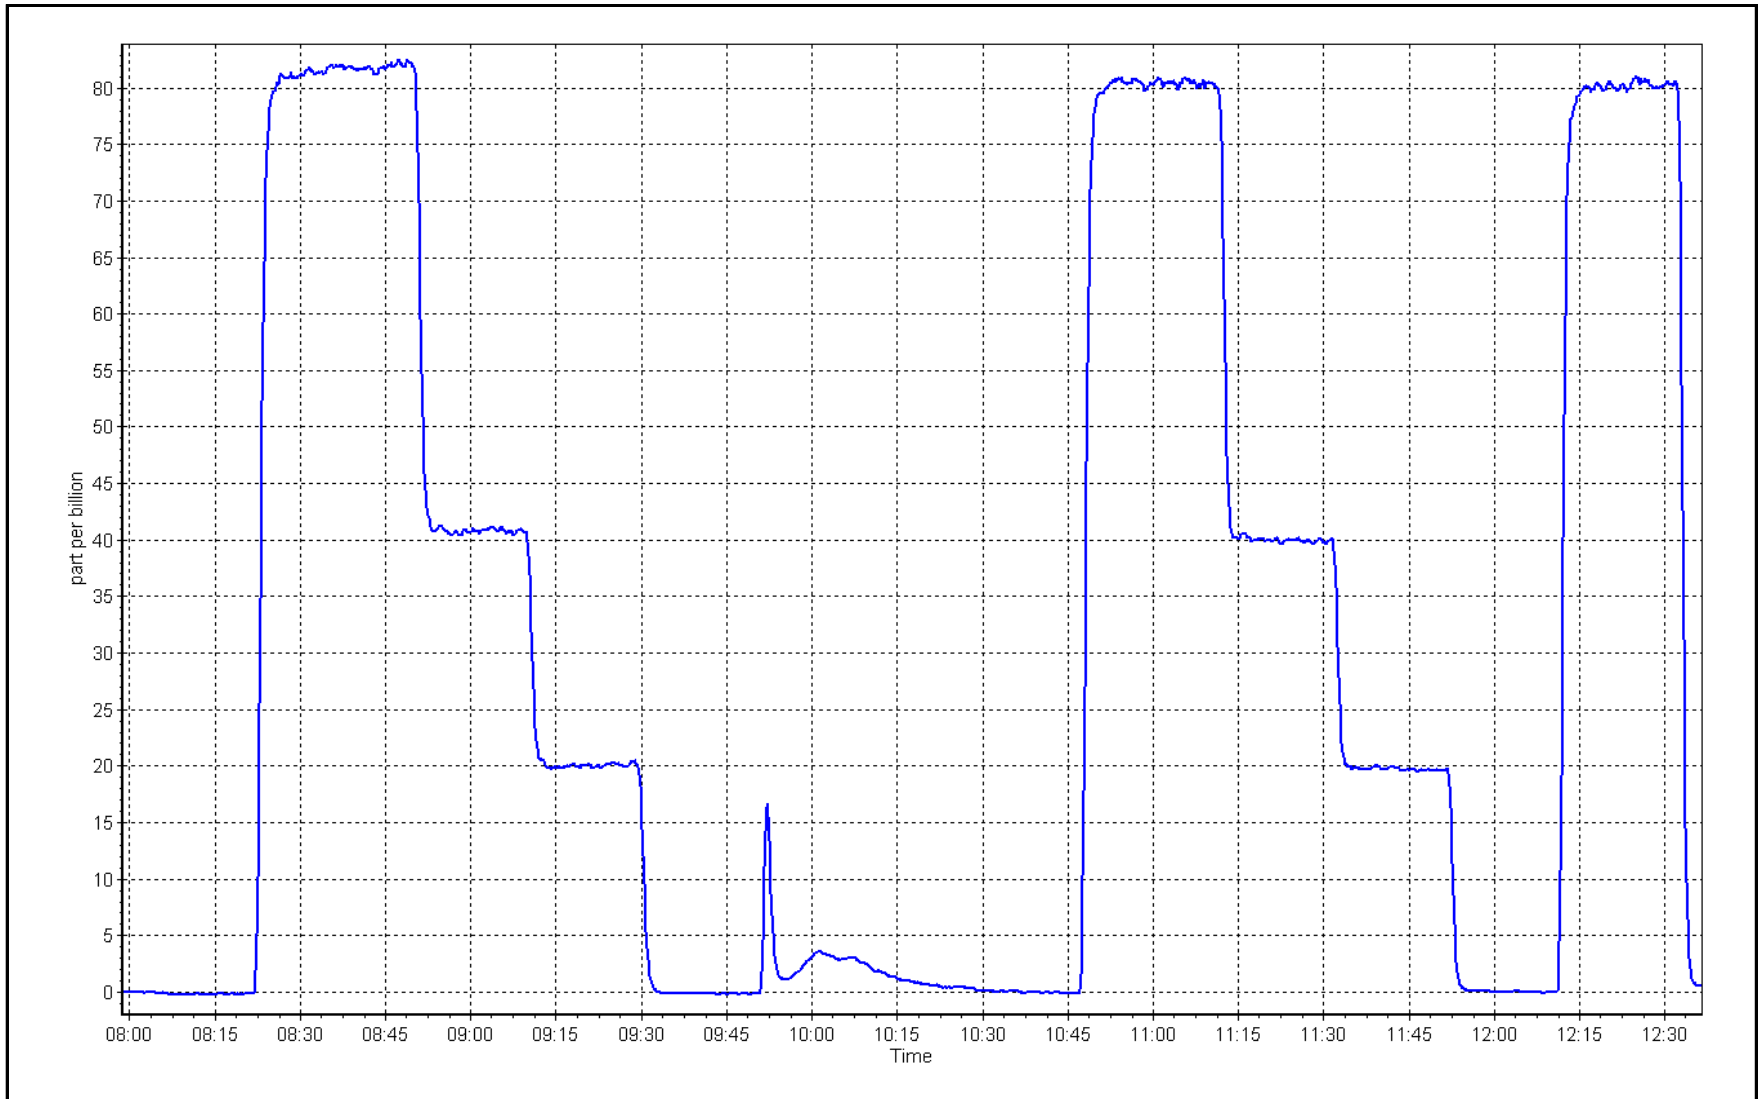



Wood Buffalo Environmental Association

THC Calibration Report

Version-01-2020

Station Information

Station Name:	Kirby North	Station number:	AMS508
Calibration Date:	January 11, 2023	Last Cal Date:	December 7, 2022
Start time (MST):	9:07	End time (MST):	15:03
Reason:	Routine		

Calibration Standards

Gas Cert Reference:	CC303554	Cal Gas Expiry Date:	March 23, 2025
CH4 Cal Gas Conc.	496.6 ppm	CH4 Equiv Conc.	1061.7 ppm
C3H8 Cal Gas Conc.	205.5 ppm		
Removed Gas Cert:	NA	Removed Gas Expiry:	NA
Removed CH4 Conc.	496.6 ppm	CH4 Equiv Conc.	1061.7 ppm
Removed C3H8 Conc.	205.5 ppm	Diff between cyl:	
Calibrator Make/Model:	API T700	Serial Number:	3804
ZAG Make/Model:	API T701H	Serial Number:	880

Analyzer Information

Analyzer make:	Thermo 51i	Analyzer serial #:	1182340005
Analyzer Range:	0 - 20 ppm		

	<u>Start</u>	<u>Finish</u>		<u>Start</u>	<u>Finish</u>
Calibration slope:	0.996667	0.999219	Background:	4.750	2.820
Calibration intercept:	0.016195	-0.026583	Coefficient:	5.494	3.789

THC Calibration Data

Set Point	Dilution air flow rate (sccm)	Source gas flow rate (sccm)	Calculated Concentration (ppm) (Cc)	Indicated Concentration (ppm) (Ic)	Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.00	-0.91	----
as found span	4919	81.3	17.26	16.61	1.039
as found 2nd point	4959	40.7	8.64	7.75	1.116
as found 3rd point	4980	20.3	4.31	3.37	1.279
new cylinder response					
calibrator zero	5000	0.0	0.00	0.01	----
high point	4919	81.3	17.26	17.25	1.001
second point	4959	40.7	8.64	8.56	1.010
third point	4980	20.3	4.31	4.27	1.009
as left zero	5000	0.0	0.00	-0.04	----
as left span	4919	81.3	17.26	17.31	0.997
Average Correction Factor					1.007
Baseline Corr As found:	17.52	Previous response	17.22	*% change	1.7%
Baseline Corr 2nd AF pt:	8.66	AF Slope:	1.016184	AF Intercept:	-0.972986
Baseline Corr 3rd AF pt:	4.28	AF Correlation:	0.999937		

* = > +/-5% change initiates investigation

Notes: Changed sample inlet filter after as founds. Changed internal pump on the 51i after MPAF's. Zero and span adjusted.

Calibration Performed By: Braiden Boutillier



Wood Buffalo Environmental Association

THC Calibration Summary


Version-01-2020

Station Information

Calibration Date:	January 11, 2023	Previous Calibration:	December 7, 2022
Station Name:	Kirby North	Station Number:	AMS508
Start Time (MST):	9:07	End Time (MST):	15:03
Analyzer make:	Thermo 51i	Analyzer serial #:	1182340005

Calibration Data


Calculated Concentration (ppm) (Cc)	Indicated Concentration (ppm) (lc)	Correction factor (Cc/lc)	Statistical Evaluation	<u>Limits</u>	
0.00	0.01	----	Correlation Coefficient	0.999973	
17.26	17.25	1.0007			≥0.995
8.64	8.56	1.0097	Slope	0.999219	
4.31	4.27	1.0094			0.90 - 1.10
			Intercept	-0.026583	+/-1.5

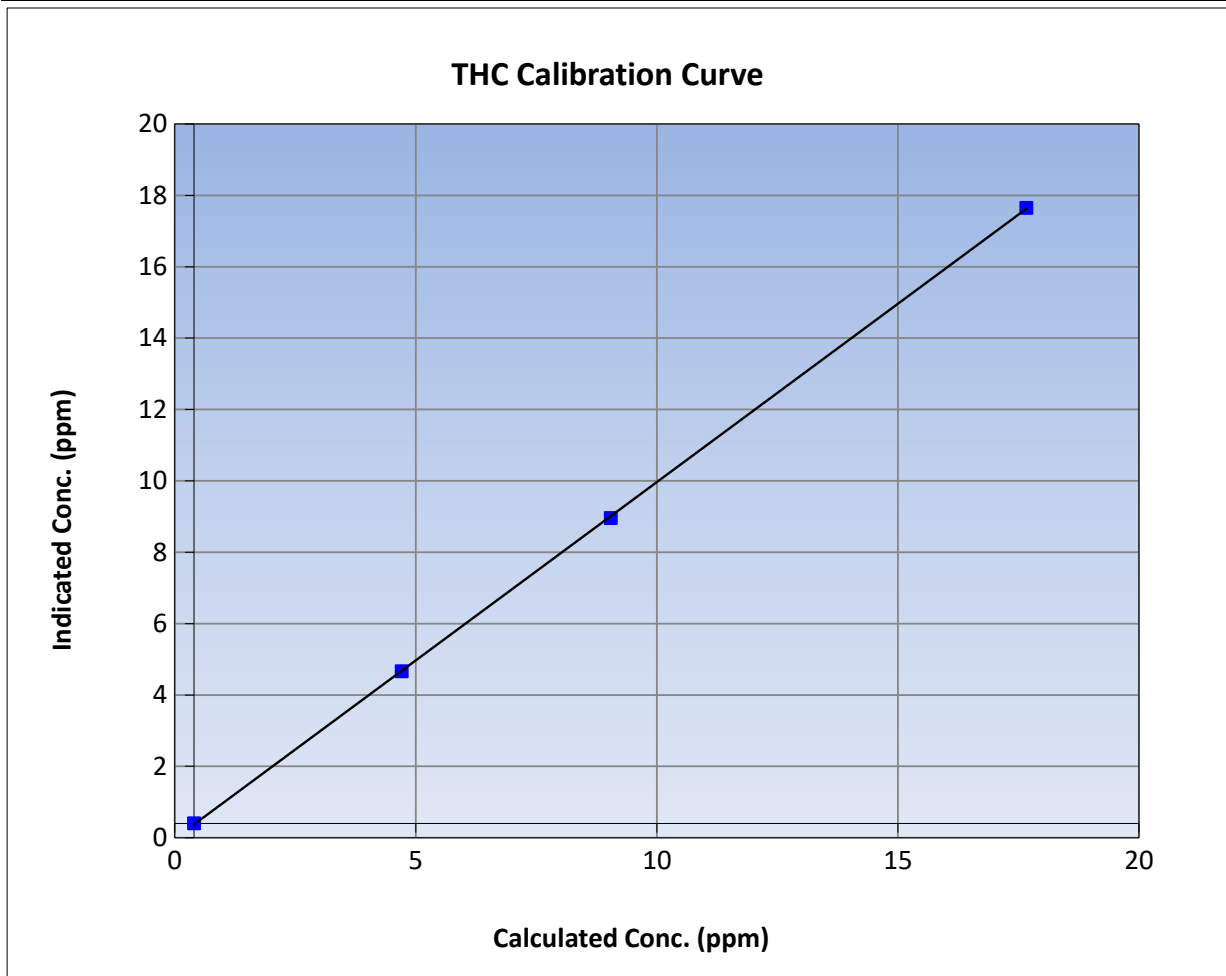

THC Calibration Plot

Date: January 11, 2023

Location: Kirby North

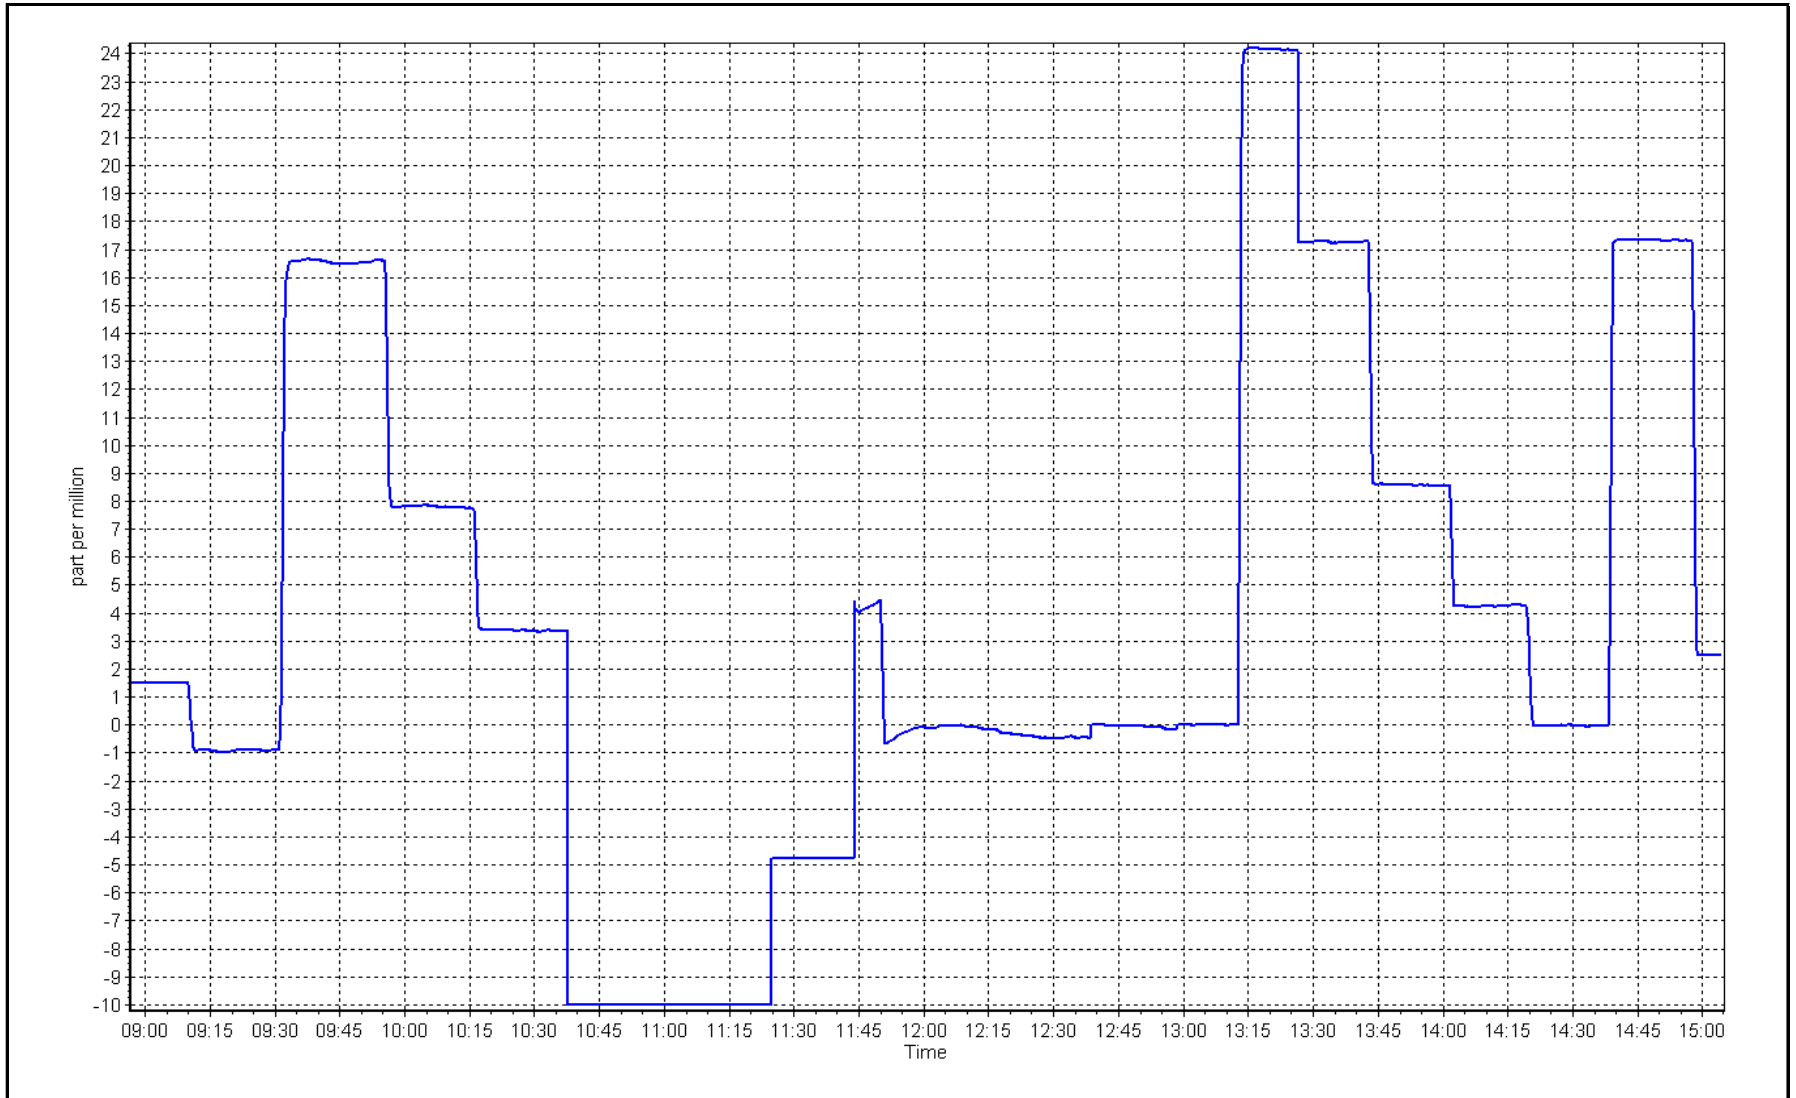



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.1	-0.2	0.3	----	----
as found span	4919	81.0	800.1	794.1	6.0	796.5	788.0	8.5	1.0045	1.0078
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.0	-0.1	0.1	----	----
high point	4919	81.0	800.1	794.1	6.0	799.1	793.7	5.4	1.0013	1.0005
second point	4960	40.5	400.0	397.0	3.0	400.0	394.8	5.2	1.0000	1.0056
third point	4980	20.2	199.5	198.0	1.5	198.2	194.9	3.3	1.0067	1.0161
as left zero	5000	0.0	0.0	0.0	0.0	0.0	-0.2	0.2	----	----
as left span	4919	81.0	800.1	412.3	387.8	794.1	406.8	387.3	1.0076	1.0136
Average Correction Factor									1.0027	1.0074

Corrected As found	NO _x = 796.4 ppb	NO = 788.2 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -0.9%	
Previous Response	NO _x = 804.0 ppb	NO = 797.8 ppb		*Percent Change	NO = -1.2%	
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:	Nx Int:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:	NO Int:
			As found	NO ₂ r ² :	NO ₂ SI:	NO ₂ Int:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO ₂)						
as found GPT point (200 ppb NO ₂)						
as found GPT point (100 ppb NO ₂)						
1st GPT point (400 ppb O ₃)	789.8	408.0	387.8	388.4	0.9984	100.2%
2nd GPT point (200 ppb O ₃)	789.8	593.6	202.2	203.5	0.9936	100.6%
3rd GPT point (100 ppb O ₃)	789.8	696.1	99.7	102.0	0.9774	102.3%
Average Correction Factor					0.9898	101.0%

Notes:

Changed sample inlet filter after as founds. No adjustments made.

Calibration Performed By:

Braiden Boutilier



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 7, 2022
Station Name:	Kirby North	Station Number:	AMS508
Start Time (MST):	11:48	End Time (MST):	17:00
Analyzer make:	API T200	Analyzer serial #:	7029

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.0	----	Correlation Coefficient 0.999997	≥0.995	
800.1	799.1	1.0013			
400.0	400.0	1.0000			
199.5	198.2	1.0067			
			Slope	0.999259	0.90 - 1.10
			Intercept	-0.331803	+/-20

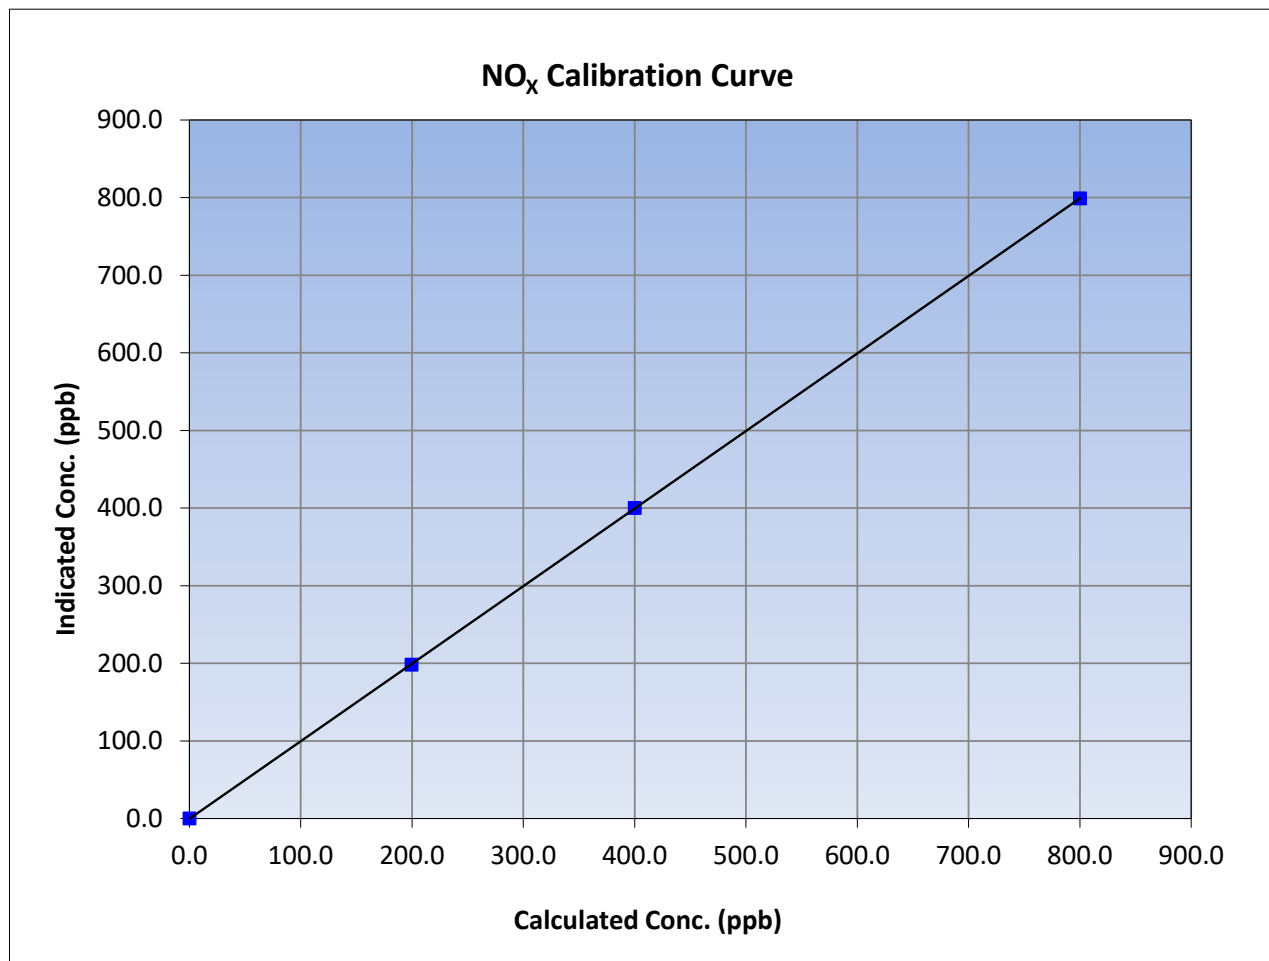



Wood Buffalo Environmental Association

NO Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 7, 2022
Station Name:	Kirby North	Station Number:	AMS508
Start Time (MST):	11:48	End Time (MST):	17:00
Analyzer make:	API T200	Analyzer serial #:	7029

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>
0.0	-0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
794.1	793.7	1.0005		
397.0	394.8	1.0056		
198.0	194.9	1.0161		
			0.999982	
			1.000587	
			-1.673511	

NO Calibration Curve

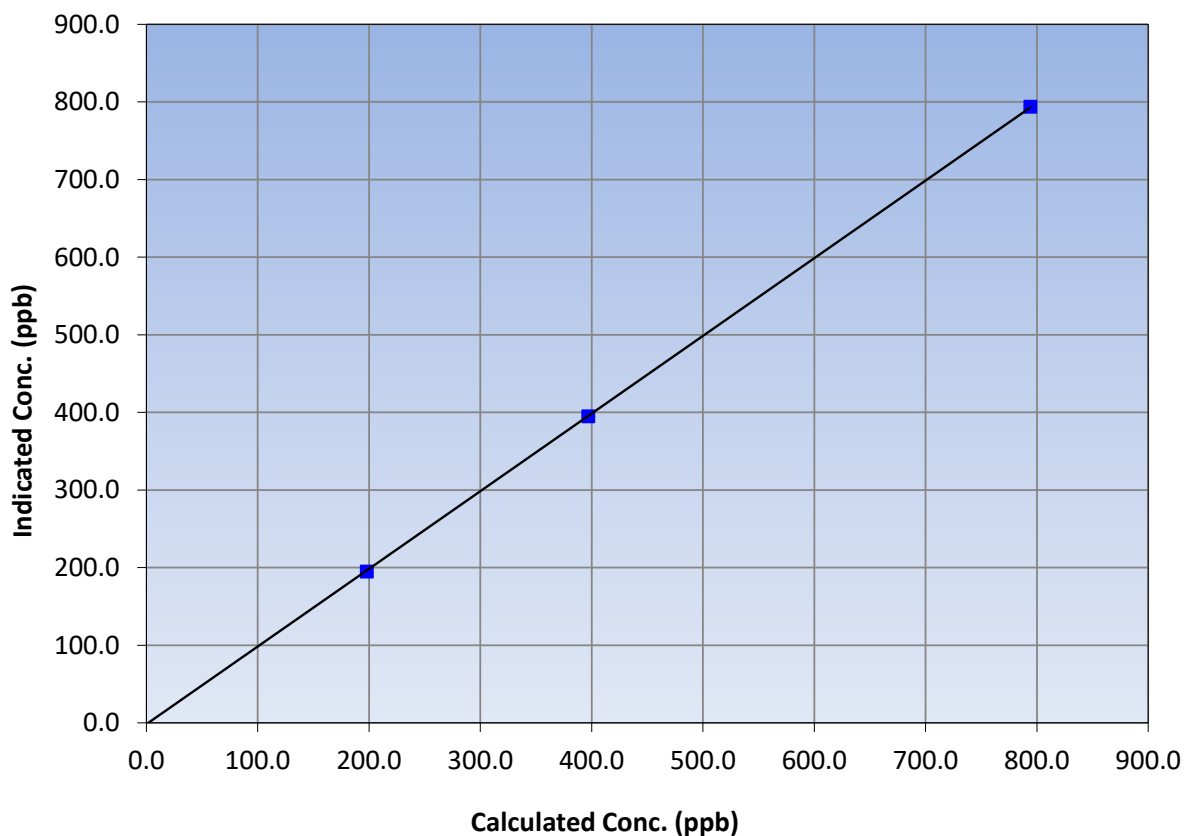



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 10, 2023	Previous Calibration:	December 7, 2022
Station Name:	Kirby North	Station Number:	AMS508
Start Time (MST):	11:48	End Time (MST):	17:00
Analyzer make:	API T200	Analyzer serial #:	7029

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20	
387.8	388.4	0.9984			
202.2	203.5	0.9936			
99.7	102.0	0.9774			
			Correlation Coefficient	0.999967	≥0.995
			Slope	0.999811	0.90 - 1.10
			Intercept	1.112079	+/-20


NO₂ Calibration Curve

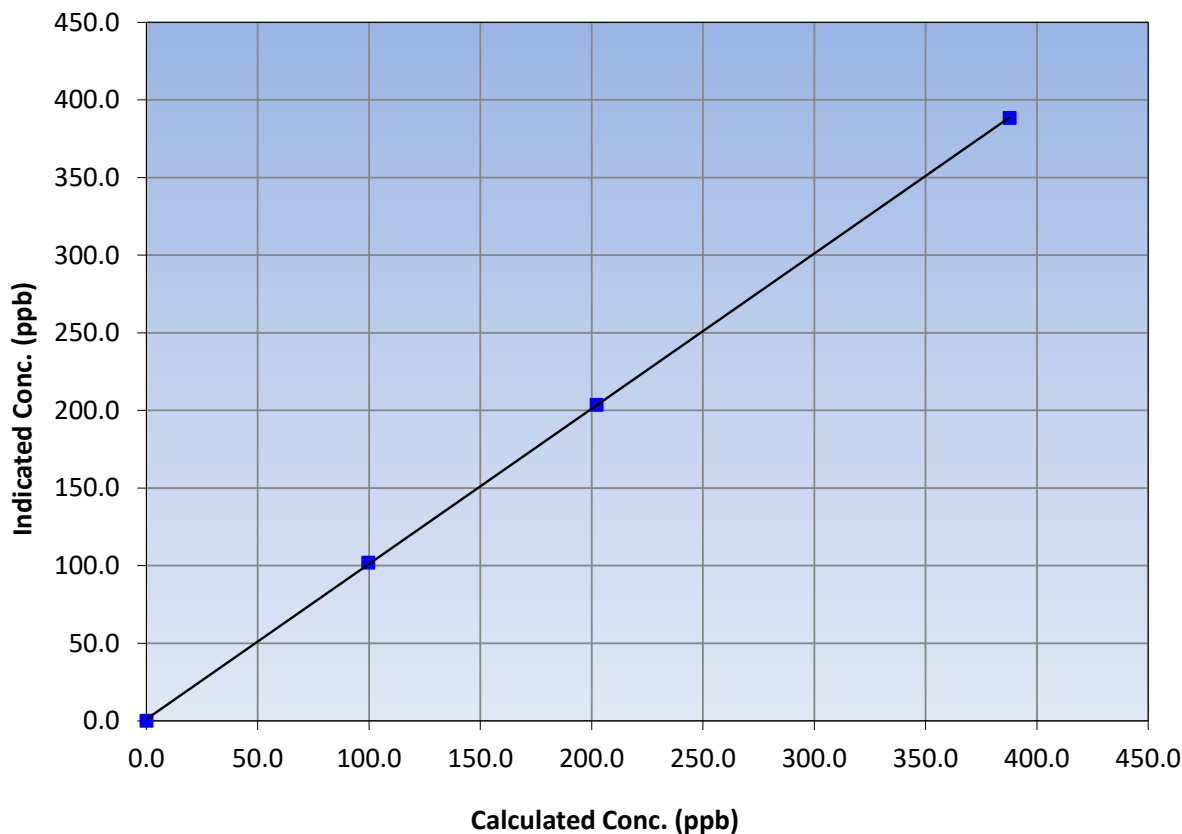

NO_x Calibration Plot

Date: January 10, 2023

Location: Kirby North

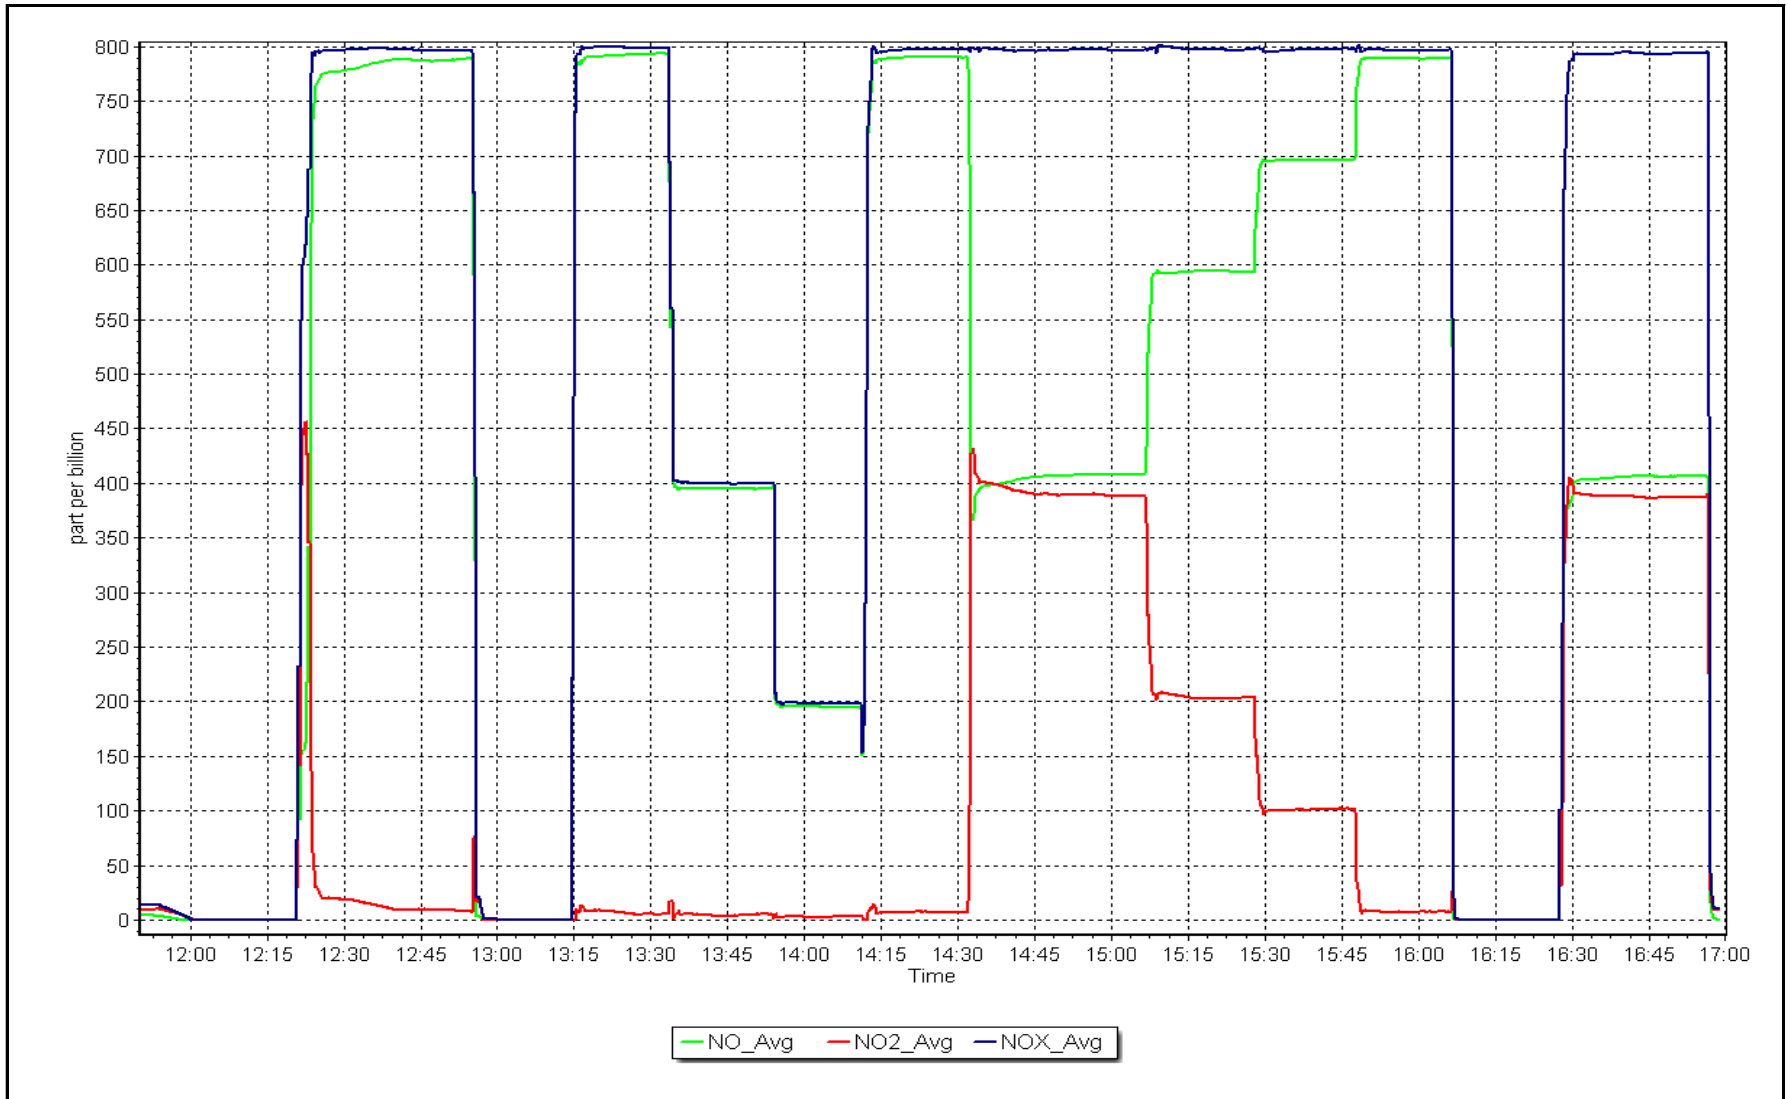



Wood Buffalo Environmental Association

NO_x \ NO \ NO₂ Calibration Report

Version-04-2020

Dilution Calibration Data

Set Point	Dilution flow rate (sccm)	Source gas flow rate (sccm)	Calculated NO _x concentration (ppb) (Cc)	Calculated NO concentration (ppb) (Cc)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO _x concentration (ppb) (Ic)	Indicated NO concentration (ppb) (Ic)	Indicated NO ₂ concentration (ppb) (Ic)	NO _x Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>	NO Correction factor (Cc/Ic) <i>Limit = 0.95-1.05</i>
as found zero	5000	0.0	0.0	0.0	0.0	0.1	-0.2	0.3	----	----
as found span	4919	81.0	800.1	794.1	6.0	733.2	726.9	6.3	1.0913	1.0925
as found 2nd										
as found 3rd										
new cyl resp										
calibrator zero	5000	0.0	0.0	0.0	0.0	0.0	-0.1	0.1	----	----
high point	4919	81.0	800.1	794.1	6.0	800.0	795.0	5.4	1.0001	0.9989
second point	4960	40.5	400.0	397.0	3.0	398.2	392.6	5.6	1.0046	1.0113
third point	4980	20.2	199.5	198.0	1.5	195.3	192.6	2.8	1.0216	1.0282
as left zero	5000	0.0	0.0	0.0	0.0	0.0	-0.1	0.1	----	----
as left span	4919	81.0	800.1	411.7	388.4	794.0	406.1	387.8	1.0077	1.0138
Average Correction Factor									1.0088	1.0128

Corrected As found	NO _x = 733.1 ppb	NO = 727.1 ppb	* = > +/-5% change initiates investigation	*Percent Change	NO _x = -9.0%
Previous Response	NO _x = 799.2 ppb	NO = 792.9 ppb		*Percent Change	NO = -9.1%
Baseline Corr 2nd pt	NO _x = NA ppb	NO = NA ppb	As found	NO _x r ² :	Nx SI:
Baseline Corr 3rd pt	NO _x = NA ppb	NO = NA ppb	As found	NO r ² :	NO SI:
			As found	NO ₂ r ² :	NO ₂ SI:

GPT Calibration Data

O3 Setpoint (ppb)	Indicated NO Reference concentration (ppb)	Indicated NO Drop concentration (ppb)	Calculated NO ₂ concentration (ppb) (Cc)	Indicated NO ₂ concentration (ppb) (Ic)	NO ₂ Correction factor (Cc/Ic) <i>Calibration Limit = 0.95-1.05</i> <i>As Found Limit = 0.90-1.10</i>	Converter Efficiency <i>Calibration Limit = 96-104%</i>
as found GPT zero						
as found GPT point (400 ppb NO2)						
as found GPT point (200 ppb NO2)						
as found GPT point (100 ppb NO2)						
1st GPT point (400 ppb O3)	790.3	407.9	388.4	388.2	1.0005	100.0%
2nd GPT point (200 ppb O3)	790.3	594.3	202.0	203.6	0.9921	100.8%
3rd GPT point (100 ppb O3)	790.3	696.3	100.0	101.3	0.9871	101.3%
Average Correction Factor					0.9932	100.7%

Notes: Changed out external pump. Adjusted span. Large adjustment made, over 6%.

Calibration Performed By: Braiden Boutillier



Wood Buffalo Environmental Association

NO_x Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 22, 2023	Previous Calibration:	January 10, 2023
Station Name:	Kirby North	Station Number:	AMS508
Start Time (MST):	11:22	End Time (MST):	16:54
Analyzer make:	API T200	Analyzer serial #:	7029

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>
0.0	0.0	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
800.1	800.0	1.0001		
400.0	398.2	1.0046		
199.5	195.3	1.0216		
			0.999969	
			1.001403	
			-2.032210	

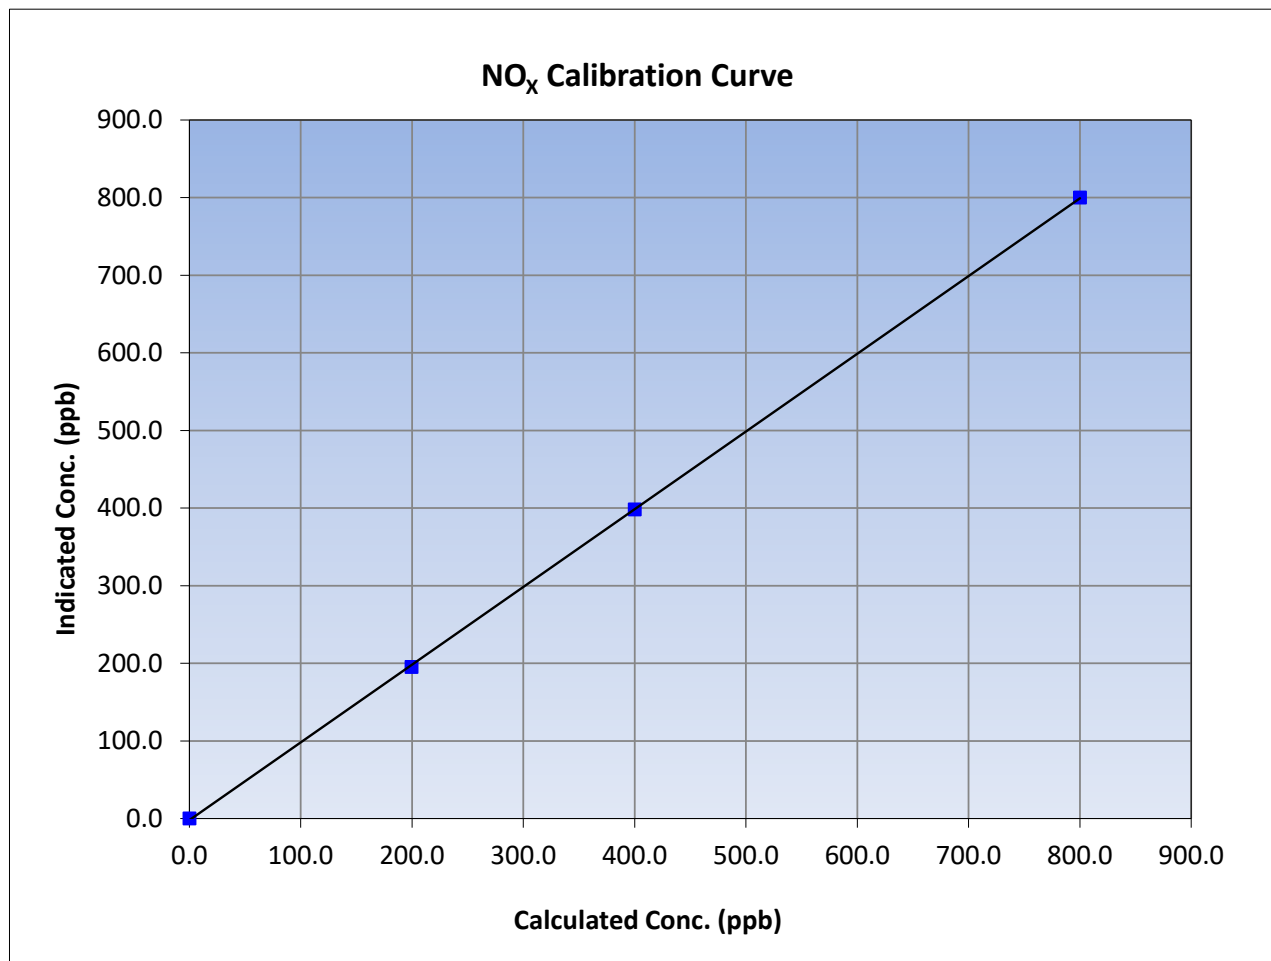



Wood Buffalo Environmental Association

NO Calibration Summary


Version-04-2020

Station Information

Calibration Date:	January 22, 2023	Previous Calibration:	January 10, 2023
Station Name:	Kirby North	Station Number:	AMS508
Start Time (MST):	11:22	End Time (MST):	16:54
Analyzer make:	API T200	Analyzer serial #:	7029

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>
0.0	-0.1	----	Correlation Coefficient Slope Intercept	≥0.995 0.90 - 1.10 +/-20
794.1	795.0	0.9989		
397.0	392.6	1.0113		
198.0	192.6	1.0282		

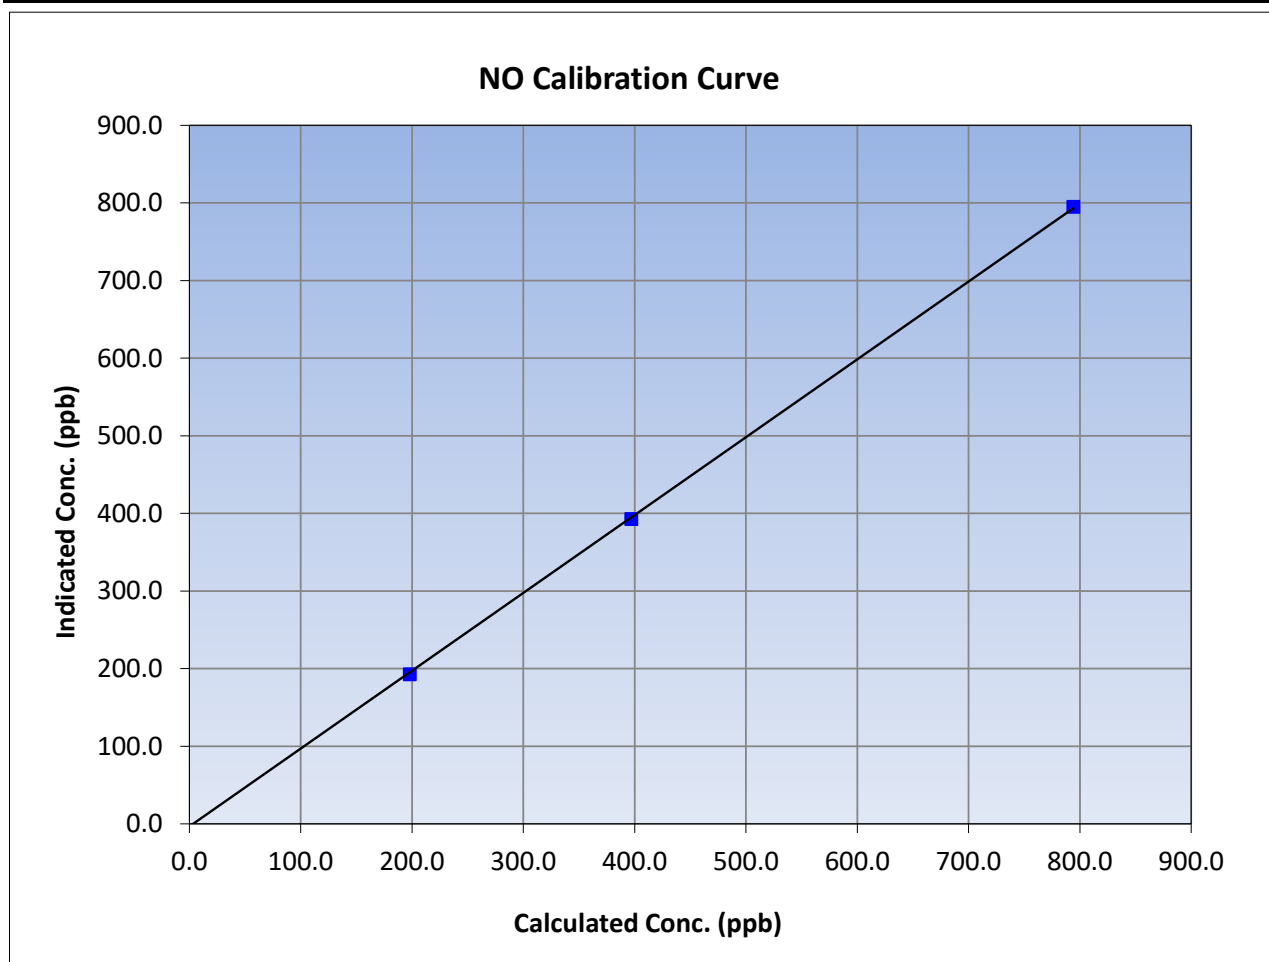



Wood Buffalo Environmental Association

NO₂ Calibration Summary

Version-04-2020


Station Information

Calibration Date:	January 22, 2023	Previous Calibration:	January 10, 2023
Station Name:	Kirby North	Station Number:	AMS508
Start Time (MST):	11:22	End Time (MST):	16:54
Analyzer make:	API T200	Analyzer serial #:	7029

Calibration Data

Calculated concentration (ppb) (Cc)	Indicated concentration (ppb) (Ic)	Correction factor (Cc/Ic)	Statistical Evaluation	<u>Limits</u>	
0.0	0.1	----	Correlation Coefficient	≥0.995	
388.4	388.2	1.0005			
202.0	203.6	0.9921			
100.0	101.3	0.9871			
			Slope	0.998706	0.90 - 1.10
			Intercept	0.927800	+/-20


NO₂ Calibration Curve

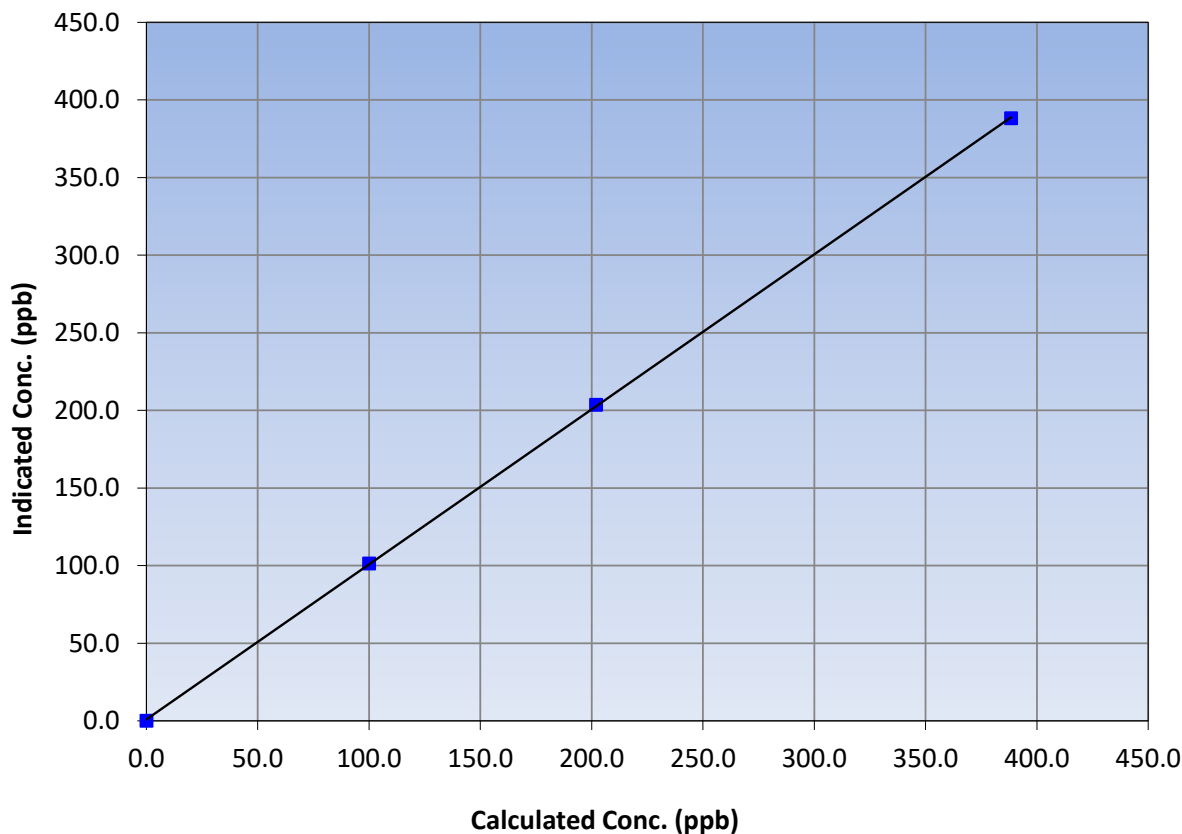

NO_x Calibration Plot

Date: January 22, 2023

Location: Kirby North

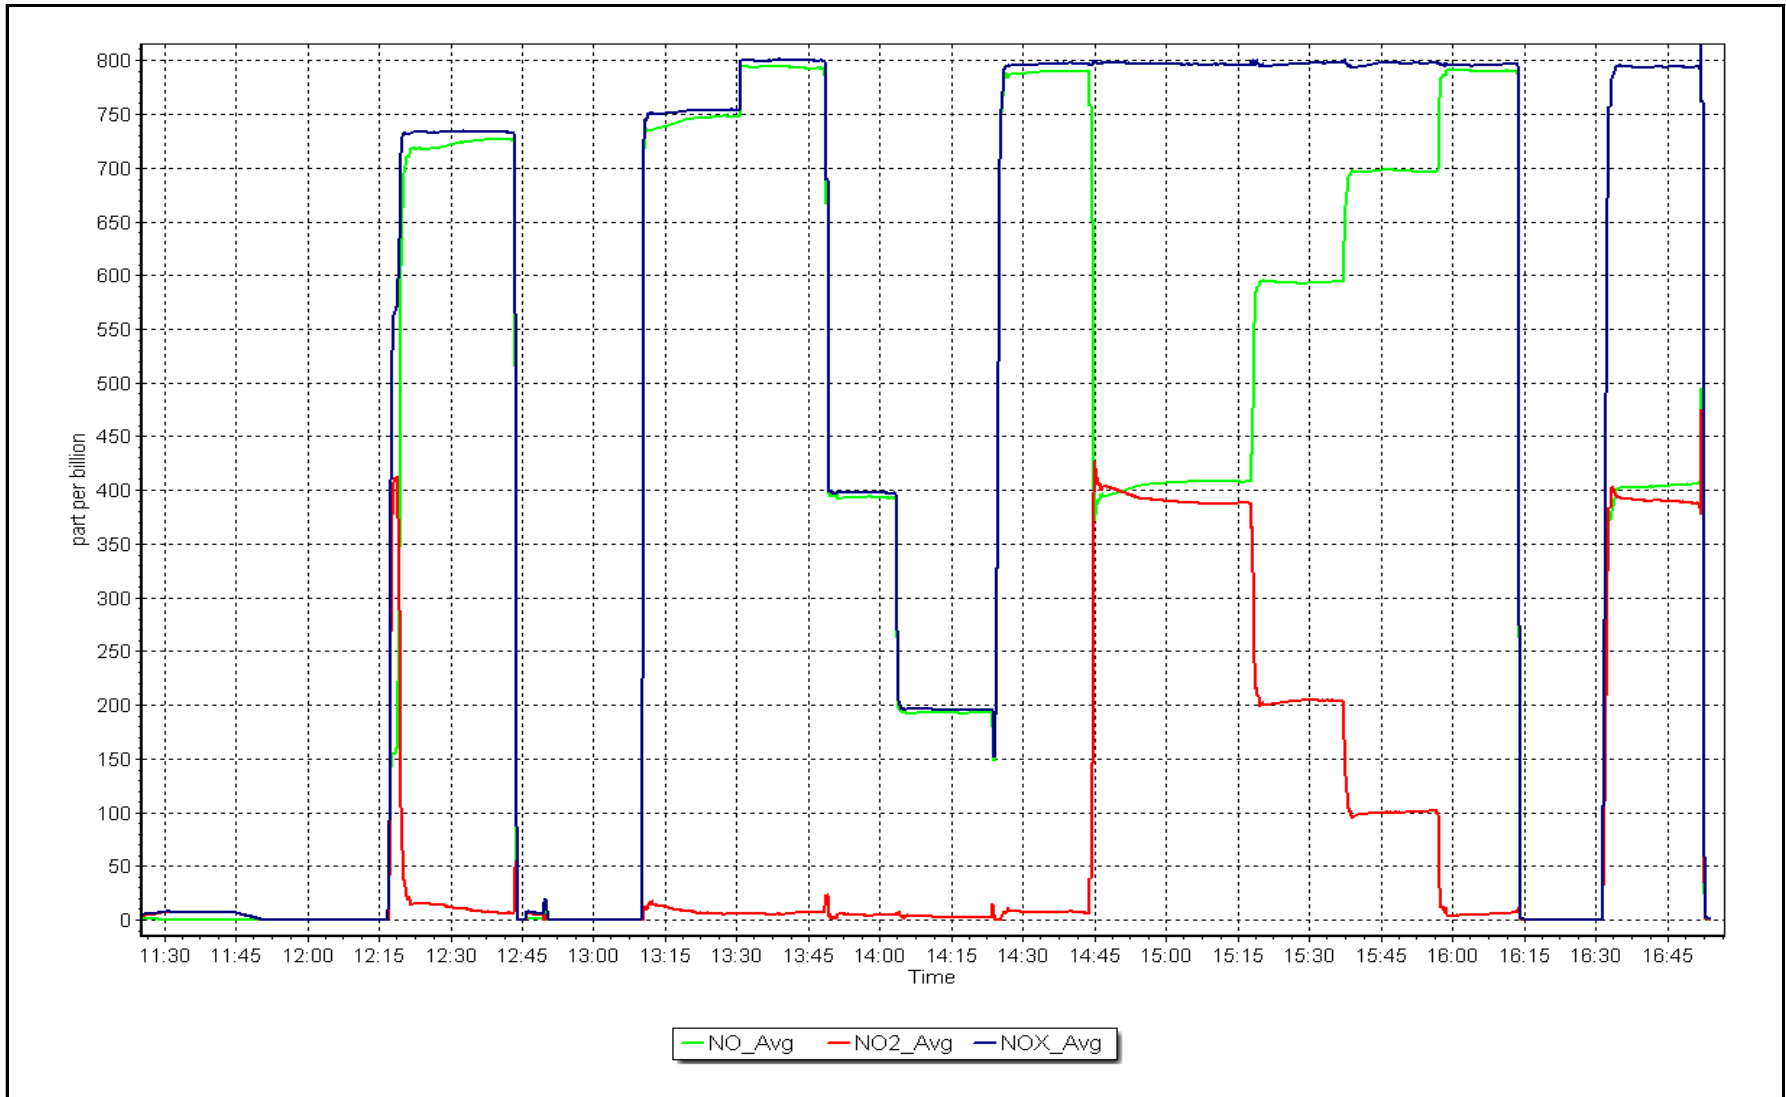



End of Report